
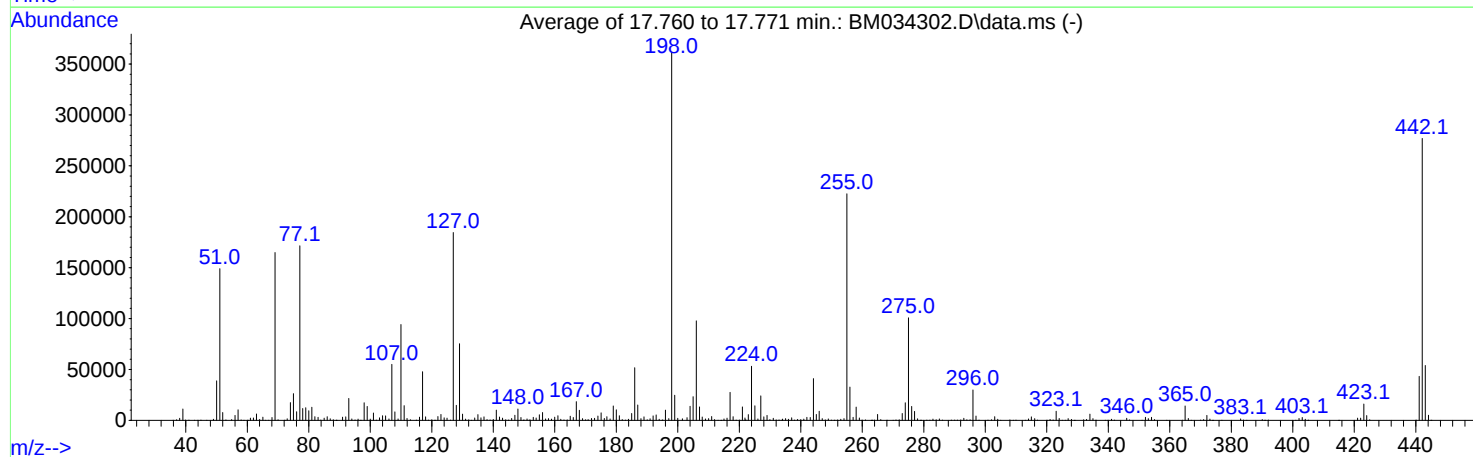


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034302.D
 Acq On : 22 Mar 2022 08:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 16 02:38:26 2022

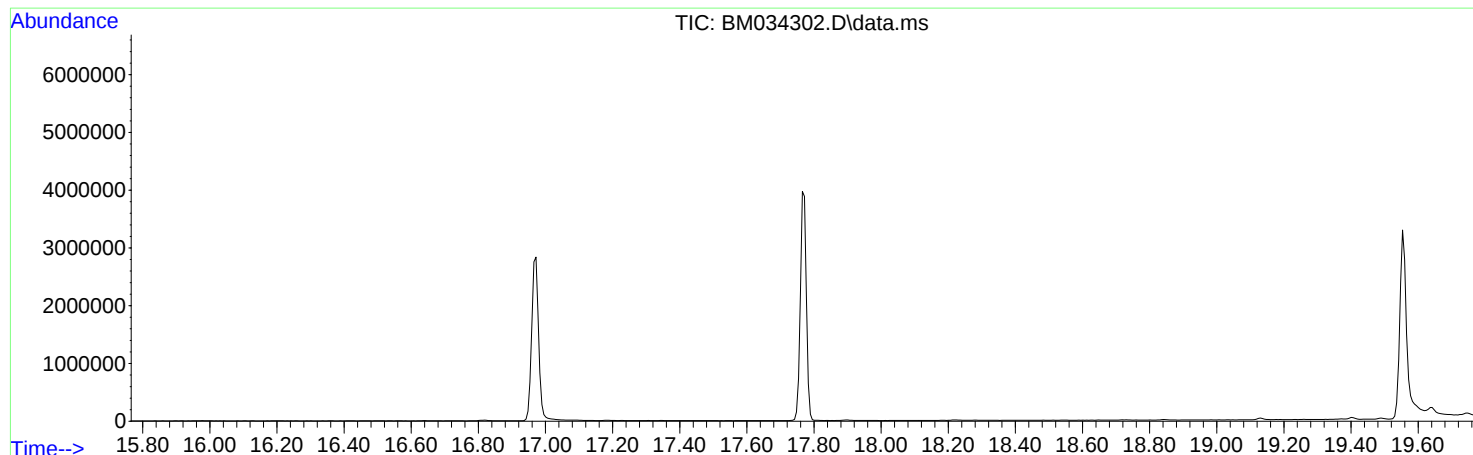




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	148944	PASS
68	69	0.00	2	1.8	2905	PASS
69	198	0.00	100	45.6	164899	PASS
70	69	0.00	2	0.4	674	PASS
127	198	10	80	51.0	184448	PASS
197	198	0.00	2	0.5	1713	PASS
198	198	100	100	100.0	361344	PASS
199	198	5	9	6.8	24624	PASS
275	198	10	60	27.9	100693	PASS
365	198	1	100	3.9	14204	PASS
441	198	0.01	100	12.0	43221	PASS
442	442	50	100	100.0	276925	PASS
443	442	15	24	19.4	53859	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034302.D
Acq On : 22 Mar 2022 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 22 14:34:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

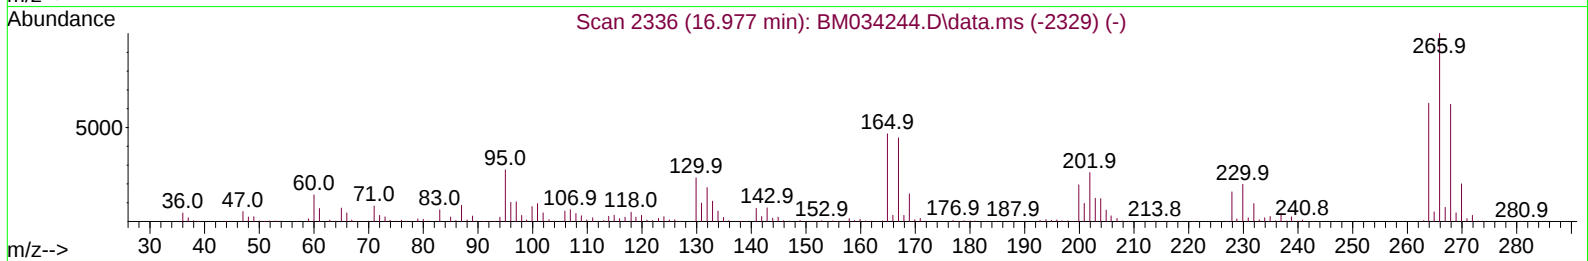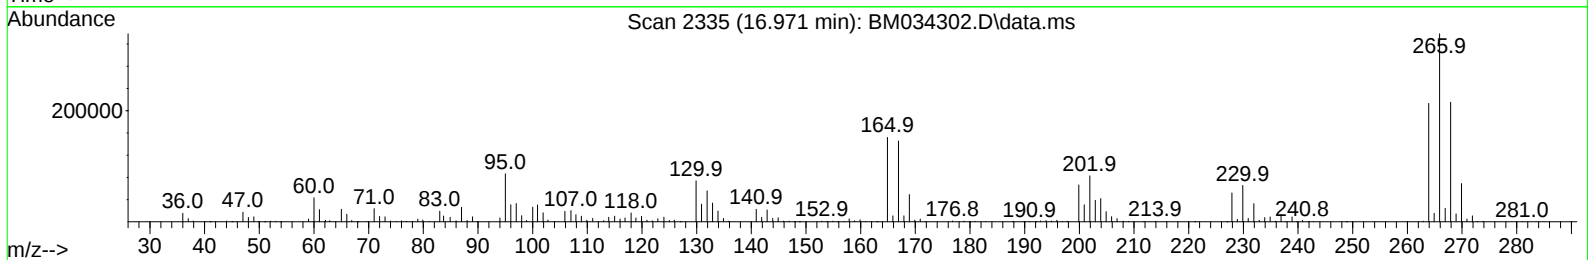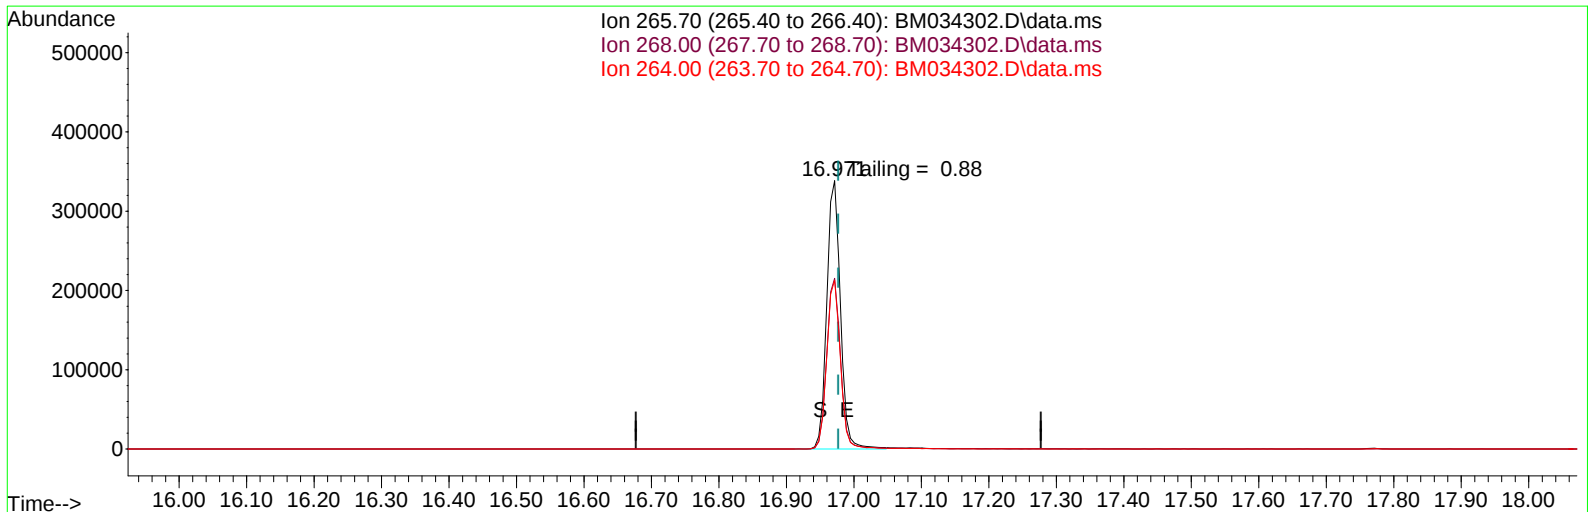

TIC: BM034302.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.006) 48844.44 ng




response 477003

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.63
264.00	62.90	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034302.D
Acq On : 22 Mar 2022 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 22 14:34:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

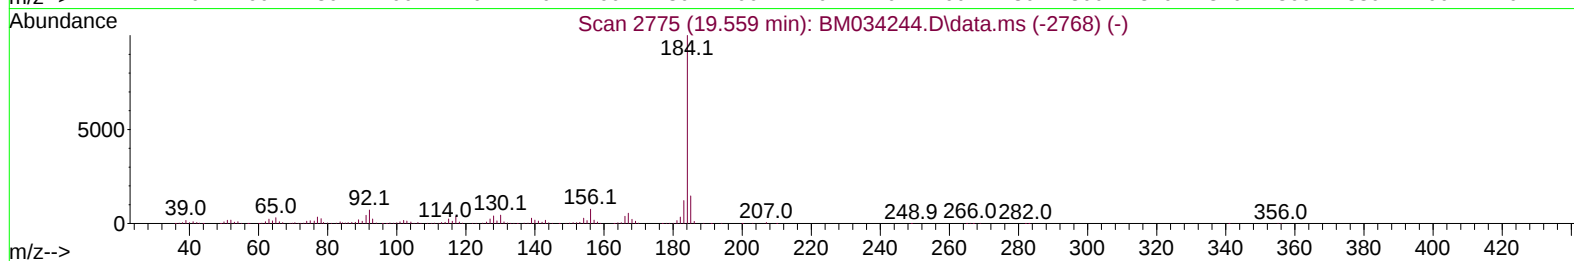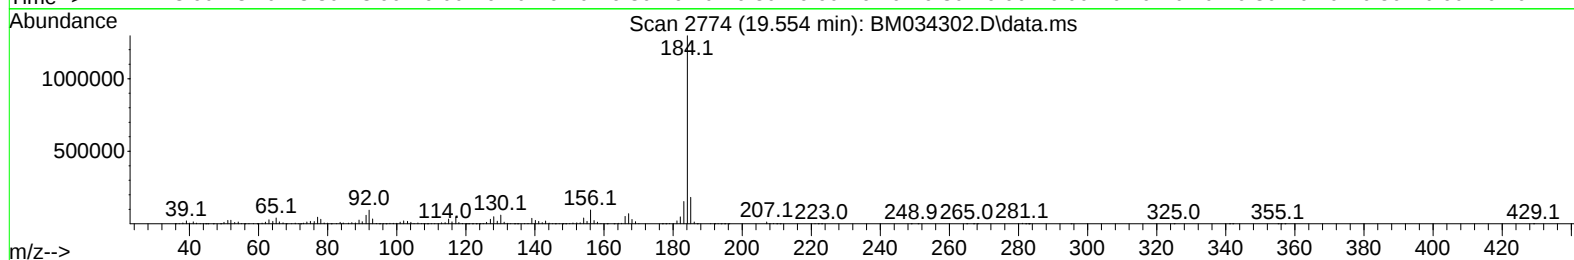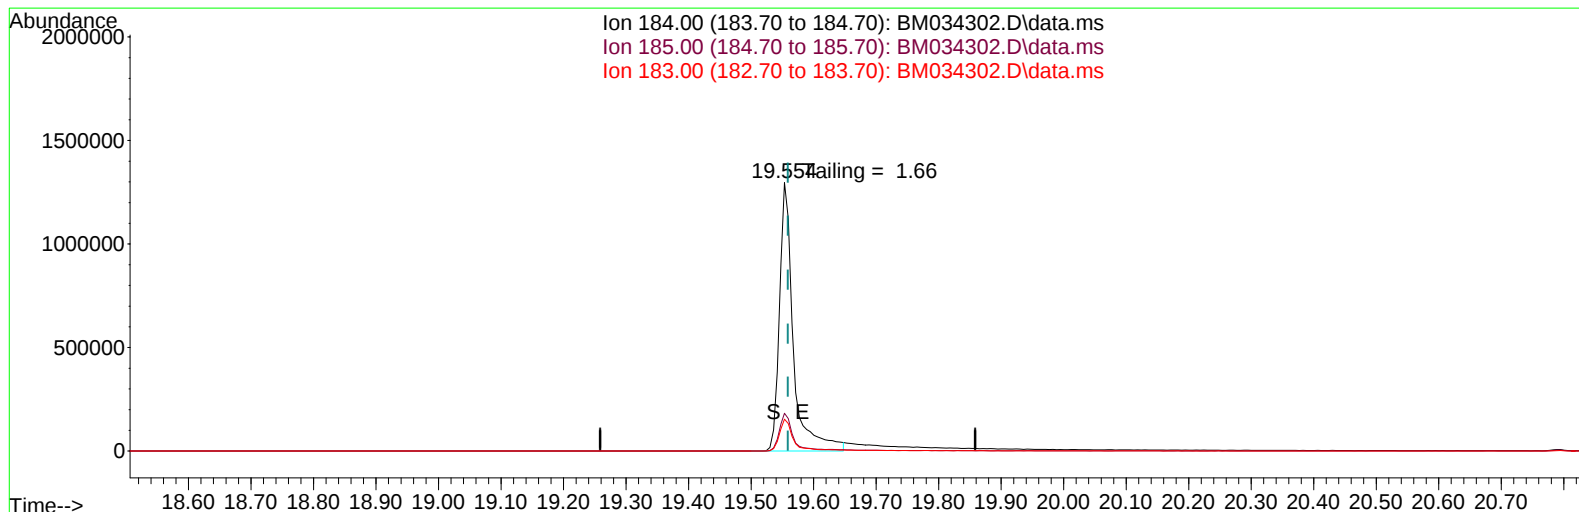

TIC: BM034302.D\data.ms

(77) Benzidine

19.554min (-0.005) 26931.94 ng

response 2250805

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.06
183.00	12.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_M	<u>BM034302.D</u>
Compound Name	Response	Retention Time
DDT	1477033	20.79
DDD	10571	20.35
DDE	1622	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12193	1489226	0.82

Instrument :
BNA_M
ClientSampleId :
DFTPP