
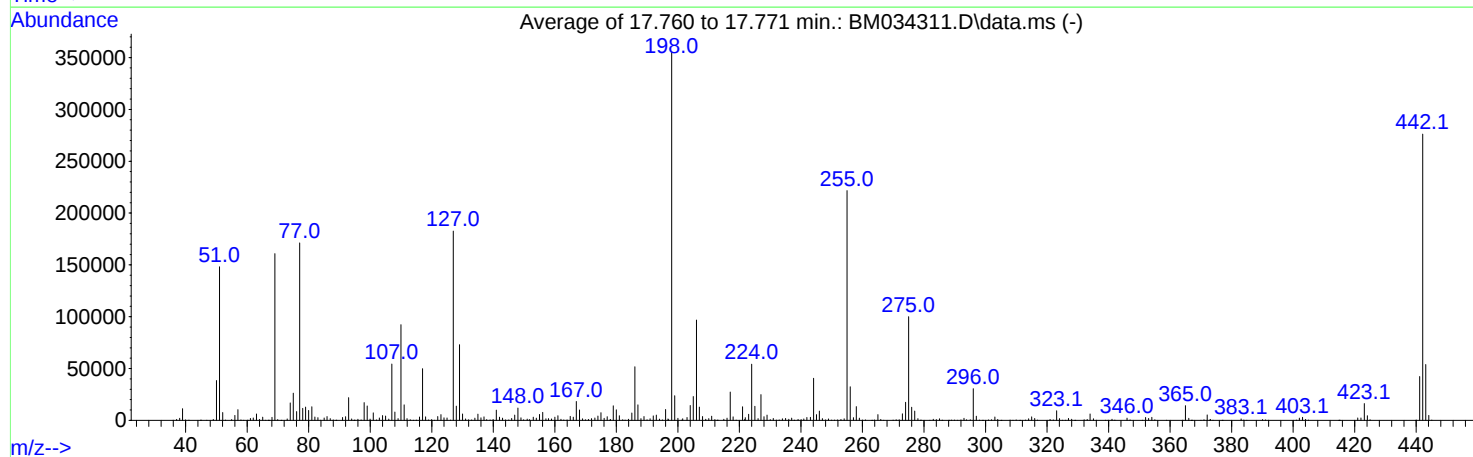


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034311.D
 Acq On : 22 Mar 2022 15:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 16 02:38:26 2022

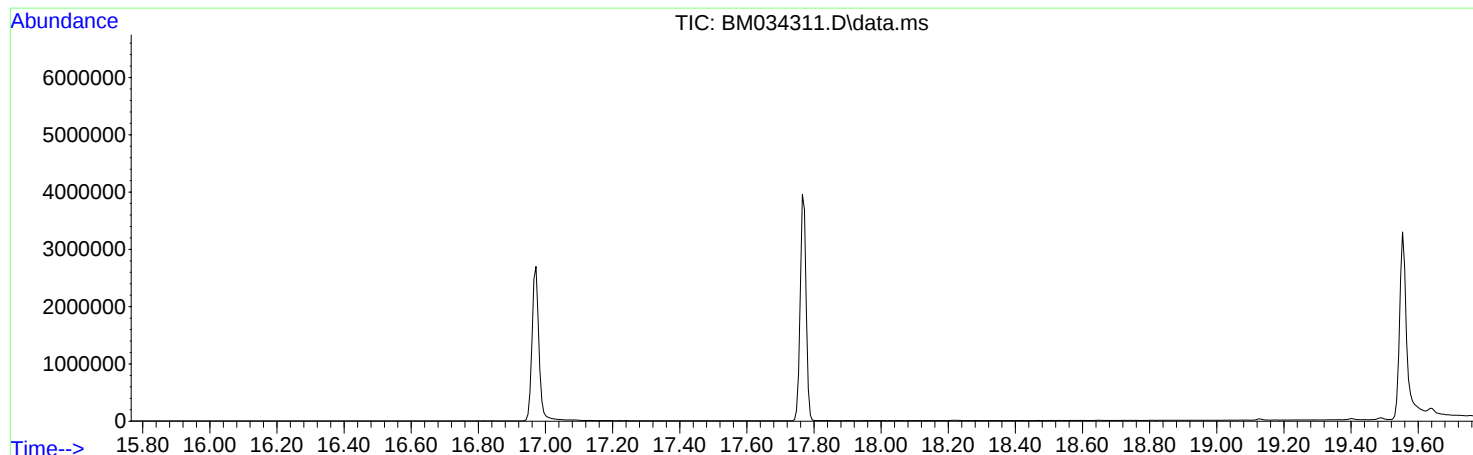




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	148155	PASS
68	69	0.00	2	1.8	2954	PASS
69	198	0.00	100	45.3	160853	PASS
70	69	0.00	2	0.5	805	PASS
127	198	10	80	51.4	182571	PASS
197	198	0.00	2	0.4	1331	PASS
198	198	100	100	100.0	354901	PASS
199	198	5	9	6.7	23776	PASS
275	198	10	60	28.2	100085	PASS
365	198	1	100	4.0	14261	PASS
441	198	0.01	100	11.9	42381	PASS
442	442	50	100	100.0	276245	PASS
443	442	15	24	19.5	53867	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034311.D
Acq On : 22 Mar 2022 15:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 22 17:28:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

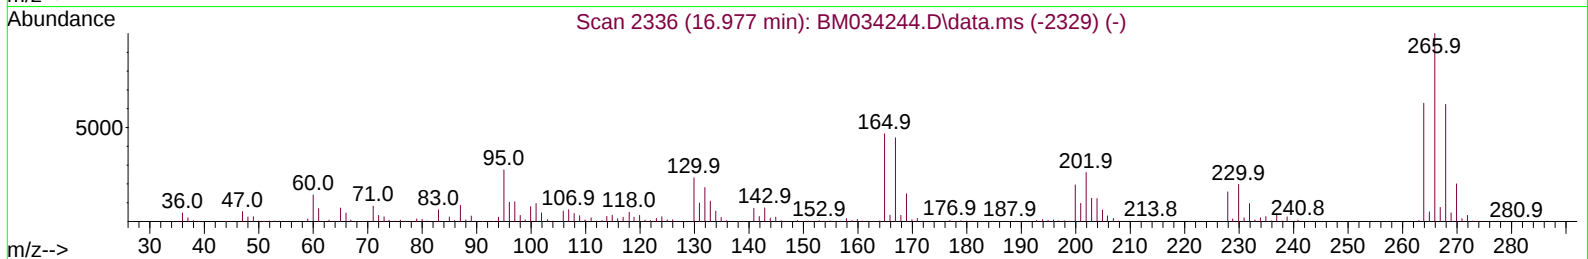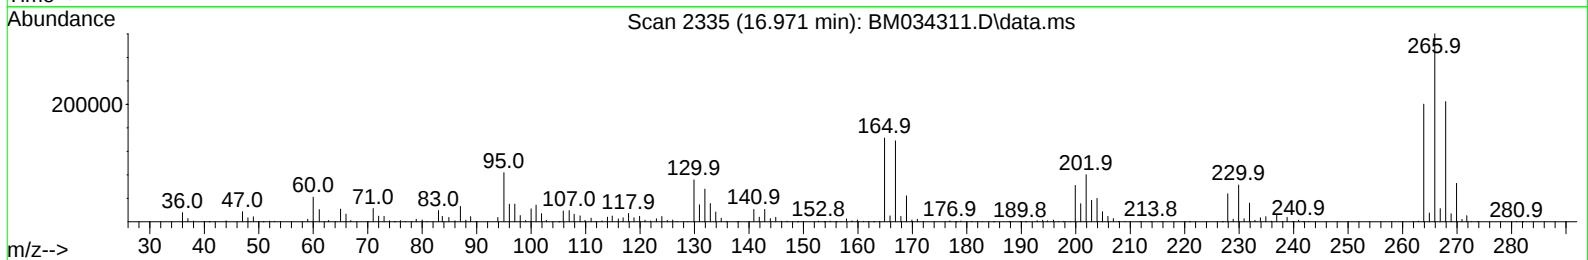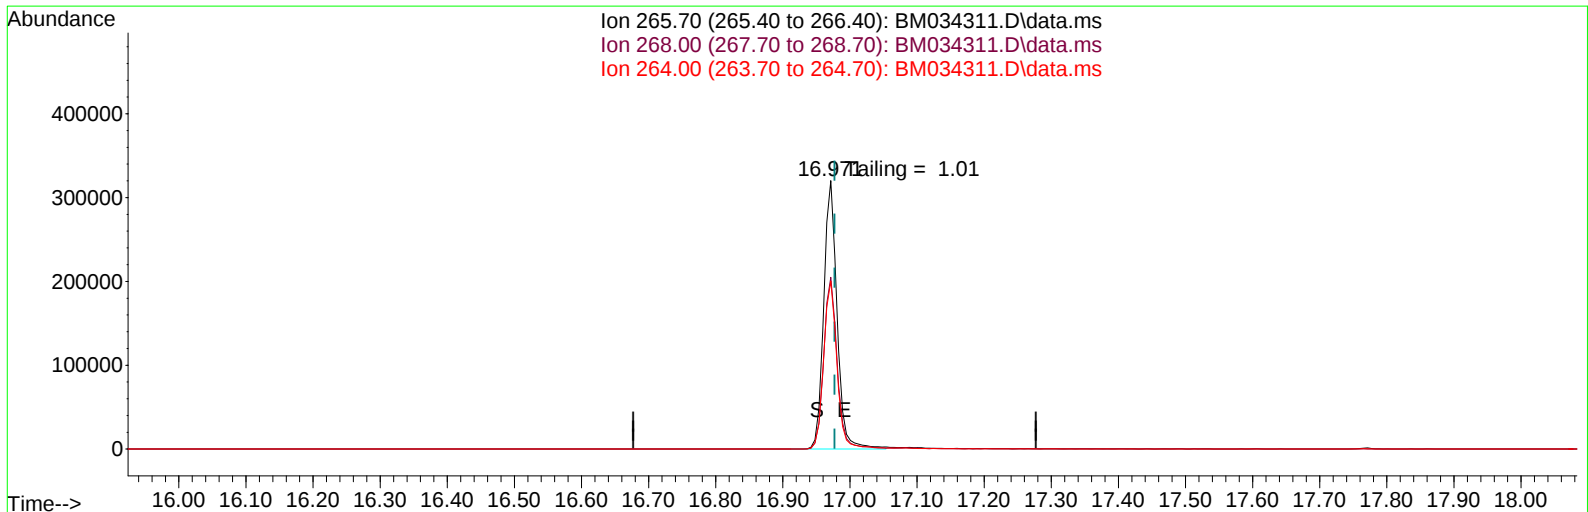

TIC: BM034311.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.006) 0.00 ng




response 444446

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.97
264.00	62.90	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034311.D
Acq On : 22 Mar 2022 15:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 22 17:28:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

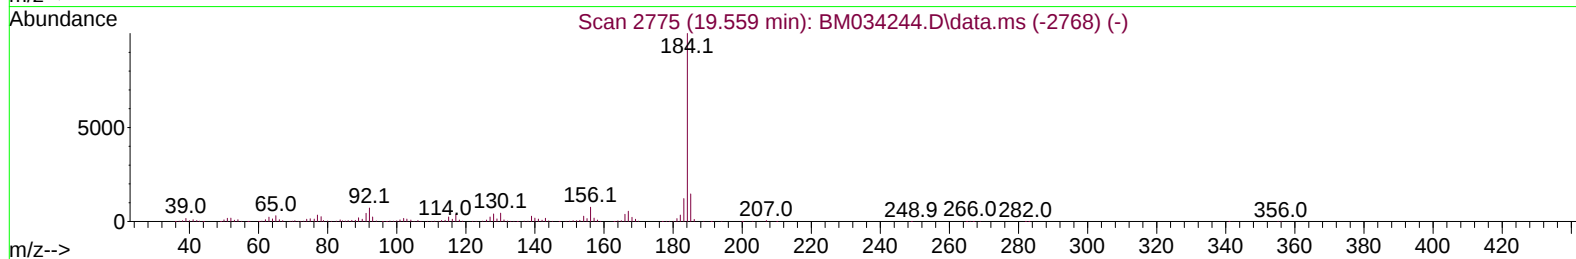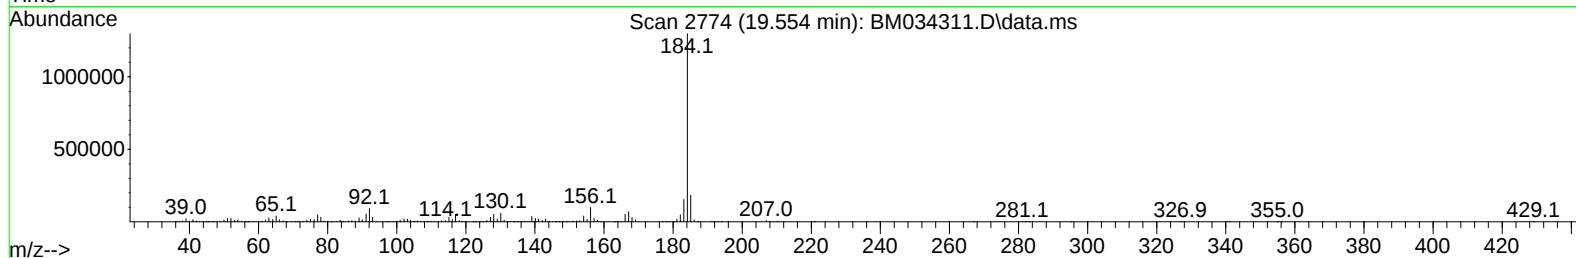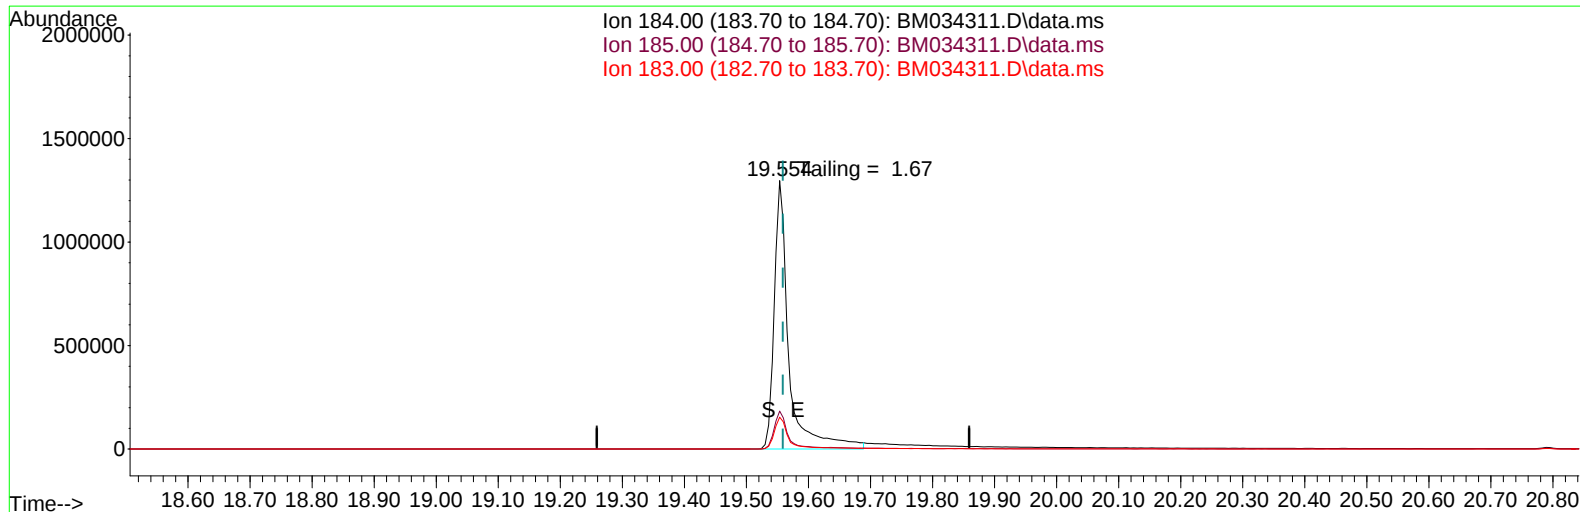

TIC: BM034311.D\data.ms

(77) Benzidine

19.554min (-0.005) 501225.62 ng

response 2306374

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.17
183.00	12.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_M	<u>BM034311.D</u>
Compound Name	Response	Retention Time
DDT	1465581	20.79
DDD	10769	20.35
DDE	1010	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11779	1477360	0.80

Instrument :
BNA_M
ClientSampleId :
DFTPP