




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

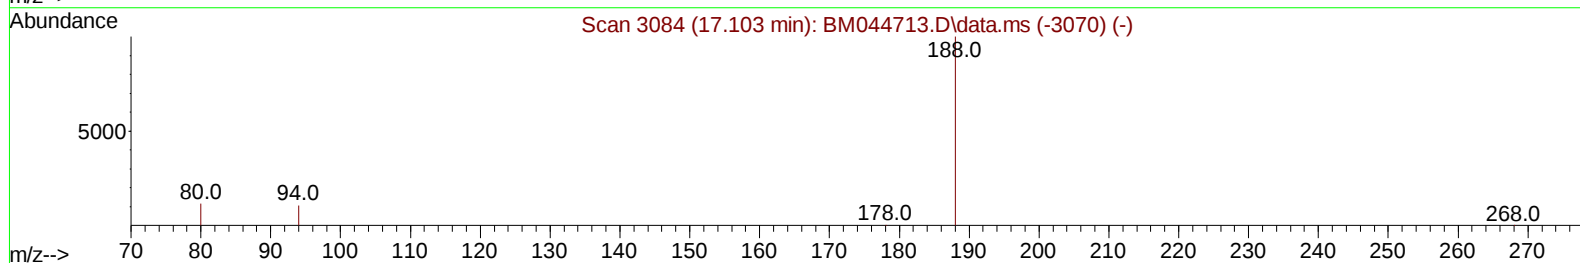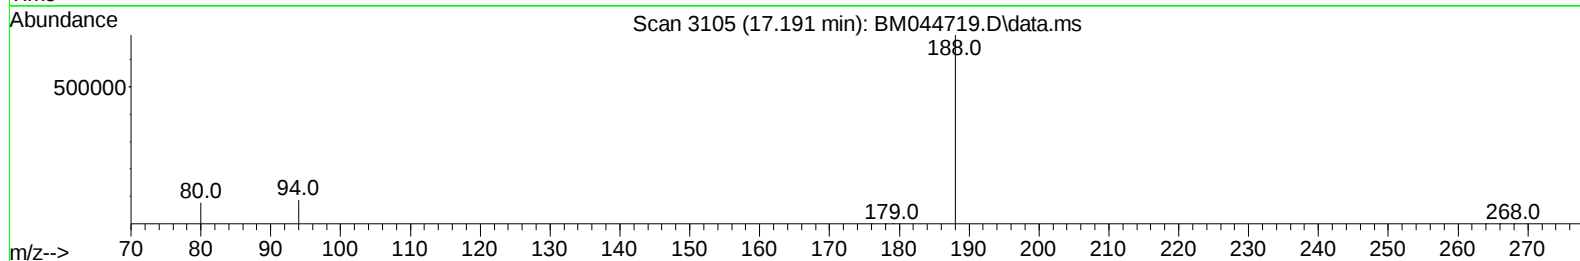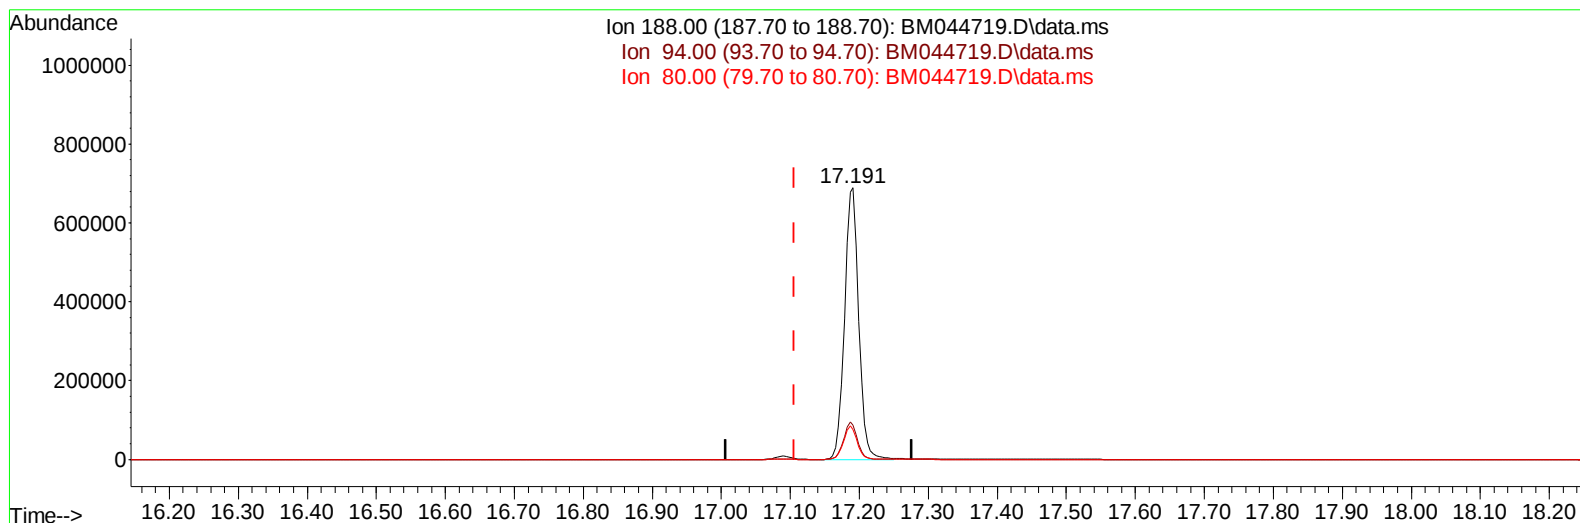

TIC: BM044719.D\data.ms

(13) Phenanthrene-d10 (I)

17.191min (+ 0.085) 0.40 ng/u1

response 981425

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	12.63
80.00	12.90	11.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

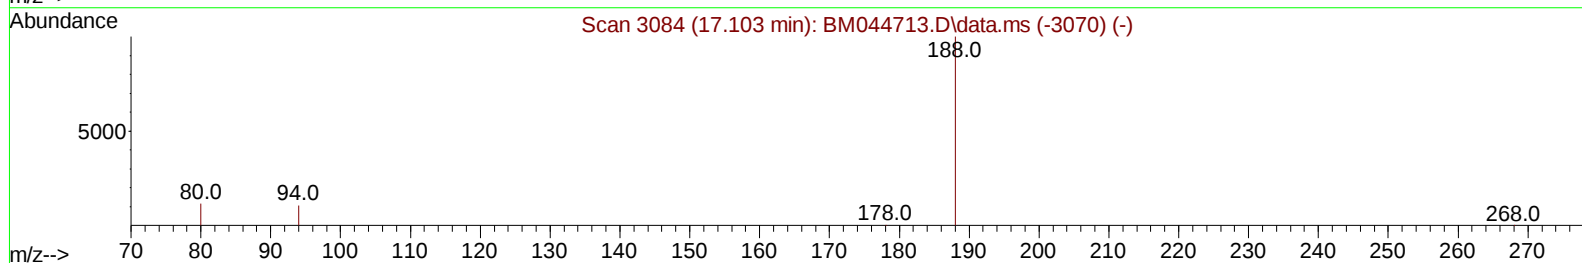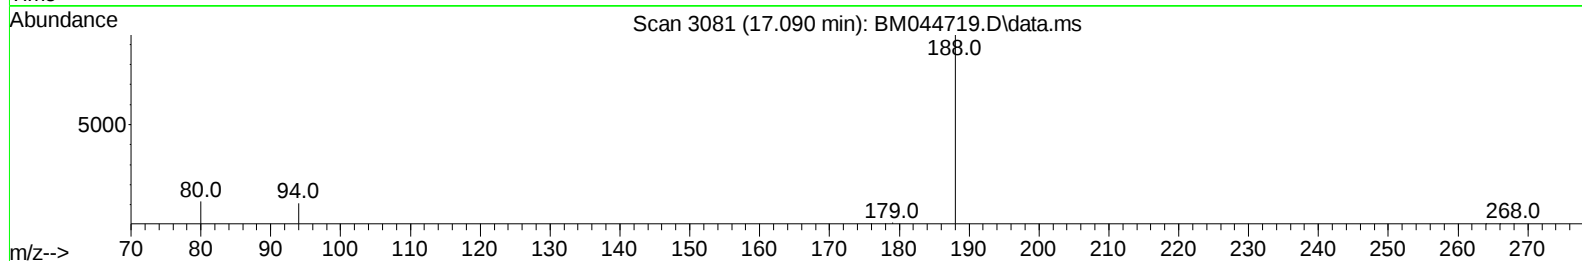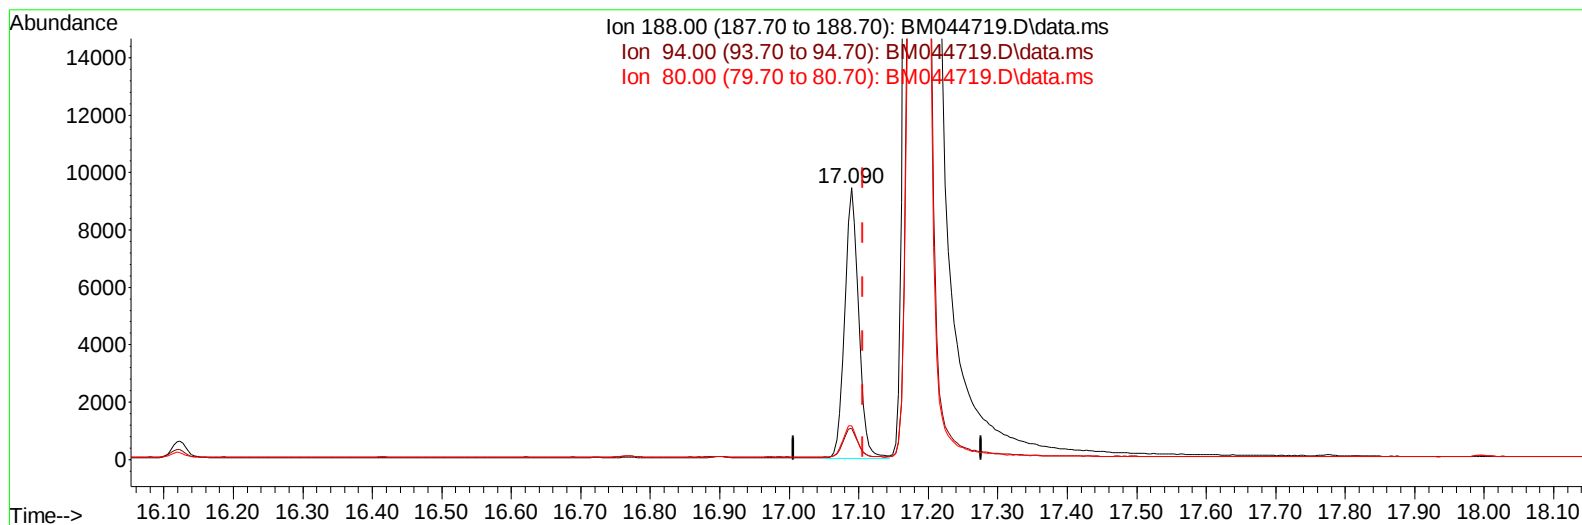

TIC: BM044719.D\data.ms

(13) Phenanthrene-d10 (I)

17.090min (-0.017) 0.40 ng/u1 m

response 13108

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	11.45
80.00	12.90	12.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

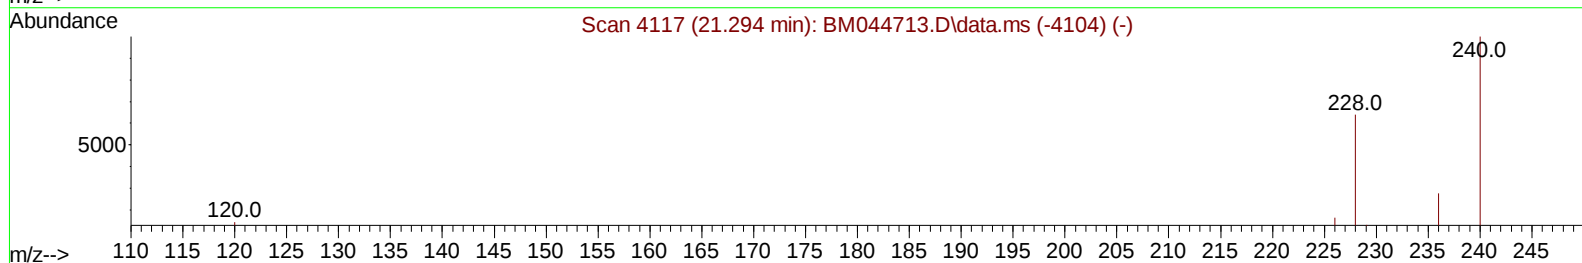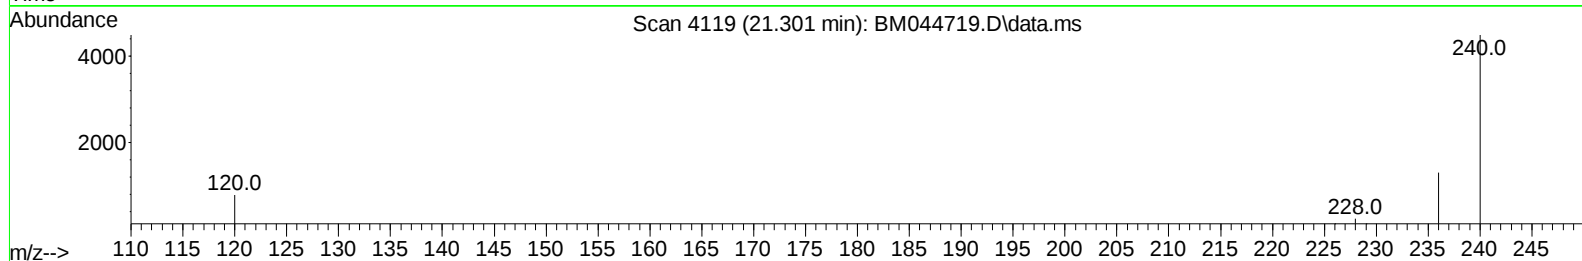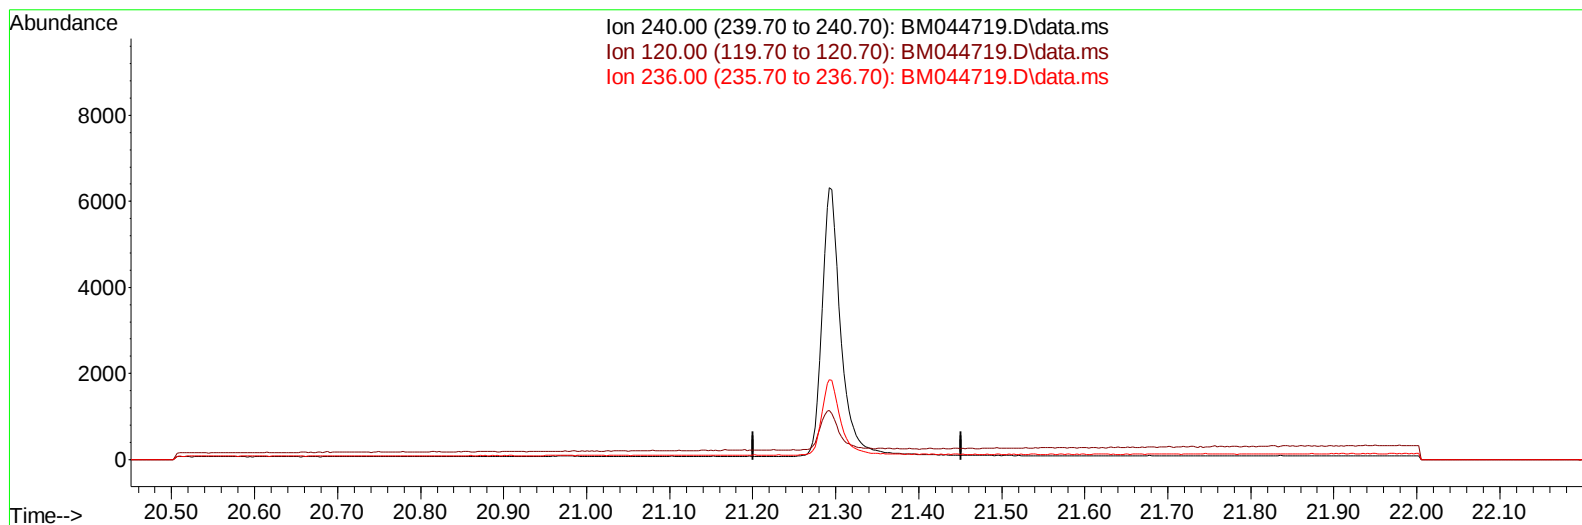

TIC: BM044719.D\data.ms

(17) Chrysene-d12

21.301min (-21.301) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.10	0.00#
236.00	28.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

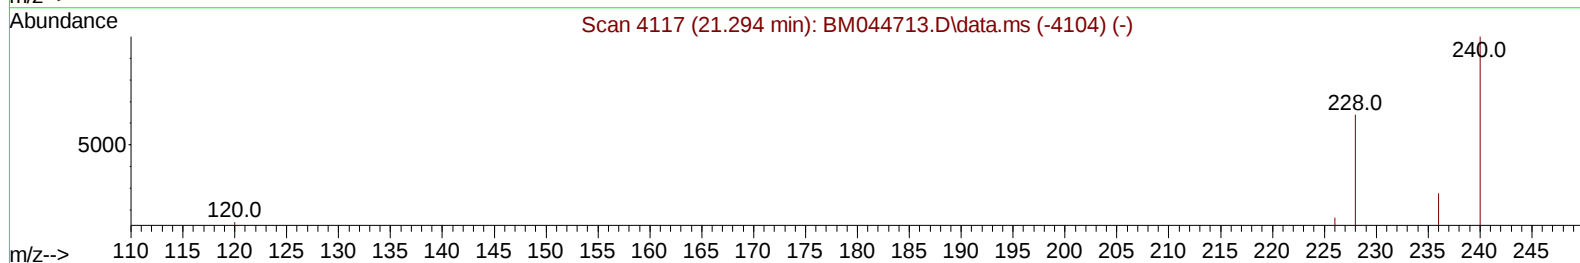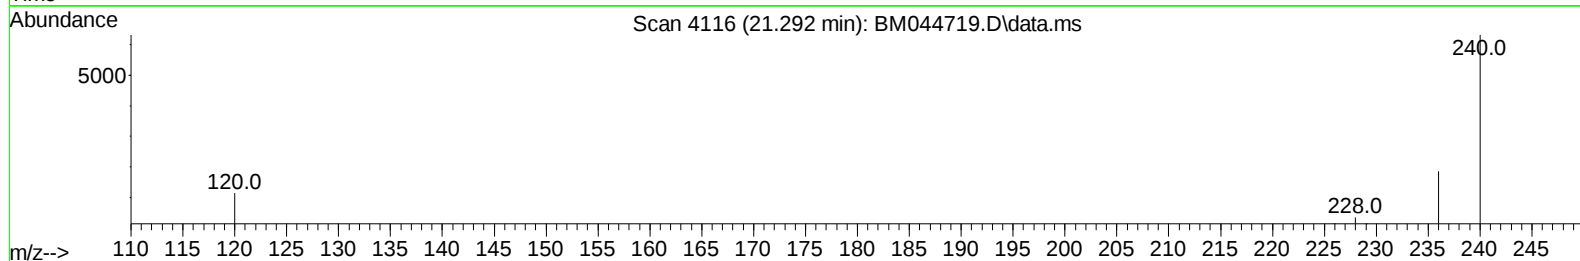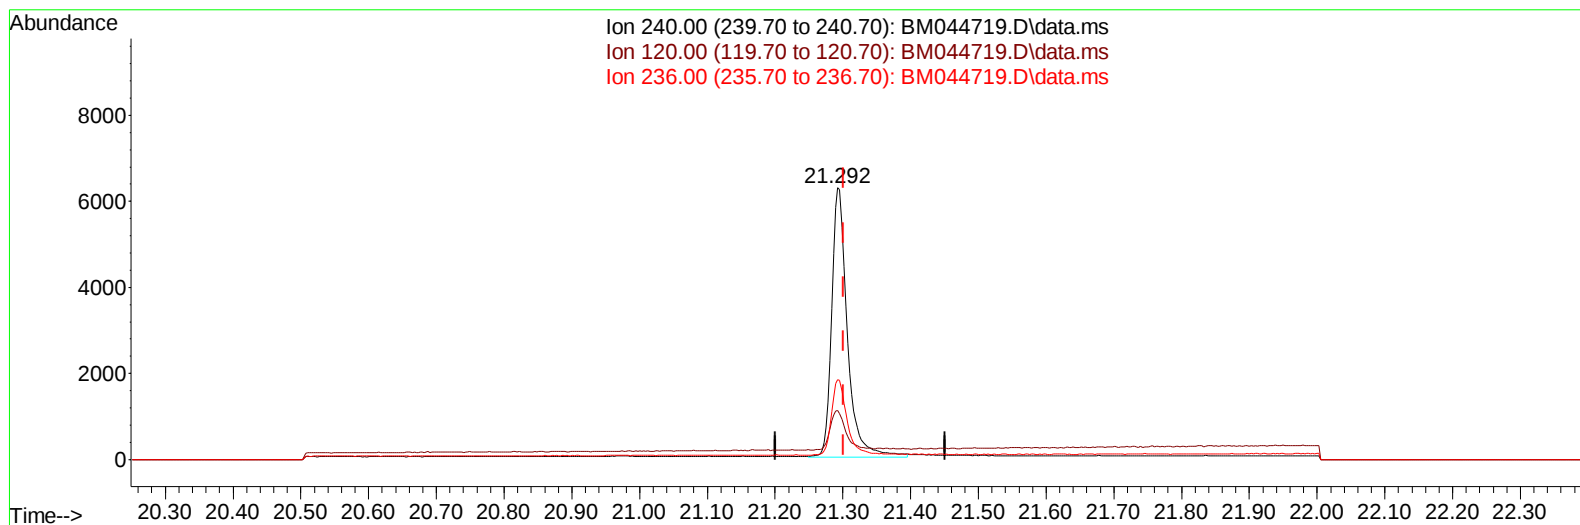

TIC: BM044719.D\data.ms

(17) Chrysene-d12

21.292min (-0.009) 0.40 ng/ul m

response 10021

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.10	18.04
236.00	28.90	29.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

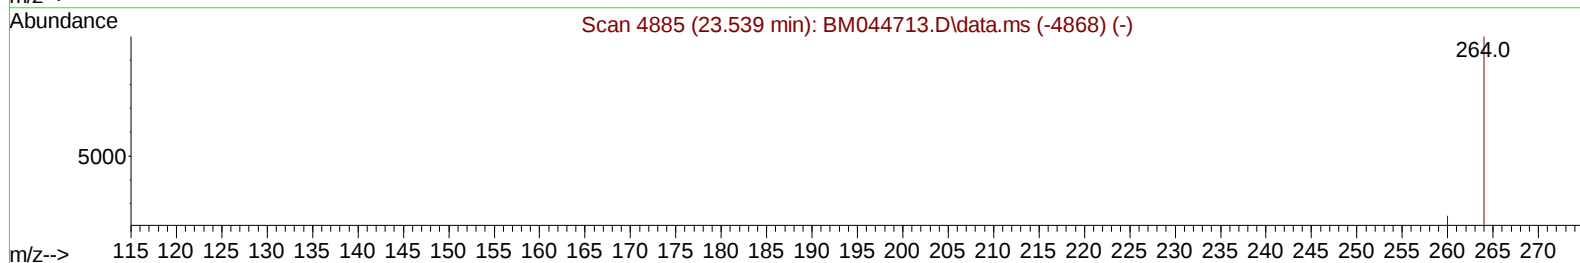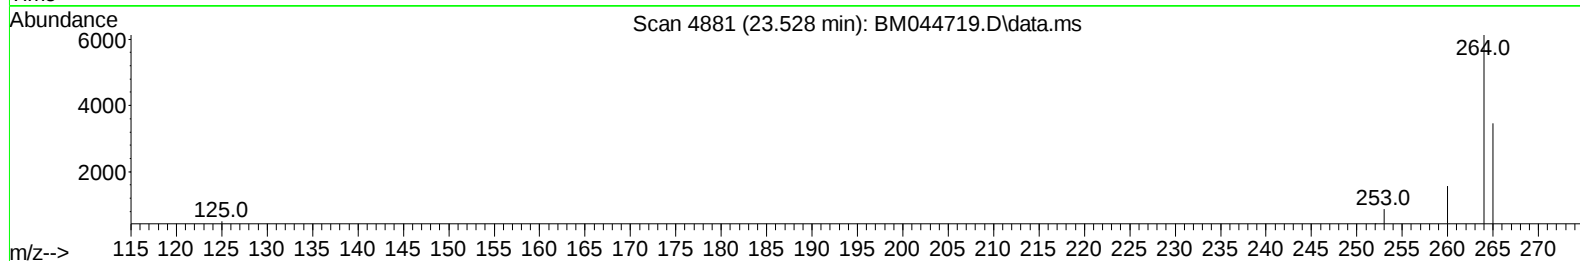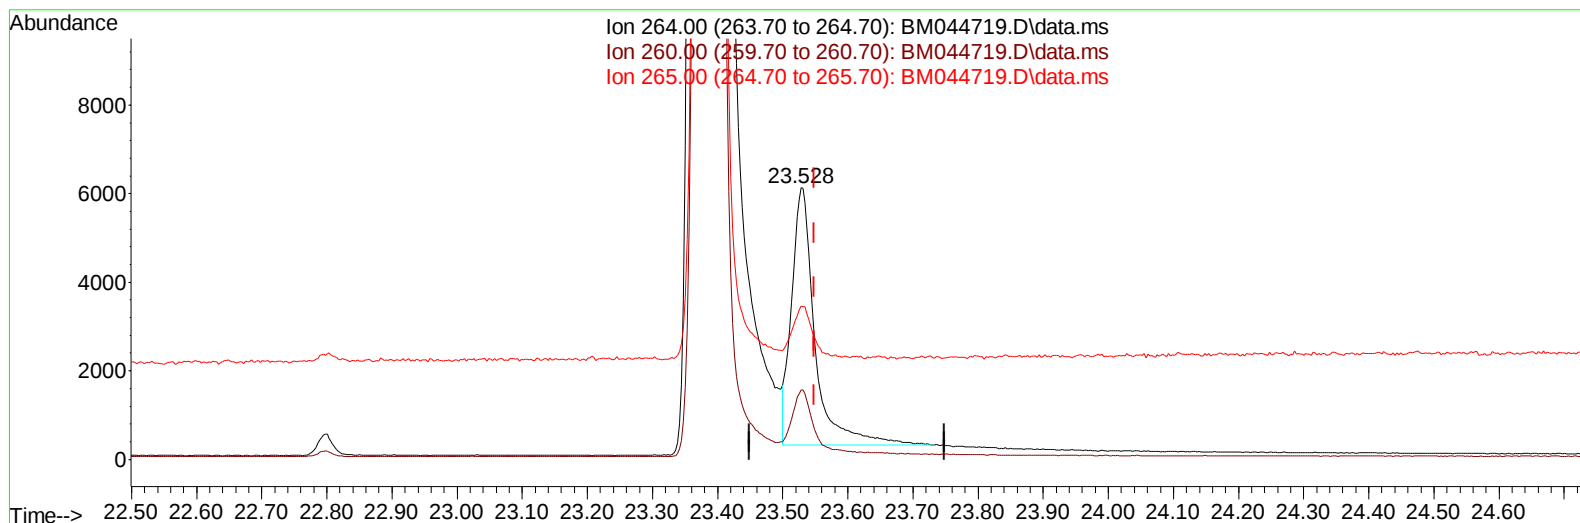

TIC: BM044719.D\data.ms

(23) Perylene-d12 (I)

23.528min (-0.020) 0.40 ng/u1

response 14534

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	25.65
265.00	60.10	56.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

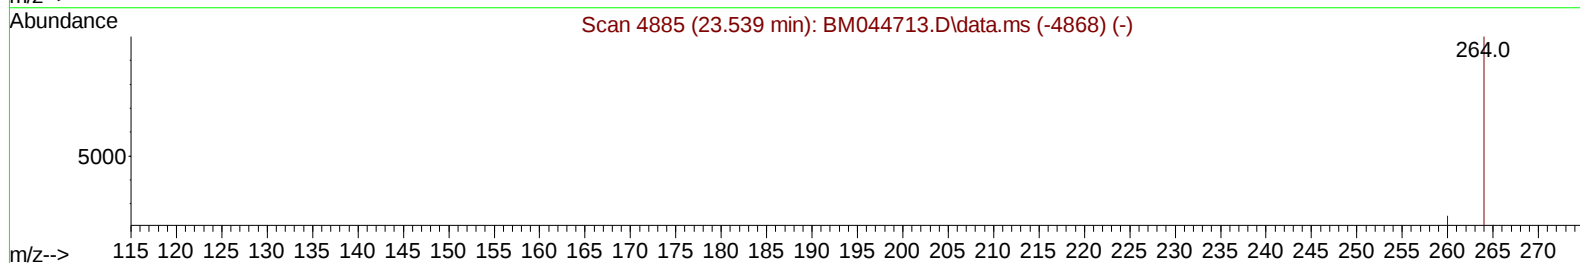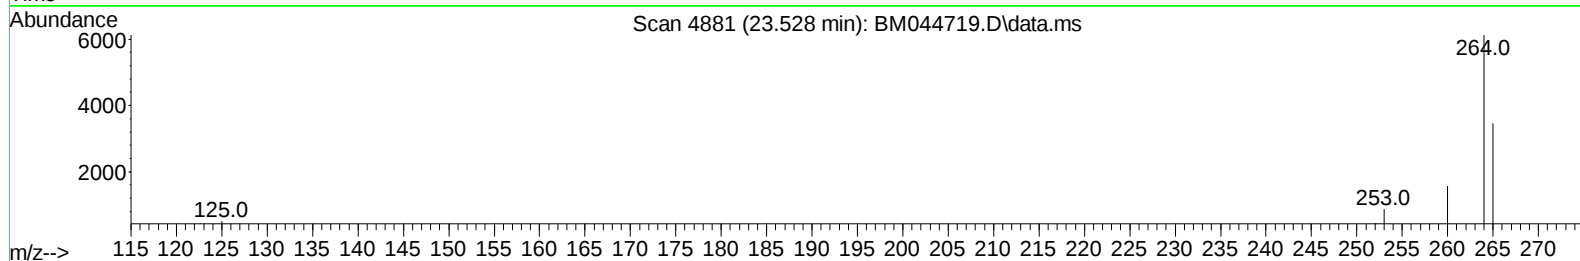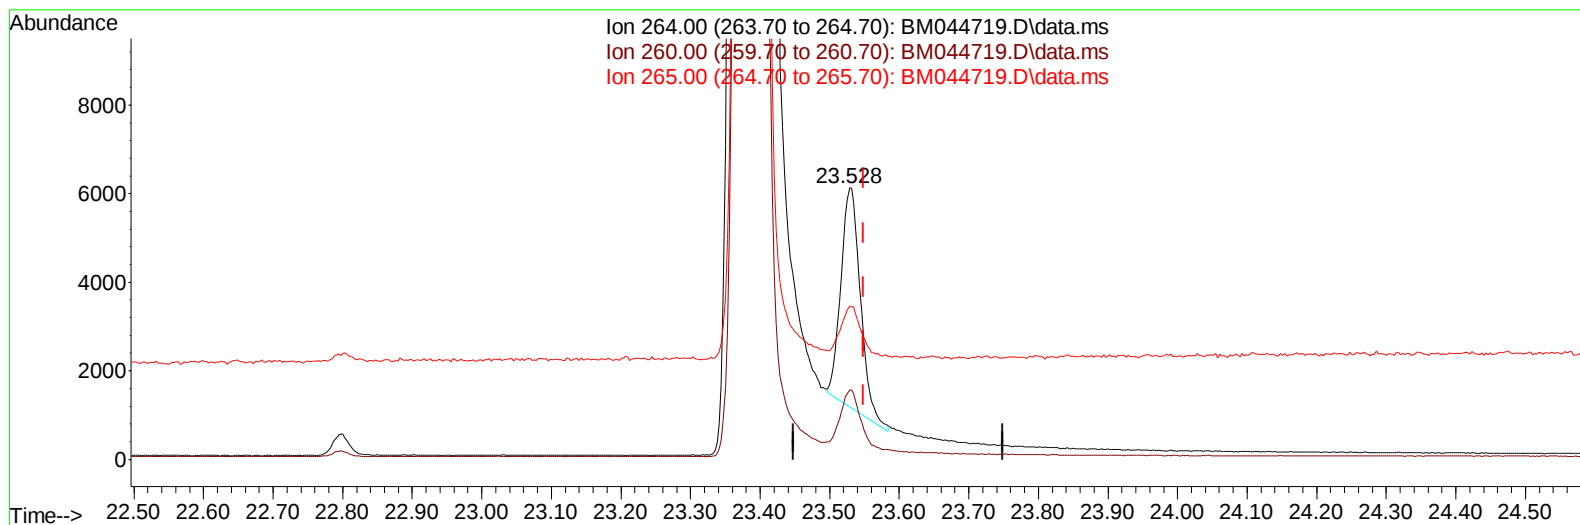

TIC: BM044719.D\data.ms

(23) Perylene-d12 (I)

23.528min (-0.020) 0.40 ng/u1 m

response 9607

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	25.65
265.00	60.10	56.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
 Data File : BM044719.D
 Acq On : 22 Mar 2024 03:45
 Operator : MA/JU
 Sample : P1813-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/22/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 22 04:25:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 20 10:51:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.694	152	4460	0.400	ng/ul	0.00
4) Naphthalene-d8	10.468	136	13977	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.334	164	6597	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.090	188	13108m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.292	240	10021m	0.400	ng/ul	0.00
23) Perylene-d12	23.528	264	9607m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	29135	4.983	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.079	152	5783	0.288	ng/ul	0.00
18) Fluoranthene-d10	19.127	212	10435	0.297	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044719.D
Acq On : 22 Mar 2024 03:45
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Manual IntegrationsAPPROVED

Quant Time: Mar 22 04:25:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/22/2024
Supervised By :mohammad ahmed 03/26/2024

