
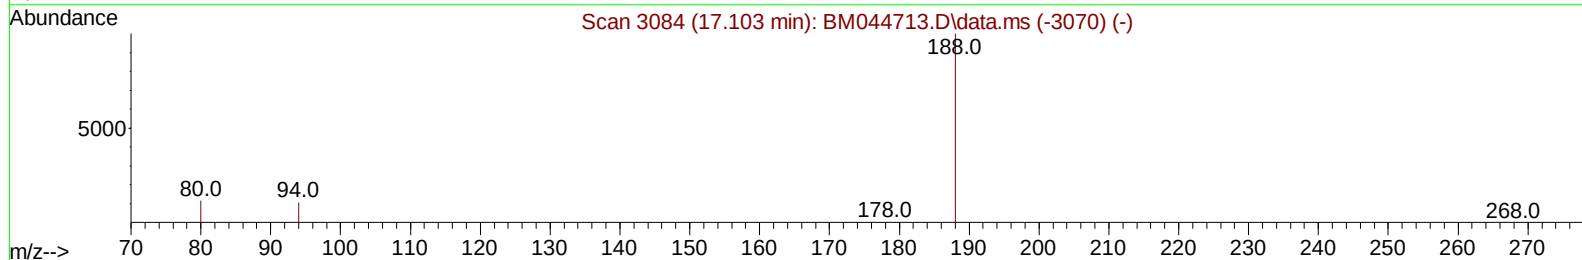
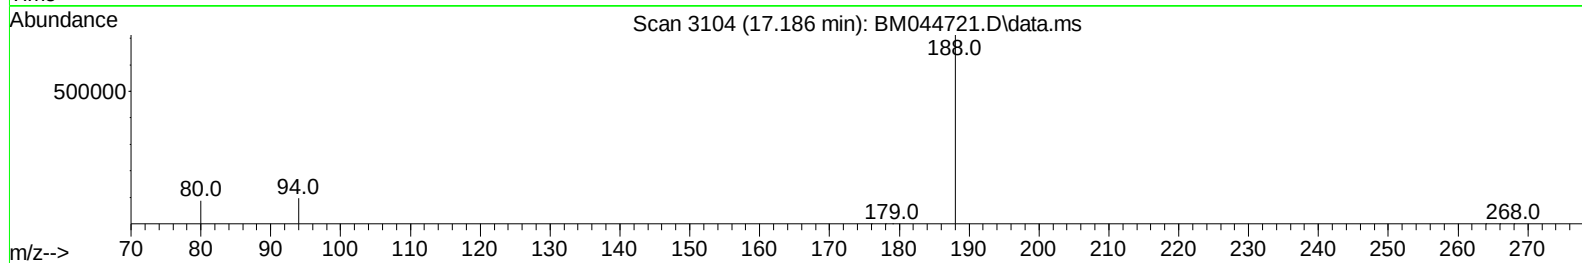


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

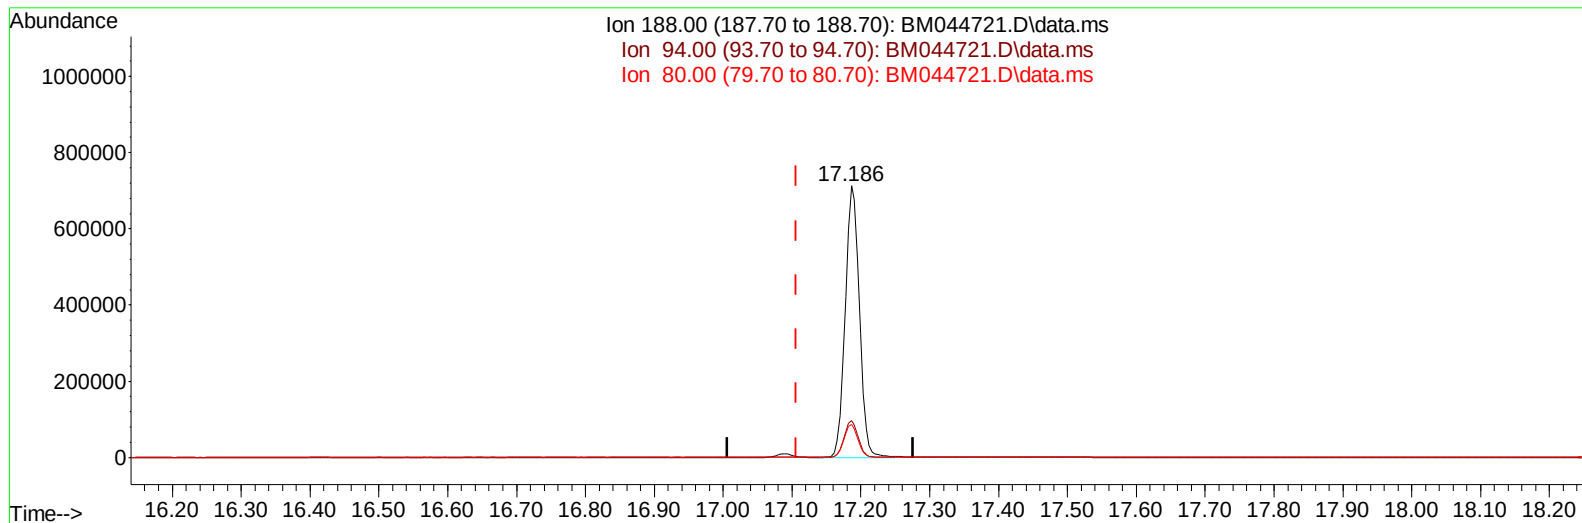

TIC: BM044721.D\data.ms

(13) Phenanthrene-d10 (I)




17.186min (+ 0.080) 0.40 ng/ul

response 1011574

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	13.52
80.00	12.90	12.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

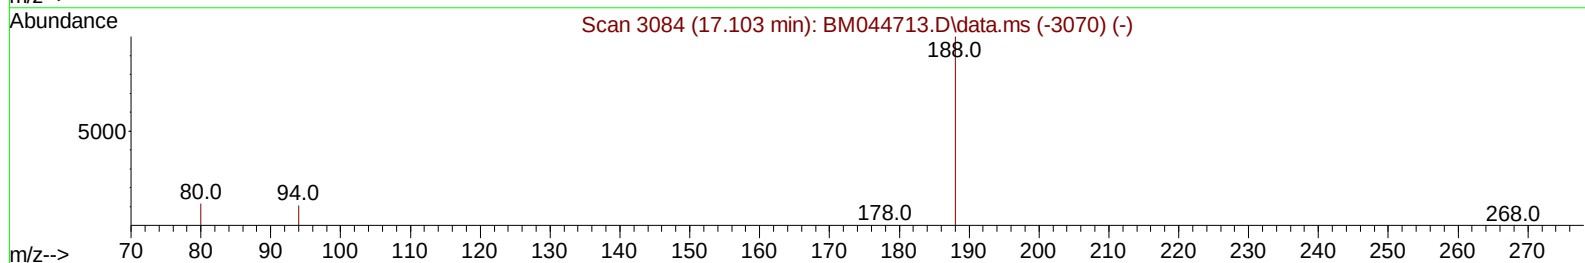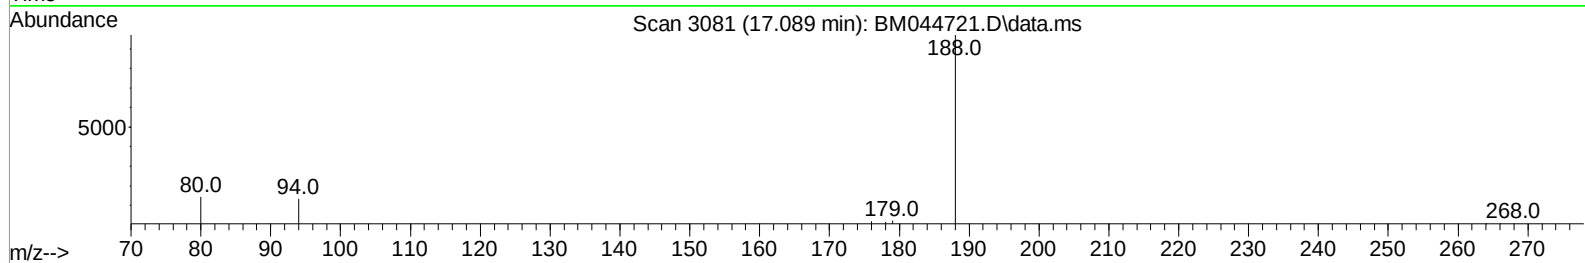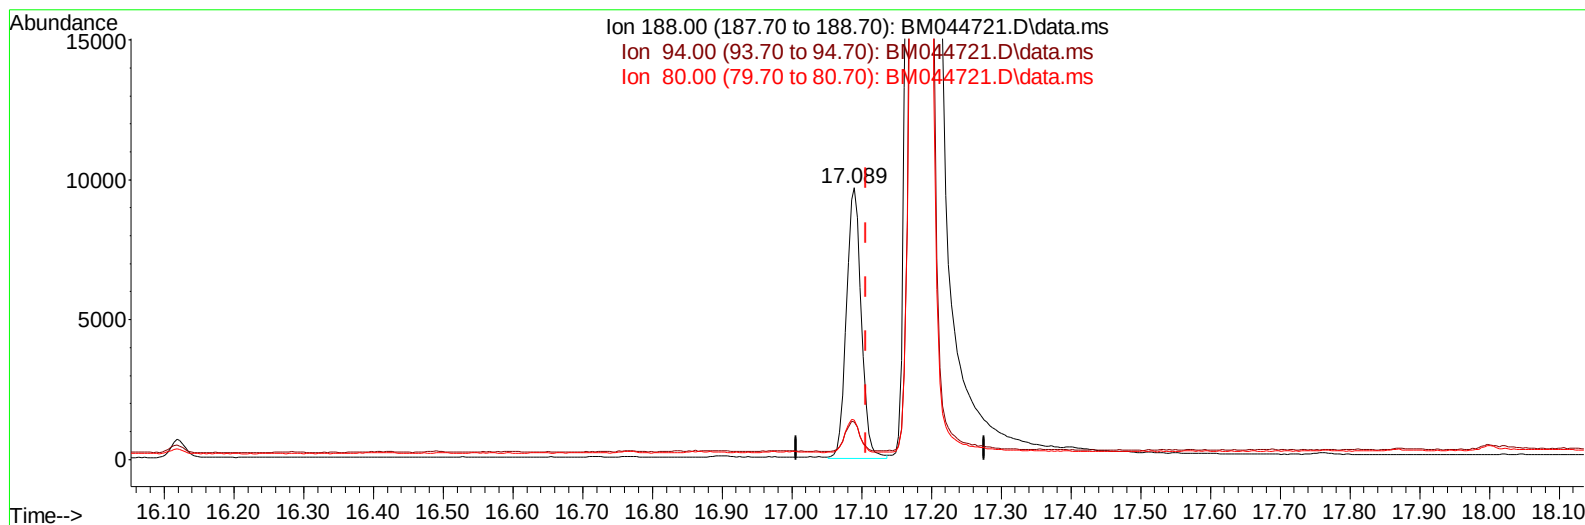

TIC: BM044721.D\data.ms

(13) Phenanthrene-d10 (I)




17.089min (-0.017) 0.40 ng/ul m

response 14291

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	13.73
80.00	12.90	14.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

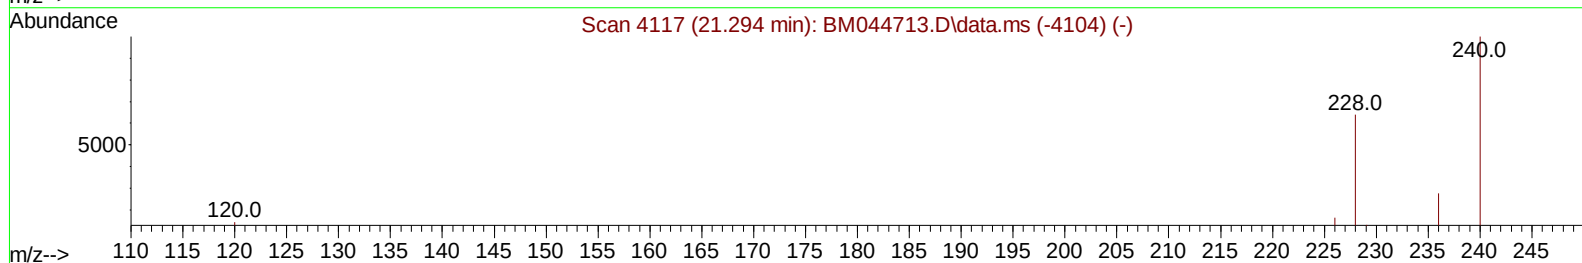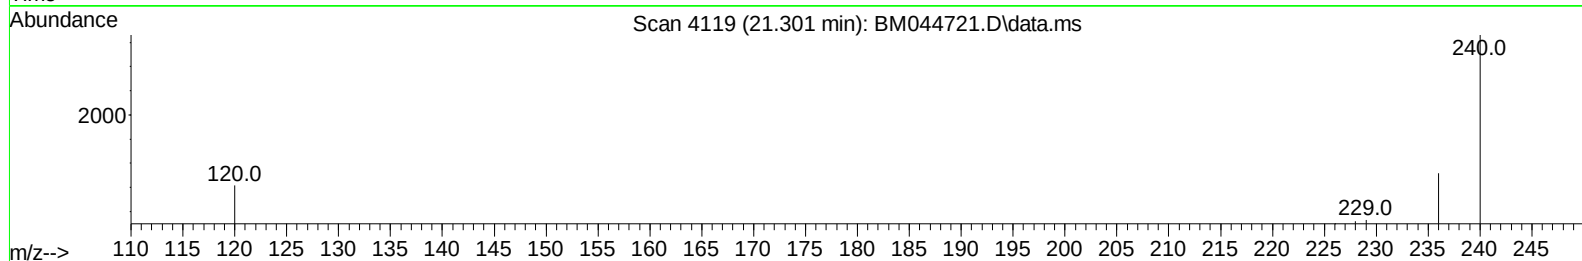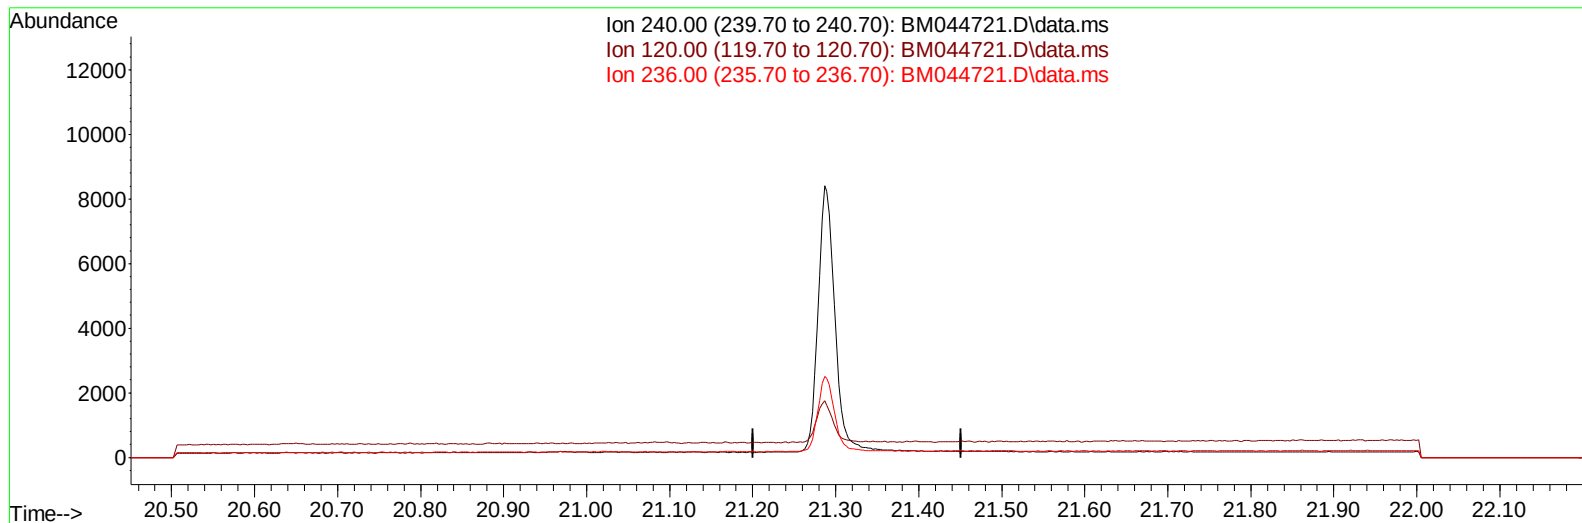

TIC: BM044721.D\data.ms

(17) Chrysene-d12




21.301min (-21.301) 0.00 ng/ul

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.10	0.00#
236.00	28.90	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

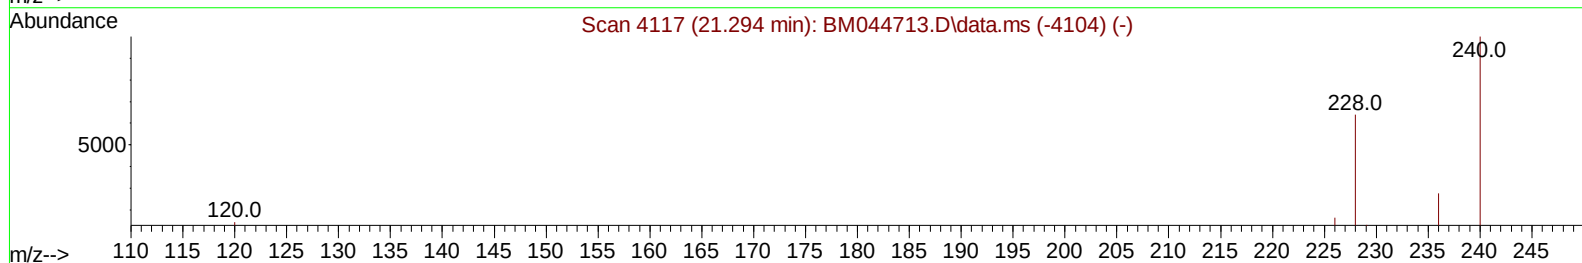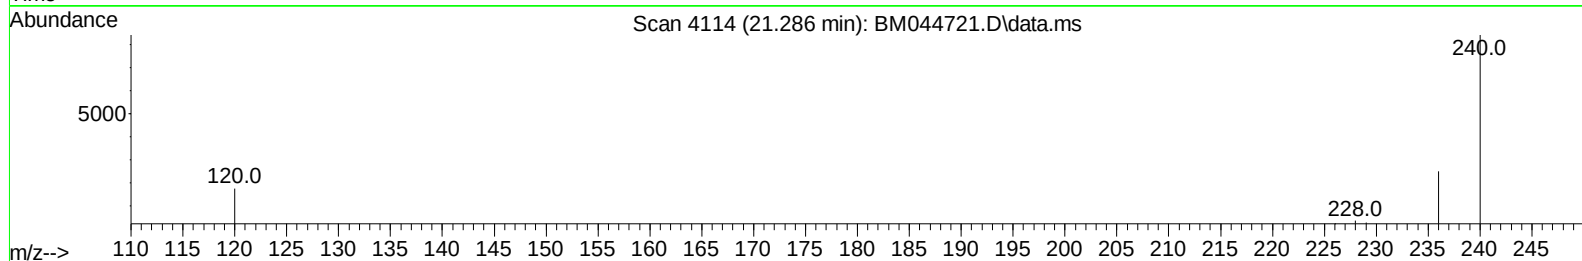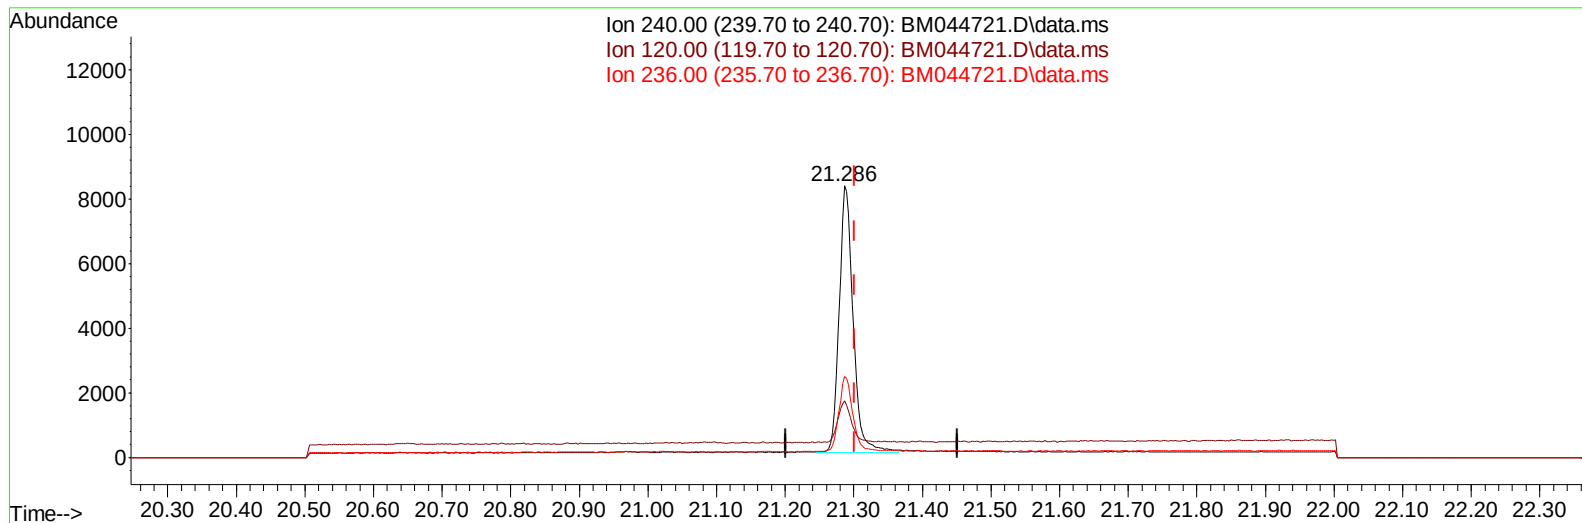

TIC: BM044721.D\data.ms

(17) Chrysene-d12




21.286min (-0.015) 0.40 ng/ul m

response 11672

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.10	20.93#
236.00	28.90	29.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

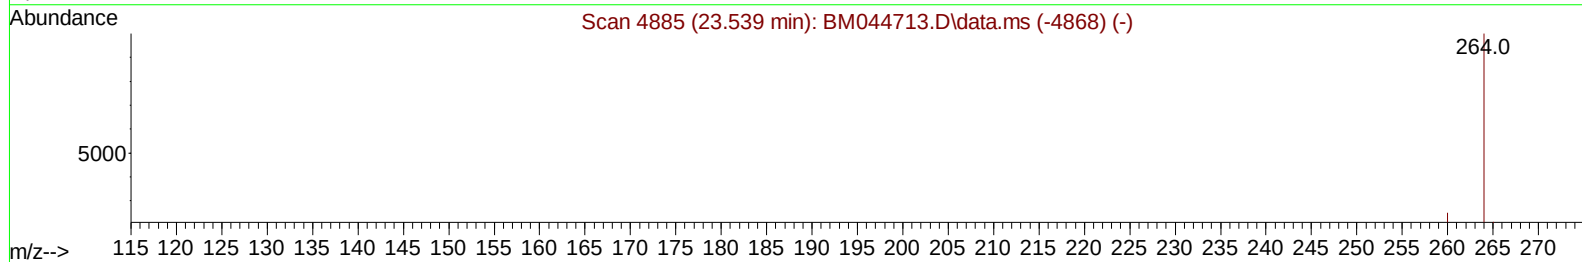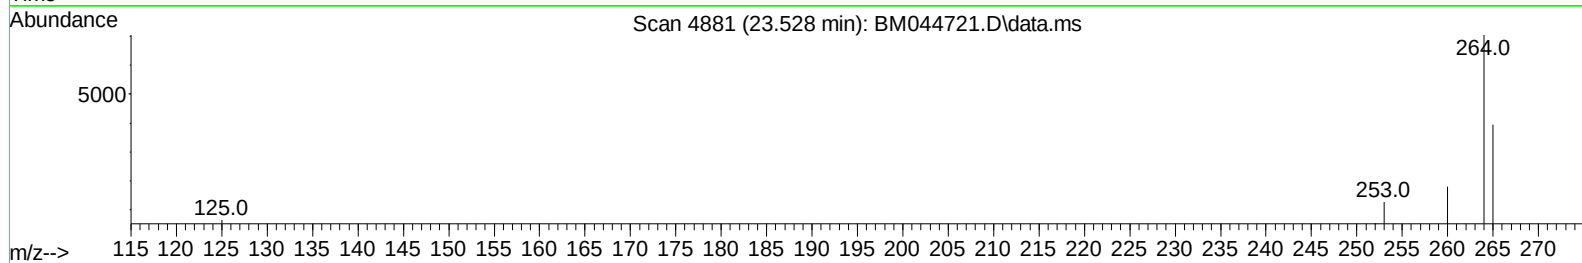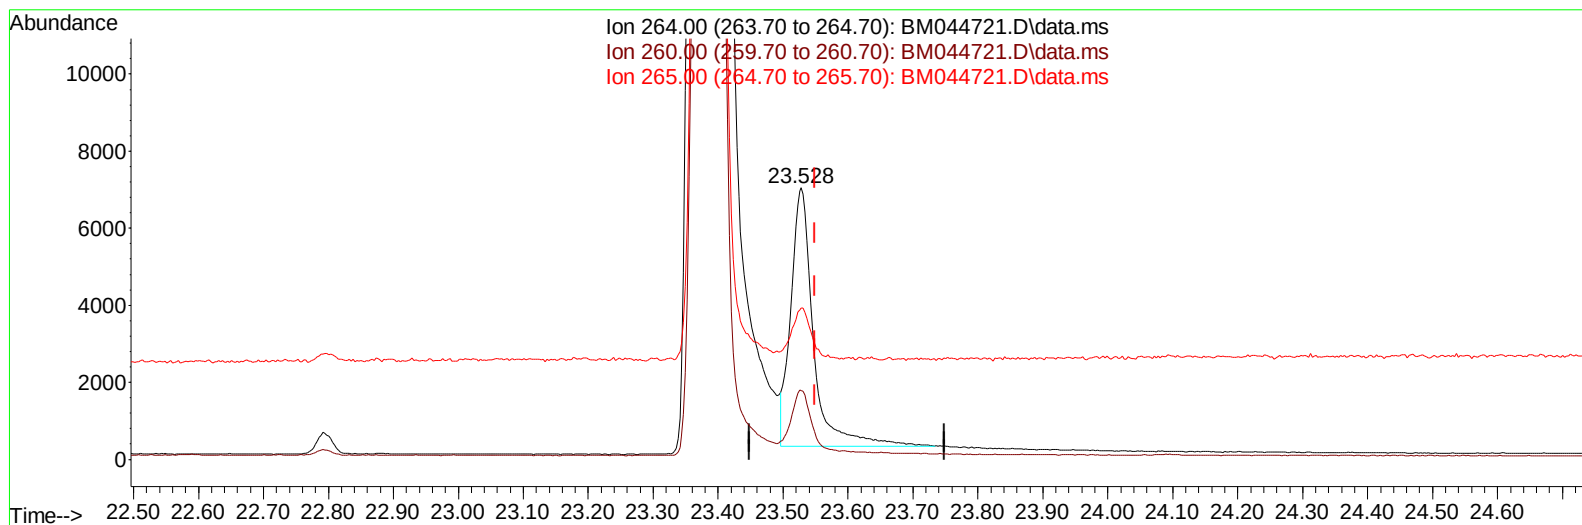

TIC: BM044721.D\data.ms

(23) Perylene-d12 (I)




23.528min (-0.021) 0.40 ng/u1

response 16567

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	25.39
265.00	60.10	55.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

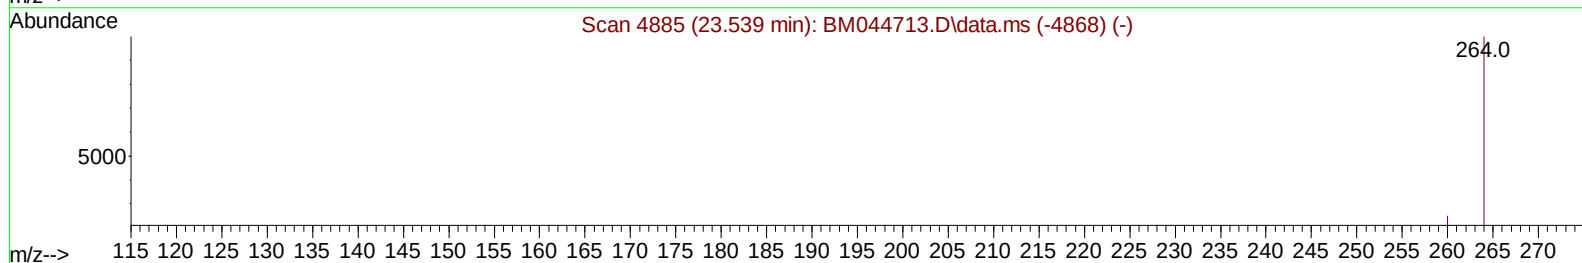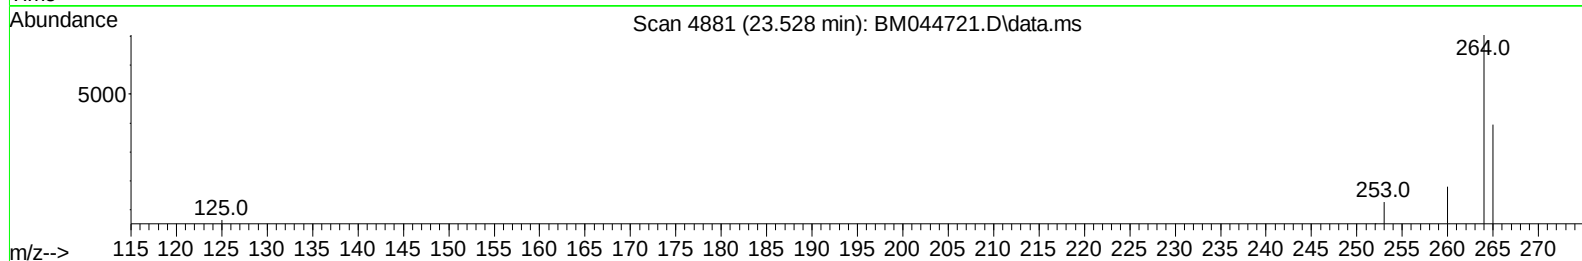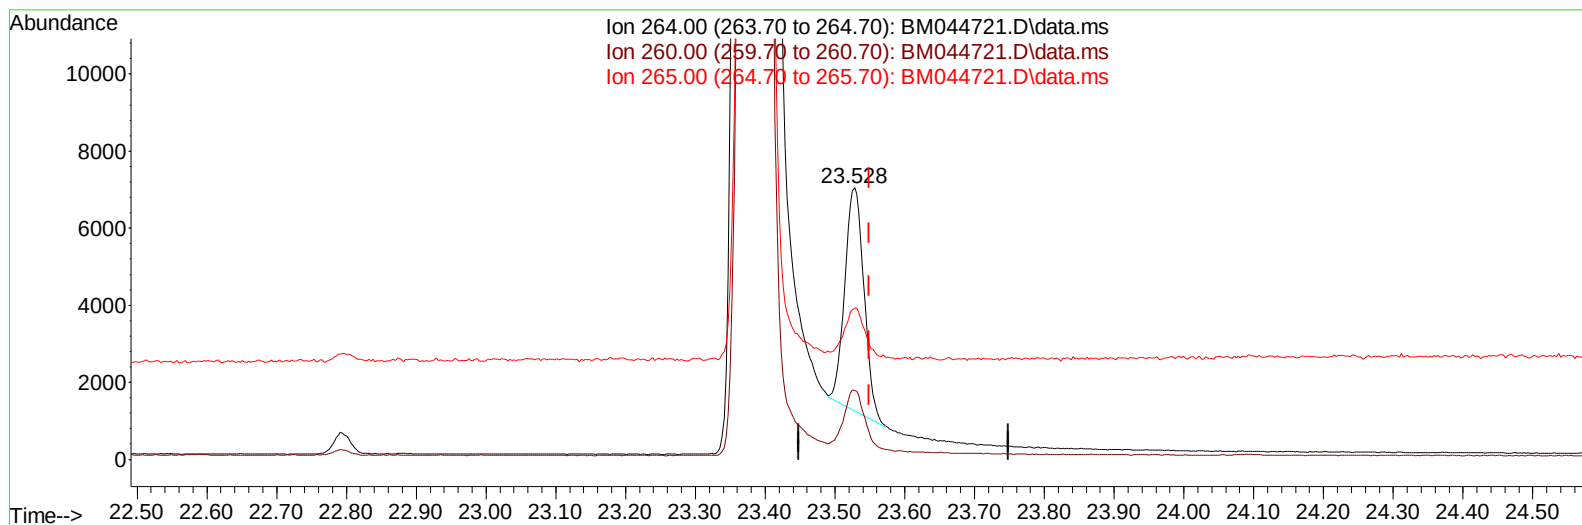

TIC: BM044721.D\data.ms

(23) Perylene-d12 (I)

23.528min (-0.021) 0.40 ng/ul m

response 11053

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	25.39
265.00	60.10	55.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
 Data File : BM044721.D
 Acq On : 22 Mar 2024 04:57
 Operator : MA/JU
 Sample : P1813-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 20 10:51:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.694	152	4600	0.400	ng/ul	0.00
4) Naphthalene-d8	10.468	136	14290	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.334	164	6683	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.089	188	14291m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.286	240	11672m	0.400	ng/ul	-0.01
23) Perylene-d12	23.528	264	11053m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	25071	4.158	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.068	152	5607	0.273	ng/ul	-0.01
18) Fluoranthene-d10	19.126	212	12313	0.301	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.293	88	851	0.138	ng/ul#	Qvalue 51

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044721.D
Acq On : 22 Mar 2024 04:57
Operator : MA/JU
Sample : P1813-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 28 01:18:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

