
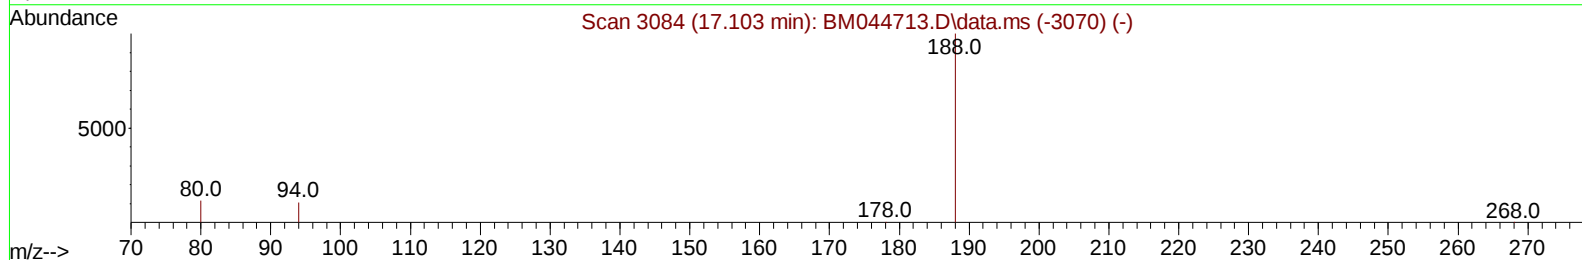
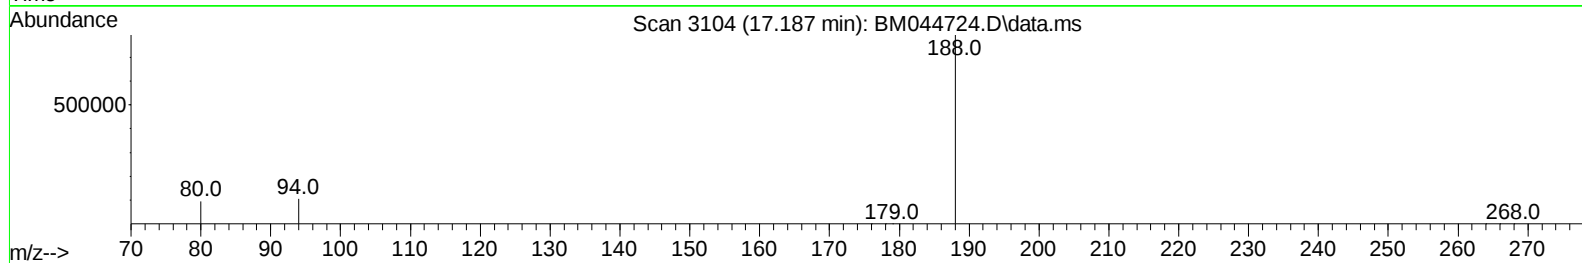


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

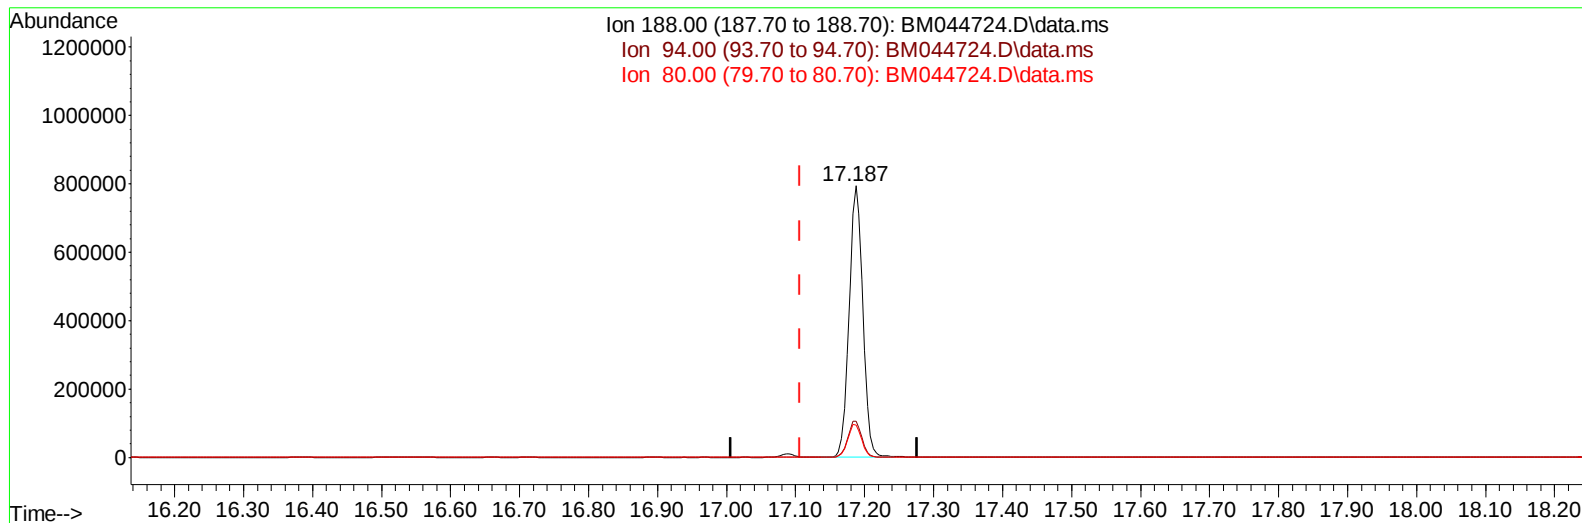

TIC: BM044724.D\data.ms

(13) Phenanthrene-d10 (I)




17.187min (+ 0.081) 0.40 ng/ul

response 1103457

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	13.38
80.00	12.90	11.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

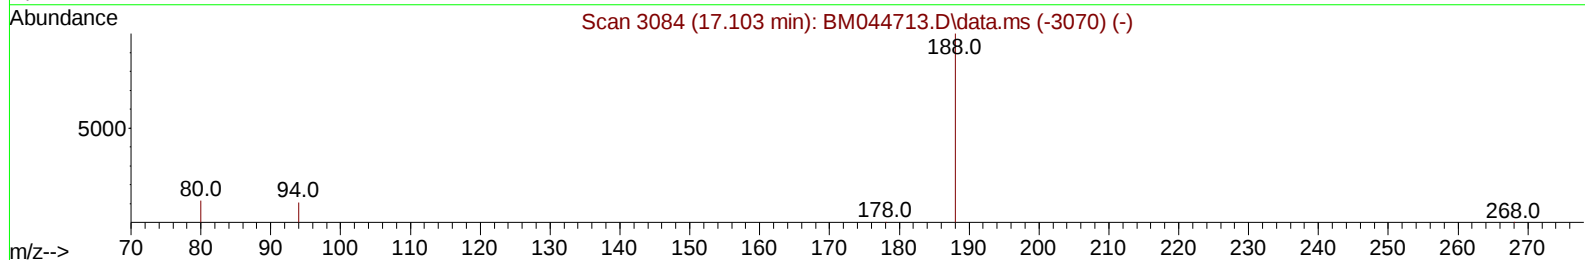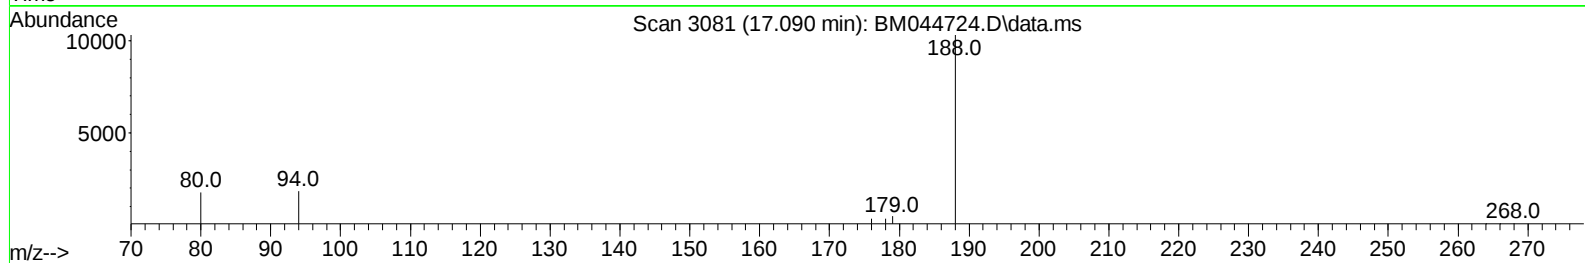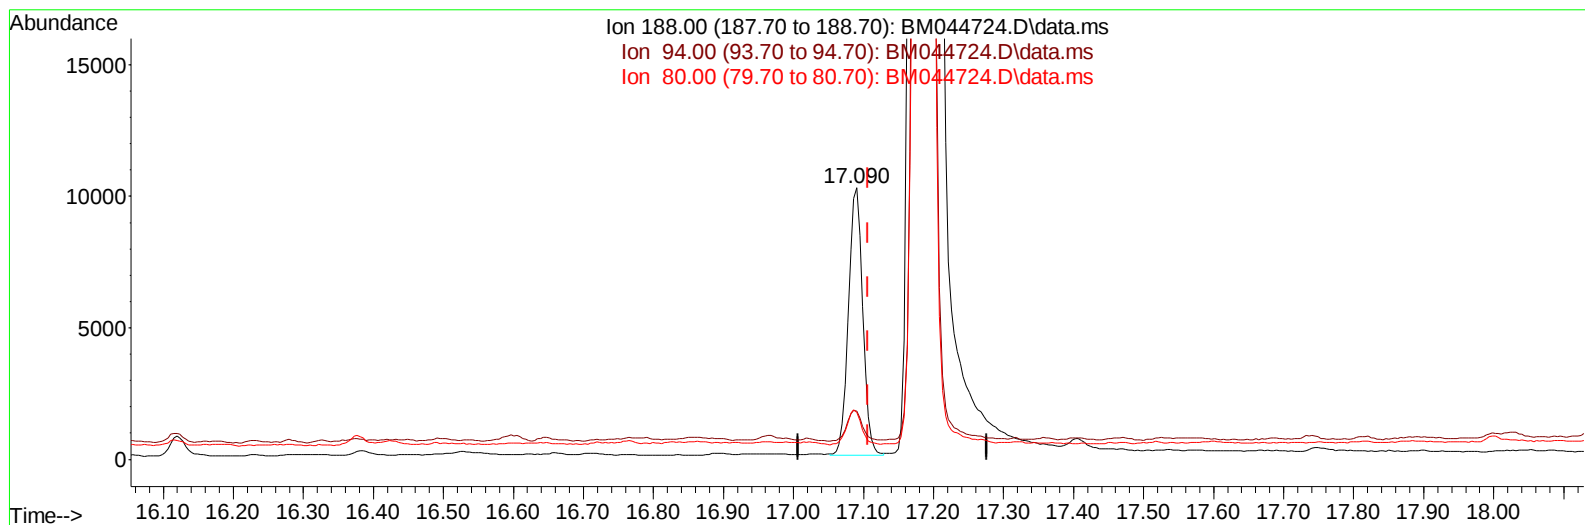

TIC: BM044724.D\data.ms

(13) Phenanthrene-d10 (I)




17.090min (-0.016) 0.40 ng/ul m

response 14447

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	17.80#
80.00	12.90	17.28#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

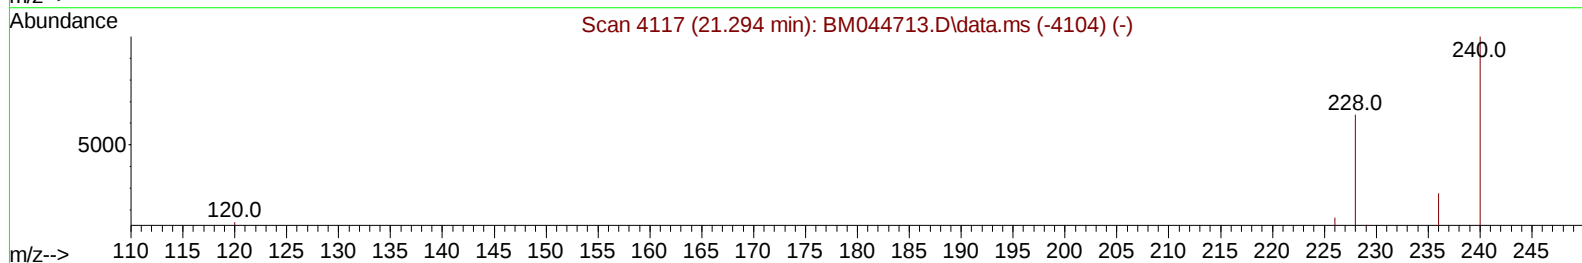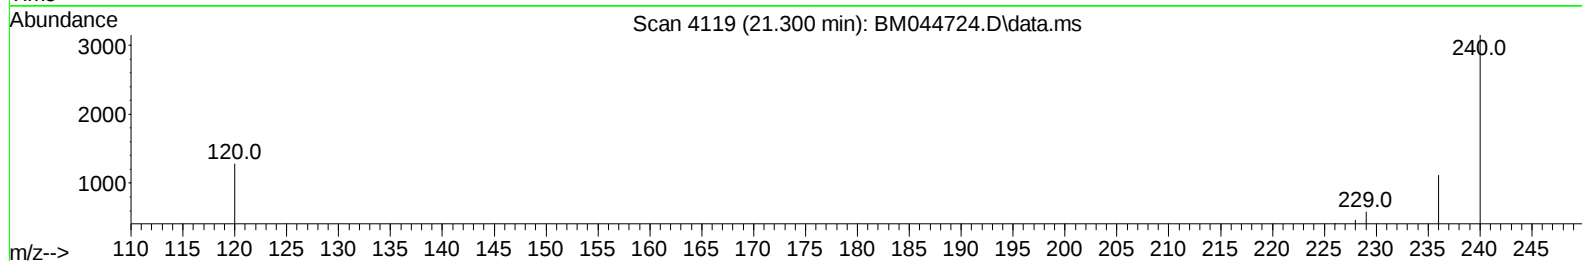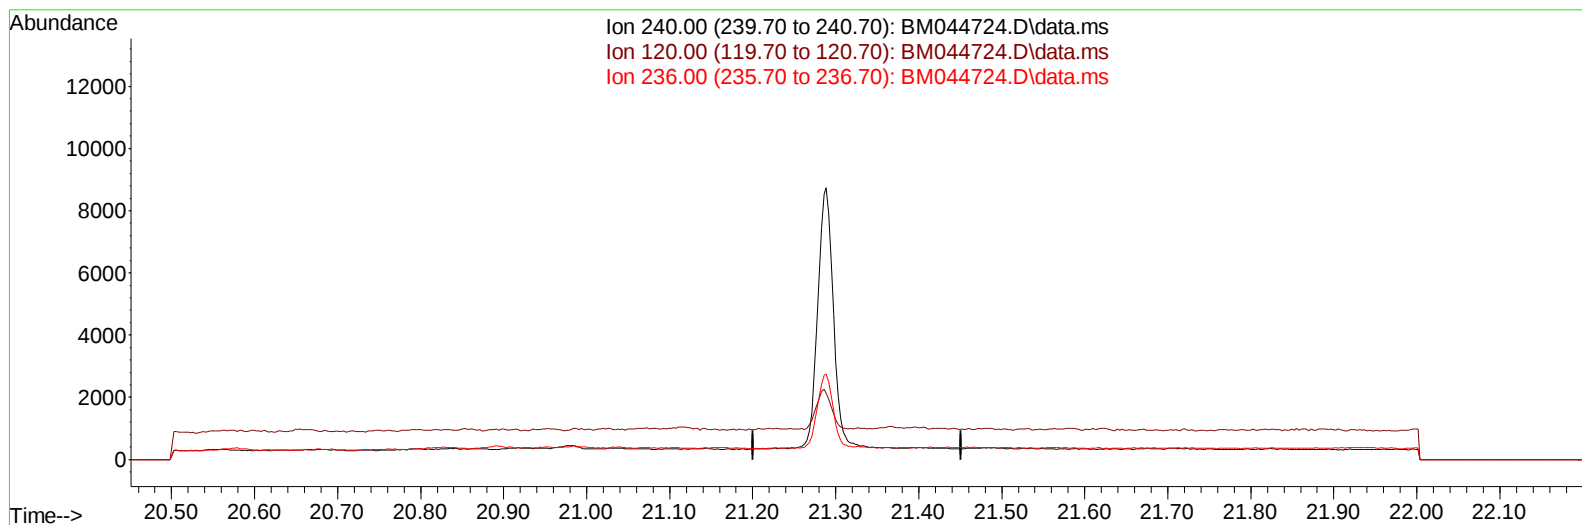

TIC: BM044724.D\data.ms

(17) Chrysene-d12




21.301min (-21.301) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.10	0.00#
236.00	28.90	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

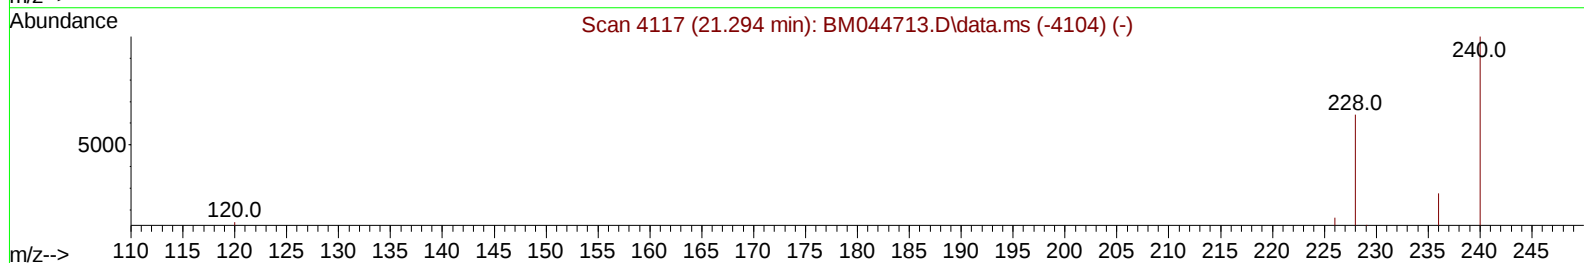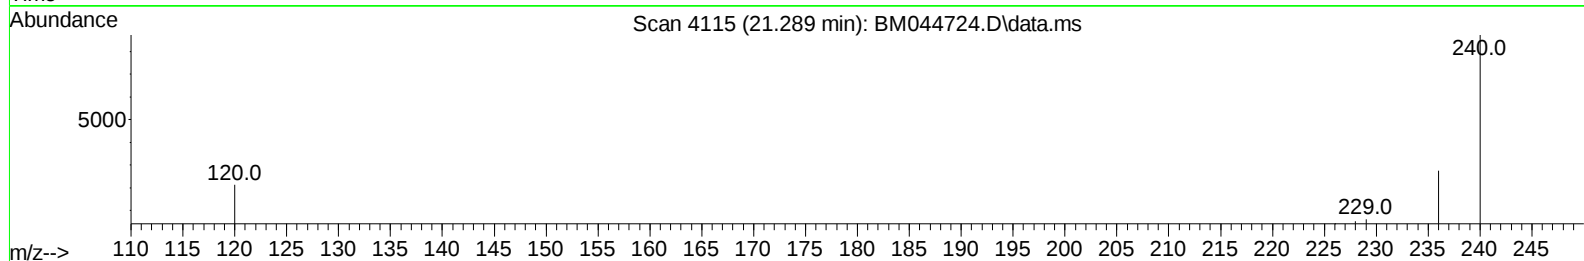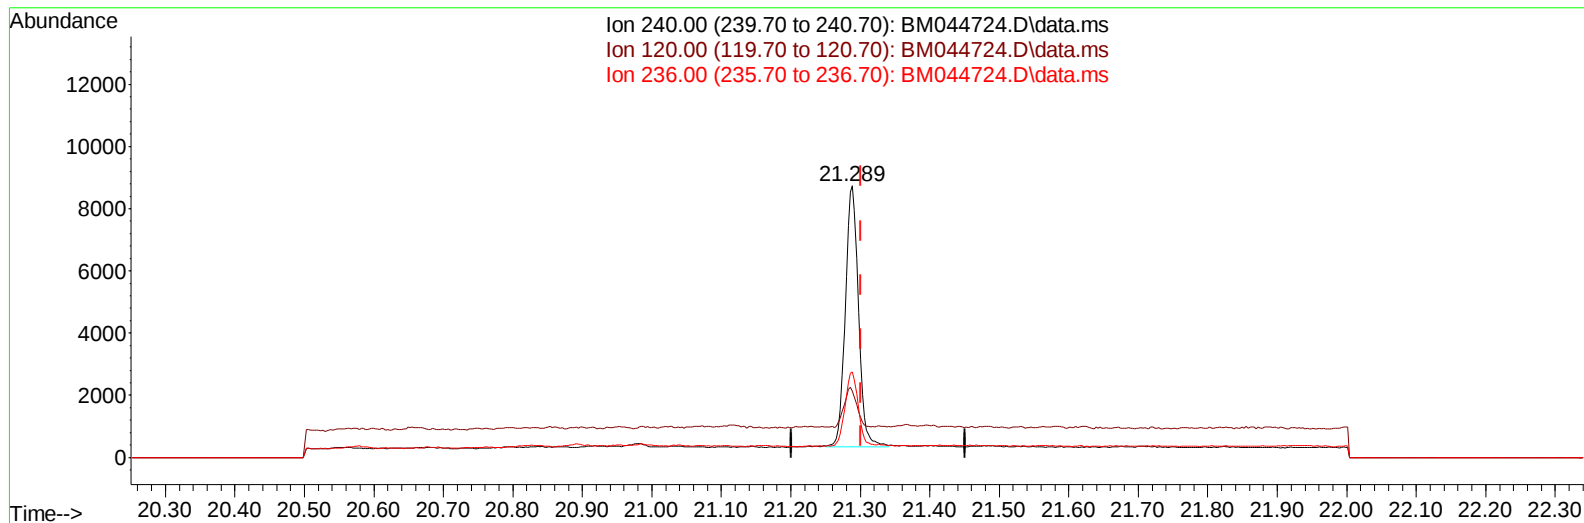

TIC: BM044724.D\data.ms

(17) Chrysene-d12




21.289min (-0.013) 0.40 ng/ul m

response 11041

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.10	24.51#
236.00	28.90	31.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

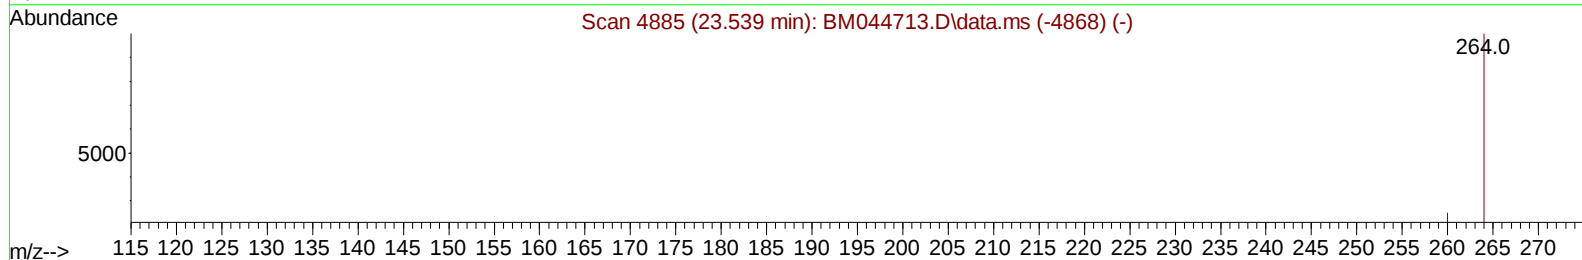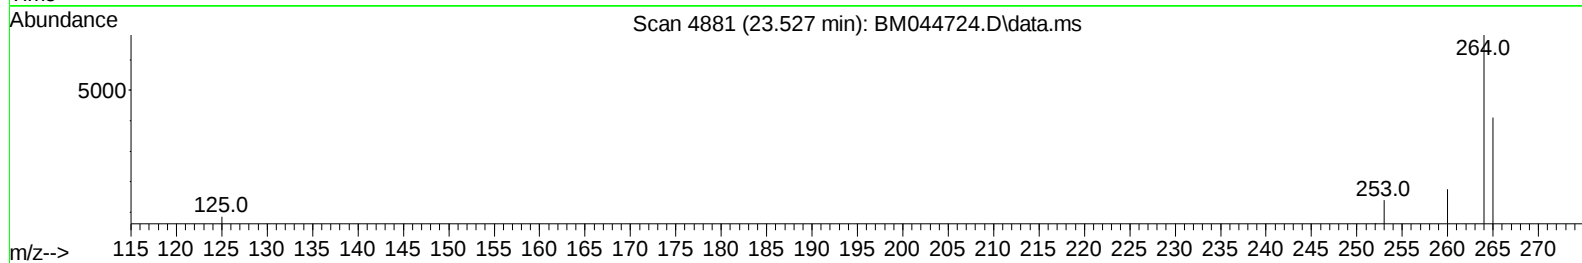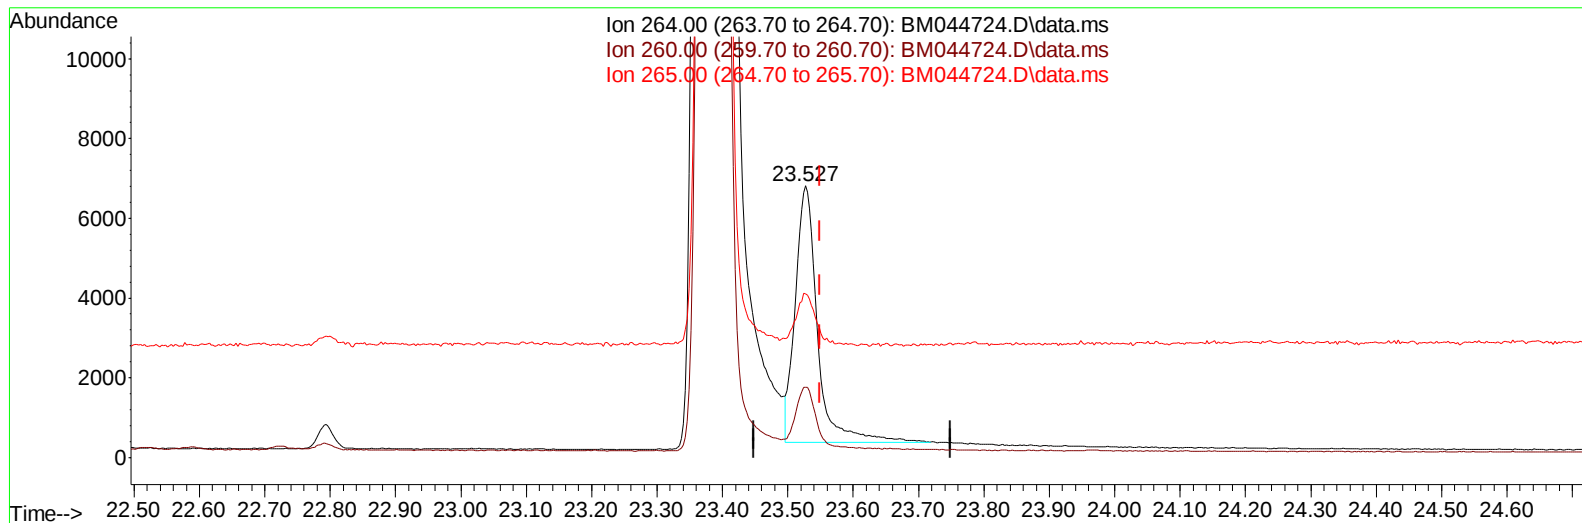

TIC: BM044724.D\data.ms

(23) Perylene-d12 (I)




23.527min (-0.021) 0.40 ng/u1

response 15150

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	25.82
265.00	60.10	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

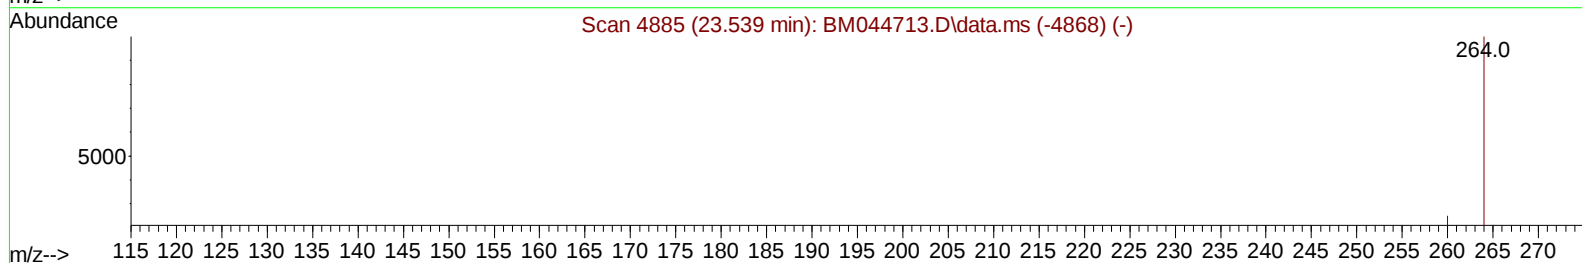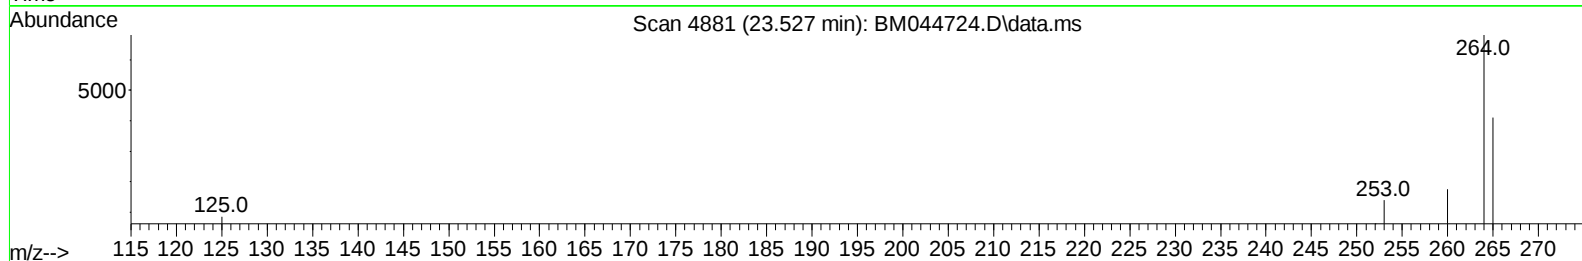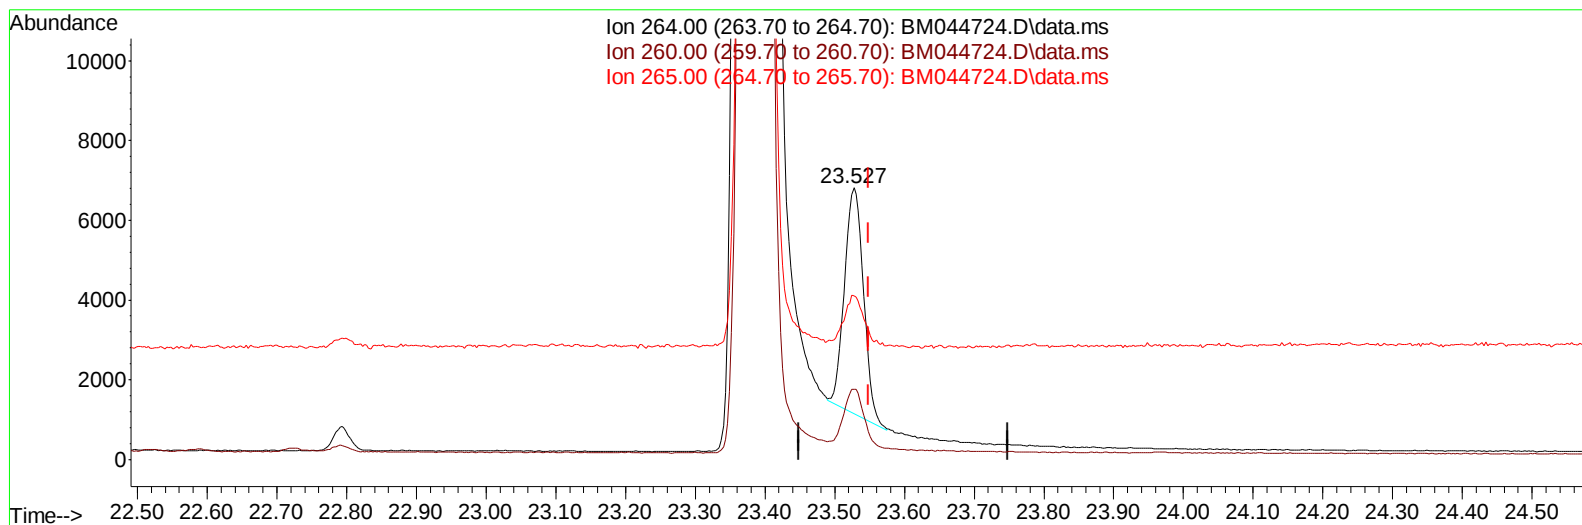

TIC: BM044724.D\data.ms

(23) Perylene-d12 (I)

23.527min (-0.021) 0.40 ng/ul m

response 10726

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	25.82
265.00	60.10	60.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
 Data File : BM044724.D
 Acq On : 22 Mar 2024 06:45
 Operator : MA/JU
 Sample : P1813-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 20 10:51:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.690	152	4393	0.400	ng/ul	0.00
4) Naphthalene-d8	10.468	136	13933	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.331	164	8086	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.090	188	14447m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.289	240	11041m	0.400	ng/ul	-0.01
23) Perylene-d12	23.527	264	10726m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	26238	4.556	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.068	152	7273	0.363	ng/ul	-0.01
18) Fluoranthene-d10	19.123	212	14008	0.361	ng/ul	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.293	88	427	0.073	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

