




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

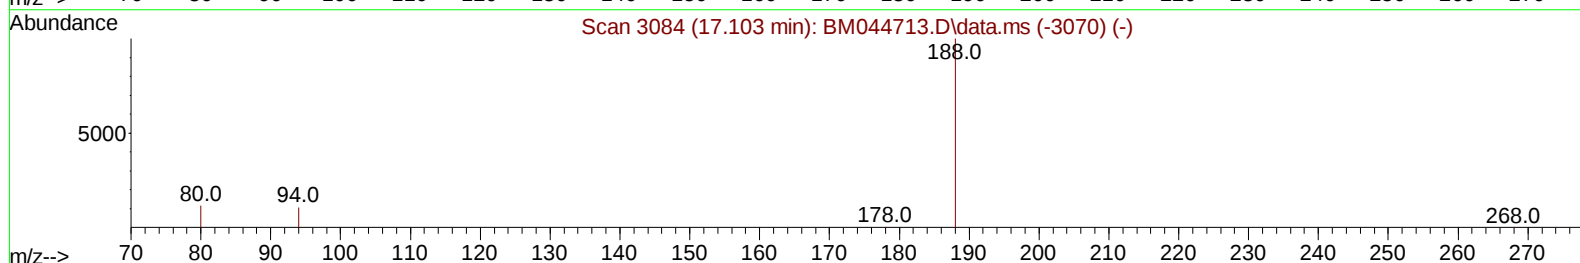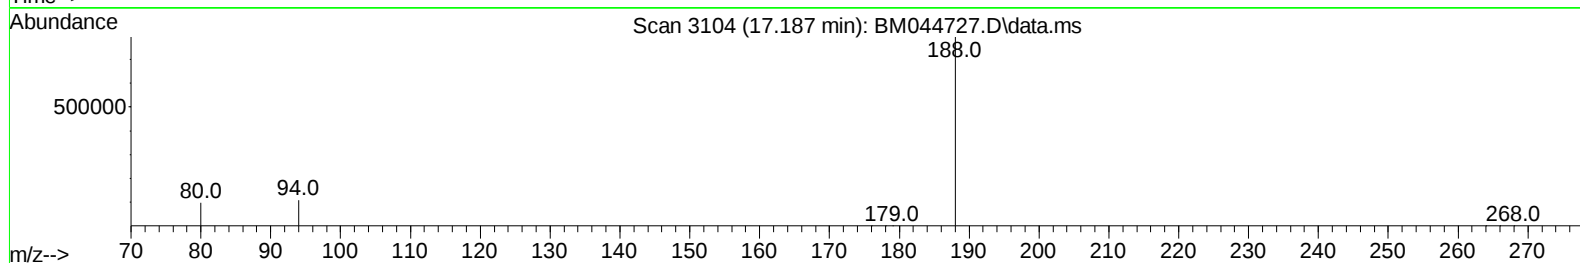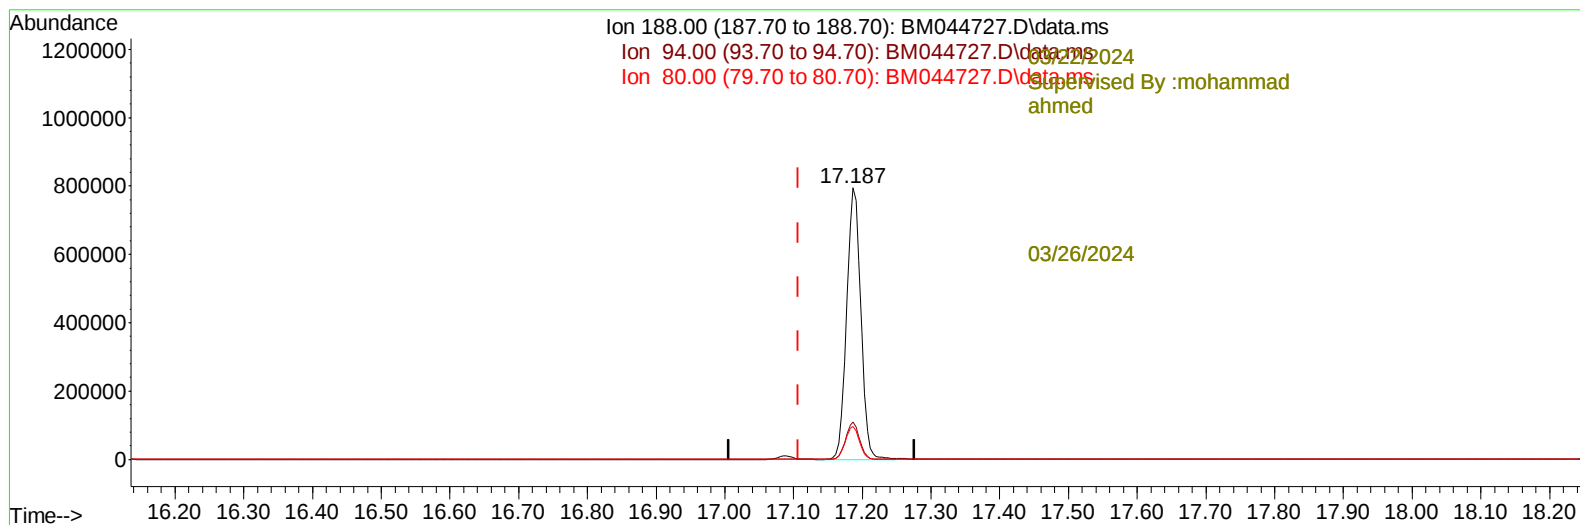

TIC: BM044727.D\data.ms

(13) Phenanthrene-d10 (I)

17.187min (+ 0.080) 0.40 ng/u1

response 1144784

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	13.72
80.00	12.90	12.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

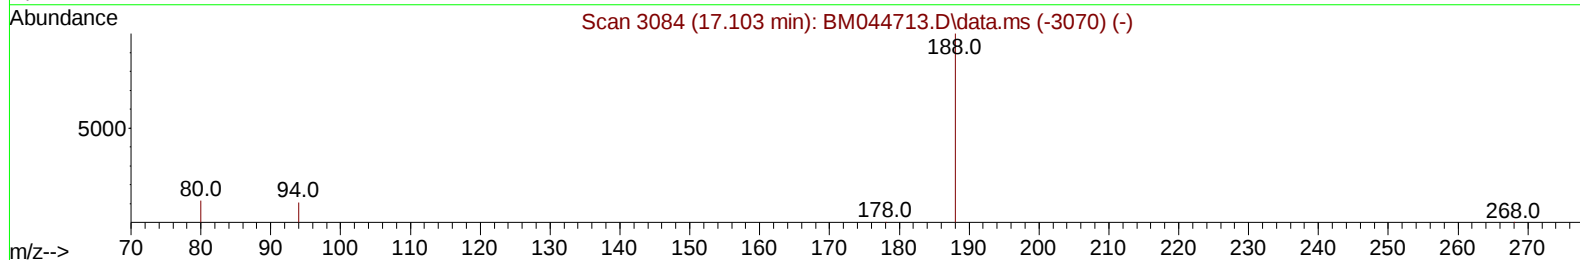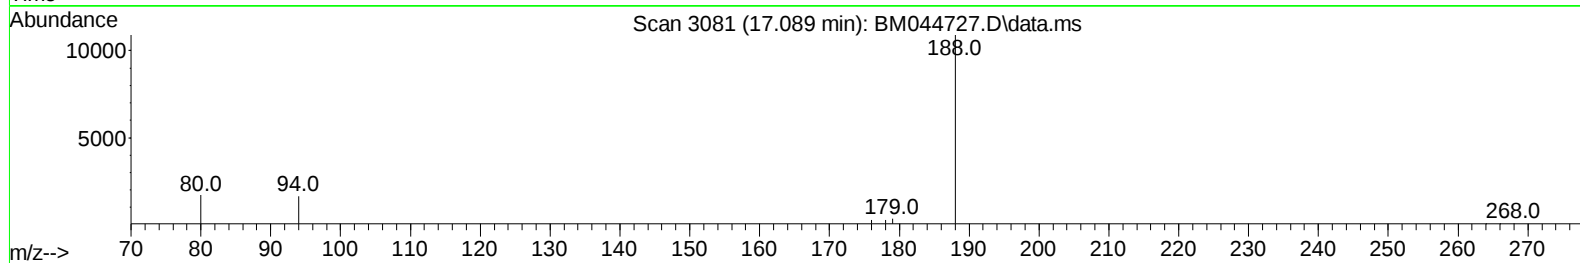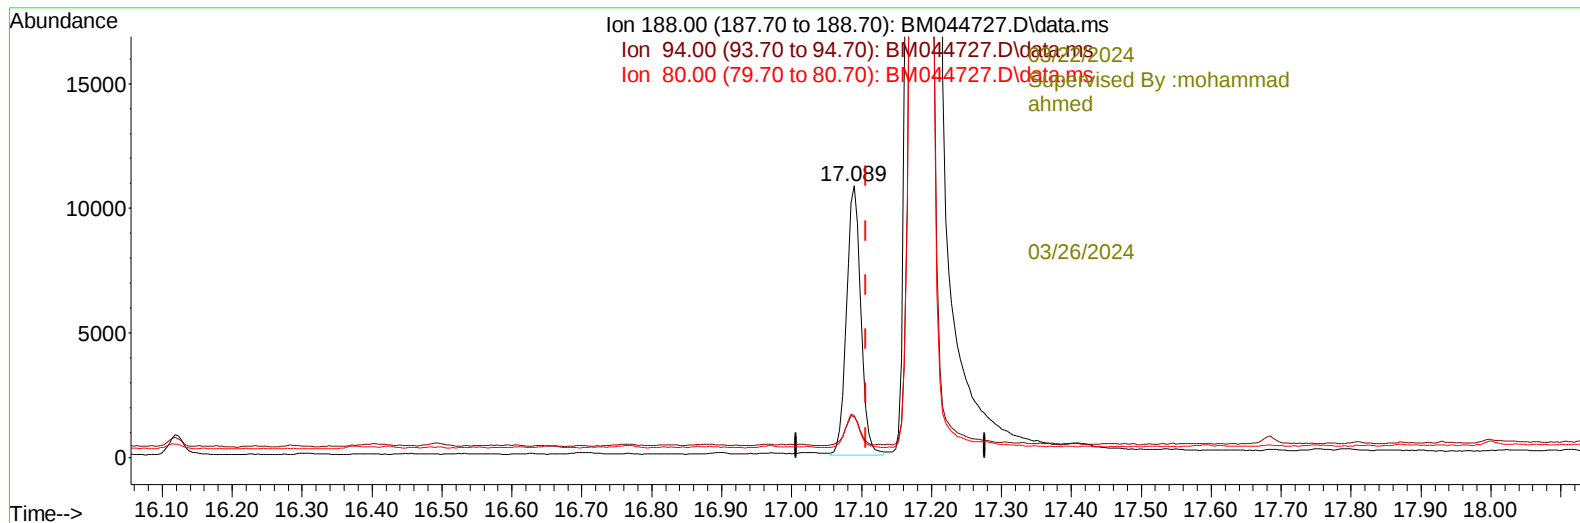

TIC: BM044727.D\data.ms

(13) Phenanthrene-d10 (I)

17.089min (-0.017) 0.40 ng/ul m

response 15341

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.60	15.07#
80.00	12.90	15.56#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

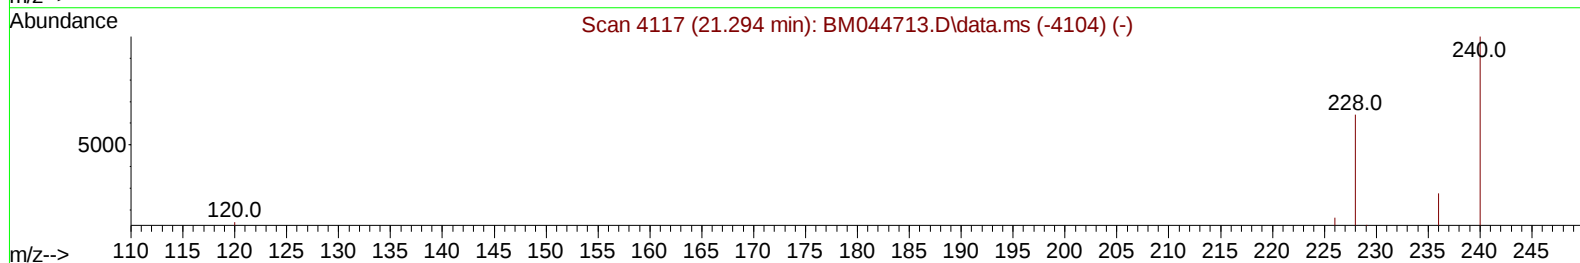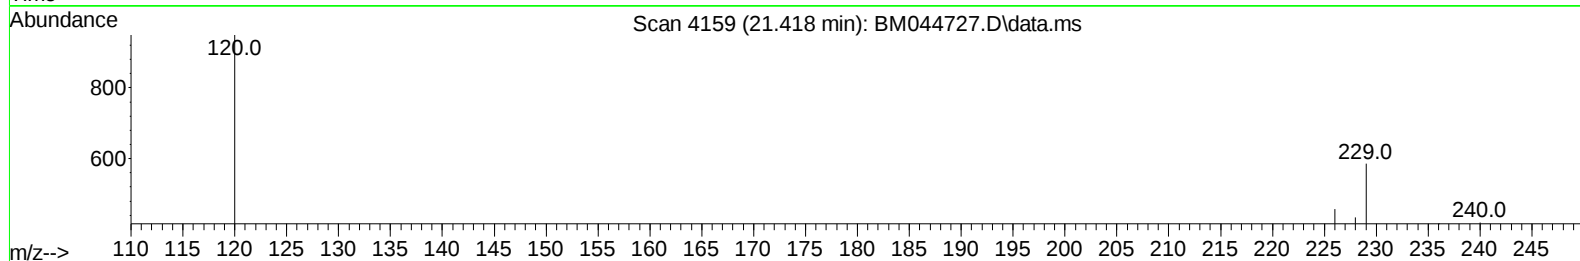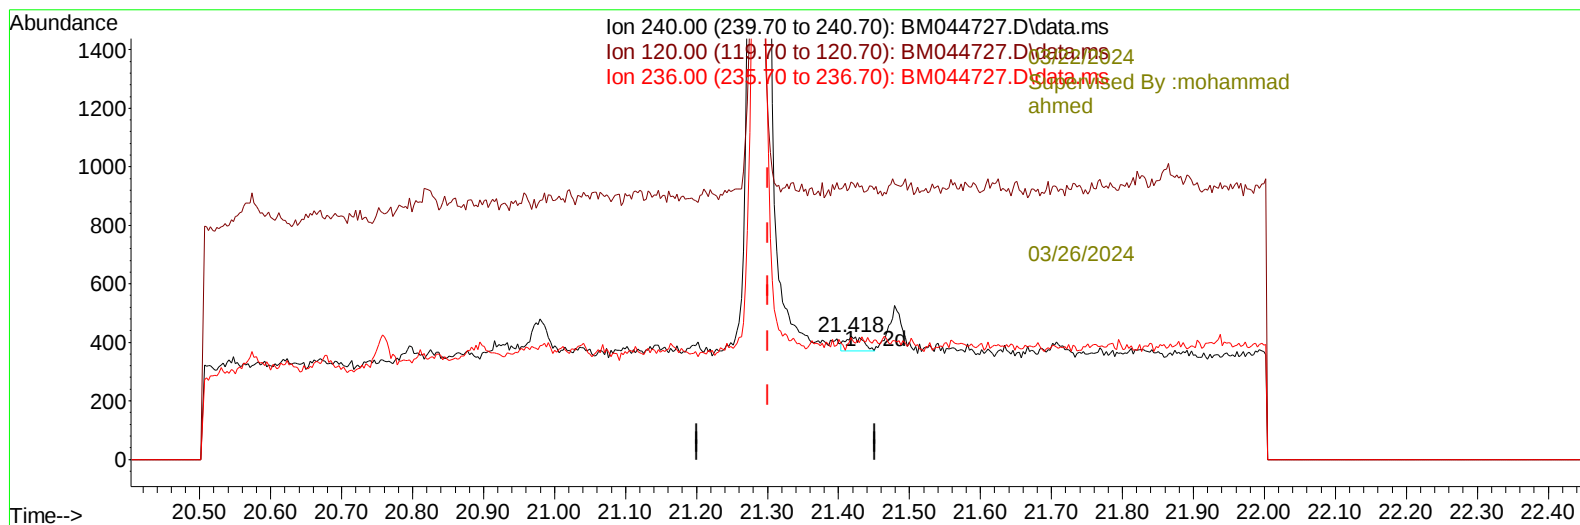

TIC: BM044727.D\data.ms

(17) Chrysene-d12

21.418min (+ 0.117) 0.40 ng/u1

response 84

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.10	225.95#
236.00	28.90	99.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

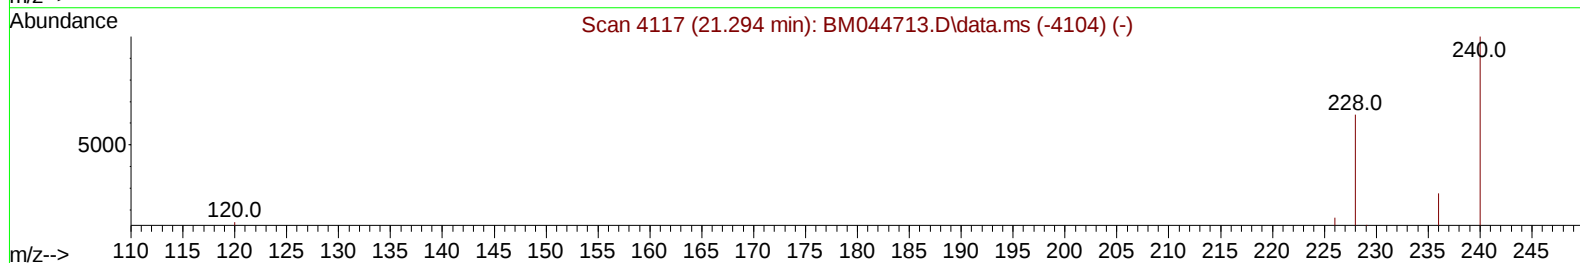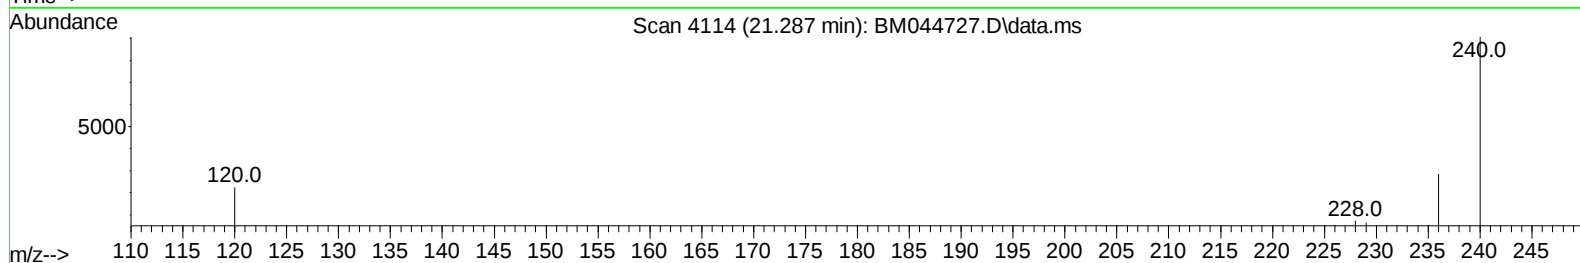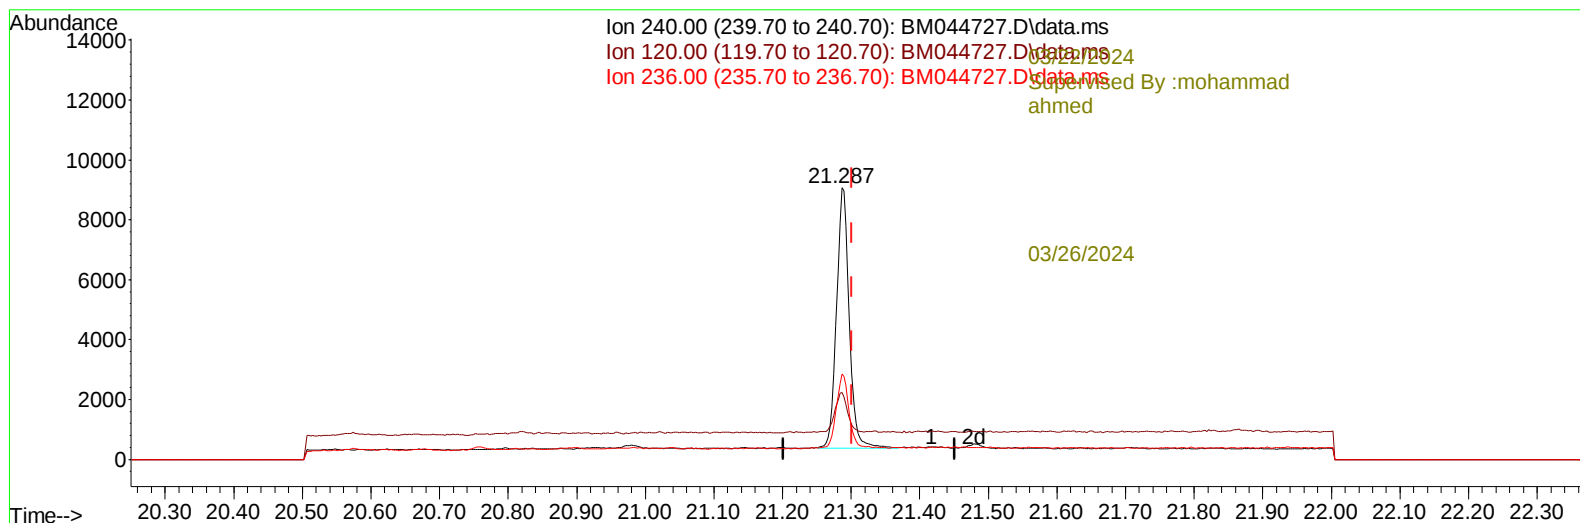

TIC: BM044727.D\data.ms

(17) Chrysene-d12

21.287min (-0.015) 0.40 ng/ul m

response 11217

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.10	24.75#
236.00	28.90	31.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

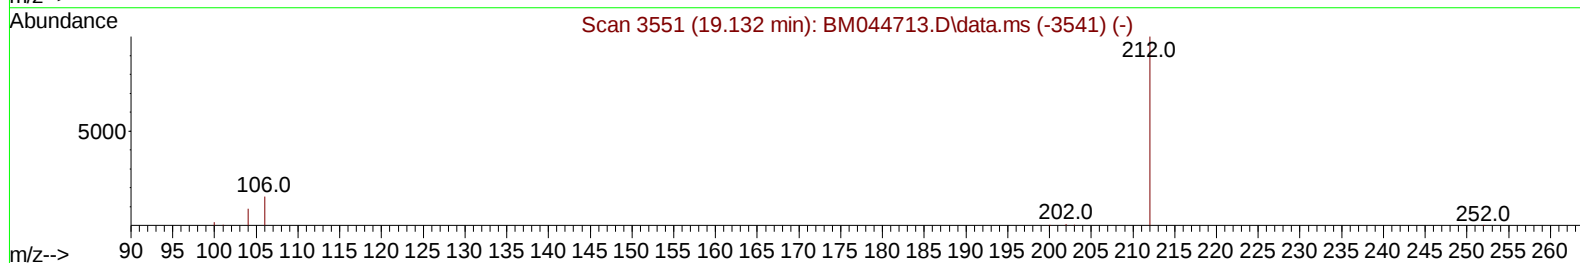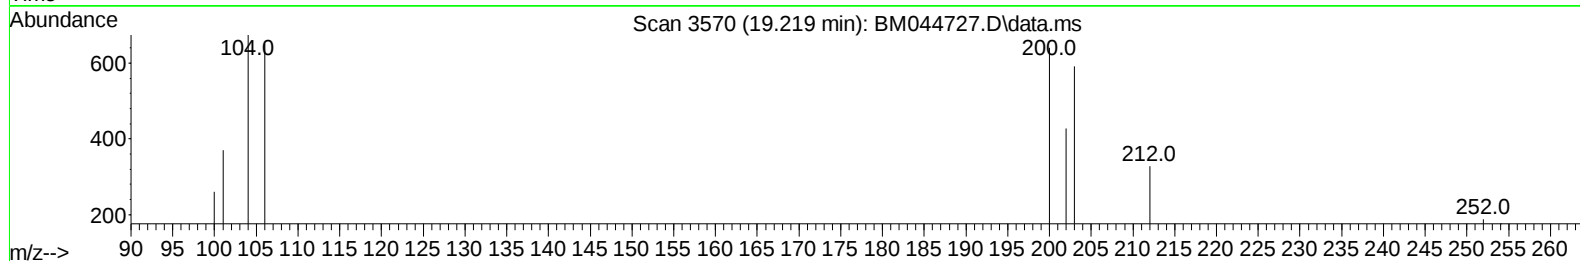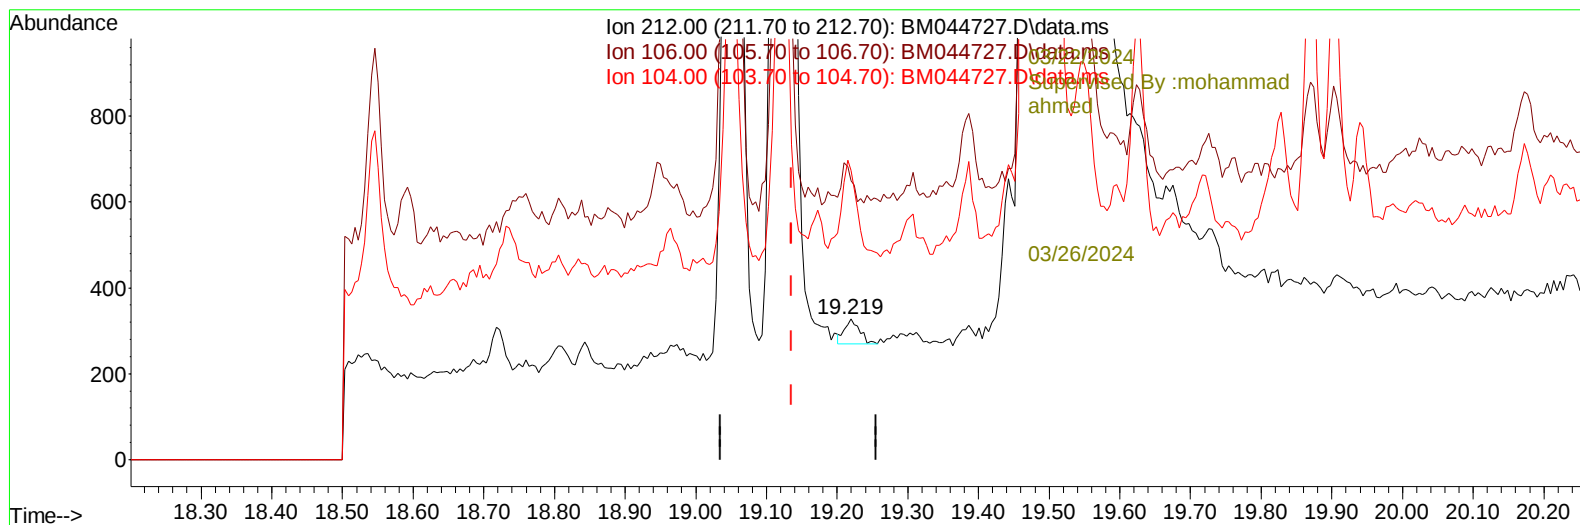

TIC: BM044727.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.219min (+ 0.084) 0.00 ng/u1

response 84

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.80	108.33#
104.00	9.00	414.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

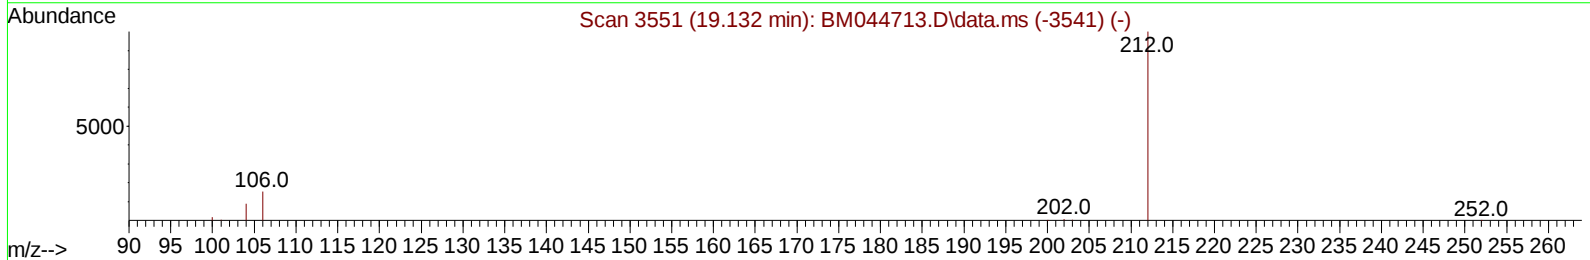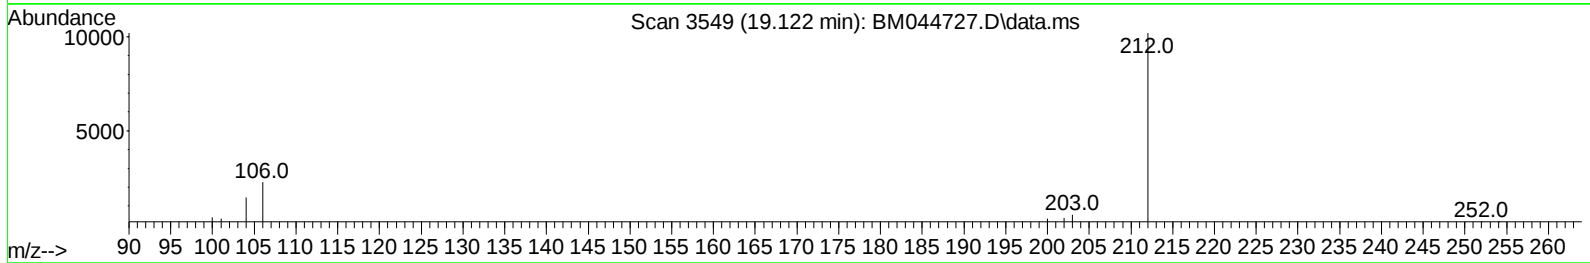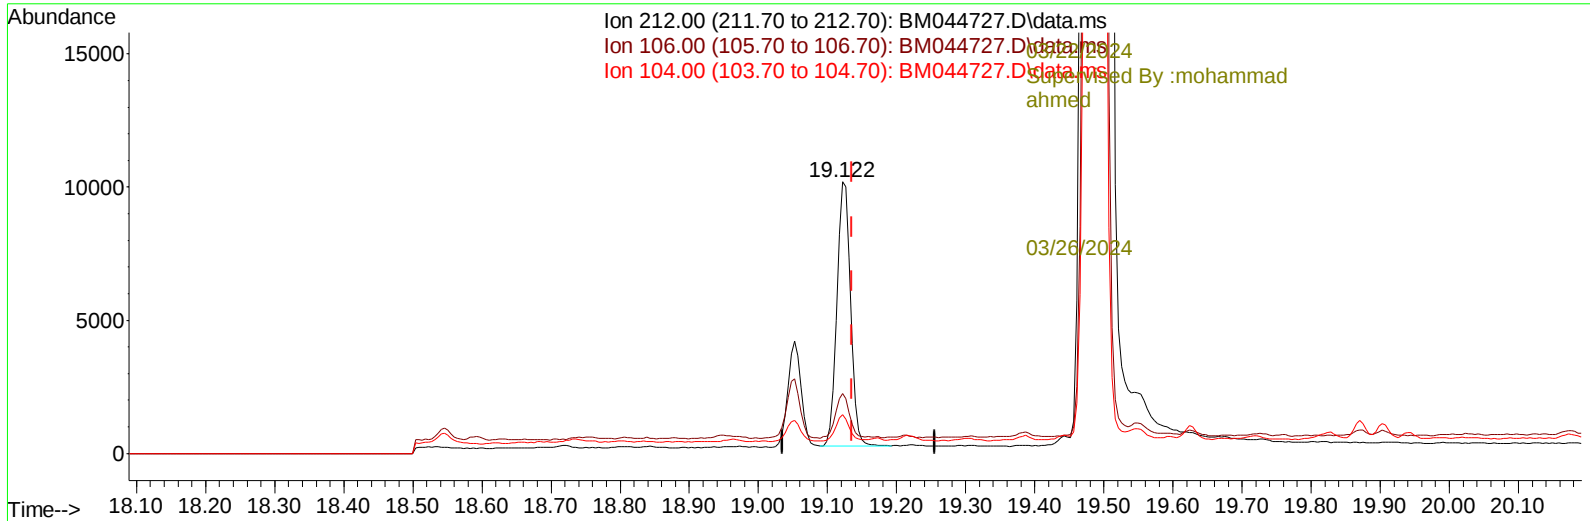

TIC: BM044727.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.122min (-0.014) 0.35 ng/u1 m

response 13756

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.80	0.66#
104.00	9.00	2.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

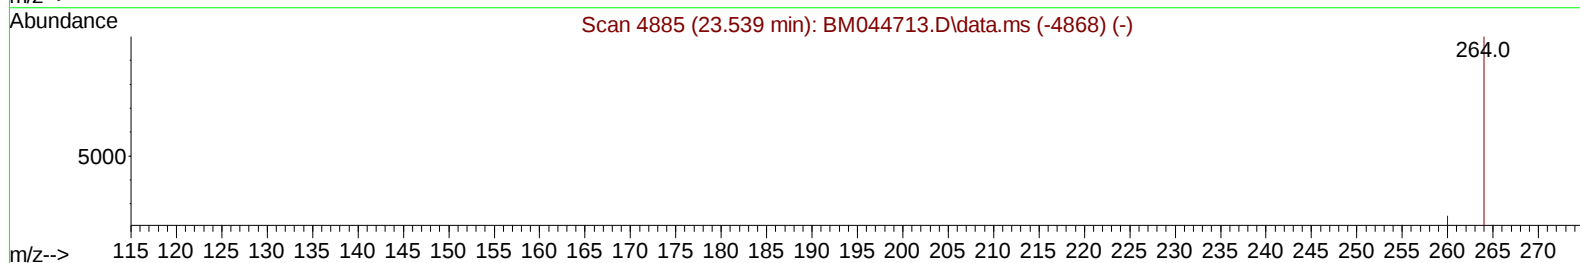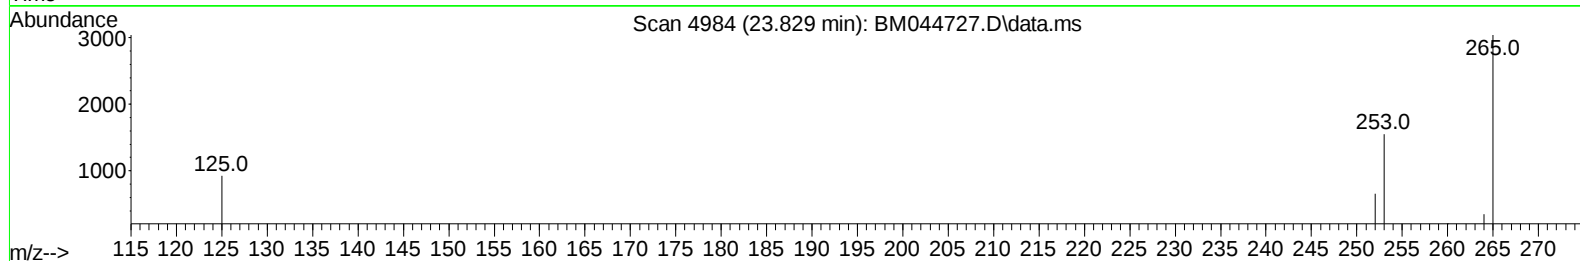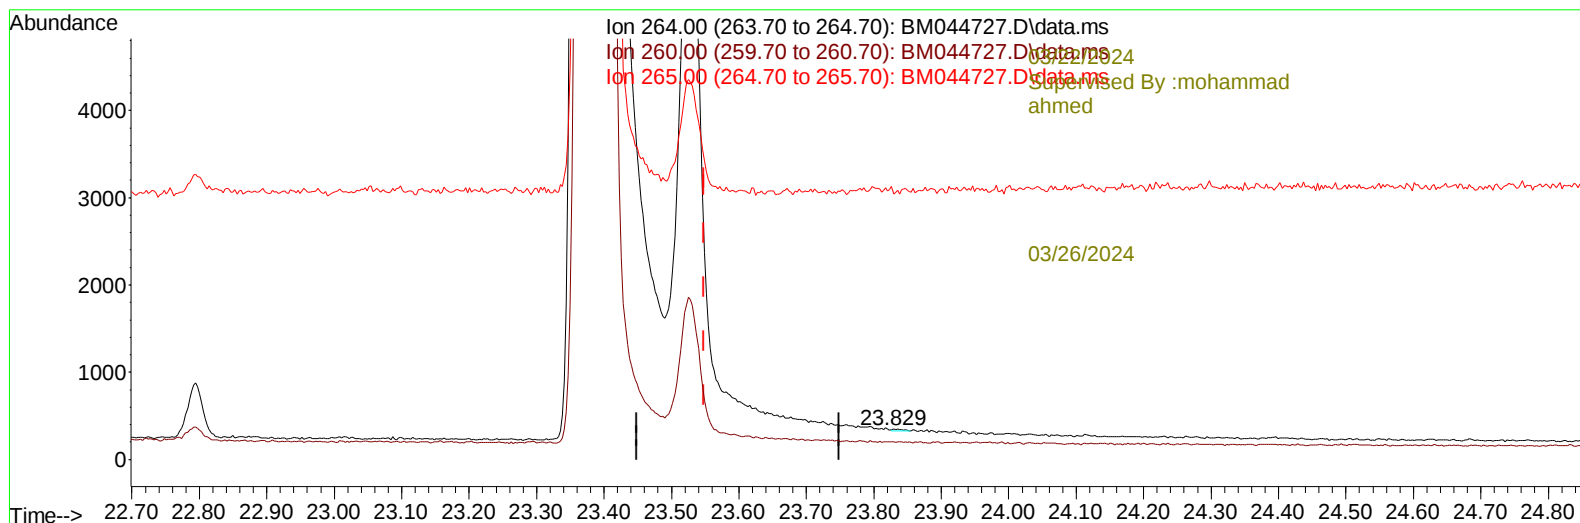

TIC: BM044727.D\data.ms

(23) Perylene-d12 (I)

23.829min (+ 0.281) 0.40 ng/u1

response 22

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	58.67#
265.00	60.10	878.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

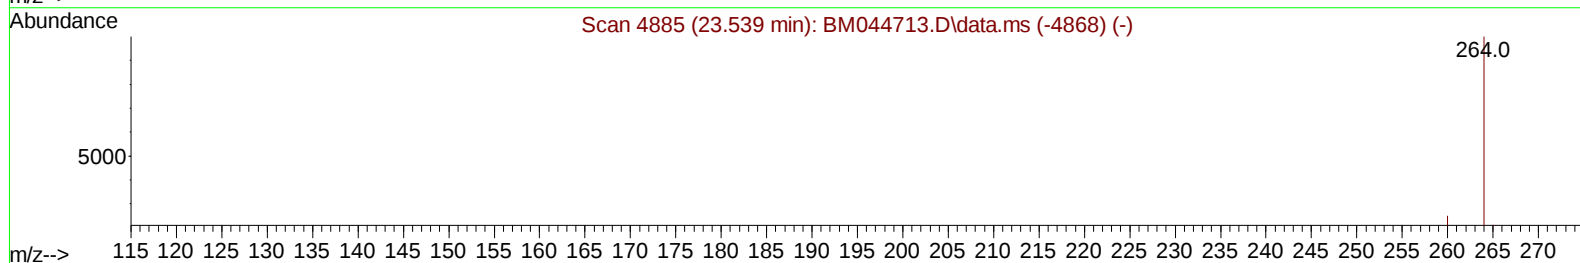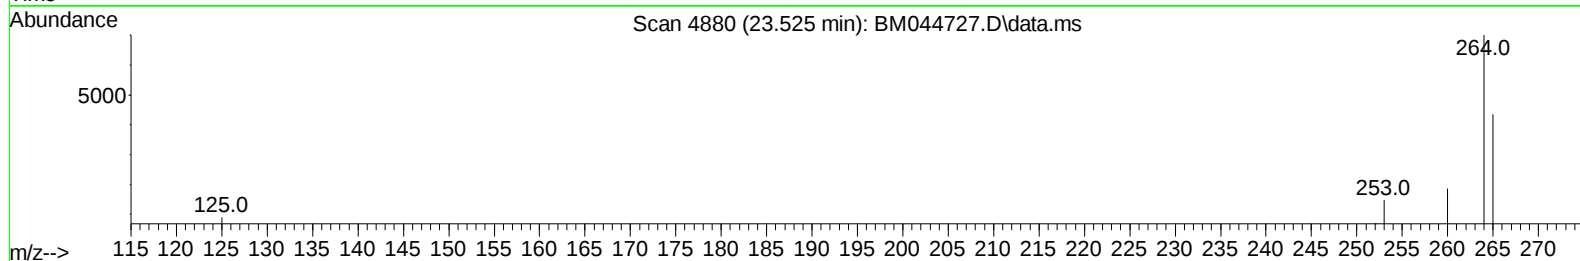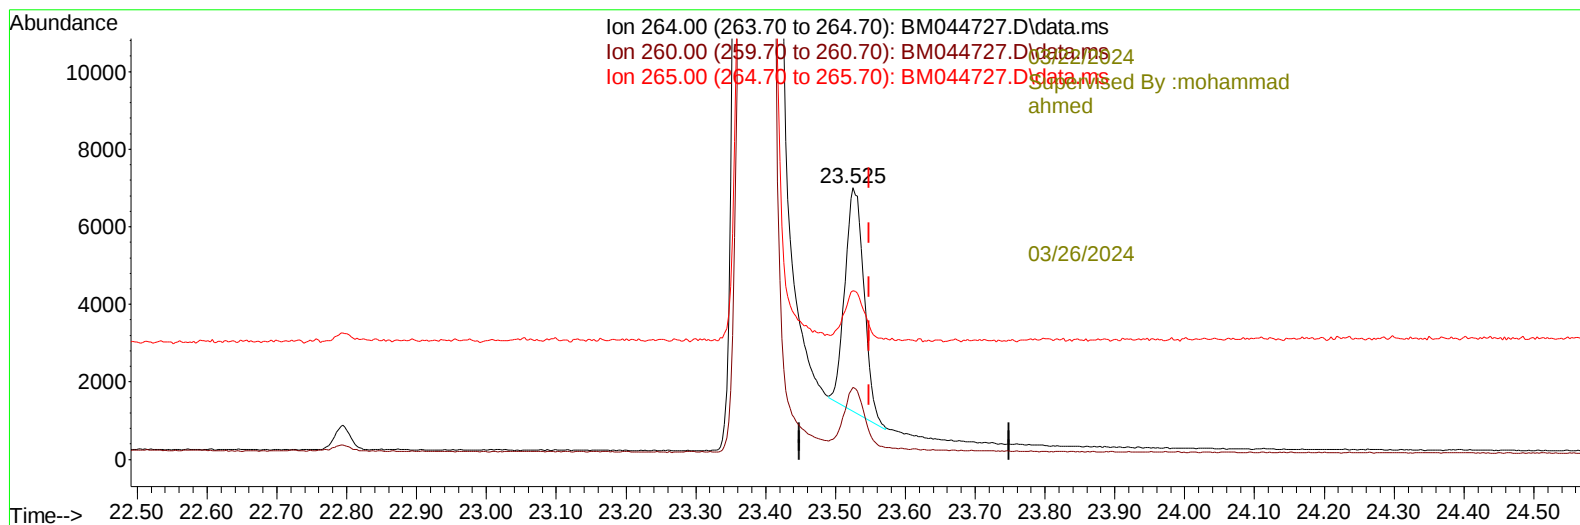

TIC: BM044727.D\data.ms

(23) Perylene-d12 (I)

23.525min (-0.023) 0.40 ng/ul m

response 10932

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.60	26.52
265.00	60.10	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
 Data File : BM044727.D
 Acq On : 22 Mar 2024 08:32
 Operator : MA/JU
 Sample : P1813-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 20 10:51:03 2024
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----03/22/2024							
Supervised By :mohammad							
aimed							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.690	152		4875	0.400	ng/ul	0.00
4) Naphthalene-d8	10.468	136		15409	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.334	164		7802	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.089	188		15341m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.287	240		11217m	0.400	ng/ul	-0.01
23) Perylene-d12	23.525	264		10932m	0.400	ng/ul	-0.02
-----03/26/2024							
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.255	96		27823	4.354	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.063	152		7617	0.344	ng/ul	-0.02
18) Fluoranthene-d10	19.122	212		13756m	0.349	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044727.D
Acq On : 22 Mar 2024 08:32
Operator : MA/JU
Sample : P1813-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX6

Manual IntegrationsAPPROVED

Quant Time: Mar 22 09:04:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

