

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
 Data File : BM044724.D
 Acq On : 22 Mar 2024 06:45
 Operator : MA/JU
 Sample : P1813-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX7

Quant Time: Mar 28 01:22:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 20 10:51:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.690	152	4393	0.400	ng/ul	0.00
4) Naphthalene-d8	10.468	136	13933	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.331	164	8086	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.090	188	14447m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.289	240	11041m	0.400	ng/ul	-0.01
23) Perylene-d12	23.527	264	10726m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	26238	4.556	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.068	152	7273	0.363	ng/ul	-0.01
18) Fluoranthene-d10	19.123	212	14008	0.361	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	427	0.073	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032224\
Data File : BM044724.D
Acq On : 22 Mar 2024 06:45
Operator : MA/JU
Sample : P1813-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX7

Quant Time: Mar 28 01:22:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 20 10:51:03 2024
Response via : Initial Calibration

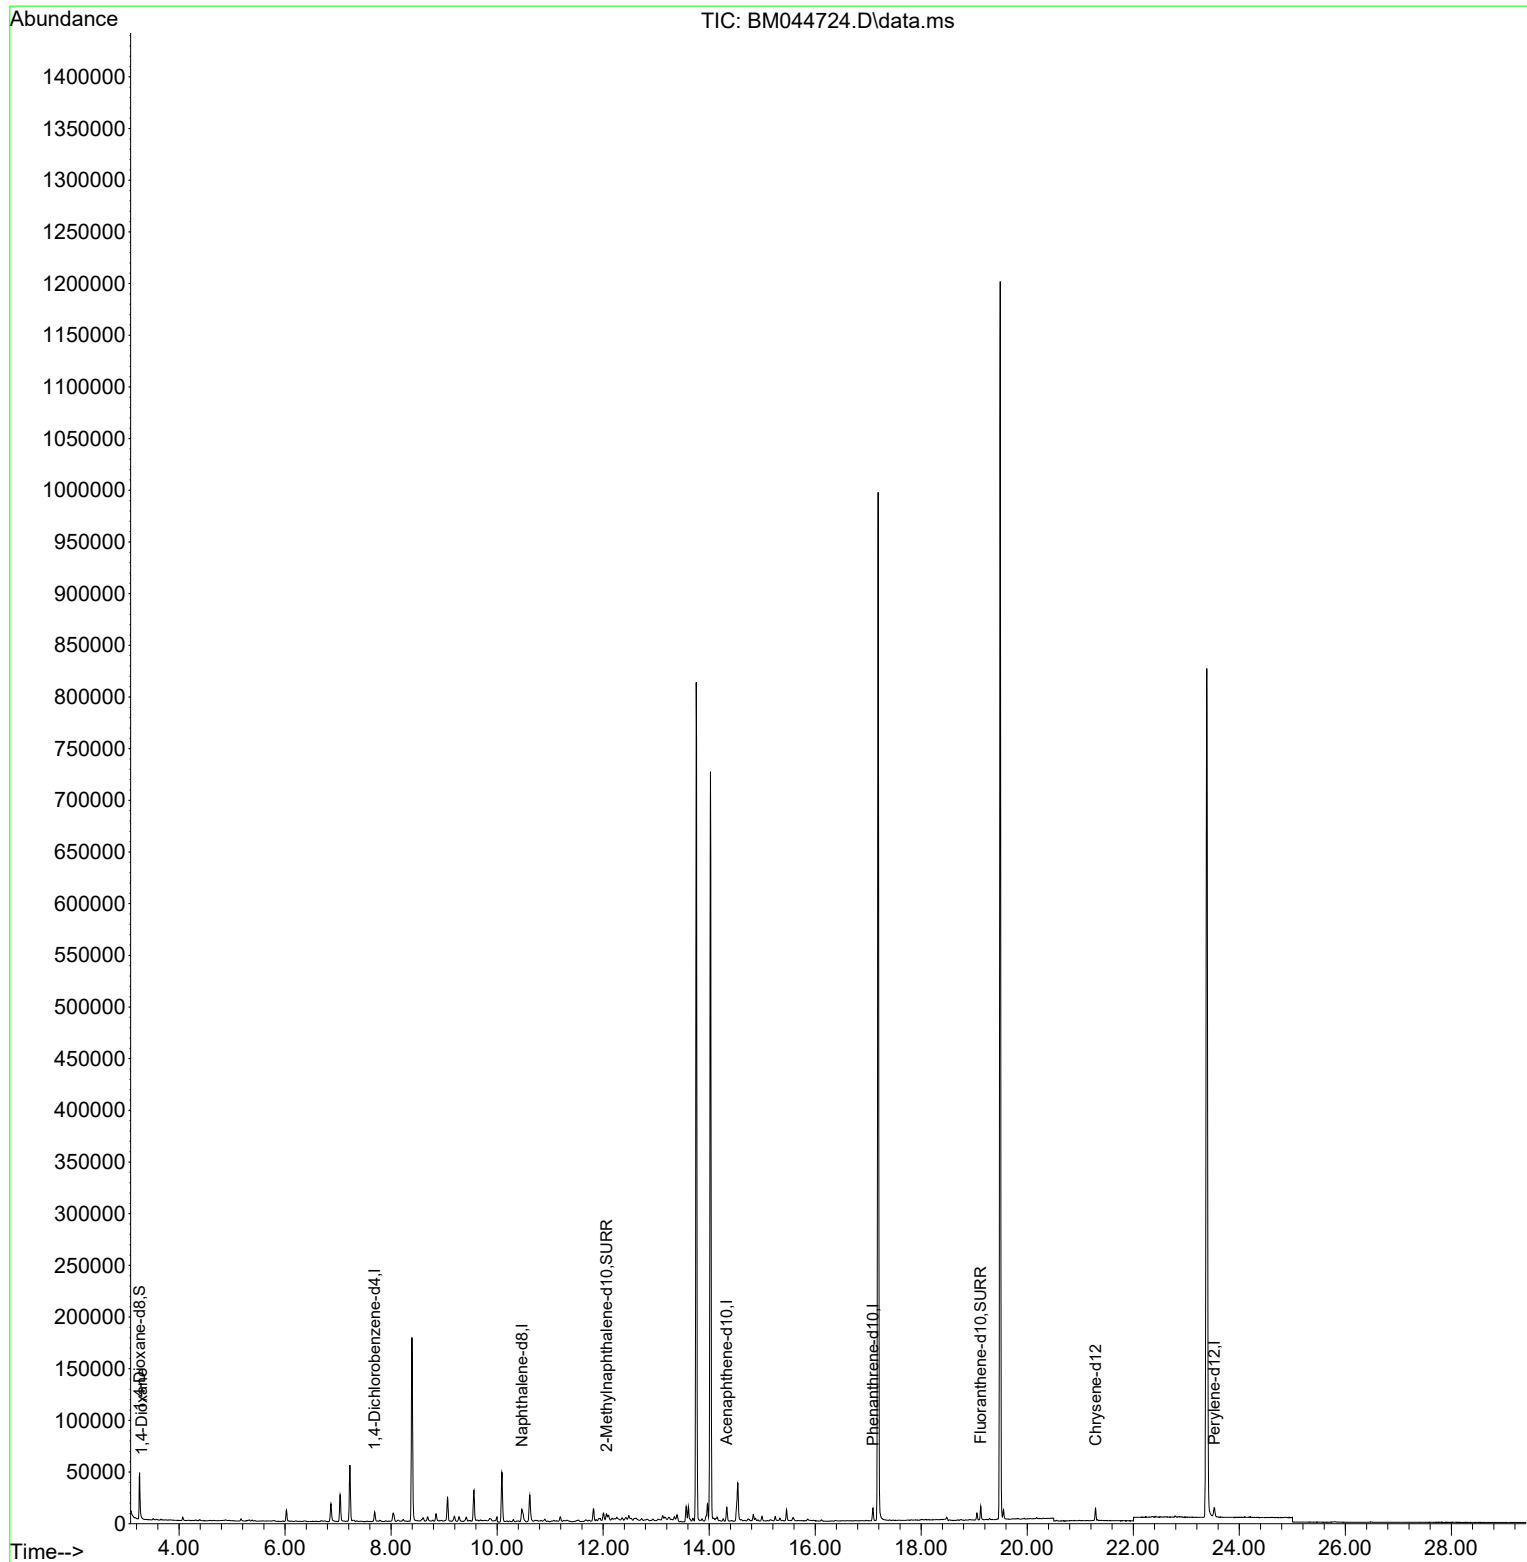

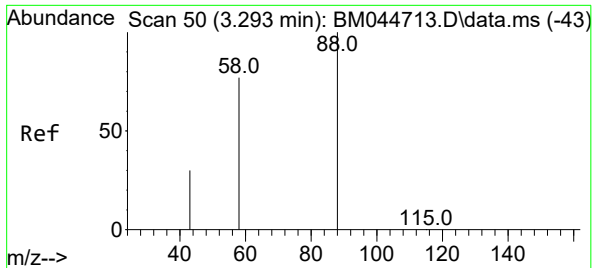

#2
 1,4-Dioxane
 Concen: 0.073 ng/ul
 RT: 3.293 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BM044724.D
 Acq: 22 Mar 2024 06:45

Instrument :
 BNA_M
 ClientSampleId :
 E0LX7

Tgt Ion: 88	Resp: 427
Ion Ratio	Lower Upper
88	100
43	266.7 21.4 32.0#
58	96.8 35.6 53.4#

