


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032315\
 Data File : BM000751.D
 Acq On : 23 Mar 2015 09:39
 Operator : TP/IZ
 Sample : DFTPP43
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP43

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM032115.M
 Title : SVOA CALIBRATION
 Last Update : Mon Mar 23 13:57:52 2015

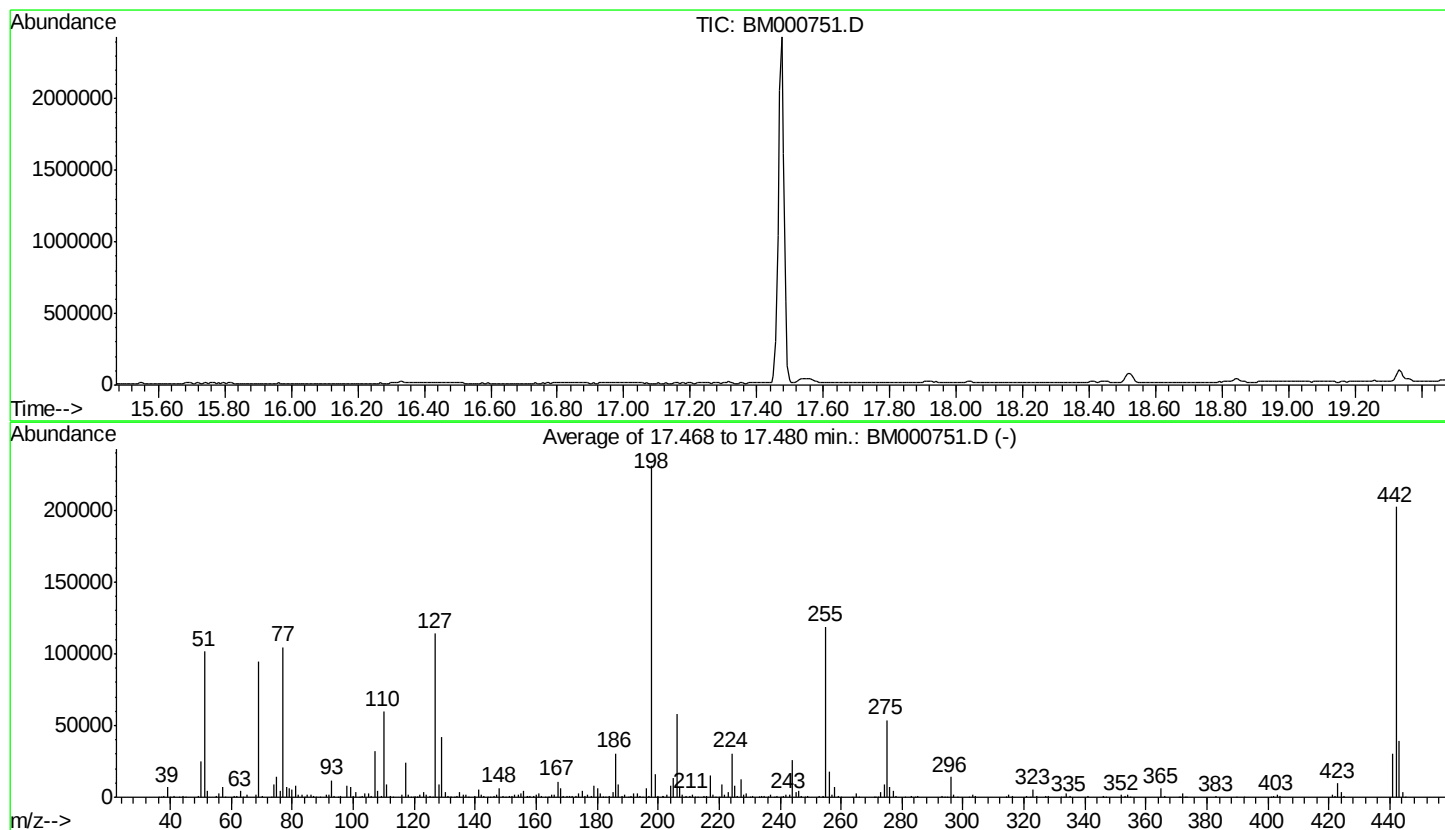

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	101277	PASS
68	69	0.00	2	1.6	1472	PASS
69	198	0.00	100	40.8	94309	PASS
70	69	0.00	2	0.6	547	PASS
127	198	10	80	49.3	113909	PASS
197	198	0.00	2	0.5	1238	PASS
198	198	100	100	100.0	230976	PASS
199	198	5	9	6.8	15687	PASS
275	198	10	60	23.3	53864	PASS
365	198	1	100	2.6	6118	PASS
441	443	0.01	100	77.0	30416	PASS
442	198	50	100	87.5	202048	PASS
443	442	15	24	19.5	39496	PASS