

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
 Data File : BM009347.D
 Acq On : 23 Mar 2017 18:14
 Operator : SJ/MA
 Sample : PB97753BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.010	661	667	677	rVB	446624	687505	19.49%	2.074%
2	7.192	690	698	708	rBV	487821	756074	21.44%	2.281%
3	7.387	724	731	738	rBV	593200	926603	26.27%	2.795%
4	7.857	803	811	817	rBV	582296	907957	25.74%	2.739%
5	8.551	920	929	938	rBV	606421	969901	27.50%	2.926%
6	9.022	1002	1009	1019	rVB	608287	988442	28.02%	2.982%
7	9.739	1124	1131	1138	rBV	476653	795020	22.54%	2.398%
8	10.269	1215	1221	1231	rBV	686587	1135332	32.19%	3.425%
9	10.657	1279	1287	1294	rBV	697042	1153266	32.70%	3.479%
10	13.904	1829	1839	1847	rBV	1239146	1716309	48.66%	5.177%
11	14.192	1881	1888	1895	rBV	1250108	1804496	51.16%	5.443%
12	14.504	1933	1941	1948	rVB2	886602	1402169	39.75%	4.230%
13	14.692	1965	1973	1984	rBV2	378851	612647	17.37%	1.848%
14	15.492	2103	2109	2119	rBV	1689051	2405550	68.20%	7.256%
15	15.610	2124	2129	2141	rVV	641094	913957	25.91%	2.757%
16	17.251	2401	2408	2414	rBV2	1164434	1662952	47.15%	5.016%
17	17.345	2418	2424	2438	rBV2	1912222	2757700	78.19%	8.319%
18	19.268	2747	2751	2757	rBV3	19841	37272	1.06%	0.112%
19	19.639	2808	2814	2820	rBV	2667951	3372285	95.61%	10.172%
20	20.956	3035	3038	3042	rVB3	60115	66522	1.89%	0.201%
21	21.321	3097	3100	3106	rVB	65124	68166	1.93%	0.206%
22	21.421	3112	3117	3123	rBV	1849386	2294135	65.04%	6.920%
23	23.603	3480	3488	3499	rVB2	1759646	3527143	100.00%	10.640%
24	23.750	3506	3513	3523	rVB	1136093	2189616	62.08%	6.605%


Sum of corrected areas: 33151019

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009347.D
Acq On : 23 Mar 2017 18:14
Operator : SJ/MA
Sample : PB97753BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

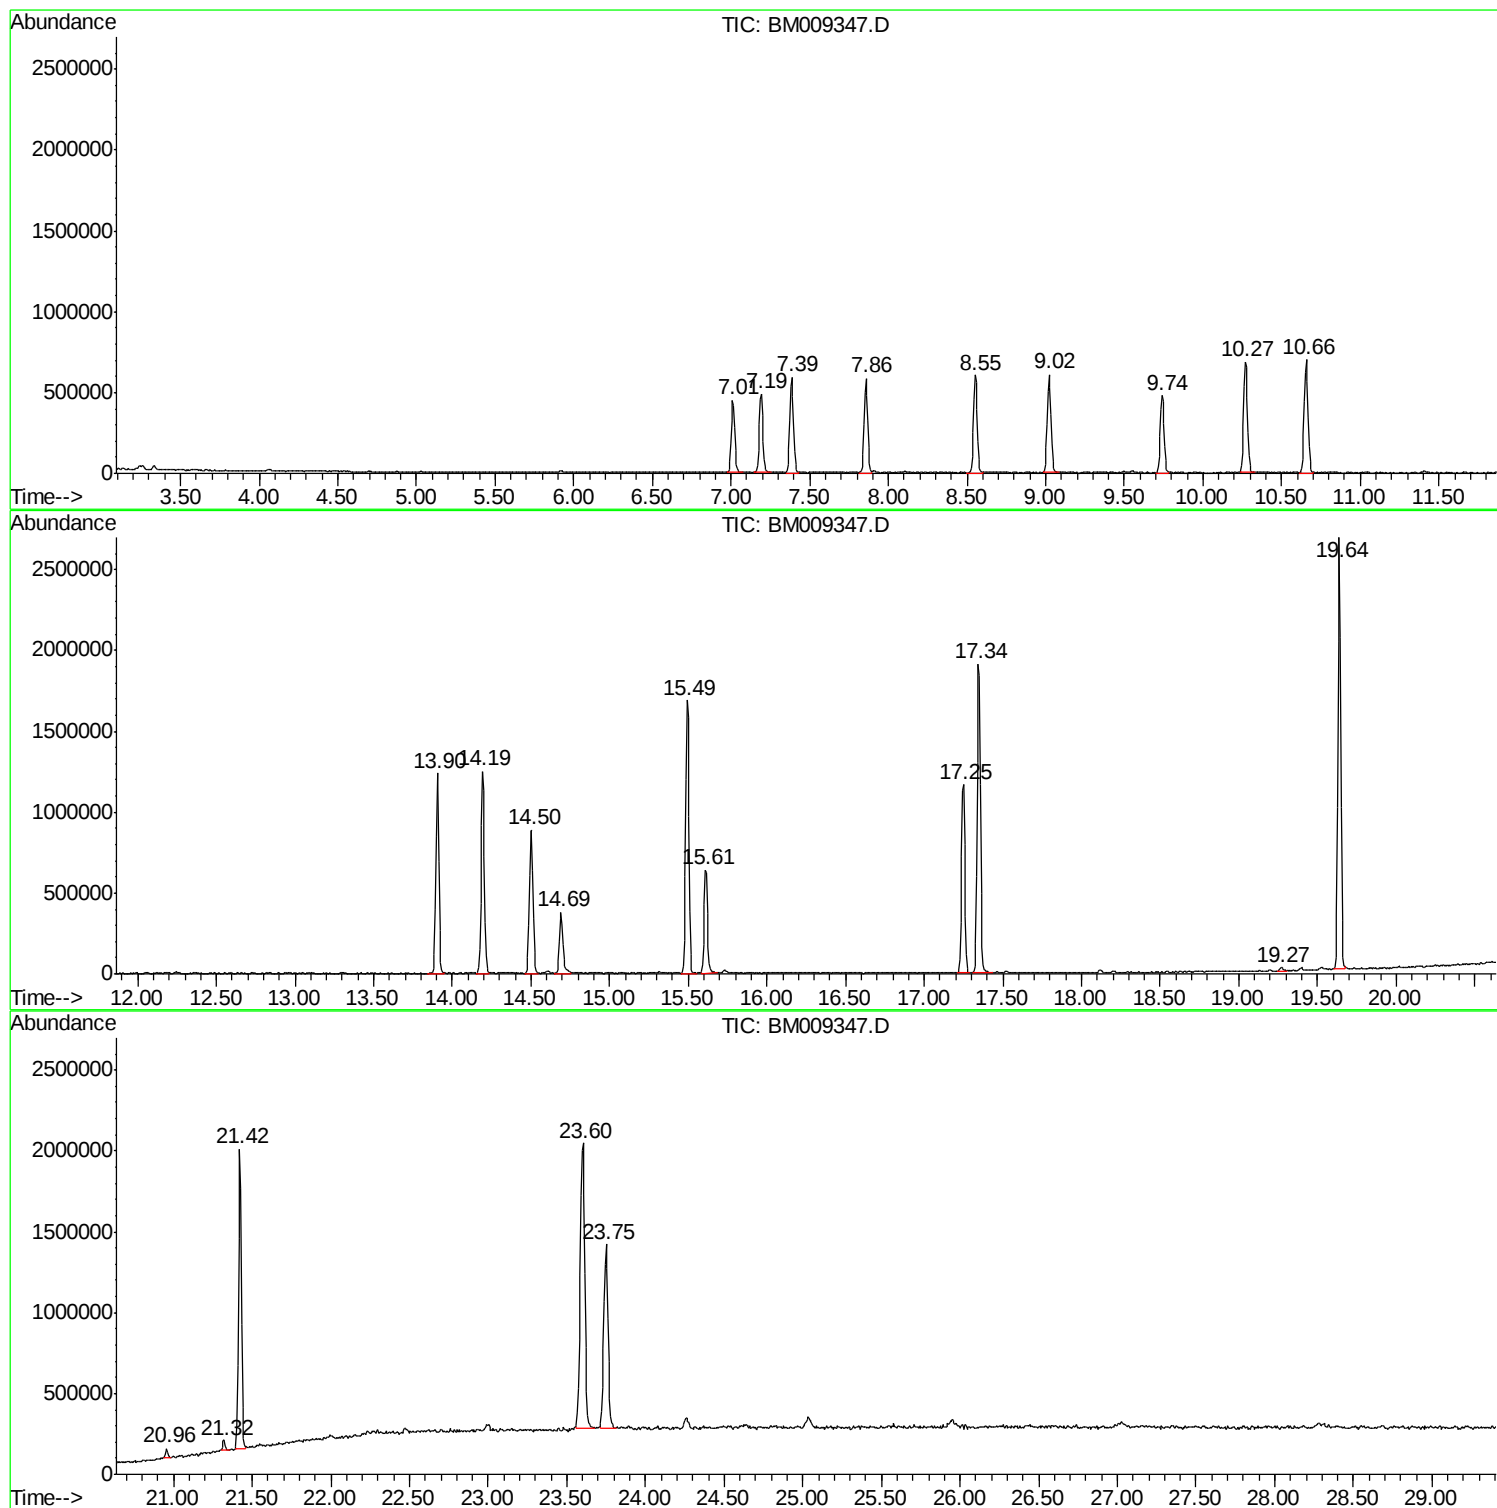

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009347.D
Acq On : 23 Mar 2017 18:14
Operator : SJ/MA
Sample : PB97753BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009347.D
Acq On : 23 Mar 2017 18:14
Operator : SJ/MA
Sample : PB97753BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK53

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc