

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
 Data File : BM009353.D
 Acq On : 23 Mar 2017 21:49
 Operator : SJ/MA
 Sample : PB97757BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	48	rBV2	36431	54560	1.74%	0.164%
2	7.010	661	667	675	rVB	522281	812533	25.87%	2.435%
3	7.187	690	697	705	rBV	514795	806937	25.69%	2.418%
4	7.387	723	731	738	rBV	652205	1039005	33.08%	3.114%
5	7.857	805	811	818	rBV	618230	987663	31.44%	2.960%
6	8.551	922	929	939	rBV	720187	1122557	35.73%	3.364%
7	9.022	1000	1009	1016	rBV	648500	1069505	34.05%	3.205%
8	9.739	1122	1131	1141	rBV	514204	852590	27.14%	2.555%
9	10.269	1214	1221	1230	rBV	743261	1216554	38.73%	3.646%
10	10.657	1279	1287	1294	rBV	755007	1255682	39.97%	3.763%
11	13.904	1833	1839	1848	rVB	1240363	1682391	53.56%	5.042%
12	14.192	1881	1888	1899	rBV	1211330	1764660	56.18%	5.288%
13	14.498	1933	1940	1948	rBV2	989751	1511106	48.10%	4.528%
14	14.692	1967	1973	1988	rBV	408034	672289	21.40%	2.015%
15	15.492	2102	2109	2119	rBV	1606369	2278367	72.53%	6.828%
16	15.610	2123	2129	2140	rVV	607749	852942	27.15%	2.556%
17	17.245	2401	2407	2416	rBV2	1236225	1810875	57.65%	5.427%
18	17.345	2418	2424	2436	rBV2	1751433	2488514	79.22%	7.457%
19	19.274	2748	2752	2757	rBV3	18484	32282	1.03%	0.097%
20	19.639	2808	2814	2820	rBV	2338096	2997060	95.41%	8.981%
21	20.956	3035	3038	3041	rBV2	47879	54105	1.72%	0.162%
22	21.315	3097	3099	3103	rBV2	54460	53768	1.71%	0.161%
23	21.421	3112	3117	3122	rBV	1989388	2429942	77.35%	7.282%
24	22.986	3381	3383	3388	rBV6	46996	65957	2.10%	0.198%
25	23.597	3479	3487	3497	rBV2	1615800	3141360	100.00%	9.414%
26	23.750	3506	3513	3520	rBV	1213293	2316491	73.74%	6.942%


Sum of corrected areas: 33369695

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009353.D
Acq On : 23 Mar 2017 21:49
Operator : SJ/MA
Sample : PB97757BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK57

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

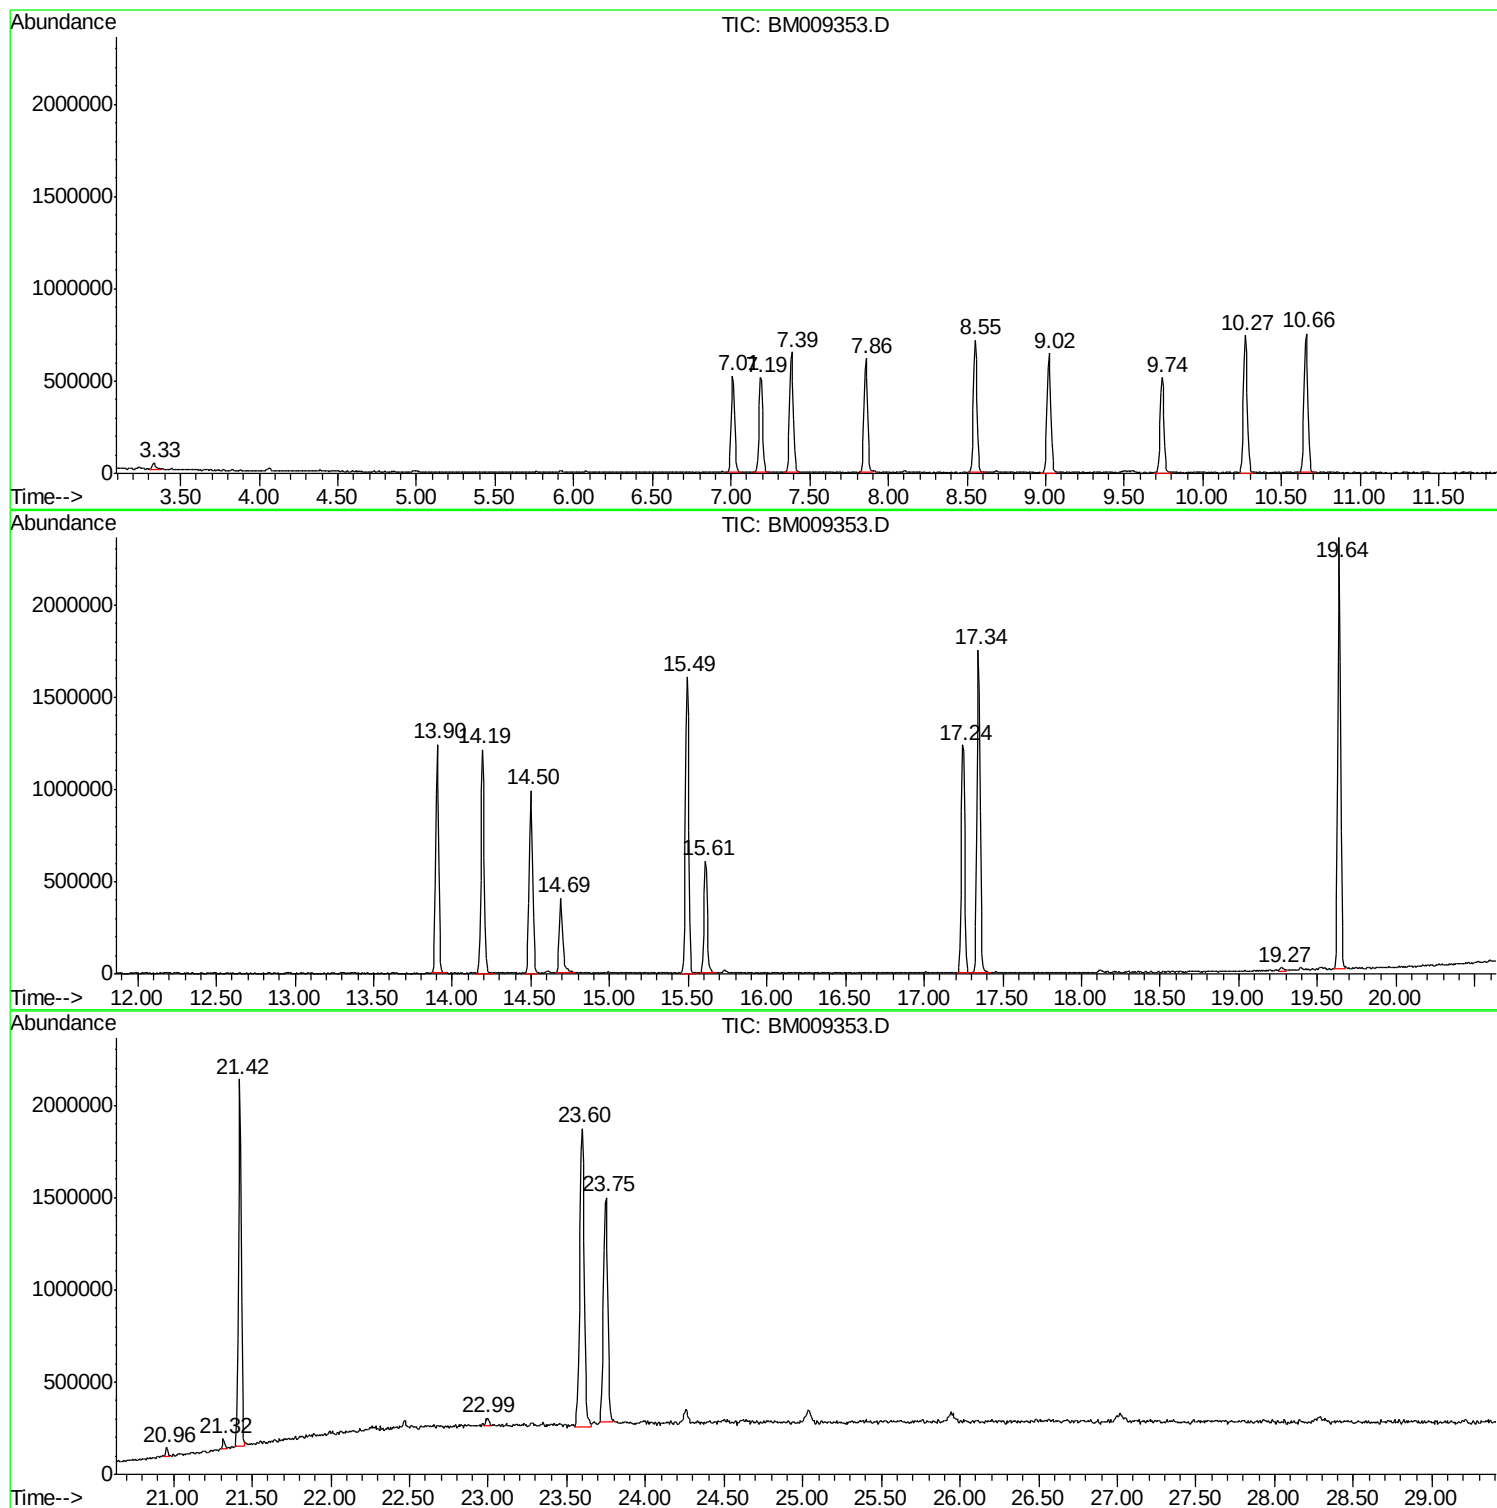

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009353.D
Acq On : 23 Mar 2017 21:49
Operator : SJ/MA
Sample : PB97757BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009353.D
Acq On : 23 Mar 2017 21:49
Operator : SJ/MA
Sample : PB97757BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc