

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
 Data File : BM009354.D
 Acq On : 23 Mar 2017 22:25
 Operator : SJ/MA
 Sample : I2326-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	50	rVB2	41601	60657	1.39%	0.161%
2	4.475	231	236	240	rVB	38060	51325	1.18%	0.136%
3	6.946	649	656	661	rBV2	30937	48415	1.11%	0.129%
4	7.010	661	667	676	rVB	196869	316592	7.28%	0.841%
5	7.187	691	697	709	rBV	609875	955973	21.98%	2.540%
6	7.387	724	731	738	rBV	675102	1070731	24.62%	2.844%
7	7.857	804	811	819	rBV	605151	931178	21.41%	2.474%
8	8.551	920	929	939	rBV2	524234	822413	18.91%	2.185%
9	9.022	1001	1009	1017	rBV	811058	1311600	30.16%	3.484%
10	9.381	1063	1070	1076	rBV2	39479	56743	1.30%	0.151%
11	9.739	1125	1131	1142	rBV	647337	1038891	23.89%	2.760%
12	10.269	1212	1221	1230	rBV	825922	1391616	32.00%	3.697%
13	10.657	1278	1287	1294	rBV	702599	1204367	27.69%	3.199%
14	11.875	1489	1494	1499	rBV3	31773	49726	1.14%	0.132%
15	13.904	1829	1839	1852	rBV	1509181	2082843	47.89%	5.533%
16	14.192	1881	1888	1895	rBV	1497020	2162869	49.73%	5.746%
17	14.498	1930	1940	1948	rBV2	952140	1454107	33.43%	3.863%
18	14.692	1966	1973	1987	rBV	138307	233679	5.37%	0.621%
19	15.492	2102	2109	2118	rBV2	2152812	3076228	70.73%	8.172%
20	15.610	2123	2129	2140	rBV	761749	1061177	24.40%	2.819%
21	17.245	2401	2407	2414	rBV	1198743	1714675	39.43%	4.555%
22	17.345	2418	2424	2434	rBV	2515463	3458540	79.52%	9.188%
23	19.274	2746	2752	2760	rBV3	24679	50252	1.16%	0.133%
24	19.639	2808	2814	2821	rBV	3129198	4073214	93.66%	10.821%
25	21.321	3097	3100	3104	rVB3	61771	65635	1.51%	0.174%
26	21.421	3112	3117	3123	rBV	1893740	2330783	53.59%	6.192%
27	23.597	3480	3487	3497	rVB2	2272271	4349089	100.00%	11.554%
28	23.750	3506	3513	3519	rVB	1165308	2219656	51.04%	5.897%


Sum of corrected areas: 37642974

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009354.D
Acq On : 23 Mar 2017 22:25
Operator : SJ/MA
Sample : I2326-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

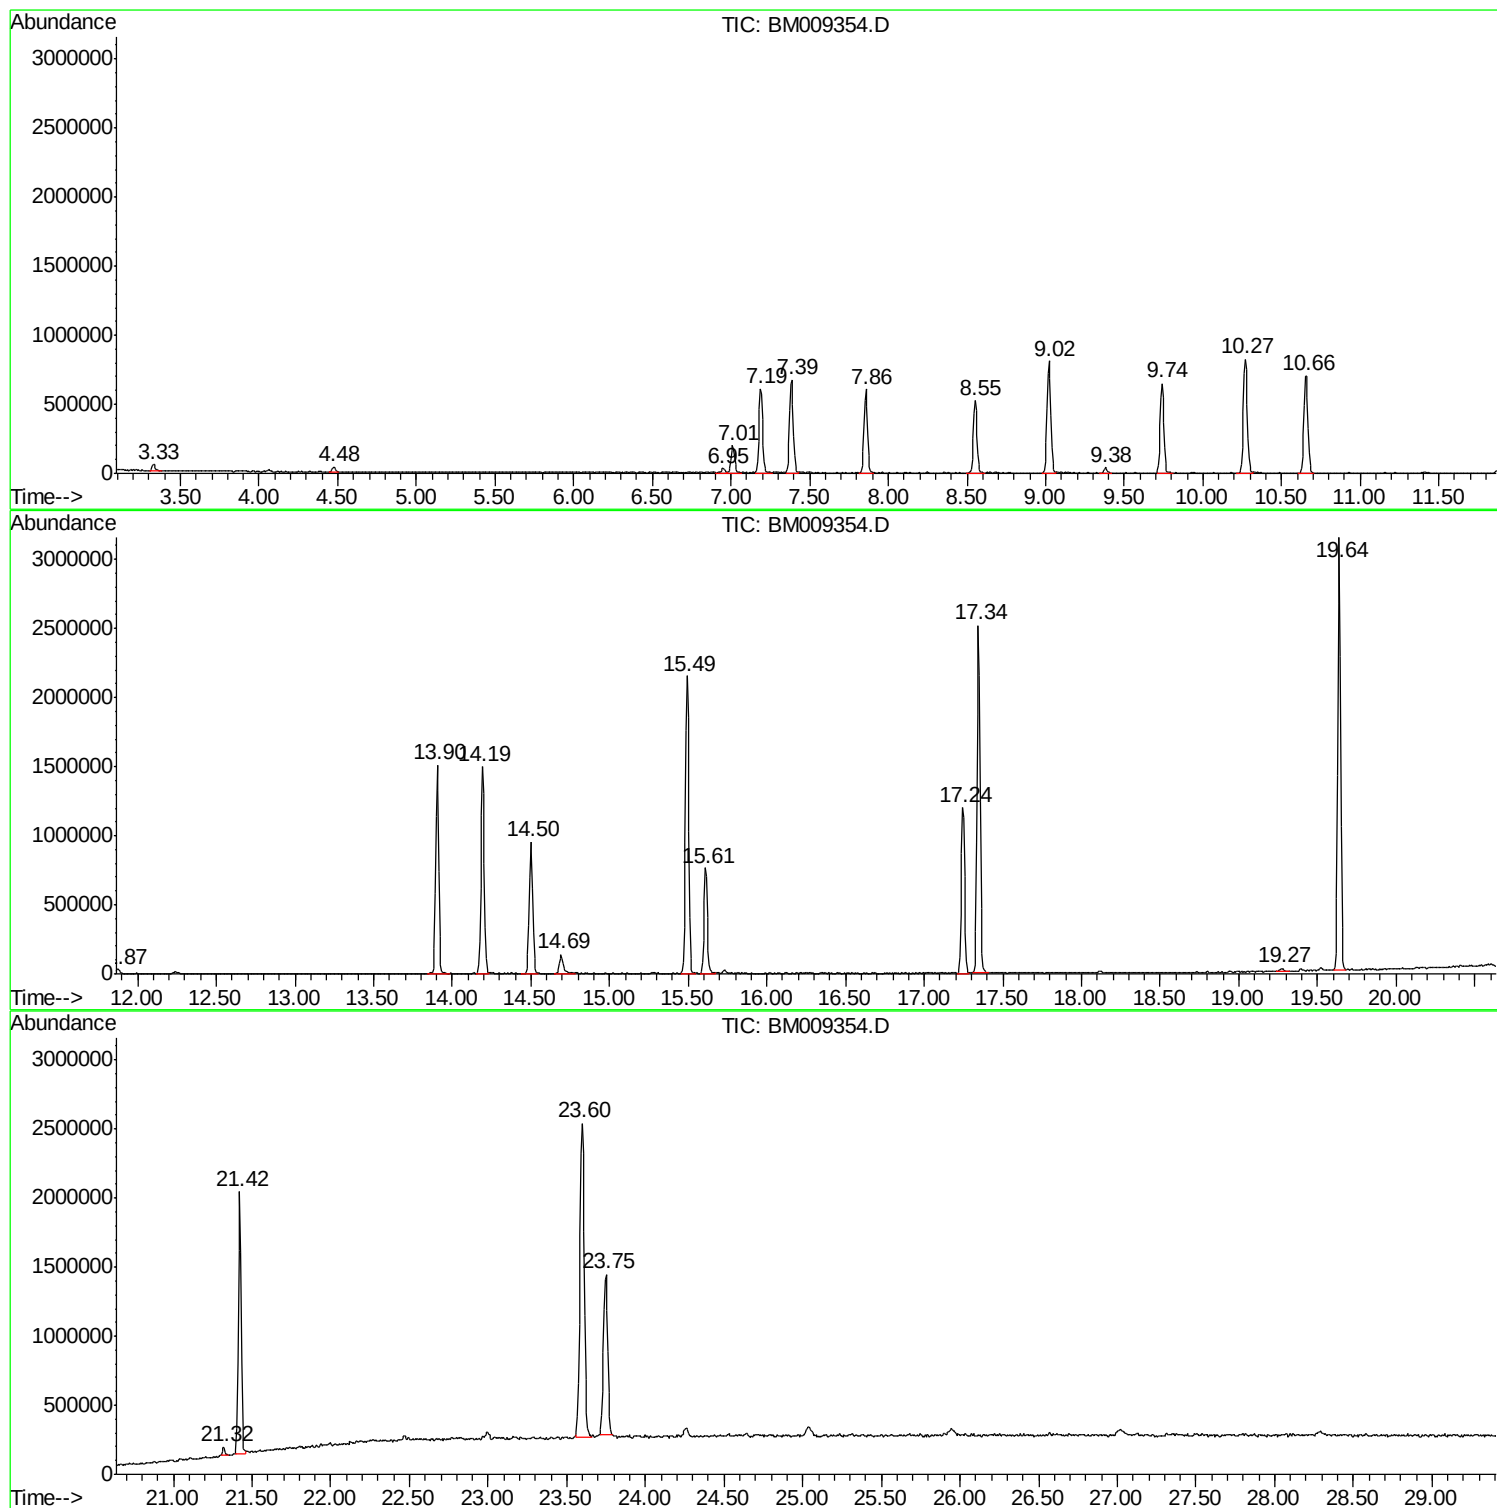

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009354.D
Acq On : 23 Mar 2017 22:25
Operator : SJ/MA
Sample : I2326-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009354.D
Acq On : 23 Mar 2017 22:25
Operator : SJ/MA
Sample : I2326-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc