

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
 Data File : BM009355.D
 Acq On : 23 Mar 2017 23:01
 Operator : SJ/MA
 Sample : I2326-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rBV2	50164	71641	1.75%	0.191%
2	7.010	661	667	674	rBV	220498	328029	8.00%	0.874%
3	7.187	691	697	708	rBV	665452	1037067	25.30%	2.762%
4	7.387	724	731	742	rVB	719273	1159156	28.27%	3.087%
5	7.857	803	811	819	rBV	603956	935321	22.81%	2.491%
6	8.551	922	929	938	rVB	552015	873383	21.30%	2.326%
7	9.022	1001	1009	1021	rBV	868456	1423268	34.71%	3.790%
8	9.739	1124	1131	1140	rVB	715283	1141364	27.84%	3.039%
9	10.269	1213	1221	1231	rBV	939979	1547037	37.73%	4.120%
10	10.657	1279	1287	1295	rBV	729068	1214131	29.61%	3.233%
11	11.404	1407	1414	1420	rBV2	22055	41166	1.00%	0.110%
12	13.904	1833	1839	1849	rBV	1658251	2210836	53.92%	5.887%
13	14.192	1880	1888	1894	rBV	941663	1415045	34.51%	3.768%
14	14.498	1934	1940	1949	rVB2	944725	1479221	36.08%	3.939%
15	14.692	1967	1973	1984	rBV2	141943	236717	5.77%	0.630%
16	15.492	2101	2109	2117	rBV	2289176	3257047	79.44%	8.673%
17	15.610	2123	2129	2143	rBV	799999	1119653	27.31%	2.982%
18	15.733	2143	2150	2155	rVB4	25655	41854	1.02%	0.111%
19	17.245	2400	2407	2414	rBV	1234652	1736565	42.36%	4.624%
20	17.345	2416	2424	2438	rBV	2500869	3521315	85.89%	9.377%
21	19.639	2808	2814	2821	rBV	3087043	4059566	99.02%	10.810%
22	21.421	3112	3117	3122	rBV	1959083	2343376	57.16%	6.240%
23	23.597	3480	3487	3497	rVB	2054884	4099868	100.00%	10.918%
24	23.744	3506	3512	3523	rVB2	1153551	2260310	55.13%	6.019%


Sum of corrected areas: 37552936

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009355.D
Acq On : 23 Mar 2017 23:01
Operator : SJ/MA
Sample : I2326-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

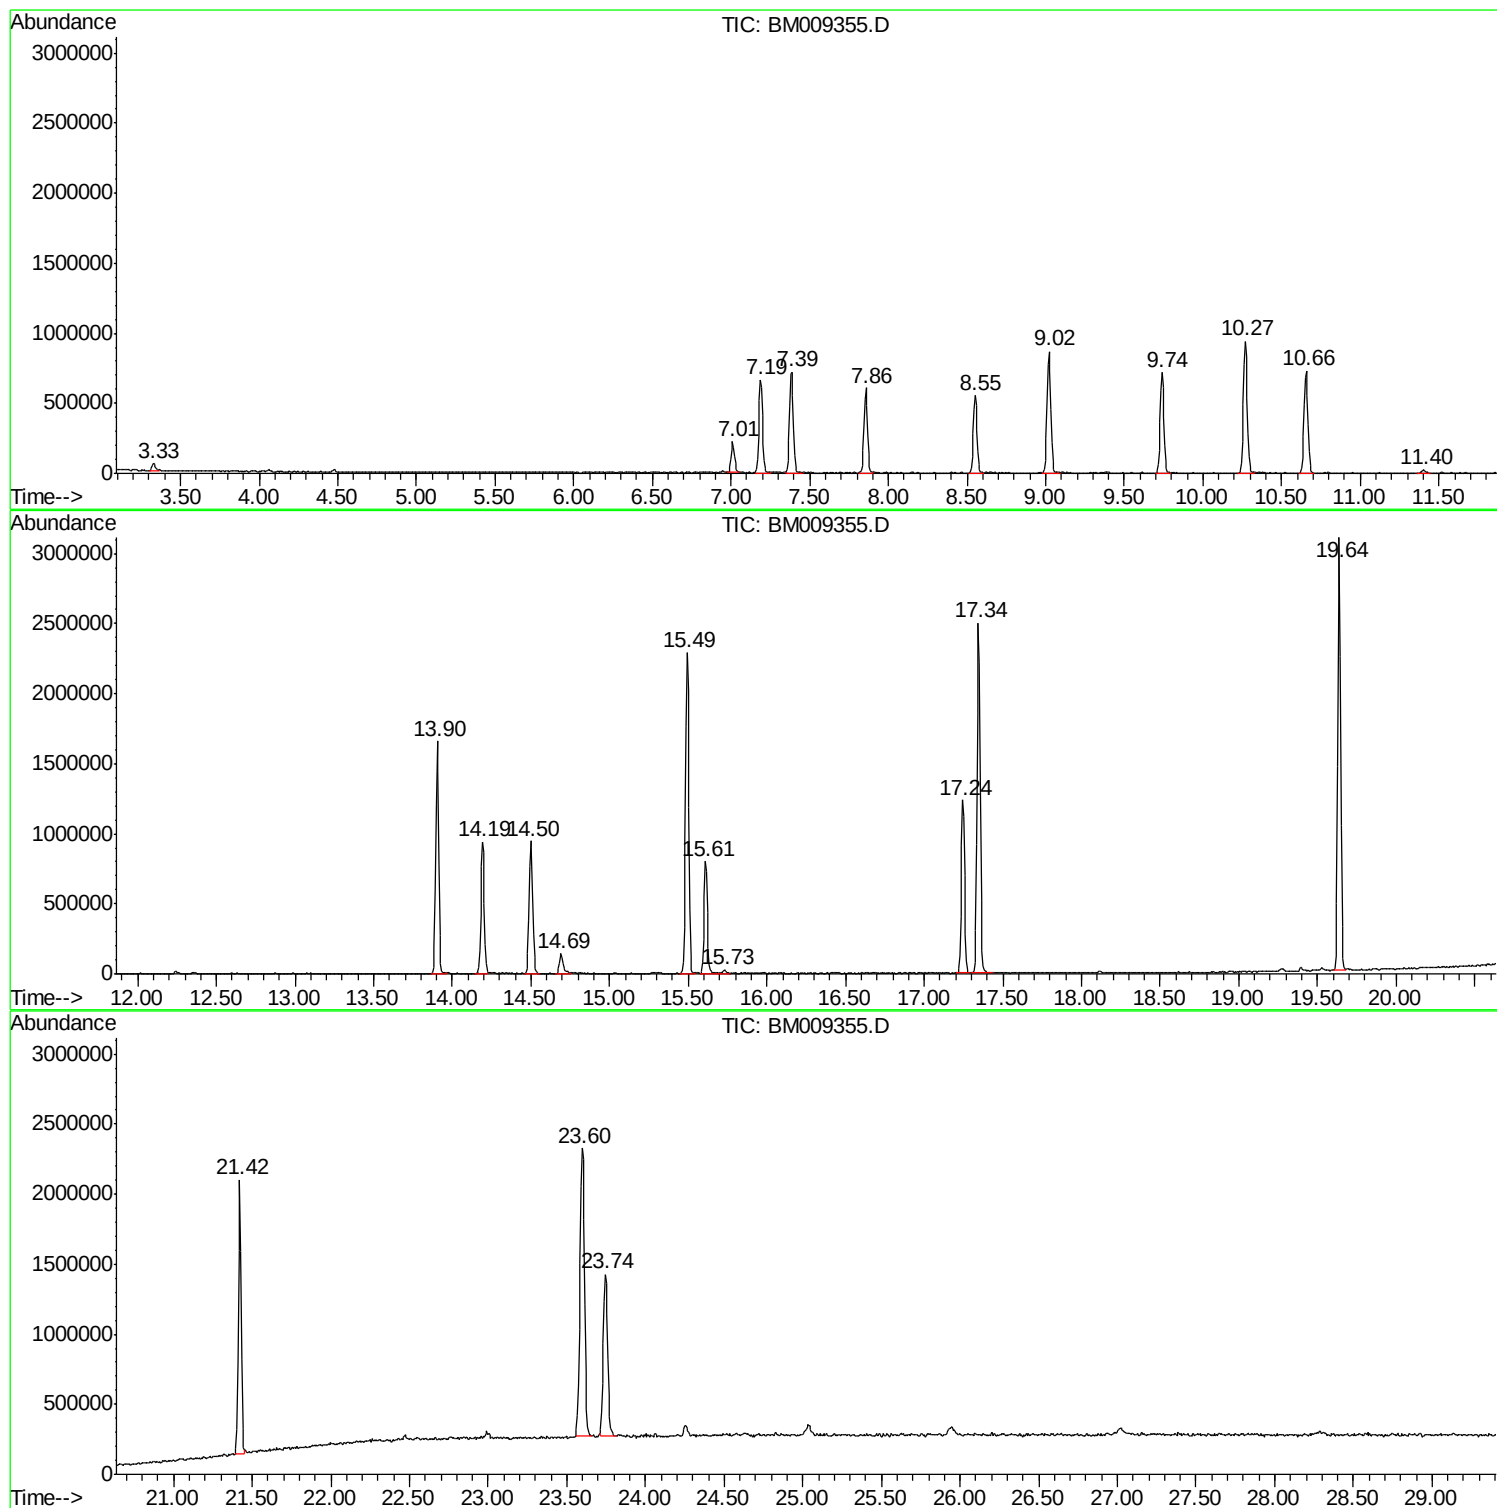

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009355.D
Acq On : 23 Mar 2017 23:01
Operator : SJ/MA
Sample : I2326-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009355.D
Acq On : 23 Mar 2017 23:01
Operator : SJ/MA
Sample : I2326-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc