

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
 Data File : BM009356.D
 Acq On : 23 Mar 2017 23:37
 Operator : SJ/MA
 Sample : I2326-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	47	rVB	49488	67536	1.41%	0.165%
2	7.010	661	667	674	rBV	218593	333824	6.99%	0.818%
3	7.187	691	697	705	rBV	666840	1030078	21.56%	2.524%
4	7.387	723	731	739	rVB	705186	1135367	23.76%	2.782%
5	7.857	804	811	819	rVB	577687	916672	19.18%	2.246%
6	8.551	923	929	939	rBV	543158	852474	17.84%	2.088%
7	9.022	1000	1009	1018	rBV	869973	1422757	29.77%	3.486%
8	9.386	1063	1071	1075	rBV4	31042	53667	1.12%	0.131%
9	9.739	1123	1131	1140	rBV2	697926	1136110	23.78%	2.783%
10	10.269	1214	1221	1233	rBV	944238	1536690	32.16%	3.765%
11	10.657	1279	1287	1295	rBV	717895	1195520	25.02%	2.929%
12	13.904	1829	1839	1848	rBV	1697060	2295092	48.03%	5.623%
13	14.192	1880	1888	1895	rBV	1802101	2615435	54.73%	6.408%
14	14.498	1935	1940	1951	rVB2	946579	1464547	30.65%	3.588%
15	14.692	1967	1973	1982	rBV2	143105	238677	4.99%	0.585%
16	15.492	2101	2109	2116	rBV	2448808	3401177	71.18%	8.333%
17	15.610	2123	2129	2138	rBV	850329	1187461	24.85%	2.909%
18	17.245	2401	2407	2416	rVB	1242270	1752769	36.68%	4.294%
19	17.345	2416	2424	2439	rBV	2753850	3869591	80.98%	9.480%
20	19.268	2745	2751	2755	rBV3	32549	49681	1.04%	0.122%
21	19.639	2807	2814	2823	rBV	3555728	4588510	96.02%	11.241%
22	21.421	3112	3117	3123	rBV	1958026	2365290	49.50%	5.795%
23	23.597	3480	3487	3496	rVB2	2489250	4778564	100.00%	11.707%
24	23.750	3506	3513	3519	rBV	1096225	2153136	45.06%	5.275%
25	24.256	3596	3599	3606	rVB5	93469	161964	3.39%	0.397%
26	25.032	3727	3731	3739	rVB5	99981	215235	4.50%	0.527%


Sum of corrected areas: 40817824

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009356.D
Acq On : 23 Mar 2017 23:37
Operator : SJ/MA
Sample : I2326-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

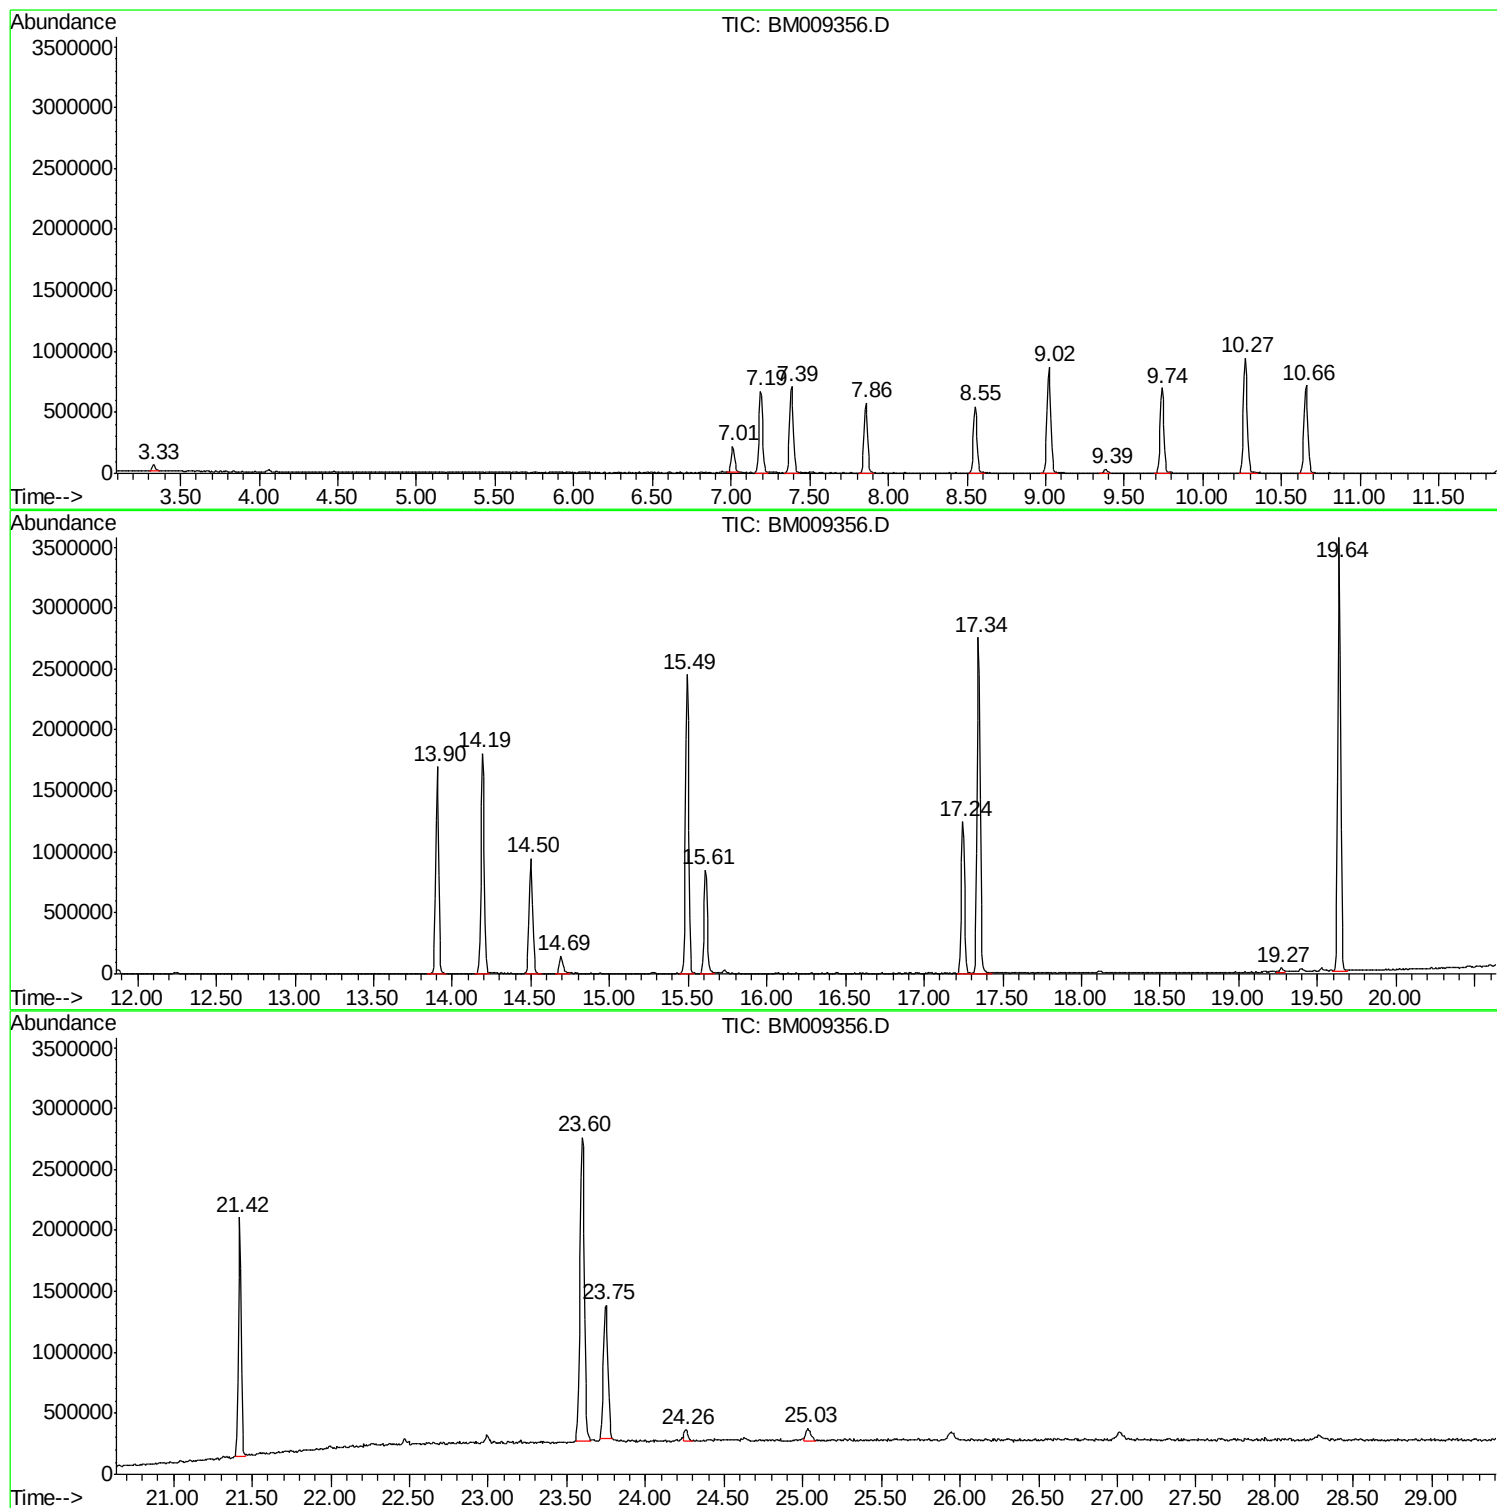

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009356.D
Acq On : 23 Mar 2017 23:37
Operator : SJ/MA
Sample : I2326-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009356.D
Acq On : 23 Mar 2017 23:37
Operator : SJ/MA
Sample : I2326-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc