

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
 Data File : BM009359.D
 Acq On : 24 Mar 2017 01:24
 Operator : SJ/MA
 Sample : I2357-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9XT9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rBV	51165	61458	1.31%	0.145%
2	7.010	660	667	674	rBV	200410	314370	6.72%	0.743%
3	7.186	691	697	711	rBV	671140	1048754	22.42%	2.478%
4	7.381	724	730	738	rBV	700213	1128173	24.12%	2.666%
5	7.857	804	811	822	rVB	651538	1031341	22.05%	2.437%
6	8.551	922	929	939	rBV	524614	831838	17.78%	1.966%
7	9.022	1002	1009	1019	rVB	875303	1428926	30.55%	3.376%
8	9.739	1125	1131	1141	rVB	715413	1144430	24.47%	2.704%
9	10.269	1213	1221	1231	rBV	948320	1572195	33.61%	3.715%
10	10.657	1279	1287	1295	rBV	785579	1342283	28.70%	3.172%
11	10.804	1304	1312	1317	rBV3	27309	49654	1.06%	0.117%
12	13.904	1833	1839	1849	rBV	1754674	2332576	49.87%	5.512%
13	14.192	1881	1888	1896	rBV	1901422	2662455	56.92%	6.291%
14	14.498	1934	1940	1954	rVB2	1132136	1705889	36.47%	4.031%
15	14.692	1967	1973	1988	rBV2	133362	246477	5.27%	0.582%
16	15.492	2102	2109	2116	rBV	2440325	3441721	73.58%	8.132%
17	15.609	2123	2129	2143	rBV	887097	1199128	25.64%	2.833%
18	17.245	2401	2407	2417	rVB2	1453315	2039904	43.61%	4.820%
19	17.345	2417	2424	2433	rBV	2765961	3873739	82.82%	9.153%
20	19.274	2746	2752	2756	rBV2	33790	51757	1.11%	0.122%
21	19.392	2766	2772	2777	rBV6	23892	48776	1.04%	0.115%
22	19.639	2808	2814	2820	rBV	3556560	4603775	98.43%	10.878%
23	21.421	3112	3117	3124	rBV	2328605	2803558	59.94%	6.625%
24	23.597	3480	3487	3496	rBV	2510237	4677210	100.00%	11.052%
25	23.744	3505	3512	3520	rBV	1361358	2680361	57.31%	6.333%


Sum of corrected areas: 42320748

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009359.D
Acq On : 24 Mar 2017 01:24
Operator : SJ/MA
Sample : I2357-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XT9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

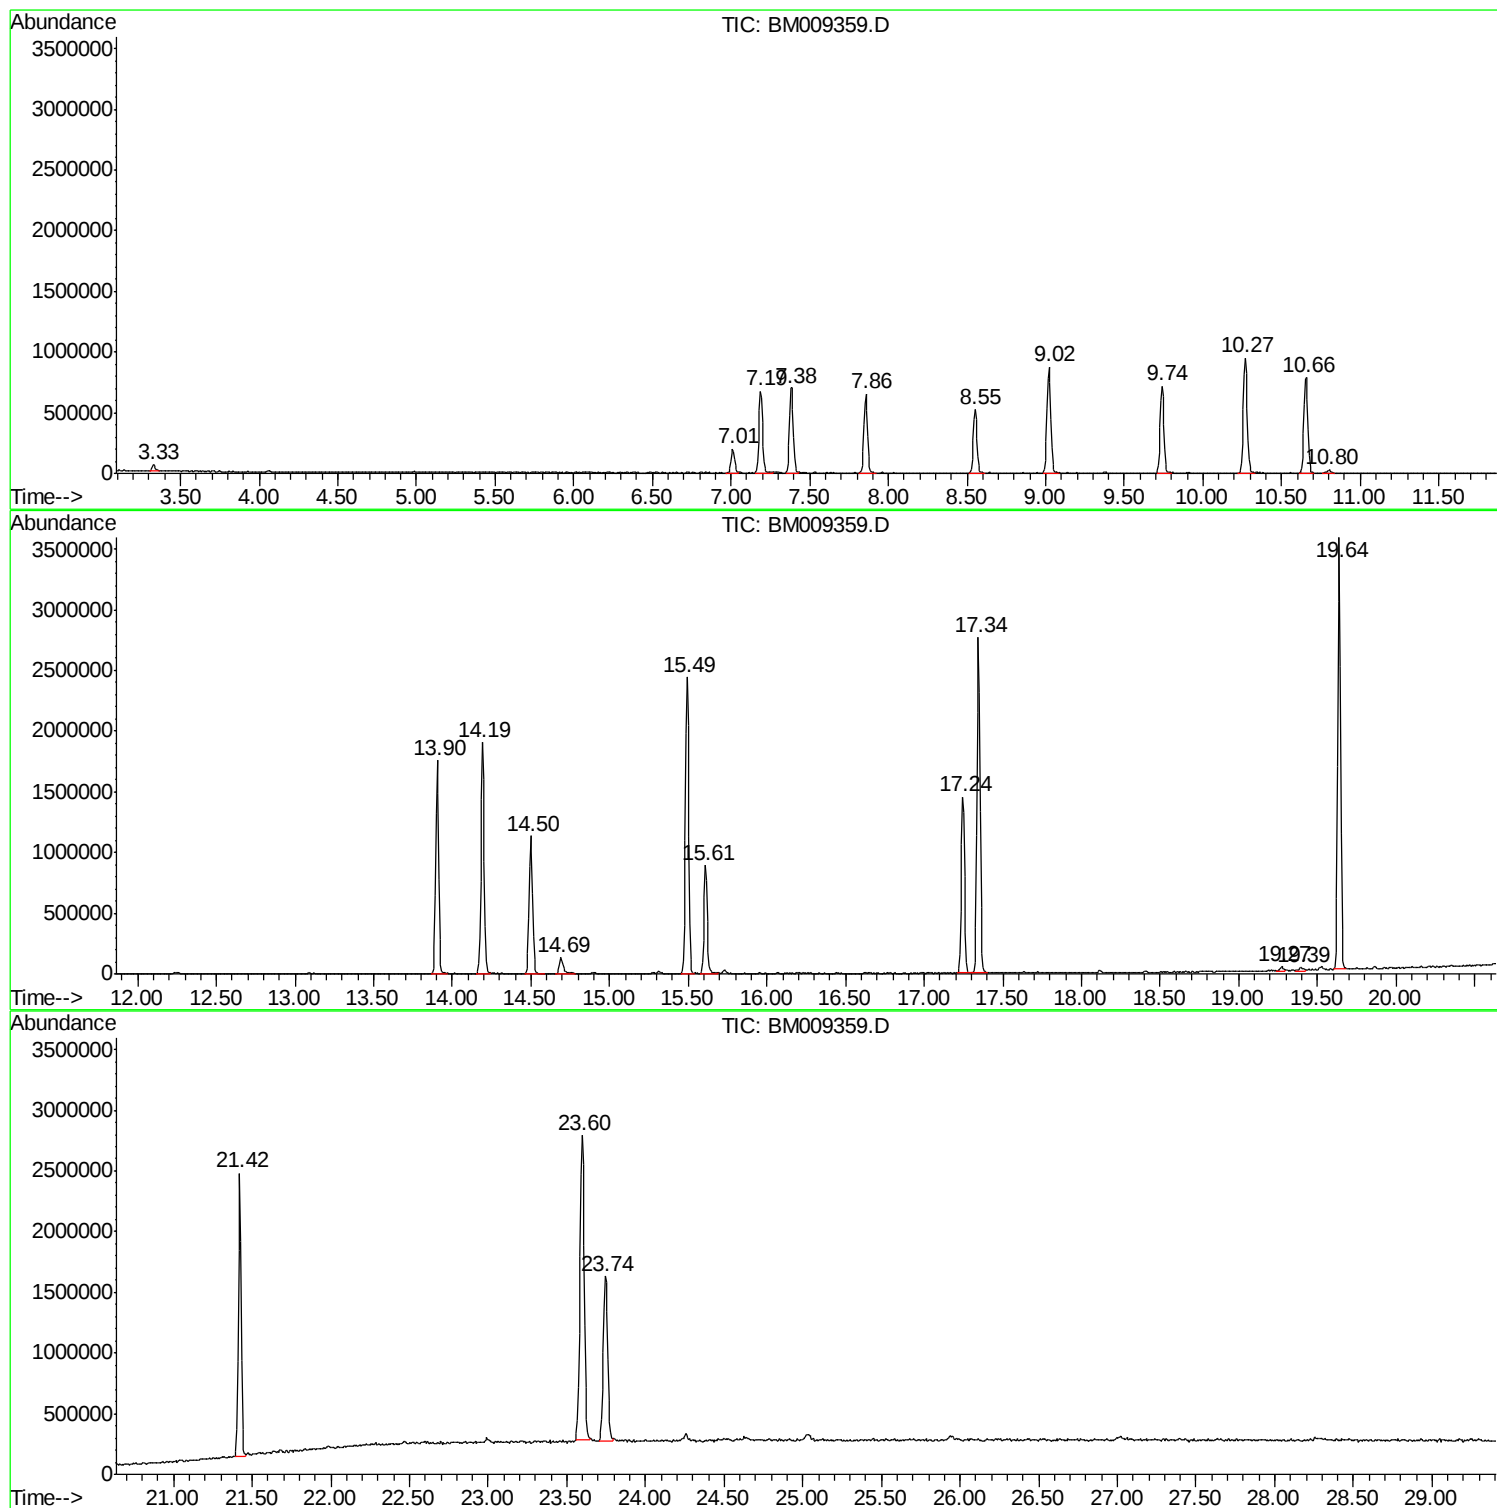

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009359.D
Acq On : 24 Mar 2017 01:24
Operator : SJ/MA
Sample : I2357-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XT9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032317\
Data File : BM009359.D
Acq On : 24 Mar 2017 01:24
Operator : SJ/MA
Sample : I2357-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XT9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc