


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032323\
Data File : BM039111.D
Acq On : 23 Mar 2023 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 22 03:36:20 2023

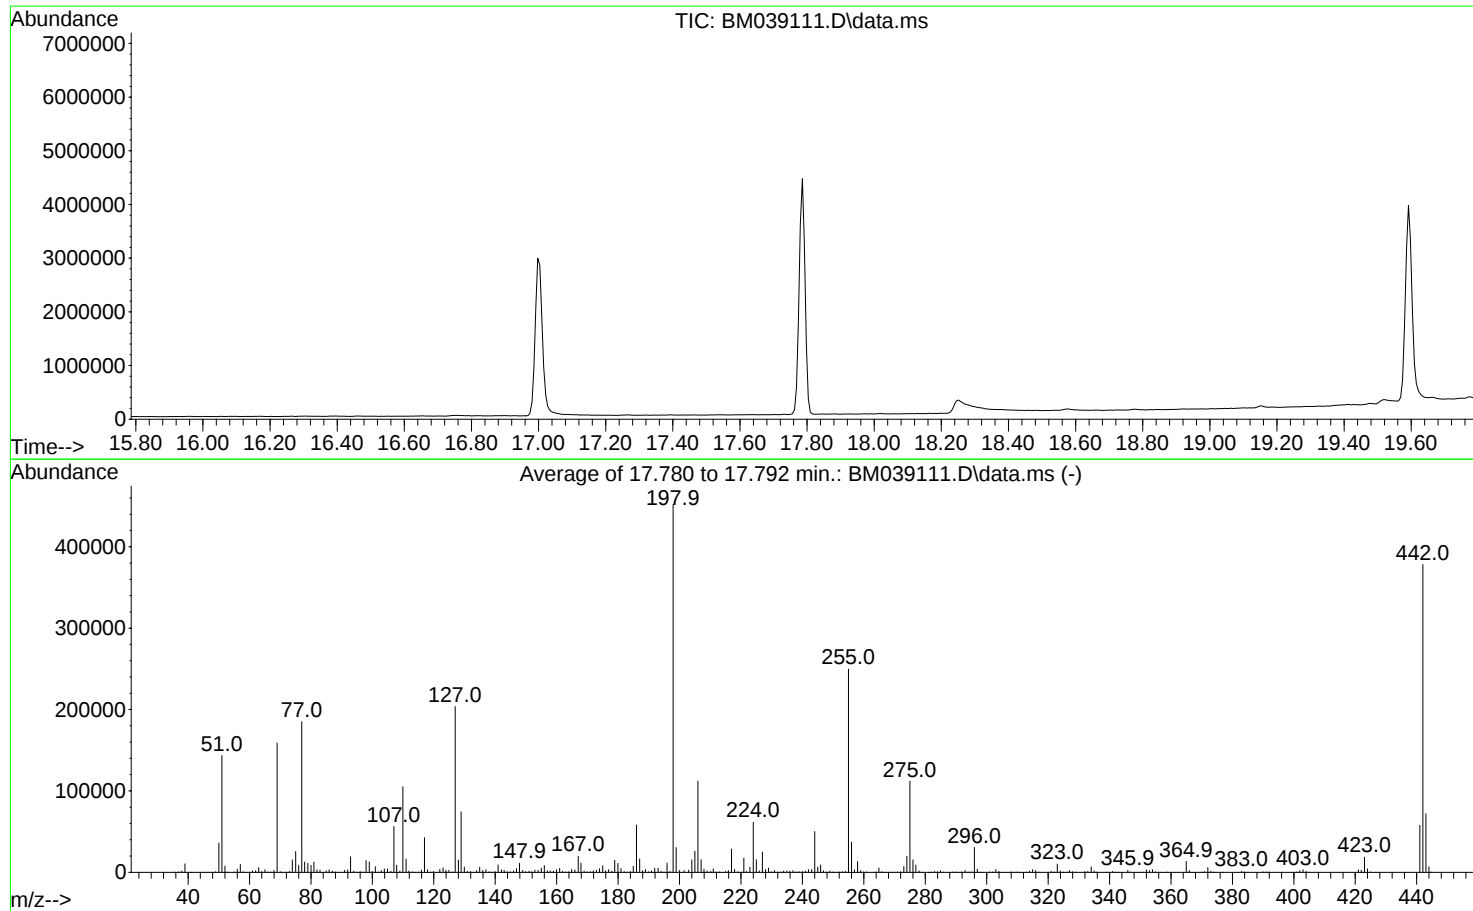




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	143524	PASS
68	69	0.00	2	1.4	2195	PASS
69	198	0.00	100	35.2	159000	PASS
70	69	0.00	2	0.4	683	PASS
127	198	10	80	45.0	203569	PASS
197	198	0.00	2	0.3	1165	PASS
198	198	100	100	100.0	452032	PASS
199	198	5	9	6.7	30293	PASS
275	198	10	60	24.7	111848	PASS
365	198	1	100	2.9	13333	PASS
441	198	0.01	100	12.8	57787	PASS
442	442	50	100	100.0	378112	PASS
443	442	15	24	19.0	71923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032323\
 Data File : BM039111.D
 Acq On : 23 Mar 2023 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 24 07:06:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 22 03:36:20 2023
 Response via : Initial Calibration

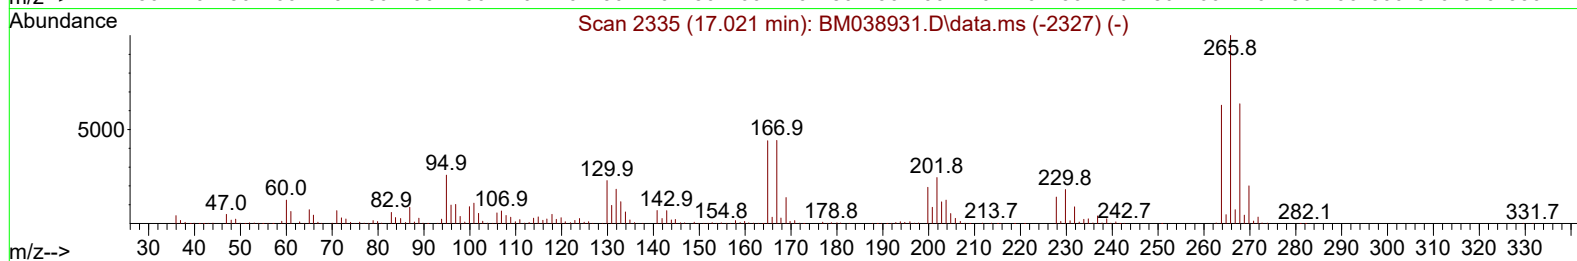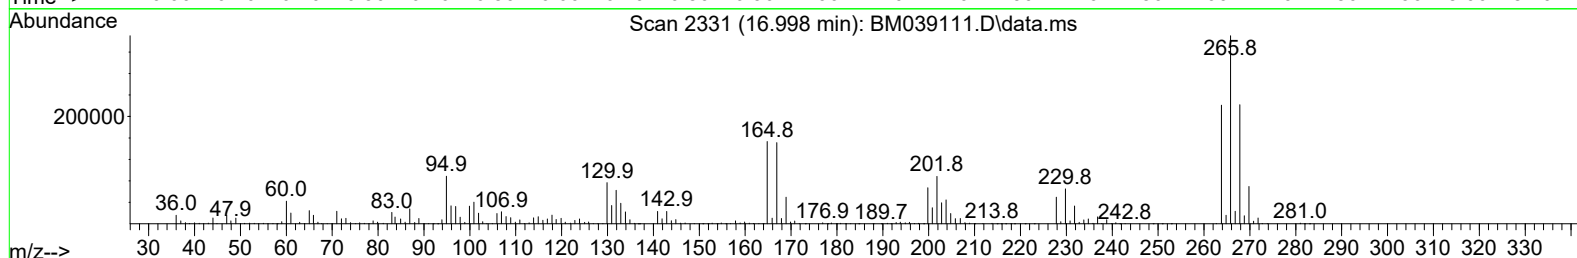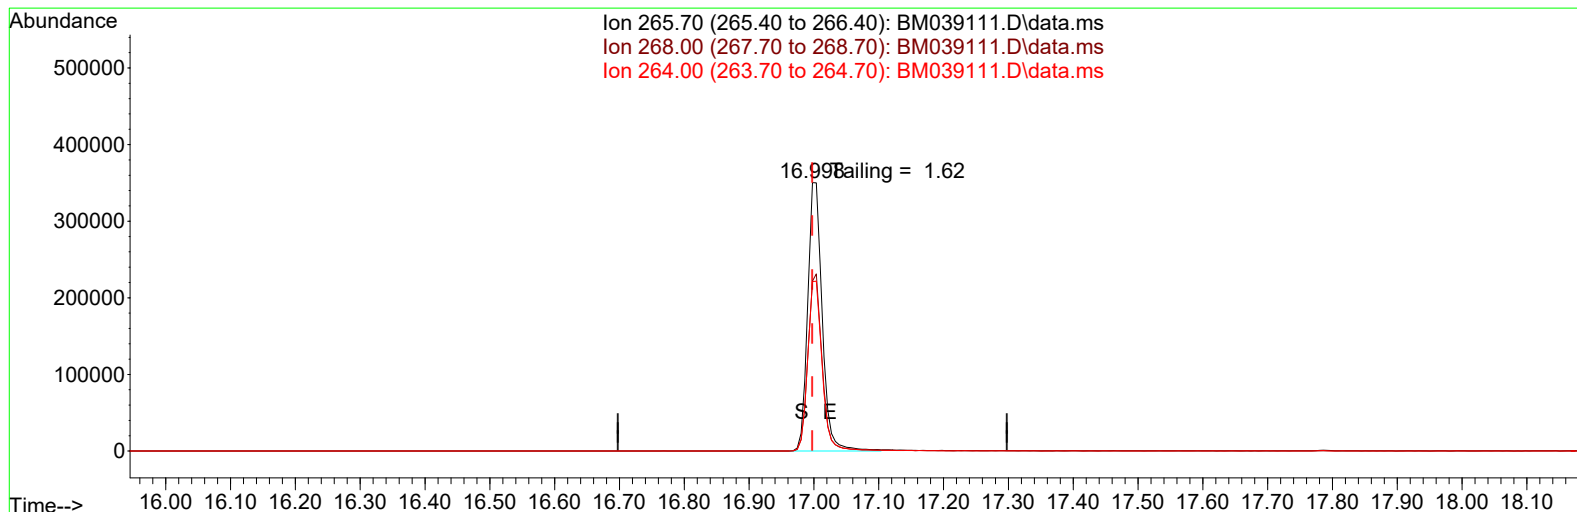

TIC: BM039111.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 91785.05 ng




response 549396

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.34
264.00	62.90	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032323\
Data File : BM039111.D
Acq On : 23 Mar 2023 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 24 07:06:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

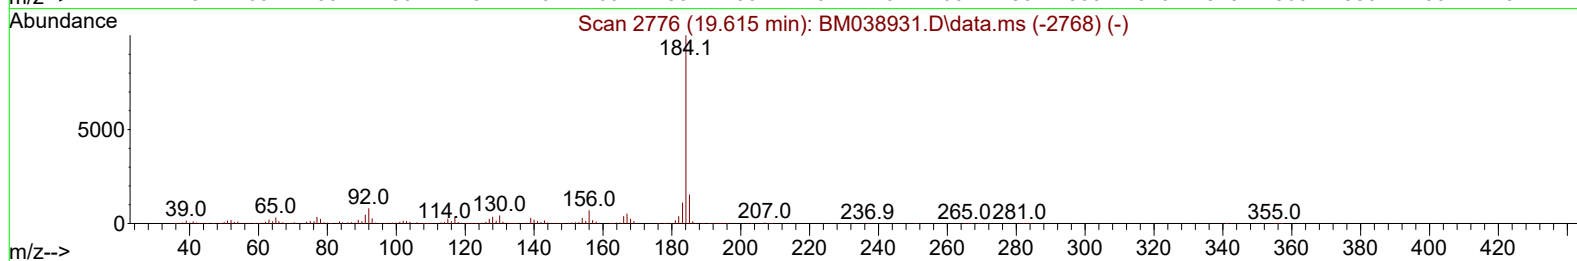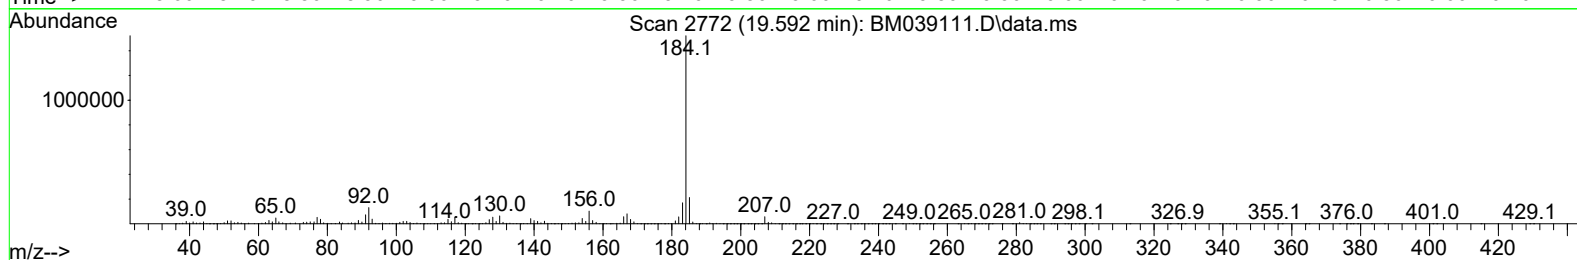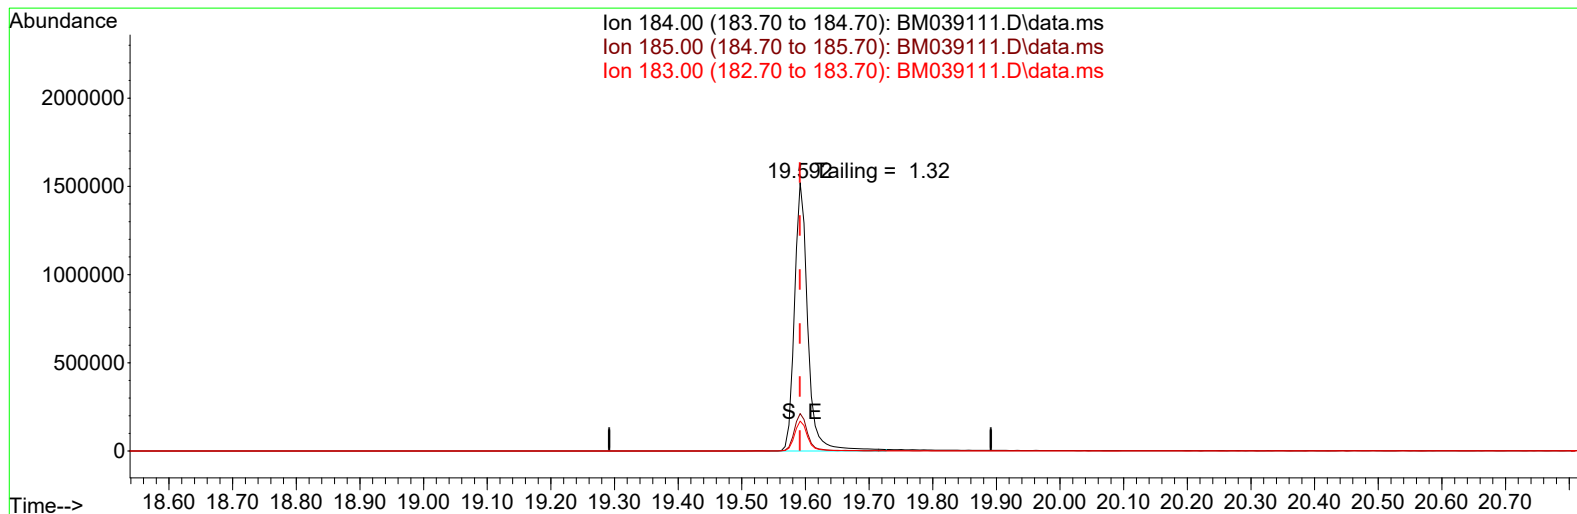

TIC: BM039111.D\data.ms

(77) Benzidine

19.592min (+ 0.000) 17645.31 ng

response 2243667

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	13.98
183.00	11.00	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2023	BNA_M	<u>BM039111.D</u>
Compound Name	Response	Retention Time
DDT	1511410	20.821
DDD	34881	20.386
DDE	1563	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36444	1547854	2.35

Instrument :
BNA_M
ClientSampleId :
DFTPP