


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032323\
Data File : BM039118.D
Acq On : 23 Mar 2023 15:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 22 03:36:20 2023

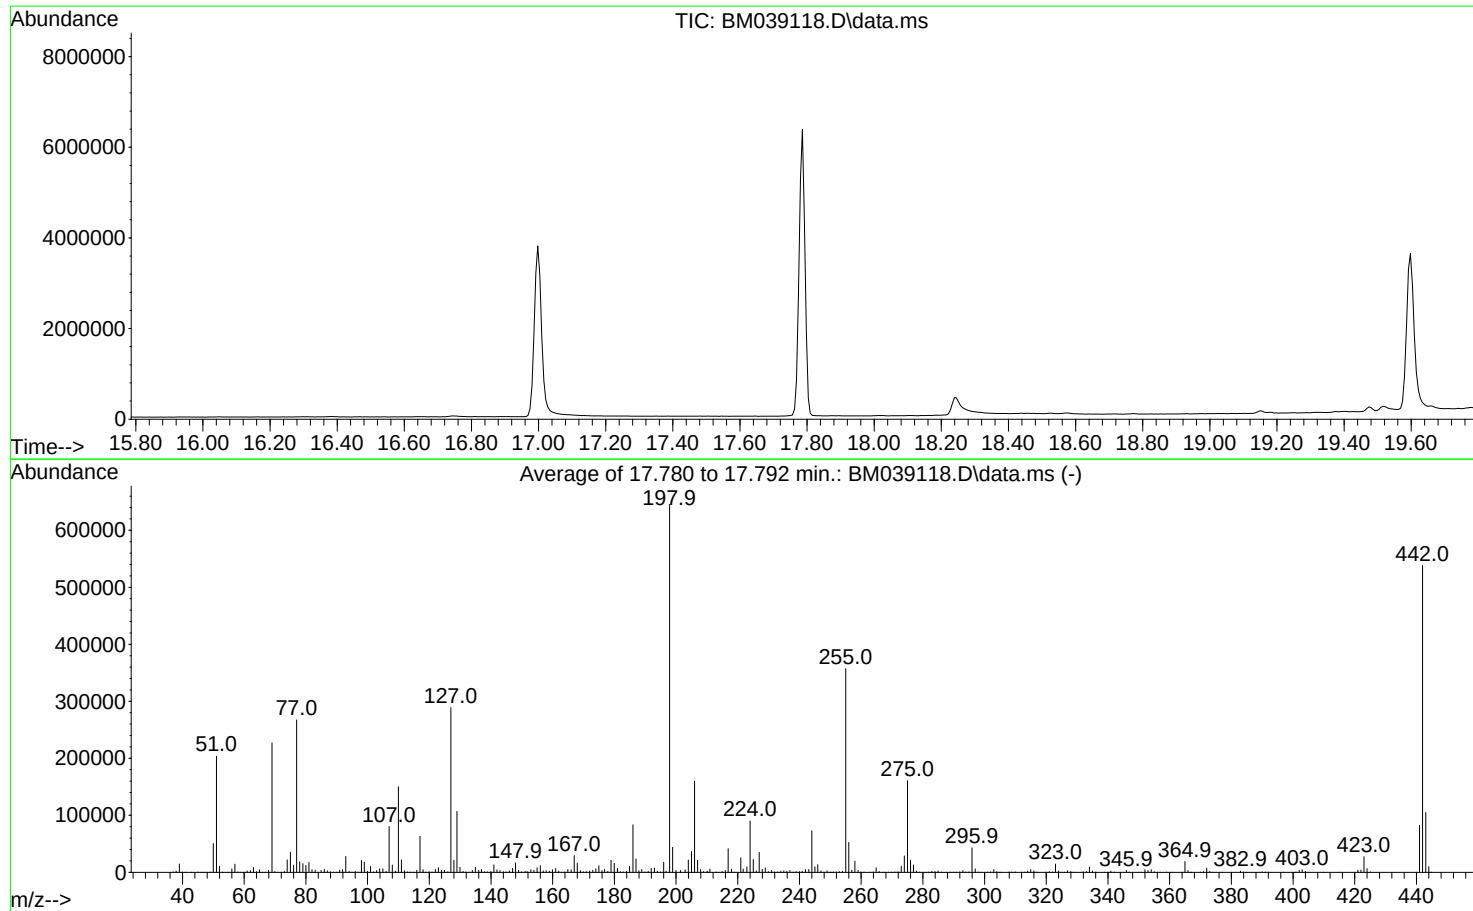




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	203555	PASS
68	69	0.00	2	1.4	3274	PASS
69	198	0.00	100	35.2	226932	PASS
70	69	0.00	2	0.5	1223	PASS
127	198	10	80	44.8	288906	PASS
197	198	0.00	2	0.3	1763	PASS
198	198	100	100	100.0	645483	PASS
199	198	5	9	6.8	43659	PASS
275	198	10	60	24.9	160725	PASS
365	198	1	100	2.9	19003	PASS
441	198	0.01	100	12.8	82536	PASS
442	442	50	100	100.0	538475	PASS
443	442	15	24	19.5	104741	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032323\
Data File : BM039118.D
Acq On : 23 Mar 2023 15:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 24 07:07:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

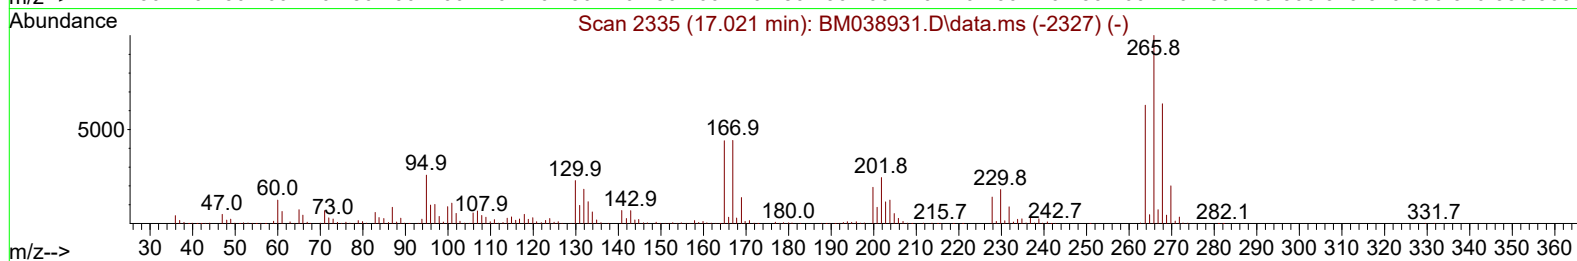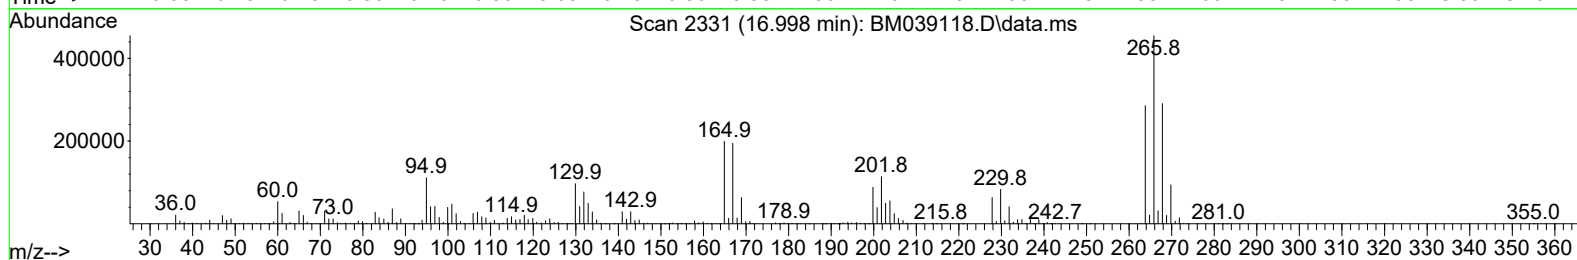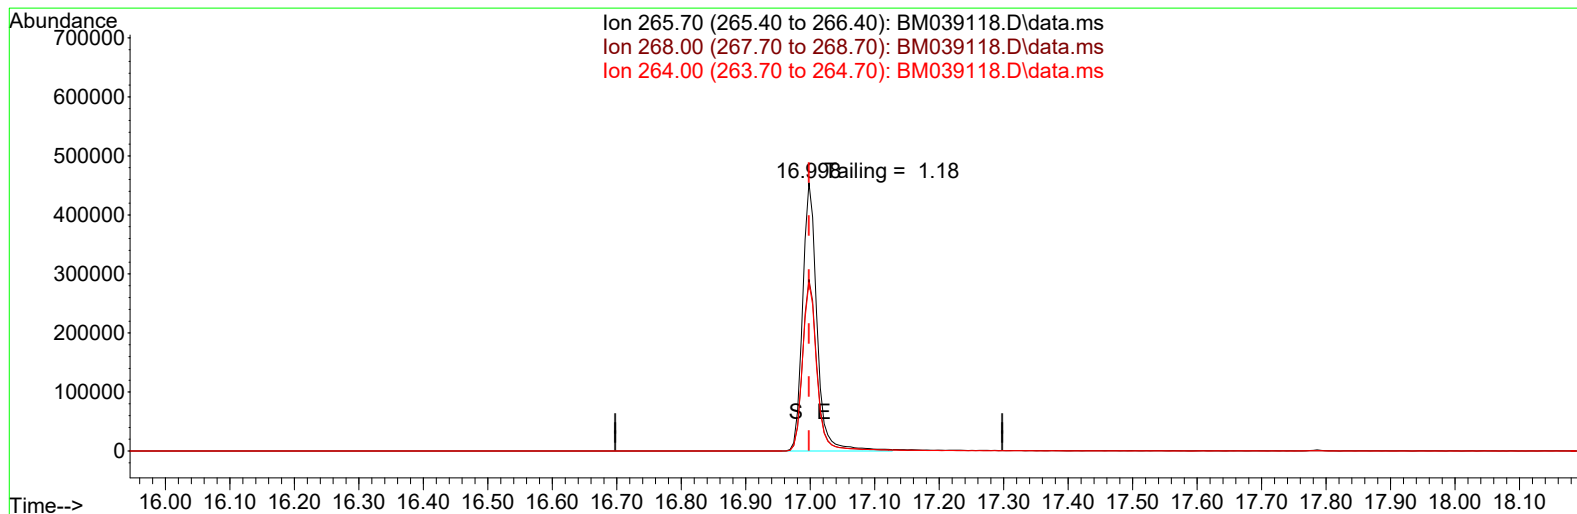

TIC: BM039118.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 98592.35 ng




response 714475

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.93
264.00	62.90	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032323\
Data File : BM039118.D
Acq On : 23 Mar 2023 15:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 24 07:07:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

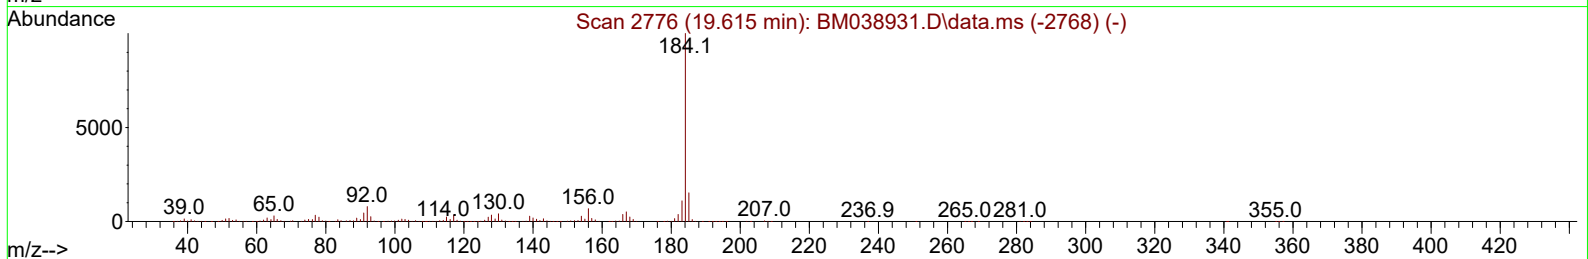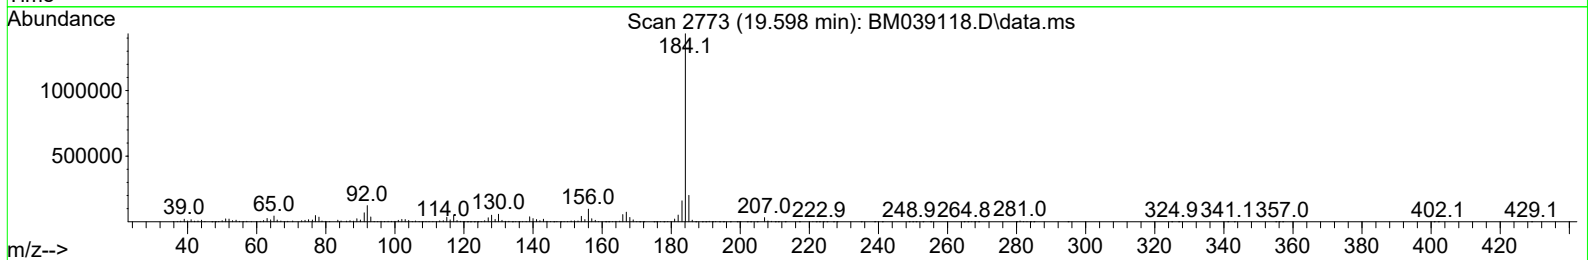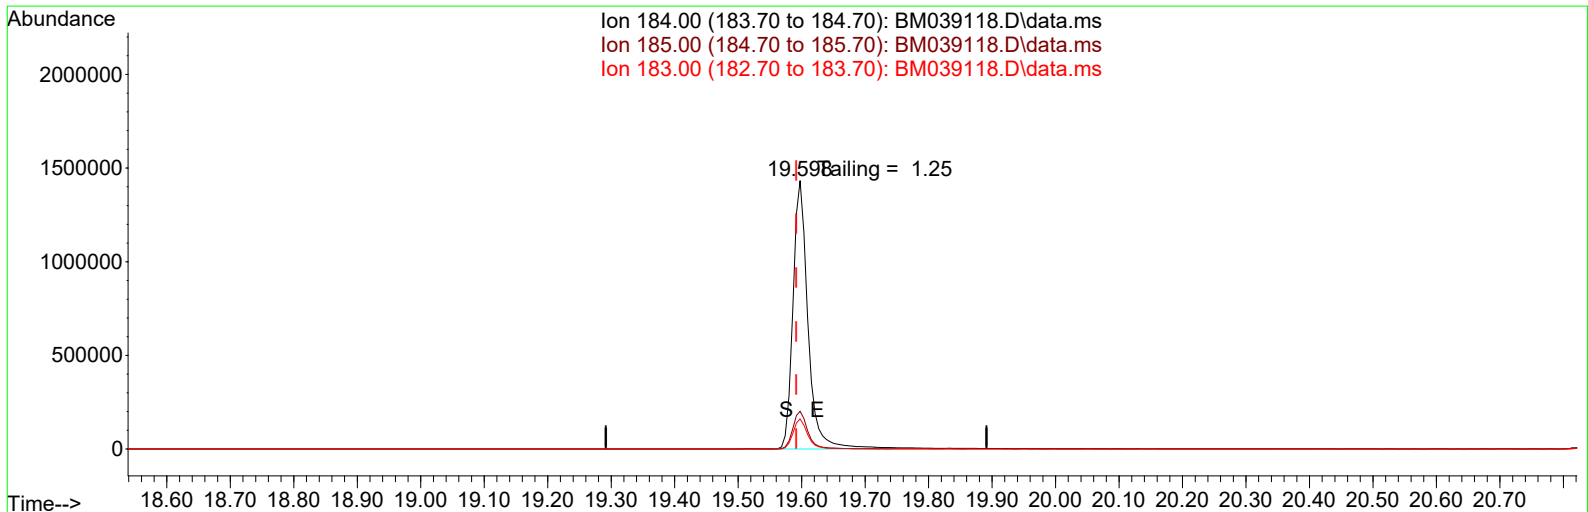

TIC: BM039118.D\data.ms

(77) Benzidine

19.598min (+ 0.006) 14102.96 ng

response 2386176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.08
183.00	11.00	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2023	BNA_M	<u>BM039118.D</u>
Compound Name	Response	Retention Time
DDT	1835874	20.821
DDD	54192	20.38
DDE	2094	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56286	1892160	2.97

Instrument :
BNA_M
ClientSampleId :
DFTPP