

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044738.D
Acq On : 22 Mar 2024 17:14
Operator : MA/JU
Sample : PB159682BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159682BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044738.D\data.ms




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.310	371	378	394	rBV	4388985	6573037	76.01%	13.680%
2	6.875	635	644	660	rBV	3942515	6360213	73.55%	13.237%
3	7.687	775	782	790	rBV	775504	1249763	14.45%	2.601%
4	8.851	971	980	990	rBV	2391858	4045505	46.78%	8.420%
5	10.463	1247	1254	1268	rBV	886900	1554707	17.98%	3.236%
6	12.945	1669	1676	1695	rBV	506084			

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044738.D
Acq On : 22 Mar 2024 17:14
Operator : MA/JU
Sample : PB159682BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159682BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

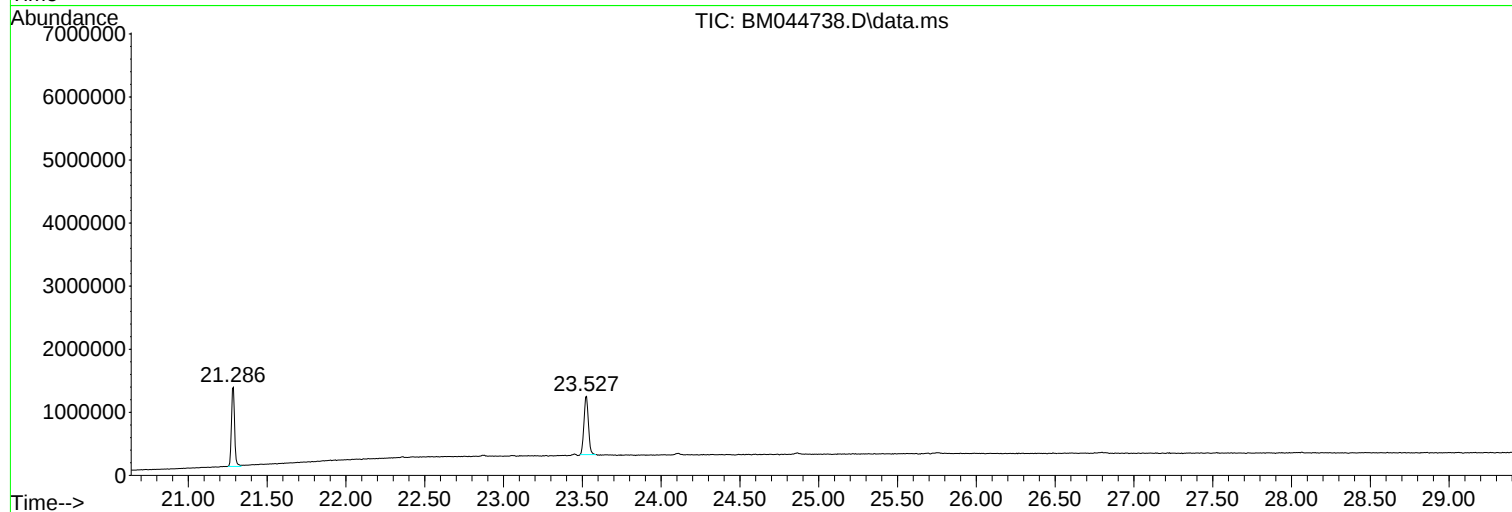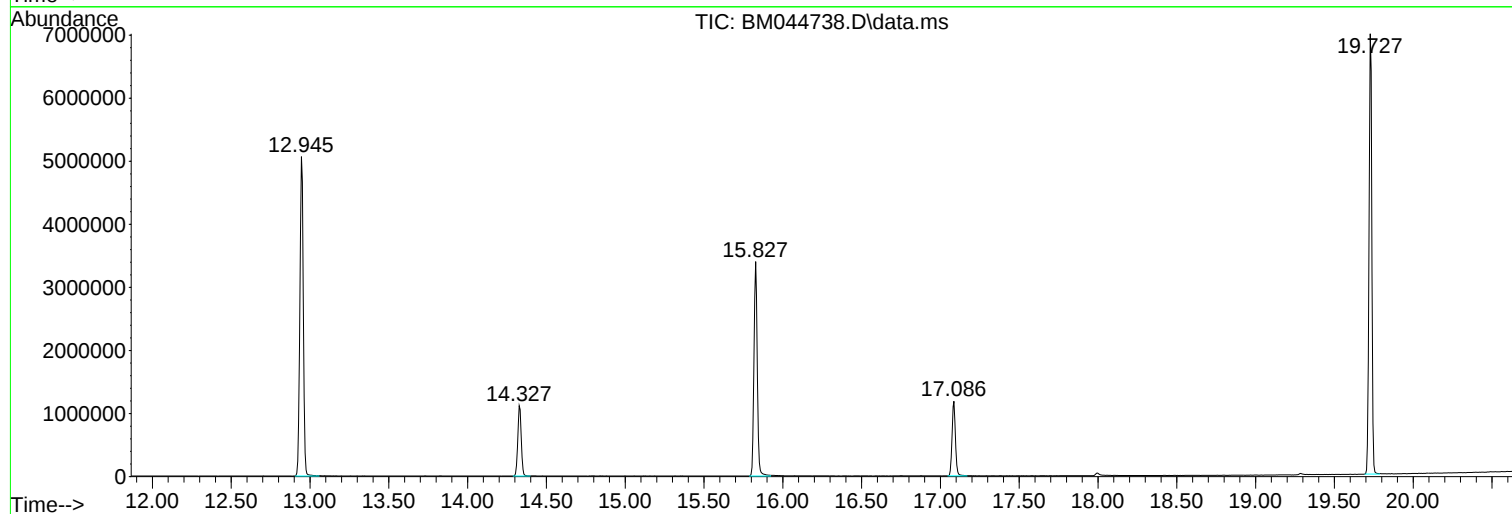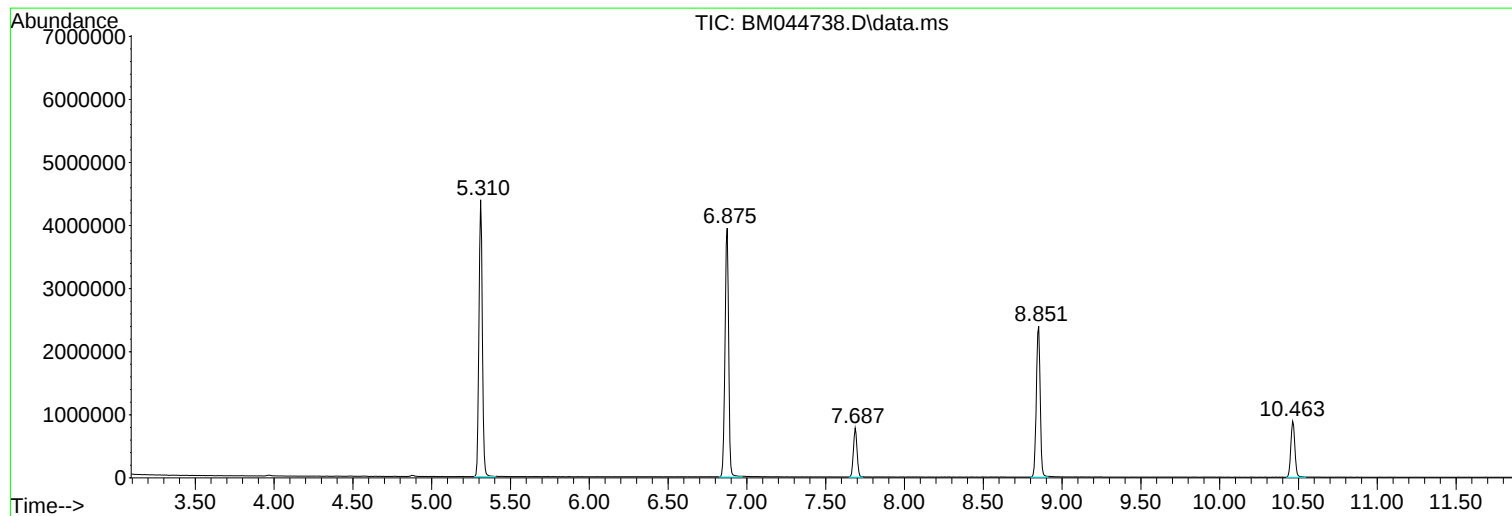

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044738.D
Acq On : 22 Mar 2024 17:14
Operator : MA/JU
Sample : PB159682BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159682BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044738.D
Acq On : 22 Mar 2024 17:14
Operator : MA/JU
Sample : PB159682BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159682BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------