

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
 Data File : BM044740.D
 Acq On : 22 Mar 2024 18:27
 Operator : MA/JU
 Sample : PB159703BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB159703BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.310	371	378	392	rBV	4103441	6204061	76.93%	13.720%
2	6.875	636	644	659	rBV	3599877	5977980	74.13%	13.220%
3	7.687	775	782	792	rBV	766869	1211335	15.02%	2.679%
4	8.851	971	980	994	rBV	2173324	3794081	47.05%	8.390%
5	10.463	1247	1254	1270	rBV	847558	1494598	18.53%	3.305%
6	12.945	1669	1676	1691	rBV	4711744	7099050	88.03%	15.699%
7	14.327	1905	1911	1923	rBV	1100161	1613936	20.01%	3.569%
8	15.827	2159	2166	2193	rBV	3174422	4650151	57.66%	10.283%
9	17.086	2372	2380	2396	rBV	1092303	1669166	20.70%	3.691%
10	19.727	2823	2829	2839	rBV	6446720	8064704	100.00%	17.835%
11	21.280	3088	3093	3102	rBV	1179691	1653895	20.51%	3.657%
12	23.527	3468	3475	3489	rVB	884320	1786597	22.15%	3.951%




Sum of corrected areas: 45219554

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044740.D
Acq On : 22 Mar 2024 18:27
Operator : MA/JU
Sample : PB159703BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159703BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

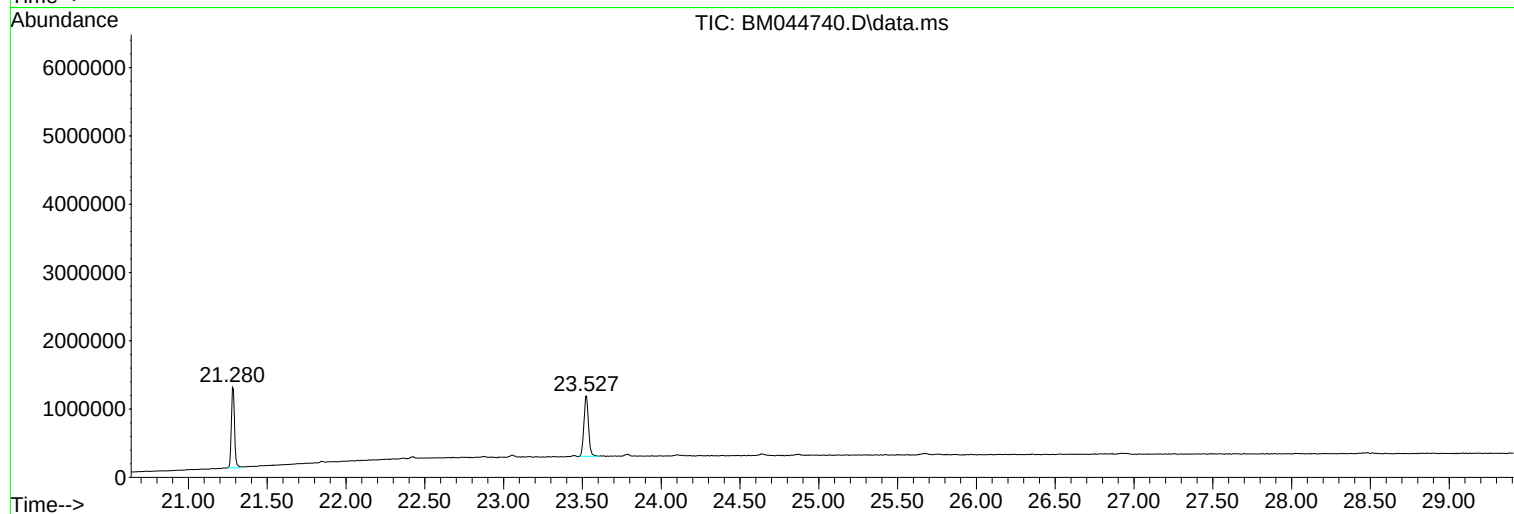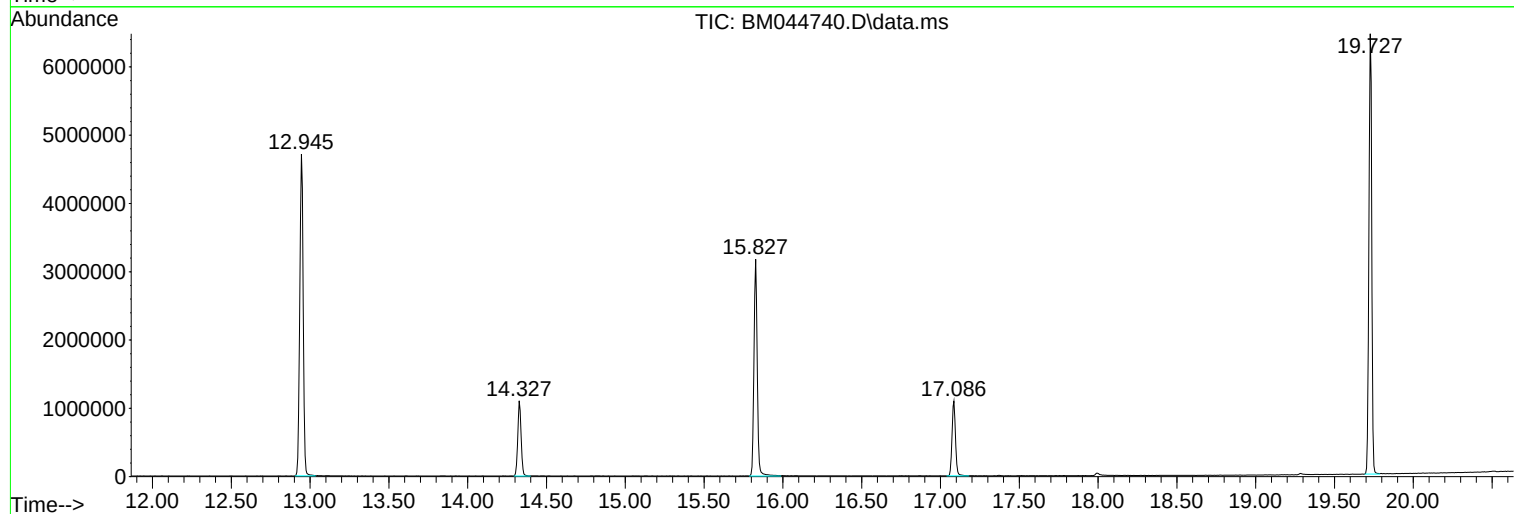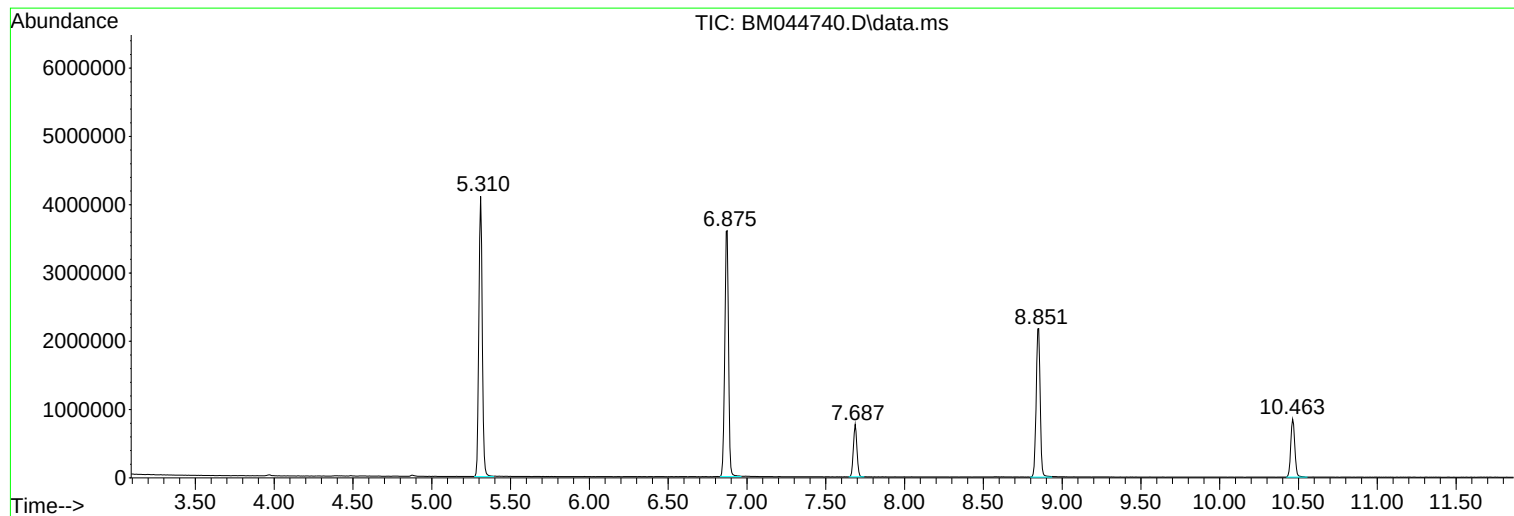

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044740.D
Acq On : 22 Mar 2024 18:27
Operator : MA/JU
Sample : PB159703BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159703BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044740.D
Acq On : 22 Mar 2024 18:27
Operator : MA/JU
Sample : PB159703BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159703BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------