

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044742.D
Acq On : 22 Mar 2024 19:39
Operator : MA/JU
Sample : PB159737BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159737BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.310	371	378	392	rBV	4075872	6157788	77.69%	13.716%
2	6.869	636	643	662	rBV	3622005	5959388	75.19%	13.274%
3	7.687	775	782	793	rBV	766502	1214249	15.32%	2.705%
4	8.845	970	979	990	rBV	2201663	3758666	47.42%	8.372%
5	10.463	1245	1254	1269	rBV	873000	1505749	19.00%	3.354%
6	12.945	1668	1676	1689	rBV	4737236	7059977	89.07%	15.725%
7	14.327	1904	1911	1924	rBV	1071548	1630014	20.57%	3.631%
8	15.827	2158	2166	2183	rBV	3177567	4623931	58.34%	10.299%
9	17.086	2371	2380	2391	rBV	1092507	1662782	20.98%	3.704%
10	19.727	2823	2829	2837	rBV	6258887	7926044	100.00%	17.654%
11	21.280	3088	3093	3102	rBV	1178768	1645066	20.76%	3.664%
12	23.521	3468	3474	3488	rVB	888785	1752717	22.11%	3.904%




Sum of corrected areas: 44896371

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044742.D
Acq On : 22 Mar 2024 19:39
Operator : MA/JU
Sample : PB159737BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

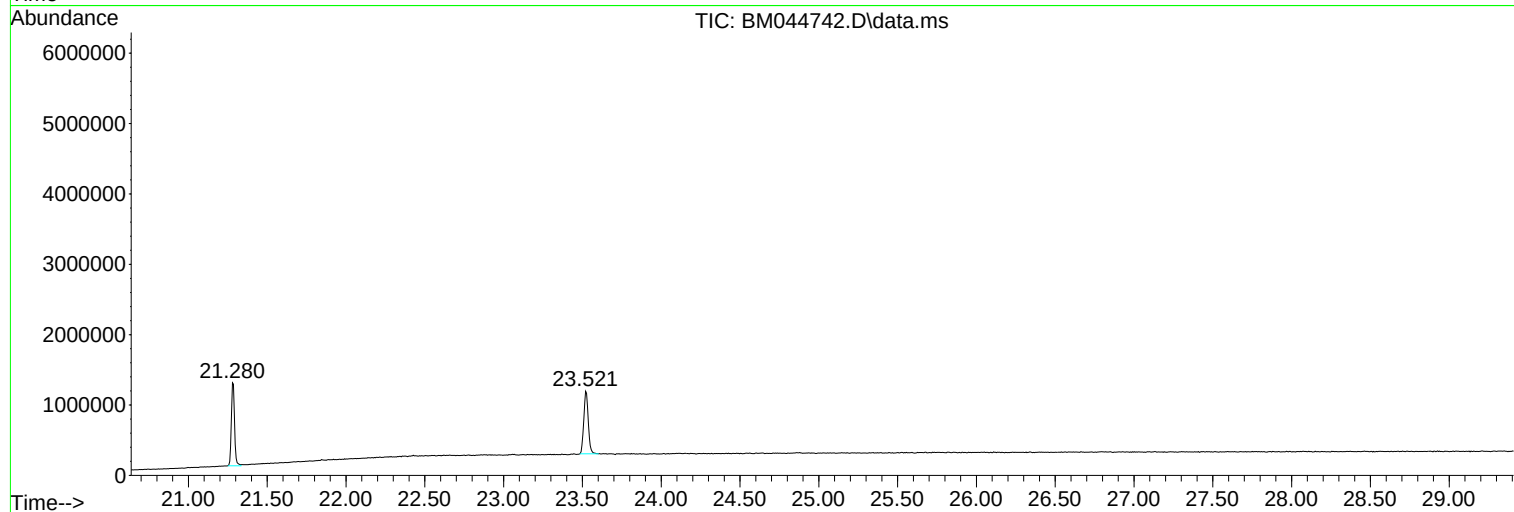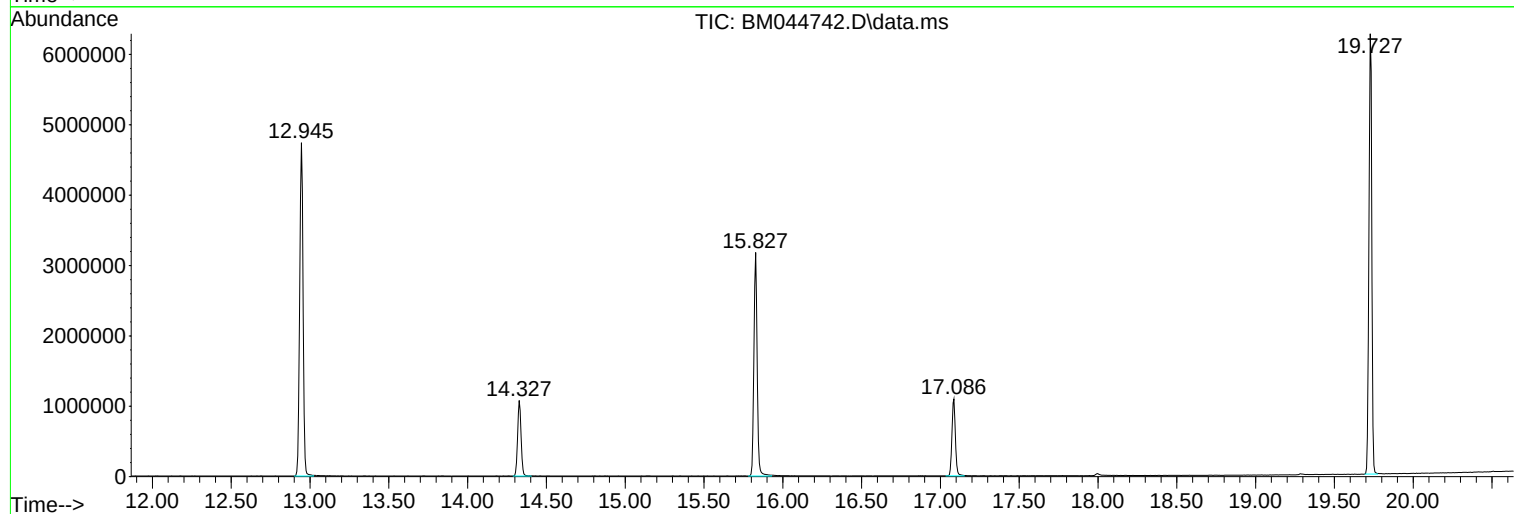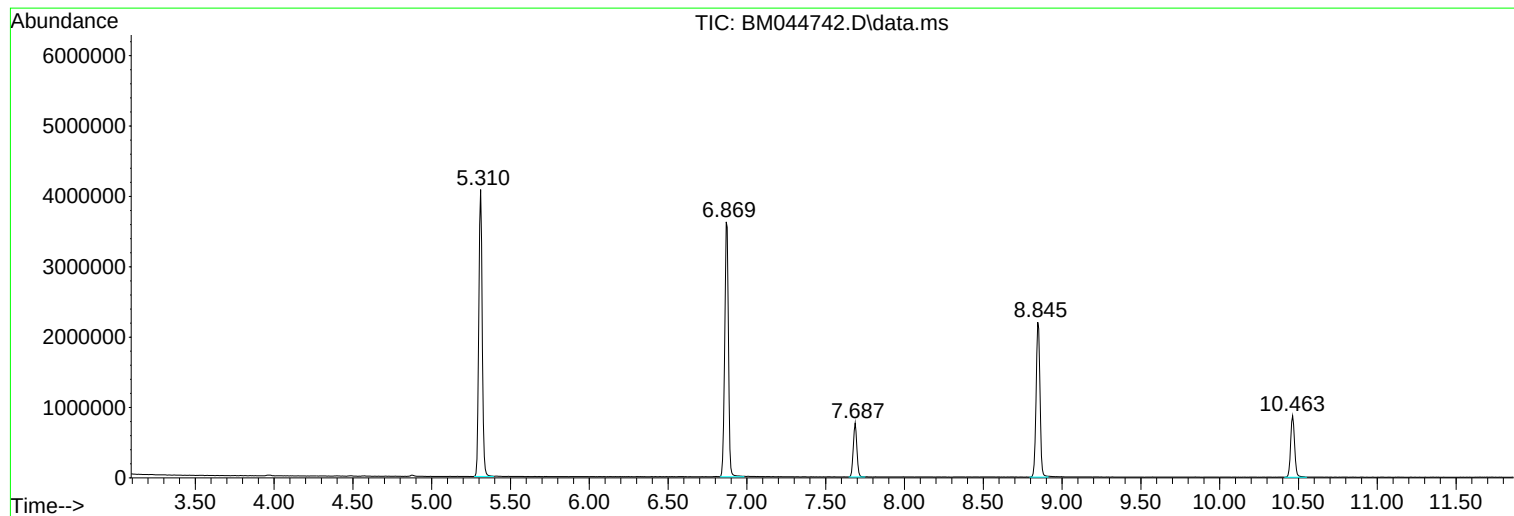

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044742.D
Acq On : 22 Mar 2024 19:39
Operator : MA/JU
Sample : PB159737BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044742.D
Acq On : 22 Mar 2024 19:39
Operator : MA/JU
Sample : PB159737BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------