

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
 Data File : BM044749.D
 Acq On : 22 Mar 2024 23:52
 Operator : MA/JU
 Sample : P1830-02 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-206

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.975	147	151	161	rVB5	10331	23278	1.16%	0.165%
2	5.310	371	378	391	rBV	272961	520750	25.92%	3.681%
3	6.869	637	643	657	rBV	258801	482596	24.02%	3.412%
4	7.687	775	782	796	rVB	765762	1317985	65.61%	9.317%
5	8.851	972	980	989	rBV	162498	302092	15.04%	2.136%
6	10.463	1246	1254	1268	rBV	971190	1660615	82.66%	11.739%
7	12.945	1669	1676	1688	rBV	415392	623744	31.05%	4.409%
8	13.228	1717	1724	1731	rVB4	15925	31277	1.56%	0.221%
9	14.327	1904	1911	1919	rBV	1261656	1857083	92.44%	13.128%
10	15.827	2159	2166	2173	rBV	245190	374672	18.65%	2.649%
11	17.086	2373	2380	2392	rBV	1277346	1992790	99.20%	14.087%
12	17.992	2529	2534	2544	rBV	93622	169737	8.45%	1.200%
13	19.280	2750	2753	2758	rBV3	54381	89547	4.46%	0.633%
14	19.727	2824	2829	2836	rBV	557494	757699	37.72%	5.356%
15	21.280	3089	3093	3098	rBV	1487972	1933189	96.23%	13.666%
16	23.521	3469	3474	3482	rVB	1037494	2008911	100.00%	14.201%




Sum of corrected areas: 14145965

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044749.D
Acq On : 22 Mar 2024 23:52
Operator : MA/JU
Sample : P1830-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

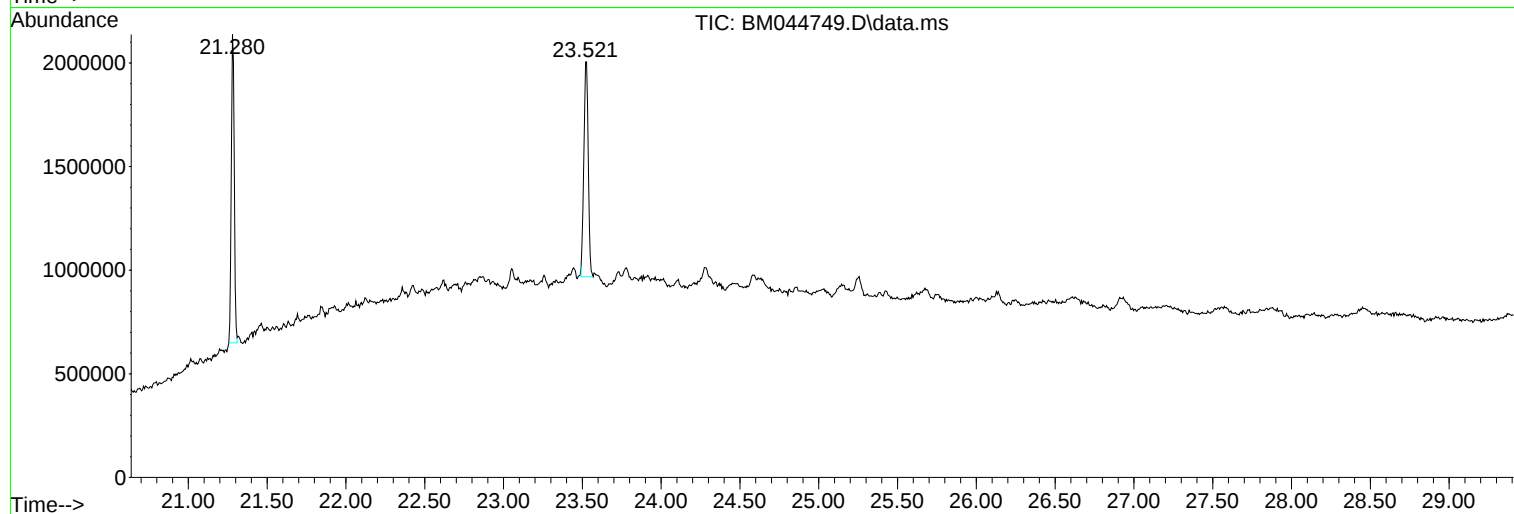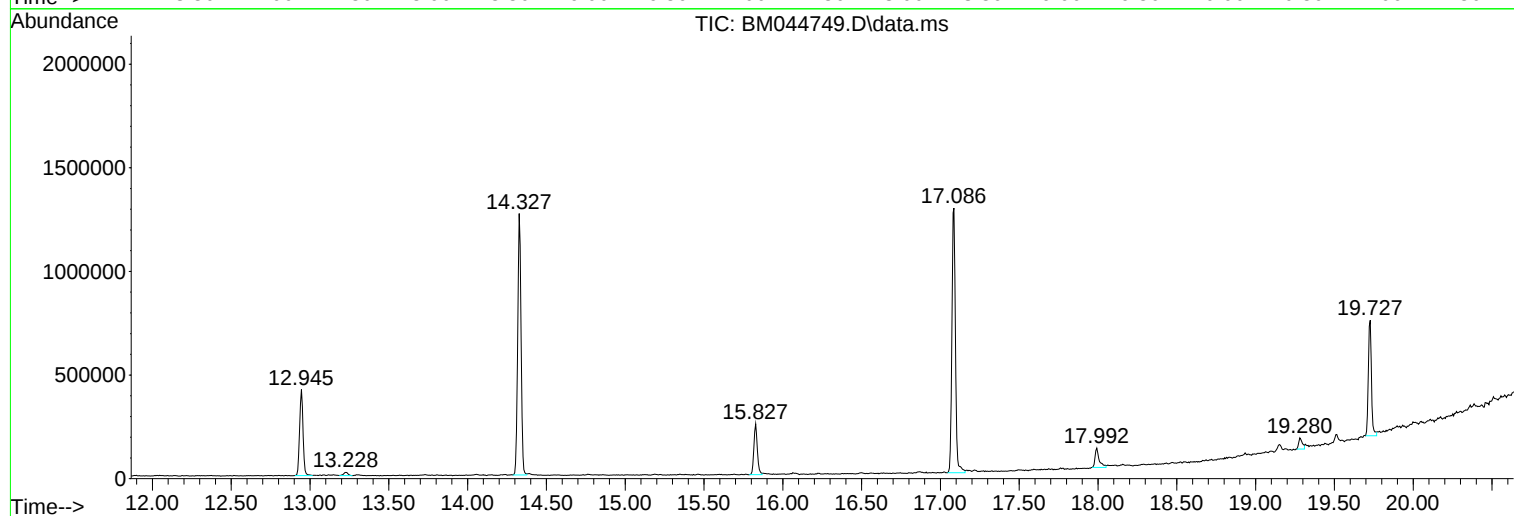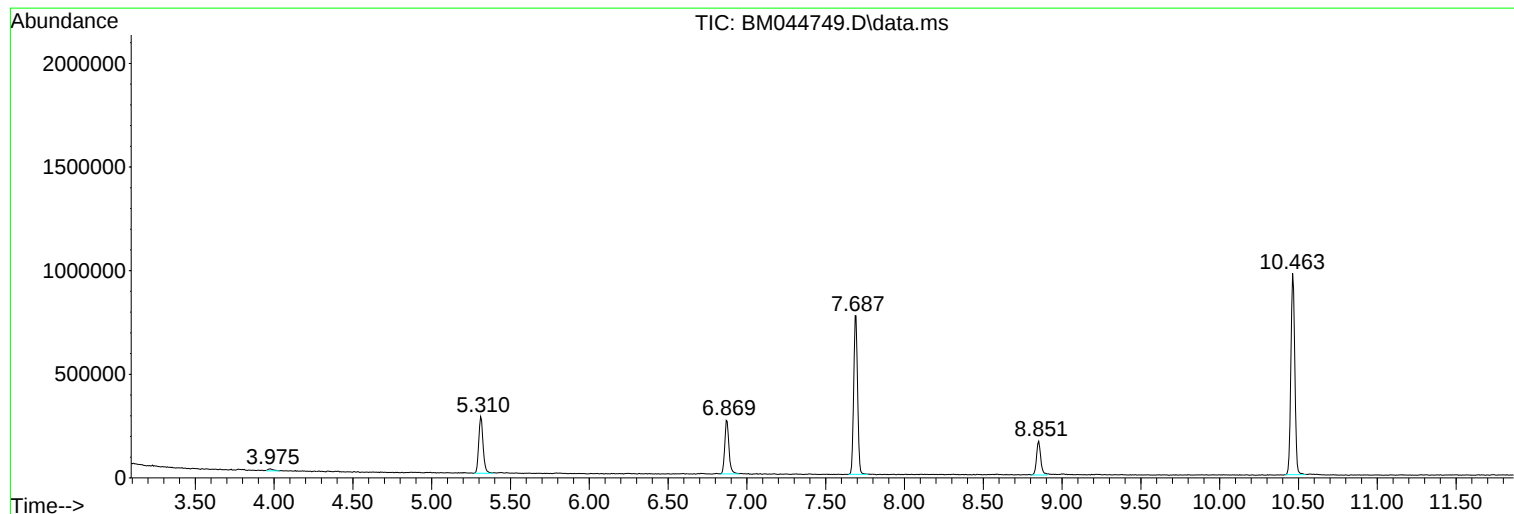

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044749.D
Acq On : 22 Mar 2024 23:52
Operator : MA/JU
Sample : P1830-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044749.D
Acq On : 22 Mar 2024 23:52
Operator : MA/JU
Sample : P1830-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc