


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044730.D
Acq On : 22 Mar 2024 12:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 02:28:24 2024

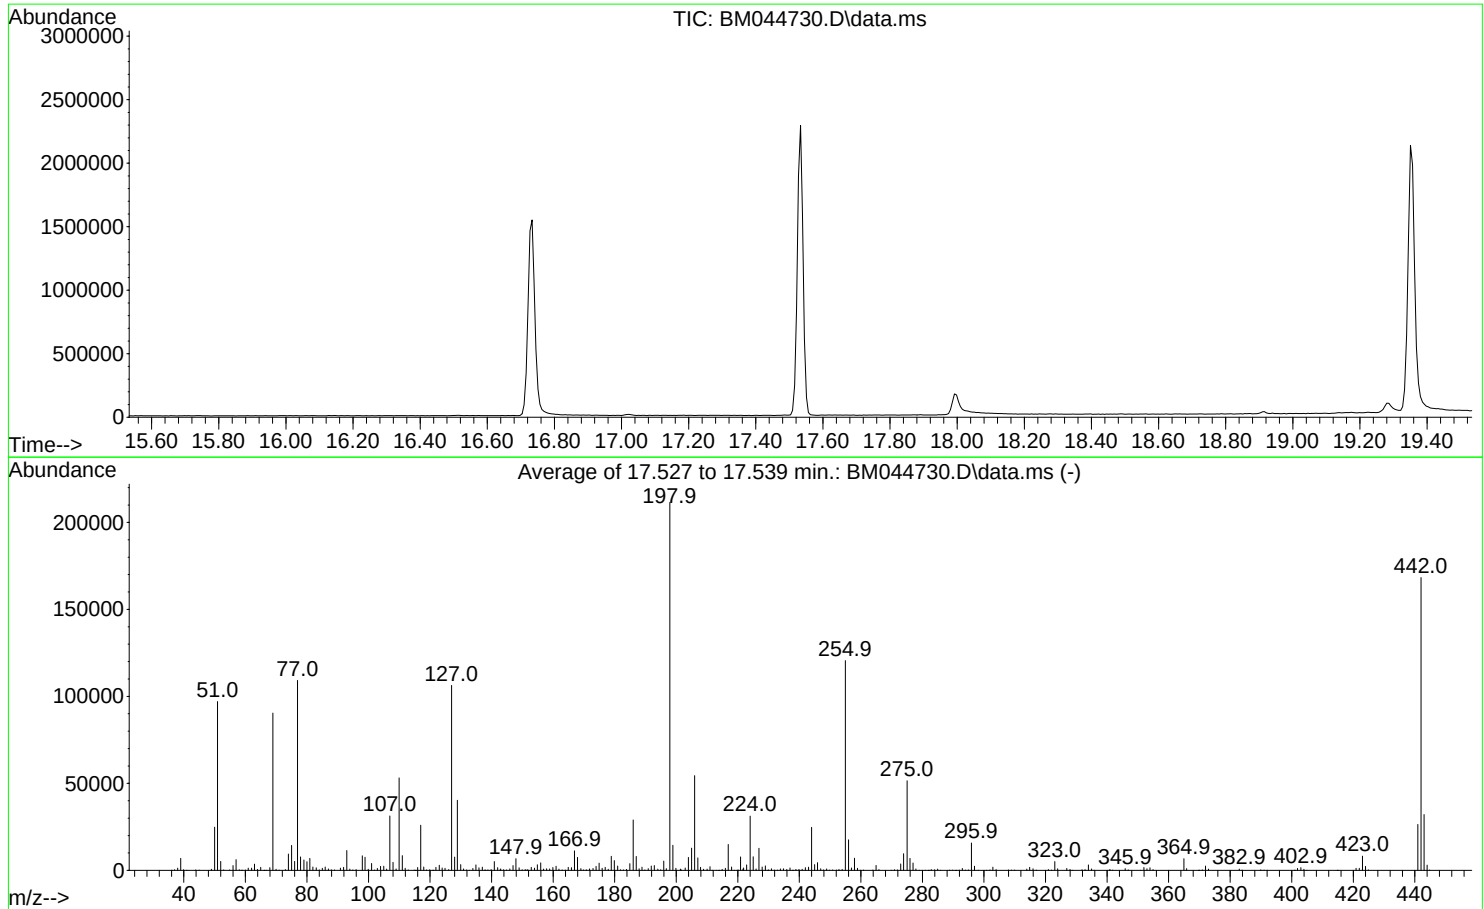




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	97062	PASS
68	69	0.00	2	1.7	1535	PASS
69	198	0.00	100	42.8	90416	PASS
70	69	0.00	2	0.7	620	PASS
127	198	10	80	50.3	106296	PASS
197	198	0.00	2	0.5	989	PASS
198	198	100	100	100.0	211435	PASS
199	198	5	9	6.8	14473	PASS
275	198	10	60	24.4	51485	PASS
365	198	1	100	3.2	6713	PASS
441	198	0.01	100	12.5	26437	PASS
442	442	50	100	100.0	168339	PASS
443	442	15	24	19.0	32061	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
Data File : BM044730.D
Acq On : 22 Mar 2024 12:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 22 20:24:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

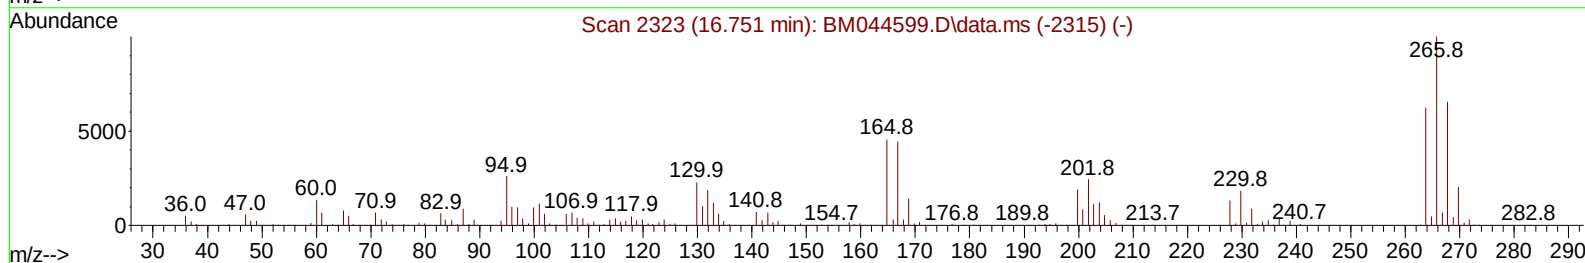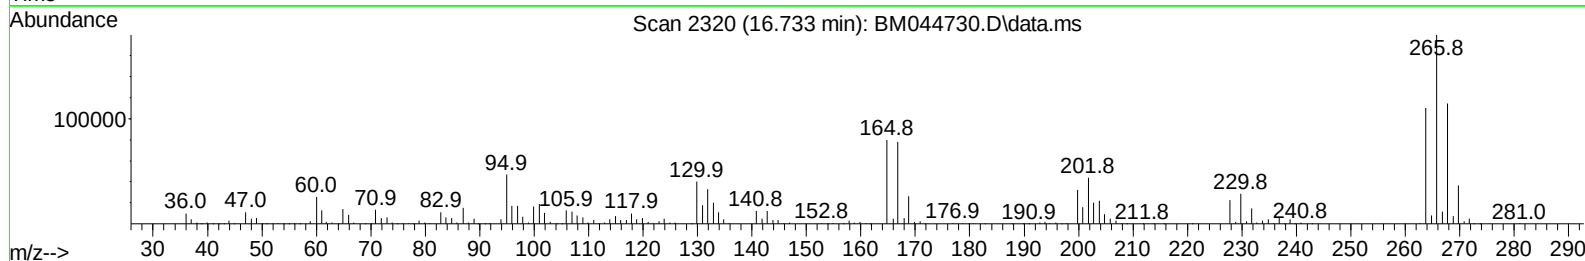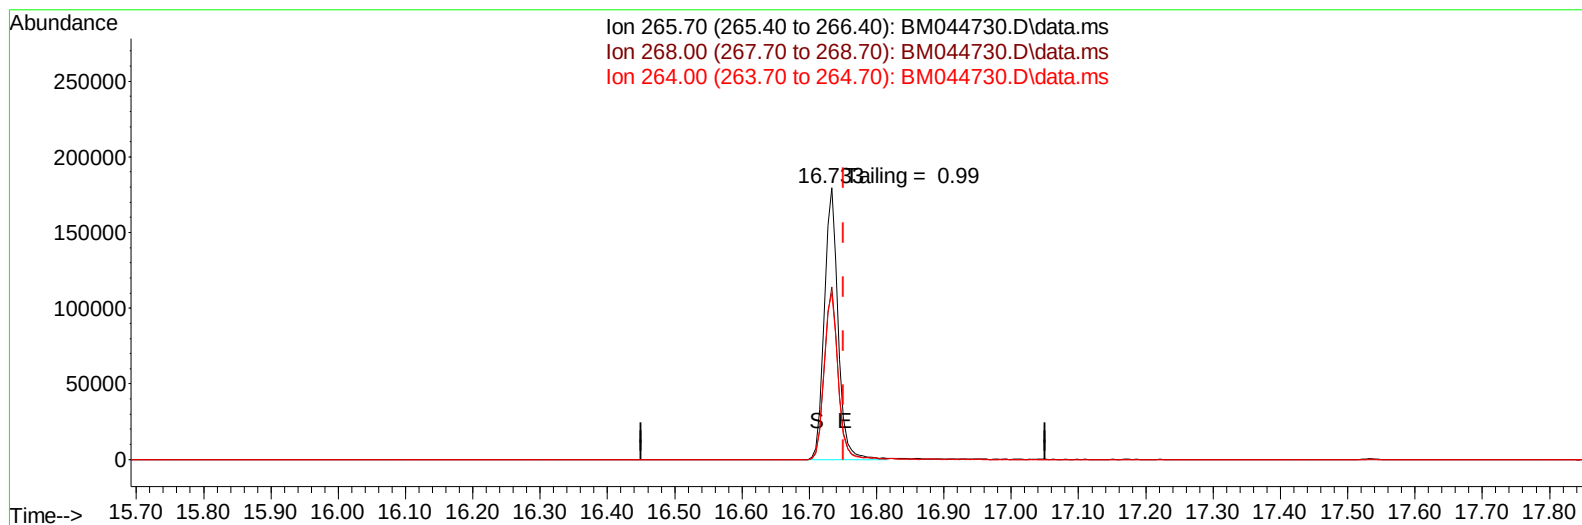

TIC: BM044730.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.017) 140964.02 ng




response 255308

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	63.62
264.00	62.30	61.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032324\
 Data File : BM044730.D
 Acq On : 22 Mar 2024 12:12
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 20:24:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 14 02:28:24 2024
 Response via : Initial Calibration

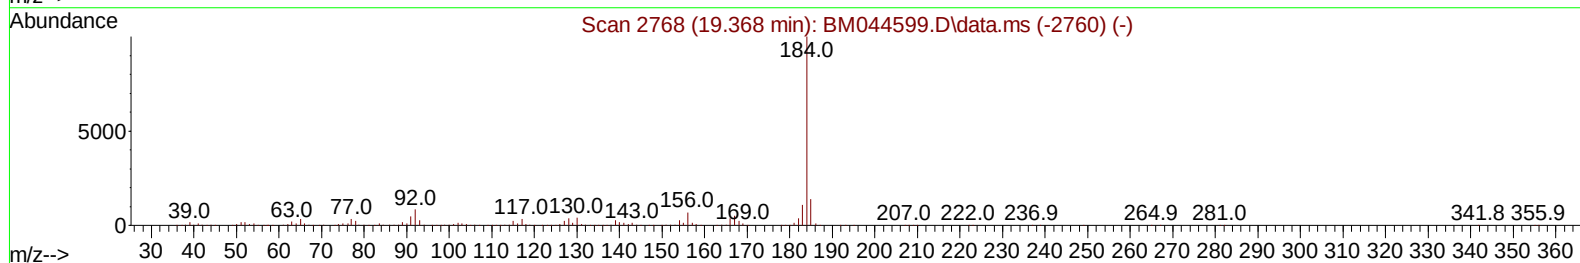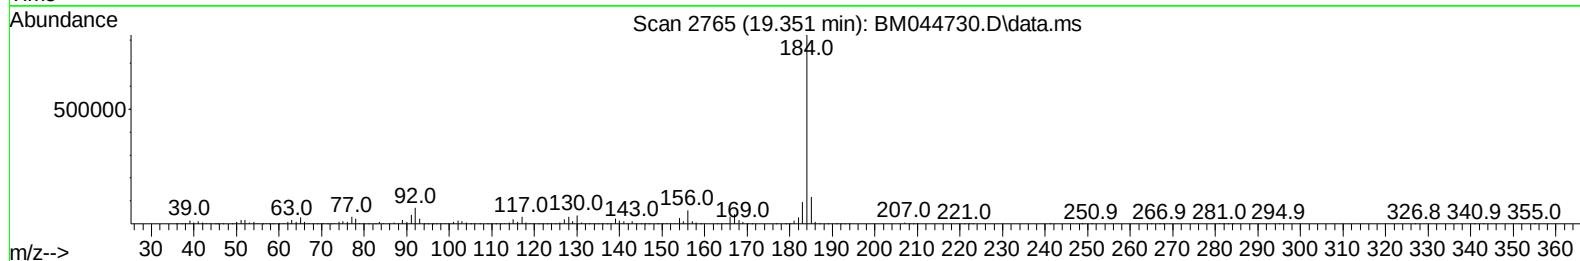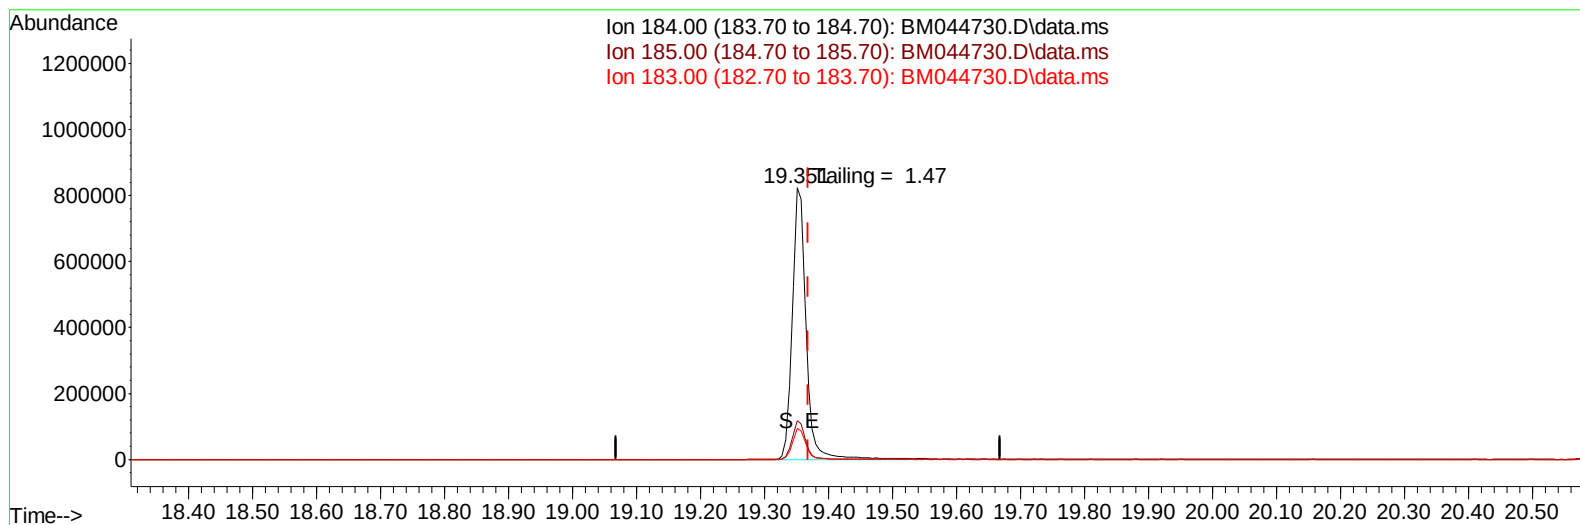

TIC: BM044730.D\data.ms

(77) Benzidine

19.351min (-0.017) 193701.98 ng

response 1226536

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.23
183.00	10.90	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2024	BNA_M	<u>BM044730.D</u>
Compound Name	Response	Retention Time
DDT	641510	20.586
DDD	21060	20.145
DDE	1208	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22268	663778	3.35

Instrument :
BNA_M
ClientSampleId :
DFTPP