


Data Path : Z:\HPCHEM1\BNA M\Data\BM032416\
 Data File : BM004750.D
 Acq On : 24 Mar 2016 10:14
 Operator : UM/SJ
 Sample : DFTPP39
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP39

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM010216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 13:33:21 2016

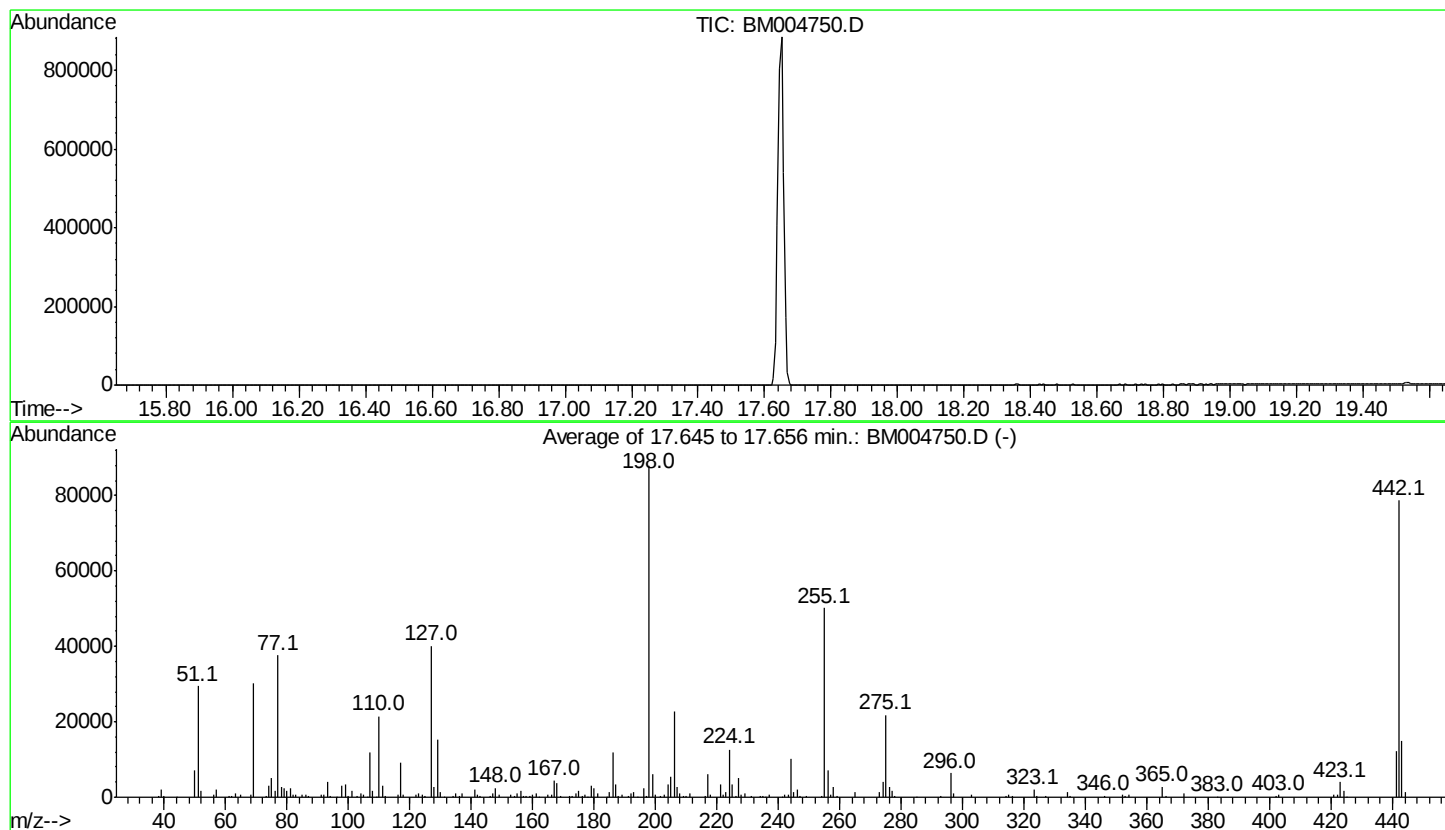

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	29474	PASS
68	69	0.00	2	1.9	567	PASS
69	198	0.00	100	34.2	30090	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	40058	PASS
197	198	0.00	2	0.4	342	PASS
198	198	100	100	100.0	87922	PASS
199	198	5	9	6.8	6010	PASS
275	198	10	60	24.9	21858	PASS
365	198	1	100	3.1	2739	PASS
441	442	0.01	24	15.5	12157	PASS
442	198	50	100	89.4	78624	PASS
443	442	15	24	19.2	15075	PASS

Scan 2537 (17.609 min): BM004750.D
DFTPP39

m/z	Abundance
44.00	626.0
207.10	502.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
38.00	392.0
39.00	2478.0
40.00	315.0
44.00	653.0
50.00	8853.0
51.10	36360.0
52.00	1838.0
56.00	1022.0
57.00	2551.0
61.00	449.0
62.00	514.0
63.00	1404.0
65.00	755.0
68.00	714.0
69.00	36464.0
73.00	313.0
74.00	3607.0
75.00	6177.0
76.00	2460.0
77.10	45544.0
78.00	3442.0
79.00	2720.0
80.00	2060.0
81.00	2944.0
82.00	725.0
82.90	780.0
84.90	631.0
86.00	844.0
87.00	432.0
91.00	629.0
92.00	882.0
93.00	4836.0
94.00	306.0
98.00	3680.0
99.00	4392.0
100.00	353.0
101.00	1846.0
103.00	530.0
104.00	1207.0
105.00	906.0
106.00	384.0
107.00	14173.0
108.00	2064.0
109.00	383.0
110.00	25392.0
111.00	3831.0
112.00	423.0
116.00	604.0
117.00	11025.0
118.00	979.0
122.00	851.0
123.00	1471.0
124.00	672.0
125.00	600.0
127.00	45960.0
128.00	3547.0
129.00	17552.0
130.00	1580.0
134.00	463.0
135.00	1435.0
136.00	560.0
137.00	1100.0
141.00	2106.0
141.90	770.0
143.00	477.0
146.10	343.0
147.00	1261.0
148.00	2771.0
149.00	793.0
153.00	849.0
154.00	492.0
155.00	1167.0
156.10	1965.0
157.00	322.0
158.00	441.0
159.00	303.0
160.00	622.0
161.00	1070.0
162.00	336.0
165.00	755.0
166.00	756.0
167.00	4897.0
168.00	4680.0
169.00	675.0
171.90	385.0
173.00	505.0
174.00	967.0
175.10	1784.0
176.00	379.0
177.00	763.0
179.00	3353.0
180.00	2732.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

181.00	1142.0
184.00	335.0
185.00	1660.0
186.00	13272.0
187.00	3608.0
188.00	560.0
189.00	796.0
191.00	408.0
192.00	1119.0
193.00	1264.0
194.00	307.0
196.00	2527.0
196.80	536.0
198.00	95960.0
199.00	6753.0
200.00	587.0
201.50	379.0
203.00	647.0
204.00	3494.0
205.10	5761.0
206.10	24592.0
207.00	3619.0
208.00	838.0
209.00	341.0
210.10	374.0
211.00	1010.0
216.00	455.0
217.00	6313.0
218.00	827.0
221.10	3413.0
221.90	844.0
223.00	1516.0
224.10	13373.0
225.10	3356.0
226.00	504.0
227.00	5515.0
228.00	839.0
229.00	1197.0
231.00	422.0
234.00	369.0
235.00	392.0
237.00	840.0
242.00	676.0
243.00	732.0
244.10	10280.0
245.00	1454.0
246.00	1974.0
247.00	406.0
249.00	343.0
254.10	387.0
255.10	52224.0
256.10	7663.0
257.00	742.0
258.00	2885.0
259.00	431.0
265.00	1231.0
273.00	1477.0
274.00	3966.0
275.10	21792.0
276.10	3105.0
277.00	1878.0
278.00	472.0
293.00	399.0
296.00	6070.0
297.00	930.0
303.00	649.0
314.00	335.0
315.00	650.0
316.00	346.0
323.10	1897.0
324.00	301.0
327.00	350.0
334.00	1154.0
335.00	382.0
346.00	411.0
352.00	546.0
353.00	433.0
354.00	506.0
365.00	2337.0
366.10	351.0
372.10	1003.0
402.00	535.0
403.00	569.0
421.00	557.0
422.10	513.0
423.10	3374.0
424.10	1630.0
441.10	10318.0
442.10	66840.0
443.10	13117.0
444.00	1244.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
38.00	353.0
39.00	2324.0
40.00	336.0
44.00	653.0
50.10	8209.0
51.10	34024.0
52.00	1892.0
56.00	921.0
57.00	2428.0
61.00	385.0
62.00	527.0
63.00	1376.0
65.00	612.0
68.00	599.0
69.00	34688.0
73.10	370.0
74.00	3514.0
75.00	5700.0
76.10	1969.0
77.10	43840.0
78.10	2976.0
79.00	2542.0
80.00	1934.0
81.00	3000.0
82.00	754.0
83.00	766.0
85.00	737.0
86.00	797.0
87.00	382.0
91.00	635.0
92.00	798.0
93.00	4713.0
94.00	397.0
96.00	304.0
98.00	3397.0
99.00	3637.0
100.00	399.0
101.00	1856.0
103.00	473.0
104.00	980.0
105.00	949.0
107.00	13399.0
108.00	2051.0
110.00	24920.0
111.00	3549.0
111.90	393.0
116.00	674.0
117.00	10727.0
117.90	746.0
122.00	887.0
123.00	1437.0
124.00	814.0
125.00	572.0
127.00	47096.0
128.00	3342.0
129.00	17800.0
130.00	1392.0
131.00	397.0
133.90	452.0
135.00	1332.0
136.00	628.0
137.00	999.0
141.00	2205.0
142.00	798.0
143.00	478.0
146.00	482.0
147.00	1255.0
148.00	2915.0
149.00	718.0
153.00	714.0
154.00	487.0
155.00	1185.0
156.00	2026.0
157.00	348.0
158.00	410.0
159.00	328.0
160.00	712.0
161.00	1149.0
164.90	849.0
166.00	780.0
167.00	4992.0
168.00	4089.0
169.00	625.0
172.00	448.0
173.00	578.0
174.00	1101.0
175.00	2078.0
176.10	418.0
177.00	948.0
177.90	333.0
179.00	3495.0
180.00	2768.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

181.00	1312.0
185.00	1747.0
186.00	13824.0
187.00	4316.0
188.00	578.0
189.00	797.0
191.00	433.0
192.00	1247.0
193.00	1391.0
196.00	2883.0
197.10	671.0
198.00	104224.0
199.00	7034.0
200.00	664.0
201.60	381.0
203.00	736.0
204.10	4022.0
205.10	6693.0
206.10	27440.0
207.10	3906.0
208.00	996.0
209.00	321.0
210.00	331.0
211.00	1092.0
216.00	552.0
217.00	7175.0
218.00	900.0
221.00	4017.0
221.80	892.0
223.00	1586.0
224.10	15255.0
225.10	4085.0
226.00	435.0
227.00	5995.0
228.00	1010.0
229.00	1346.0
231.10	510.0
234.00	369.0
235.00	470.0
235.90	335.0
237.00	793.0
241.00	305.0
242.00	737.0
243.10	906.0
244.10	12482.0
245.10	1736.0
246.00	2165.0
247.00	499.0
249.00	419.0
254.00	372.0
255.00	60104.0
256.00	8769.0
257.00	837.0
258.00	3463.0
259.00	506.0
265.00	1510.0
273.00	1858.0
274.00	4842.0
275.10	26696.0
276.10	3306.0
277.00	2102.0
278.00	439.0
285.00	390.0
293.00	516.0
296.00	7976.0
297.00	958.0
303.10	1014.0
314.00	311.0
315.00	886.0
316.00	582.0
323.10	2343.0
324.10	531.0
327.00	497.0
334.10	1732.0
335.00	375.0
346.00	497.0
352.10	750.0
353.00	524.0
354.00	710.0
365.00	3407.0
366.00	503.0
372.10	1404.0
383.00	355.0
402.00	507.0
403.00	853.0
421.00	719.0
422.00	696.0
423.10	4873.0
424.10	1909.0
425.00	351.0
441.10	14636.0
442.10	95816.0
443.10	18896.0
444.00	1779.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.00	1241.0
44.00	615.0
50.00	4385.0
51.10	18040.0
52.00	959.0
56.00	491.0
57.00	1258.0
63.00	758.0
65.00	419.0
68.00	388.0
69.00	19120.0
74.00	2125.0
75.00	3178.0
76.00	1102.0
77.10	23472.0
78.00	1719.0
79.00	1409.0
80.00	1152.0
81.00	1670.0
82.00	368.0
83.00	425.0
85.00	474.0
86.00	516.0
90.90	380.0
92.00	412.0
93.00	2523.0
98.00	2134.0
99.00	2163.0
100.90	927.0
104.00	522.0
105.00	526.0
107.00	7647.0
108.00	1209.0
110.00	14073.0
111.00	2092.0
116.00	415.0
117.00	5906.0
118.00	478.0
121.90	441.0
123.00	659.0
124.00	392.0
125.00	304.0
127.00	27120.0
128.00	1767.0
129.00	10489.0
130.00	839.0
135.00	812.0
136.00	336.0
137.00	536.0
141.00	1329.0
142.00	397.0
147.00	759.0
148.00	1685.0
149.00	421.0
153.00	410.0
154.00	338.0
155.00	742.0
156.00	1252.0
160.00	453.0
161.00	687.0
165.00	413.0
165.90	423.0
167.00	3020.0
168.00	2558.0
173.00	352.0
174.00	693.0
175.00	1139.0
176.00	347.0
177.00	493.0
179.00	2157.0
180.00	1736.0
181.00	807.0
185.00	1084.0
186.00	8438.0
187.00	2320.0
188.90	540.0
190.90	379.0
192.00	813.0
193.00	1050.0
196.00	1688.0
197.00	355.0
198.00	63584.0
199.00	4245.0
200.00	391.0
203.00	392.0
204.00	2429.0
205.00	3839.0
206.10	16361.0
207.10	2494.0
208.00	773.0
211.00	638.0
216.00	373.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

217.00	4435.0
218.00	580.0
221.00	2681.0
221.90	503.0
223.00	1018.0
224.10	9423.0
225.10	2490.0
227.00	3883.0
228.00	547.0
228.90	820.0
231.00	367.0
235.00	304.0
237.00	452.0
242.00	641.0
243.00	508.0
244.10	7594.0
245.00	1045.0
246.00	1514.0
254.10	325.0
255.00	38232.0
256.00	5444.0
257.10	441.0
258.00	2337.0
259.00	348.0
265.10	861.0
273.00	1078.0
274.00	3217.0
275.00	17088.0
276.00	2251.0
277.00	1525.0
293.00	317.0
296.00	5115.0
297.00	785.0
303.00	549.0
315.00	577.0
316.00	324.0
323.10	1584.0
326.90	411.0
334.00	1104.0
346.00	417.0
352.10	510.0
353.00	376.0
354.10	499.0
365.00	2475.0
372.10	827.0
402.00	400.0
403.00	557.0
421.00	446.0
422.00	595.0
423.10	3774.0
424.10	1222.0
441.10	11519.0
442.10	73216.0
443.10	13214.0
444.00	1176.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39