

Data Path : Z:\HPCHEM1\BNA M\DATA\BM032417\
 Data File : BM009399.D
 Acq On : 25 Mar 2017 02:37
 Operator : SJ/MA
 Sample : I2372-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9XZ0

Quant Time: Mar 25 04:26:58 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 25 01:48:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	147837	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	573463	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.50	164	321001	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	776356	20.00	ng/ul	0.00
77) Chrysene-d12	21.42	240	1096006	20.00	ng/ul	0.00
85) Perylene-d12	23.74	264	996720	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	20579	5.30	ng/uL	0.00
5) Phenol-d5	7.01	99	59717	4.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	332375	34.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.38	132	259017	28.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	129528	12.98	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	159983	37.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.74	143	171997	37.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	298379	33.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	796	0.08	ng/ul	-0.13
43) Dimethylphthalate-d6	13.90	166	1043070	46.20	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	16387	0.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	31994	7.69	ng/ul	0.00
57) Fluorene-d10	15.49	176	830124	40.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	158456	32.29	ng/ul	0.00
70) Anthracene-d10	17.34	188	837639	22.62	ng/ul	0.00
78) Pyrene-d10	19.63	212	1257878	27.07	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.60	264	529296	11.53	ng/ul	0.00


Target Compounds					Ovalue
45) 2,6-Dinitrotoluene	13.90	165	6176	1.42 ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM032417\
Data File : BM009399.D
Acq On : 25 Mar 2017 02:37
Operator : SJ/MA
Sample : I2372-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XZ0

Quant Time: Mar 25 04:26:58 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 25 01:48:31 2017
Response via : Initial Calibration

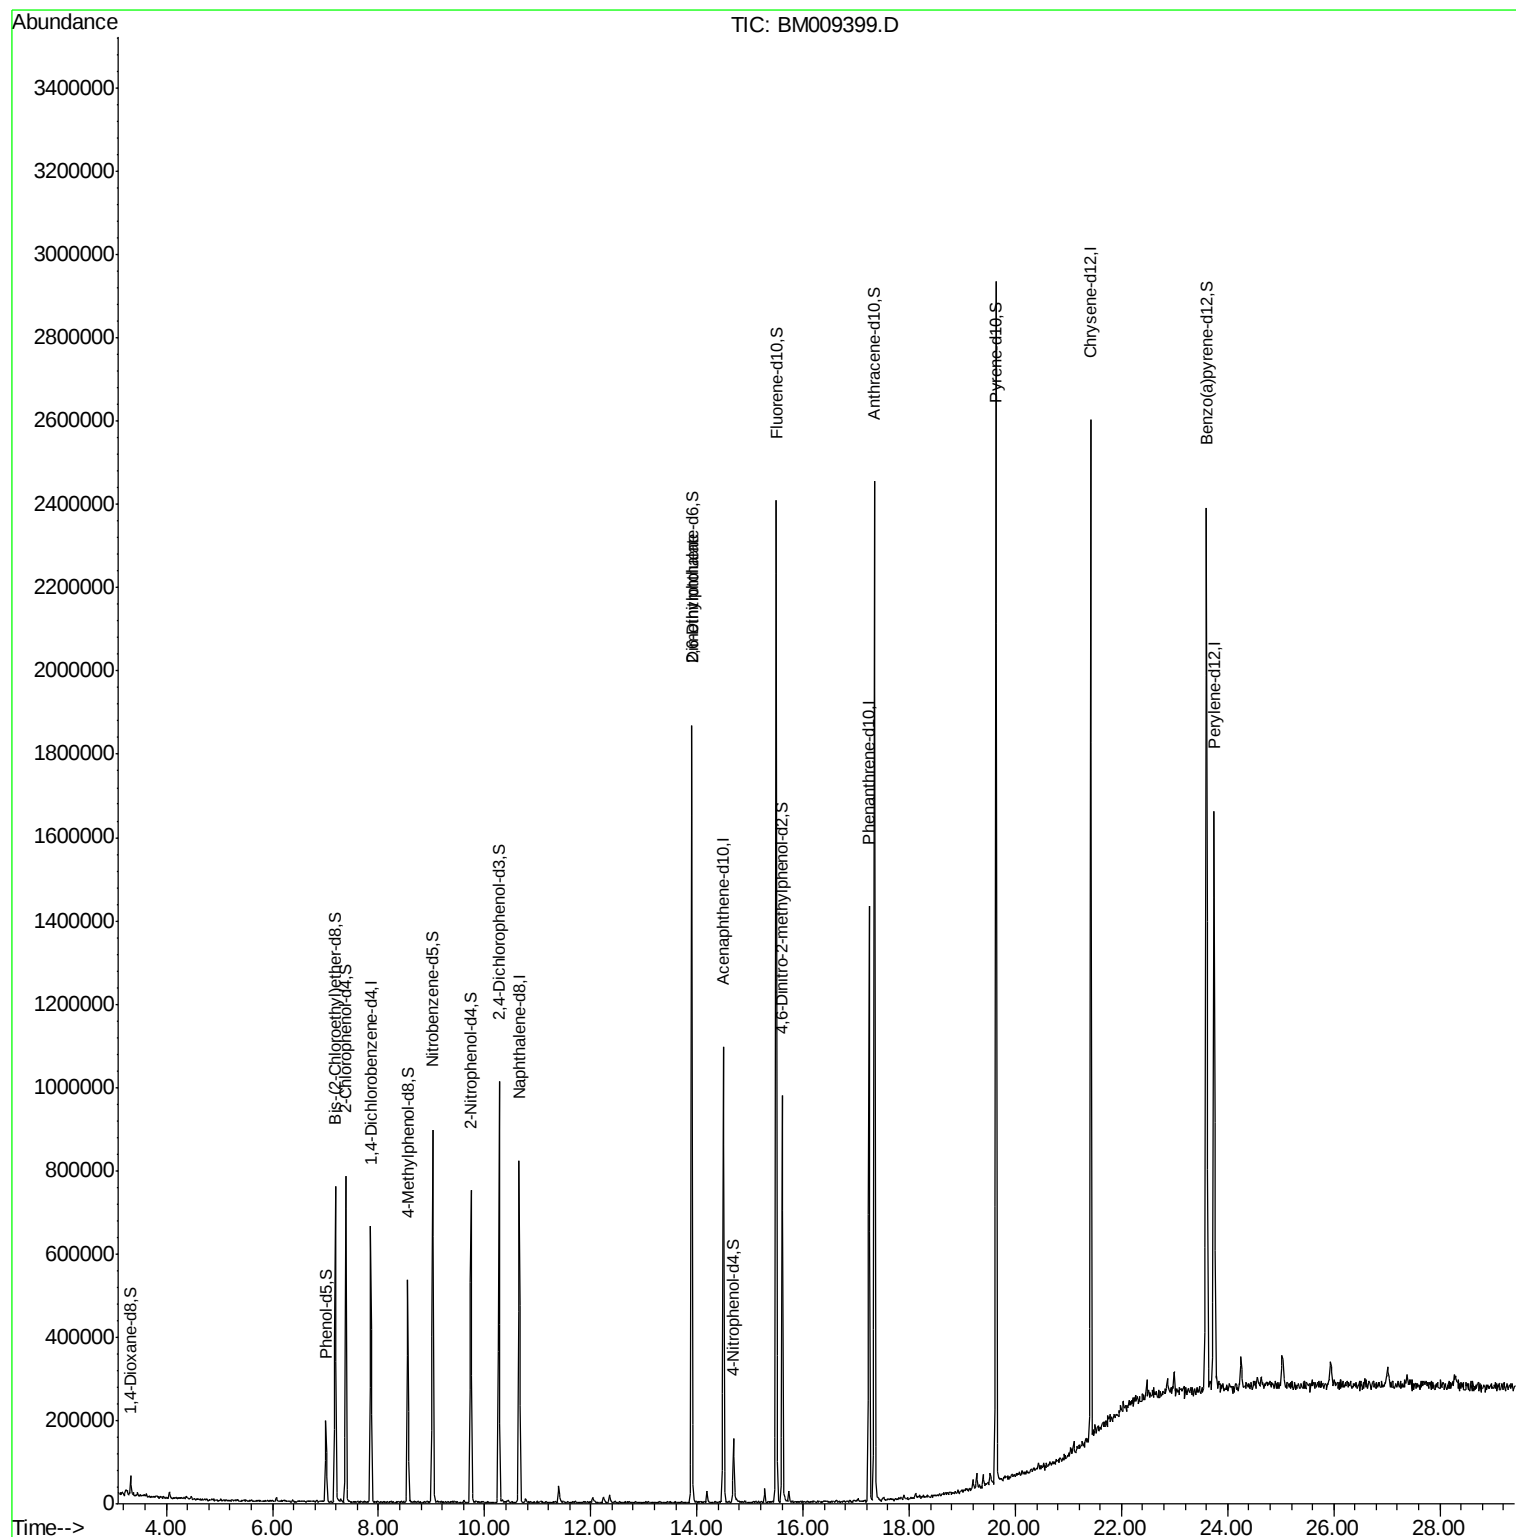

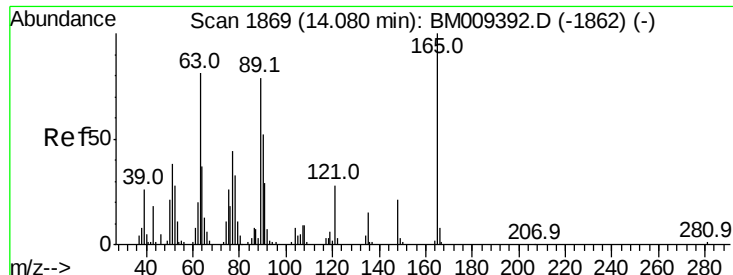

#45
 2,6-Dinitrotoluene
 Concen: 1.42 ng/ul
 RT: 13.90 min Scan# 1839
 Delta R.T. -0.18 min
 Lab File: BM009399.D
 Acq: 25 Mar 2017 02:37

Instrument :
 BNA_M
 ClientSampleId :
 G9XZ0

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	42.4	63.6#
121	38.2	16.6	24.8#

