


Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
Data File : BM009405.D
Acq On : 25 Mar 2017 06:13
Operator : SJ/MA
Sample : I2358-09DL 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 27 04:12:15 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 25 01:48:31 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0BK2DL

Manual Integrations
APPROVED

mohammad
3/27/2017 1:18:20 PM

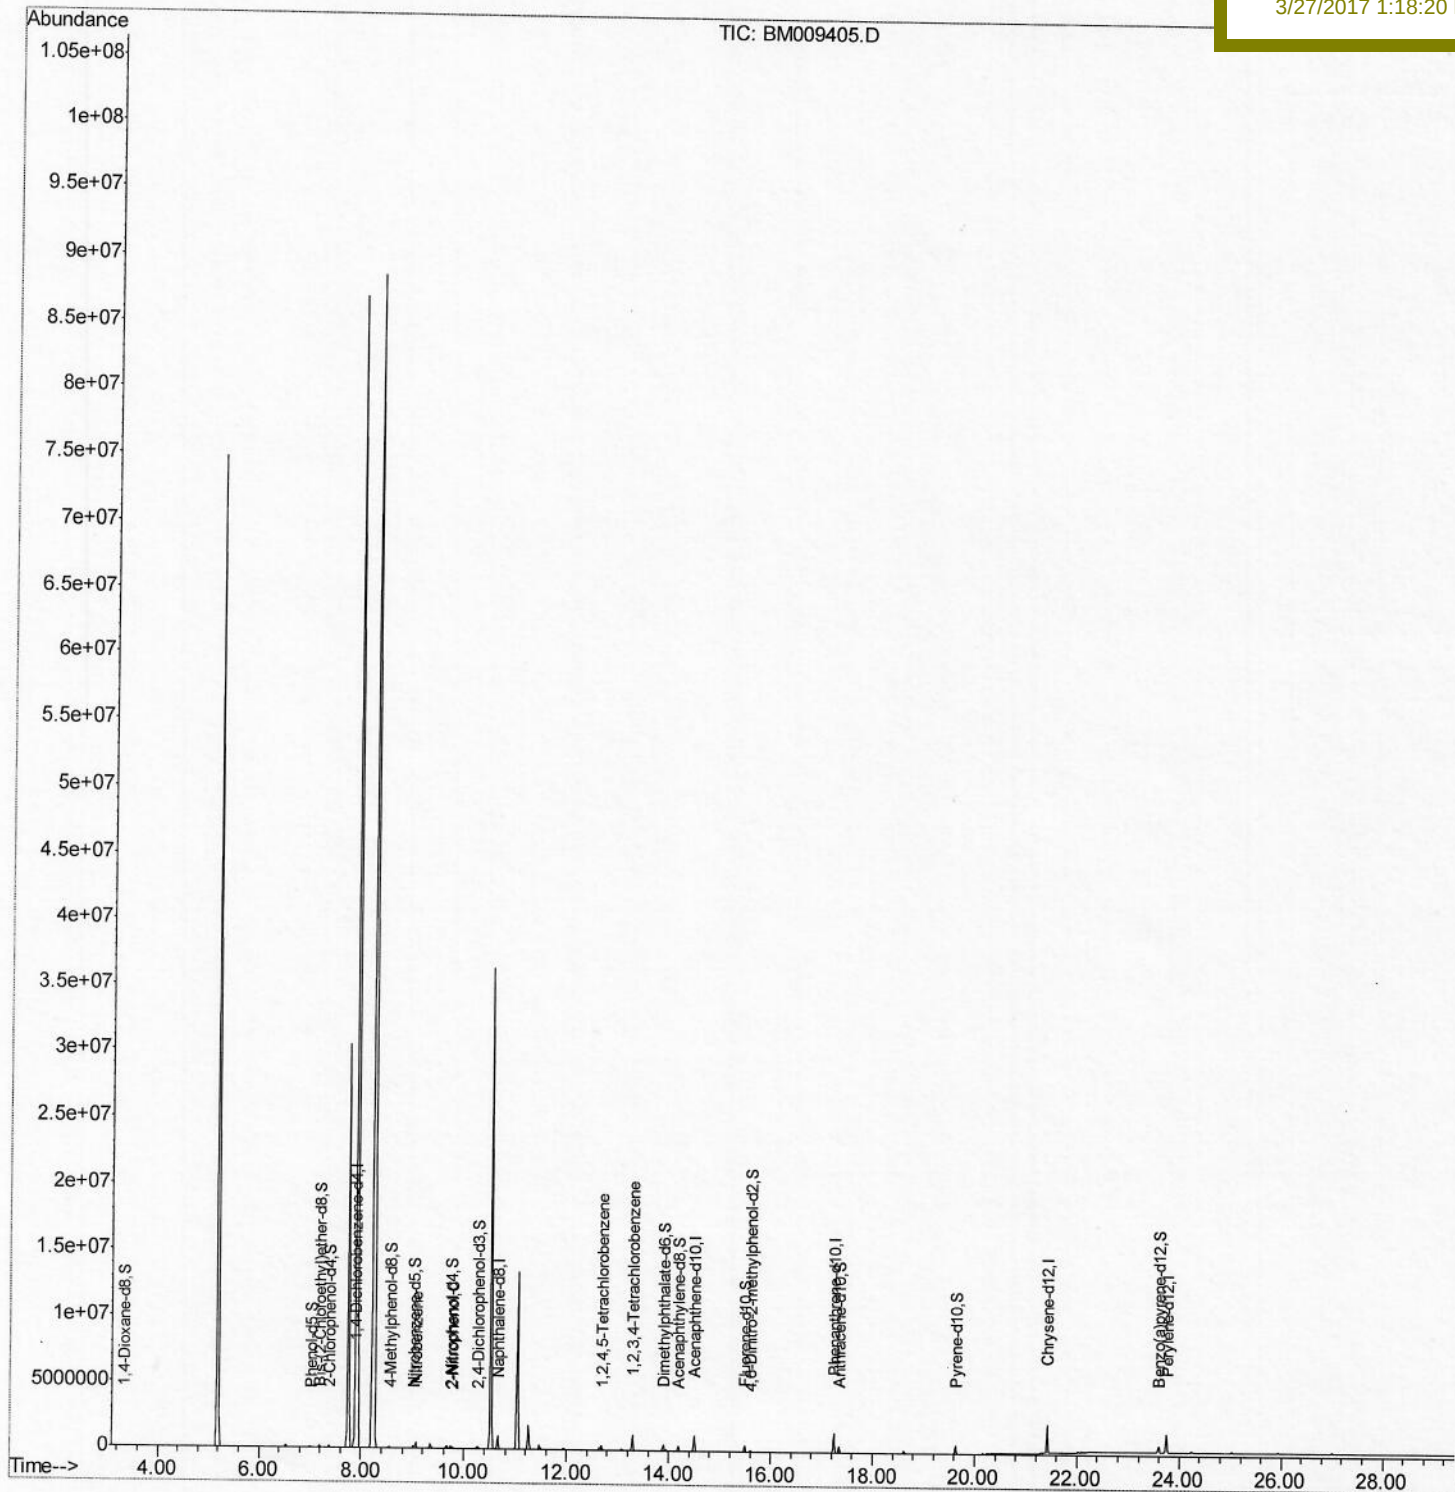

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM032417\
 Data File : BM009405.D
 Acq On : 25 Mar 2017 06:13
 Operator : SJ/MA
 Sample : I2358-09DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 25 06:46:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 25 01:48:31 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 C0BK2DL

Manual Integrations
APPROVED

mohammad
 3/27/2017 1:18:20 PM

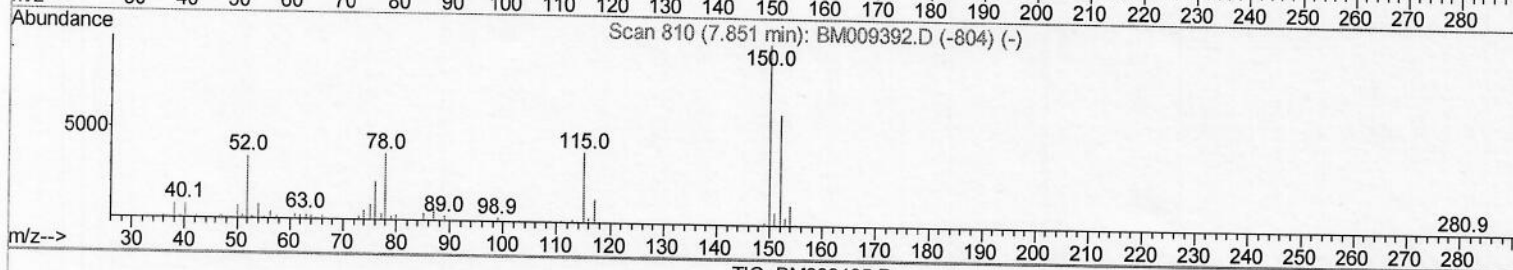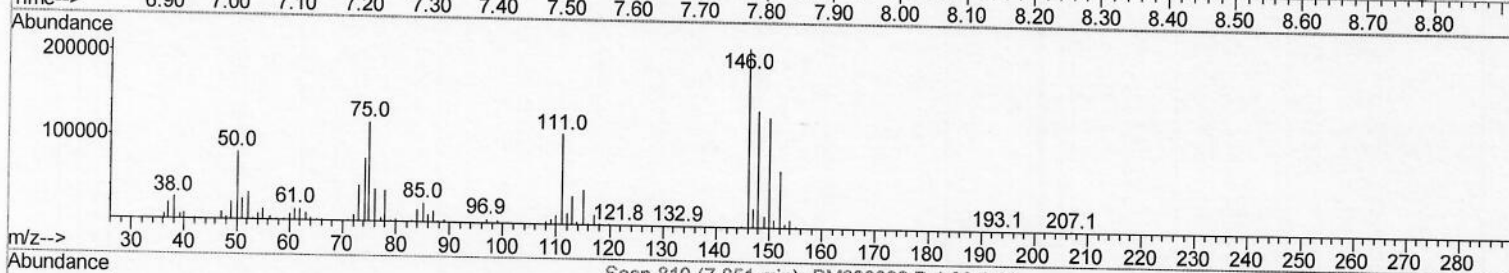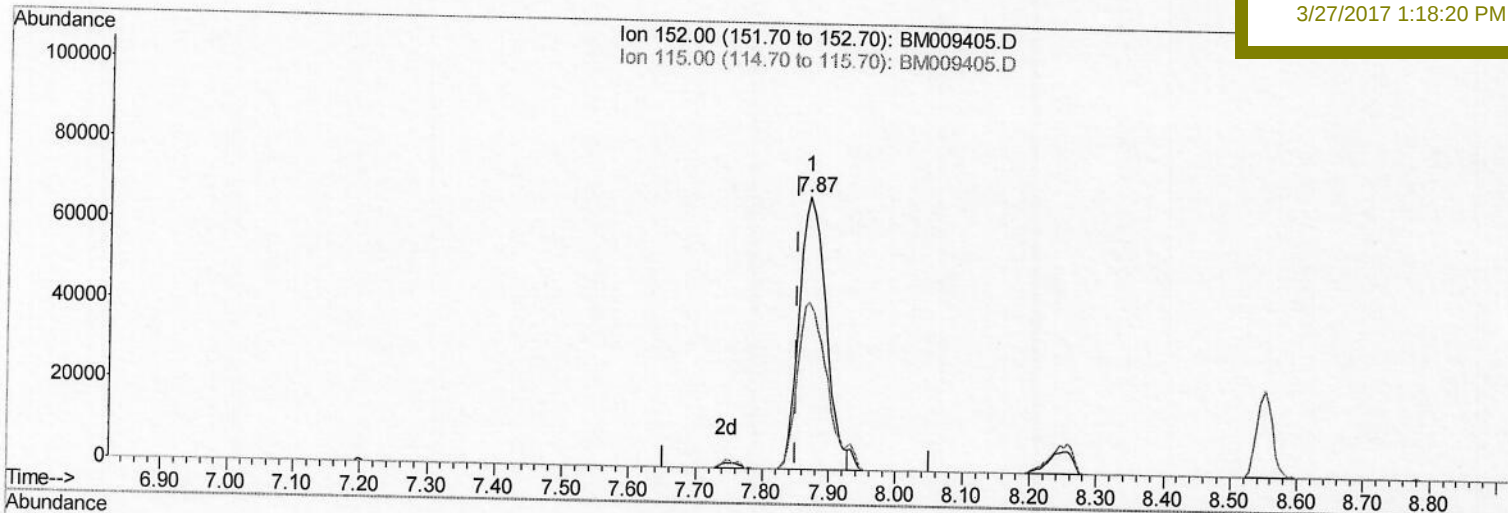

TIC: BM009405.D

(1) 1,4-Dichlorobenzene-d4 (I)

7.869min (+0.018) 20.00ng/ul

response 189372

Ion	Exp%	Act%
152.00	100	100
115.00	63.00	61.22
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM032417\
 Data File : BM009405.D
 Acq On : 25 Mar 2017 06:13
 Operator : SJ/MA
 Sample : I2358-09DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 25 06:46:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 25 01:48:31 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0BK2DL

Manual Integrations
 APPROVED

mohammad
 3/27/2017 1:18:20 PM

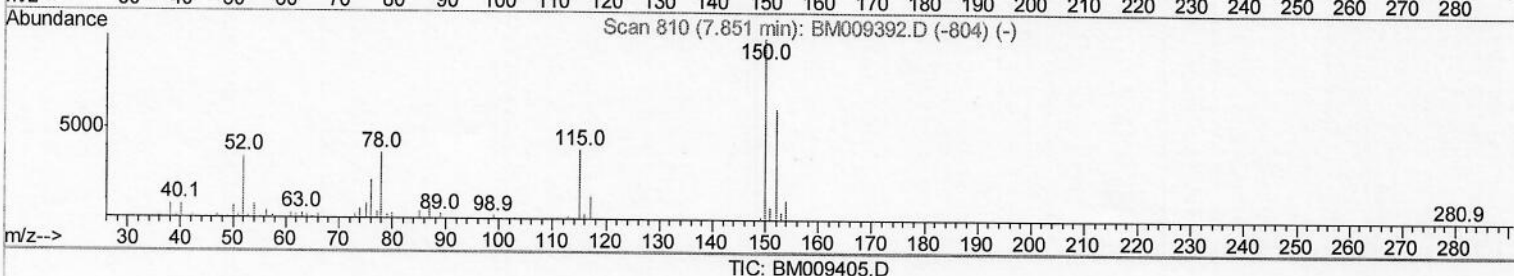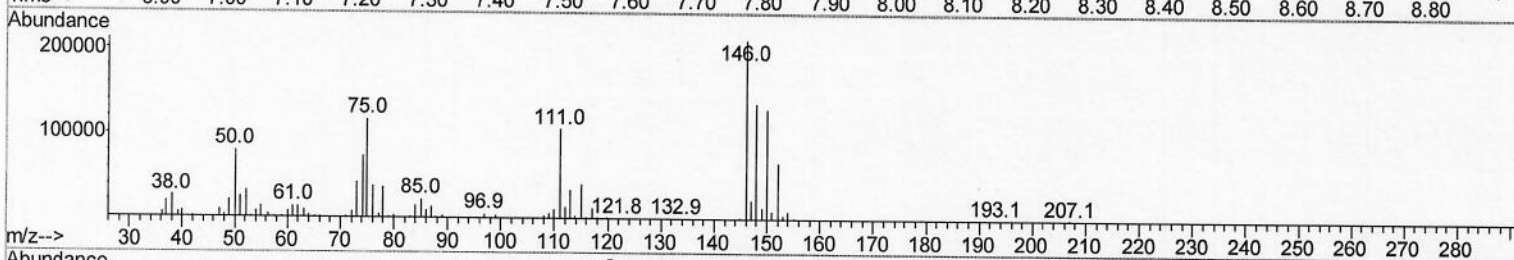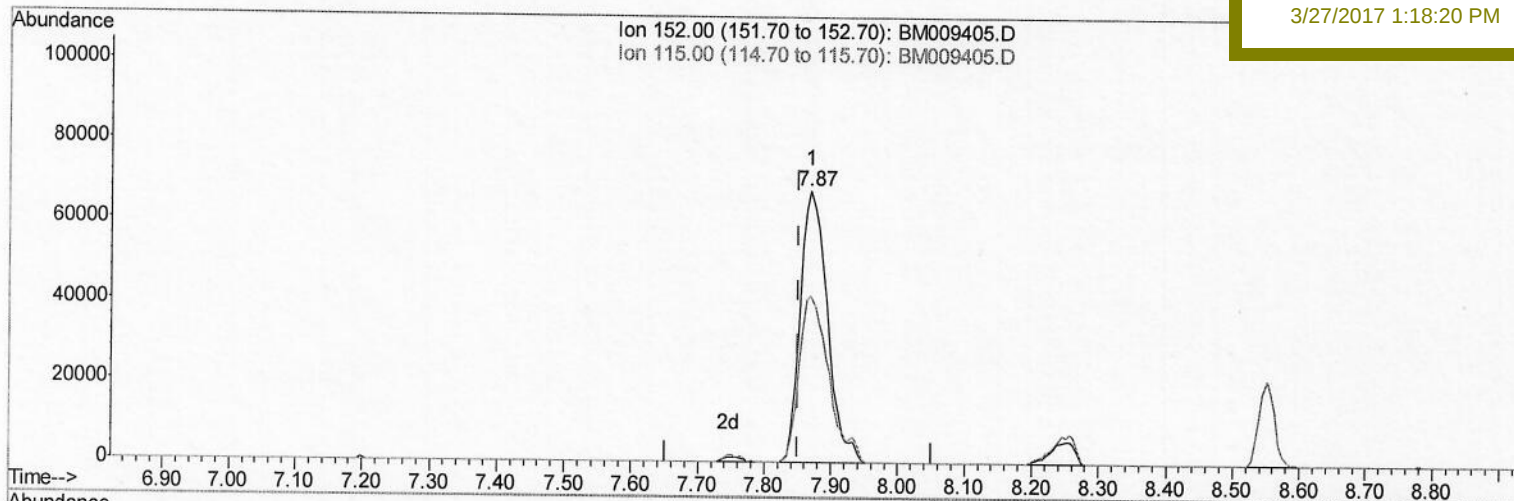

TIC: BM009405.D

(1) 1,4-Dichlorobenzene-d4 (I)

7.869min (+0.018) 20.00ng/ul m

response 192117

Ion	Exp%	Act%
152.00	100	100
115.00	63.00	61.22
0.00	0.00	0.00
0.00	0.00	0.00

SJ
 03/27/2017

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM032417\
 Data File : BM009405.D
 Acq On : 25 Mar 2017 06:13
 Operator : SJ/MA
 Sample : I2358-09DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 25 06:50:25 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 25 01:48:31 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0BK2DL

Manual Integrations
 APPROVED

mohammad
 3/27/2017 1:18:20 PM

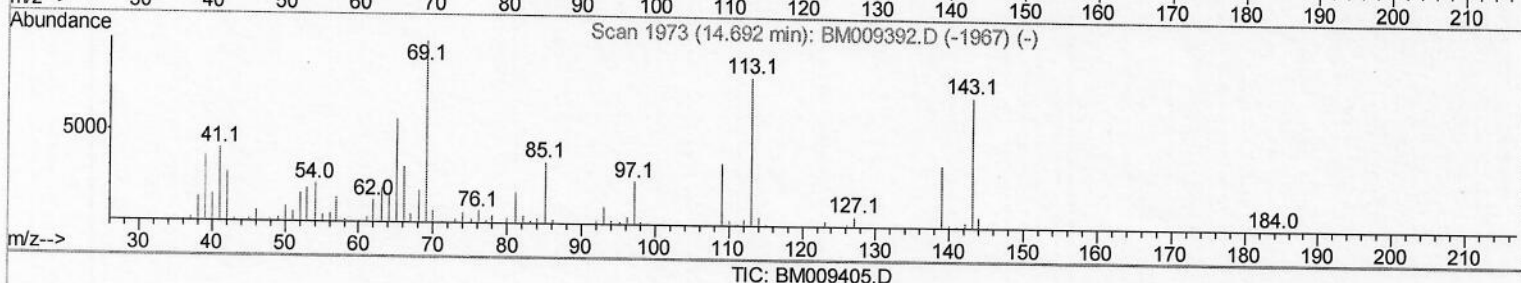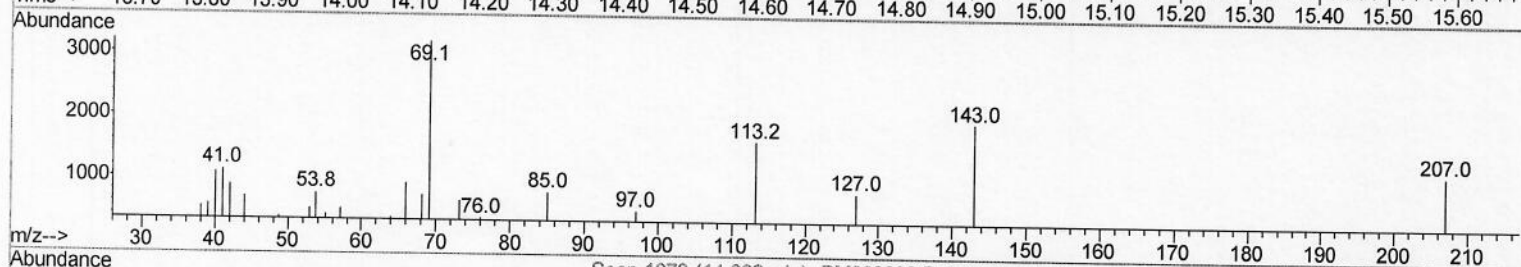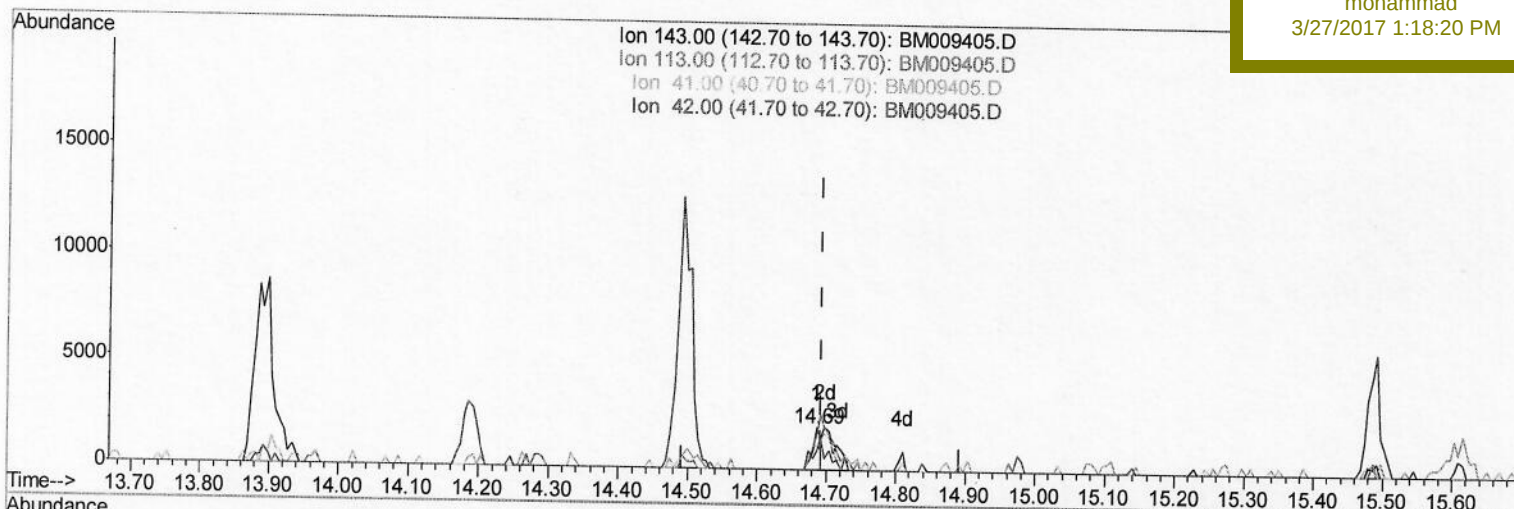

(51) 4-Nitrophenol-d4 (S)

14.686min (-0.006) 0.35ng/ul

response 1641

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	83.82
41.00	28.80	56.99#
42.00	19.10	44.50#

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM032417\
 Data File : BM009405.D
 Acq On : 25 Mar 2017 06:13
 Operator : SJ/MA
 Sample : I2358-09DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 25 06:50:25 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 25 01:48:31 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0BK2DL

Manual Integrations
 APPROVED

mohammad
 3/27/2017 1:18:20 PM

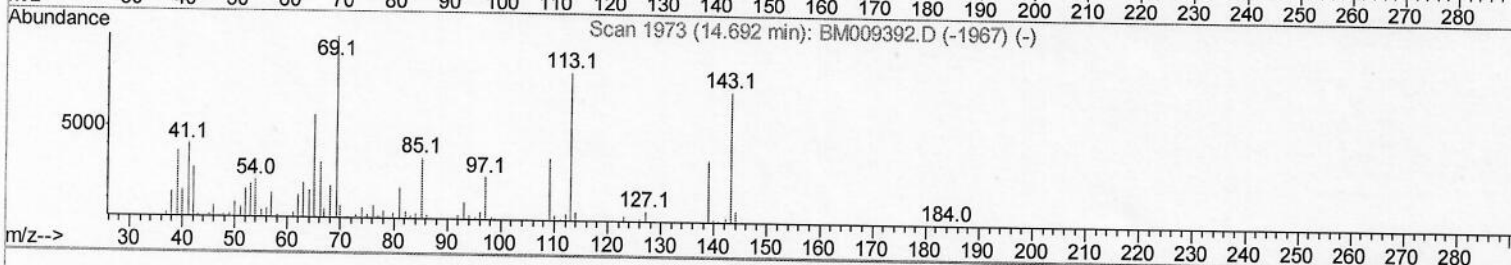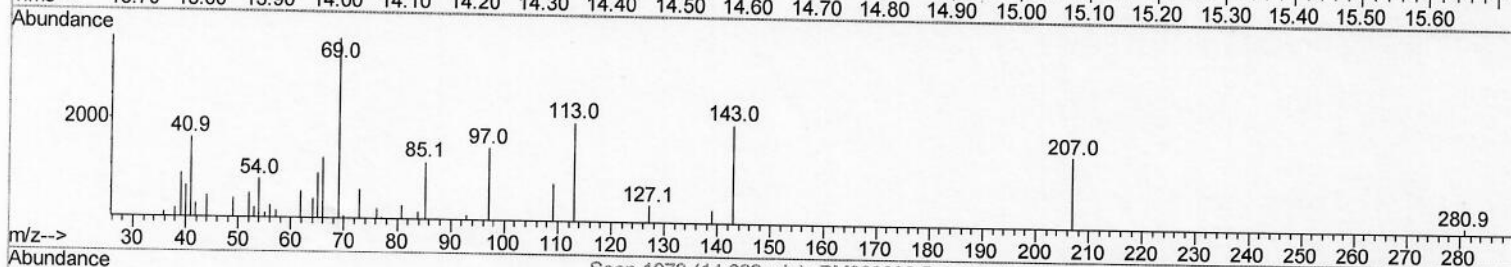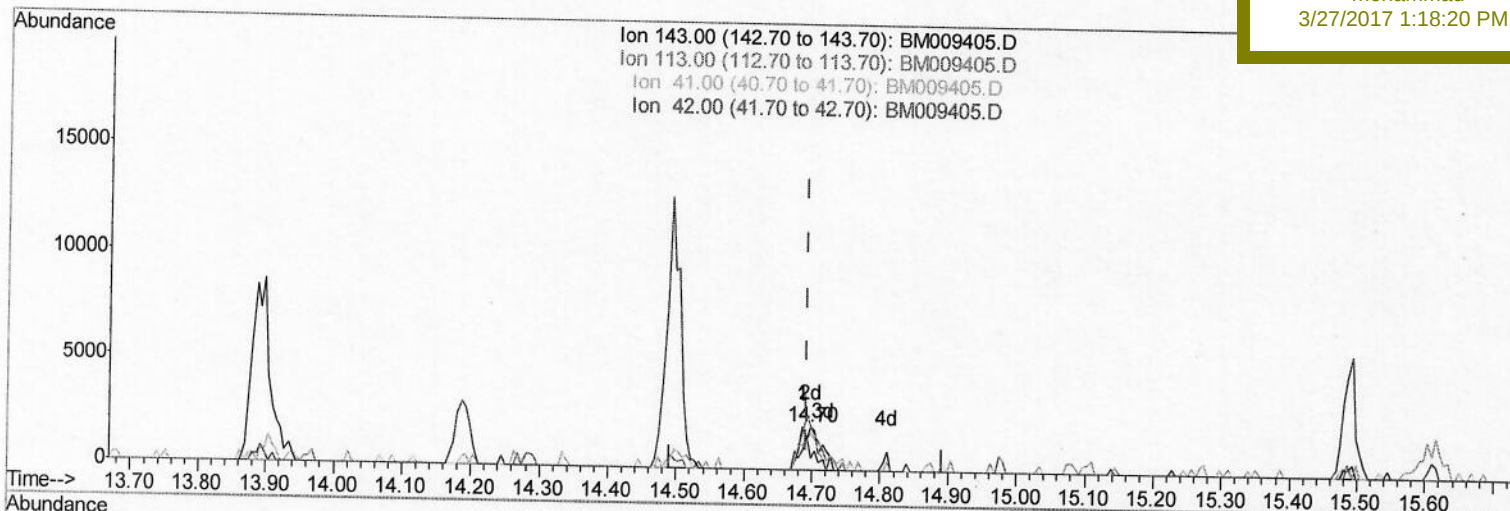

(51) 4-Nitrophenol-d4 (S)

14.698min (+0.006) 0.91ng/ul m

response 4194

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	100.05#
41.00	28.80	83.80#
42.00	19.10	27.20#

SJ
 03/27/2017

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
 Data File : BM009405.D
 Acq On : 25 Mar 2017 06:13
 Operator : SJ/MA
 Sample : I2358-09DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BK2DL

Quant Time: Mar 27 04:12:15 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 25 01:48:31 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/27/2017 1:18:20 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	192117m	20.00	ng/ul	0.02
18) Naphthalene-d8	10.66	136	659057	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.50	164	356600	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	802907	20.00	ng/ul	0.00
77) Chrysene-d12	21.42	240	1040794	20.00	ng/ul	0.00
85) Perylene-d12	23.74	264	1006688	20.00	ng/ul	0.00

SJ
 03/27/2017

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	5774	1.15	ng/uL	0.00
5) Phenol-d5	7.01	99	20395	1.17	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.19	67	69159	5.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	51825	4.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	39135	3.02	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	30412	6.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.74	143	31209	5.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	59910	5.80	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	200074	7.98	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	242203	7.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	4194m	0.91	ng/ul	0.00
57) Fluorene-d10	15.49	176	178765	7.77	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	22846	4.50	ng/ul	0.00
70) Anthracene-d10	17.34	188	264431	6.91	ng/ul	0.00
78) Pyrene-d10	19.63	212	308877	7.00	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.59	264	319673	6.90	ng/ul	0.00

SJ
 03/27/2017

Target Compounds

					Ovalue
20) Nitrobenzene	9.06	77	253130	15.50	ng/ul# 82
23) 2-Nitrophenol	9.77	139	18842	3.39	ng/ul# 66
36) 1,2,4,5-Tetrachlorobenzene	12.68	216	108016	9.02	ng/ul 96
72) 1,2,3,4-Tetrachlorobenzene	13.29	216	347451	29.43	ng/uL 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed