

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
 Data File : BM009384.D
 Acq On : 24 Mar 2017 17:38
 Operator : SJ/MA
 Sample : PB97792BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	36	42	47	rBV	49399	75165	2.03%	0.198%
2	7.010	660	667	676	rBV	721413	1118723	30.14%	2.952%
3	7.187	688	697	708	rBV	549932	850370	22.91%	2.244%
4	7.381	722	730	740	rBV	691253	1116539	30.09%	2.946%
5	7.857	804	811	821	rBV	579944	946392	25.50%	2.497%
6	8.551	921	929	939	rBV2	820984	1272541	34.29%	3.358%
7	9.022	1001	1009	1018	rBV	658738	1085252	29.24%	2.864%
8	9.739	1124	1131	1140	rBV	522183	858536	23.13%	2.265%
9	10.269	1214	1221	1229	rBV	753330	1247357	33.61%	3.291%
10	10.651	1279	1286	1297	rVB	725658	1226525	33.05%	3.236%
11	10.792	1301	1310	1320	rBV	763405	1292126	34.82%	3.410%
12	13.904	1831	1839	1851	rBV	1289755	1740463	46.90%	4.593%
13	14.192	1881	1888	1896	rBV	1375569	2013840	54.26%	5.314%
14	14.498	1934	1940	1949	rVB2	1018777	1541370	41.53%	4.067%
15	14.686	1967	1972	1986	rBV	575121	903618	24.35%	2.384%
16	15.492	2102	2109	2121	rBV	1831527	2589717	69.78%	6.834%
17	15.610	2124	2129	2139	rBV	602018	815409	21.97%	2.152%
18	17.245	2401	2407	2416	rVB	1363396	1898707	51.16%	5.010%
19	17.345	2418	2424	2434	rBV	2056754	2856592	76.97%	7.538%
20	19.639	2807	2814	2821	rBV	2622880	3425092	92.29%	9.038%
21	21.421	3112	3117	3123	rBV	2145599	2625321	70.74%	6.927%
22	23.597	3480	3487	3498	rVB	1903532	3711275	100.00%	9.793%
23	23.744	3506	3512	3521	rVB2	1251903	2495848	67.25%	6.586%
24	24.256	3596	3599	3606	rVB5	105004	190408	5.13%	0.502%


Sum of corrected areas: 37897186

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
Data File : BM009384.D
Acq On : 24 Mar 2017 17:38
Operator : SJ/MA
Sample : PB97792BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK92

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

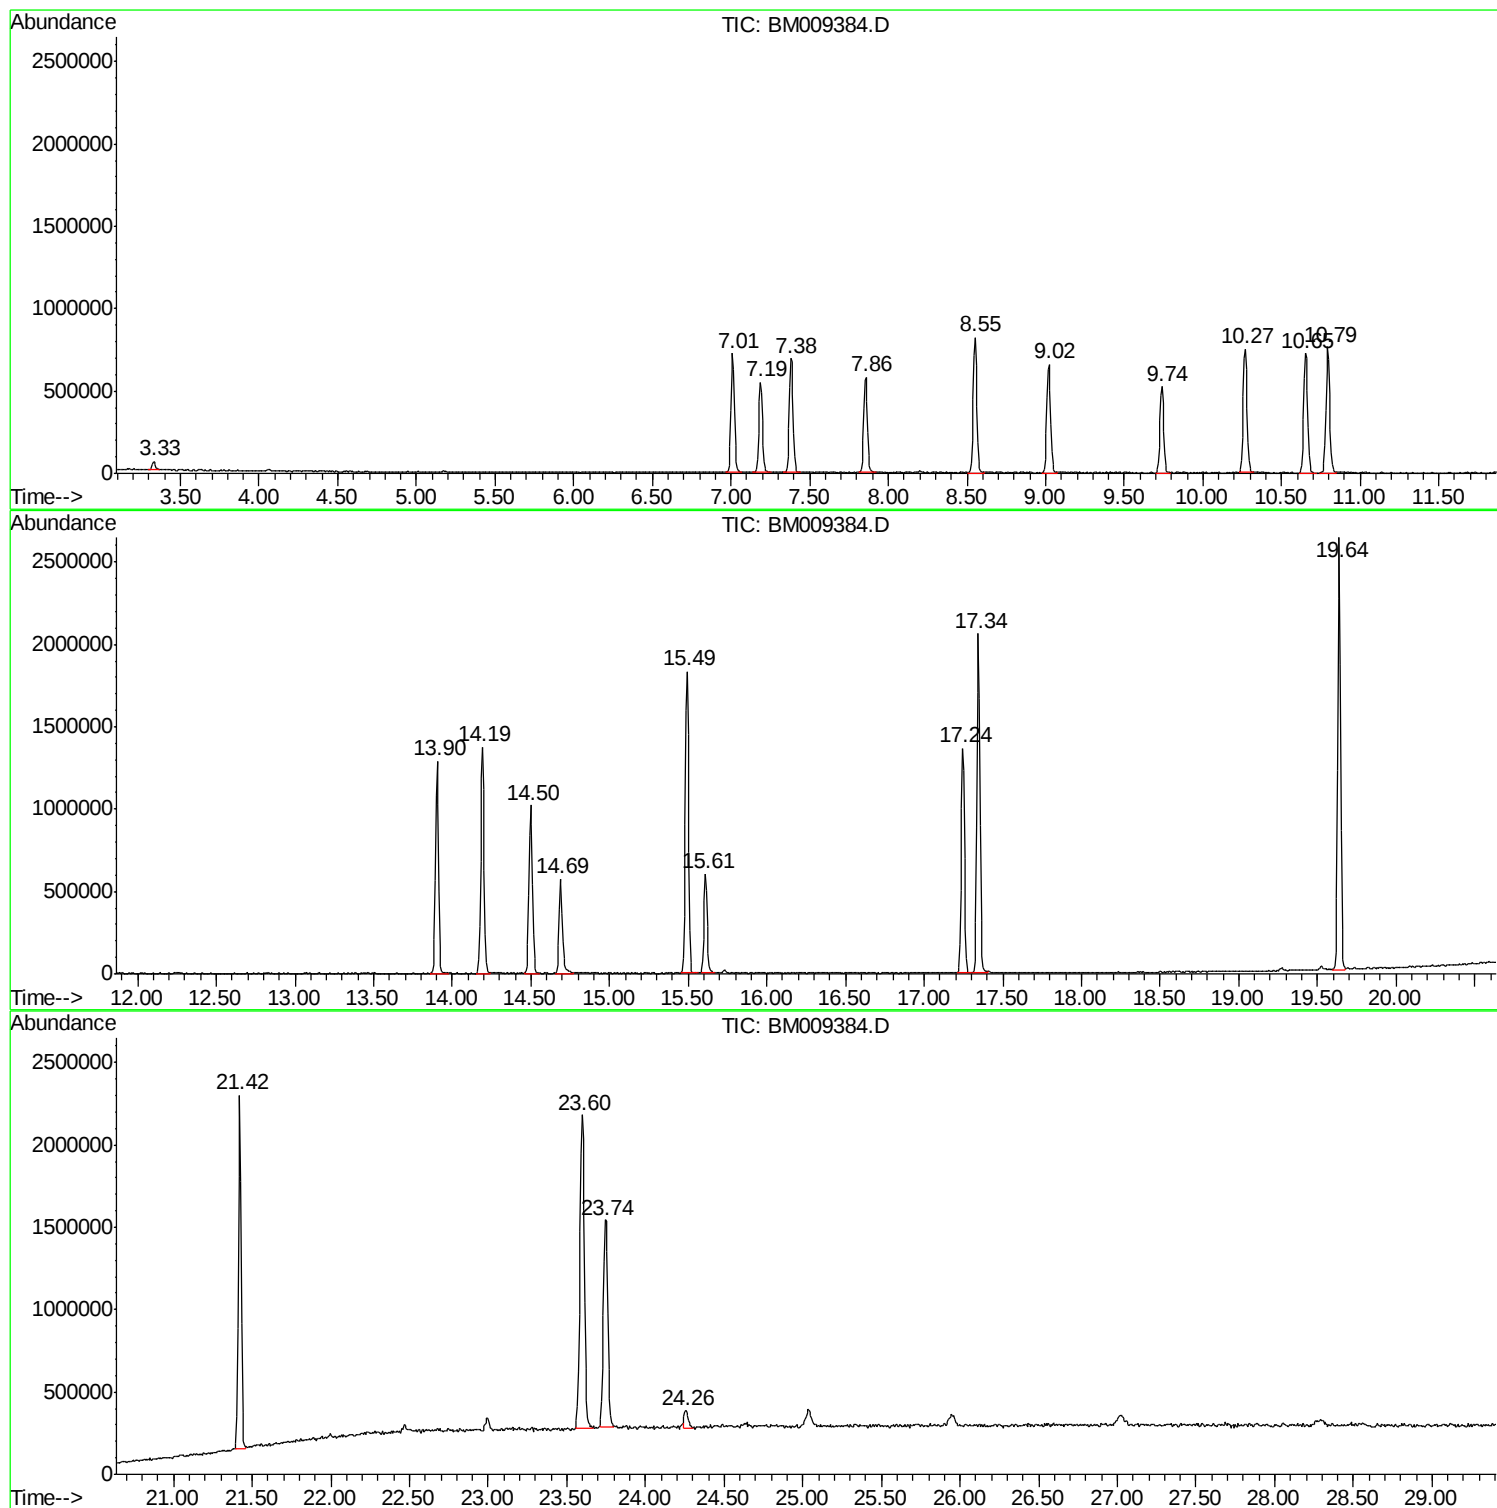

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032417\
Data File : BM009384.D
Acq On : 24 Mar 2017 17:38
Operator : SJ/MA
Sample : PB97792BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK92

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032417\
Data File : BM009384.D
Acq On : 24 Mar 2017 17:38
Operator : SJ/MA
Sample : PB97792BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK92

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc