

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
 Data File : BM009385.D
 Acq On : 24 Mar 2017 18:14
 Operator : SJ/MA
 Sample : I2357-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9XX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	47	rBV	41070	57278	1.40%	0.154%
2	7.010	662	667	675	rVB	184905	284635	6.95%	0.767%
3	7.186	691	697	706	rBV	599368	930439	22.71%	2.507%
4	7.381	724	730	741	rVB	629523	1031017	25.16%	2.778%
5	7.857	803	811	824	rBV	603342	982927	23.99%	2.649%
6	8.551	923	929	936	rBV	477555	747470	18.24%	2.014%
7	9.022	1000	1009	1018	rBV	742729	1239546	30.25%	3.340%
8	9.739	1124	1131	1140	rBV	612138	985642	24.05%	2.656%
9	10.269	1214	1221	1230	rBV	828097	1362714	33.25%	3.672%
10	10.657	1280	1287	1295	rBV	721052	1243534	30.35%	3.351%
11	10.798	1306	1311	1318	rBV3	40755	69392	1.69%	0.187%
12	13.904	1832	1839	1846	rBV	1489819	1984929	48.44%	5.349%
13	14.192	1881	1888	1895	rBV	1620157	2303549	56.21%	6.207%
14	14.498	1931	1940	1948	rBV2	1030404	1546169	37.73%	4.166%
15	14.692	1967	1973	1984	rBV2	100428	186217	4.54%	0.502%
16	15.492	2103	2109	2119	rVB	2111735	2978218	72.68%	8.025%
17	15.609	2123	2129	2141	rBV	686559	955897	23.33%	2.576%
18	17.245	2400	2407	2415	rBV	1334787	1852692	45.21%	4.992%
19	17.345	2415	2424	2435	rBV	2395507	3313138	80.85%	8.928%
20	18.115	2551	2555	2561	rBV3	34686	52753	1.29%	0.142%
21	19.397	2768	2773	2777	rBV5	63416	92225	2.25%	0.249%
22	19.639	2808	2814	2820	rBV	3004811	3921877	95.71%	10.568%
23	21.421	3112	3117	3123	rBV	2050518	2481056	60.55%	6.685%
24	23.597	3480	3487	3494	rBV2	2158263	4097847	100.00%	11.042%
25	23.744	3506	3512	3521	rVB	1239816	2410224	58.82%	6.495%


Sum of corrected areas: 37111385

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
Data File : BM009385.D
Acq On : 24 Mar 2017 18:14
Operator : SJ/MA
Sample : I2357-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XX7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

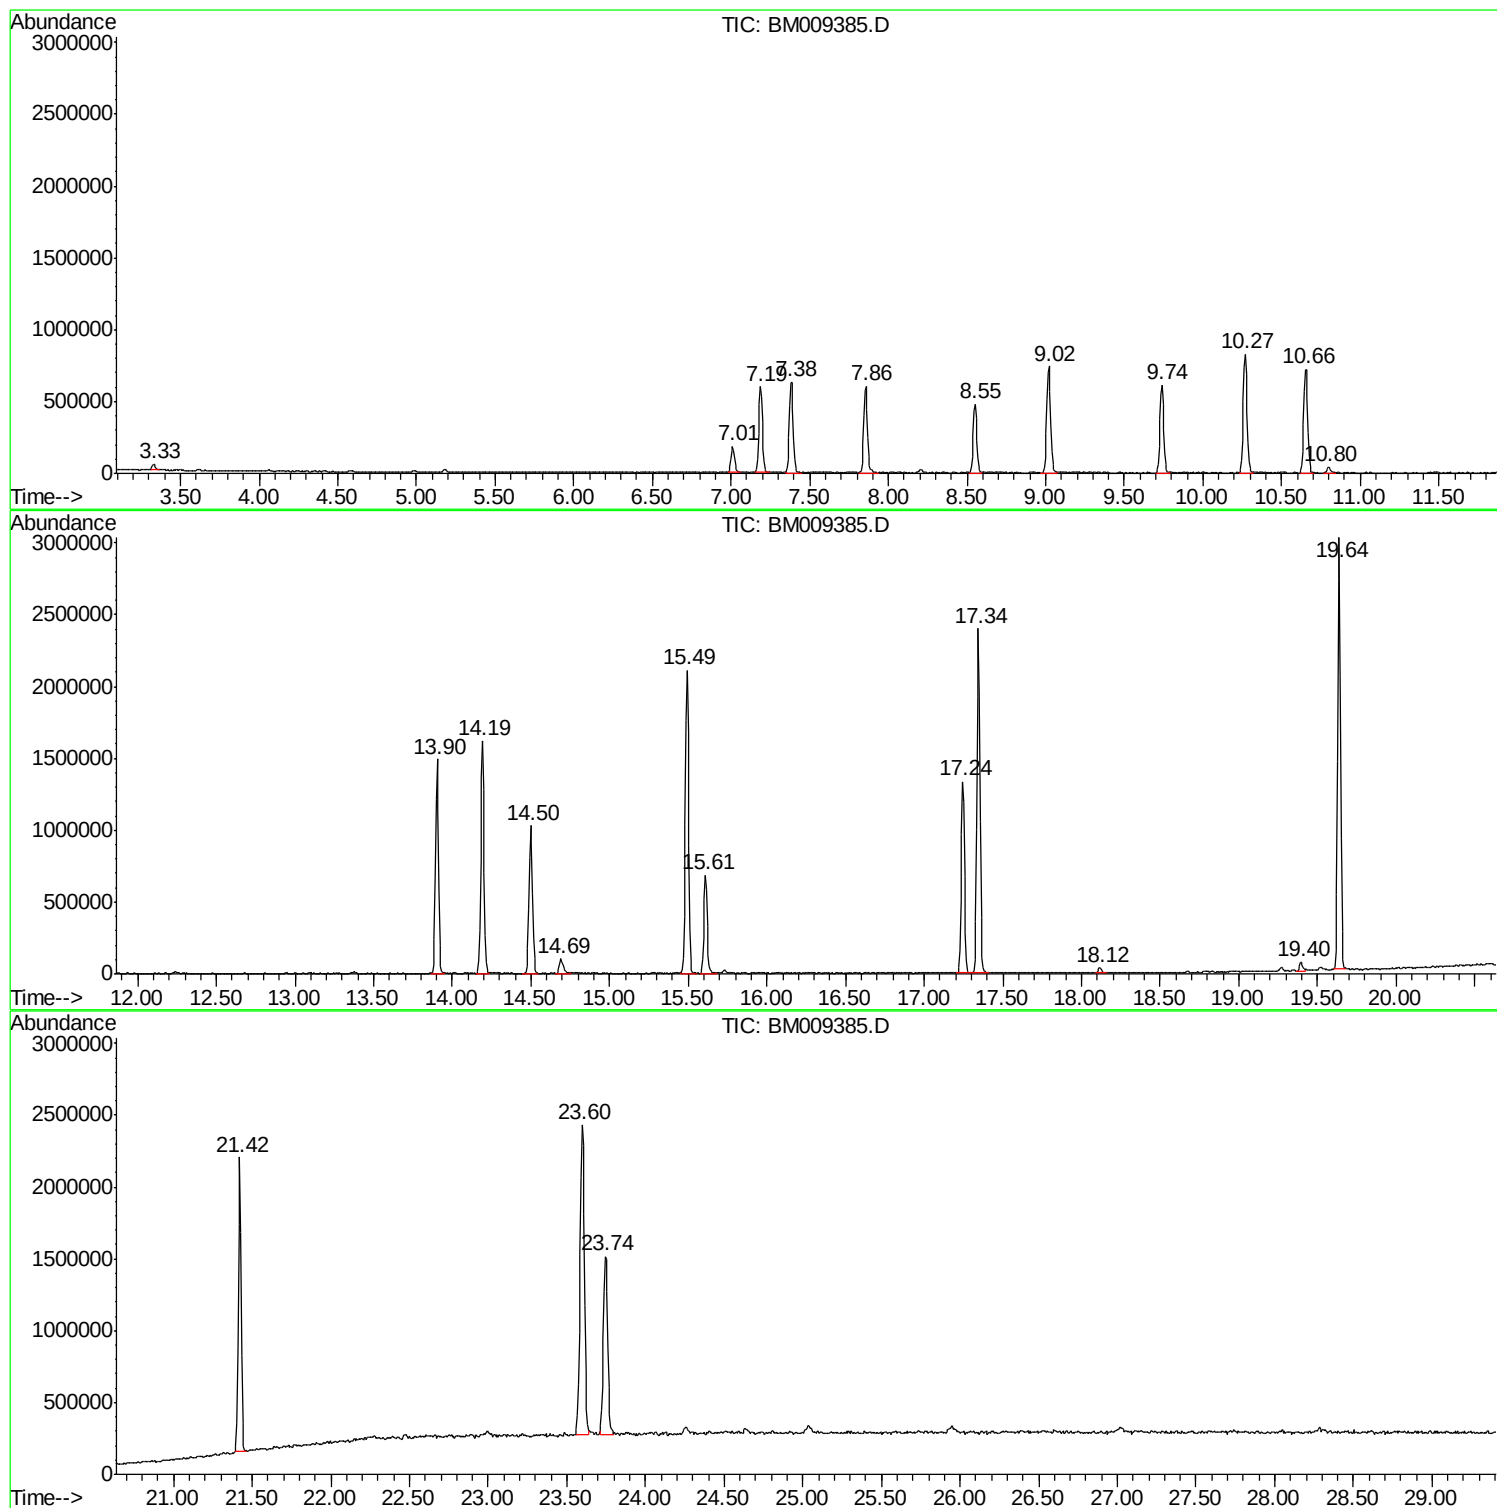

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032417\
Data File : BM009385.D
Acq On : 24 Mar 2017 18:14
Operator : SJ/MA
Sample : I2357-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XX7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032417\
Data File : BM009385.D
Acq On : 24 Mar 2017 18:14
Operator : SJ/MA
Sample : I2357-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XX7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc