

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
 Data File : BM009386.D
 Acq On : 24 Mar 2017 18:50
 Operator : SJ/MA
 Sample : I2357-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9XX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	38	41	48	rVB2	51708	70973	1.60%	0.185%
2	7.010	660	667	675	rBV	187858	295863	6.67%	0.772%
3	7.187	691	697	708	rBV	648627	979020	22.08%	2.555%
4	7.381	724	730	741	rBV	655417	1068949	24.11%	2.789%
5	7.857	803	811	821	rBV	614997	1005329	22.68%	2.623%
6	8.551	923	929	939	rBV	477674	748799	16.89%	1.954%
7	9.022	1001	1009	1019	rBV	773007	1304450	29.43%	3.404%
8	9.739	1123	1131	1140	rBV	629416	1043482	23.54%	2.723%
9	10.269	1213	1221	1233	rBV	857927	1453487	32.79%	3.793%
10	10.651	1279	1286	1293	rBV	748244	1268166	28.61%	3.309%
11	13.904	1833	1839	1846	rBV	1538413	2049823	46.24%	5.349%
12	14.192	1881	1888	1896	rBV	1569946	2319694	52.33%	6.053%
13	14.498	1933	1940	1949	rBV2	1056174	1586251	35.78%	4.139%
14	14.692	1967	1973	1983	rBV	109136	202762	4.57%	0.529%
15	15.492	2102	2109	2123	rVB	2265212	3090150	69.71%	8.063%
16	15.610	2123	2129	2141	rBV	781669	1070337	24.14%	2.793%
17	17.245	2401	2407	2415	rBV	1340955	1868810	42.16%	4.876%
18	17.345	2417	2424	2431	rBV	2374673	3315063	74.78%	8.650%
19	19.392	2769	2772	2778	rBV7	34432	51440	1.16%	0.134%
20	19.639	2808	2814	2821	rBV	3061700	4162889	93.91%	10.863%
21	21.421	3112	3117	3123	rBV	2027774	2473290	55.79%	6.454%
22	23.597	3479	3487	3495	rBV2	2226918	4432987	100.00%	11.567%
23	23.750	3505	3513	3524	rBV2	1199981	2461213	55.52%	6.422%


Sum of corrected areas: 38323227

Data Path : Z:\HPCHEM1\BNA M\Data\BM032417\
Data File : BM009386.D
Acq On : 24 Mar 2017 18:50
Operator : SJ/MA
Sample : I2357-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XX8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

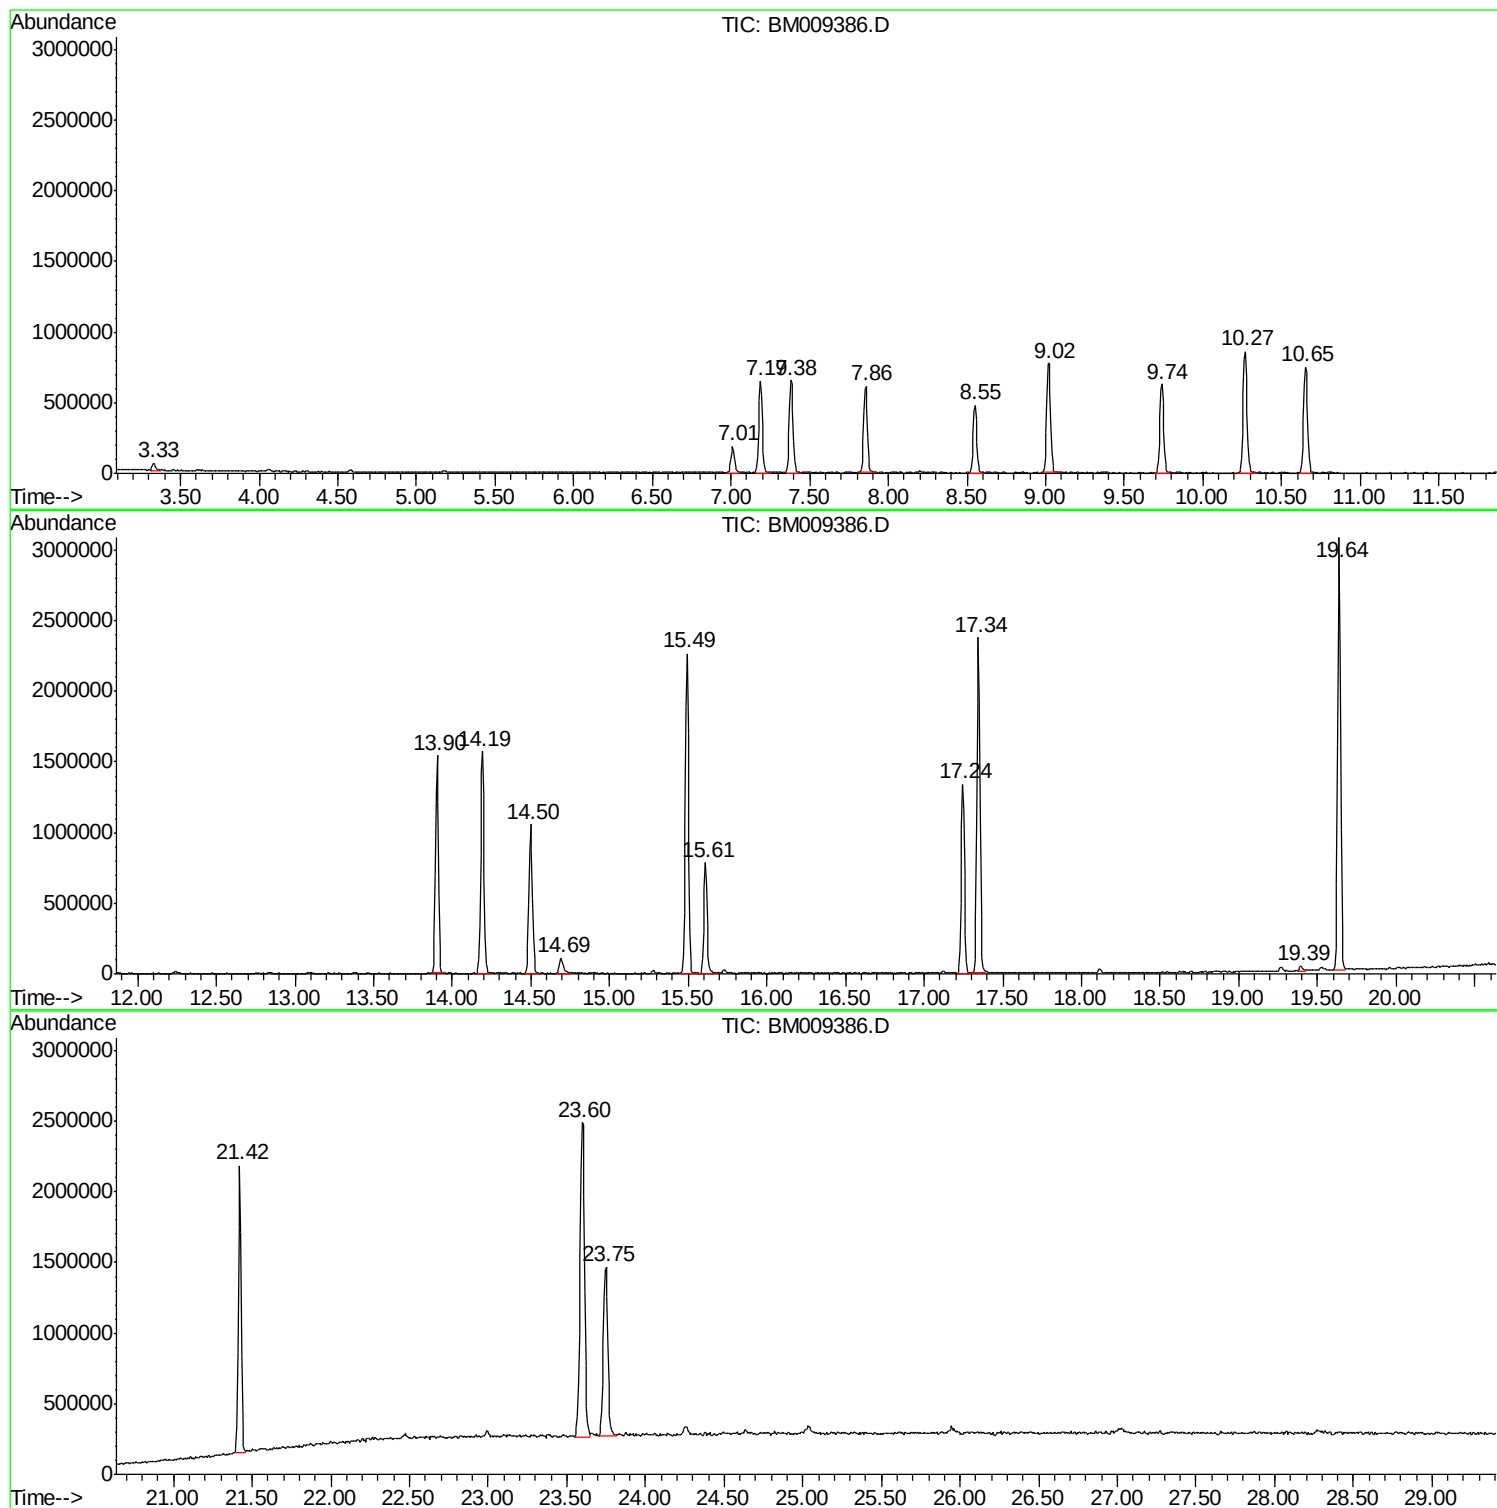

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032417\
Data File : BM009386.D
Acq On : 24 Mar 2017 18:50
Operator : SJ/MA
Sample : I2357-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XX8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032417\
Data File : BM009386.D
Acq On : 24 Mar 2017 18:50
Operator : SJ/MA
Sample : I2357-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XX8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc