

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032422\
 Data File : BM034370.D
 Acq On : 24 Mar 2022 19:52
 Operator : CG/JU
 Sample : N2094-04 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-2-(Q2)

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 03/25/2022
 Supervised By : Jagrut Upadhyay 03/25/2022

Quant Time: Mar 25 01:10:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 24 02:40:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	192094	20.000	ng	0.00
21) Naphthalene-d8	10.748	136	721455	20.000	ng	0.00
39) Acenaphthene-d10	14.577	164	404773	20.000	ng	0.00
64) Phenanthrene-d10	17.318	188	747606	20.000	ng	0.00
76) Chrysene-d12	21.495	240	682869	20.000	ng	0.00
86) Perylene-d12	23.912	264	770163	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.490	112	227651	21.260	ng	0.00
7) Phenol-d6	7.095	99	275342	17.960	ng	0.00
23) Nitrobenzene-d5	9.095	82	182075	12.287	ng	-0.01
42) 2,4,6-Tribromophenol	16.065	330	88241	16.174	ng	0.00
45) 2-Fluorobiphenyl	13.207	172	406848	13.735	ng	0.00
79) Terphenyl-d14	19.936	244	527718	13.428	ng	0.00
Target Compounds						
						Qvalue
75) Fluoranthene	19.371	202	164910	3.514	ng	98
78) Pyrene	19.736	202	169146	3.516	ng	99
81) Benzo(a)anthracene	21.477	228	106916	2.481	ng	96
83) Chrysene	21.530	228	107644	2.446	ng	97
88) Benzo(b)fluoranthene	23.177	252	151516m	3.290	ng	
90) Benzo(a)pyrene	23.806	252	101705	2.605	ng	# 71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032422\
Data File : BM034370.D
Acq On : 24 Mar 2022 19:52
Operator : CG/JU
Sample : N2094-04 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)

Quant Time: Mar 25 01:10:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 02:40:59 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

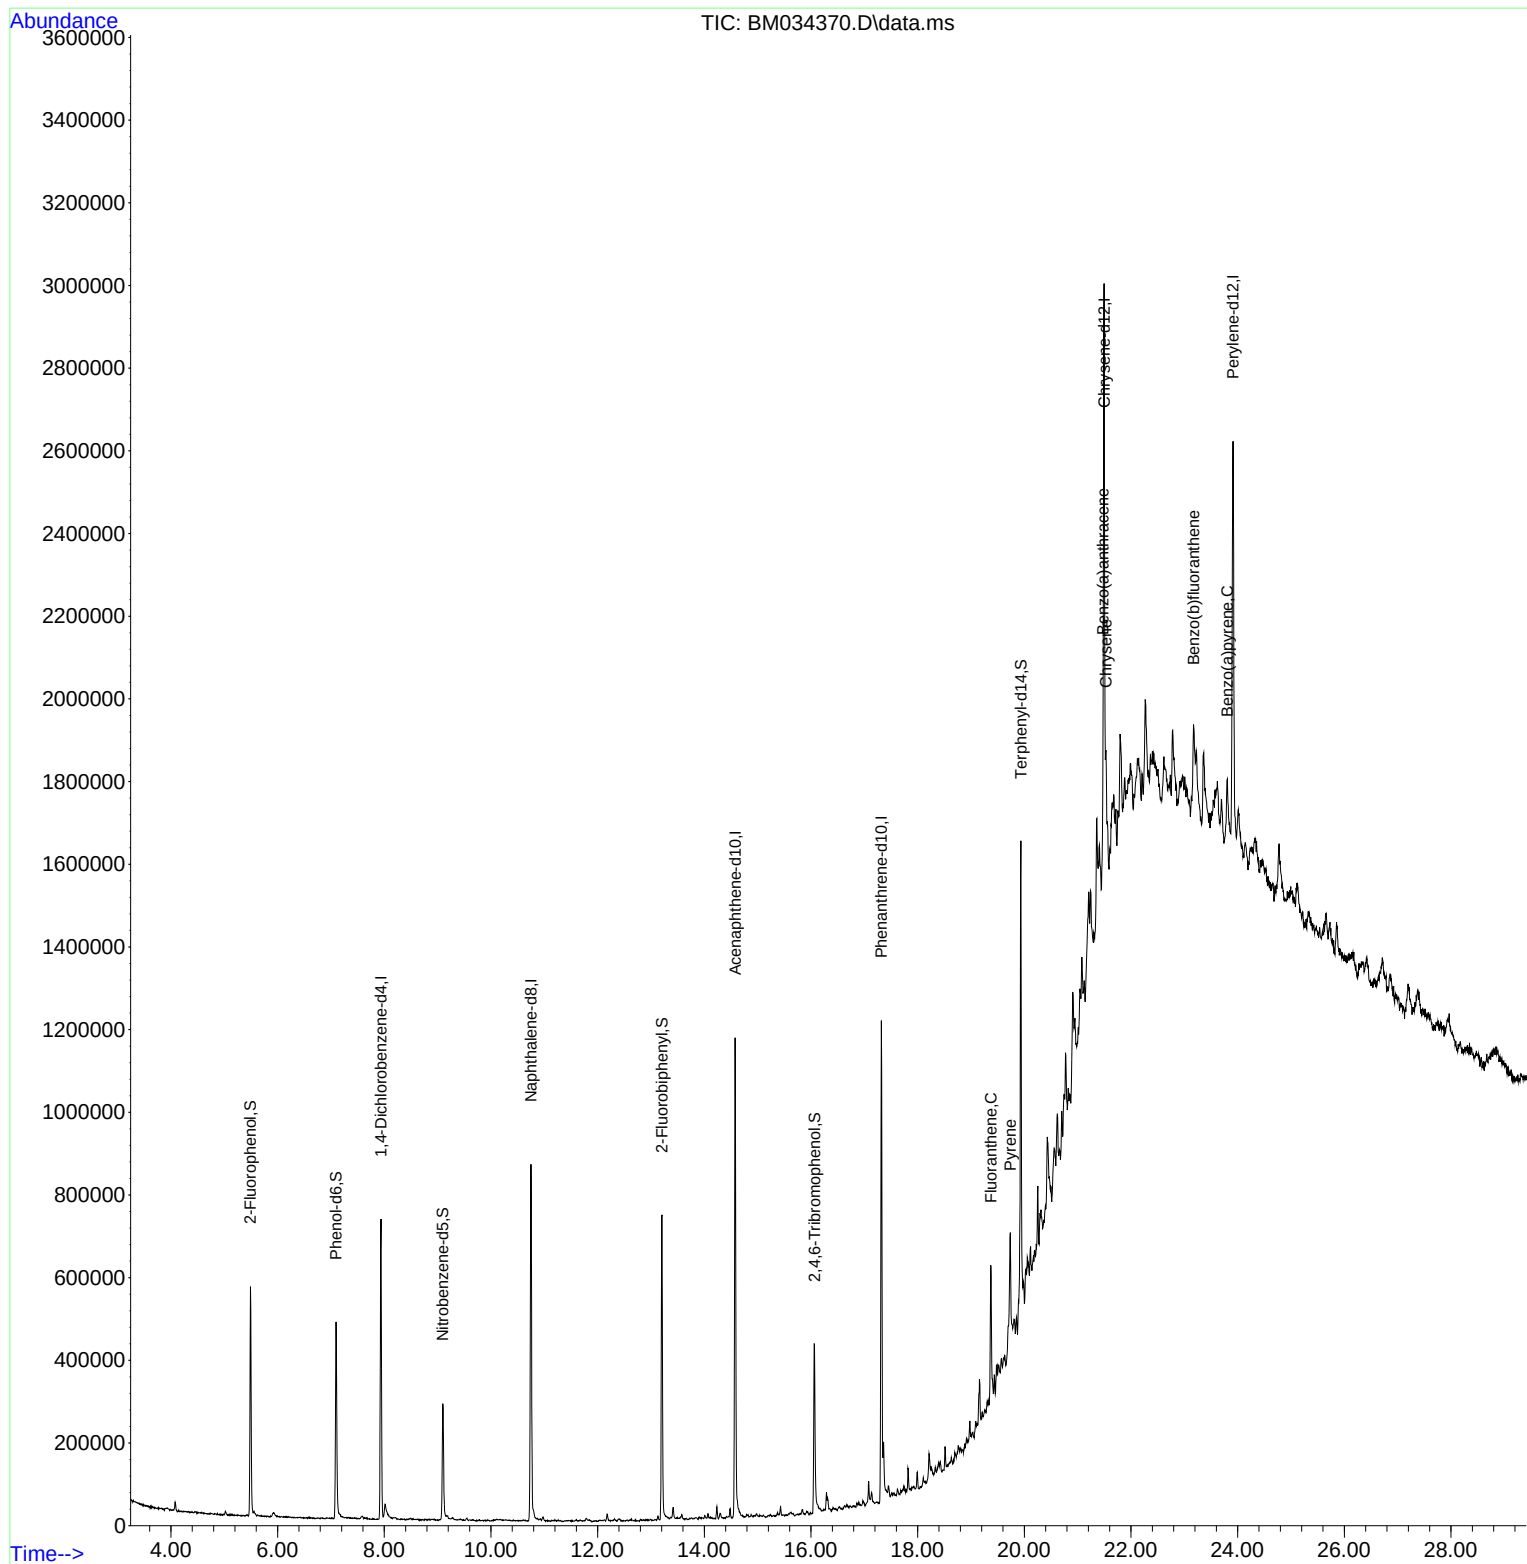



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.937 min Scan# 79
Delta R.T. -0.005 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)




Tgt Ion:152 Resp: 192094
Ion Ratio Lower Upper
152 100
150 153.8 125.4 188.2
115 62.4 50.1 75.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

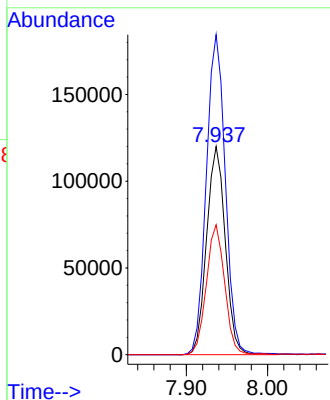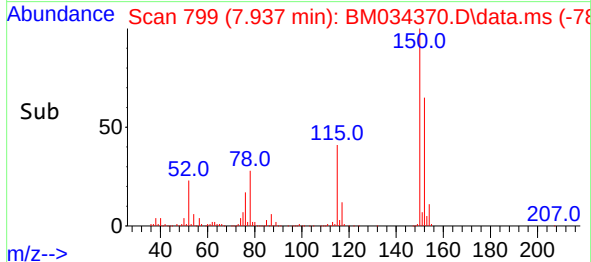


#5
2-Fluorophenol
Concen: 21.260 ng
RT: 5.490 min Scan# 383
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Tgt Ion:112 Resp: 227651
Ion Ratio Lower Upper
112 100
64 62.4 47.9 71.9
63 34.4 27.1 40.7

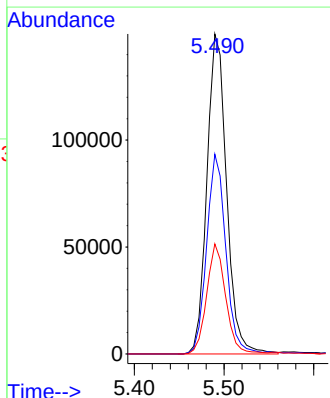



#7
Phenol-d6
Concen: 17.960 ng
RT: 7.095 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)




Tgt Ion: 99 Resp: 27534
Ion Ratio Lower Upper
99 100
42 18.8 15.6 23.4
71 35.3 30.6 46.0

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

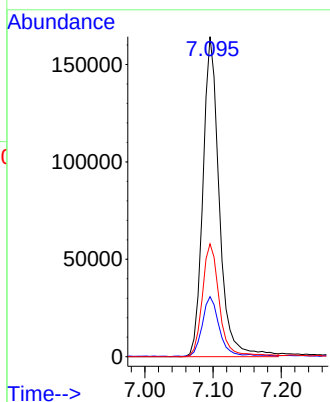


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.748 min Scan# 1277
Delta R.T. -0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Tgt Ion:136 Resp: 721455
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 8.6 6.2 9.4
68 5.8 4.3 6.5

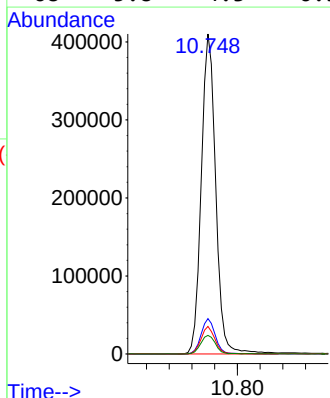



#23
Nitrobenzene-d5
Concen: 12.287 ng
RT: 9.095 min Scan# 91
Delta R.T. -0.012 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)




Tgt Ion: 82 Resp: 182075
Ion Ratio Lower Upper
82 100
128 40.5 31.9 47.9
54 50.9 40.6 61.0

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

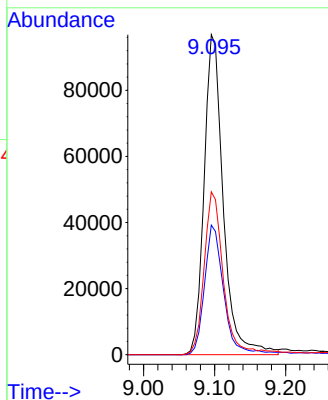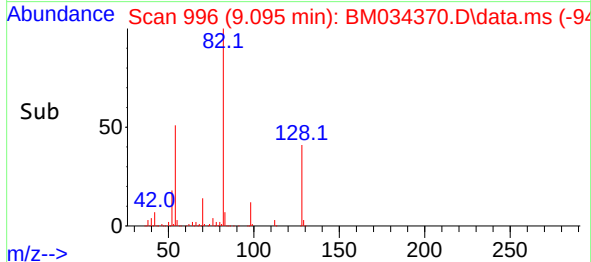


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.577 min Scan# 1928
Delta R.T. -0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52



Tgt Ion:164 Resp: 404773
Ion Ratio Lower Upper
164 100
162 101.7 81.6 122.4
160 43.6 35.6 53.4

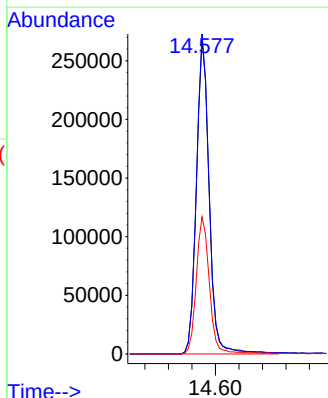







#42
2,4,6-Tribromophenol
Concen: 16.174 ng
RT: 16.065 min Scan# 2182
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)

Tgt Ion:330 Resp: 8824
Ion Ratio Lower Upper
330 100
332 100.6 78.2 117.4
141 38.6 30.6 45.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

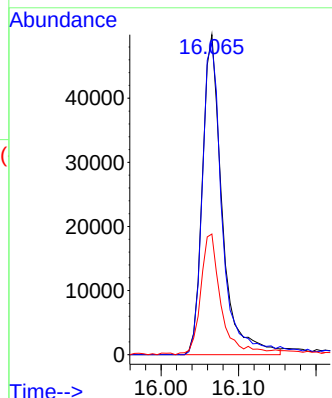

#45
2-Fluorobiphenyl
Concen: 13.735 ng
RT: 13.207 min Scan# 1695
Delta R.T. -0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Tgt Ion:172 Resp: 406848
Ion Ratio Lower Upper
172 100
171 35.4 28.0 42.0
170 22.9 18.6 28.0

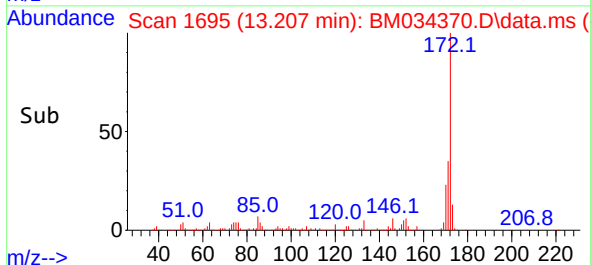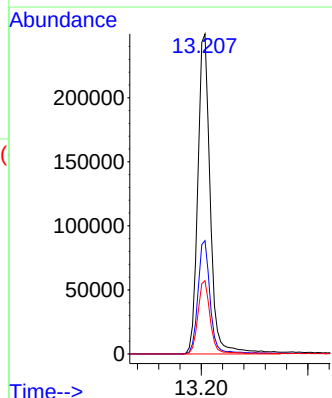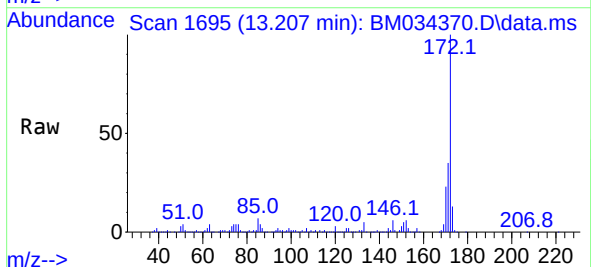







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.318 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)

Tgt Ion:188 Resp: 747600
Ion Ratio Lower Upper
188 100
94 9.4 6.6 9.8
80 10.1 7.8 11.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

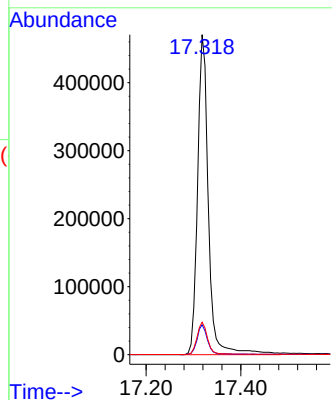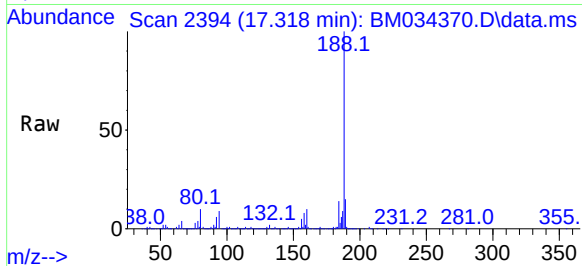

#75
Fluoranthene
Concen: 3.514 ng
RT: 19.371 min Scan# 2743
Delta R.T. -0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Tgt Ion:202 Resp: 164910
Ion Ratio Lower Upper
202 100
101 10.7 0.0 29.4
203 17.5 0.0 37.1

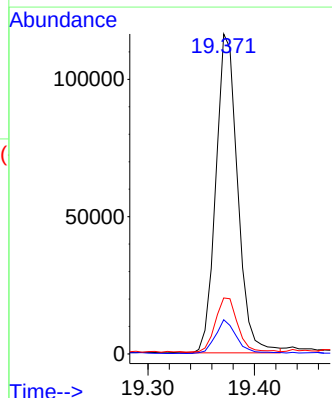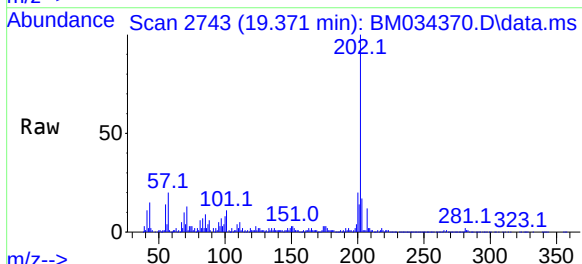







#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.495 min Scan# 3105
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)

Tgt Ion:240 Resp: 682869
Ion Ratio Lower Upper
240 100
120 9.9 7.3 10.9
236 25.7 20.2 30.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

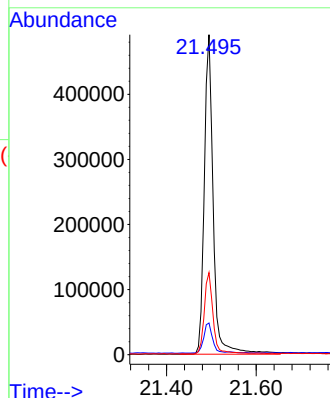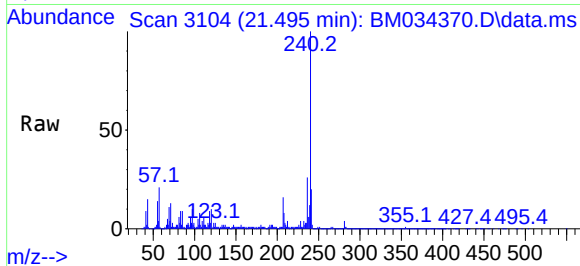

#78
Pyrene
Concen: 3.516 ng
RT: 19.736 min Scan# 2805
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52


Tgt Ion:202 Resp: 169146
Ion Ratio Lower Upper
202 100
200 20.4 16.6 24.8
203 18.3 14.1 21.1

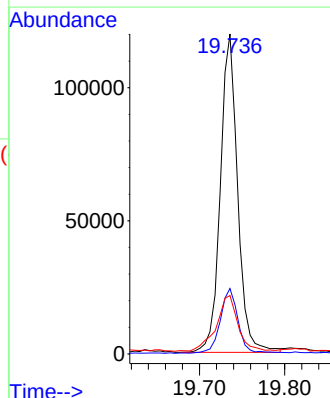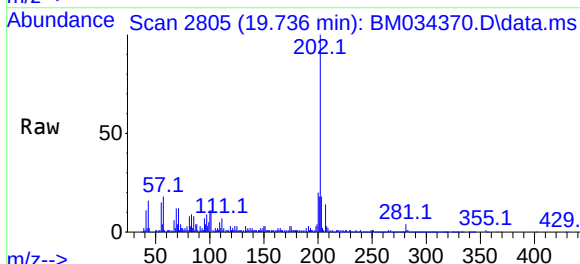



#79
Terphenyl-d14
Concen: 13.428 ng
RT: 19.936 min Scan# 2841
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)



Tgt Ion:244 Resp: 527718
Ion Ratio Lower Upper
244 100
212 7.1 5.9 8.9
122 9.9 7.8 11.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

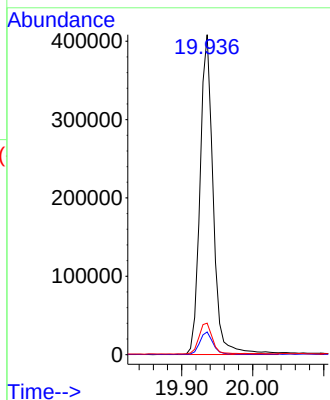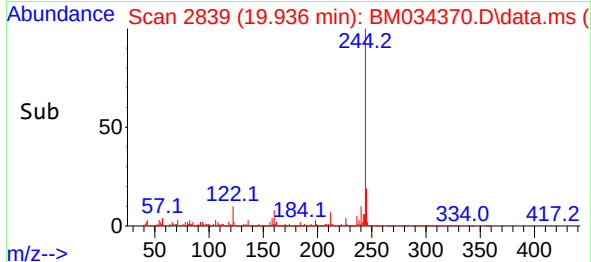

#81
Benzo(a)anthracene
Concen: 2.481 ng
RT: 21.477 min Scan# 3101
Delta R.T. -0.000 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Tgt Ion:228 Resp: 106916
Ion Ratio Lower Upper
228 100
226 28.7 21.6 32.4
229 21.6 15.8 23.6

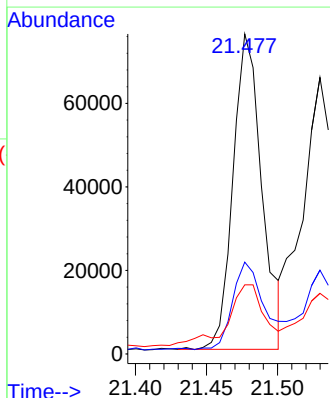







#83
Chrysene
Concen: 2.446 ng
RT: 21.530 min Scan# 3111
Delta R.T. -0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52

Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)

Tgt Ion:228 Resp: 107644
Ion Ratio Lower Upper
228 100
226 30.3 23.8 35.6
229 22.0 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

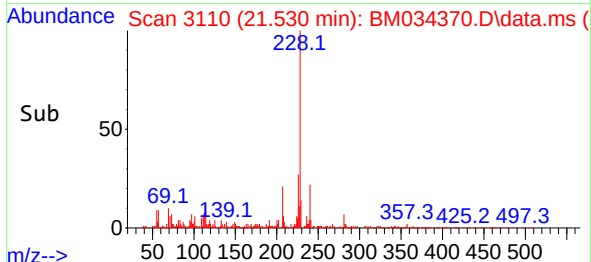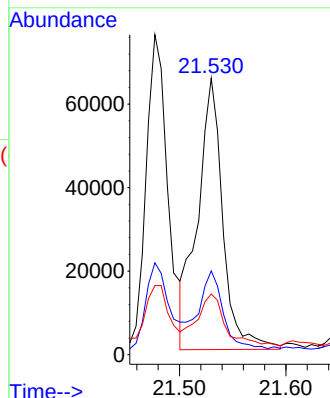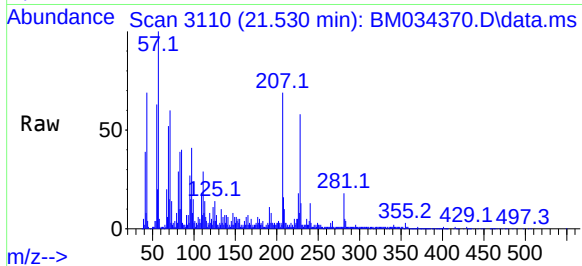

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.912 min Scan# 3515
Delta R.T. 0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52


Tgt Ion:264 Resp: 770163
Ion Ratio Lower Upper
264 100
260 23.6 18.6 28.0
265 22.3 17.6 26.4

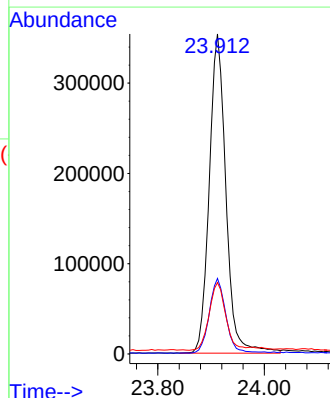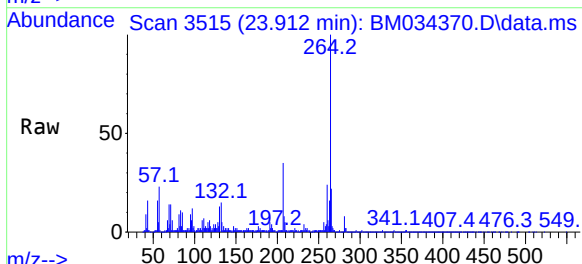



#88
Benzo(b)fluoranthene
Concen: 3.290 ng m
RT: 23.177 min Scan# 31
Delta R.T. 0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52




Instrument :
BNA_M
ClientSampleId :
WC-2-(Q2)




Tgt Ion:252 Resp: 151510
Ion Ratio Lower Upper
252 100
253 26.2 17.8 26.8
125 31.1 7.2 10.8

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 03/25/2022
Supervised By :Jagrut Upadhyay 03/25/2022

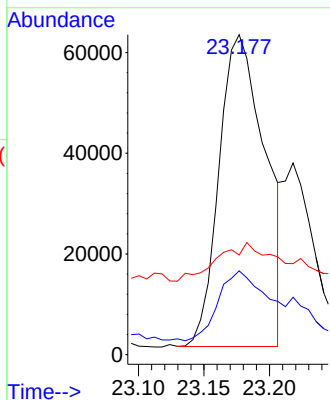

#90
Benzo(a)pyrene
Concen: 2.605 ng
RT: 23.806 min Scan# 3497
Delta R.T. 0.006 min
Lab File: BM034370.D
Acq: 24 Mar 2022 19:52



Tgt Ion:252 Resp: 101705
Ion Ratio Lower Upper
252 100
253 25.9 17.5 26.3
125 37.3 7.8 11.6

