

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:48:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

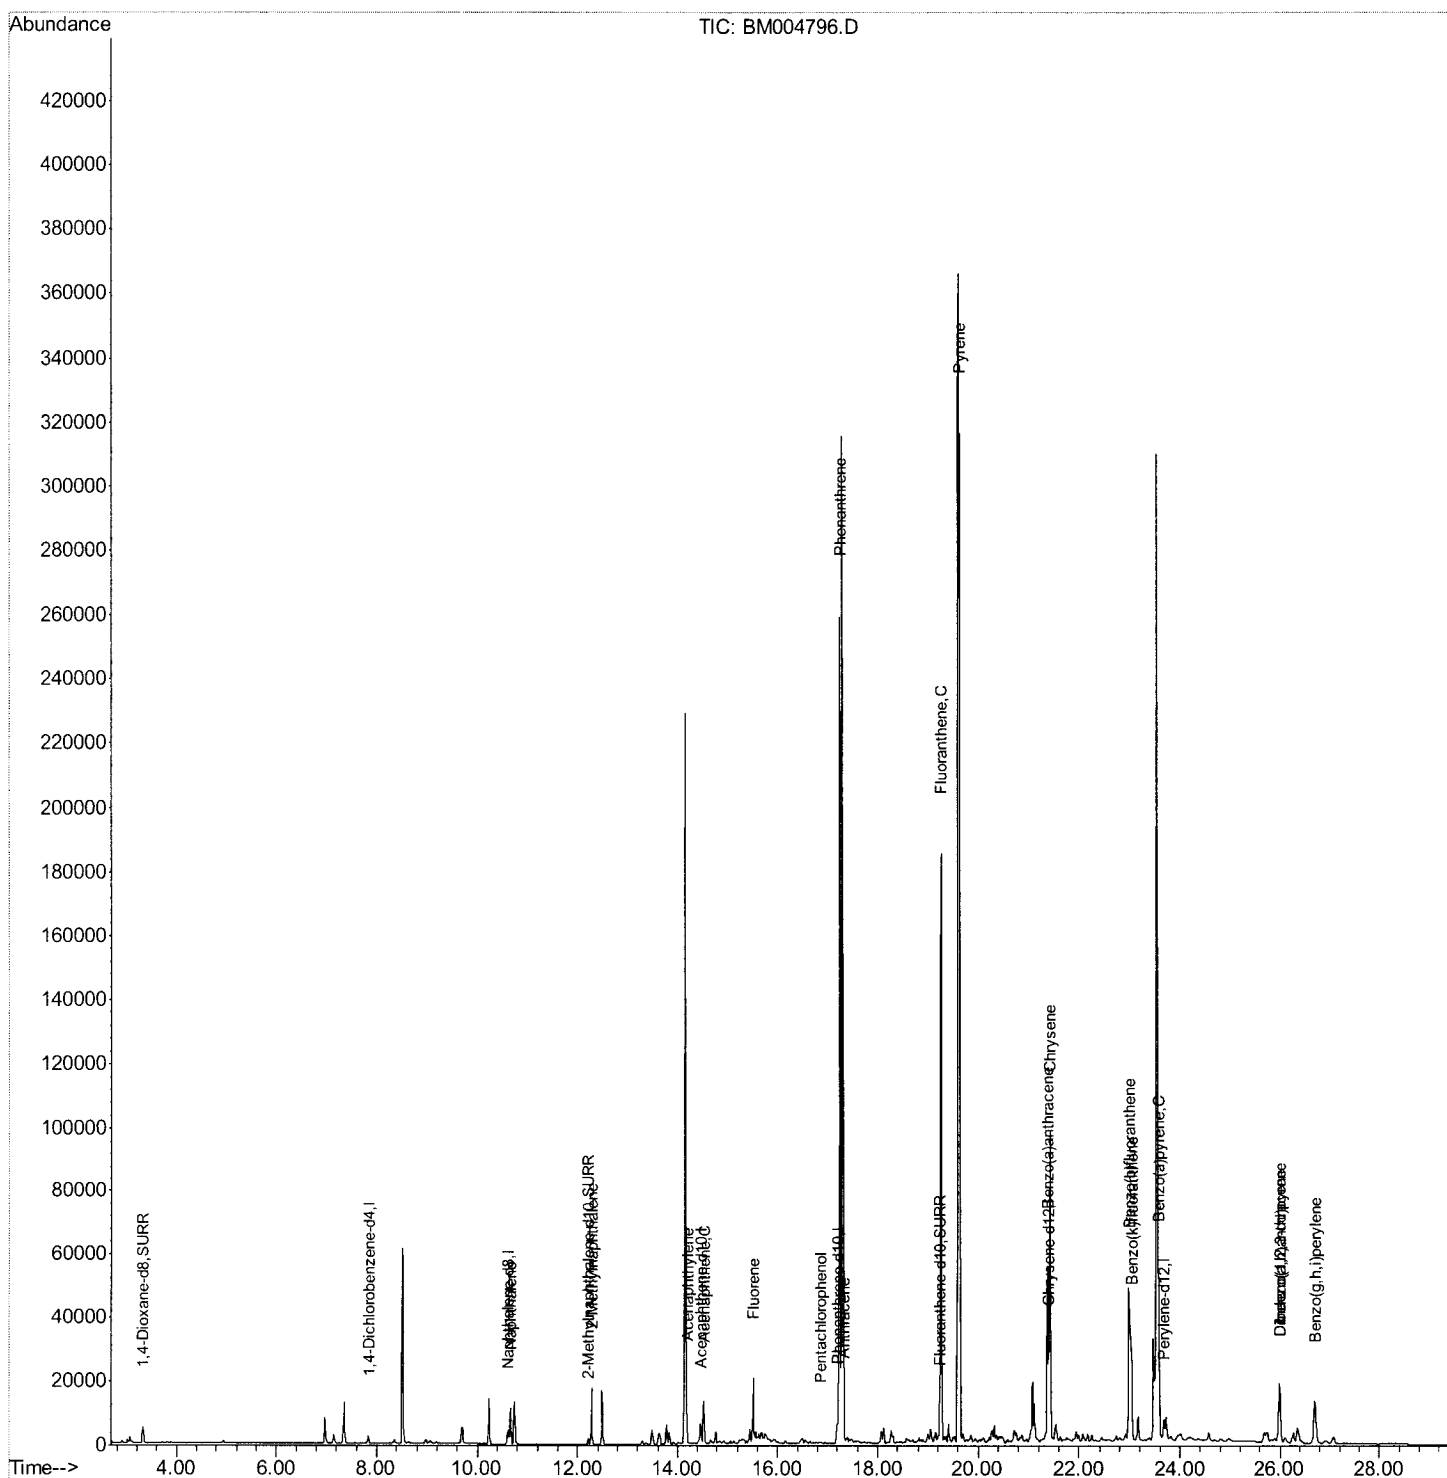

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
Data File : BM004796.D
Acq On : 26 Mar 2016 02:58
Operator : UM/SJ
Sample : H1909-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T47

Manual Integrations
APPROVED

Sohil
4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:44:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

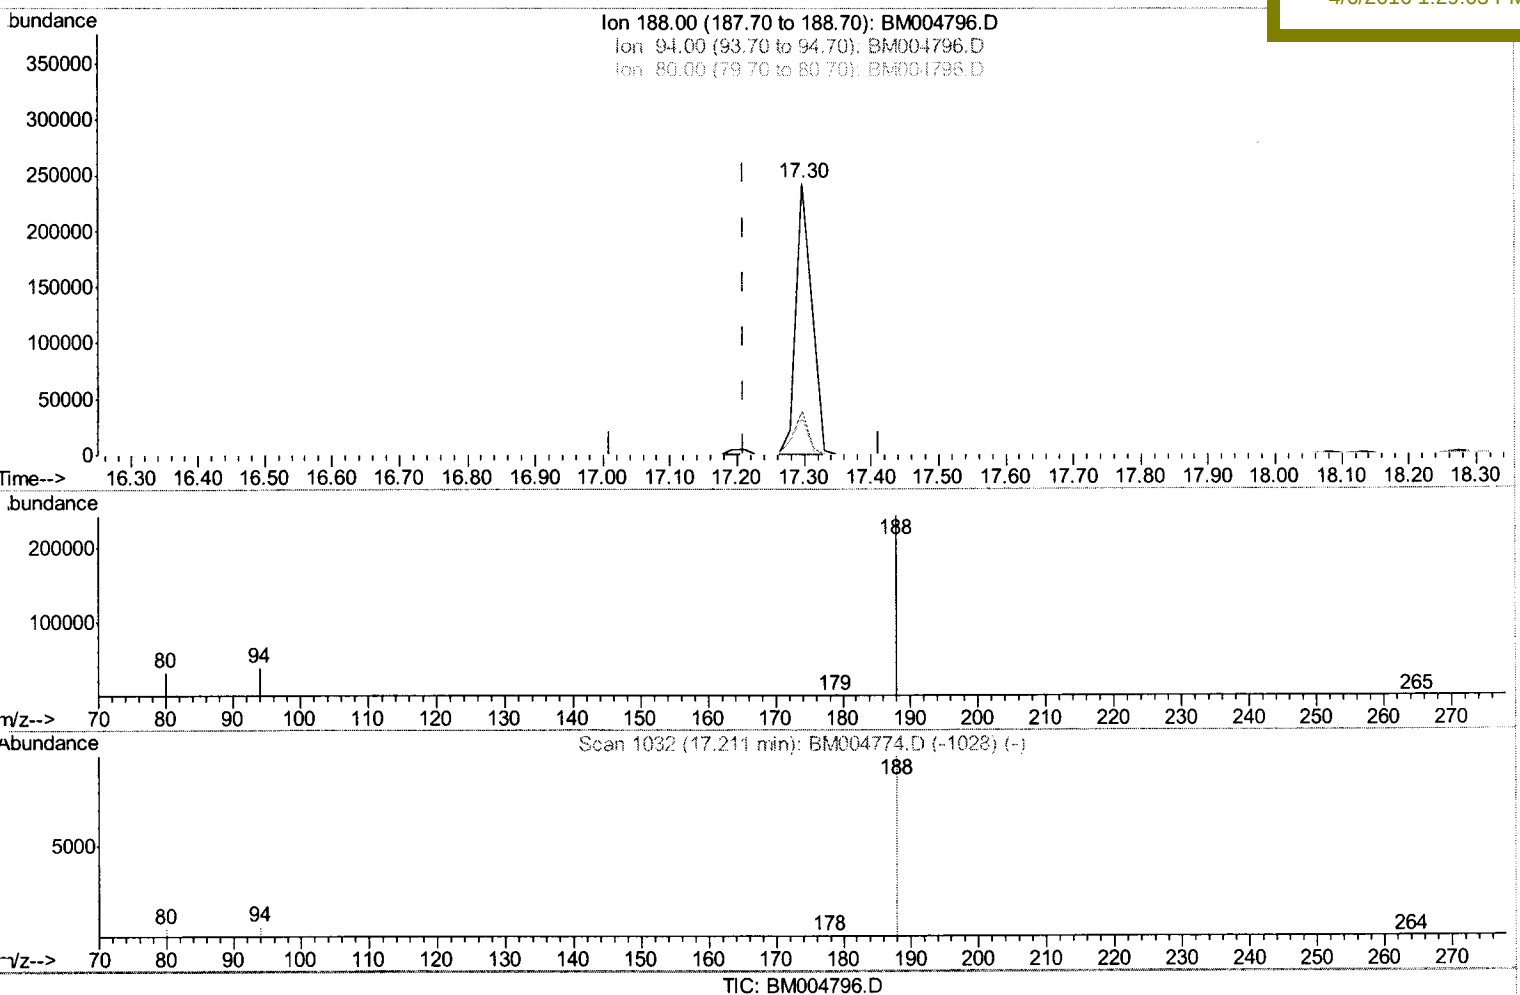

(12) Phenanthrene-d10 (I)

17.296min (+0.085) 0.40ng/ul

response 400611

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	15.90#
80.00	11.90	13.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:44:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

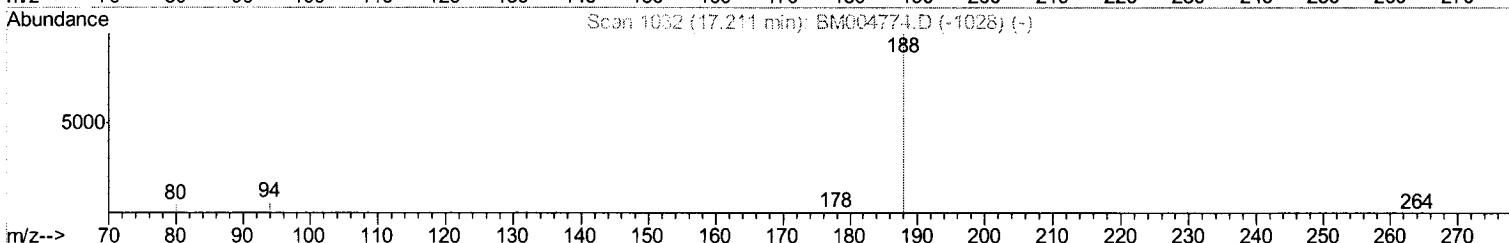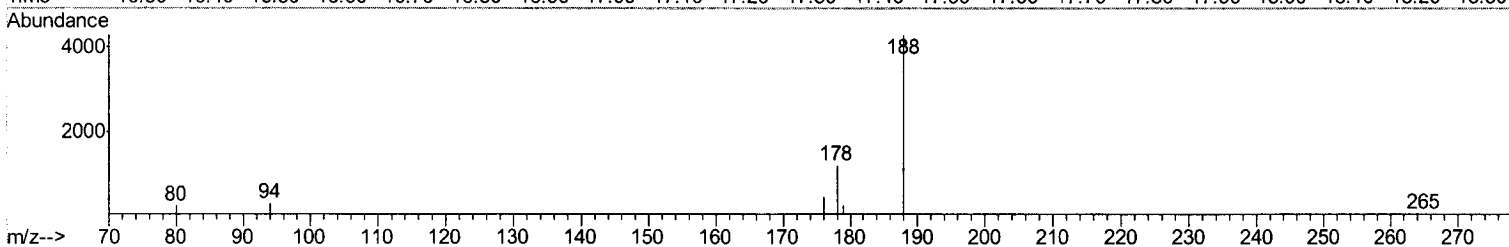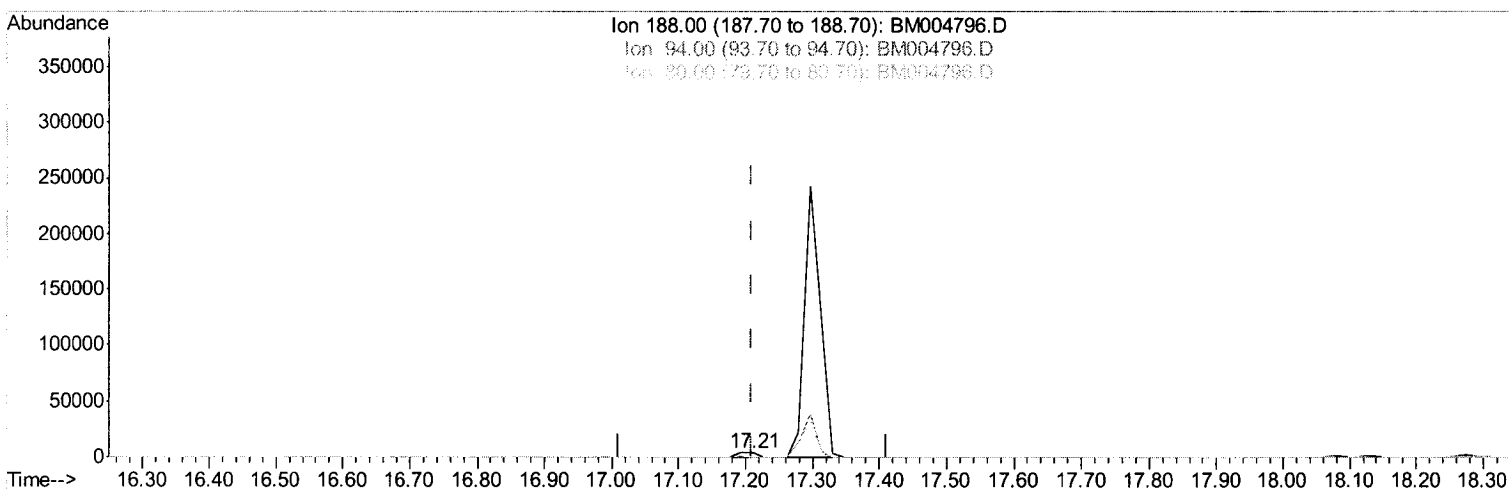

TIC: BM004796.D

(12) Phenanthrene-d10 (I)

17.210min (-0.000) 0.40ng/ul m

response 9126

U.M
 04/07/16

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	6.92#
80.00	11.90	5.82#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
Data File : BM004796.D
Acq On : 26 Mar 2016 02:58
Operator : UM/SJ
Sample : H1909-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T47

Manual Integrations
APPROVED

Sohil
4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:45:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

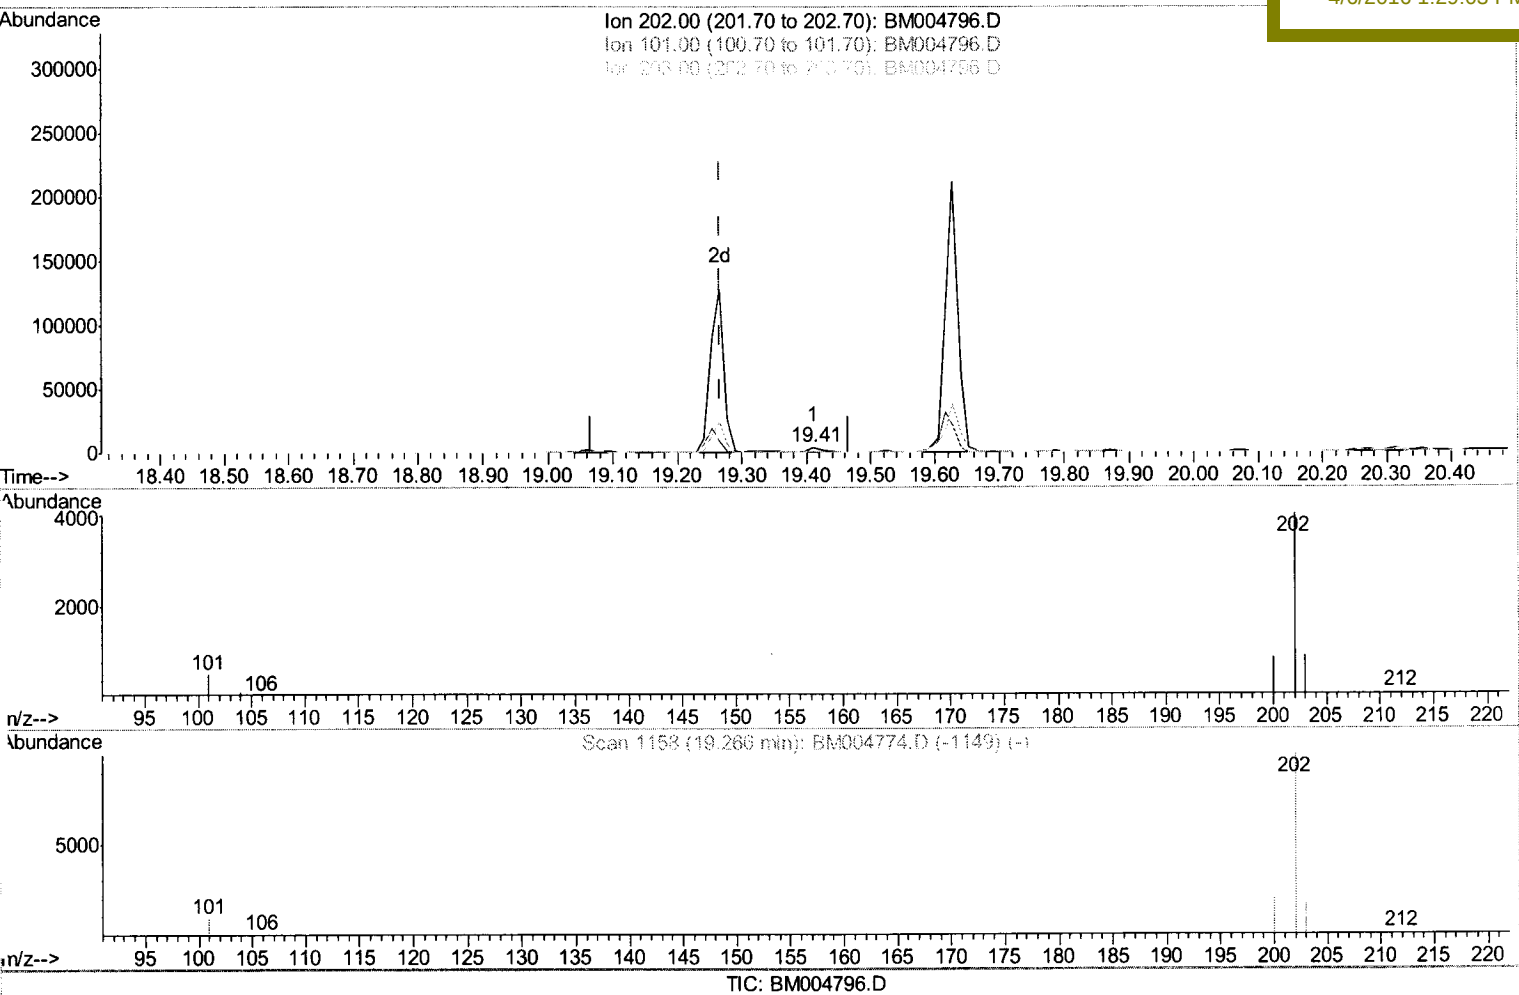

(17) Fluoranthene (C)

19.411min (+0.145) 0.20ng/ul

response 5797

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	13.90
203.00	16.30	23.31
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:45:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

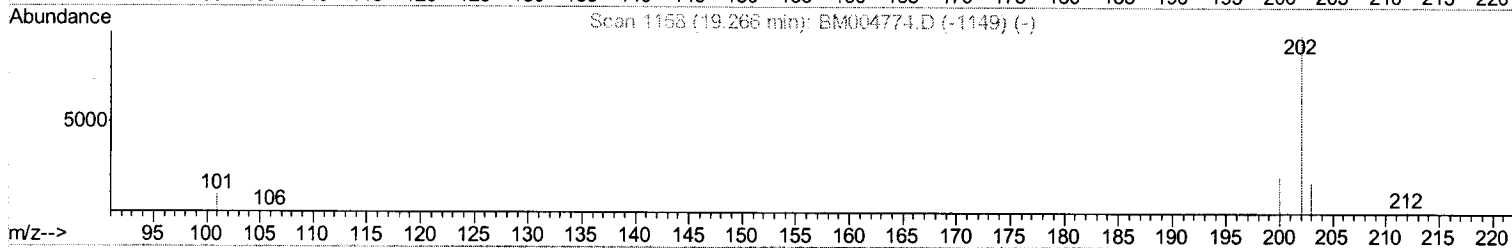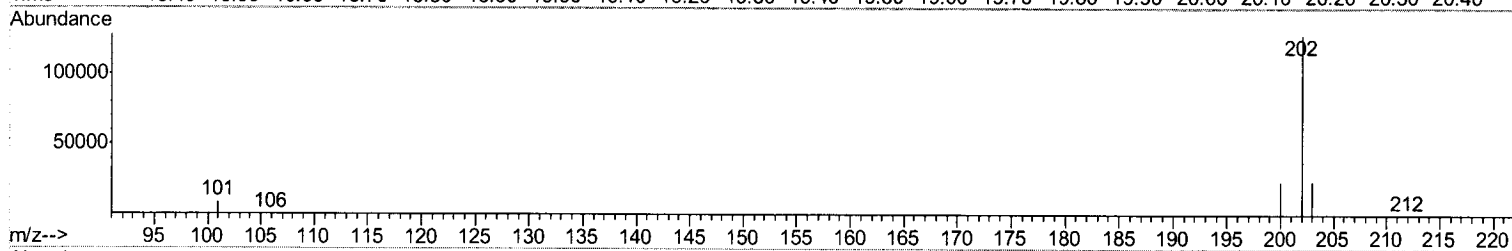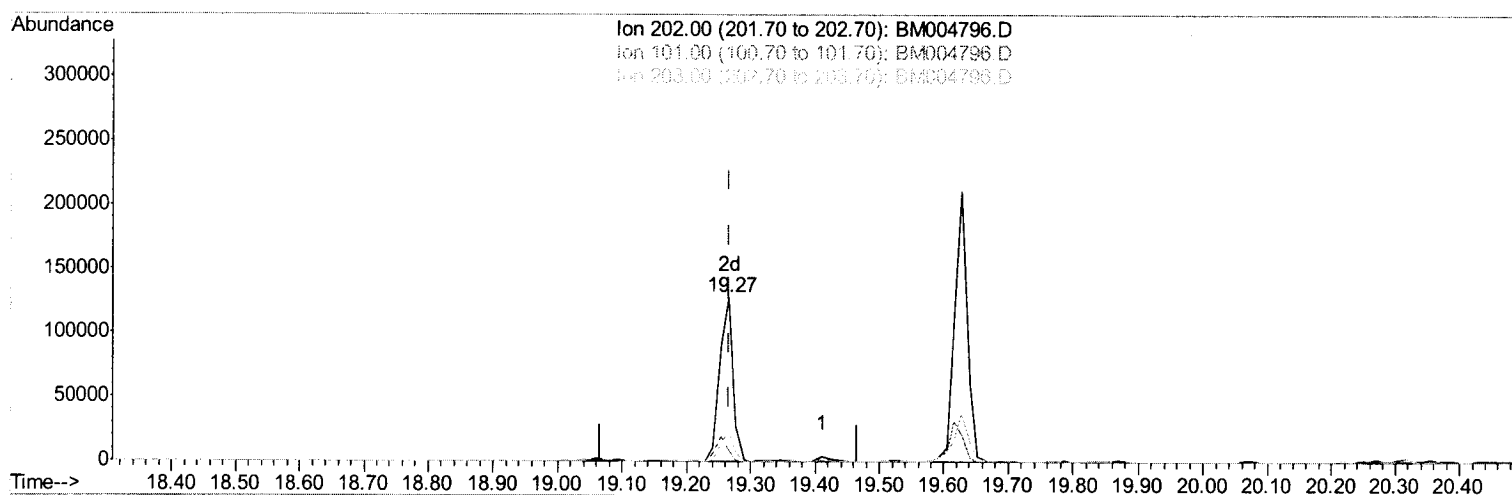

TIC: BM004796.D

(17) Fluoranthene (C)

19.266min (-0.000) 6.41ng/ul m U.M
 response 187039 04/07/16

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	7.11
203.00	16.30	18.64
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampled :
 A4T47

Quant Time: Apr 05 19:45:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
 4/6/2016 1:29:03 PM

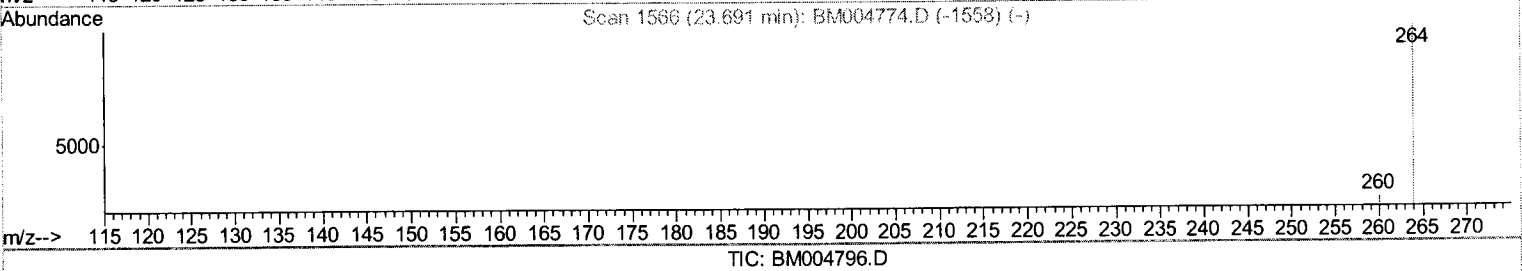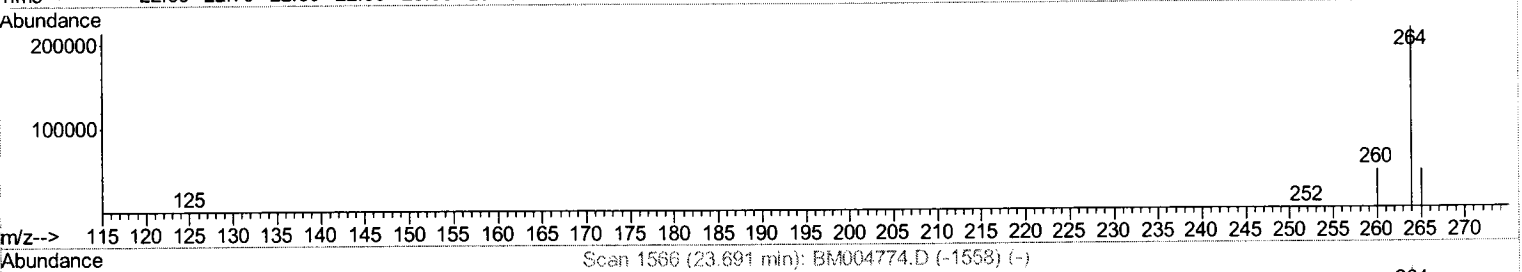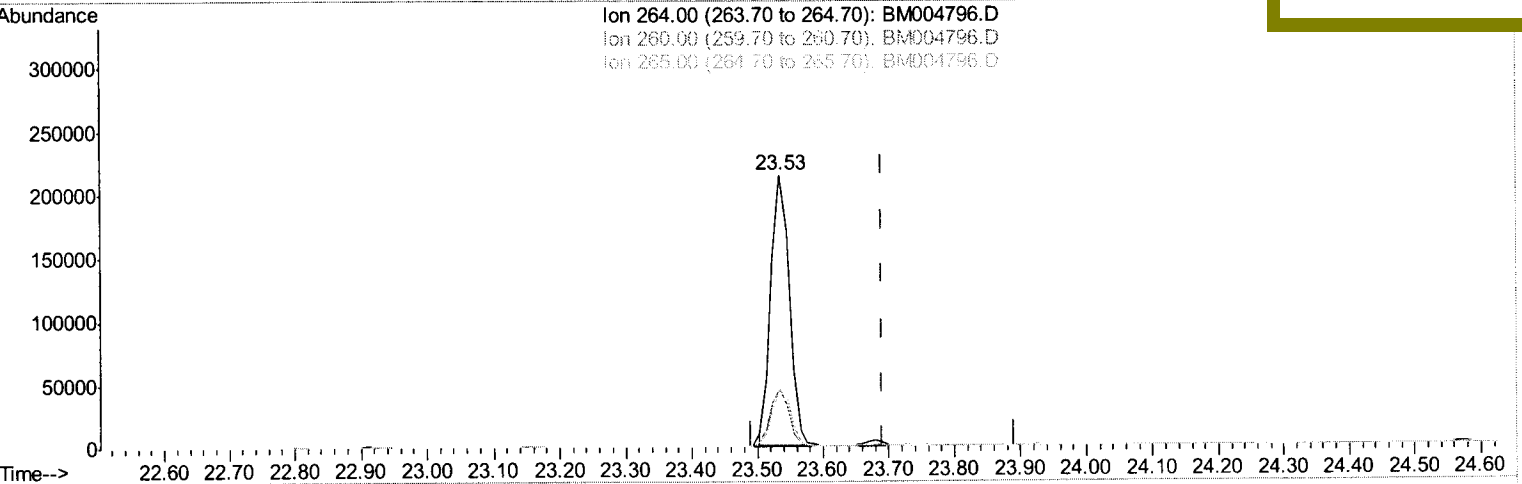

TIC: BM004796.D

(22) Perylene-d12 (I)
 23.535min (-0.157) 0.40ng/ul
 response 414864

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	21.48
265.00	38.20	21.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:45:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

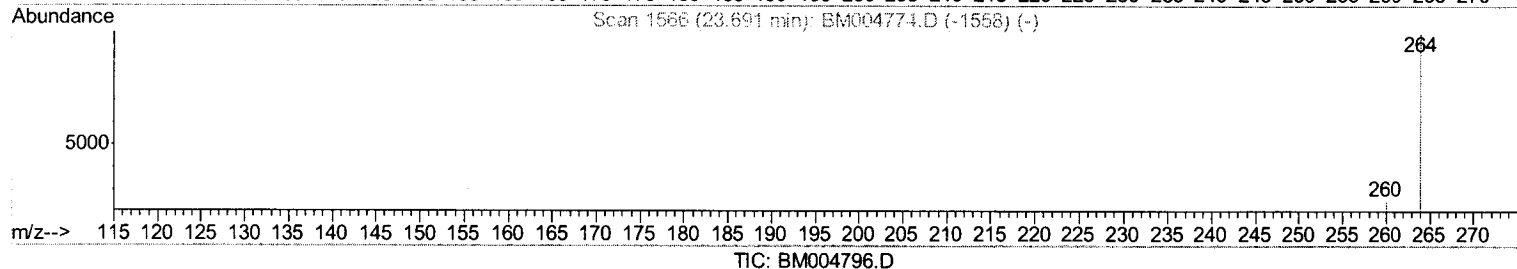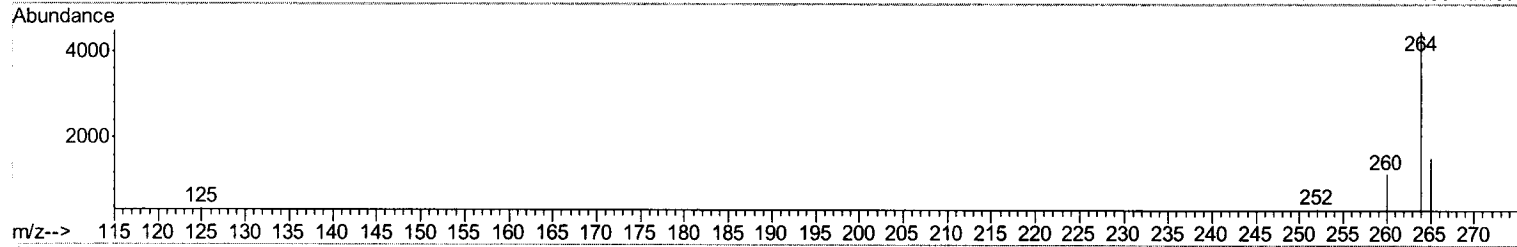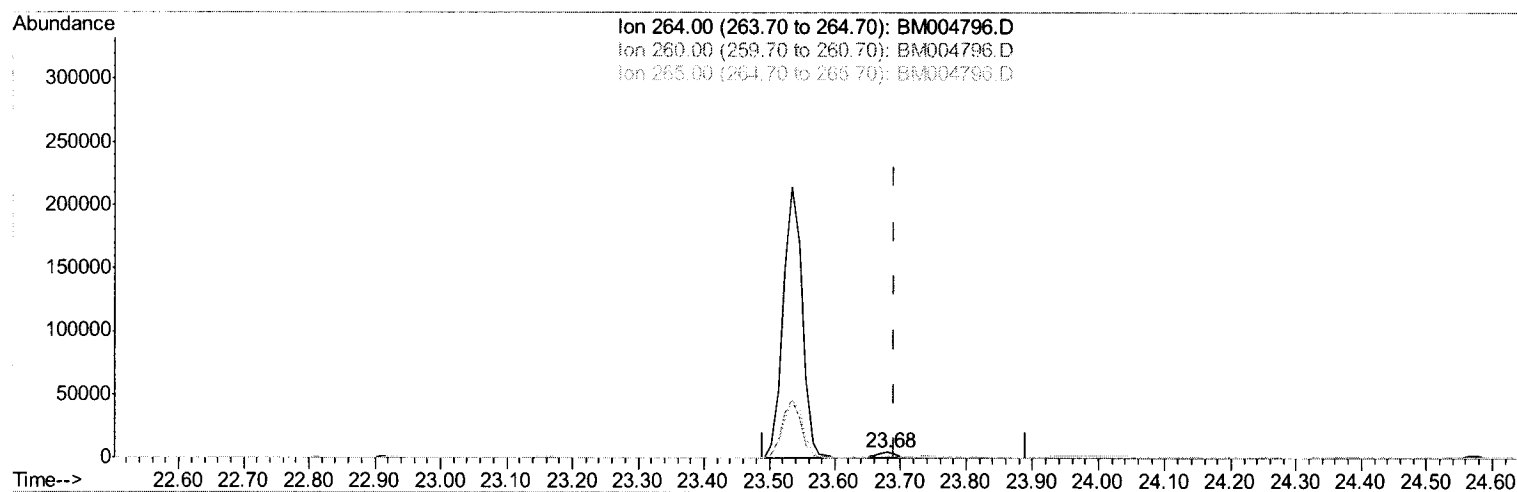

(22) Perylene-d12 (I)

23.681min (-0.011) 0.40ng/ul m

response 7899

U.M
 04/07/16

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.22
265.00	38.20	34.59
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

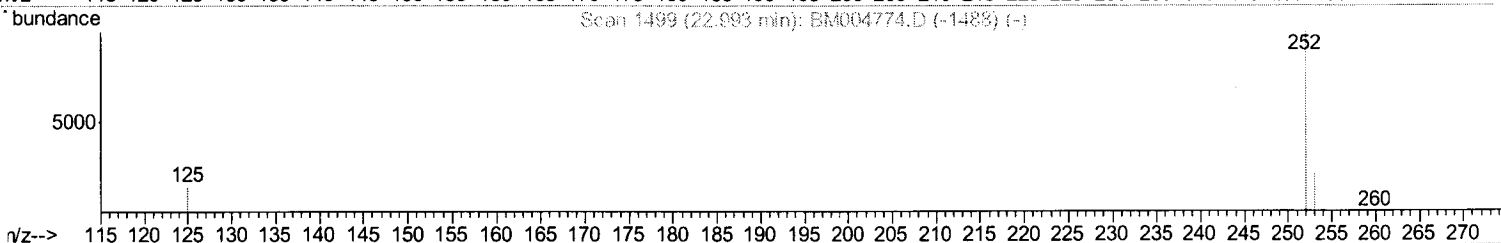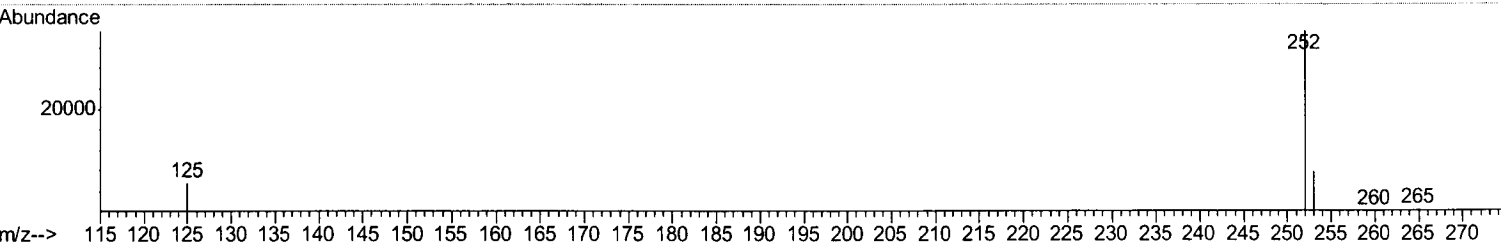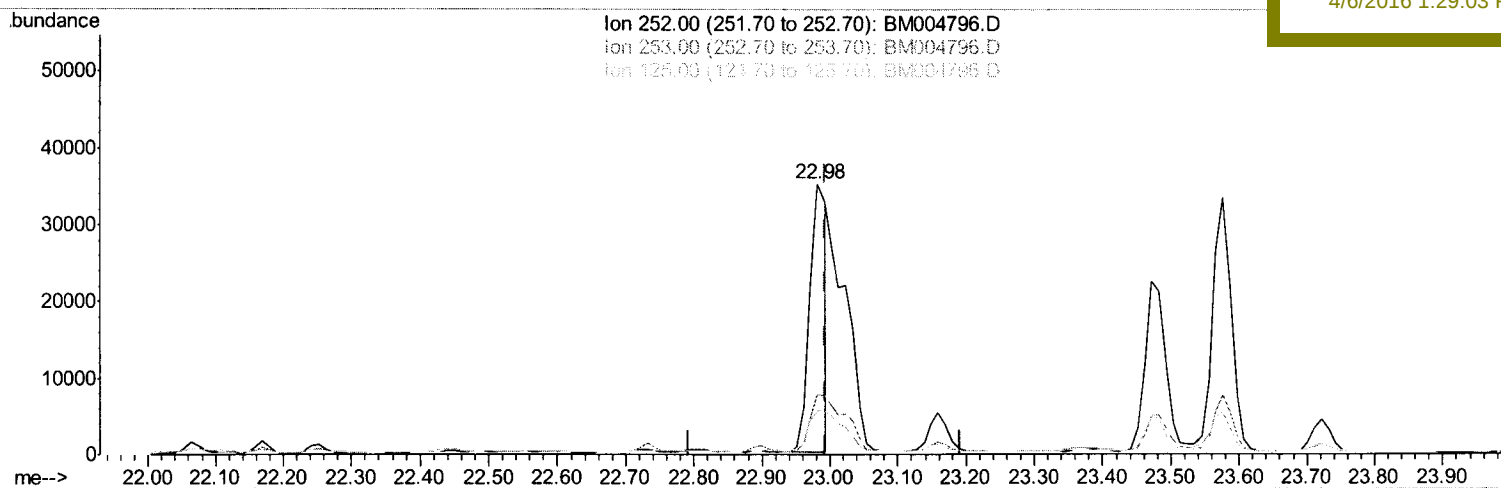

TIC: BM004796.D

(23) Benzo(b)fluoranthene

22.982min (-0.011) 2.24ng/ul

response 59620

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	22.44
125.00	14.40	16.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

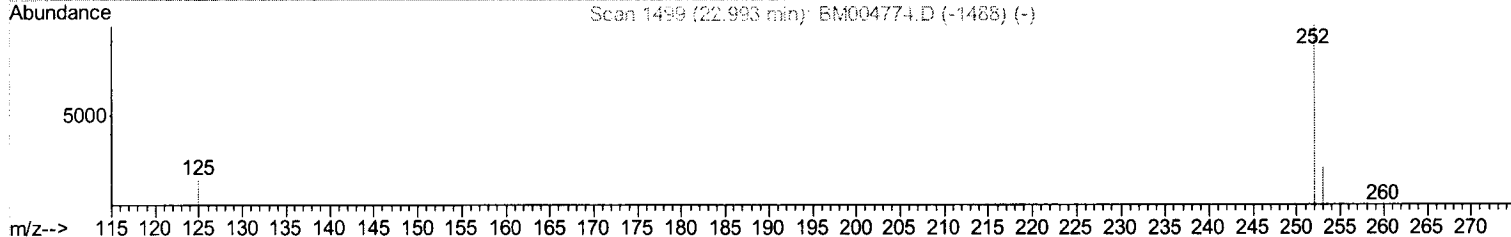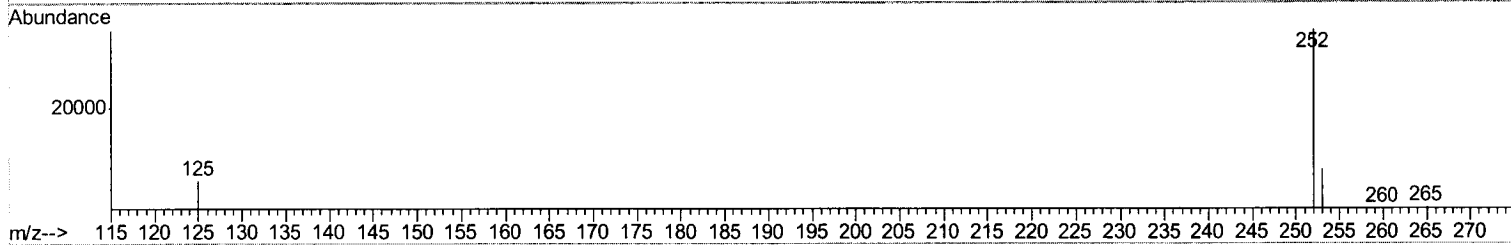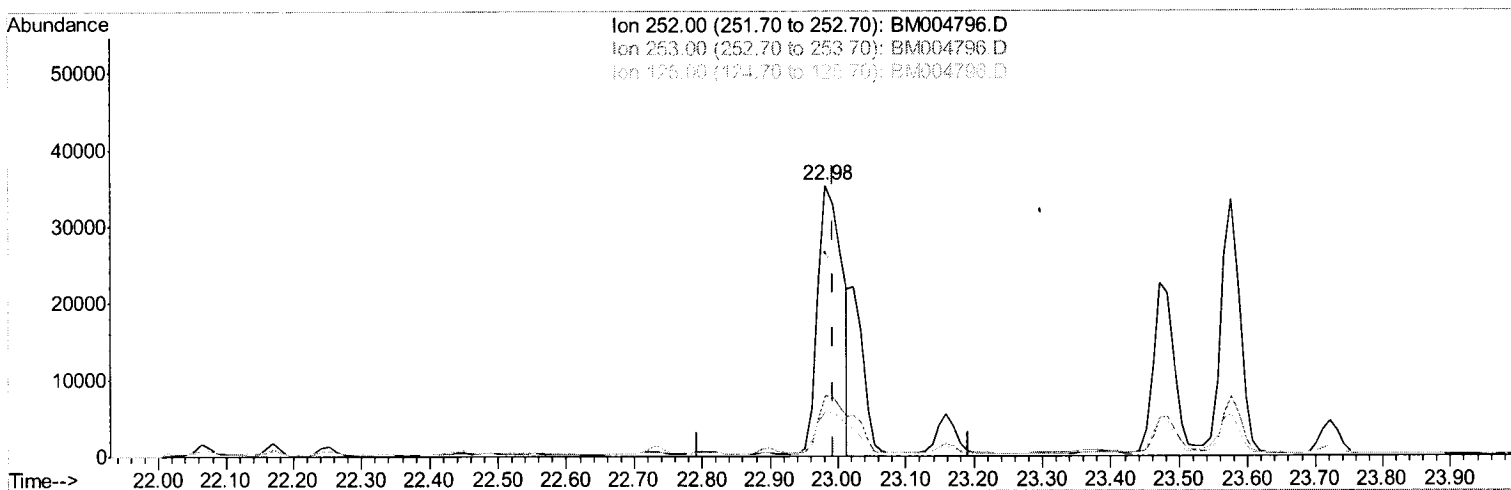

TIC: BM004796.D

(23) Benzo(b)fluoranthene

22.982min (-0.011) 3.42ng/ul m

U.M
 04/07/16

response 91072

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	22.44
125.00	14.40	16.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

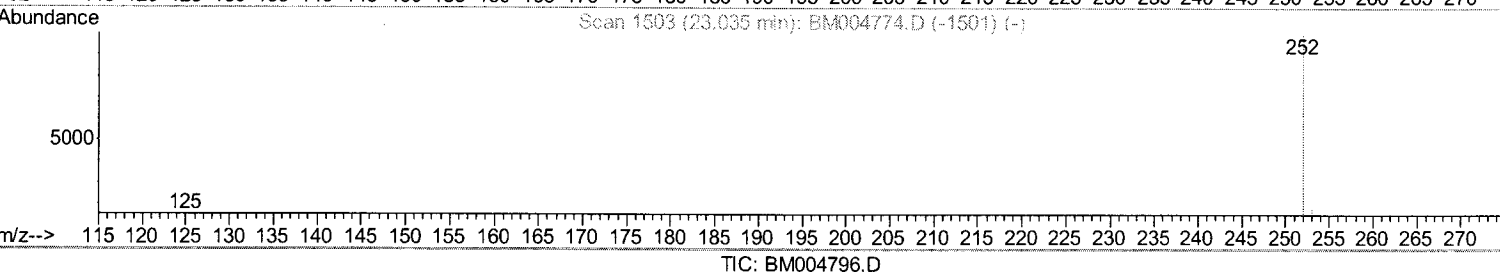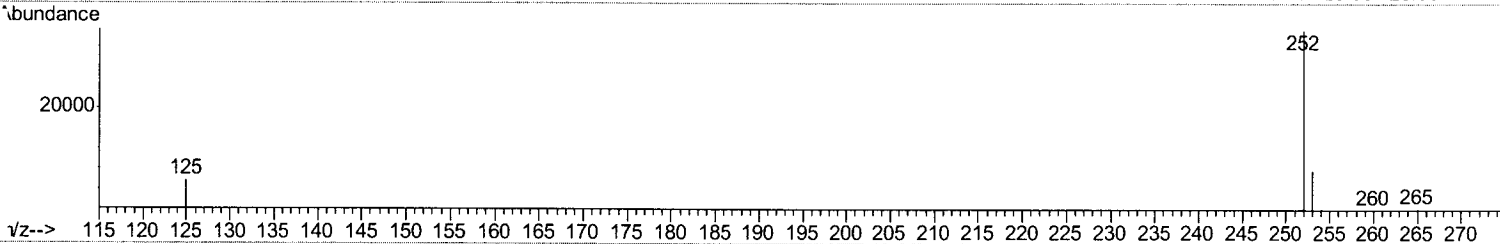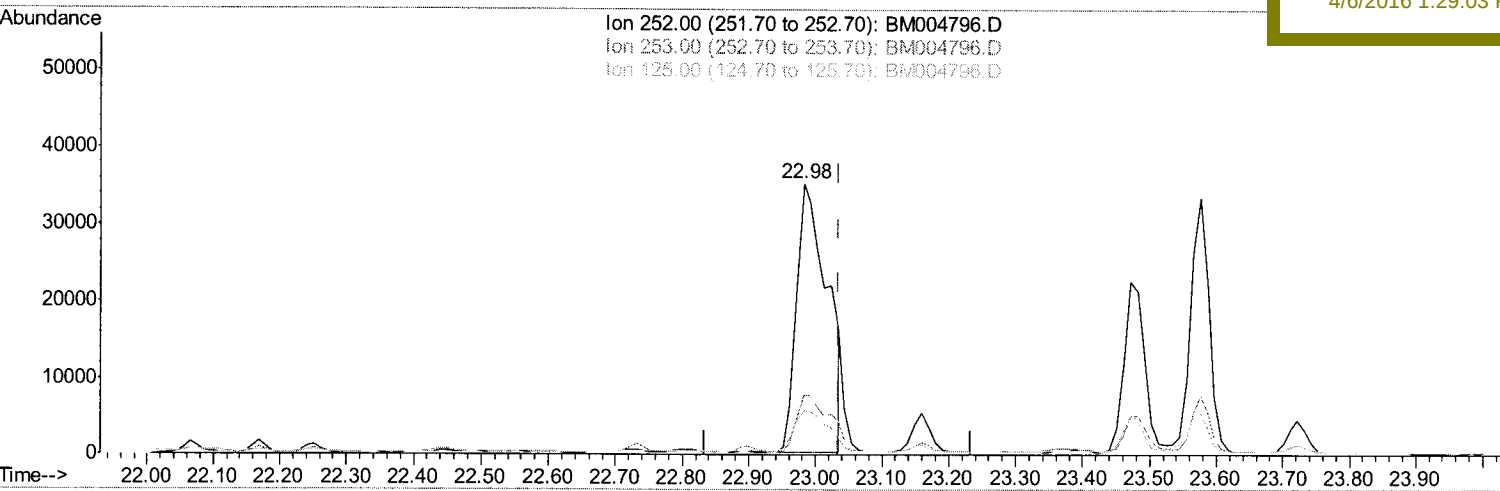

(24) Benzo(k)fluoranthene

22.982min (-0.053) 4.59ng/ul

response 113099

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	22.44
125.00	13.00	16.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

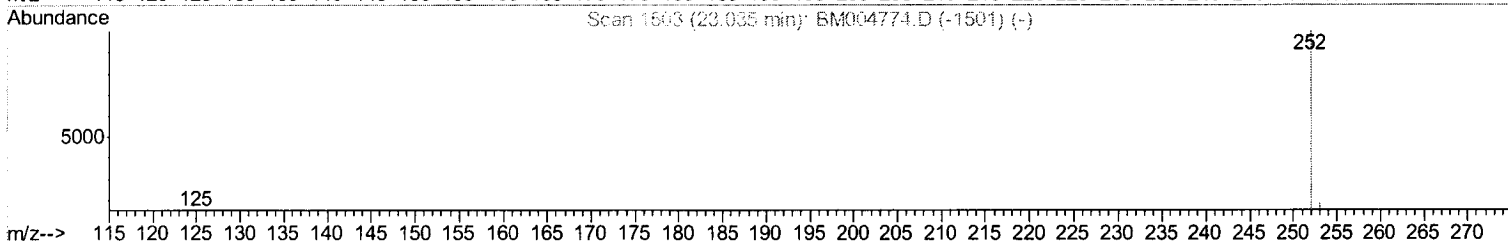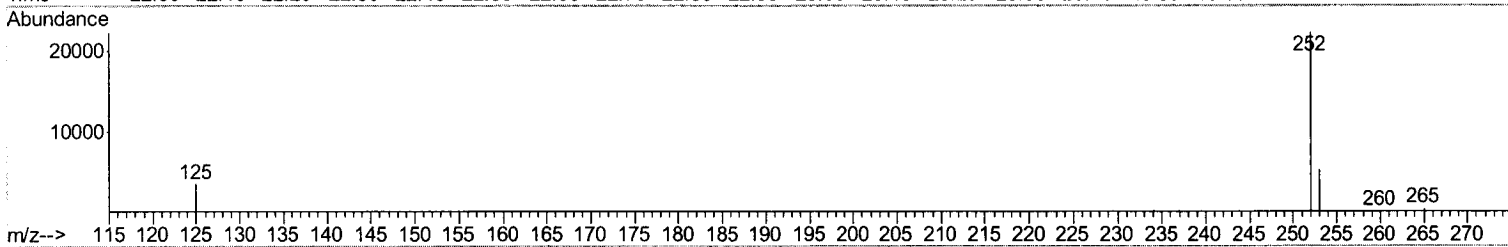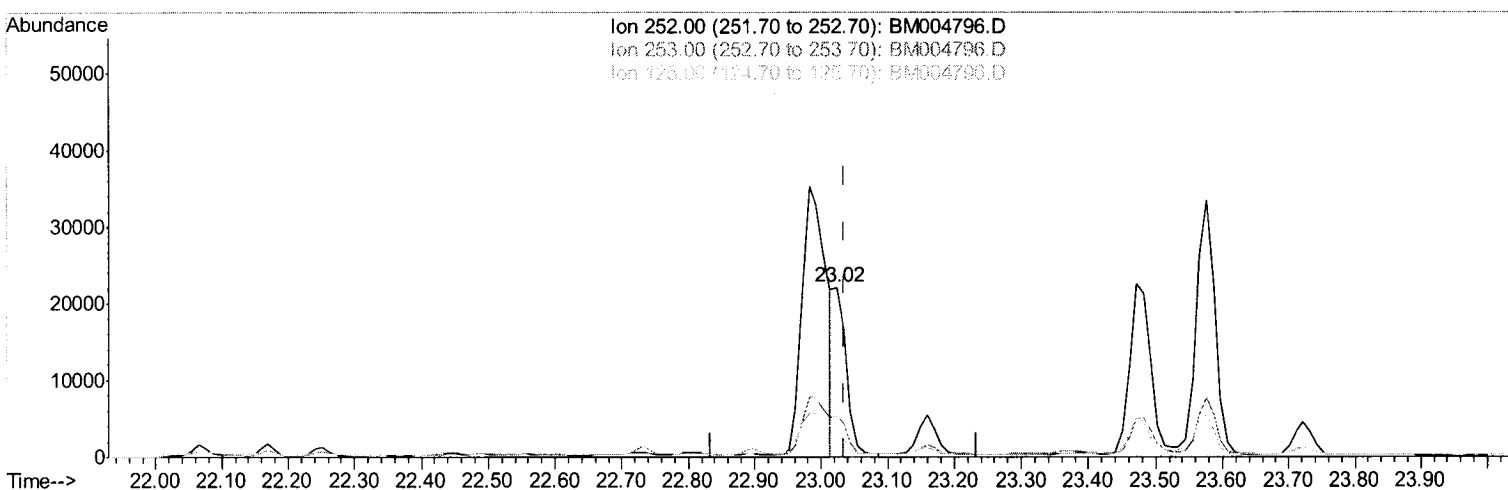

TIC: BM004796.D

(24) Benzo(k)fluoranthene

23.024min (-0.011) 1.21ng/ul m

response 29890

U.M
 24/07/16

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.52
125.00	13.00	16.06#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Apr 11 01:49:43 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 09 01:17:35 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

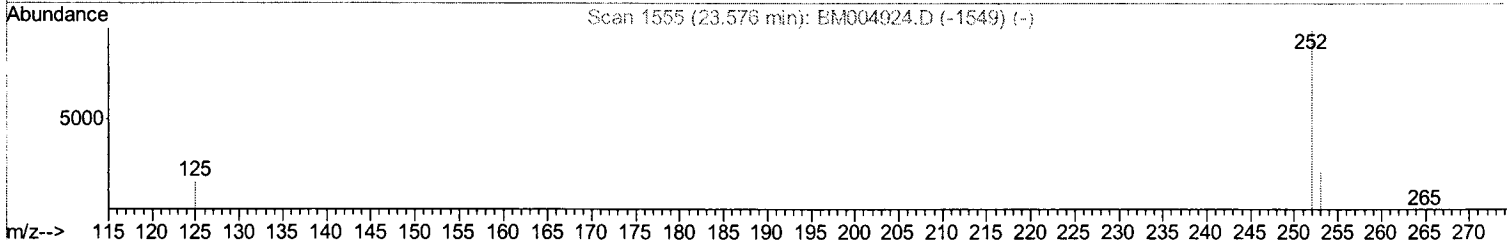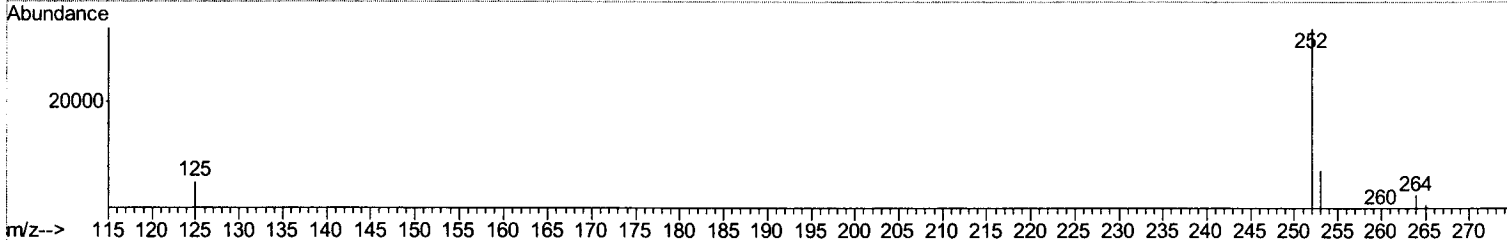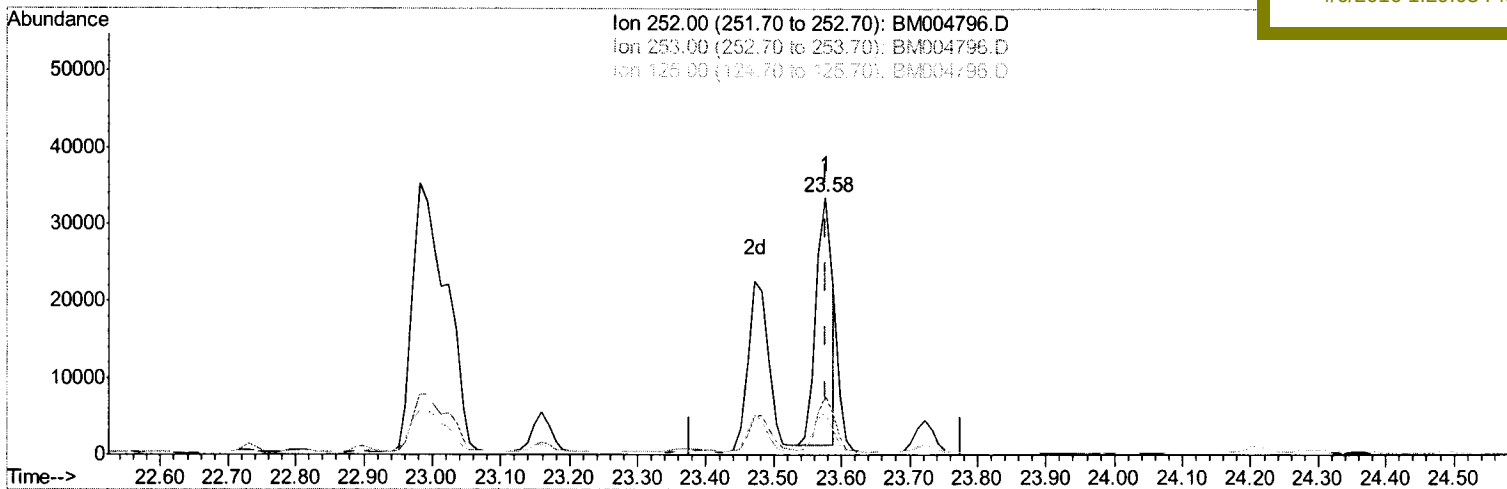

TIC: BM004796.D

(25) Benzo(a)pyrene (C)

23.576min (-0.000) 0.04ng/ul

response 54898

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	22.75
125.00	15.90	16.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

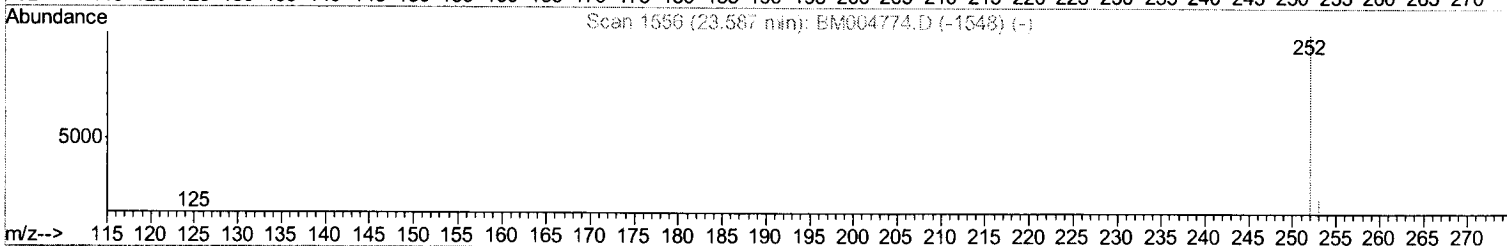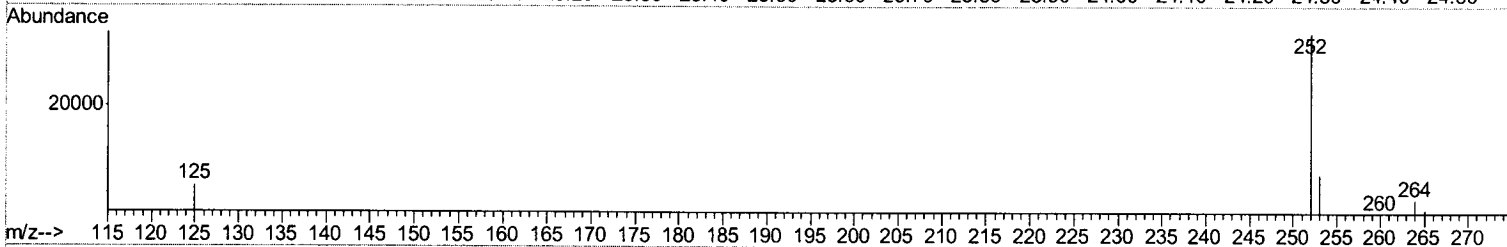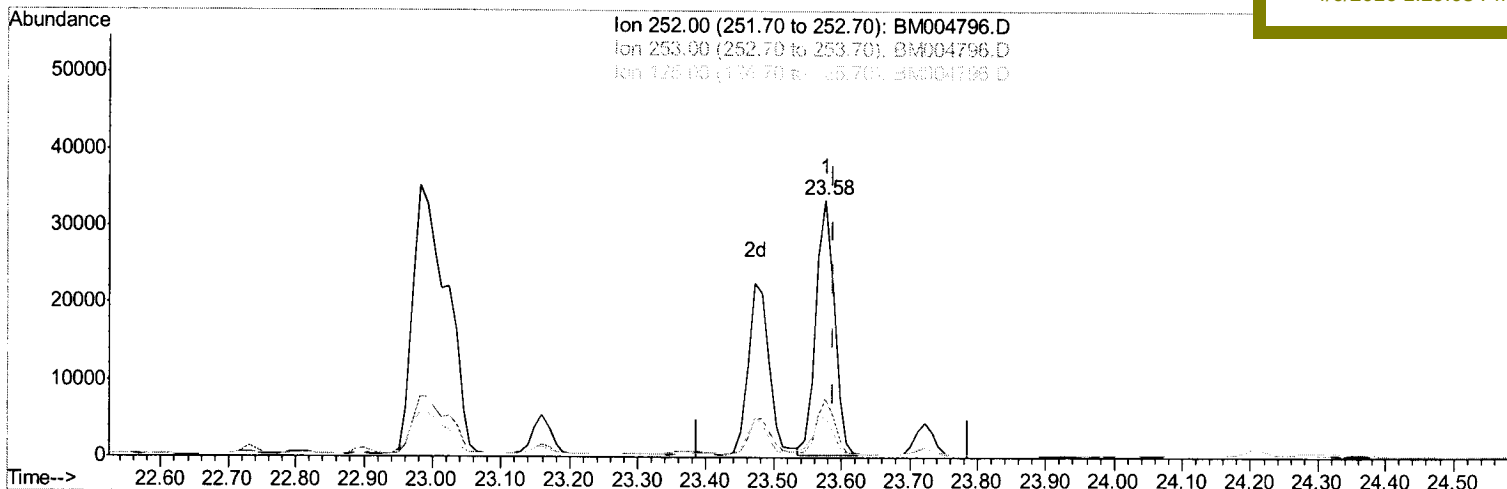

TIC: BM004796.D

(25) Benzo(a)pyrene (C)

23.576min (-0.011) 2.60ng/ul m

response 63312

Ion Exp% Act%

252.00 100 100

253.00 24.30 22.75

125.00 15.90 16.13

0.00 0.00 0.00

U.M
 04/07/16




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
Data File : BM004796.D
Acq On : 26 Mar 2016 02:58
Operator : UM/SJ
Sample : H1909-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T47

Manual Integrations
APPROVED

Sohil
4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

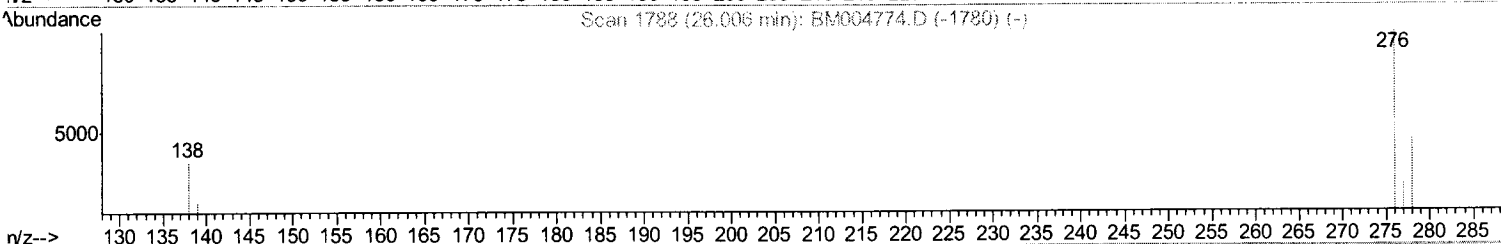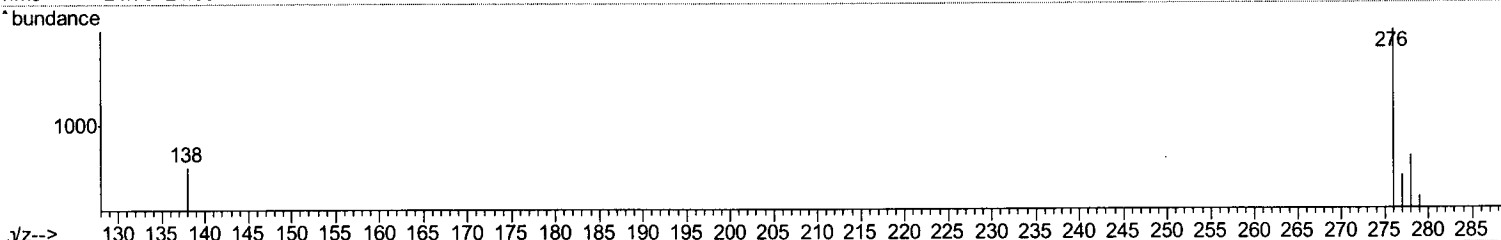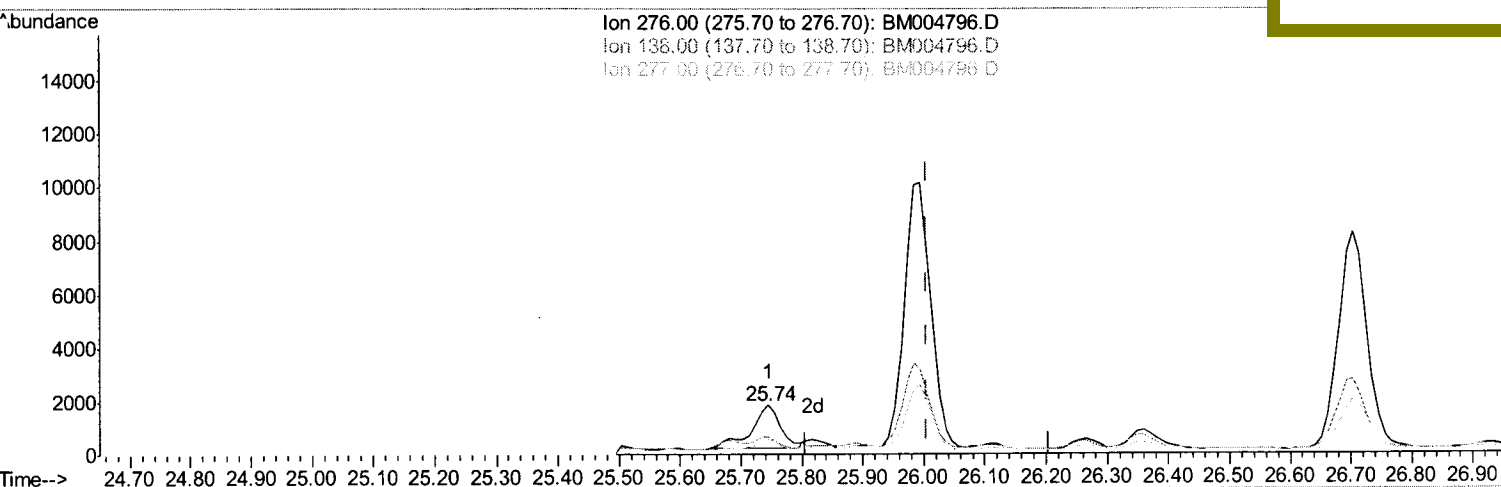

TIC: BM004796.D

(26) Indeno(1,2,3-cd)pyrene

25.745min (-0.261) 0.24ng/ul

response 5419

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	18.29
277.00	24.80	24.91
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

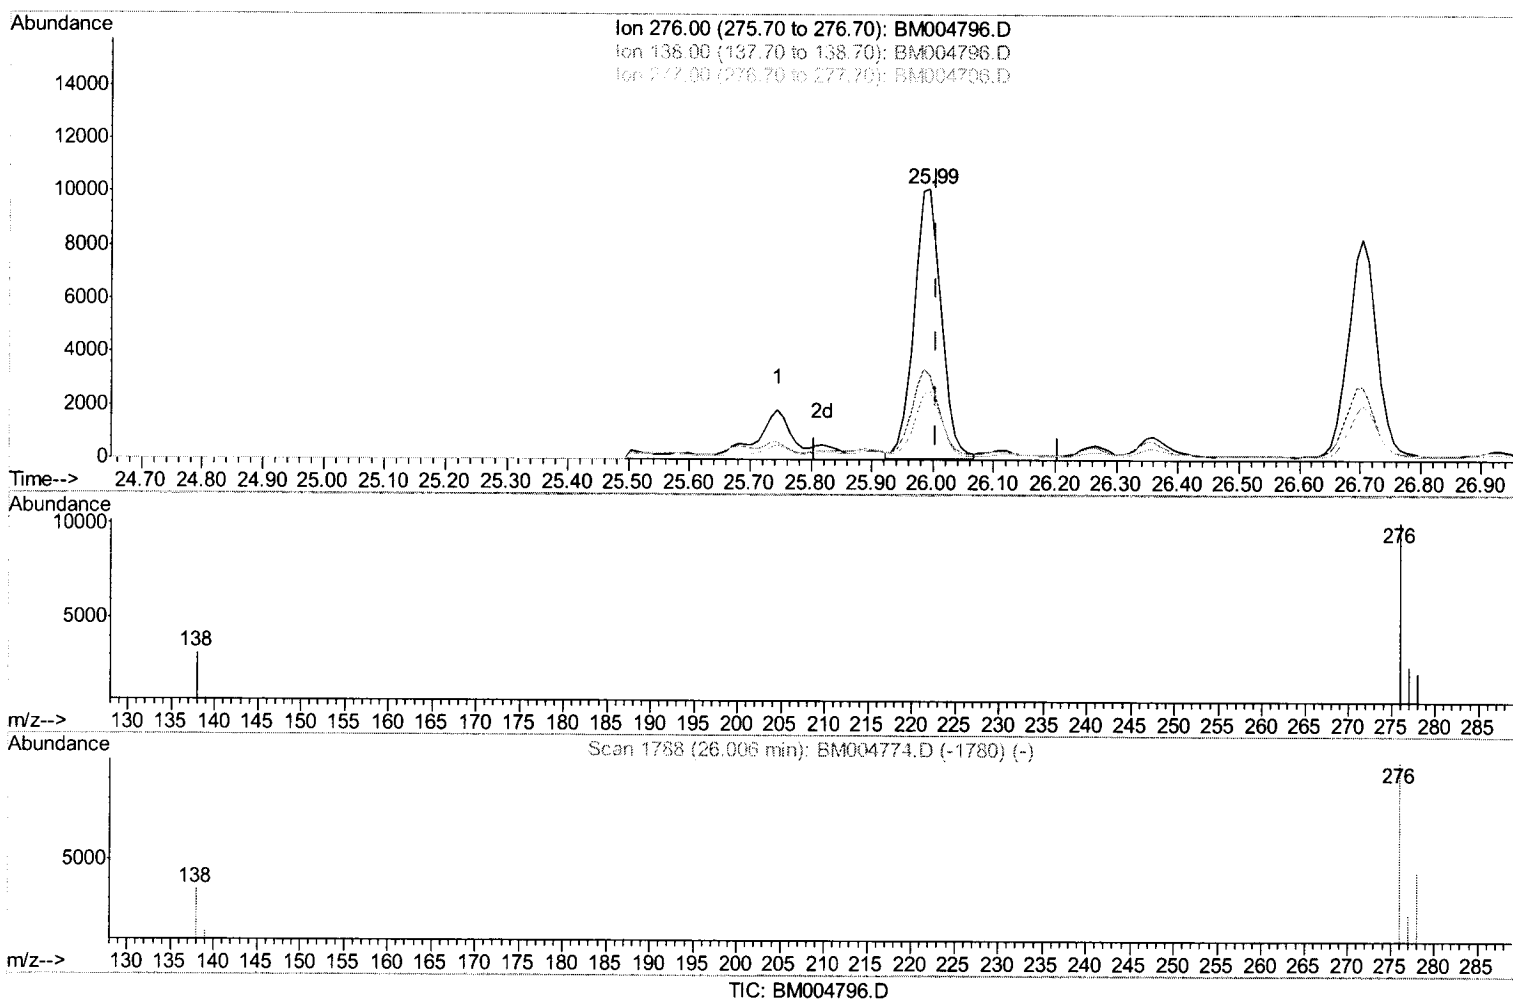

(26) Indeno(1,2,3-cd)pyrene

25.995min (-0.011) 1.39ng/ul m U.M
04/07/16
 response 31296

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	3.17#
277.00	24.80	4.31#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
Data File : BM004796.D
Acq On : 26 Mar 2016 02:58
Operator : UM/SJ
Sample : H1909-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T47

Manual Integrations
APPROVED

Sohil
4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

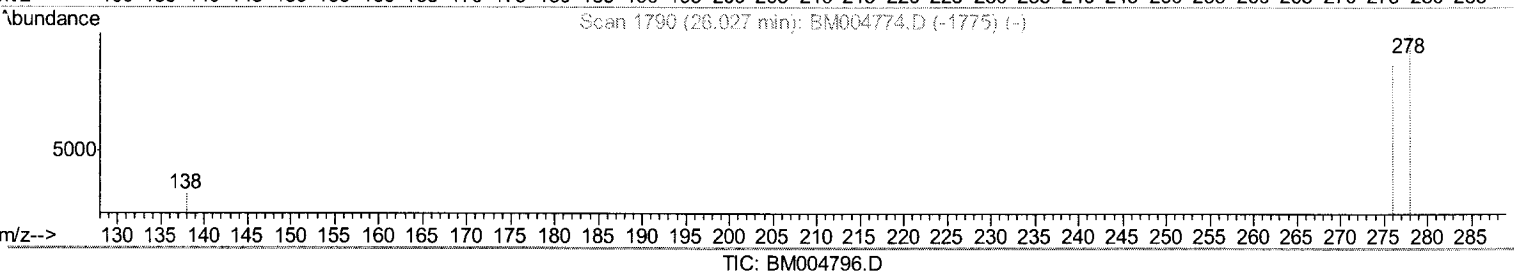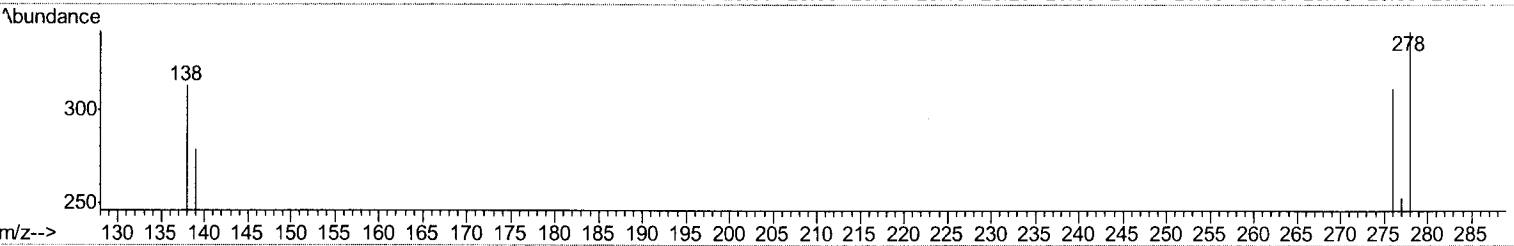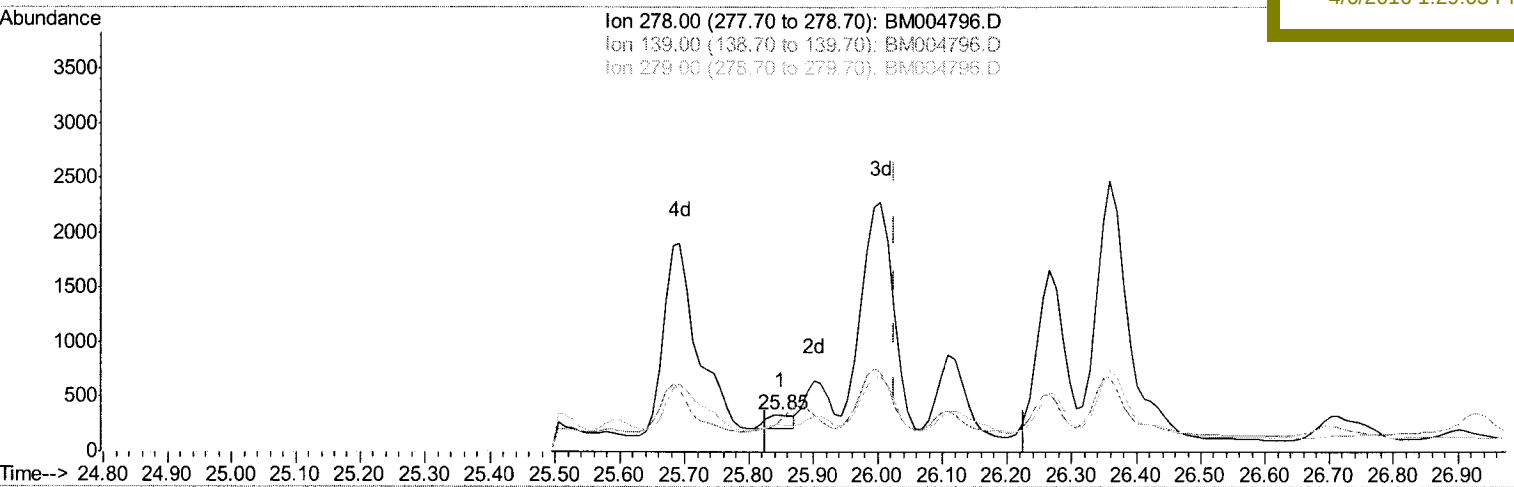

(27) Dibenzo(a,h)anthracene

25.849min (-0.178) 0.02ng/ul

response 380

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	81.58#
279.00	25.20	71.93#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

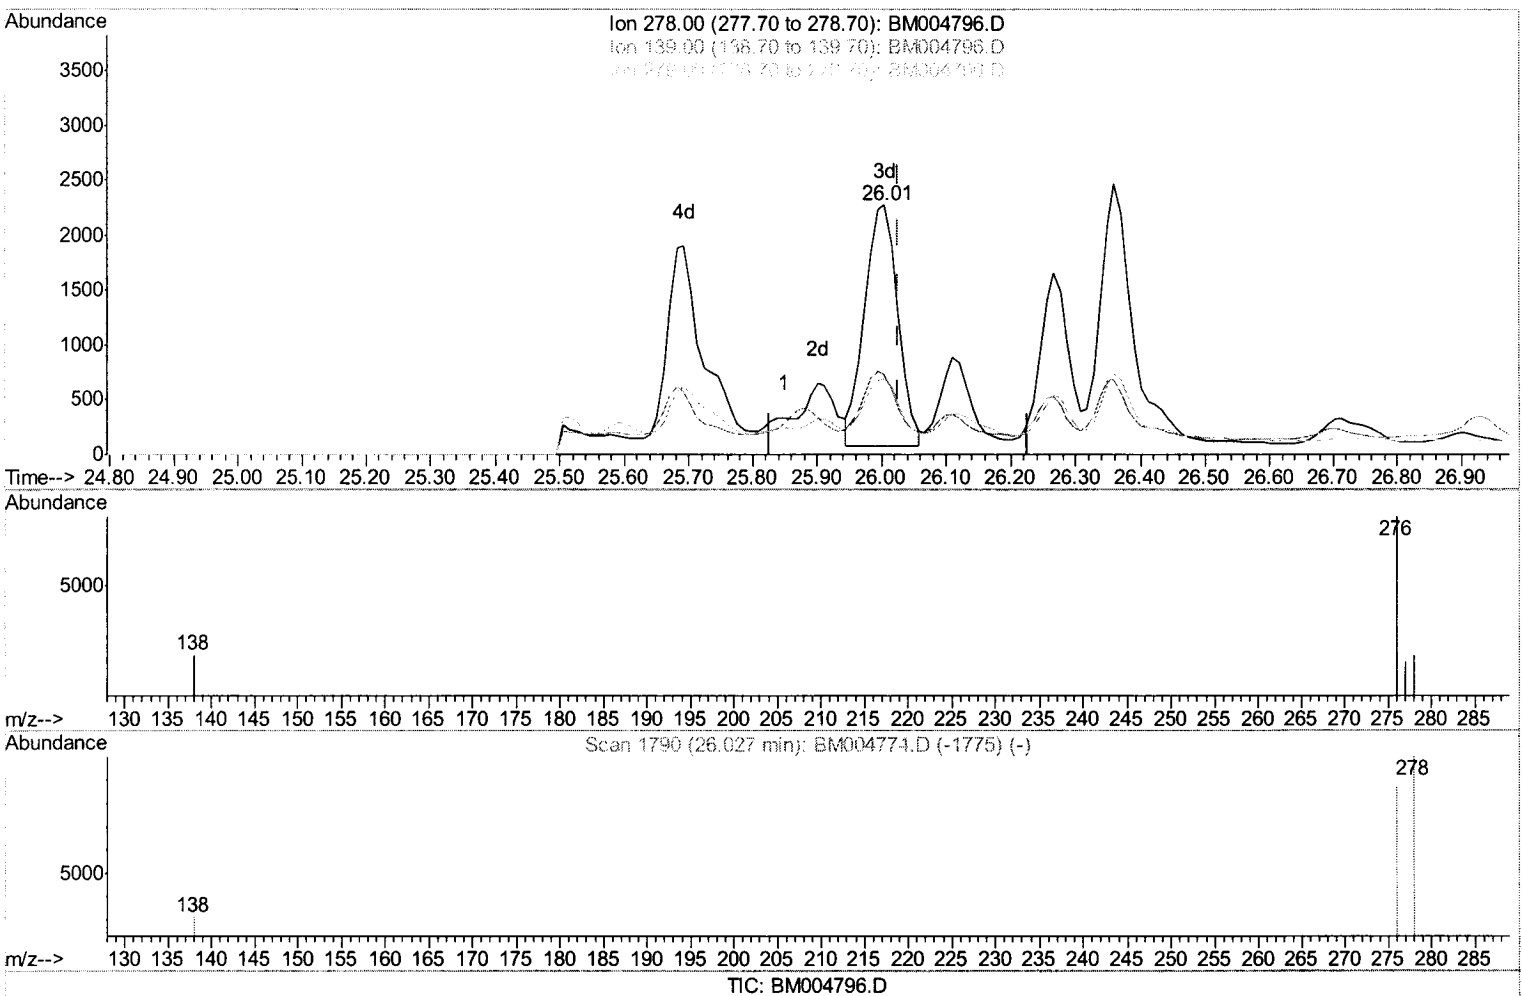

(27) Dibenzo(a,h)anthracene

26.005min (-0.021) 0.45ng/ul m U.M

response 7930

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	31.96#
279.00	25.20	30.51#
0.00	0.00	0.00

04/07/16


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
Data File : BM004796.D
Acq On : 26 Mar 2016 02:58
Operator : UM/SJ
Sample : H1909-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T47

Manual Integrations
APPROVED

Sohil
4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

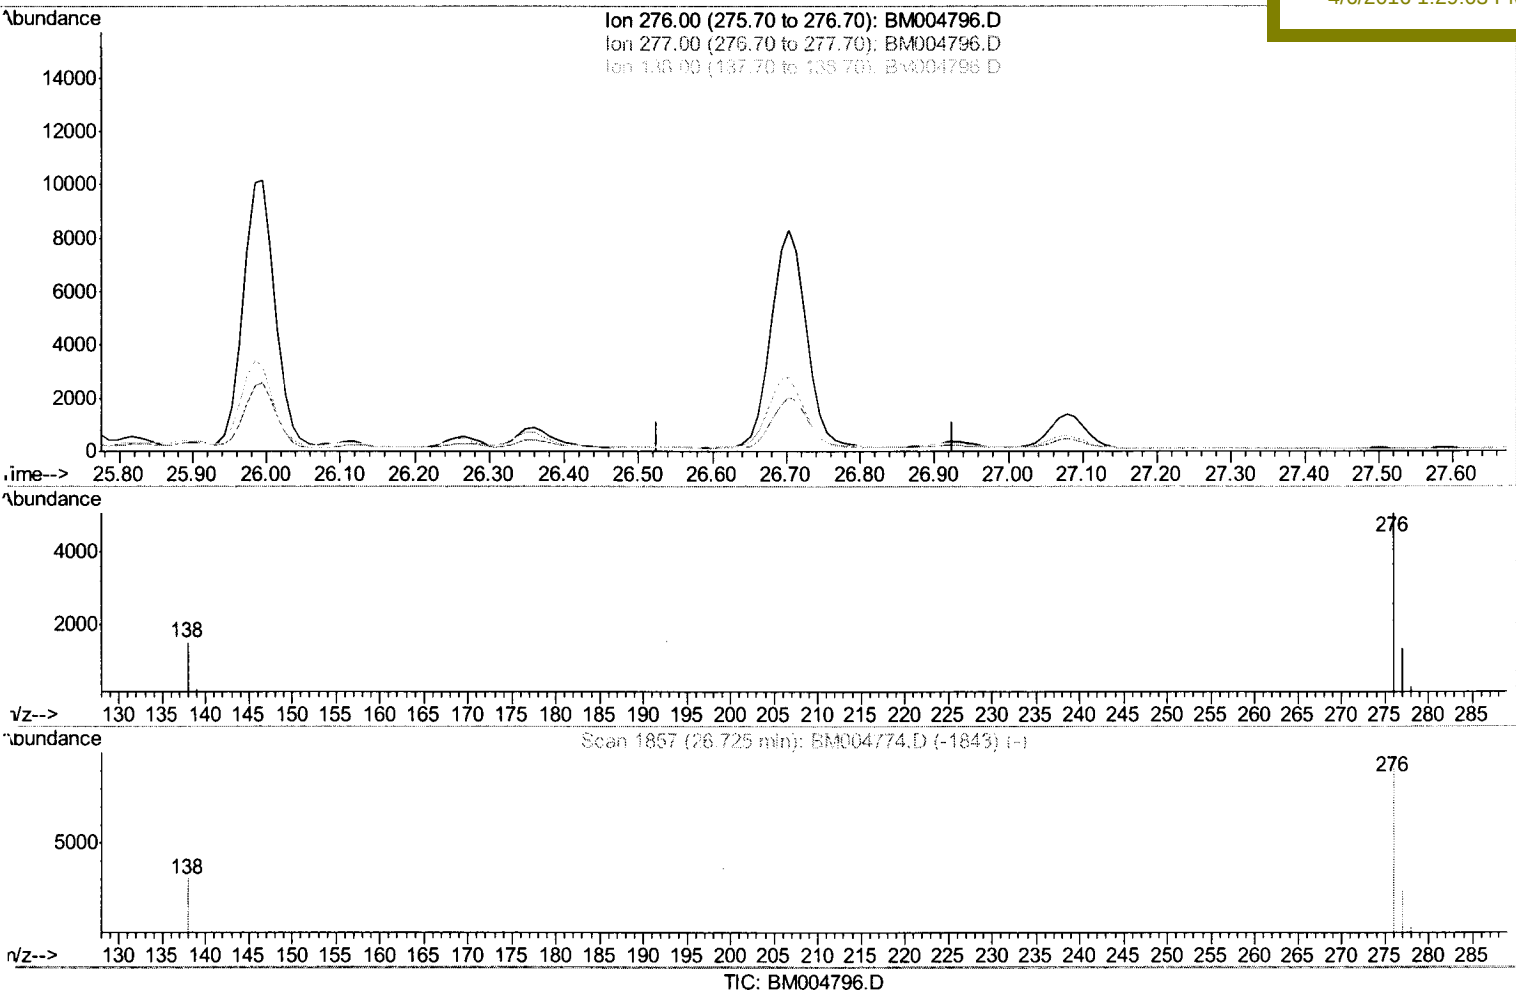

(28) Benzo(g,h,i)perylene

26.725min (-26.725) 0.00ng/ui

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	23.60	0.00#
138.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Quant Time: Apr 05 19:46:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

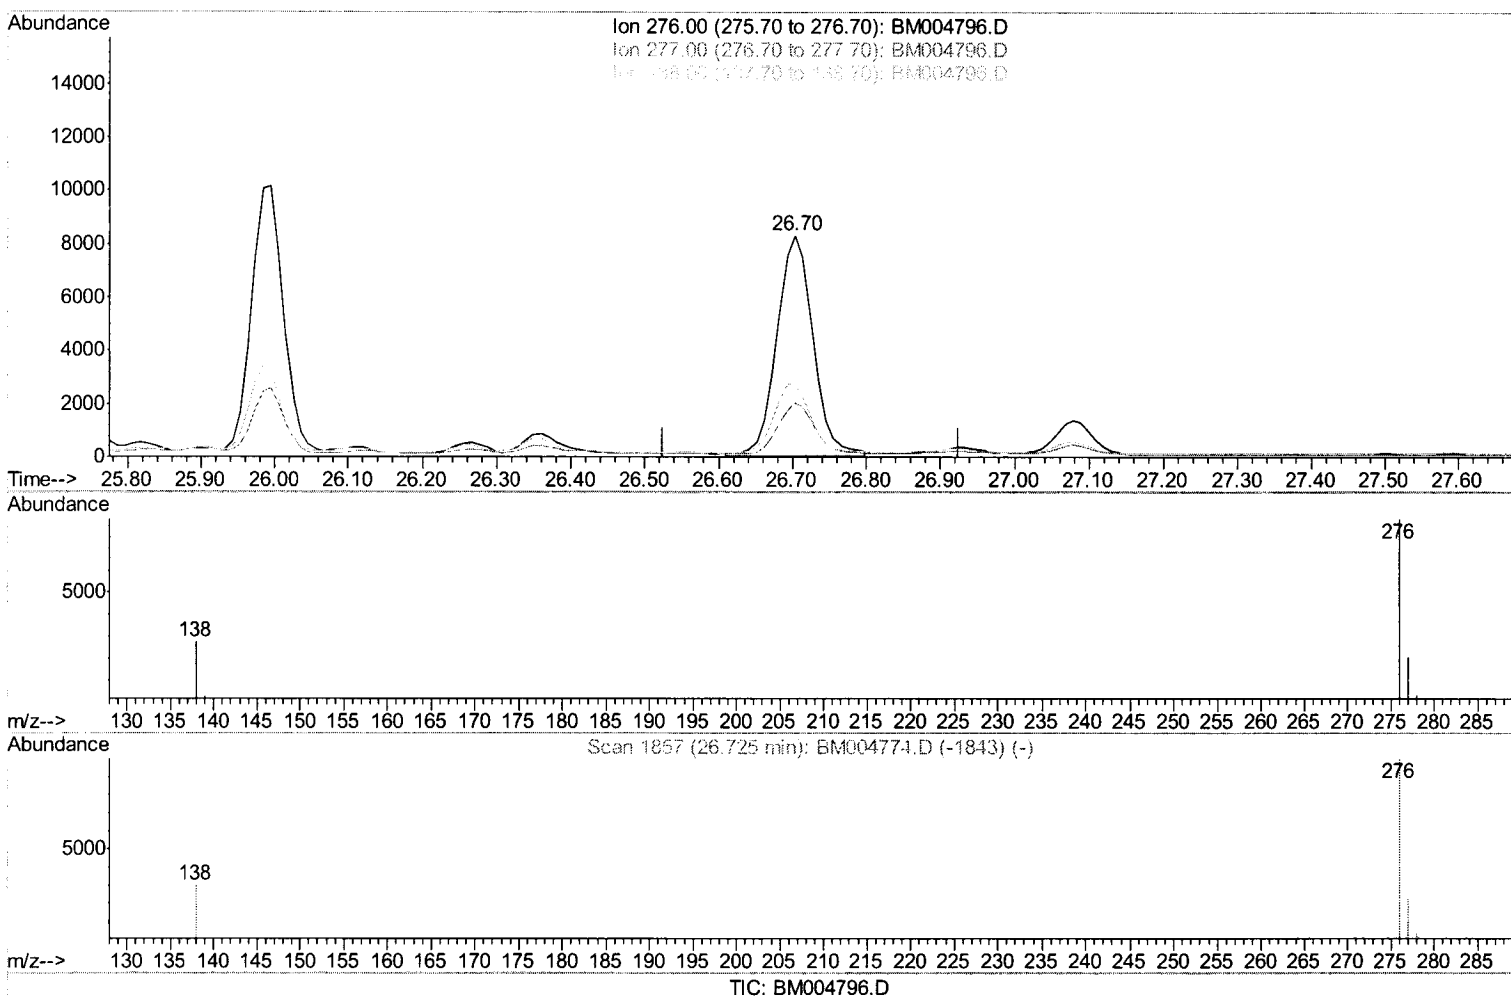

(28) Benzo(g,h,i)perylene

26.704min (-0.021) 1.50ng/ul m U.M
24/07/16

response 27912

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	24.35
138.00	28.10	33.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032516\
 Data File : BM004796.D
 Acq On : 26 Mar 2016 02:58
 Operator : UM/SJ
 Sample : H1909-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T47

Quant Time: Apr 11 11:51:53 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 1:29:03 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1389	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	6680	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.47	164	4117	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.21	188	9126m	0.40	ng/ul	0.00
18) Chrysene-d12	21.39	240	9183	0.40	ng/ul	-0.01
22) Perylene-d12	23.68	264	7899m	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.32	96	4705	7.52	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.20	152	2380	0.26	ng/ul	0.00
16) Fluoranthene-d10	19.23	212	5757	0.27	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Naphthalene	10.67	128	15579	0.97	ng/ul	98
7) 2-Methylnaphthalene	12.28	142	13018	1.13	ng/ul	100
9) Acenaphthylene	14.18	152	9153	0.48	ng/ul#	93
10) Acenaphthene	14.52	153	8294	0.62	ng/ul	92
11) Fluorene	15.51	166	17298	1.08	ng/ul	94
14) Phenanthrene	17.24	178	298392	11.64	ng/ul	96
15) Anthracene	17.33	178	6985	0.29	ng/ul	95
17) Fluoranthene	19.27	202	187039m	6.41	ng/ul	96
19) Pyrene	19.63	202	289641	9.21	ng/ul	96
20) Benzo(a)anthracene	21.37	228	50233	1.78	ng/ul#	93
21) Chrysene	21.42	228	93795	3.44	ng/ul	93
23) Benzo(b)fluoranthene	22.98	252	91072m	3.42	ng/ul	
24) Benzo(k)fluoranthene	23.02	252	29890m	1.21	ng/ul	
25) Benzo(a)pyrene	23.58	252	63312m	2.60	ng/ul	
26) Indeno(1,2,3-cd)pyrene	25.99	276	31296m	1.39	ng/ul	
27) Dibenzo(a,h)anthracene	26.01	278	7930m	0.45	ng/ul	
28) Benzo(g,h,i)perylene	26.70	276	27912m	1.50	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.m.
 04/07/2016

U.m.
 04/07/2016

U.m.
 04/07/2016