
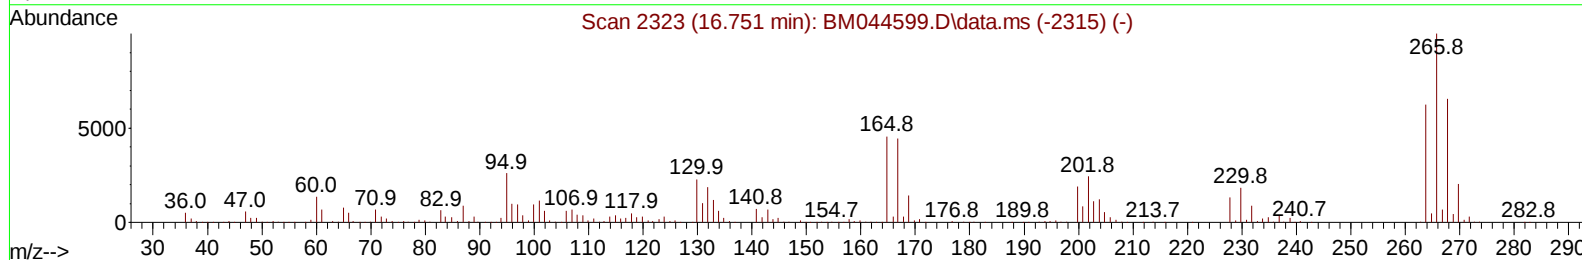
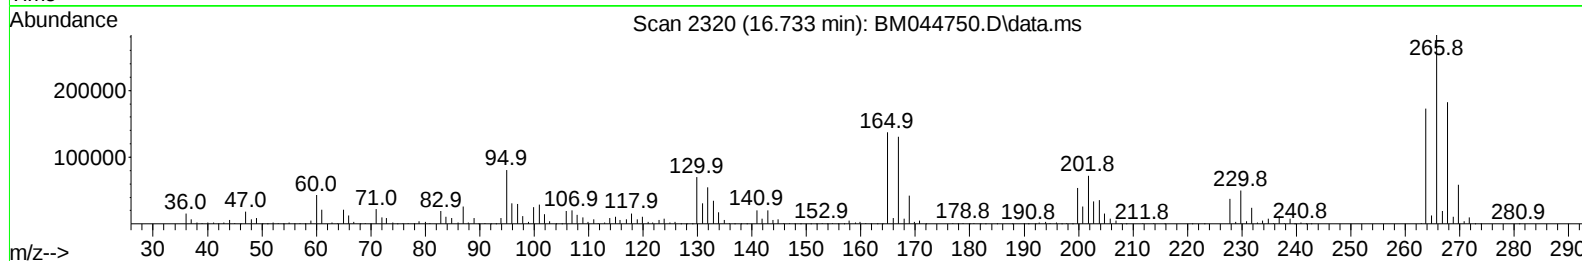


Quant Time: Mar 25 11:42:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

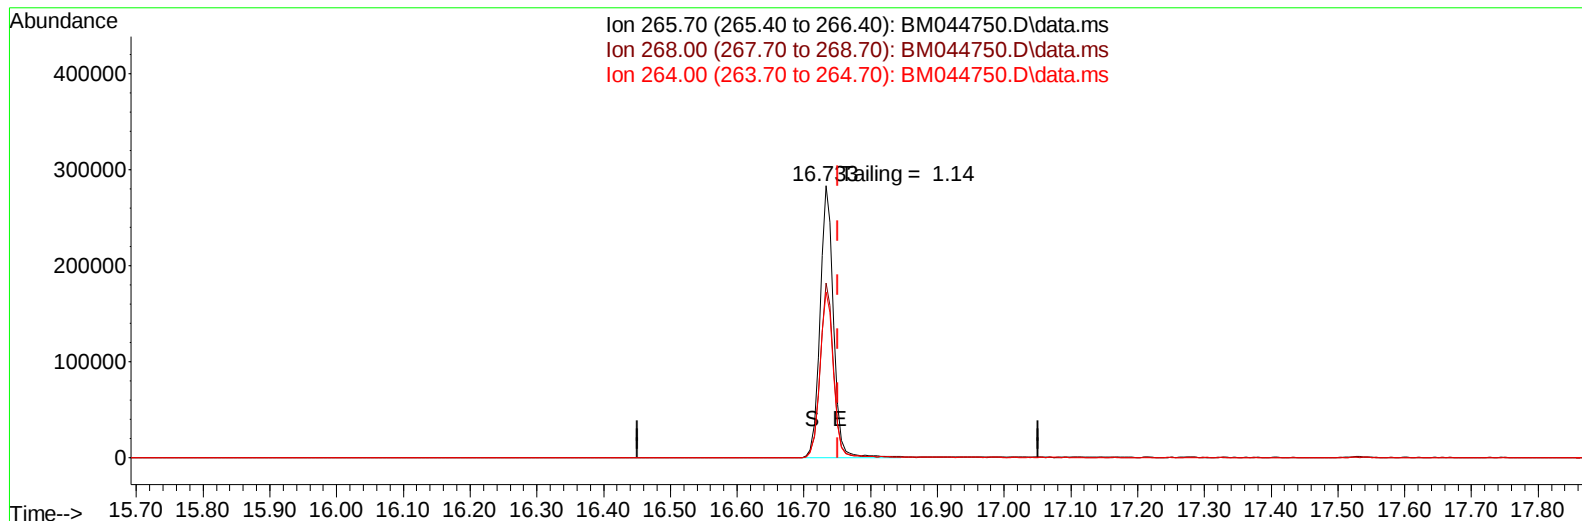

TIC: BM044750.D\data.ms




16.733min (-0.018) 842135.21 ng

response **399626**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.29
264.00	62.30	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044750.D
Acq On : 25 Mar 2024 09:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 11:42:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

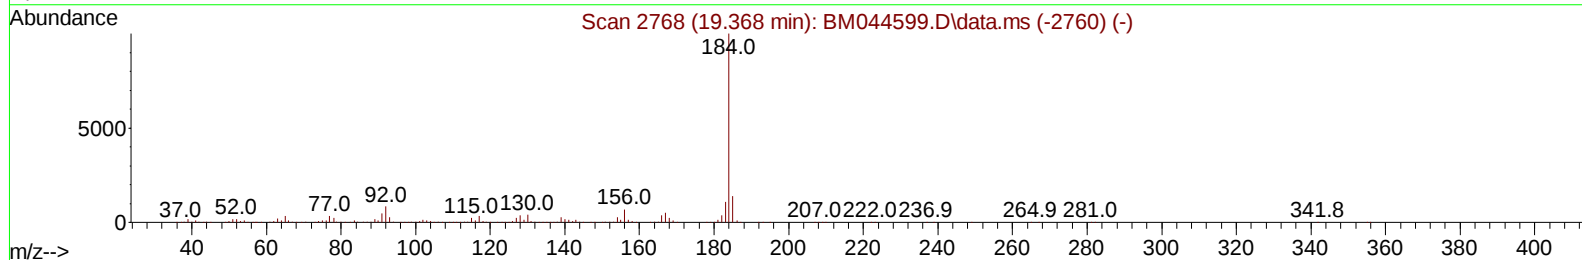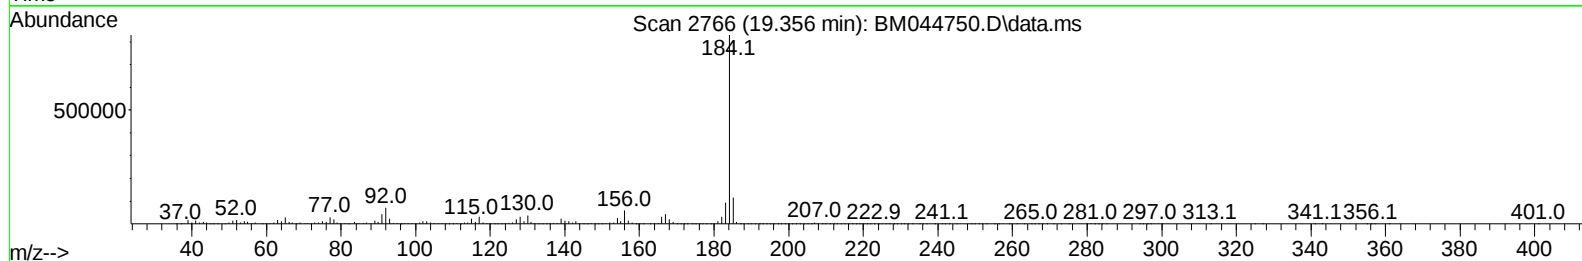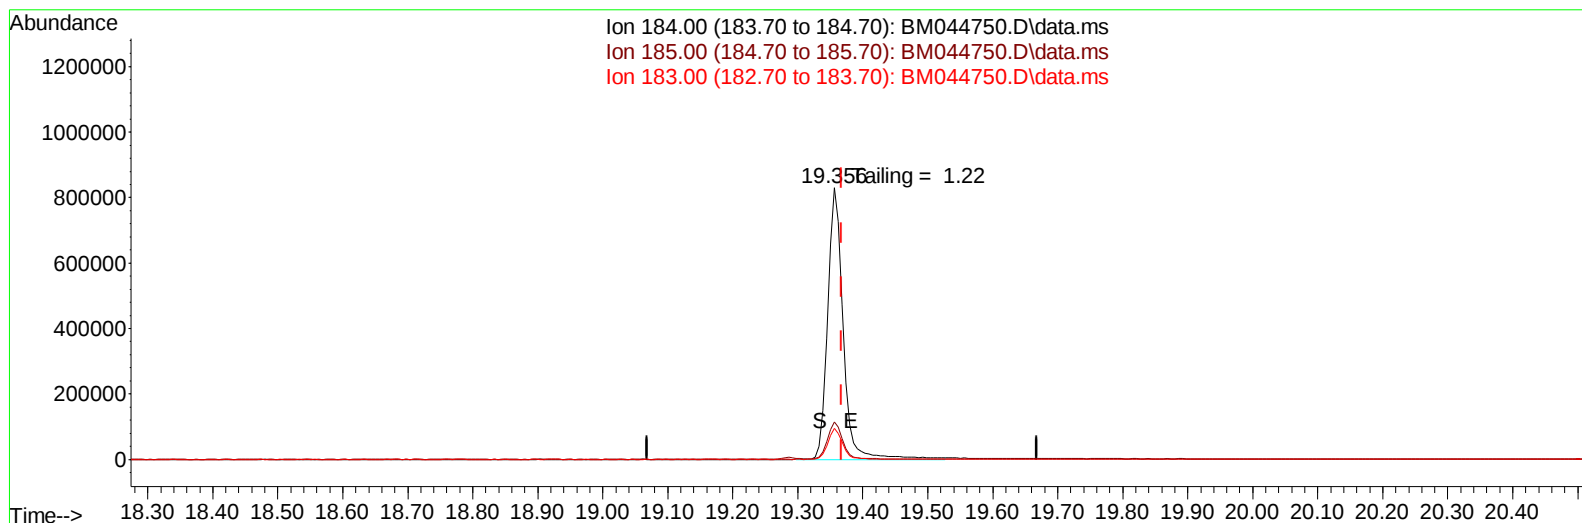

TIC: BM044750.D\data.ms

(77) Benzidine**19.356min (-0.012) 213669.98 ng****response 1369542**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.89
183.00	10.90	11.37
0.00	0.00	0.00