

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
 Data File : BM044761.D
 Acq On : 25 Mar 2024 18:24
 Operator : MA/JU
 Sample : P1847-01DL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SU-02-032224DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.311	371	378	385	rBV	188635	291844	1.19%	0.277%
2	7.699	779	784	797	rVB	664633	1085902	4.43%	1.032%
3	8.899	985	988	997	rVB	185080	272817	1.11%	0.259%
4	10.440	1244	1250	1252	rBV	248325	399138	1.63%	0.379%
5	10.475	1252	1256	1261	rVV	744594	1264833	5.16%	1.203%
6	10.528	1261	1265	1271	rVB	143735	248721	1.01%	0.236%
7	11.898	1488	1498	1504	rBV	296437	537789	2.19%	0.511%
8	12.957	1673	1678	1685	rBV	206687	302999	1.24%	0.288%
9	13.157	1707	1712	1719	rVB2	392228	589894	2.41%	0.561%
10	13.816	1817	1824	1828	rBV2	141338	289411	1.18%	0.275%
11	14.239	1891	1896	1902	rBV	472105	648582	2.64%	0.617%
12	14.339	1904	1913	1919	rVV	896574	1507593	6.15%	1.433%
13	14.404	1919	1924	1932	rVV	278132	433464	1.77%	0.412%
14	14.745	1978	1982	1987	rVB	235027	323592	1.32%	0.308%
15	15.198	2055	2059	2065	rVB	464697	590003	2.41%	0.561%
16	15.398	2087	2093	2097	rBV	356849	574893	2.34%	0.547%
17	15.604	2124	2128	2133	rVB	160464	247532	1.01%	0.235%
18	15.839	2161	2168	2175	rBV5	209222	429410	1.75%	0.408%
19	16.069	2202	2207	2215	rBV	557275	962789	3.93%	0.915%
20	16.863	2338	2342	2346	rVV	431101	503902	2.05%	0.479%
21	16.916	2346	2351	2360	rVB2	331396	584628	2.38%	0.556%
22	17.098	2377	2382	2385	rBV	958224	1396759	5.70%	1.328%
23	17.139	2385	2389	2396	rVV	2249018	3336888	13.61%	3.173%
24	17.233	2400	2405	2410	rVB	832230	1181559	4.82%	1.123%
25	17.510	2448	2452	2462	rBV	172993	311469	1.27%	0.296%
26	17.604	2464	2468	2474	rBV2	387962	542709	2.21%	0.516%
27	17.674	2478	2480	2489	rVB2	166300	268131	1.09%	0.255%
28	17.786	2493	2499	2503	rBV	4689241	5978933	24.38%	5.685%
29	17.974	2527	2531	2534	rBV	359243	538792	2.20%	0.512%
30	18.021	2534	2539	2546	rVB2	619597	1318133	5.38%	1.253%
31	18.104	2549	2553	2558	rVV	274418	421398	1.72%	0.401%
32	18.169	2559	2564	2568	rVV2	760386	1392533	5.68%	1.324%
33	18.204	2568	2570	2577	rVB	310104	420116	1.71%	0.399%
34	18.298	2582	2586	2590	rBV	395124	556061	2.27%	0.529%
35	18.480	2613	2617	2621	rBV2	276565	399205	1.63%	0.380%
36	18.533	2623	2626	2634	rVB3	219145	321754	1.31%	0.306%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044761.D
Acq On : 25 Mar 2024 18:24
Operator : MA/JU
Sample : P1847-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SU-02-032224DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.780	2664	2668	2671	rBV	223427	270507	1.10%	0.257%
38	18.816	2671	2674	2680	rVB2	207287	278523	1.14%	0.265%
39	18.898	2684	2688	2690	rBV	509674	734209	2.99%	0.698%
40	18.939	2690	2695	2698	rVV	15481314	24521797	100.00%	23.314%
41	18.974	2698	2701	2709	rVB3	11134206	15907415	64.87%	15.124%
42	19.045	2709	2713	2718	rBV4	207591	380031	1.55%	0.361%
43	19.098	2718	2722	2727	rVB	2328707	2704600	11.03%	2.571%
44	19.168	2727	2734	2741	rBV	4008804	6532567	26.64%	6.211%
45	19.533	2786	2796	2804	rBV	3749863	6442644	26.27%	6.125%
46	19.610	2805	2809	2815	rVB3	287655	469745	1.92%	0.447%
47	19.857	2848	2851	2858	rVB3	293064	614883	2.51%	0.585%
48	19.998	2872	2875	2877	rBV3	191699	284973	1.16%	0.271%
49	20.027	2877	2880	2884	rVB2	559346	714723	2.91%	0.680%
50	20.127	2894	2897	2901	rVB	592128	690900	2.82%	0.657%
51	20.186	2904	2907	2913	rVB2	515364	840951	3.43%	0.800%
52	20.327	2927	2931	2935	rBV	506763	631514	2.58%	0.600%
53	20.374	2935	2939	2942	rVV	451773	586141	2.39%	0.557%
54	20.945	3033	3036	3039	rBV	360747	419025	1.71%	0.398%
55	21.286	3089	3094	3099	rBV2	2348690	4513913	18.41%	4.292%
56	21.333	3099	3102	3110	rVB	1680571	2320261	9.46%	2.206%
57	22.874	3360	3364	3369	rBV	1074195	2225612	9.08%	2.116%
58	23.451	3457	3462	3469	rVB	1435854	2619452	10.68%	2.490%


Sum of corrected areas: 105178562

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044761.D
Acq On : 25 Mar 2024 18:24
Operator : MA/JU
Sample : P1847-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SU-02-032224DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

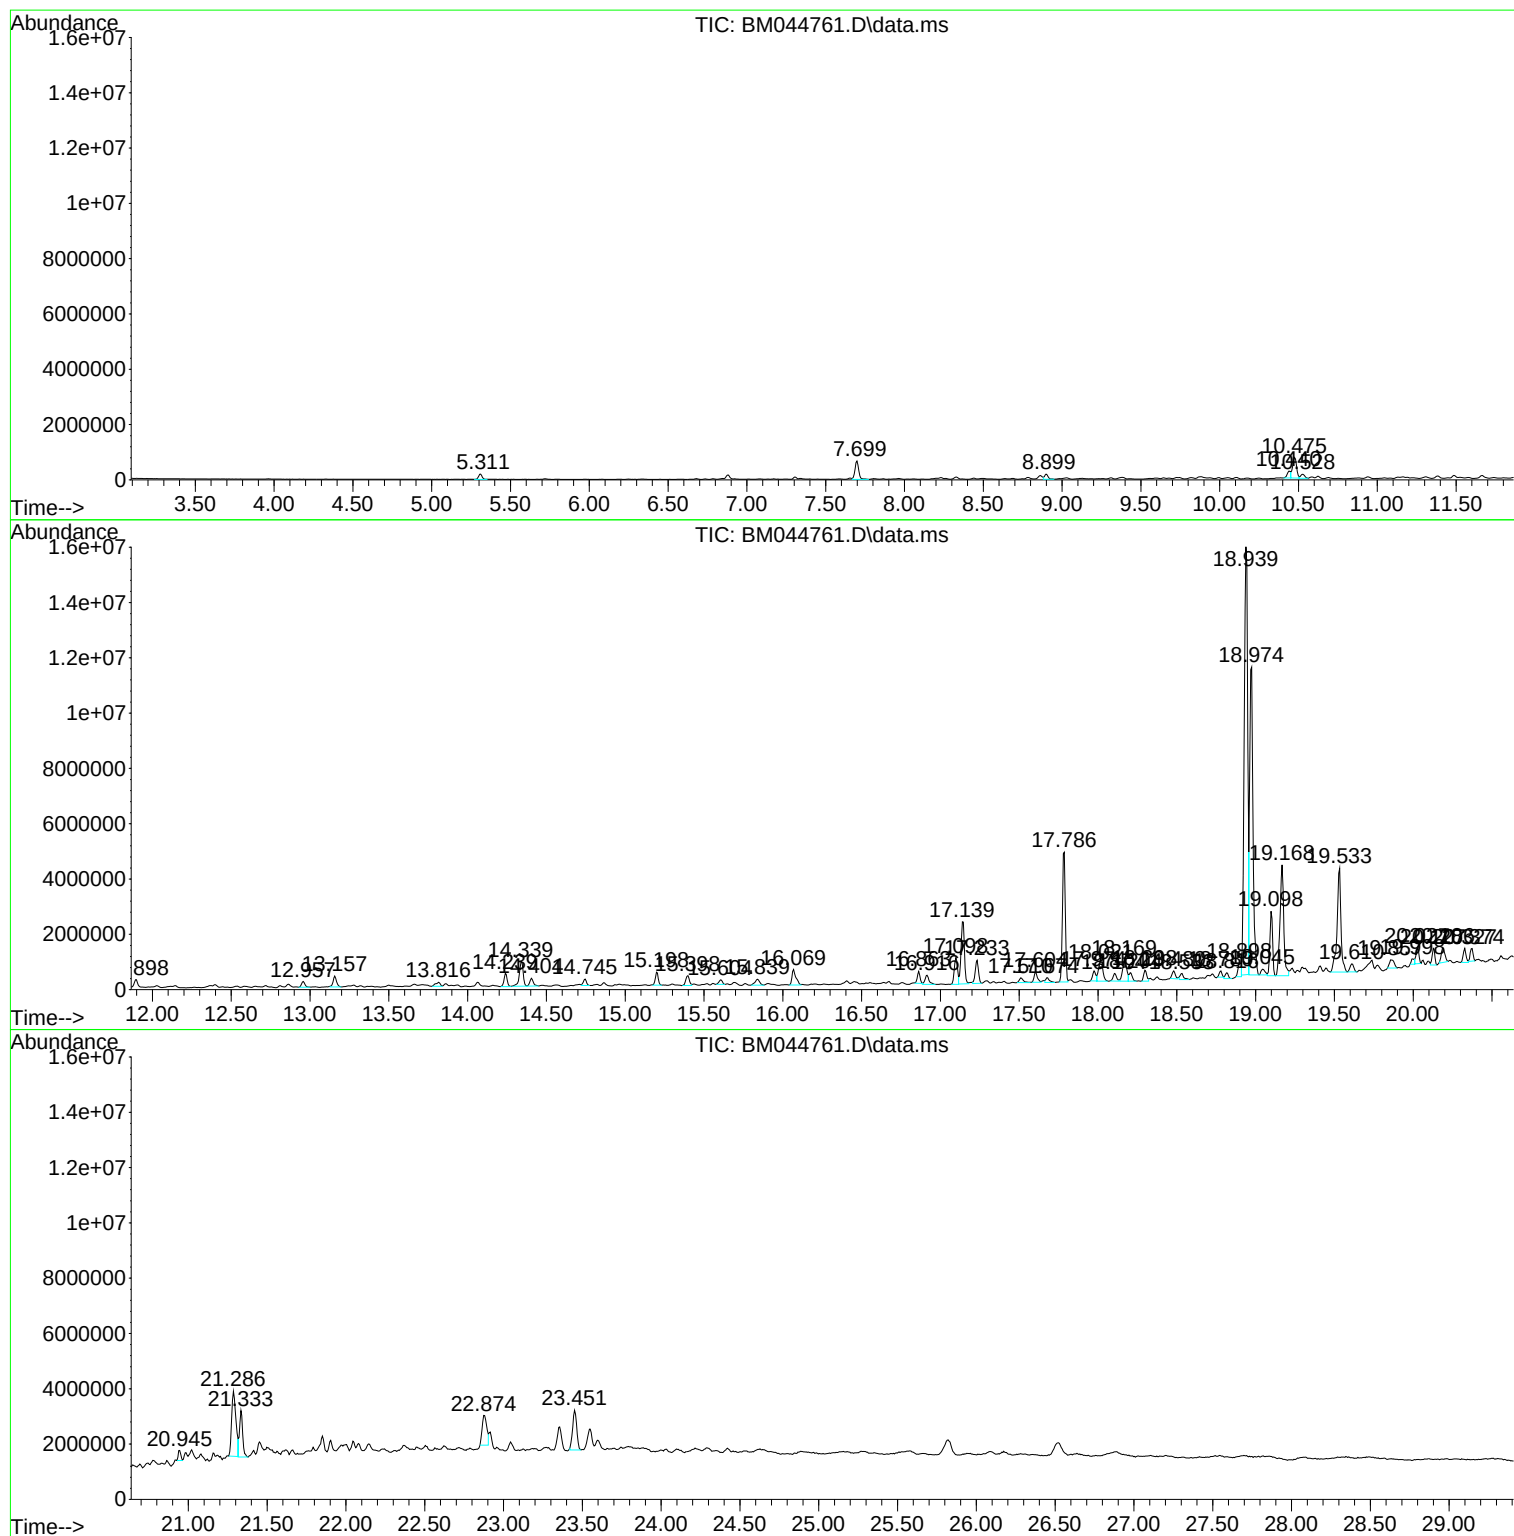

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044761.D
Acq On : 25 Mar 2024 18:24
Operator : MA/JU
Sample : P1847-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SU-02-032224DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044761.D
Acq On : 25 Mar 2024 18:24
Operator : MA/JU
Sample : P1847-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SU-02-032224DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------