


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044750.D
Acq On : 25 Mar 2024 09:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 02:28:24 2024

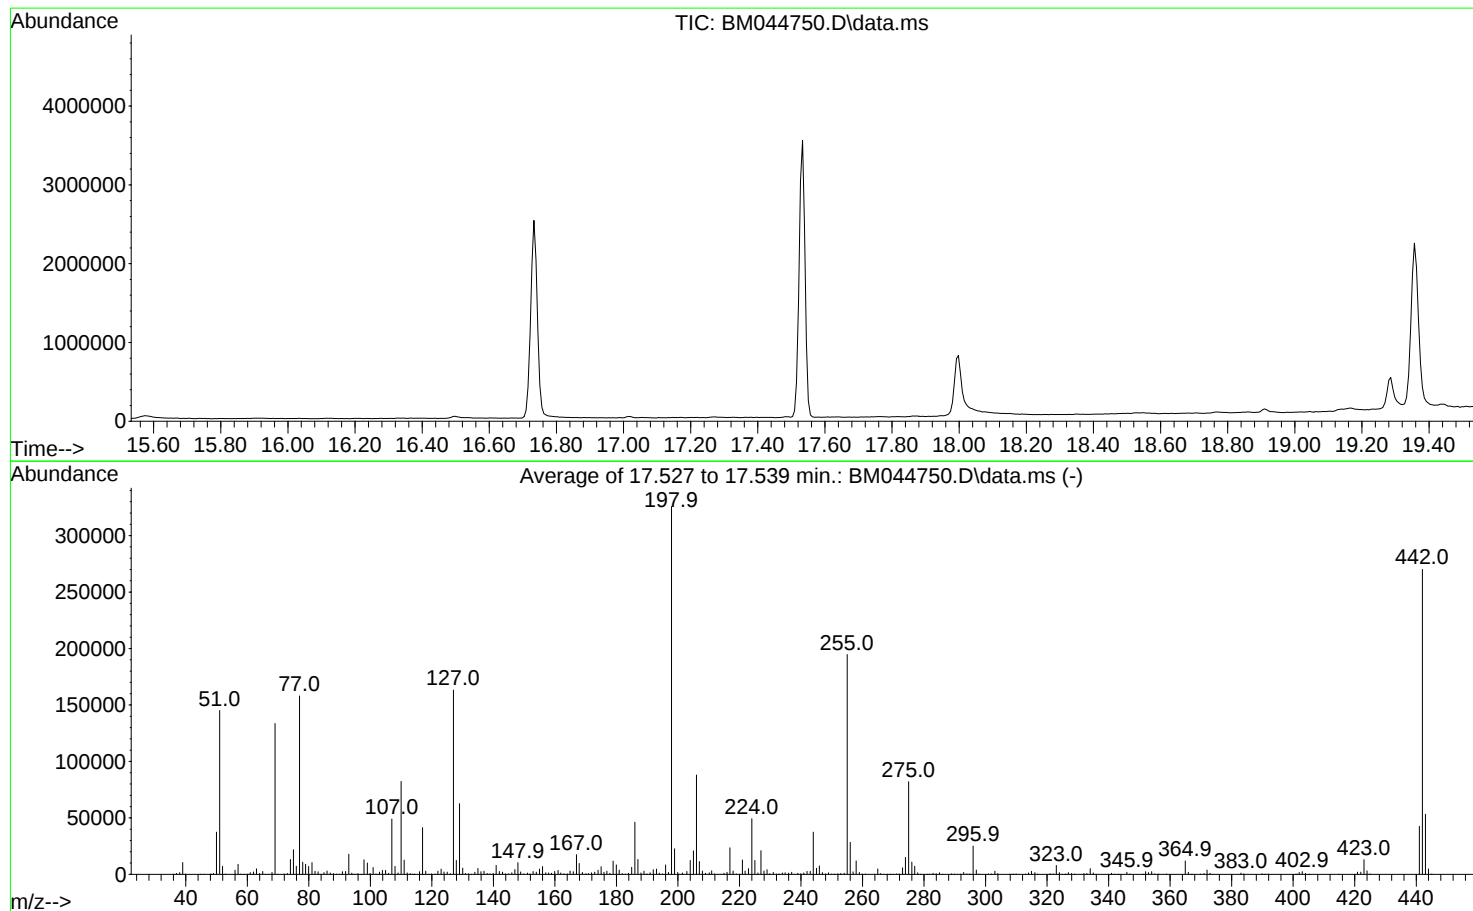




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	145125	PASS
68	69	0.00	2	1.3	1723	PASS
69	198	0.00	100	41.0	133595	PASS
70	69	0.00	2	0.1	105	PASS
127	198	10	80	50.1	163253	PASS
197	198	0.00	2	0.5	1732	PASS
198	198	100	100	100.0	325781	PASS
199	198	5	9	7.0	22651	PASS
275	198	10	60	25.2	82112	PASS
365	198	1	100	3.7	11944	PASS
441	198	0.01	100	13.0	42477	PASS
442	442	50	100	100.0	270101	PASS
443	442	15	24	19.7	53232	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044750.D
Acq On : 25 Mar 2024 09:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 25 11:42:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

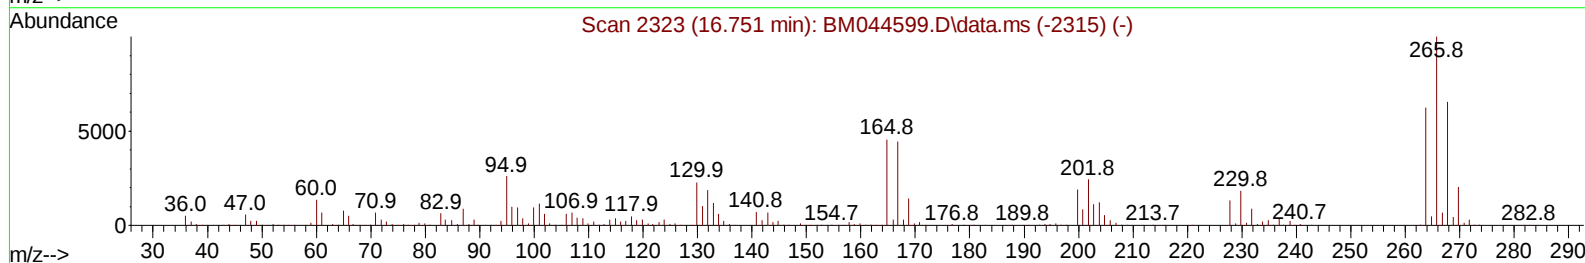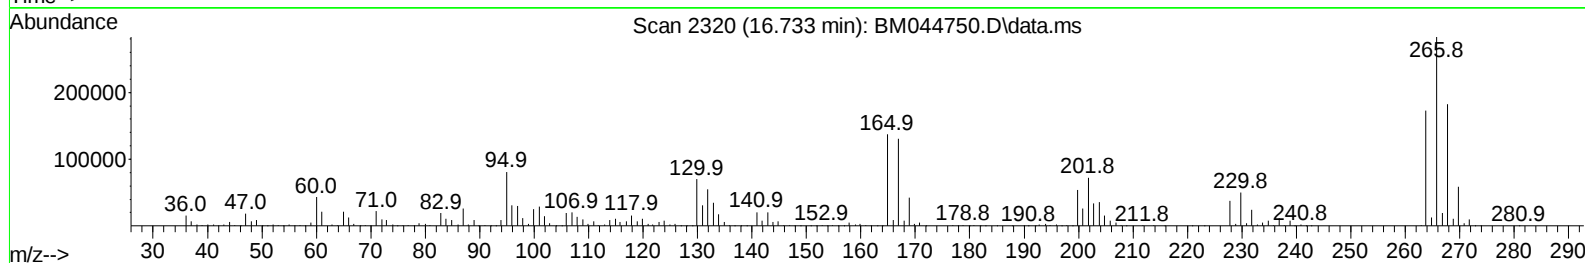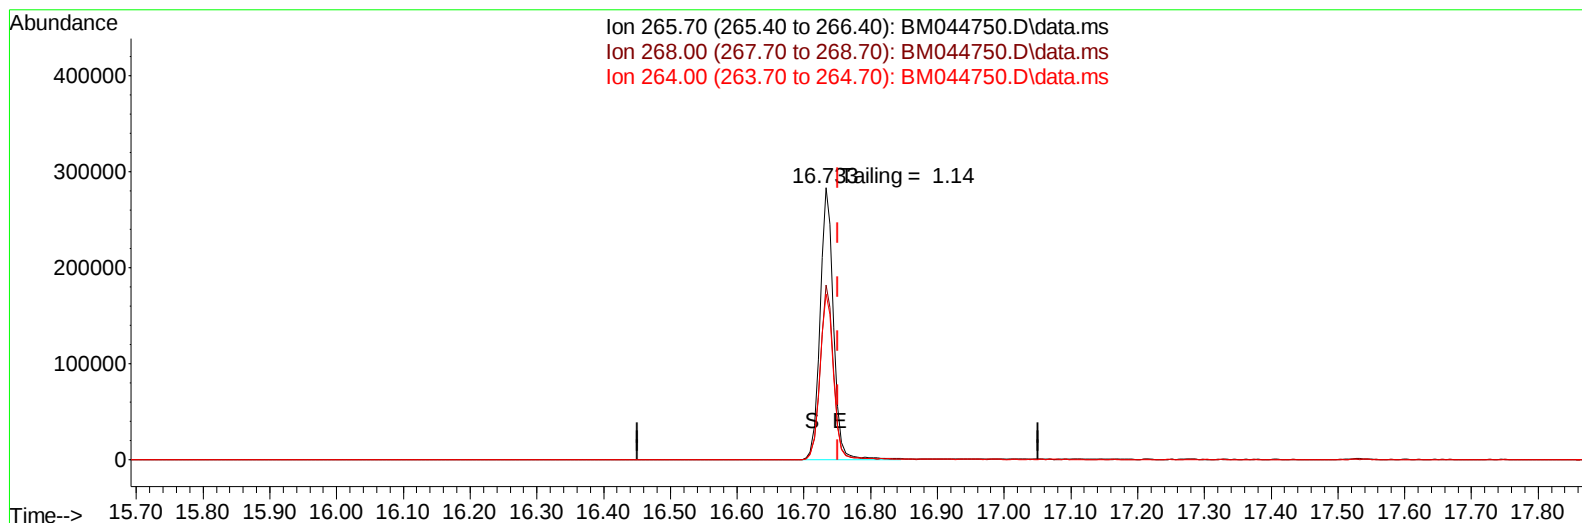

TIC: BM044750.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.018) 842135.21 ng




response 399626

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.29
264.00	62.30	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032524\
Data File : BM044750.D
Acq On : 25 Mar 2024 09:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 25 11:42:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

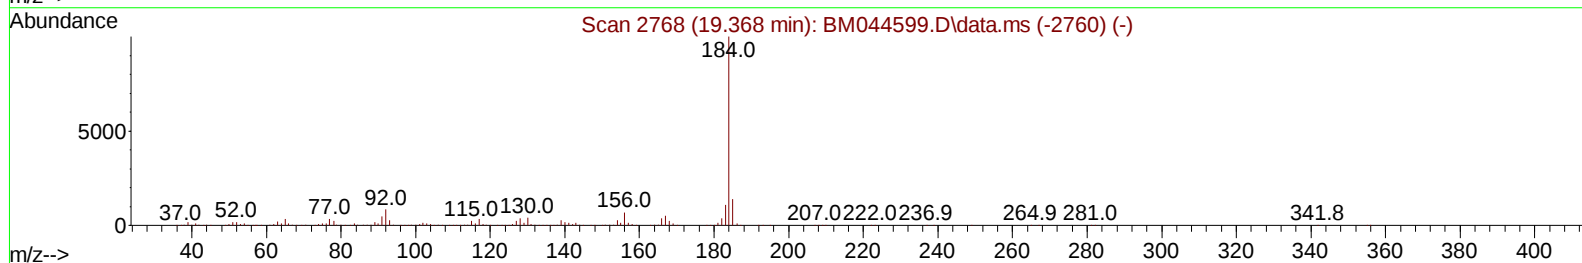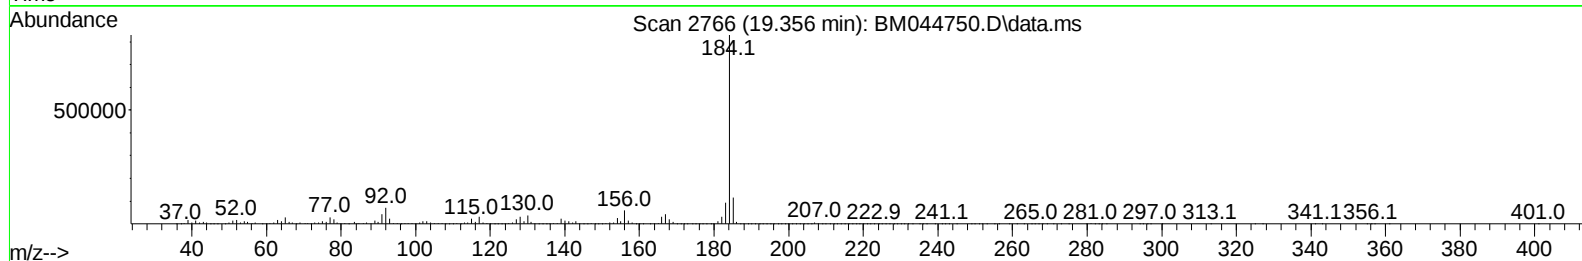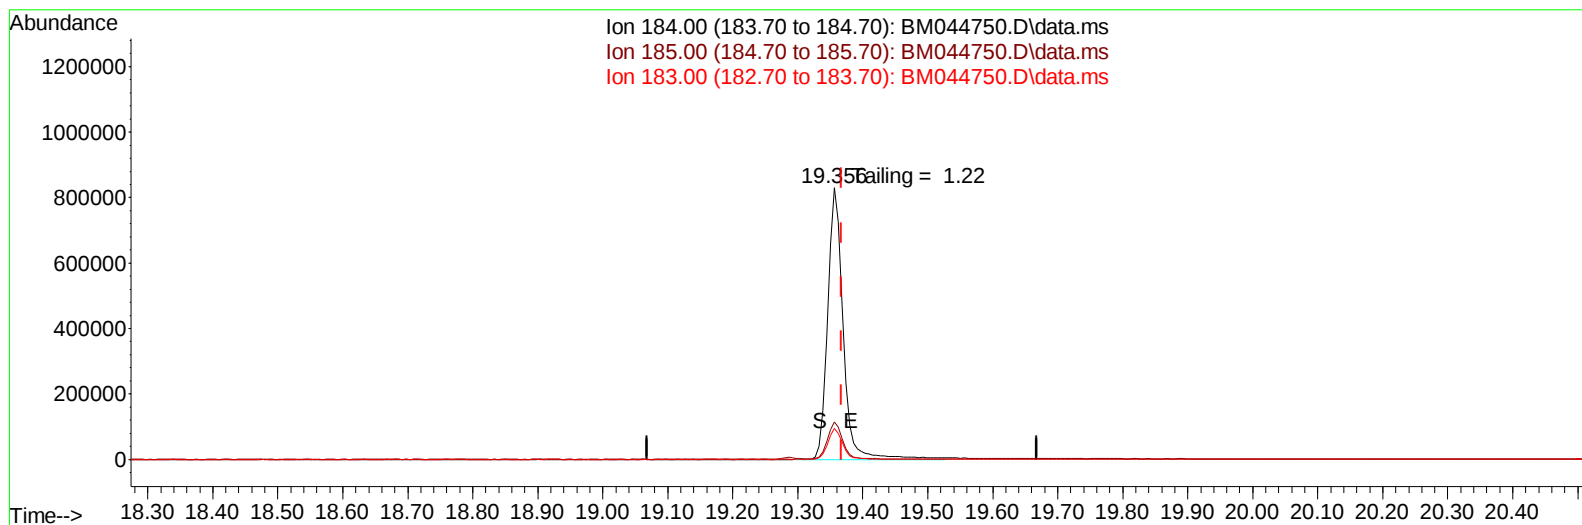

TIC: BM044750.D\data.ms

(77) Benzidine

19.356min (-0.012) 213669.98 ng

response 1369542

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.89
183.00	10.90	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2024	BNA_M	<u>BM044750.D</u>
Compound Name	Response	Retention Time
DDT	1043198	20.586
DDD	57016	20.145
DDE	3131	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
60147	1103345	5.45

Instrument :
BNA_M
ClientSampleId :
DFTPP