
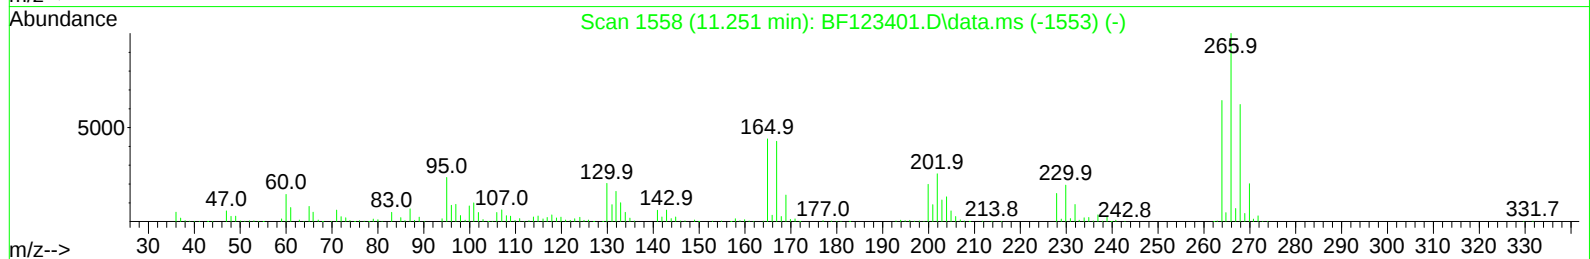
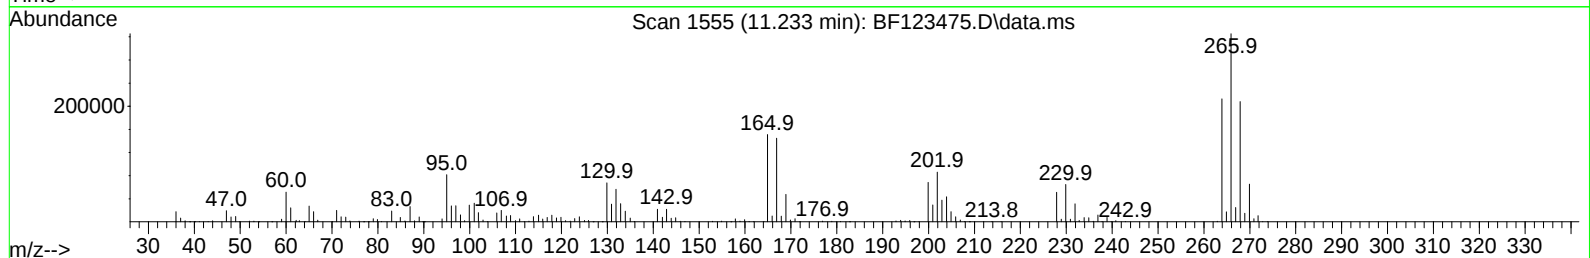


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032621\
Data File : BF123475.D
Acq On : 26 Mar 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 12:47:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 17:06:59 2021
Response via : Initial Calibration

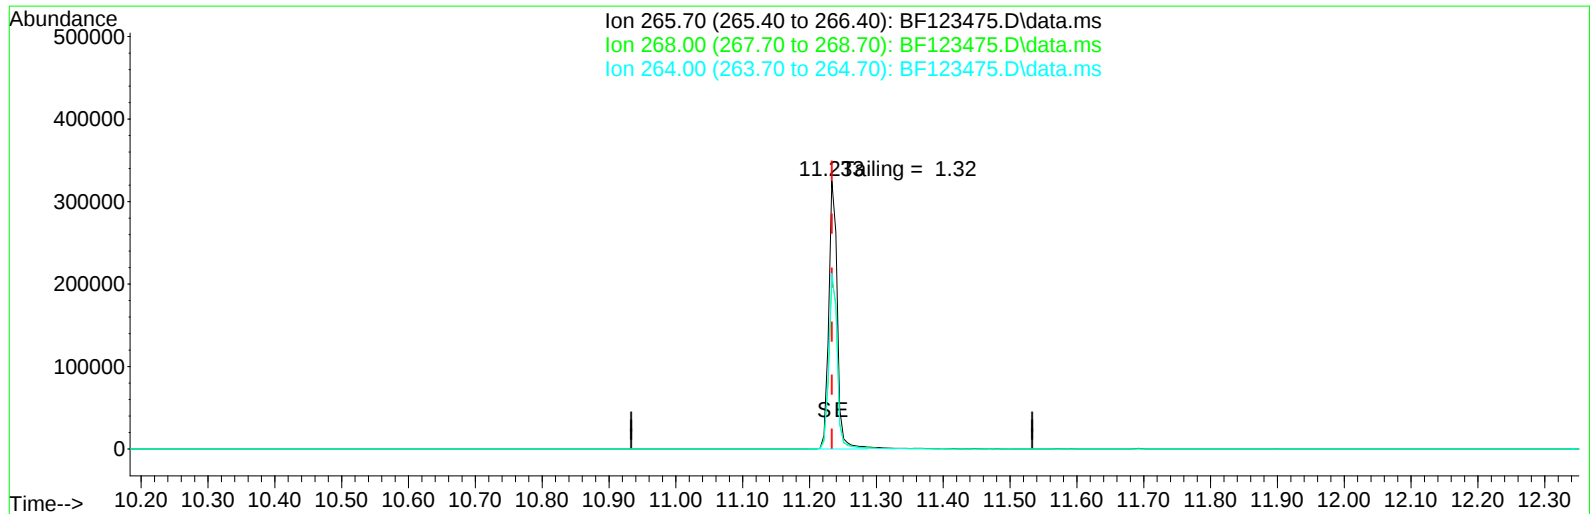

TIC: BF123475.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 36040.21 ng

response 293881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.93
264.00	62.30	65.40
0.00	0.00	0.00