
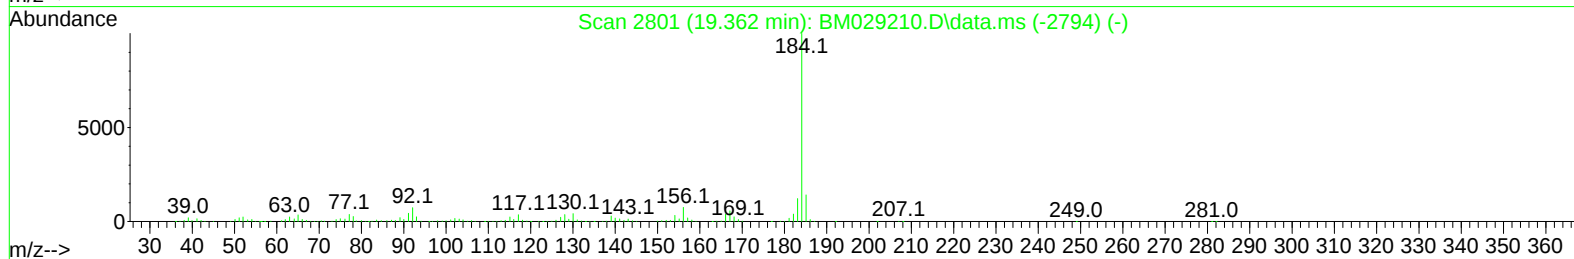
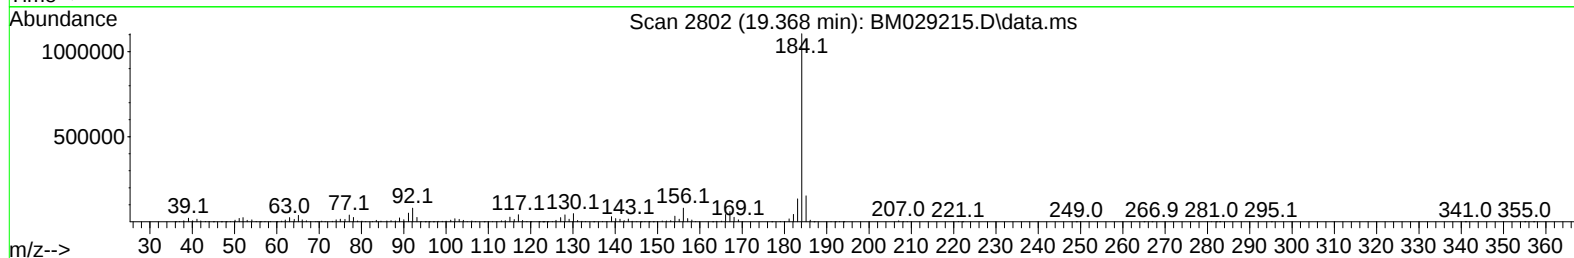


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
Data File : BM029215.D
Acq On : 25 Mar 2021 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 12:54:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 12:50:01 2021
Response via : Initial Calibration

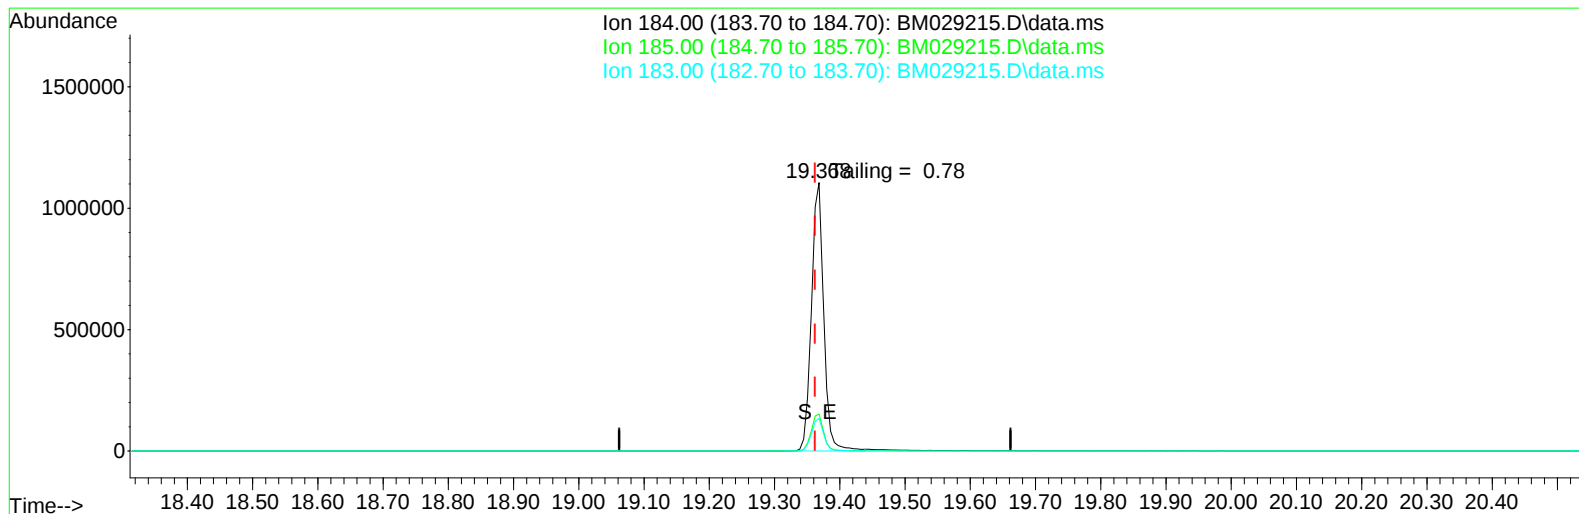

TIC: BM029215.D\data.ms

(77) Benzidine




19.368min (+ 0.006) 0.00 ng

response 1468364

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.79
183.00	12.20	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
Data File : BM029215.D
Acq On : 25 Mar 2021 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 12:54:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 12:50:01 2021
Response via : Initial Calibration

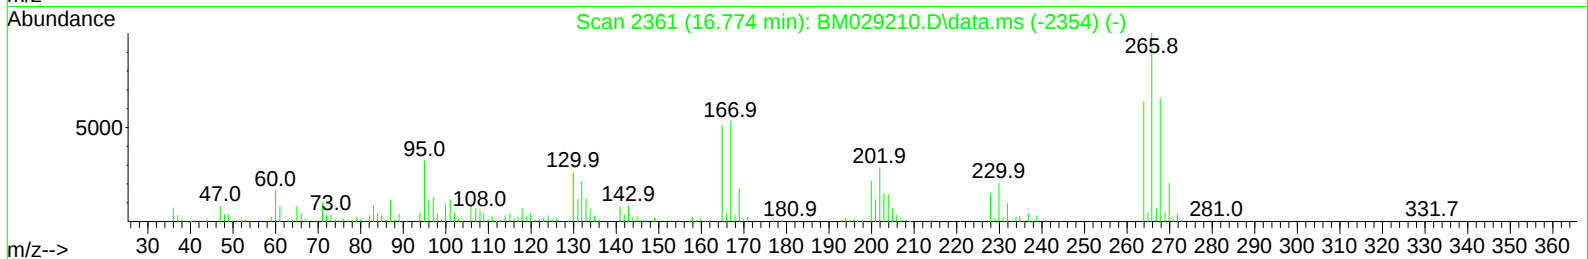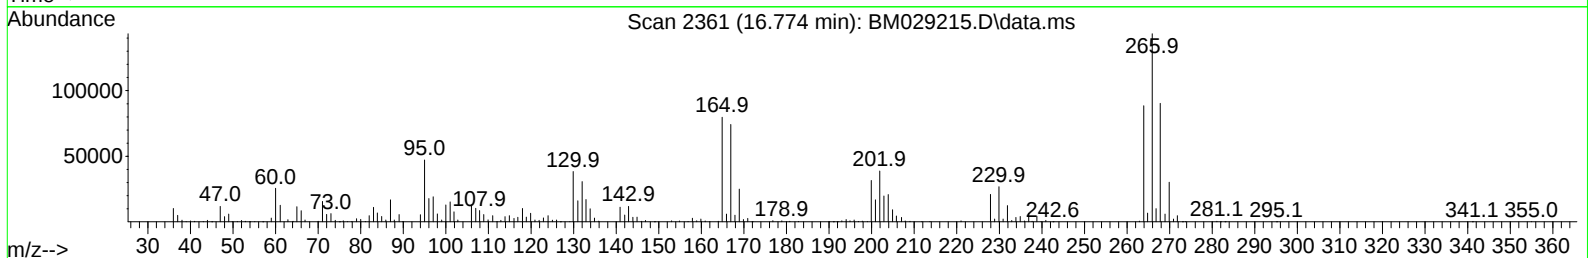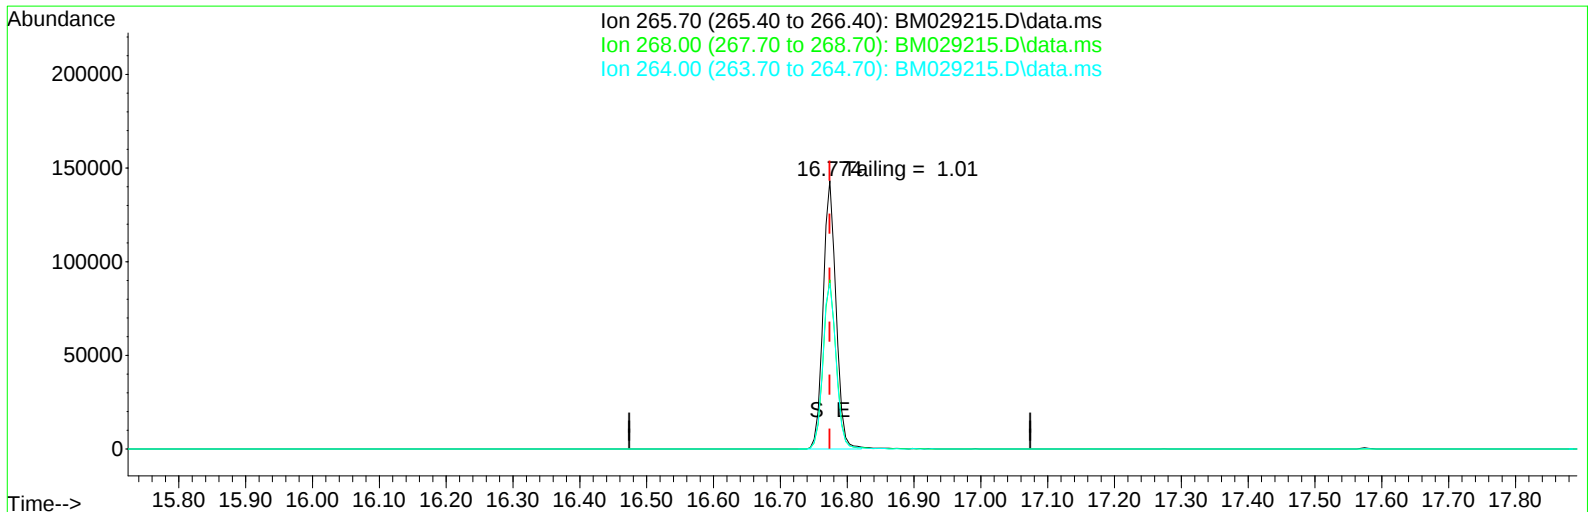

TIC: BM029215.D\data.ms

(70) Pentachlorophenol (C)

16.774min (+ 0.000) 0.00 ng

response 193434

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	63.01
264.00	63.60	61.76
0.00	0.00	0.00