
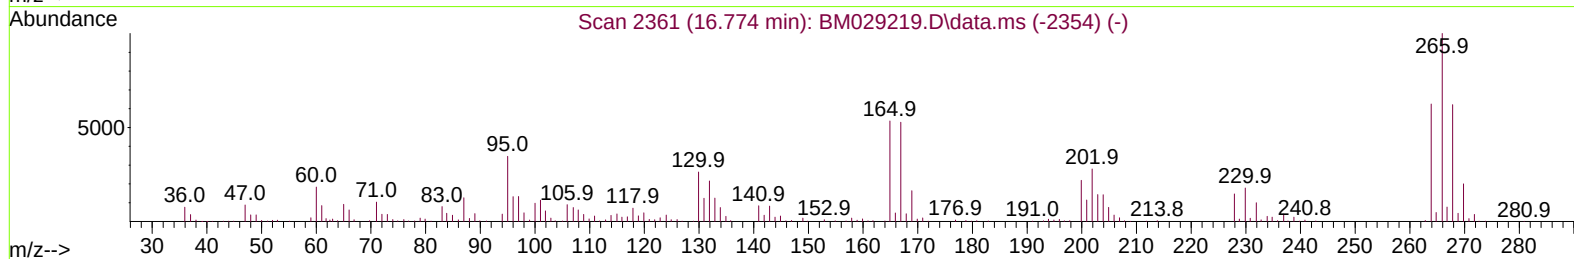
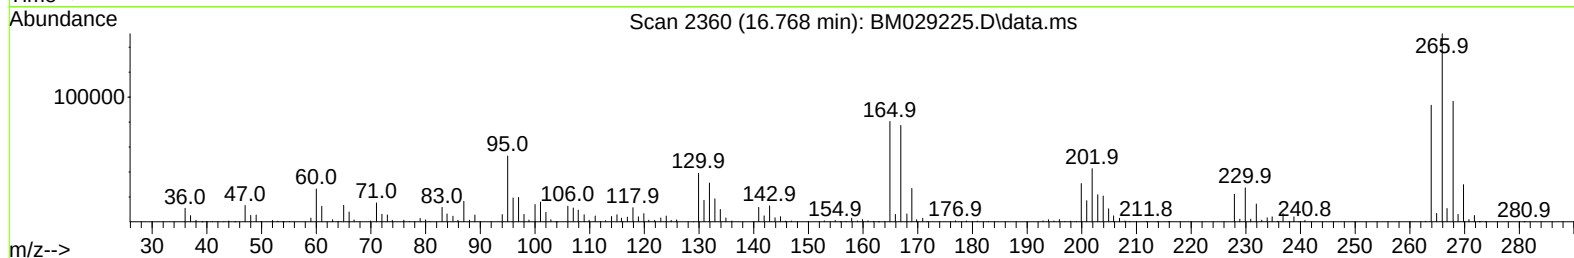


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM032621\  
 Data File : BM029225.D  
 Acq On : 26 Mar 2021 08:41  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 09:57:34 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM032621.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Mar 25 16:05:40 2021  
 Response via : Initial Calibration

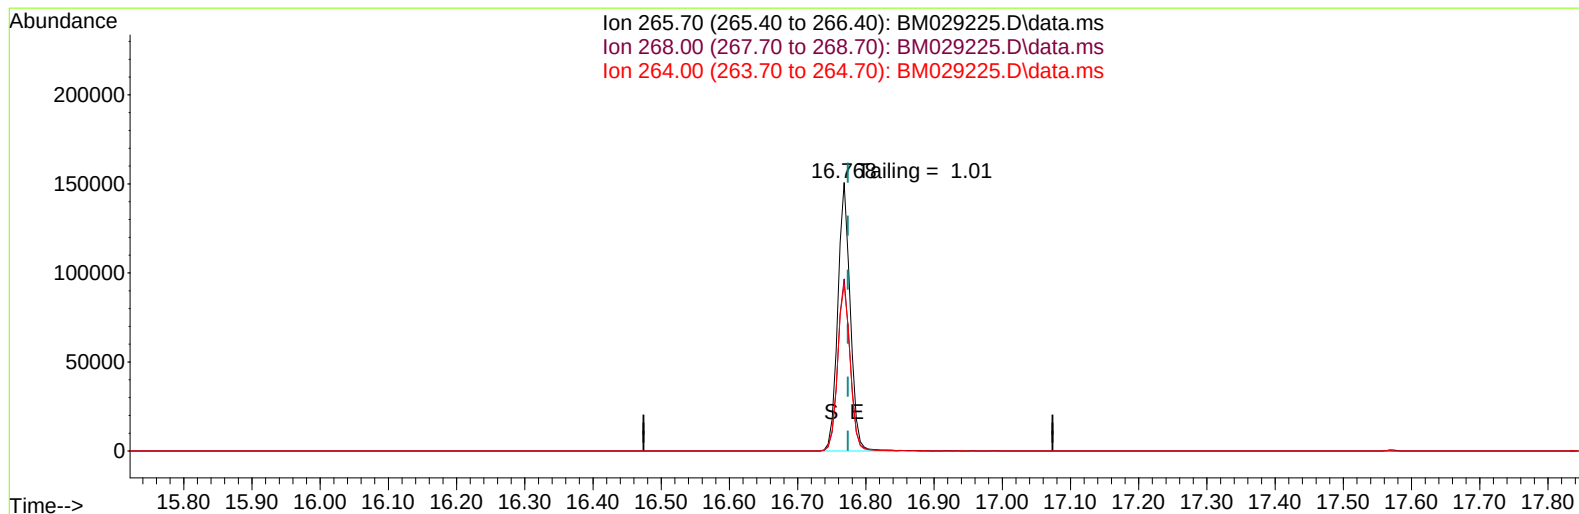

TIC: BM029225.D\data.ms

**(70) Pentachlorophenol (C)**




16.768min (-0.006) 539057.67 ng m

response 189827

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.20  | 64.10  |
| 264.00 | 63.60  | 61.99  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM032621\  
Data File : BM029225.D  
Acq On : 26 Mar 2021 08:41  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 09:57:34 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM032621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 25 16:05:40 2021  
Response via : Initial Calibration

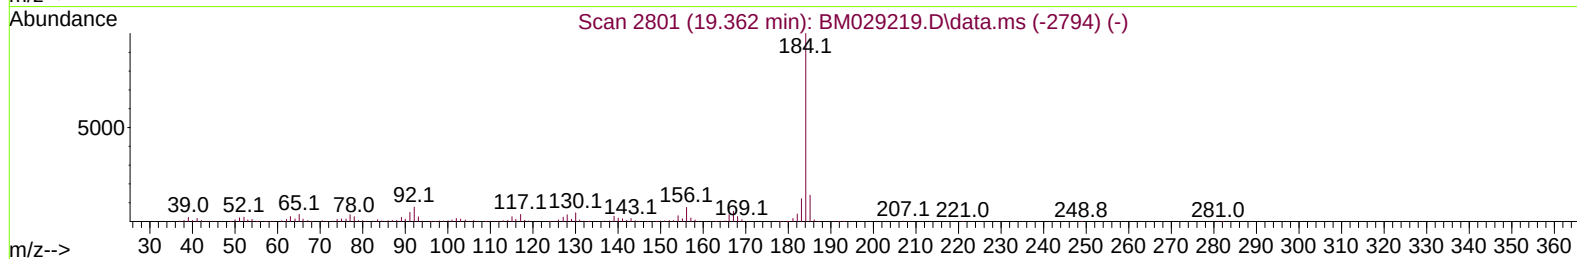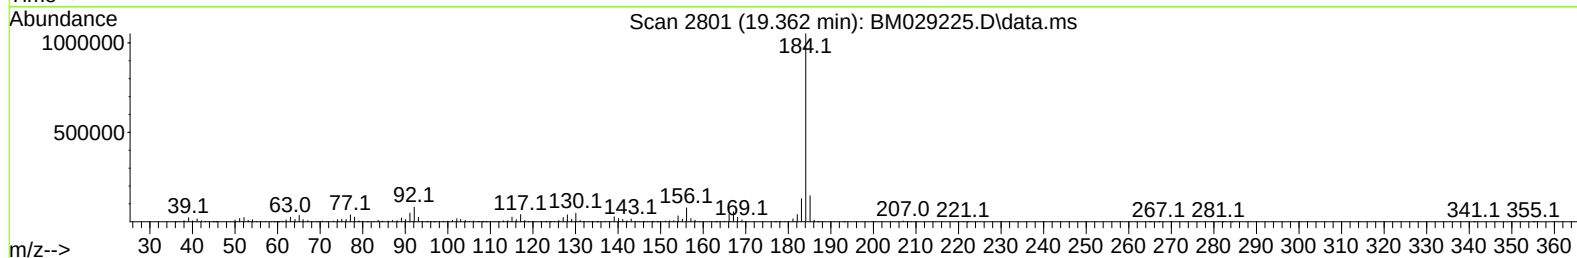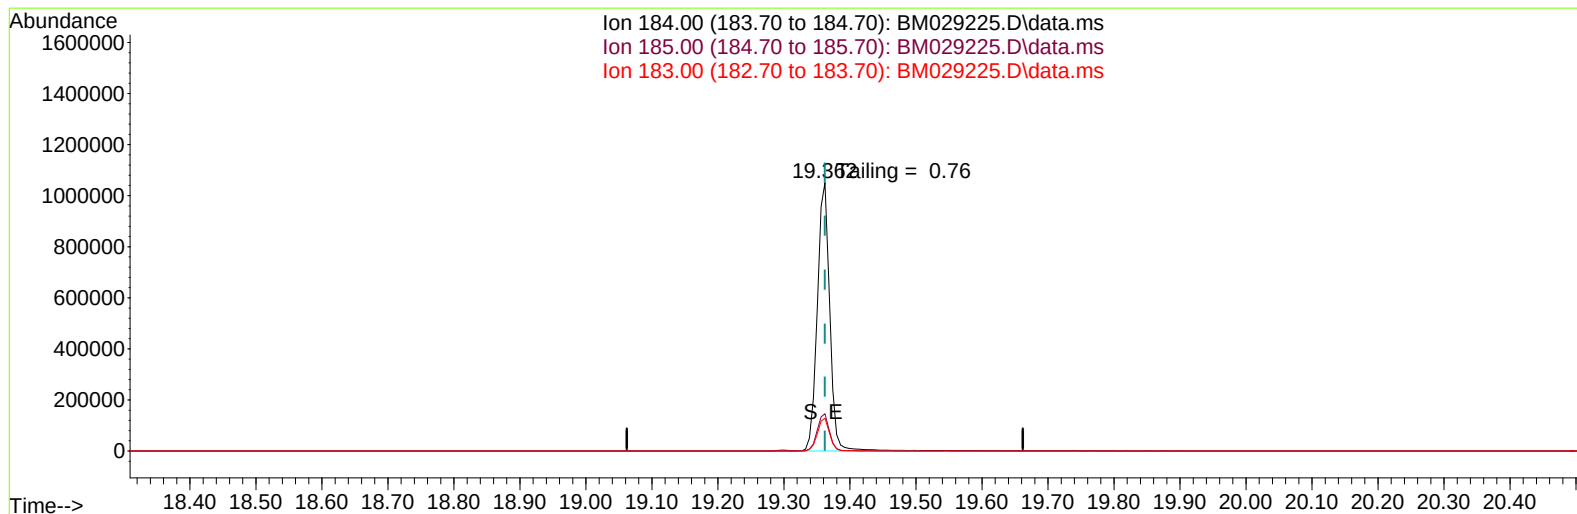

TIC: BM029225.D\data.ms

**(77) Benzidine**

19.362min (+ 0.000) 9245.47 ng m

response 1386014

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 13.93  |
| 183.00 | 12.20  | 12.26  |
| 0.00   | 0.00   | 0.00   |