
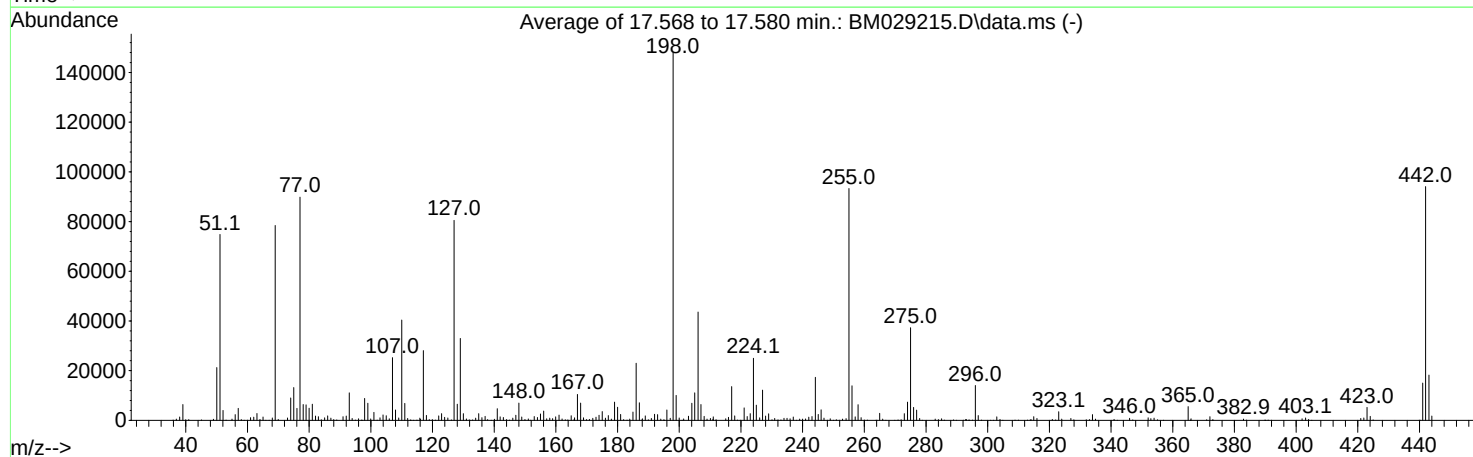


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
 Data File : BM029215.D
 Acq On : 25 Mar 2021 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 16:05:40 2021

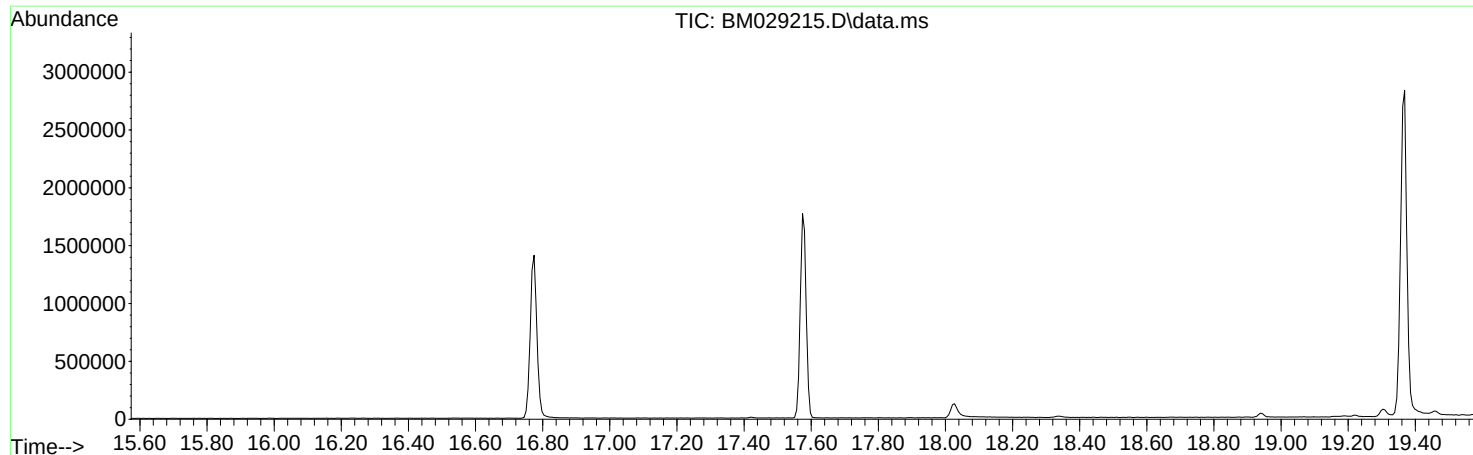

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	74808	PASS
68	69	0.00	2	1.2	936	PASS
69	198	0.00	100	53.0	78448	PASS
70	69	0.00	2	0.5	409	PASS
127	198	10	80	54.4	80493	PASS
197	198	0.00	2	0.6	830	PASS
198	198	100	100	100.0	148032	PASS
199	198	5	9	6.8	10024	PASS
275	198	10	60	25.2	37264	PASS
365	198	1	100	3.8	5554	PASS
441	198	0.01	100	10.1	14986	PASS
442	442	50	100	100.0	94093	PASS
443	442	15	24	19.4	18252	PASS

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/26/2021	BNA_M	<u>BM029215.D</u>
Compound Name	Response	Retention Time
DDT	650166	20.6
DDD	2351	20.15
DDE	672	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3023	653189	0.46

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
 Data File : BM029215.D
 Acq On : 25 Mar 2021 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 12:54:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 12:50:01 2021
 Response via : Initial Calibration

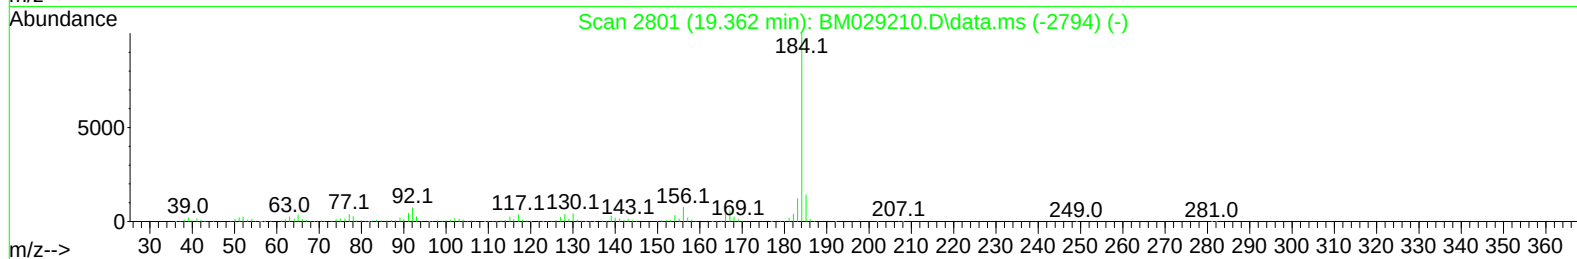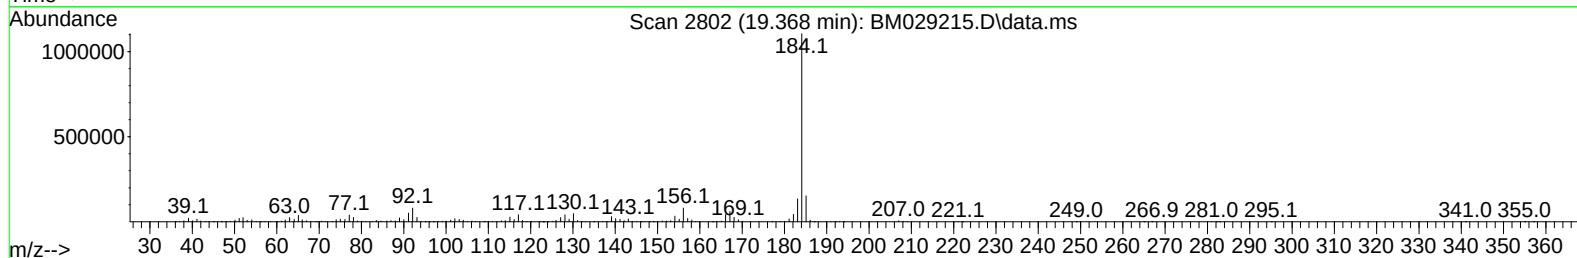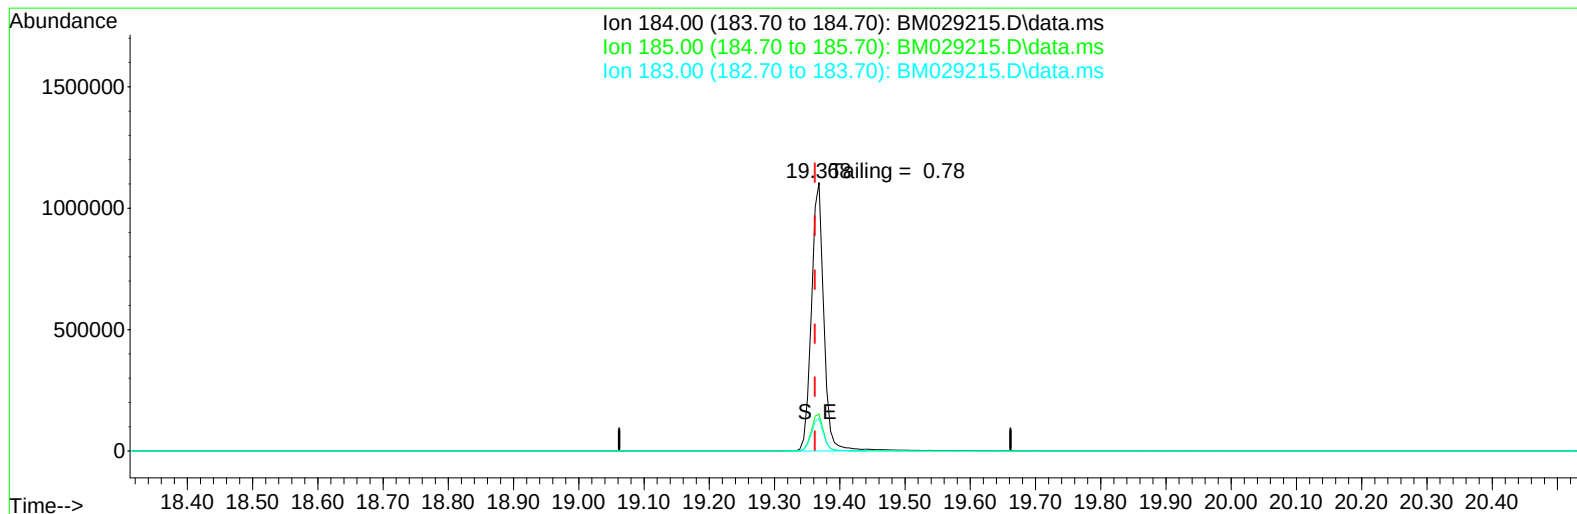

TIC: BM029215.D\data.ms

(77) Benzidine

19.368min (+ 0.006) 0.00 ng




response 1468364

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.79
183.00	12.20	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
Data File : BM029215.D
Acq On : 25 Mar 2021 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 25 12:54:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 12:50:01 2021
Response via : Initial Calibration

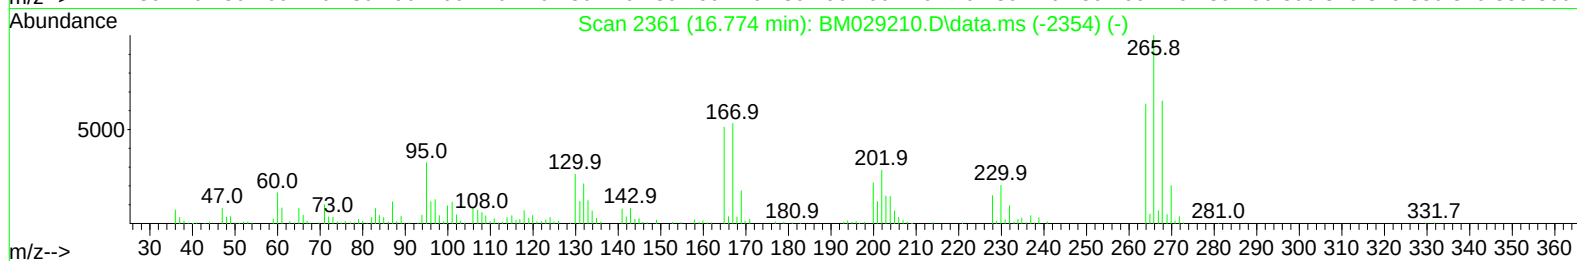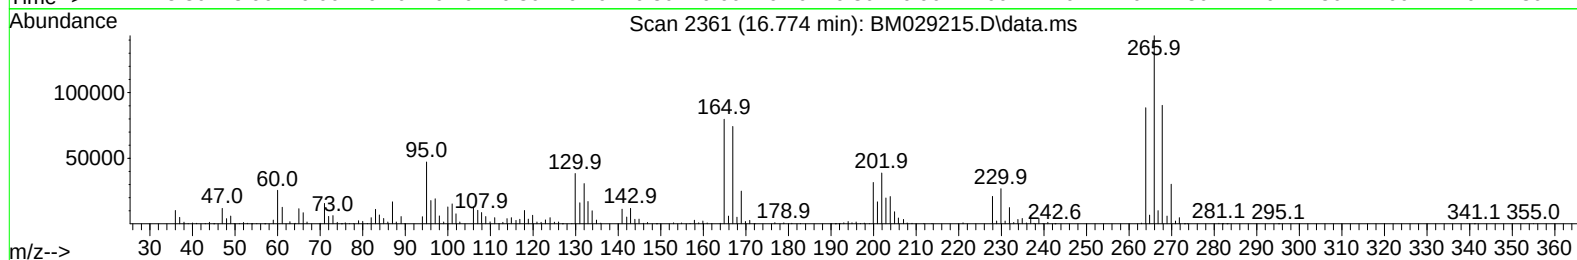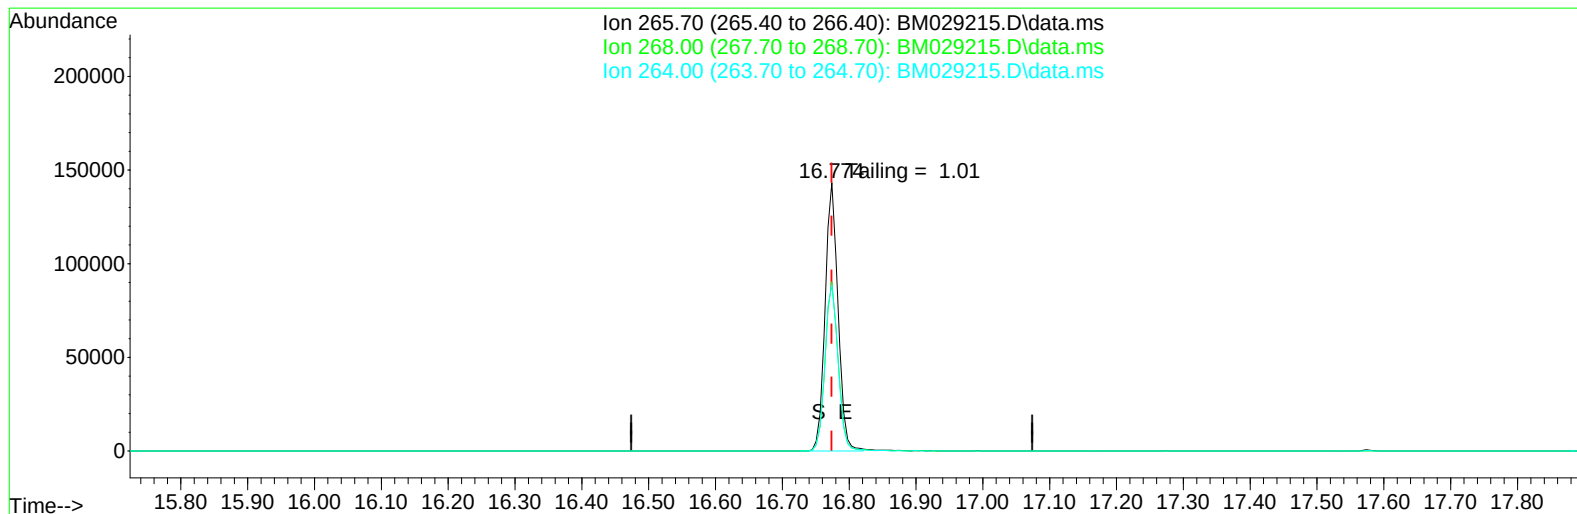

TIC: BM029215.D\data.ms

(70) Pentachlorophenol (C)

16.774min (+ 0.000) 0.00 ng

response 193434

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	63.01
264.00	63.60	61.76
0.00	0.00	0.00