
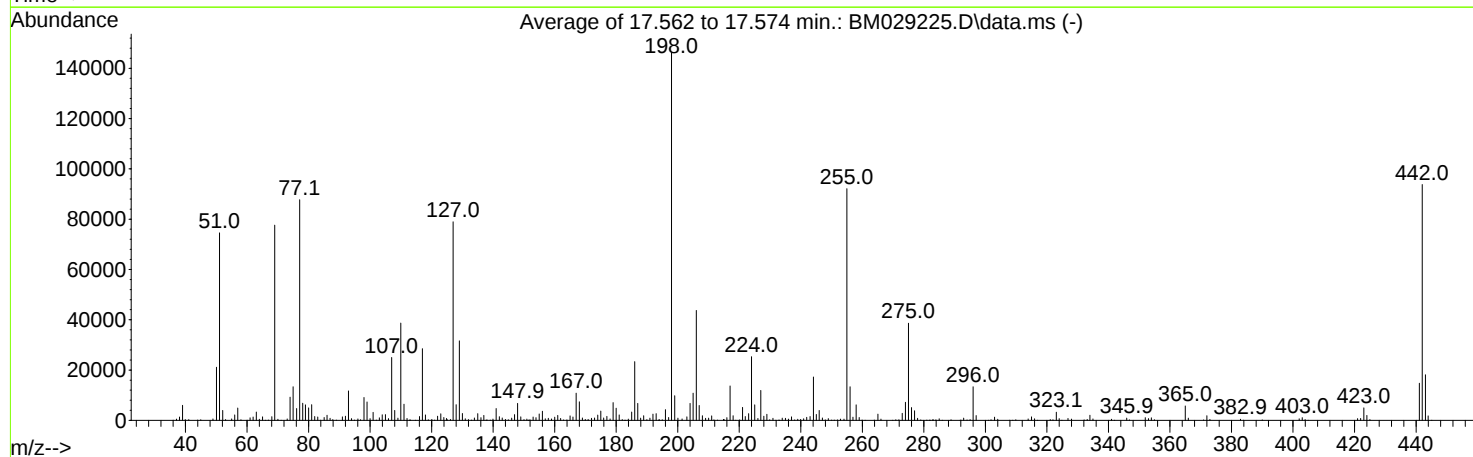


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
 Data File : BM029225.D
 Acq On : 26 Mar 2021 08:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 16:05:40 2021

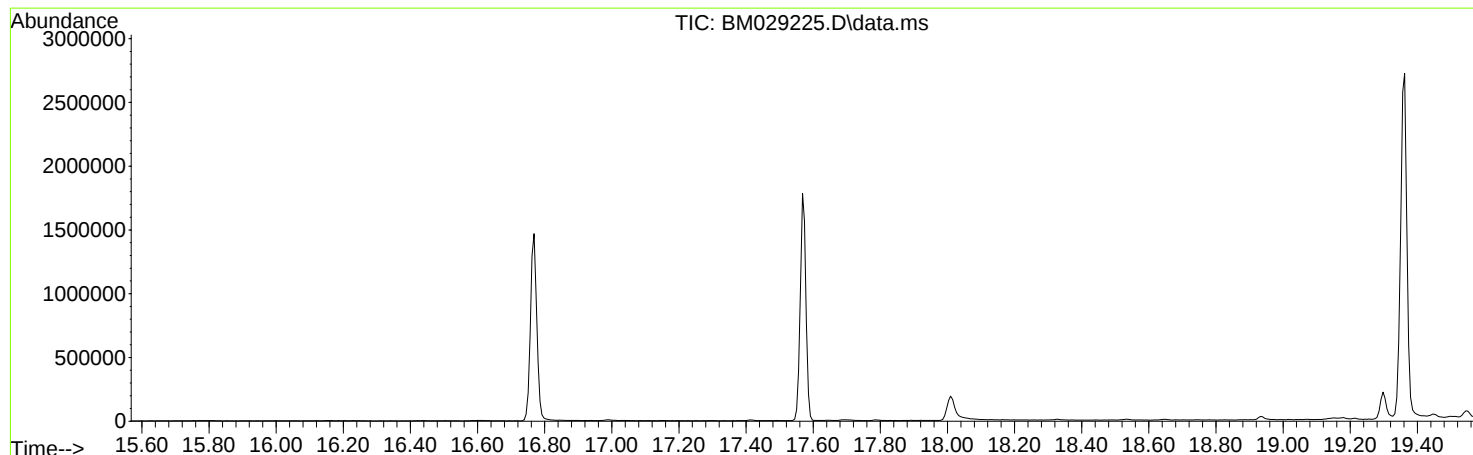

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	74567	PASS
68	69	0.00	2	1.9	1482	PASS
69	198	0.00	100	53.1	77621	PASS
70	69	0.00	2	0.6	459	PASS
127	198	10	80	54.0	78931	PASS
197	198	0.00	2	0.8	1152	PASS
198	198	100	100	100.0	146275	PASS
199	198	5	9	6.7	9796	PASS
275	198	10	60	26.4	38635	PASS
365	198	1	100	3.9	5759	PASS
441	198	0.01	100	10.1	14781	PASS
442	442	50	100	100.0	93795	PASS
443	442	15	24	19.3	18128	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/26/2021	BNA_M	<u>BM029225.D</u>
Compound Name	Response	Retention Time
DDT	580451	20.597
DDD	5194	20.15
DDE	716	19.656
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5910	586361	1.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
Data File : BM029225.D
Acq On : 26 Mar 2021 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 26 09:57:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 16:05:40 2021
Response via : Initial Calibration

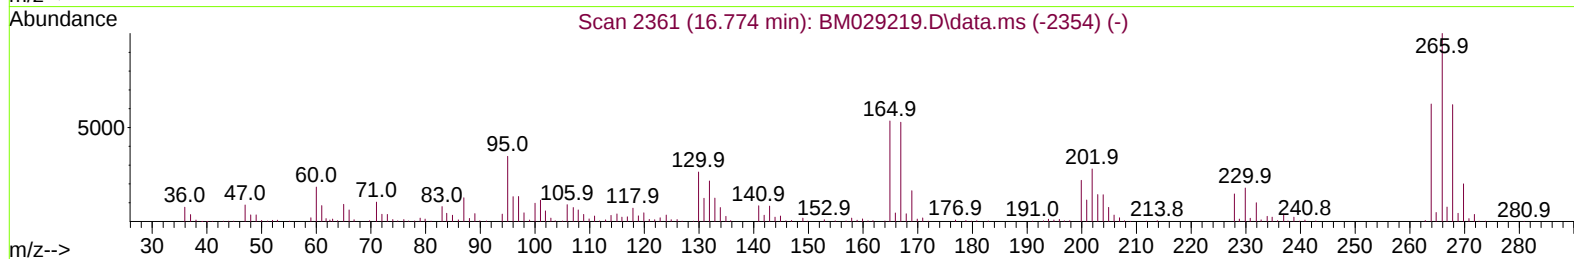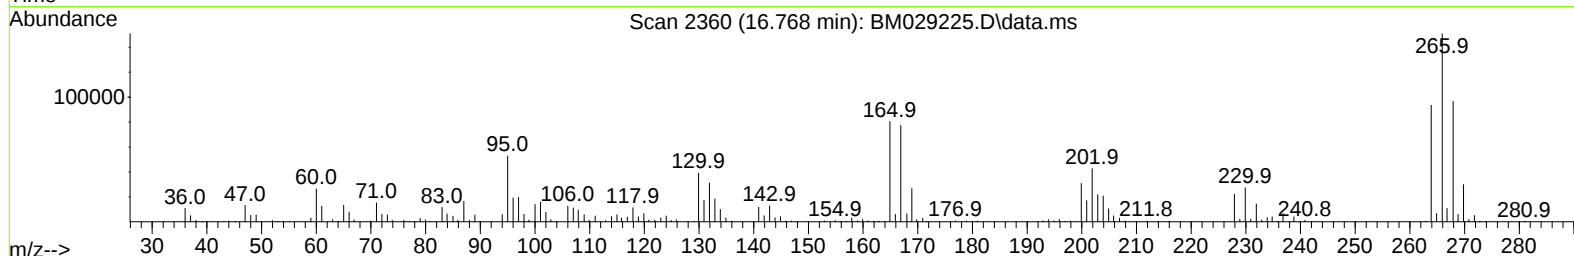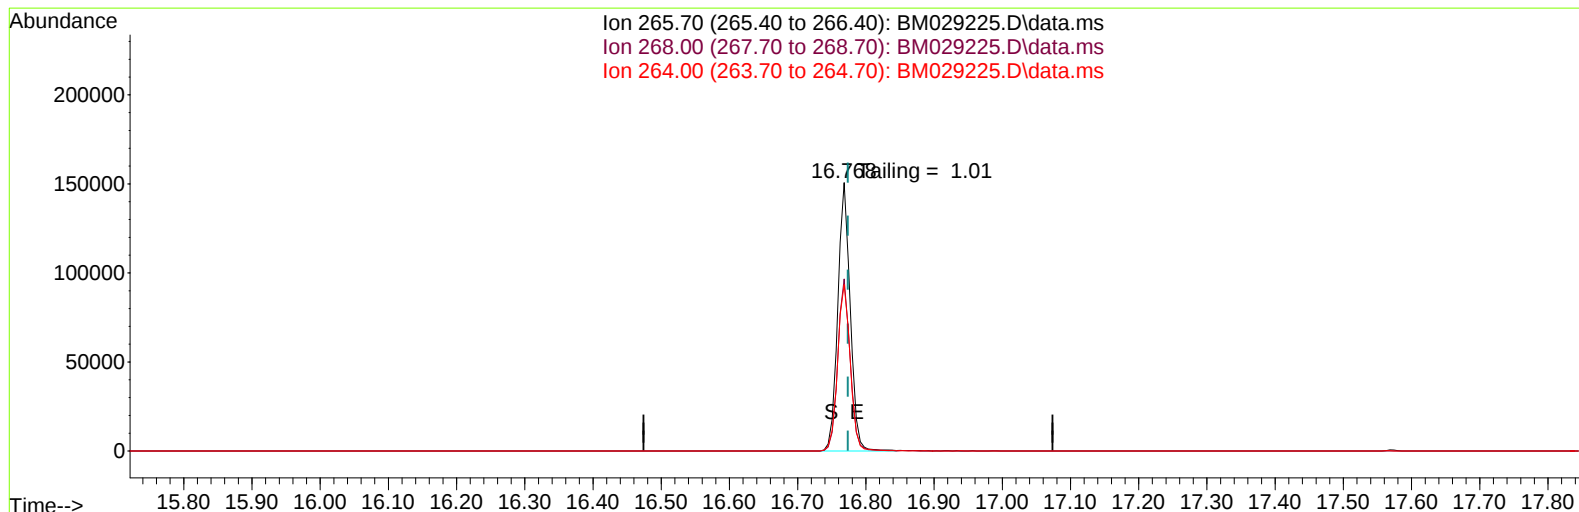

TIC: BM029225.D\data.ms

(70) Pentachlorophenol (C)

16.768min (-0.006) 539057.67 ng m




response 189827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.10
264.00	63.60	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032621\
Data File : BM029225.D
Acq On : 26 Mar 2021 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 26 09:57:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 16:05:40 2021
Response via : Initial Calibration

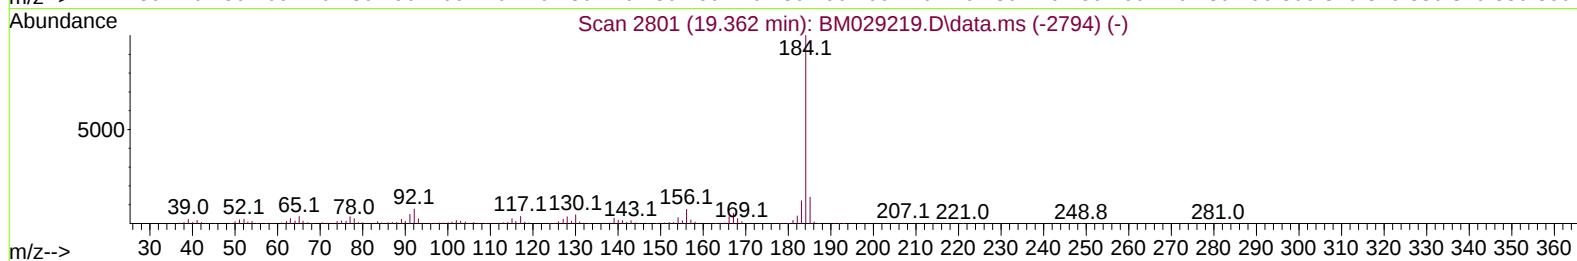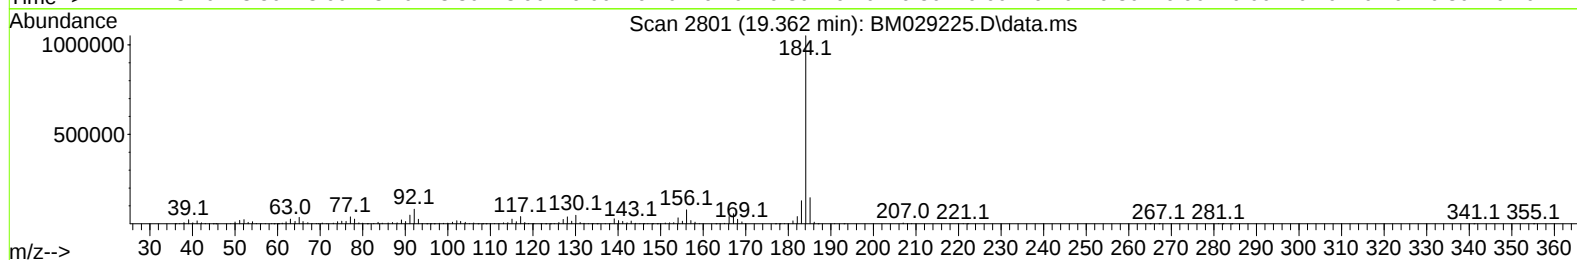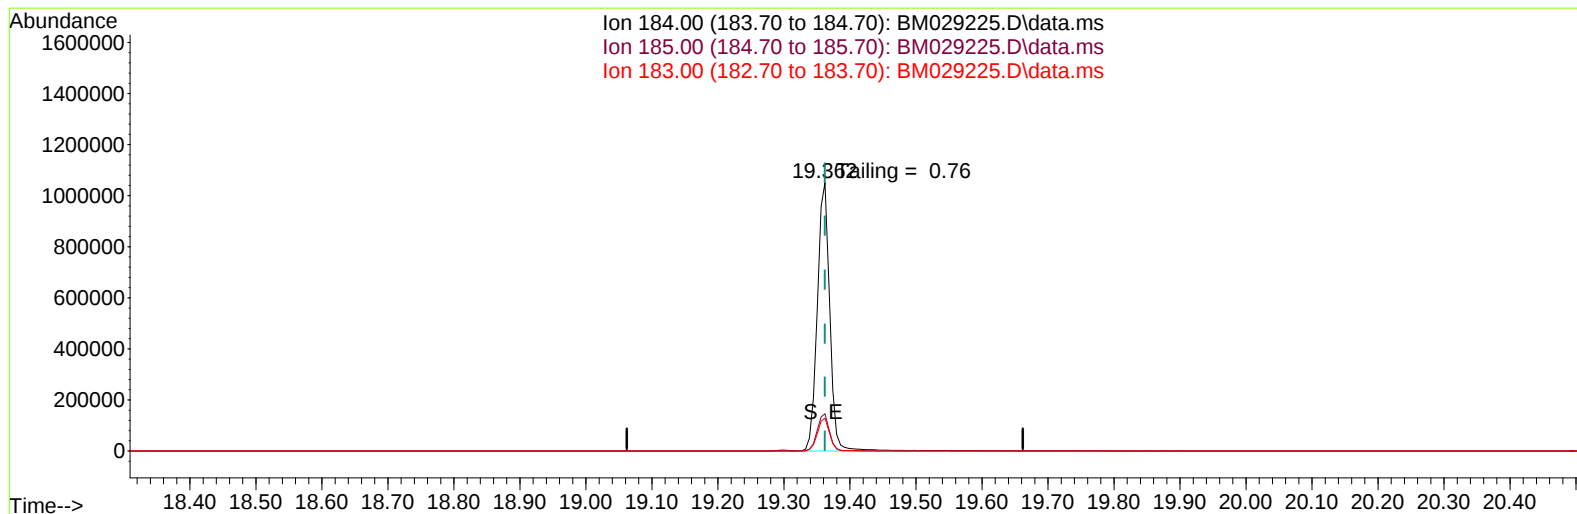

TIC: BM029225.D\data.ms

(77) Benzidine

19.362min (+ 0.000) 9245.47 ng m

response 1386014

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.93
183.00	12.20	12.26
0.00	0.00	0.00