
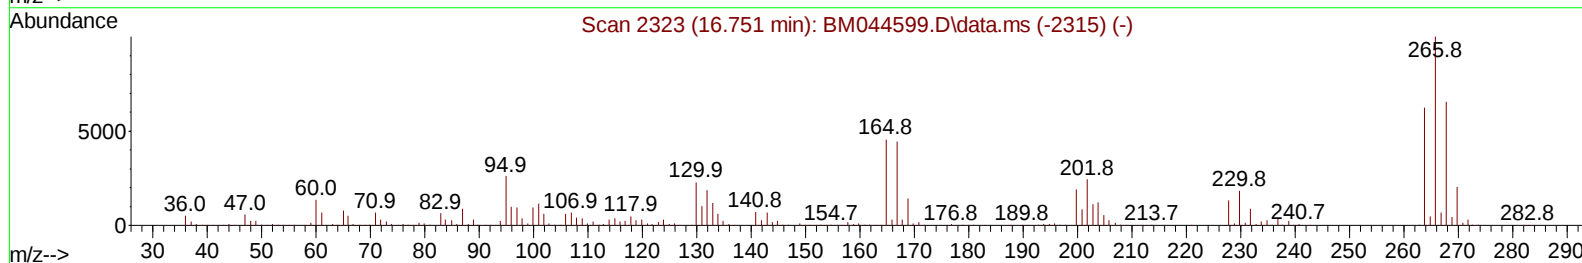
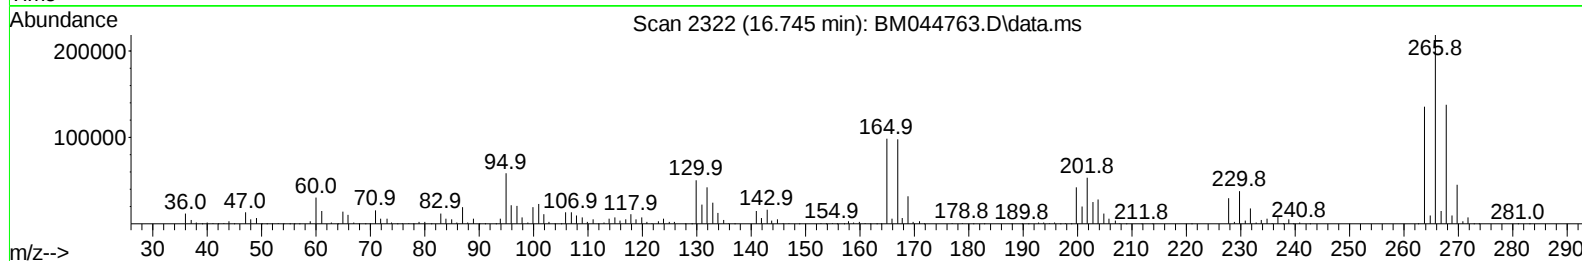


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032624\
Data File : BM044763.D
Acq On : 26 Mar 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 04:12:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

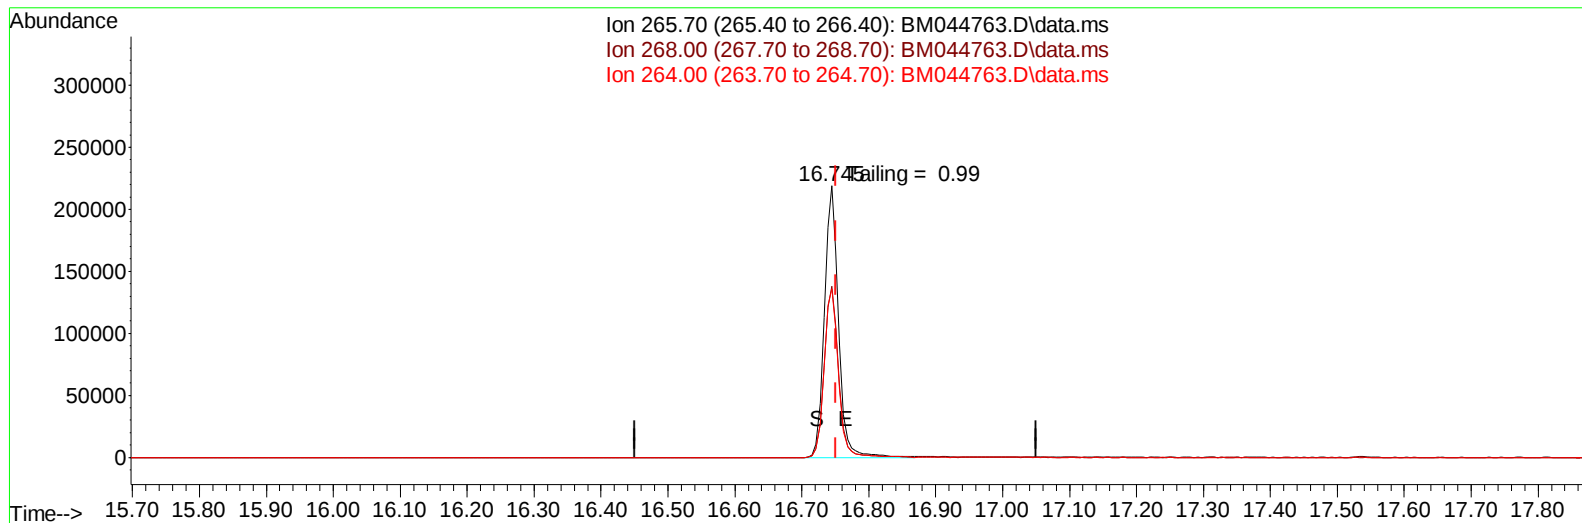

TIC: BM044763.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.006) 0.00 ng

response 324357

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	63.01
264.00	62.30	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032624\
Data File : BM044763.D
Acq On : 26 Mar 2024 10:26
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 04:12:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

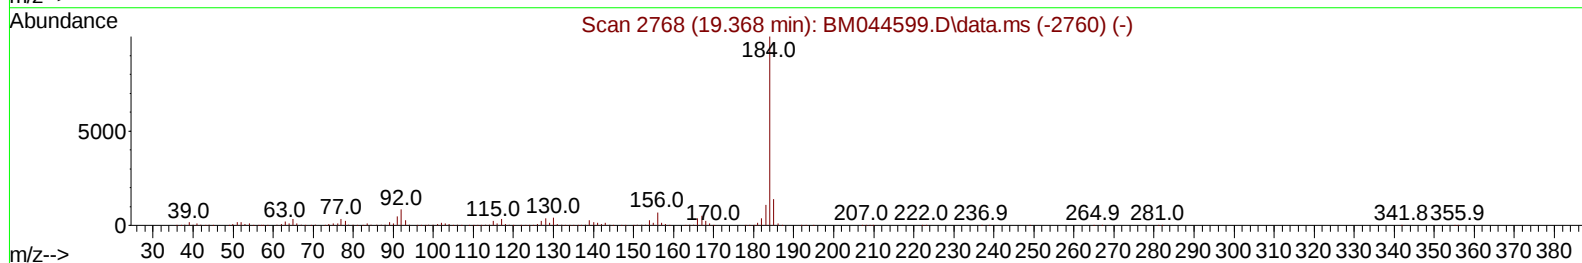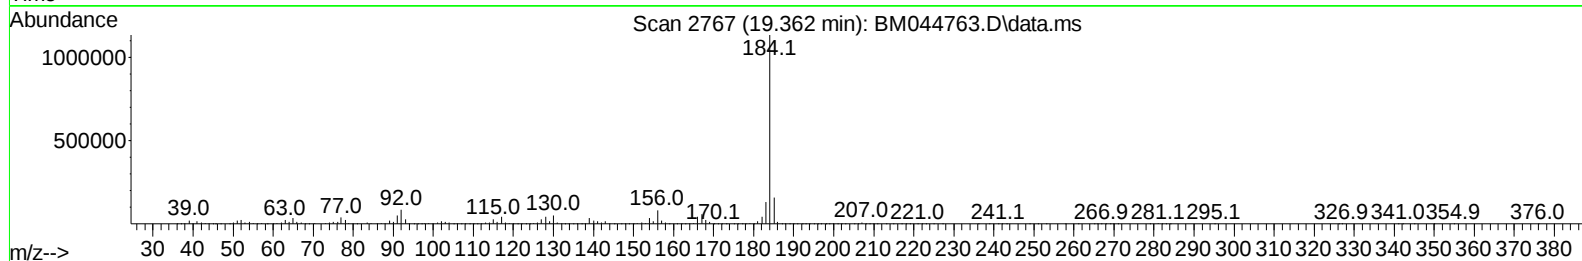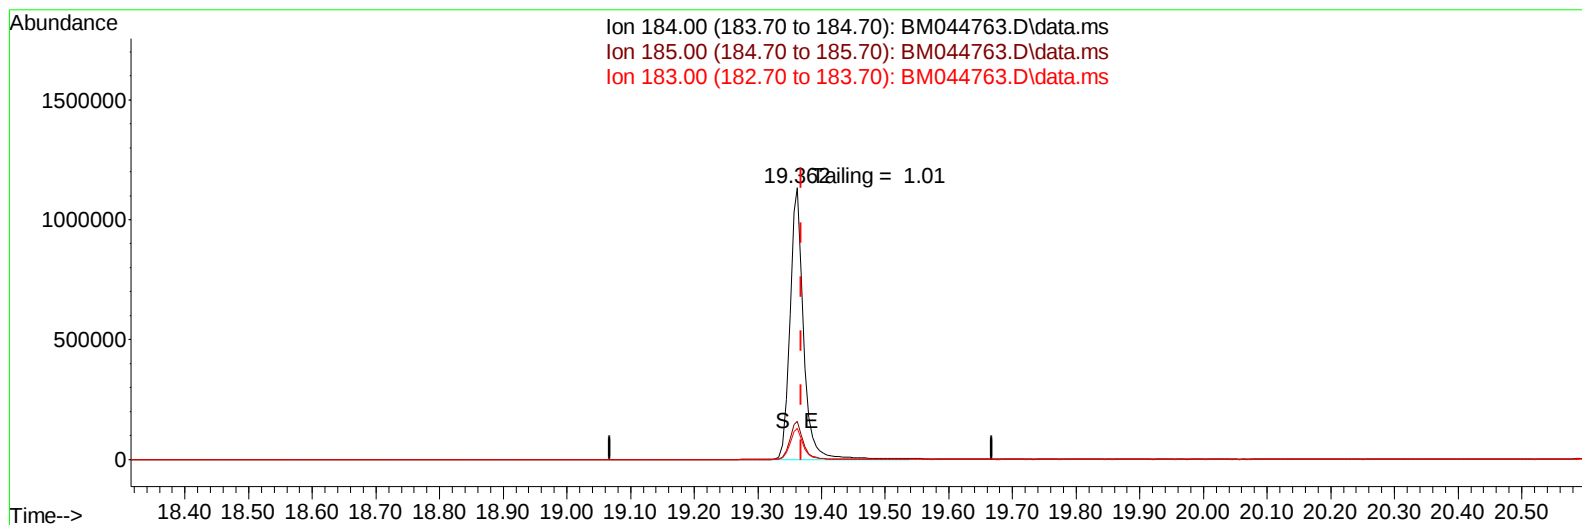

TIC: BM044763.D\data.ms

(77) Benzidine**19.362min (-0.006) 120558.74 ng****response 1704379**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.95
183.00	10.90	11.42
0.00	0.00	0.00