

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032717\
 Data File : BM009413.D
 Acq On : 27 Mar 2017 14:44
 Operator : SJ/MA
 Sample : I2326-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA4

Manual Integrations
 APPROVED

mohammad
 3/27/2017 4:32:42 PM

Quant Time: Mar 27 15:30:58 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 27 14:15:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	84	0.40	ng/ul	0.00
2) Naphthalene-d8	10.66	136	263	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.49	164	165	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	341m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	429	0.40	ng/ul	0.00
20) Perylene-d12	23.74	264	398m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.24	152	156	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	451m	0.42	ng/ul	-0.01
Target Compounds						
8) Acenaphthene	14.55	153	216	0.33	ng/ul#	51

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032717\
Data File : BM009413.D
Acq On : 27 Mar 2017 14:44
Operator : SJ/MA
Sample : I2326-05
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AA4

Manual Integrations
APPROVED

mohammad
3/27/2017 4:32:42 PM

Quant Time: Mar 27 15:30:58 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 14:15:51 2017
Response via : Initial Calibration

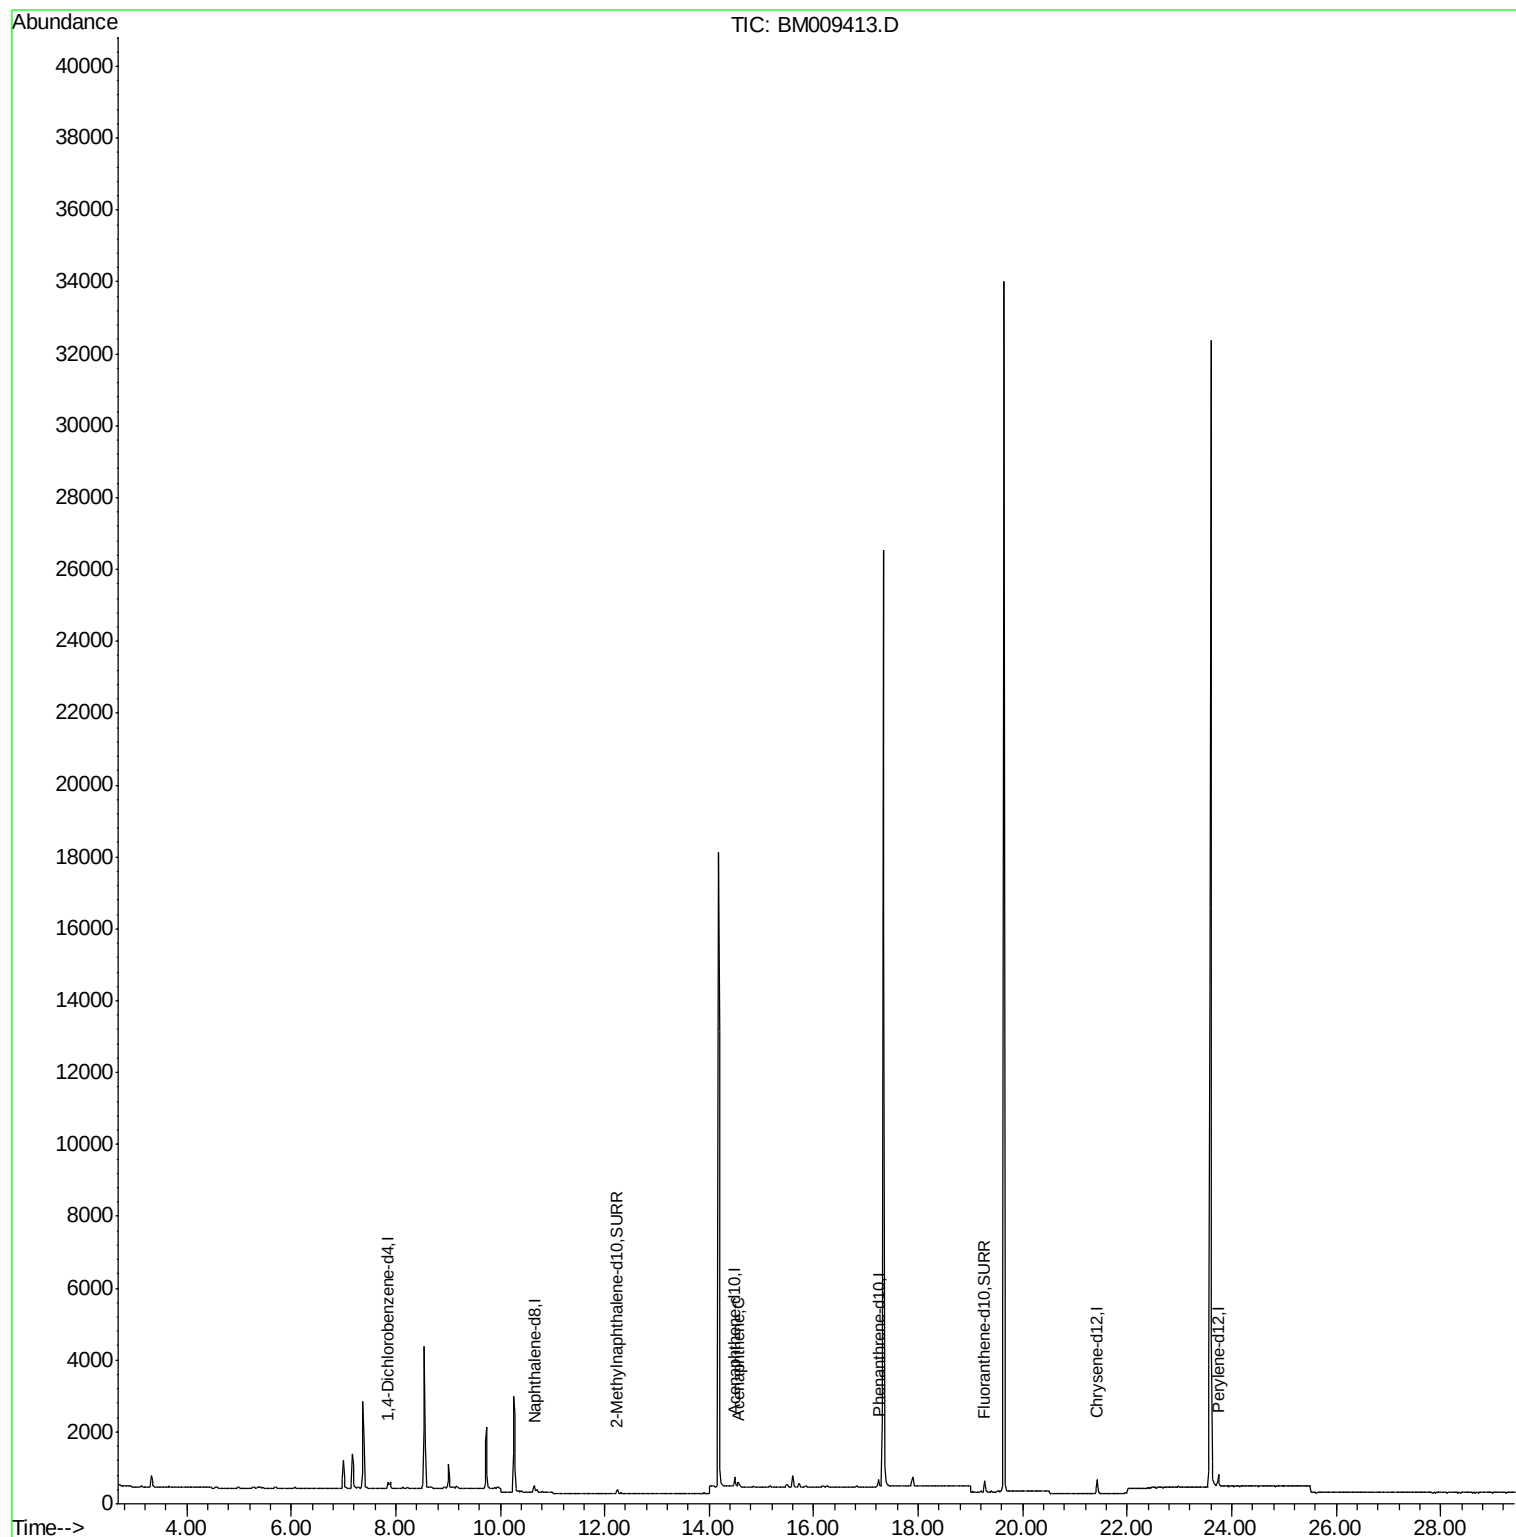

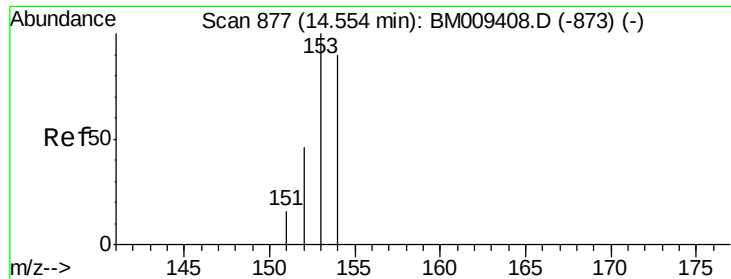

#8
 Acenaphthene
 Concen: 0.33 ng/ul
 RT: 14.55 min Scan# 877
 Delta R.T. 0.00 min
 Lab File: BM009413.D
 Acq: 27 Mar 2017 14:44

Instrument :
 BNA_M
 ClientSampleId :
 C0AA4

Tgt Ion	Ratio	Lower	Upper
153	100		
152	28.6	40.3	60.5#
154	33.9	71.4	107.2#

Manual Integrations
 APPROVED

mohammad
 3/27/2017 4:32:42 PM

