
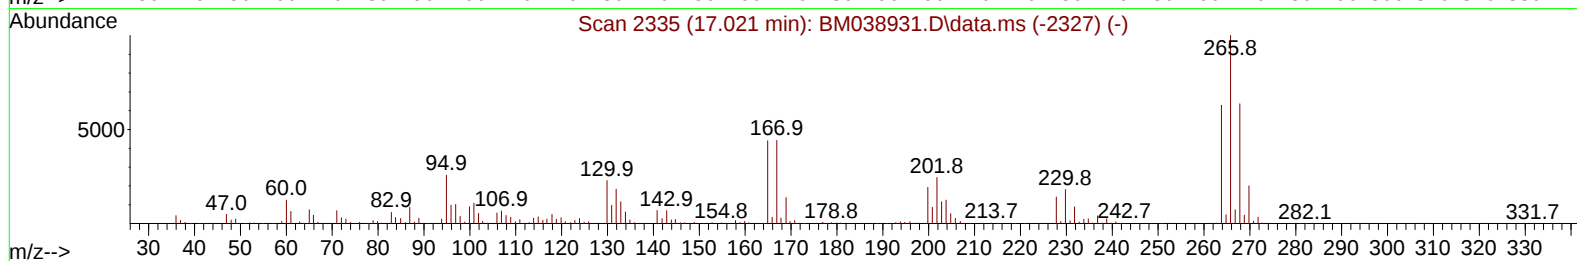
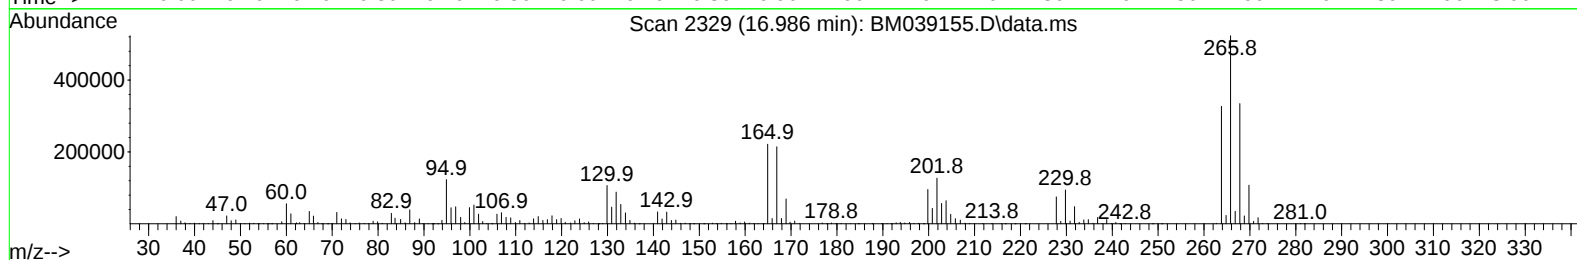


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
 Data File : BM039155.D
 Acq On : 27 Mar 2023 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 04:55:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 28 01:46:09 2023
 Response via : Initial Calibration

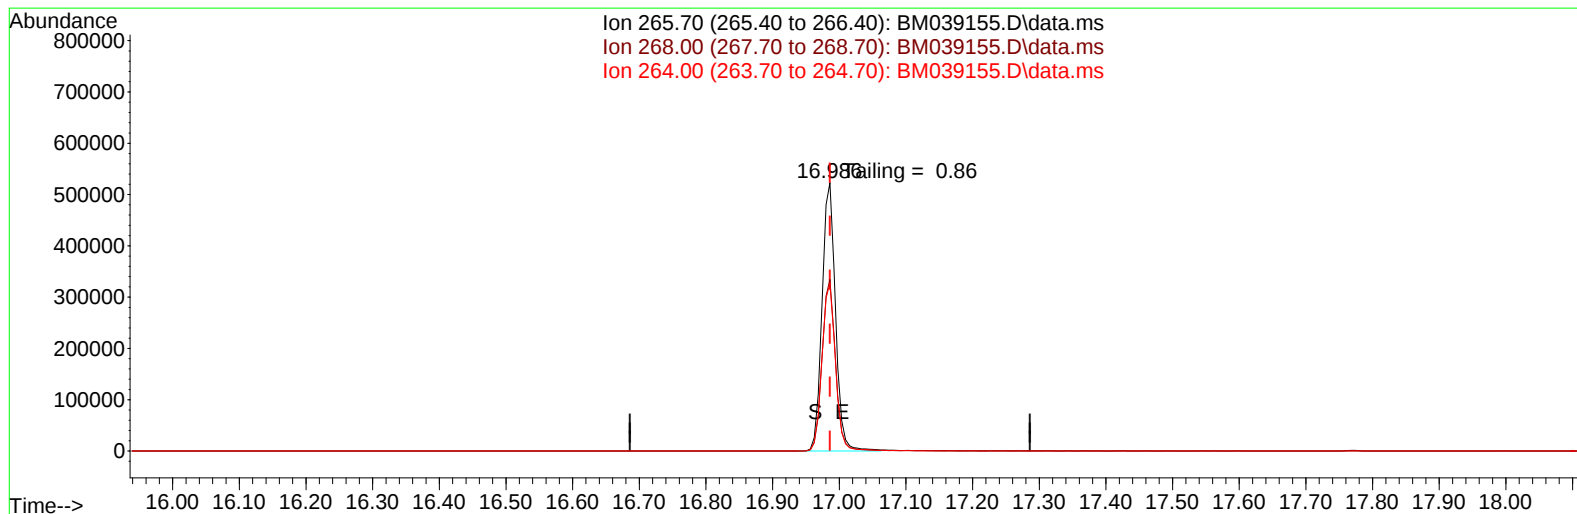

TIC: BM039155.D\data.ms

(70) Pentachlorophenol (C)




16.986min (-0.000) 453431.27 ng

response 736913

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.93
264.00	62.90	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
Data File : BM039155.D
Acq On : 27 Mar 2023 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 04:55:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 01:46:09 2023
Response via : Initial Calibration

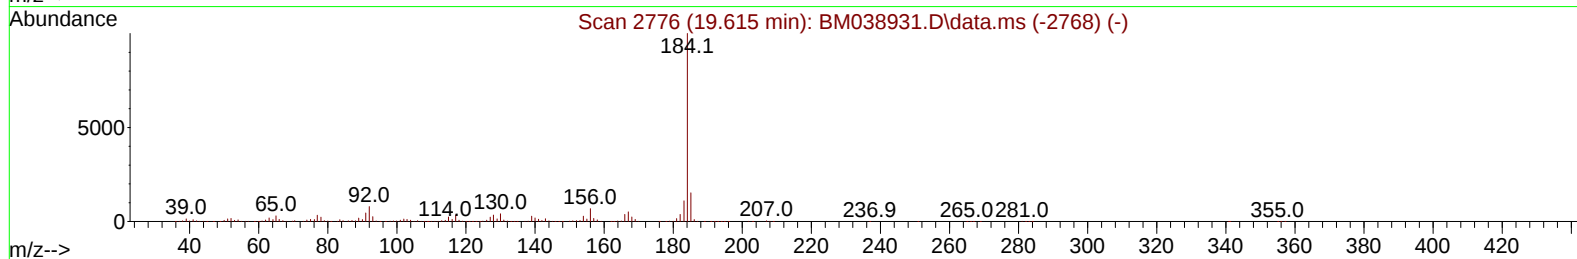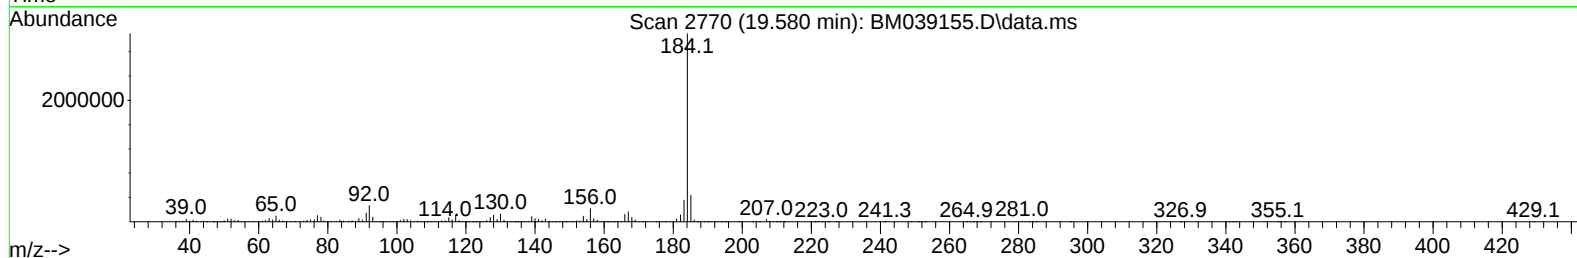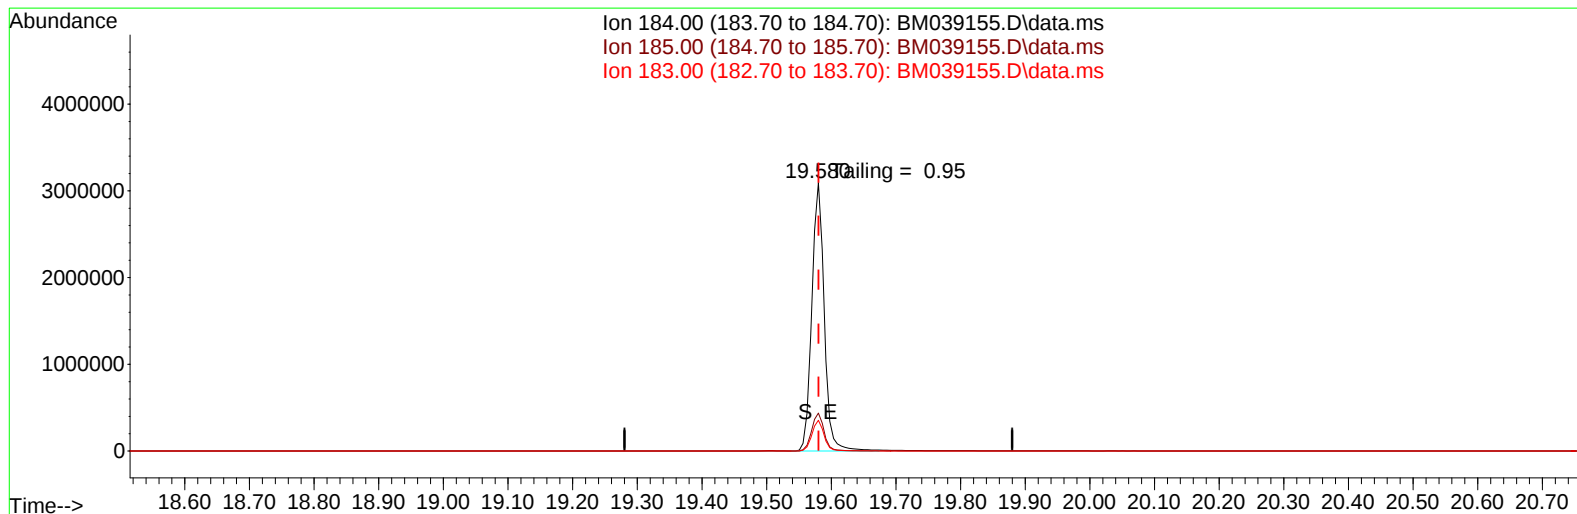

TIC: BM039155.D\data.ms

(77) Benzidine**19.580min (-0.000) 48147.24 ng****response 4162731**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.15
183.00	11.00	11.49
0.00	0.00	0.00