

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
 Data File : BM039168.D
 Acq On : 27 Mar 2023 19:54
 Operator : CG/JU
 Sample : 01998-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BROAD-CHANNEL-SUBSTATION-TP2

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 03/28/2023
 Supervised By :Jagrut Upadhyay 03/28/2023

Quant Time: Mar 28 01:52:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 28 01:46:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	269473	20.000	ng	0.00
21) Naphthalene-d8	10.757	136	1077526	20.000	ng	0.00
39) Acenaphthene-d10	14.586	164	617932	20.000	ng	0.00
64) Phenanthrene-d10	17.333	188	1273672	20.000	ng	0.00
76) Chrysene-d12	21.521	240	1170599	20.000	ng	0.00
86) Perylene-d12	23.950	264	1367517	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	1777534	100.217	ng	0.00
7) Phenol-d6	7.116	99	2244655	97.431	ng	0.00
23) Nitrobenzene-d5	9.116	82	1346337	61.375	ng	0.00
42) 2,4,6-Tribromophenol	16.080	330	718722	100.542	ng	0.00
45) 2-Fluorobiphenyl	13.216	172	2630289	55.412	ng	0.00
79) Terphenyl-d14	19.956	244	3701731	57.816	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	10.810	128	351251	5.717	ng	99
49) Acenaphthylene	14.310	152	168501	2.680	ng	98
52) Acenaphthene	14.651	154	391681	10.136	ng	99
55) Dibenzofuran	14.986	168	289468	4.787	ng	99
58) Fluorene	15.633	166	447550	9.448	ng	99
71) Phenanthrene	17.380	178	6508288	87.064	ng	99
72) Anthracene	17.468	178	1824774	24.478	ng	100
73) Carbazole	17.739	167	978677	14.385	ng	100
74) Di-n-butylphthalate	18.304	149	23457	2.071	ng	# 75
75) Fluoranthene	19.398	202	10346555	131.090	ng	97
78) Pyrene	19.762	202	9361489	106.475	ng	99
81) Benzo(a)anthracene	21.503	228	5291545	62.770	ng	97
83) Chrysene	21.556	228	4742903	57.848	ng	97
84) Bis(2-ethylhexyl)phtha...	21.421	149	93151	4.119	ng	# 99
87) Indeno(1,2,3-cd)pyrene	26.480	276	3542650	34.045	ng	96
88) Benzo(b)fluoranthene	23.215	252	7053673	80.737	ng	98
89) Benzo(k)fluoranthene	23.256	252	2191550m	24.104	ng	
90) Benzo(a)pyrene	23.844	252	4977765	59.201	ng	98
91) Dibenzo(a,h)anthracene	26.485	278	916980	10.406	ng	# 82
92) Benzo(g,h,i)perylene	27.268	276	3601697	41.775	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
Data File : BM039168.D
Acq On : 27 Mar 2023 19:54
Operator : CG/JU
Sample : 01998-03
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2

Quant Time: Mar 28 01:52:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 01:46:09 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 03/28/2023
Supervised By : Jagrut Upadhyay 03/28/2023

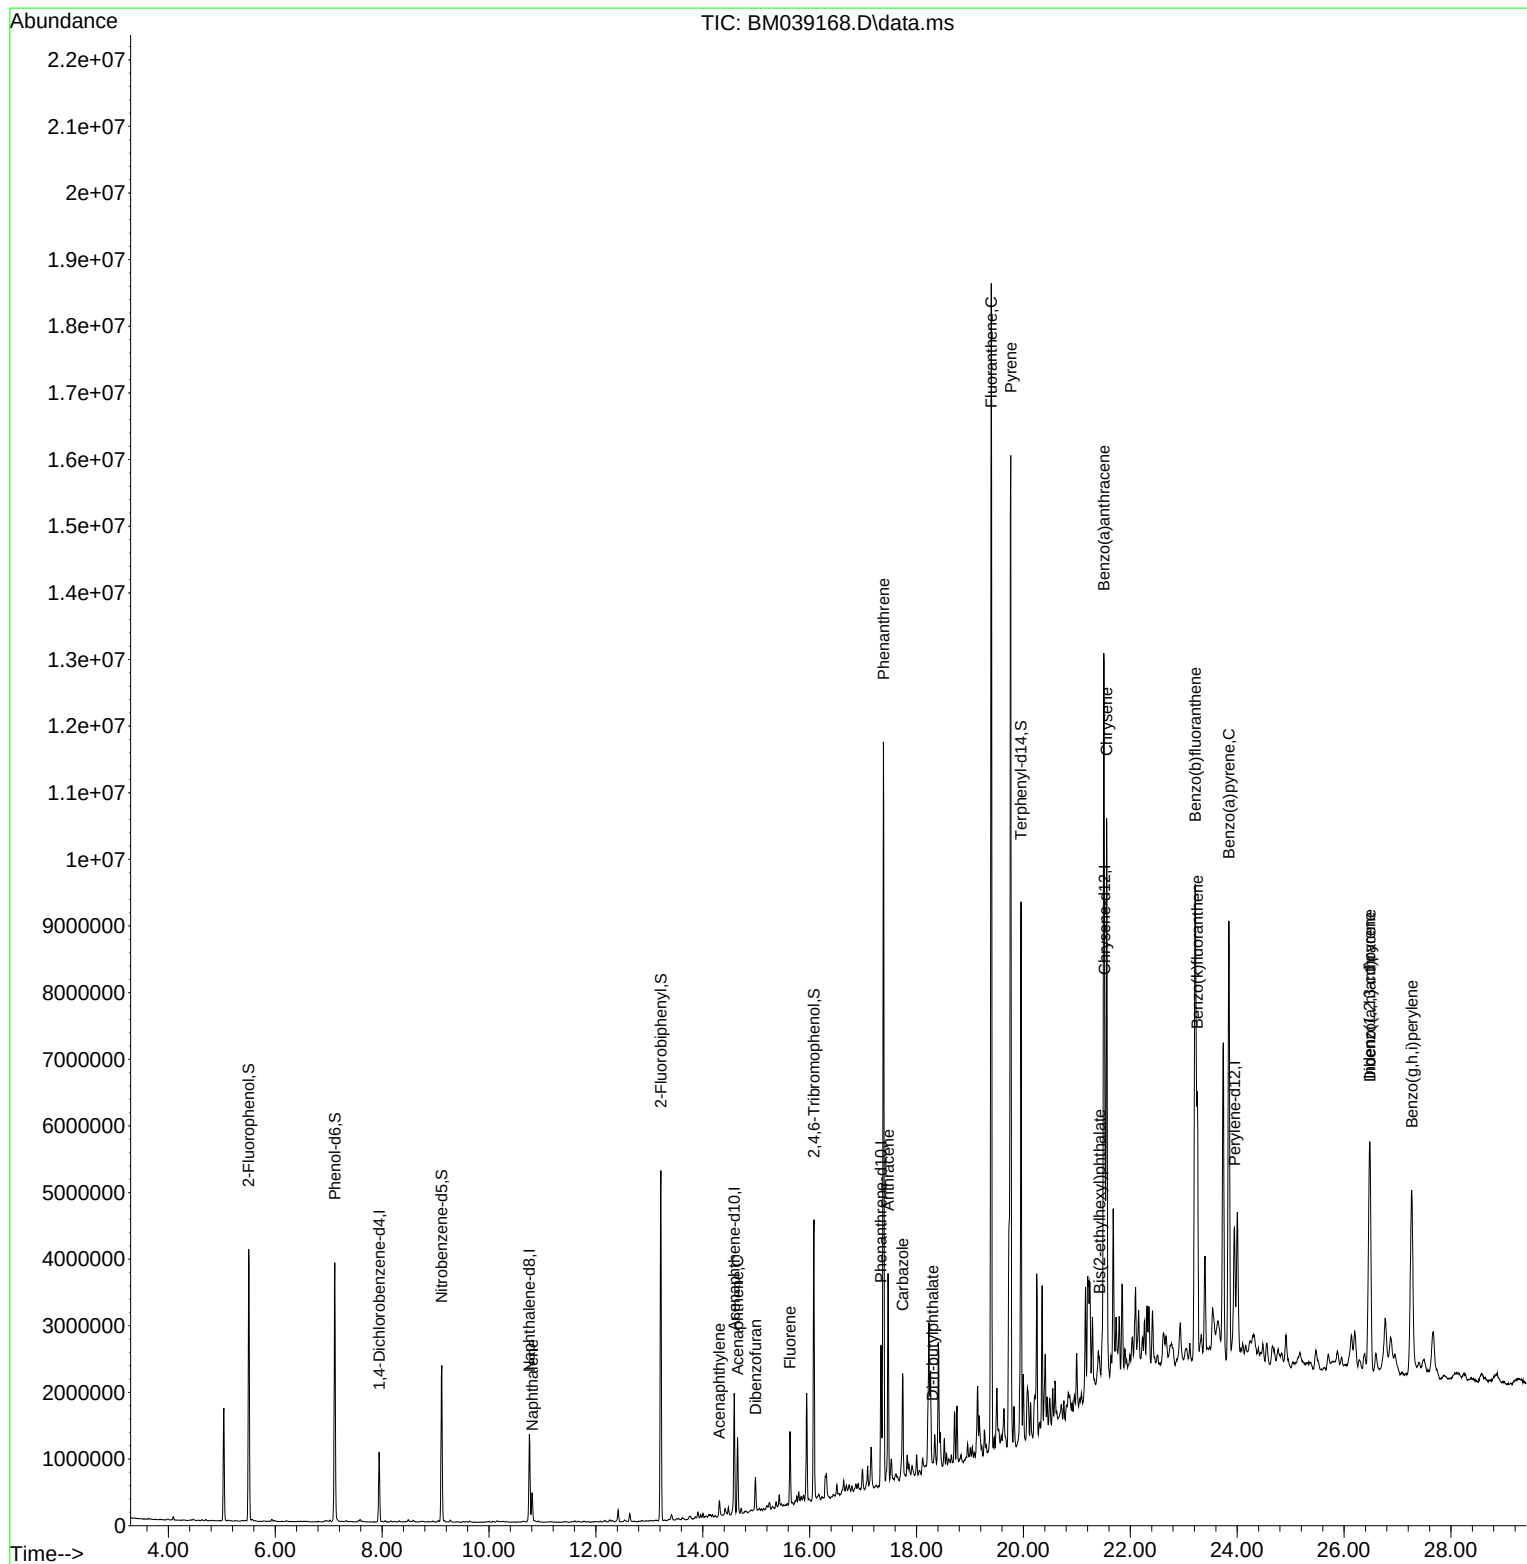



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.945 min Scan# 79
Delta R.T. 0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2



Tgt Ion:152 Resp: 269473
Ion Ratio Lower Upper
152 100
150 158.4 125.1 187.7
115 61.5 49.6 74.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

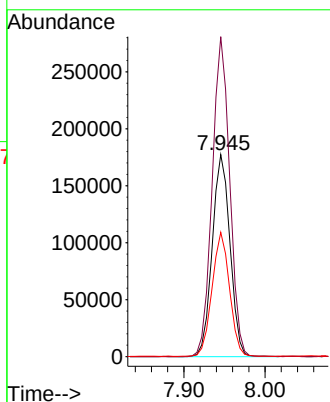

#5
2-Fluorophenol
Concen: 100.217 ng
RT: 5.504 min Scan# 377
Delta R.T. 0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54


Tgt Ion:112 Resp: 1777534
Ion Ratio Lower Upper
112 100
64 57.8 45.9 68.9
63 29.3 23.8 35.8

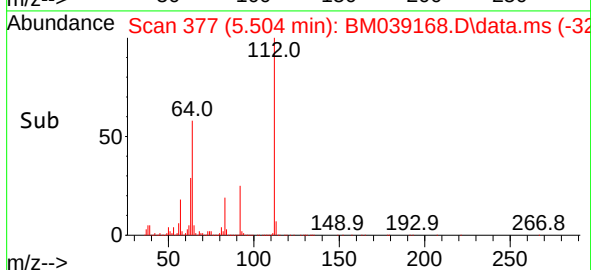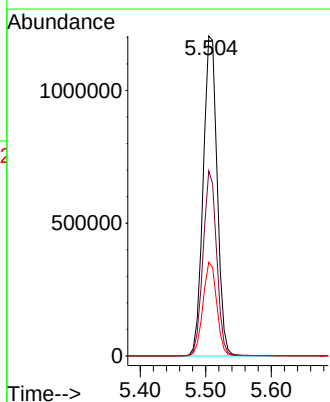



#7
Phenol-d6
Concen: 97.431 ng
RT: 7.116 min Scan# 61
Delta R.T. 0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2




Tgt Ion: 99 Resp: 2244655
Ion Ratio Lower Upper
99 100
42 16.3 13.5 20.3
71 31.9 25.6 38.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

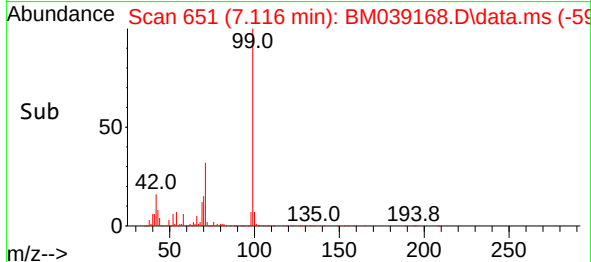


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.757 min Scan# 1270
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

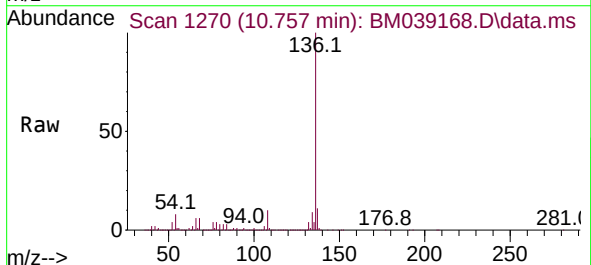


Tgt Ion:136 Resp: 1077526
Ion Ratio Lower Upper
136 100
137 10.9 8.7 13.1
54 7.8 6.3 9.5
68 6.5 5.0 7.6

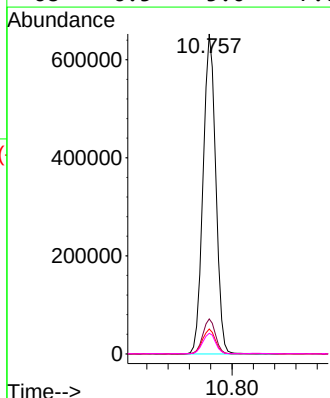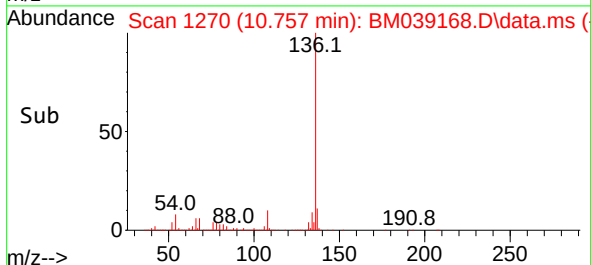



#23
Nitrobenzene-d5
Concen: 61.375 ng
RT: 9.116 min Scan# 999
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2




Tgt Ion: 82 Resp: 134633
Ion Ratio Lower Upper
82 100
128 44.5 34.4 51.6
54 47.3 38.8 58.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

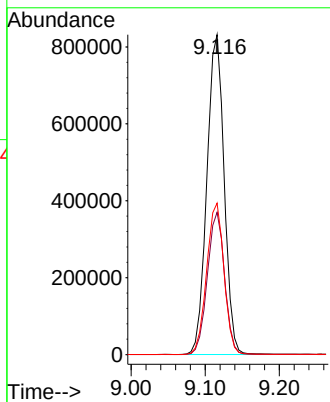


#31
Naphthalene
Concen: 5.717 ng
RT: 10.810 min Scan# 1279
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

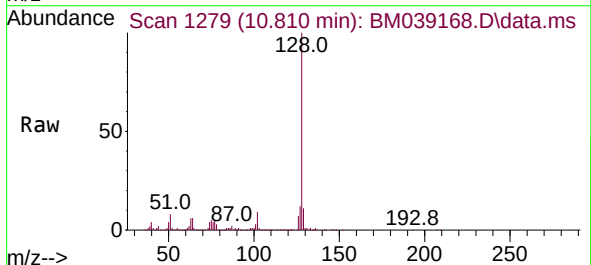


Tgt Ion:128 Resp: 351251
Ion Ratio Lower Upper
128 100
129 11.0 8.6 13.0
127 12.3 10.2 15.4

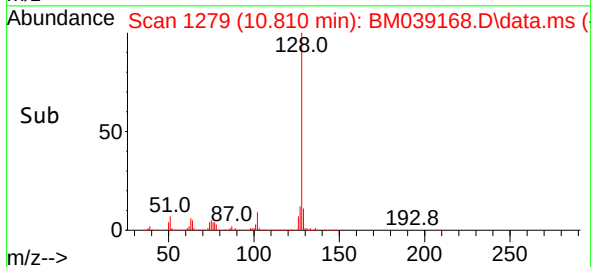



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.586 min Scan# 19
Delta R.T. -0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2



Tgt Ion:164 Resp: 617932
Ion Ratio Lower Upper
164 100
162 98.3 79.2 118.8
160 44.0 35.5 53.3




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023



#42
2,4,6-Tribromophenol
Concen: 100.542 ng
RT: 16.080 min Scan# 2175
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54


Tgt Ion:330 Resp: 718722
Ion Ratio Lower Upper
330 100
332 96.3 77.4 116.0
141 36.9 32.2 48.4

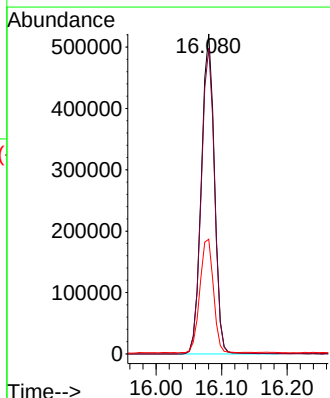

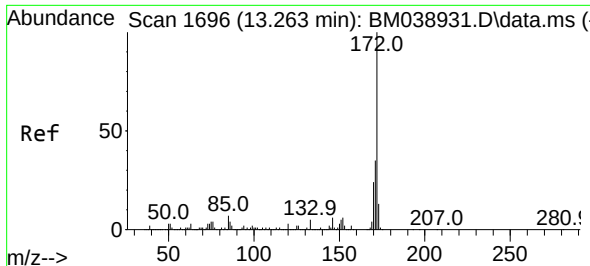

#45
2-Fluorobiphenyl
Concen: 55.412 ng
RT: 13.216 min Scan# 1696
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2

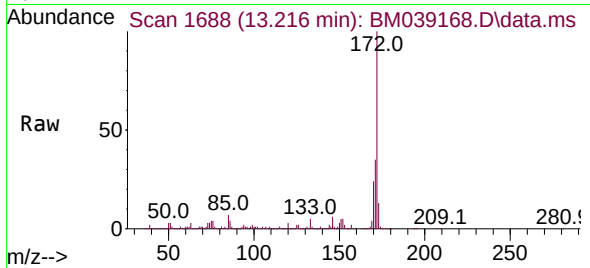

Tgt Ion:172 Resp: 2630289
Ion Ratio Lower Upper
172 100
171 34.8 28.2 42.2
170 23.5 19.1 28.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

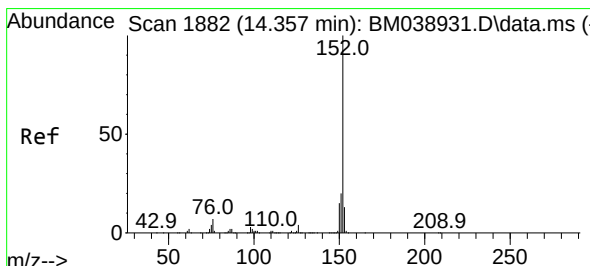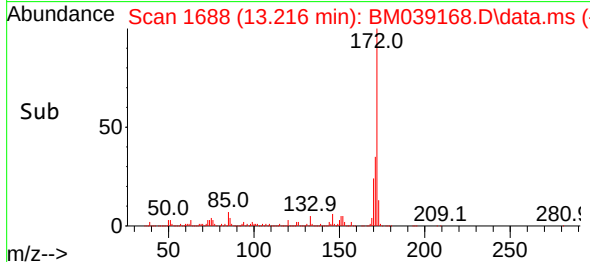

#49
Acenaphthylene
Concen: 2.680 ng
RT: 14.310 min Scan# 1874
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54


Tgt Ion:152 Resp: 168501
Ion Ratio Lower Upper
152 100
151 20.5 15.8 23.8
153 13.8 10.4 15.6

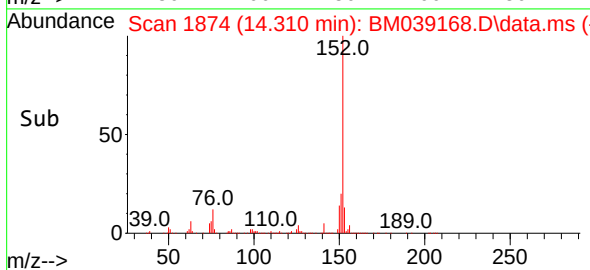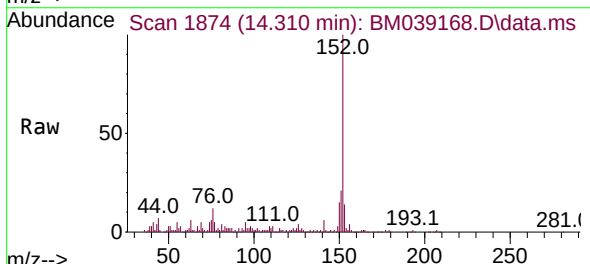

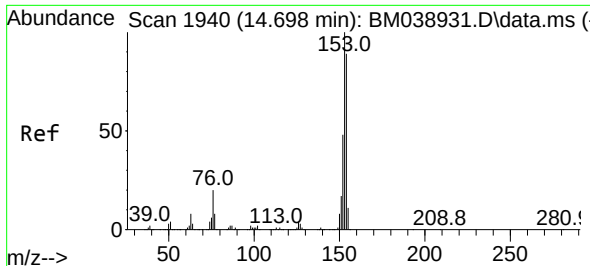

#52
Acenaphthene
Concen: 10.136 ng
RT: 14.651 min Scan# 1932
Delta R.T. -0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2

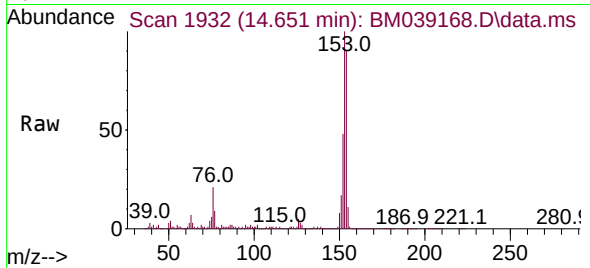


Tgt Ion:154 Resp: 391681
Ion Ratio Lower Upper
154 100
153 111.2 90.2 135.2
152 53.7 43.4 65.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

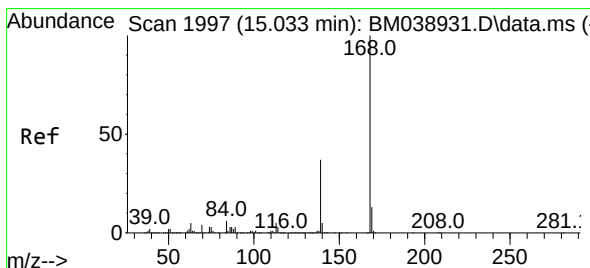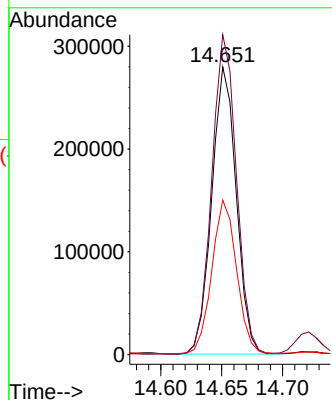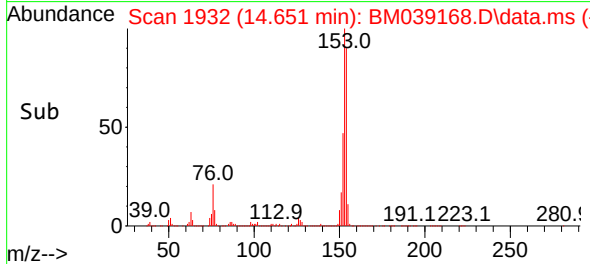


#55
Dibenzofuran
Concen: 4.787 ng
RT: 14.986 min Scan# 1989
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

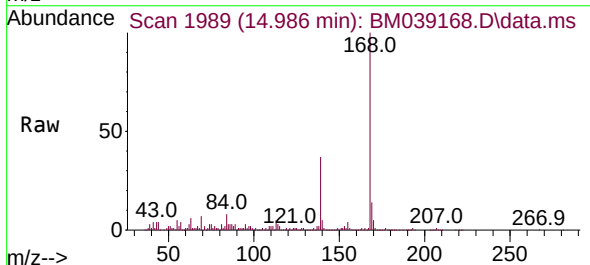


Tgt Ion:168 Resp: 289468
Ion Ratio Lower Upper
168 100
139 37.4 29.9 44.9
169 14.4 10.7 16.1

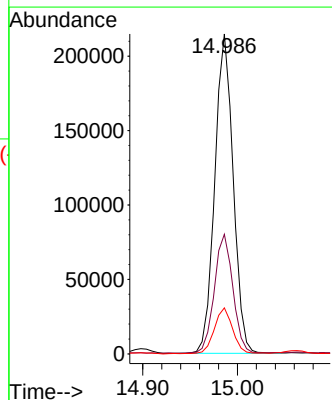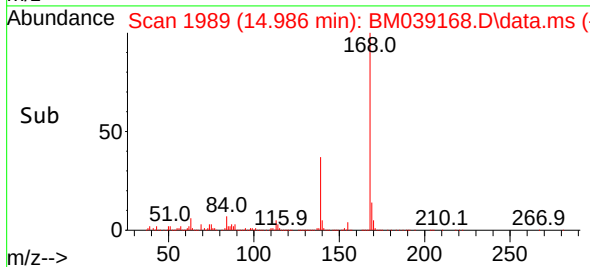

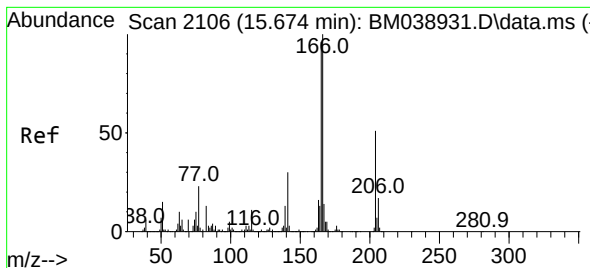

#58
Fluorene
Concen: 9.448 ng
RT: 15.633 min Scan# 2099
Delta R.T. -0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2

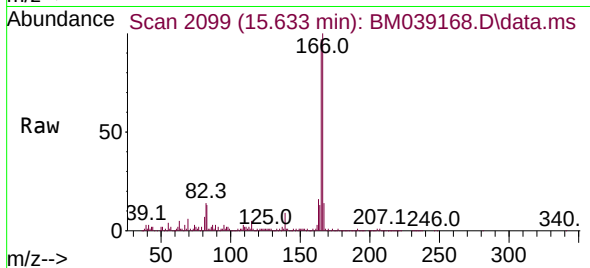


Tgt Ion:166 Resp: 447550
Ion Ratio Lower Upper
166 100
165 97.1 77.1 115.7
167 13.5 10.9 16.3

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

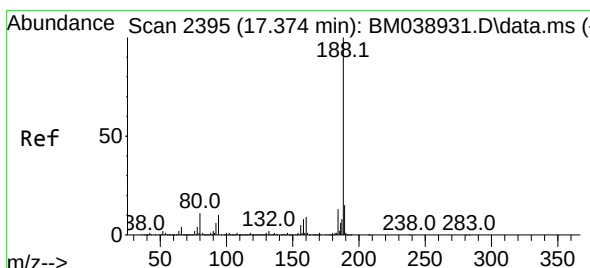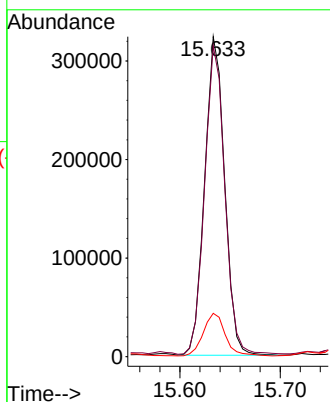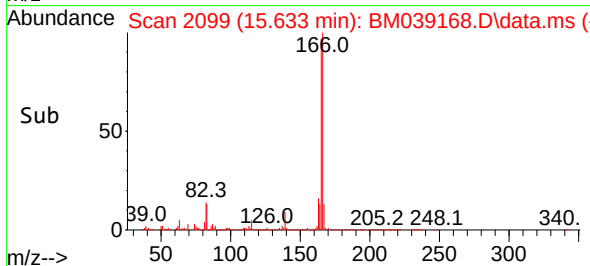


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.333 min Scan# 2388
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

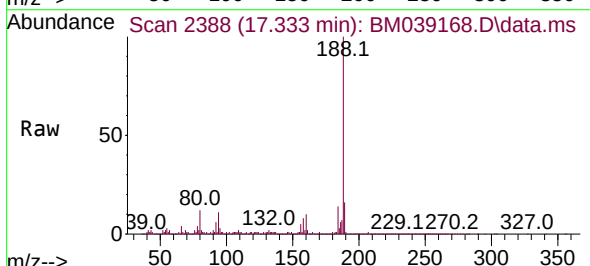


Tgt Ion:188 Resp: 1273672
Ion Ratio Lower Upper
188 100
94 10.8 7.9 11.9
80 11.7 8.5 12.7

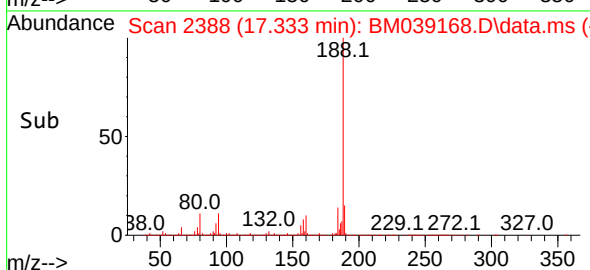



#71
Phenanthrene
Concen: 87.064 ng
RT: 17.380 min Scan# 2402
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2



Tgt Ion:178 Resp: 6508288
Ion Ratio Lower Upper
178 100
176 19.7 15.6 23.4
179 15.9 12.5 18.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023



#72
Anthracene
Concen: 24.478 ng
RT: 17.468 min Scan# 2411
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54


Tgt Ion:178 Resp: 1824774
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.7 12.5 18.7

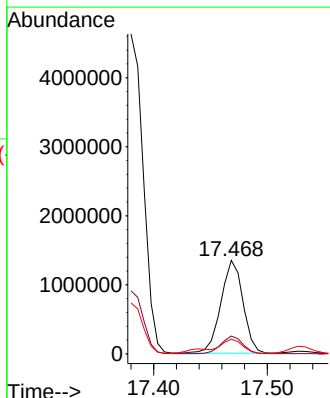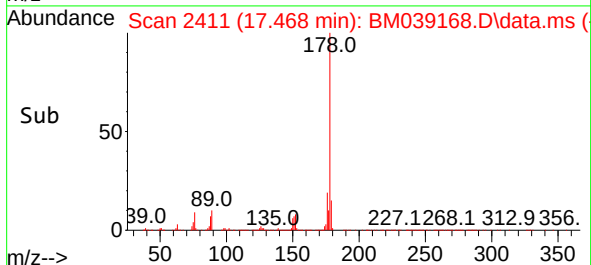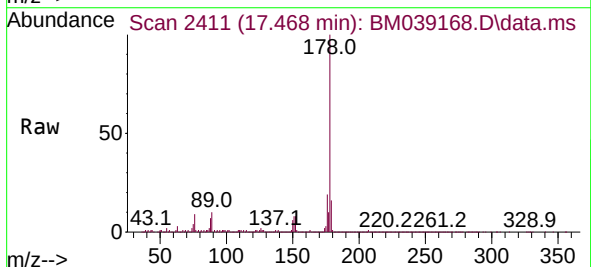



#73
 Carbazole
 Concen: 14.385 ng
 RT: 17.739 min Scan# 2464
 Delta R.T. -0.000 min
 Lab File: BM039168.D
 Acq: 27 Mar 2023 19:54




Instrument :
 BNA_M
 ClientSampleId :
 BROAD-CHANNEL-SUBSTATION-TP2

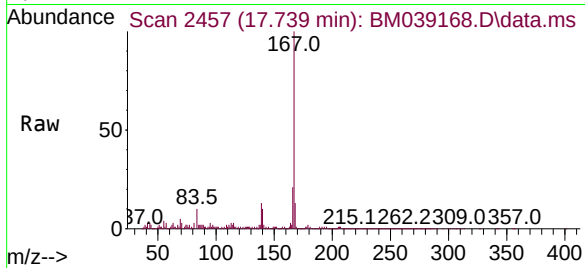


Tgt Ion:167 Resp: 97867
 Ion Ratio Lower Upper
 167 100
 166 21.2 17.0 25.4
 139 13.2 10.3 15.5

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 03/28/2023
 Supervised By :Jagrut Upadhyay 03/28/2023




#74
 Di-n-butylphthalate
 Concen: 2.071 ng
 RT: 18.304 min Scan# 2553
 Delta R.T. -0.000 min
 Lab File: BM039168.D
 Acq: 27 Mar 2023 19:54

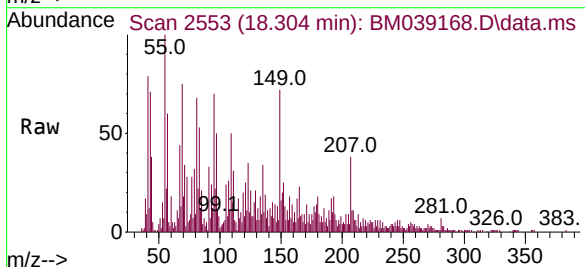


Tgt Ion:149 Resp: 23457
 Ion Ratio Lower Upper
 149 100
 150 21.9 7.4 11.2#
 104 8.2 4.3 6.5#

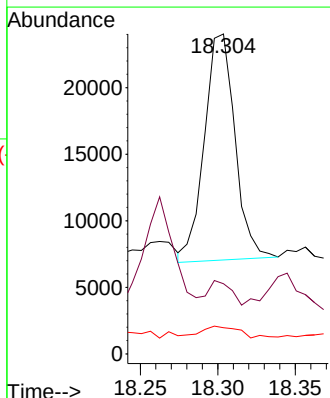



#75
Fluoranthene
Concen: 131.090 ng
RT: 19.398 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2



Tgt Ion:202 Resp:1034655
Ion Ratio Lower Upper
202 100
101 12.8 0.0 31.7
203 18.7 0.0 37.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.521 min Scan# 3100
Delta R.T. 0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54


Tgt Ion:240 Resp: 1170599
Ion Ratio Lower Upper
240 100
120 11.7 9.2 13.8
236 26.5 20.8 31.2

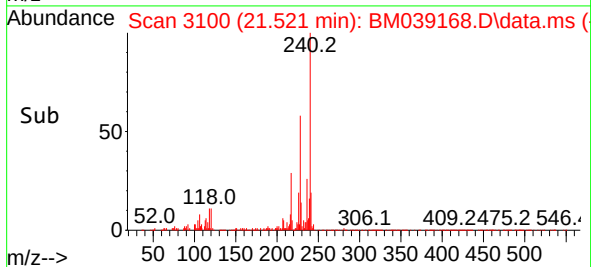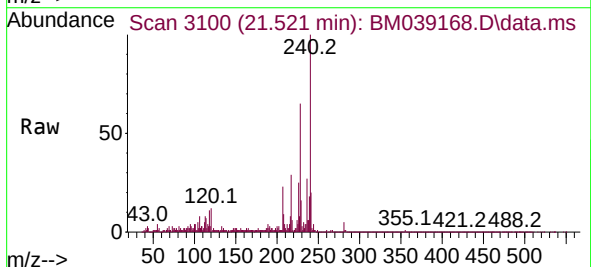



#78
Pyrene
Concen: 106.475 ng
RT: 19.762 min Scan# 2806
Delta R.T. 0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2




Tgt Ion:202 Resp: 9361489
Ion Ratio Lower Upper
202 100
200 21.8 17.1 25.7
203 18.6 14.1 21.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023




#79
Terphenyl-d14
Concen: 57.816 ng
RT: 19.956 min Scan# 2834
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54



Tgt Ion:244 Resp: 3701731
Ion Ratio Lower Upper
244 100
212 7.1 5.5 8.3
122 11.7 9.0 13.4

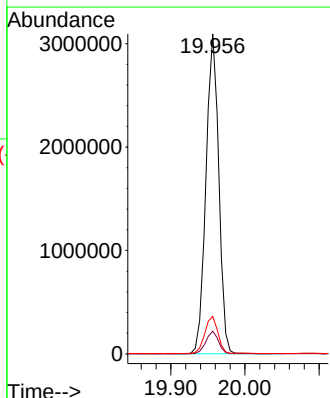



#81

Benzo(a)anthracene

Concen: 62.770 ng

RT: 21.503 min Scan# 30

Delta R.T. 0.006 min

Lab File: BM039168.D

Acq: 27 Mar 2023 19:54

Instrument :

BNA_M

ClientSampleId :

BROAD-CHANNEL-SUBSTATION-TP2

Tgt Ion:228 Resp: 529154

Ion Ratio Lower Upper

228 100

226 28.2 21.4 32.2





229 20.9 15.7 23.5

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 03/28/2023

Supervised By :Jagrut Upadhyay 03/28/2023

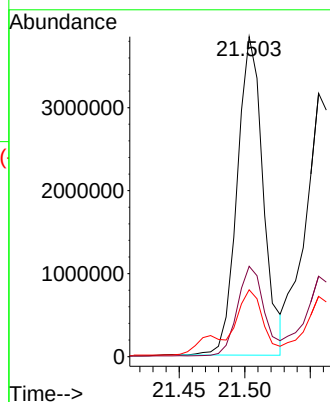

#83

Chrysene

Concen: 57.848 ng

RT: 21.556 min Scan# 3106

Delta R.T. 0.006 min

Lab File: BM039168.D

Acq: 27 Mar 2023 19:54




Tgt Ion:228 Resp: 4742903


Ion Ratio Lower Upper

228 100

226 30.5 24.0 36.0

229 22.9 16.0 24.0

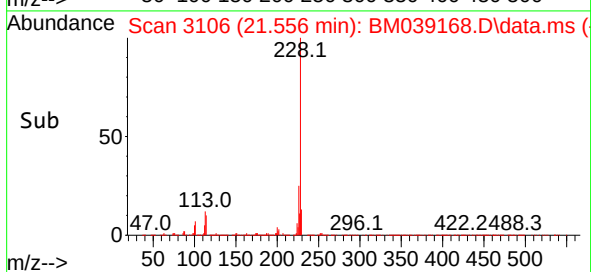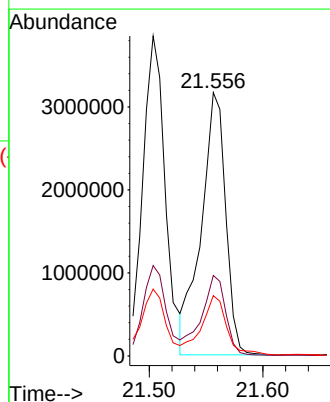







#84
Bis(2-ethylhexyl)phthalate
Concen: 4.119 ng
RT: 21.421 min Scan# 3091
Delta R.T. -0.000 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2

Tgt Ion:149 Resp: 9315
Ion Ratio Lower Upper
149 100
167 27.5 22.3 33.5
279 5.1 3.2 4.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

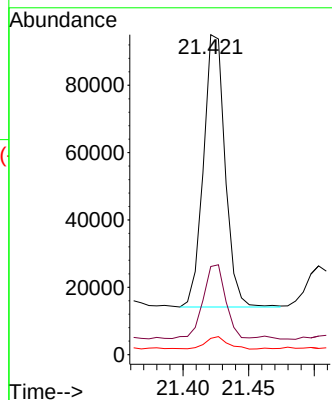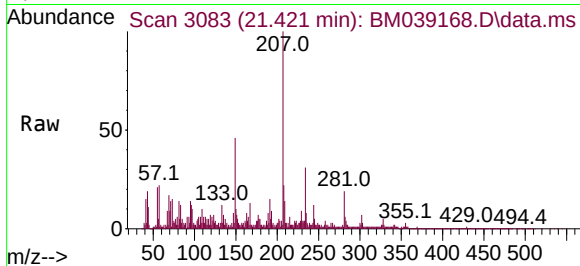

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.950 min Scan# 3513
Delta R.T. 0.012 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

Tgt Ion:264 Resp: 1367517
Ion Ratio Lower Upper
264 100
260 23.9 18.7 28.1
265 23.9 17.9 26.9

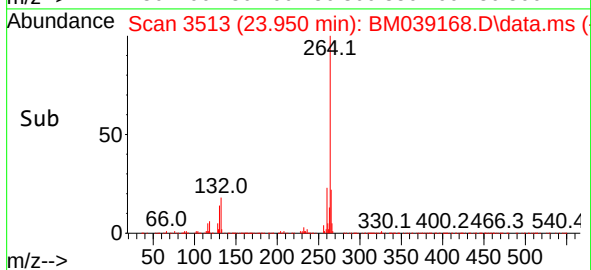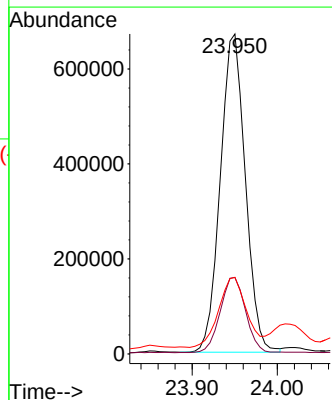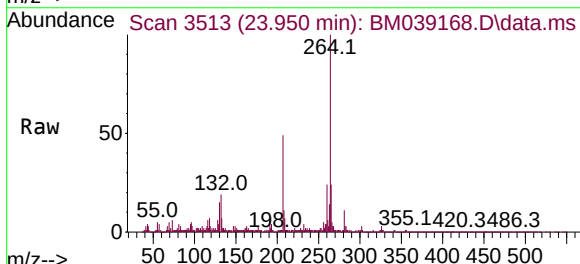







#87
Indeno(1,2,3-cd)pyrene
Concen: 34.045 ng
RT: 26.480 min Scan# 3957
Delta R.T. 0.012 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2

Tgt Ion:276 Resp: 3542650
Ion Ratio Lower Upper
276 100
138 23.7 22.1 33.1
277 24.9 20.1 30.1




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

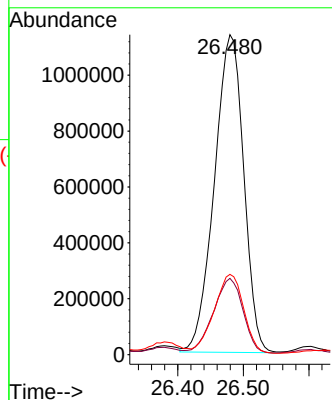

#88
Benzo(b)fluoranthene
Concen: 80.737 ng
RT: 23.215 min Scan# 3388
Delta R.T. 0.018 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54


Tgt Ion:252 Resp: 7053673
Ion Ratio Lower Upper
252 100
253 23.0 17.6 26.4
125 11.9 8.8 13.2

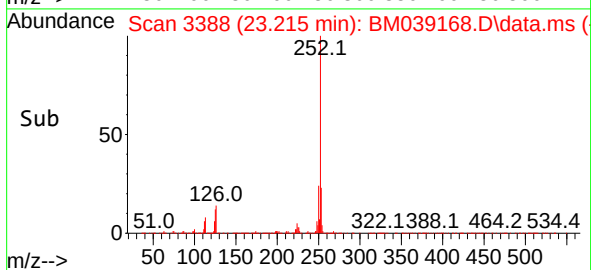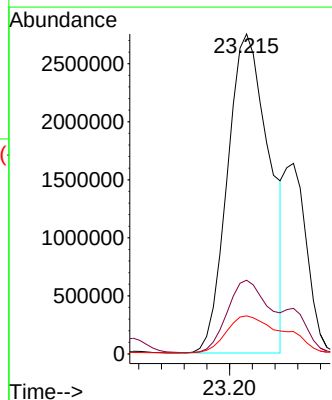



#89
Benzo(k)fluoranthene
Concen: 24.104 ng m
RT: 23.256 min Scan# 3403
Delta R.T. 0.006 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54




Instrument :
BNA_M
ClientSampleId :
BROAD-CHANNEL-SUBSTATION-TP2



Tgt Ion:252 Resp: 2191550
Ion Ratio Lower Upper
252 100
253 23.9 17.5 26.3
125 11.7 8.9 13.3




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/28/2023
Supervised By :Jagrut Upadhyay 03/28/2023

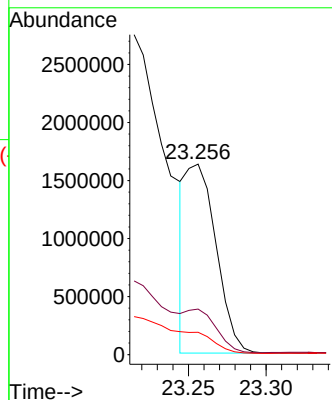

#90
Benzo(a)pyrene
Concen: 59.201 ng
RT: 23.844 min Scan# 3495
Delta R.T. 0.012 min
Lab File: BM039168.D
Acq: 27 Mar 2023 19:54

Tgt Ion:252 Resp: 4977765
Ion Ratio Lower Upper
252 100
253 23.2 17.6 26.4
125 12.2 9.8 14.8

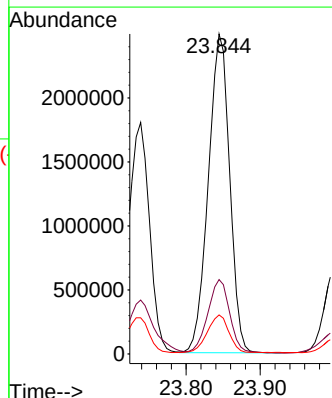



#91

Dibenzo(a,h)anthracene

Concen: 10.406 ng

RT: 26.485 min Scan# 39

Delta R.T. 0.006 min

Lab File: BM039168.D

Acq: 27 Mar 2023 19:54

Instrument :

BNM

ClientSampleId :

BROAD-CHANNEL-SUBSTATION-TP2

Tgt Ion:278 Resp: 916980

Ion Ratio Lower Upper

278 100

139 0.0 13.7 20.5





279 25.0 18.9 28.3

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 03/28/2023

Supervised By :Jagrut Upadhyay 03/28/2023

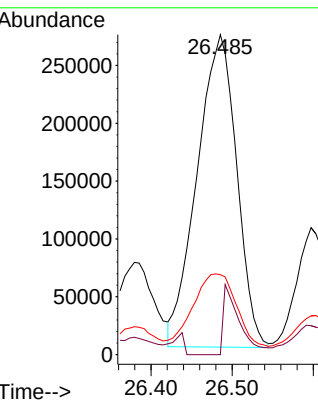

#92

Benzo(g,h,i)perylene

Concen: 41.775 ng

RT: 27.268 min Scan# 4077

Delta R.T. 0.023 min

Lab File: BM039168.D

Acq: 27 Mar 2023 19:54

Tgt Ion:276 Resp: 3601697

Ion Ratio Lower Upper

276 100

277 24.4 19.3 28.9

138 23.7 19.0 28.6

