

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
 Data File : BM039160.D
 Acq On : 27 Mar 2023 14:08
 Operator : CG/JU
 Sample : PB151521BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151521BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	291	297	306	rVB	1536851	2038583	19.25%	3.647%
2	5.498	370	376	388	rBV	3597315	5229097	49.39%	9.354%
3	7.110	642	650	669	rBV	3336051	5183550	48.96%	9.273%
4	7.945	785	792	801	rVB	962175	1529296	14.44%	2.736%
5	9.116	982	991	1001	rBV	2896054	4880182	46.09%	8.730%
6	10.757	1263	1270	1279	rBV	1265100	2096074	19.80%	3.750%
7	13.216	1680	1688	1696	rBV	6498368	9733066	91.93%	17.412%
8	14.586	1914	1921	1934	rBV	1779828	2487078	23.49%	4.449%
9	16.074	2167	2174	2189	rBV	2760027	3941006	37.22%	7.050%
10	17.333	2381	2388	2398	rBV	1824517	2561525	24.19%	4.582%
11	18.227	2535	2540	2548	rBV	76042	157372	1.49%	0.282%
12	19.503	2753	2757	2763	rBV3	62578	119732	1.13%	0.214%
13	19.950	2828	2833	2843	rBV	8458999	10587729	100.00%	18.941%
14	21.509	3094	3098	3104	rBV	1958167	2586569	24.43%	4.627%
15	23.933	3505	3510	3521	rVB2	1386112	2769071	26.15%	4.954%




Sum of corrected areas: 55899930

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
Data File : BM039160.D
Acq On : 27 Mar 2023 14:08
Operator : CG/JU
Sample : PB151521BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151521BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

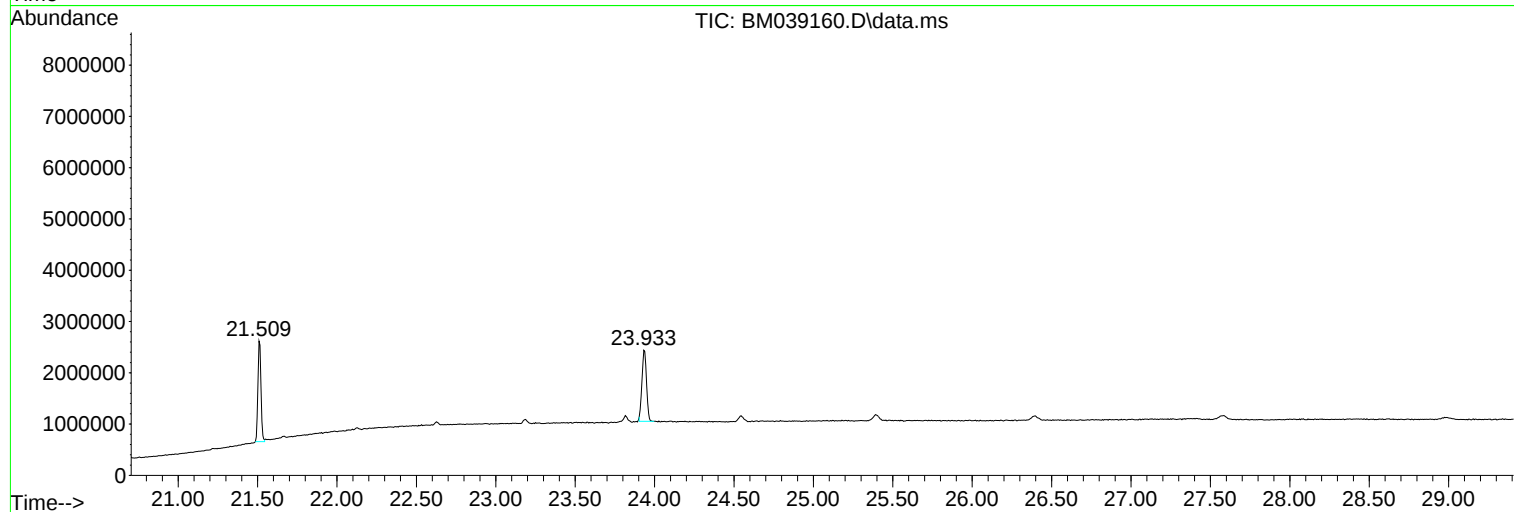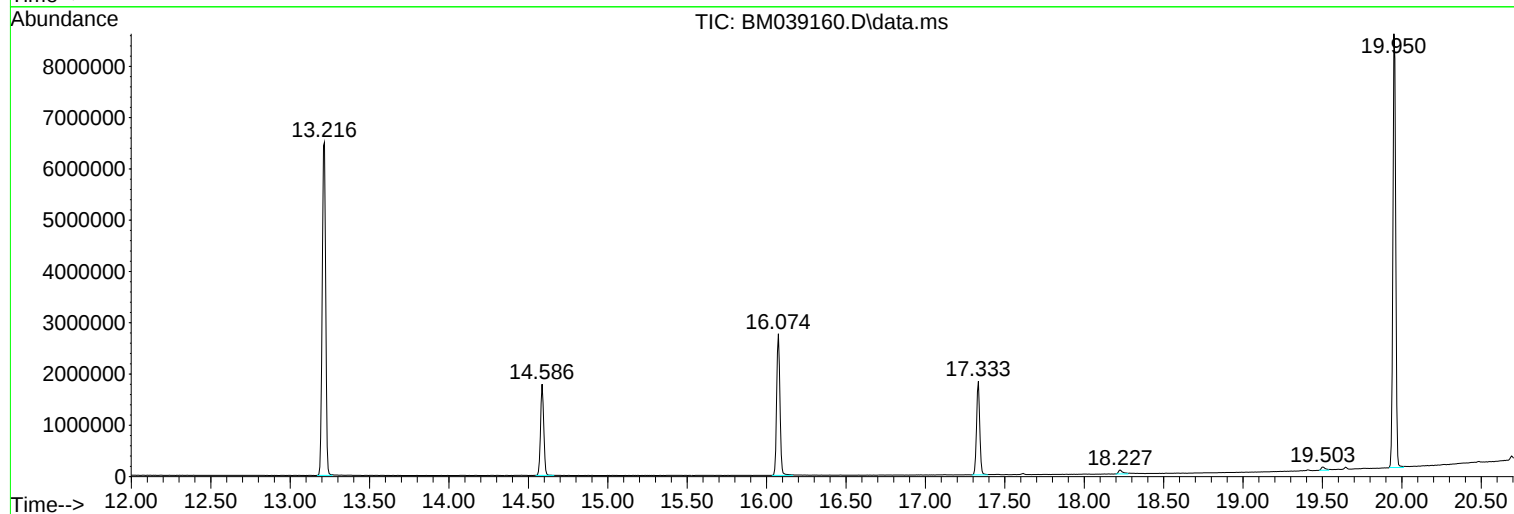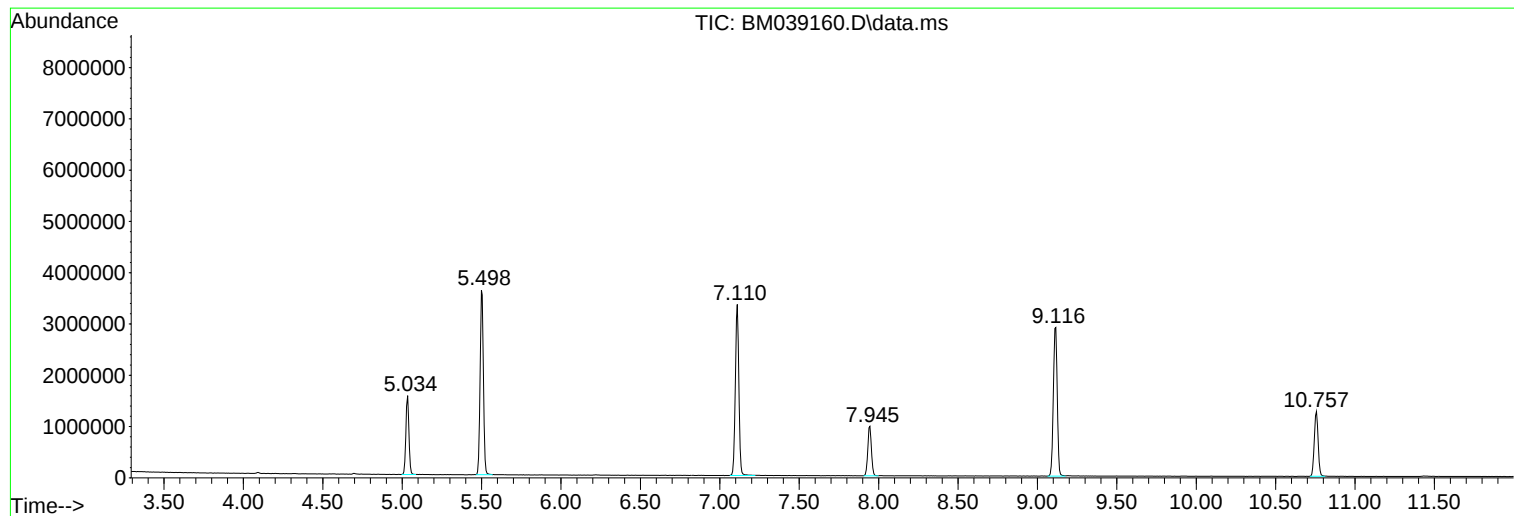

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
Data File : BM039160.D
Acq On : 27 Mar 2023 14:08
Operator : CG/JU
Sample : PB151521BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151521BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.034	26.66 ng	2038580	1,4-Dichlorobenzene-d4	7.945

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
3			5-Hexen-2-one	98	C6H10O	000109-49-9	9
4			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

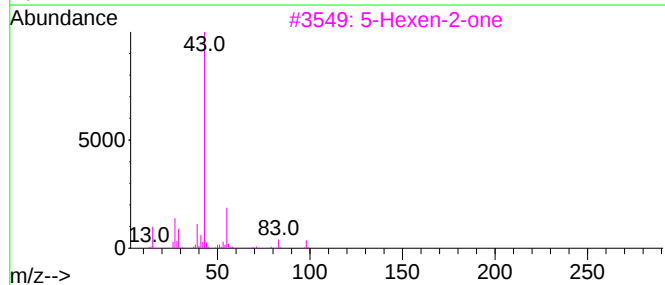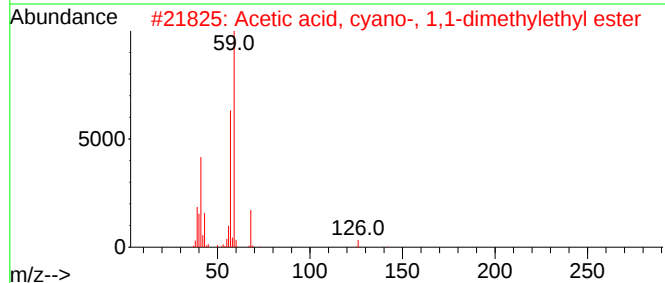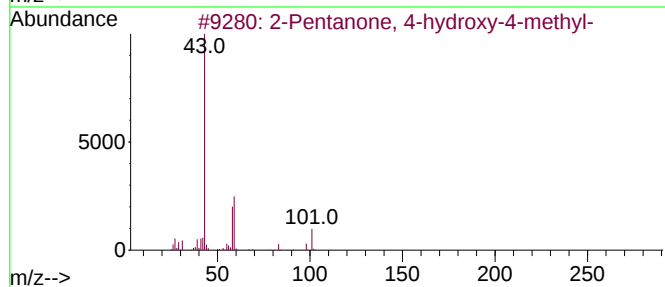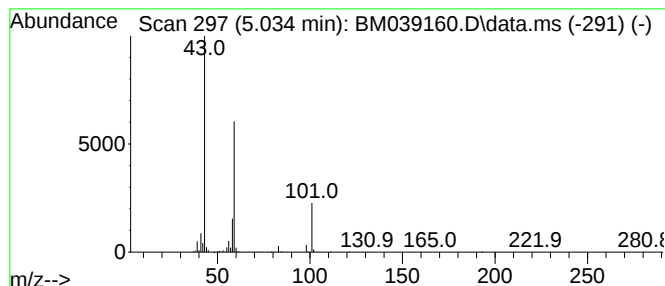

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
Data File : BM039160.D
Acq On : 27 Mar 2023 14:08
Operator : CG/JU
Sample : PB151521BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151521BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.034	26.7	ng	2038580	1	7.945	1529300	20.0