


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
 Data File : BM039155.D
 Acq On : 27 Mar 2023 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 28 01:46:09 2023

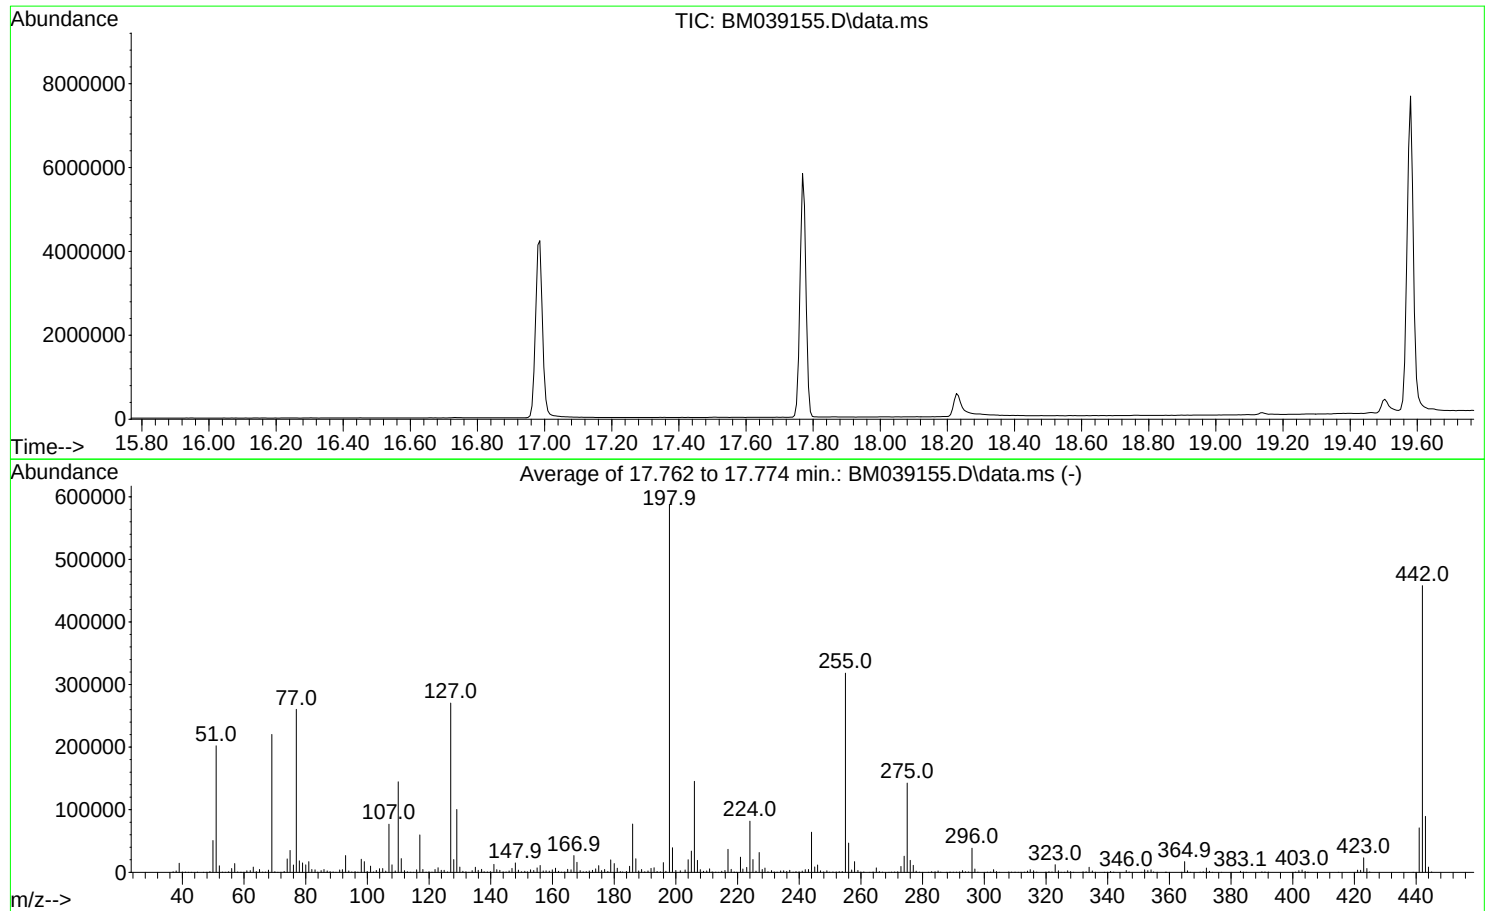




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	202065	PASS
68	69	0.00	2	1.6	3454	PASS
69	198	0.00	100	37.5	220235	PASS
70	69	0.00	2	0.5	1002	PASS
127	198	10	80	46.0	270357	PASS
197	198	0.00	2	0.3	1681	PASS
198	198	100	100	100.0	587819	PASS
199	198	5	9	6.7	39365	PASS
275	198	10	60	24.3	142643	PASS
365	198	1	100	2.9	17005	PASS
441	198	0.01	100	12.1	70971	PASS
442	442	50	100	100.0	458005	PASS
443	442	15	24	19.5	89475	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
 Data File : BM039155.D
 Acq On : 27 Mar 2023 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 28 04:55:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 28 01:46:09 2023
 Response via : Initial Calibration

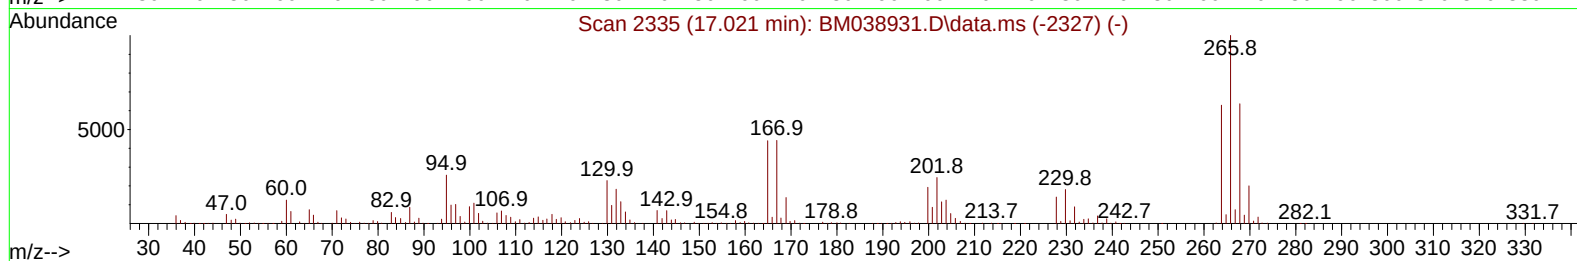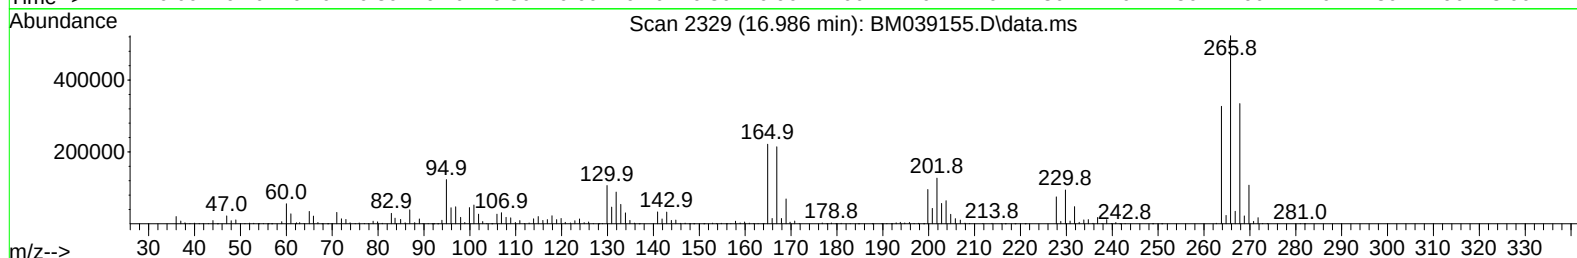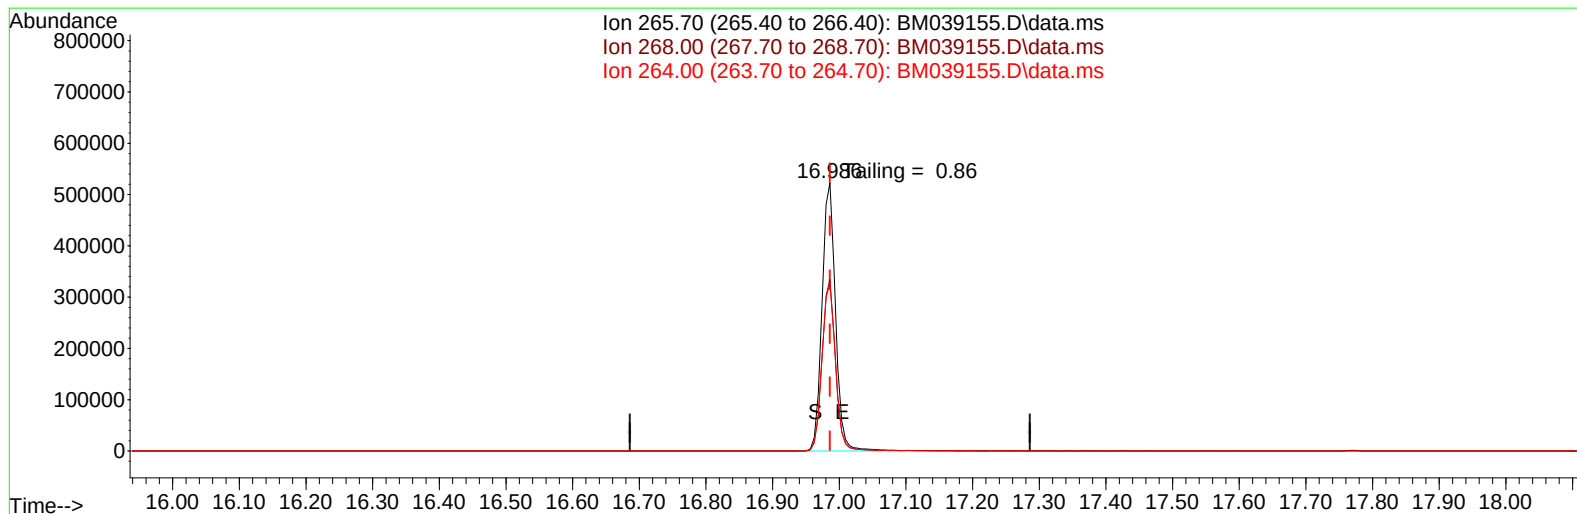

TIC: BM039155.D\data.ms

(70) Pentachlorophenol (C)

16.986min (-0.000) 453431.27 ng




response 736913

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.93
264.00	62.90	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032723\
Data File : BM039155.D
Acq On : 27 Mar 2023 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 28 04:55:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 01:46:09 2023
Response via : Initial Calibration

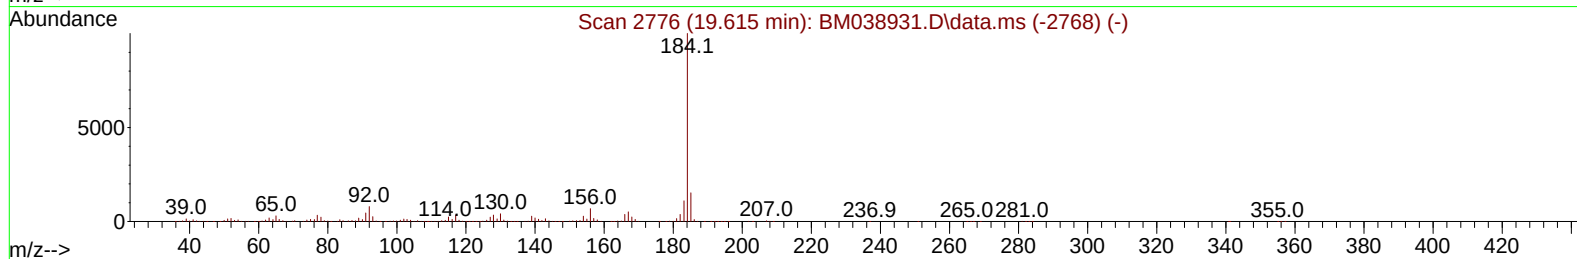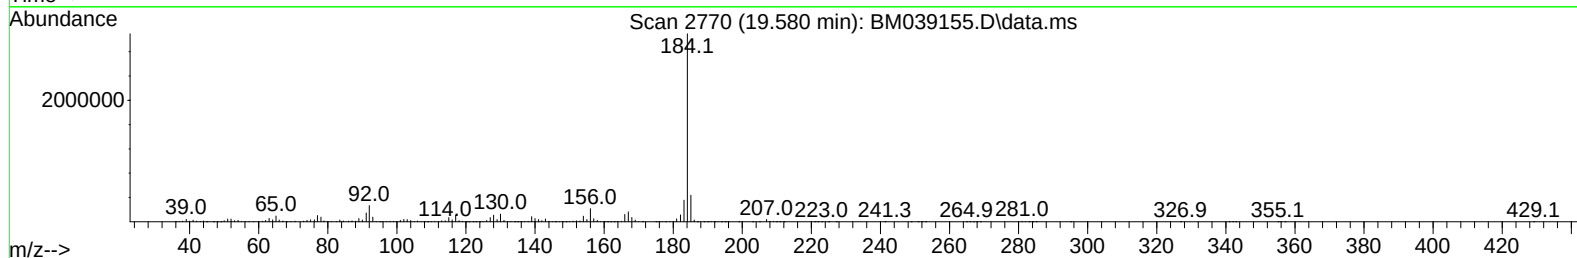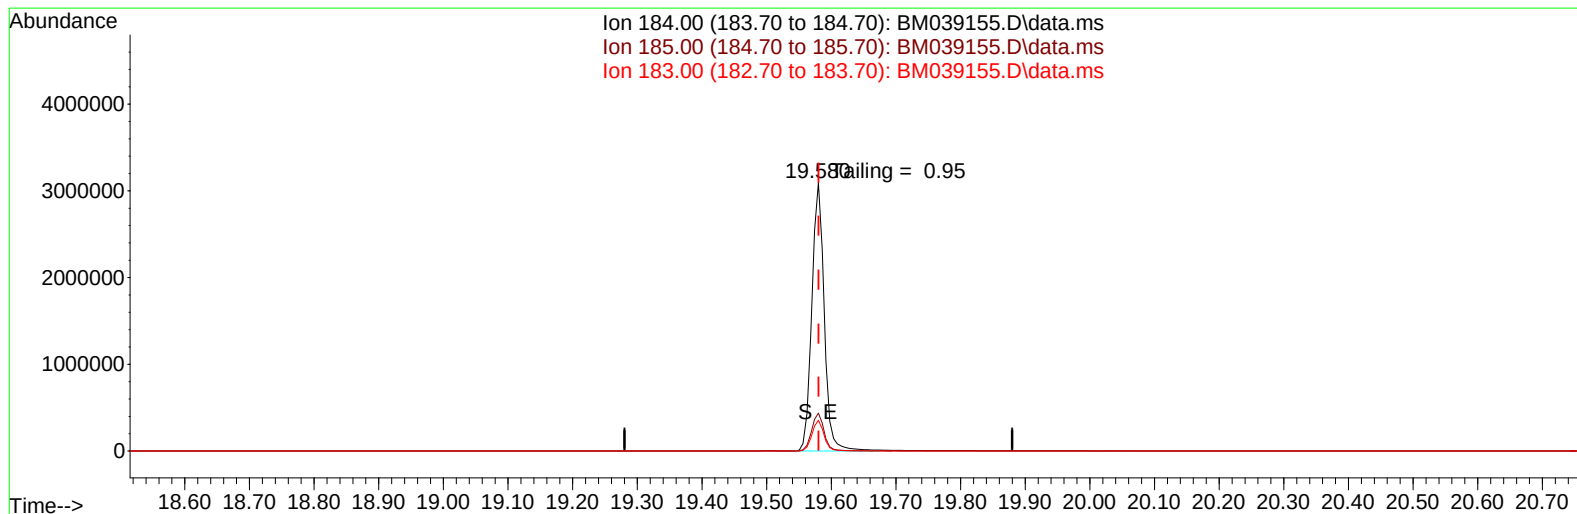

TIC: BM039155.D\data.ms

(77) Benzidine

19.580min (-0.000) 48147.24 ng

response 4162731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.15
183.00	11.00	11.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/27/2023	BNA_M	<u>BM039155.D</u>
Compound Name	Response	Retention Time
DDT	2005975	20.809
DDD	57355	20.368
DDE	1777	19.862
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
59132	2065107	2.86

Instrument :
BNA_M
ClientSampleId :
DFTPP