


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Apr 05 19:56:54 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4T41

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

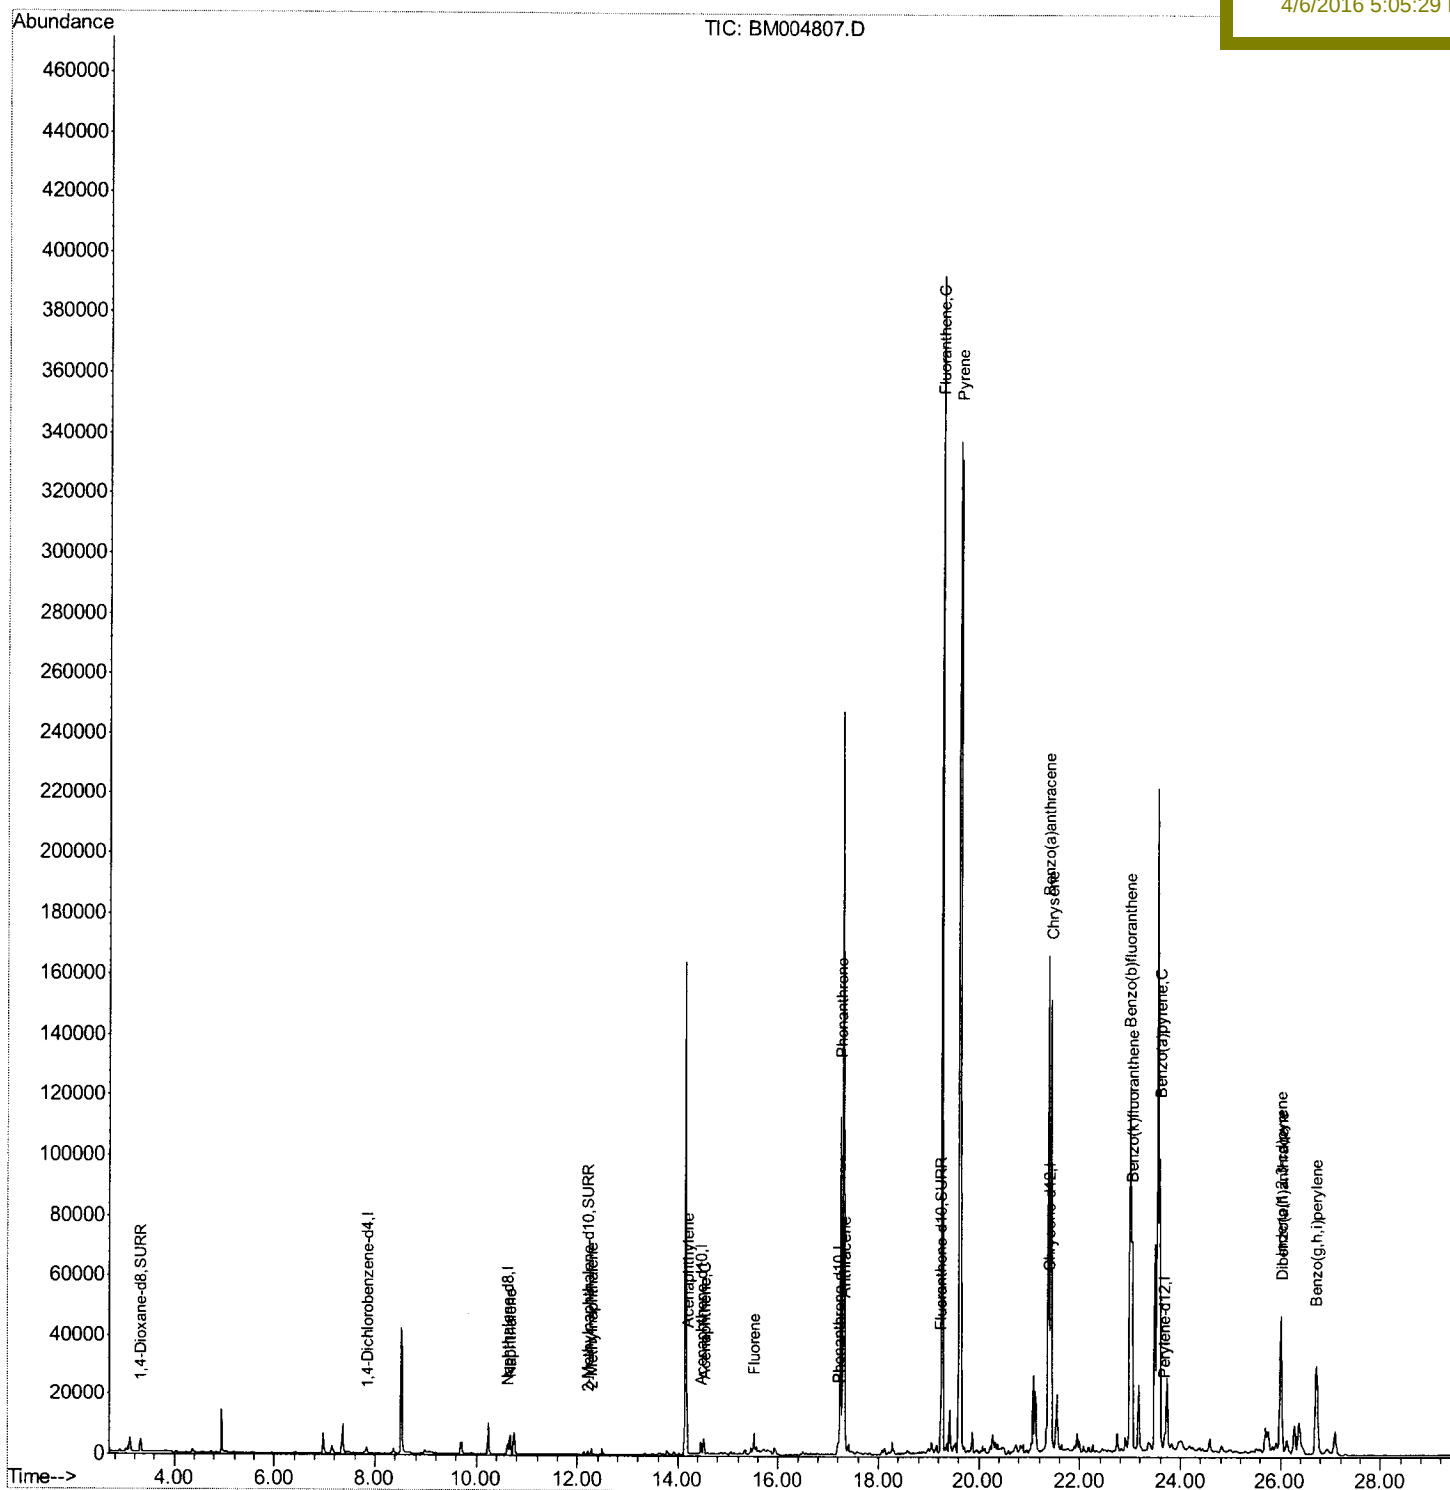

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Quant Time: Apr 05 19:50:06 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

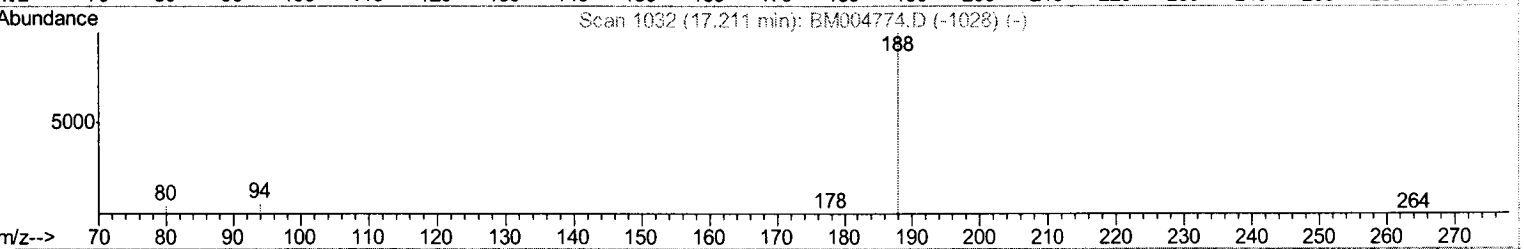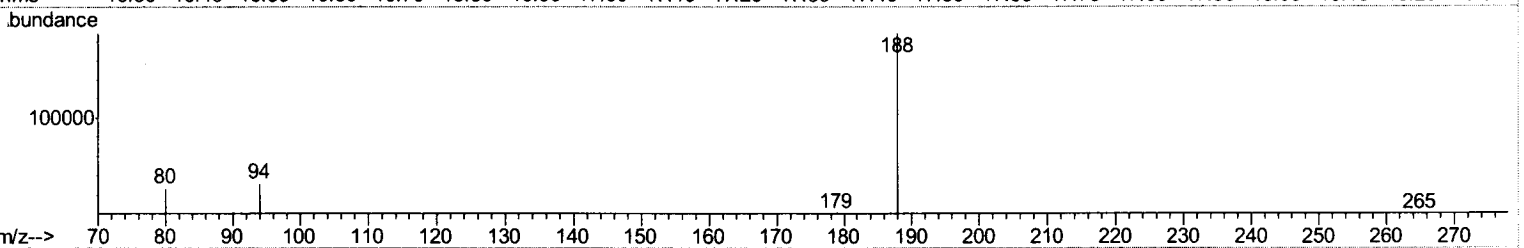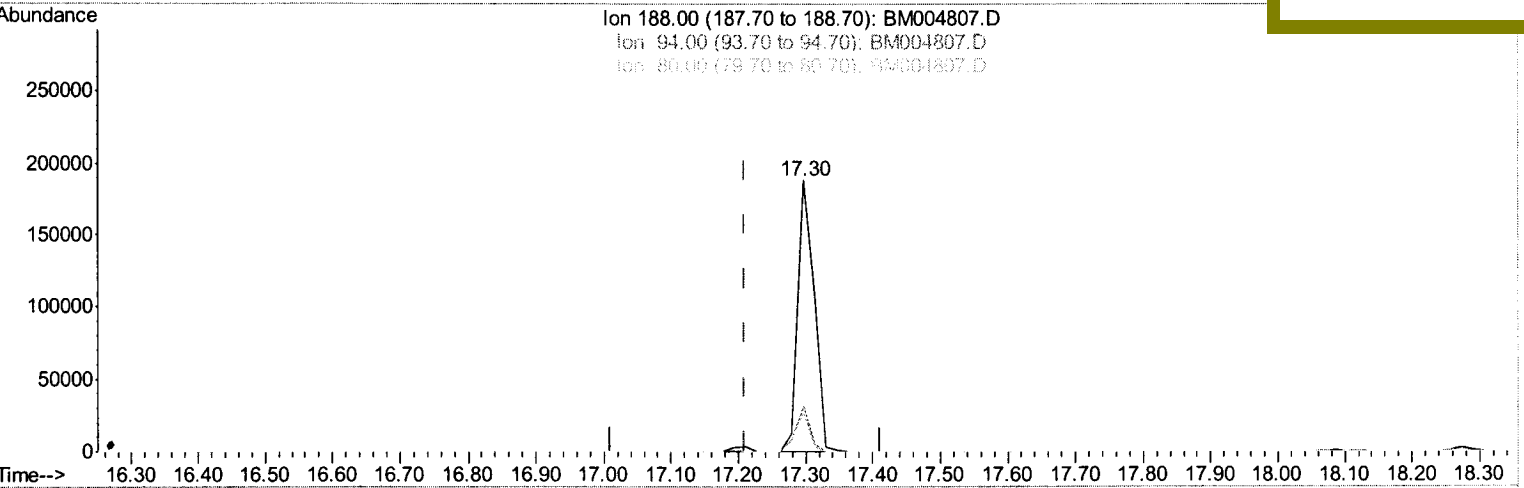

TIC: BM004807.D

(12) Phenanthrene-d10 (I)

17.296min (+0.085) 0.40ng/ul

response 320633

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	16.69#
80.00	11.90	14.03
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:50:06 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

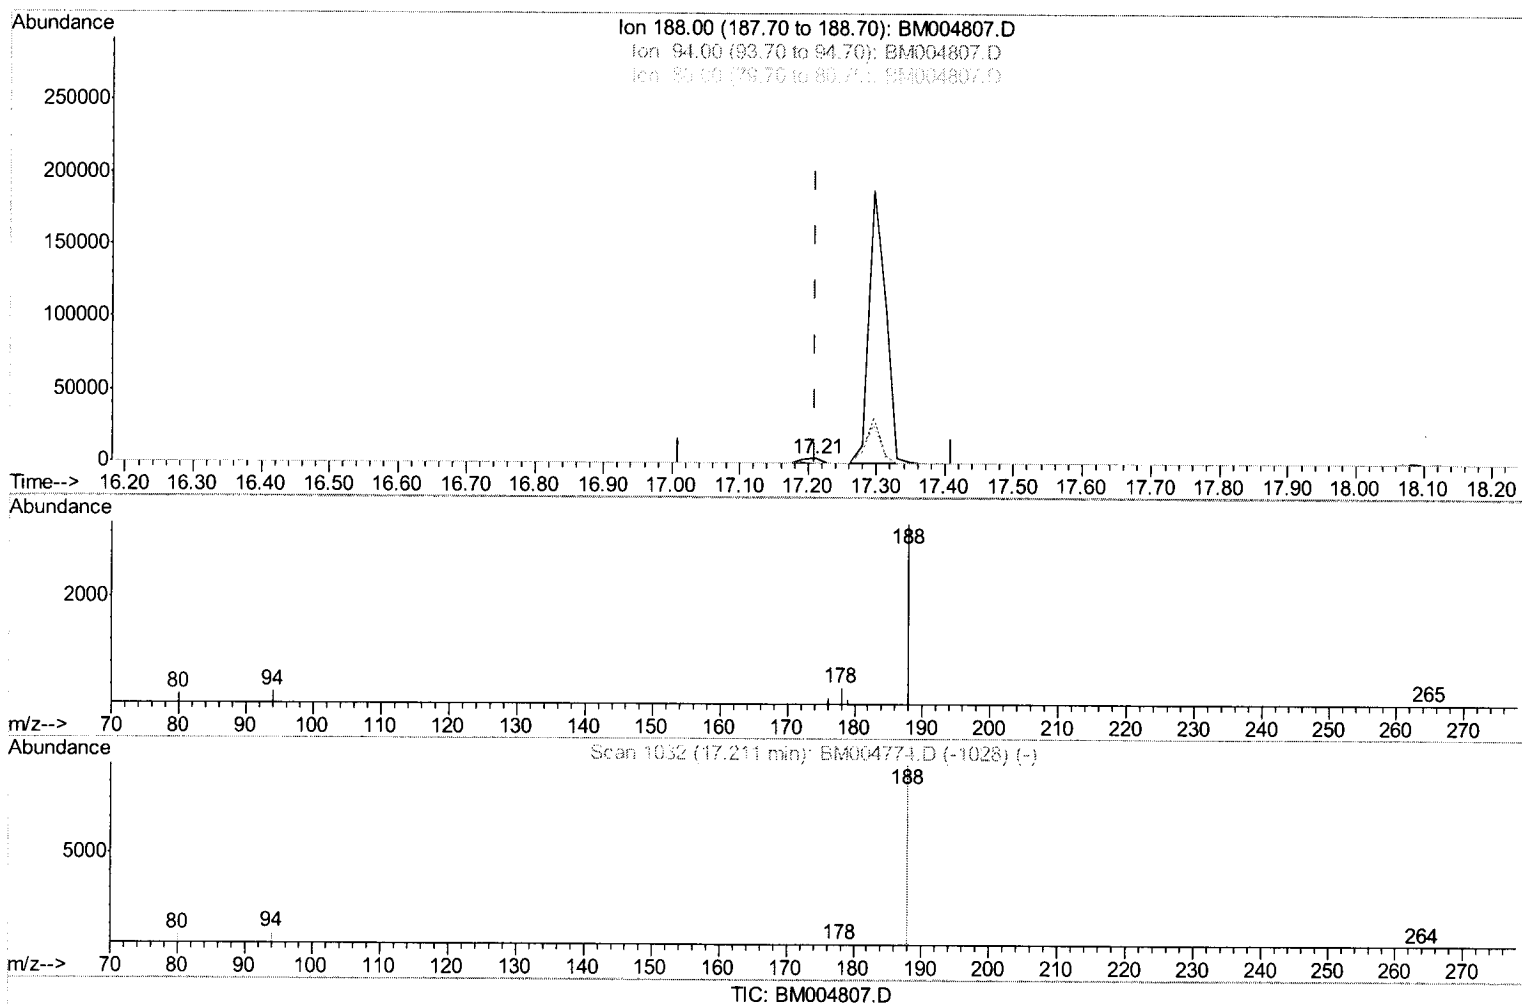

(12) Phenanthrene-d10 (I)

17.210min (-0.000) 0.40ng/ul m

response 6401

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.95#
80.00	11.90	6.80#
0.00	0.00	0.00

U.M
 04/07/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Apr 05 19:51:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4T41

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

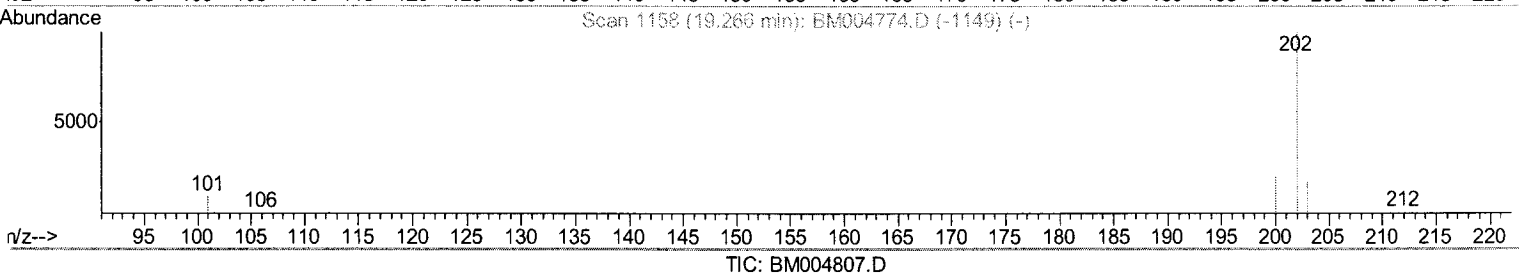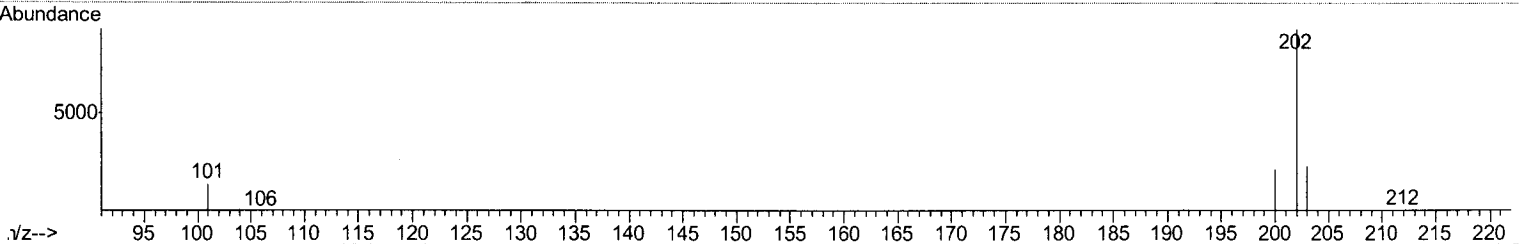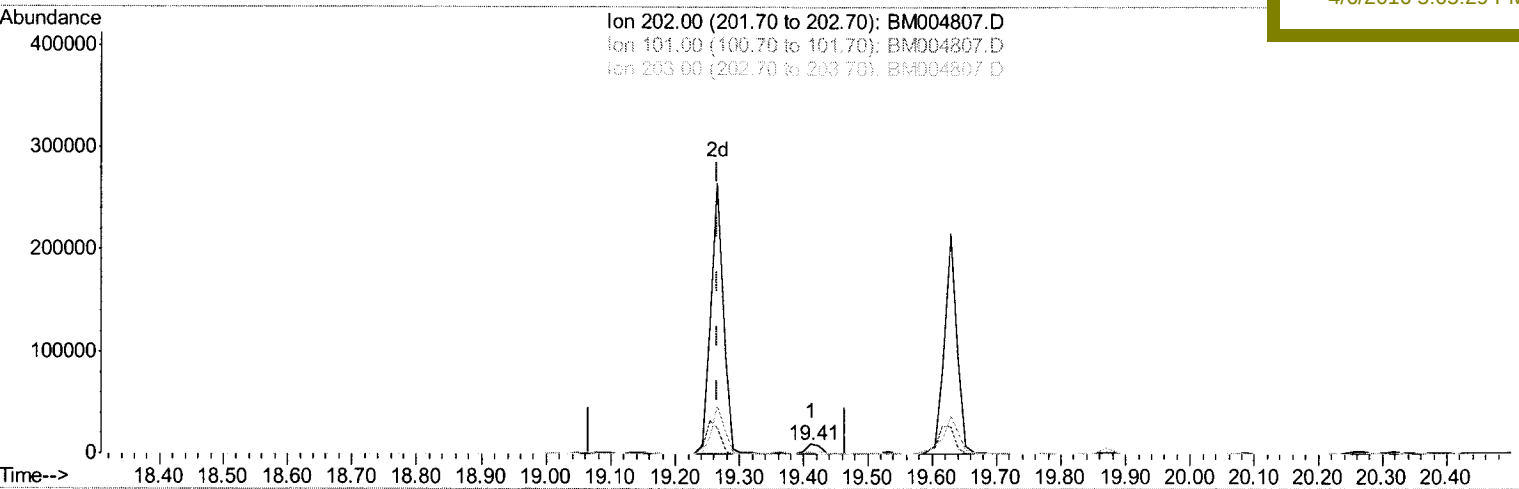

(17) Fluoranthene (C)

19.411min (+0.145) 0.70ng/ul

response 14332

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	15.50
203.00	16.30	25.66
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

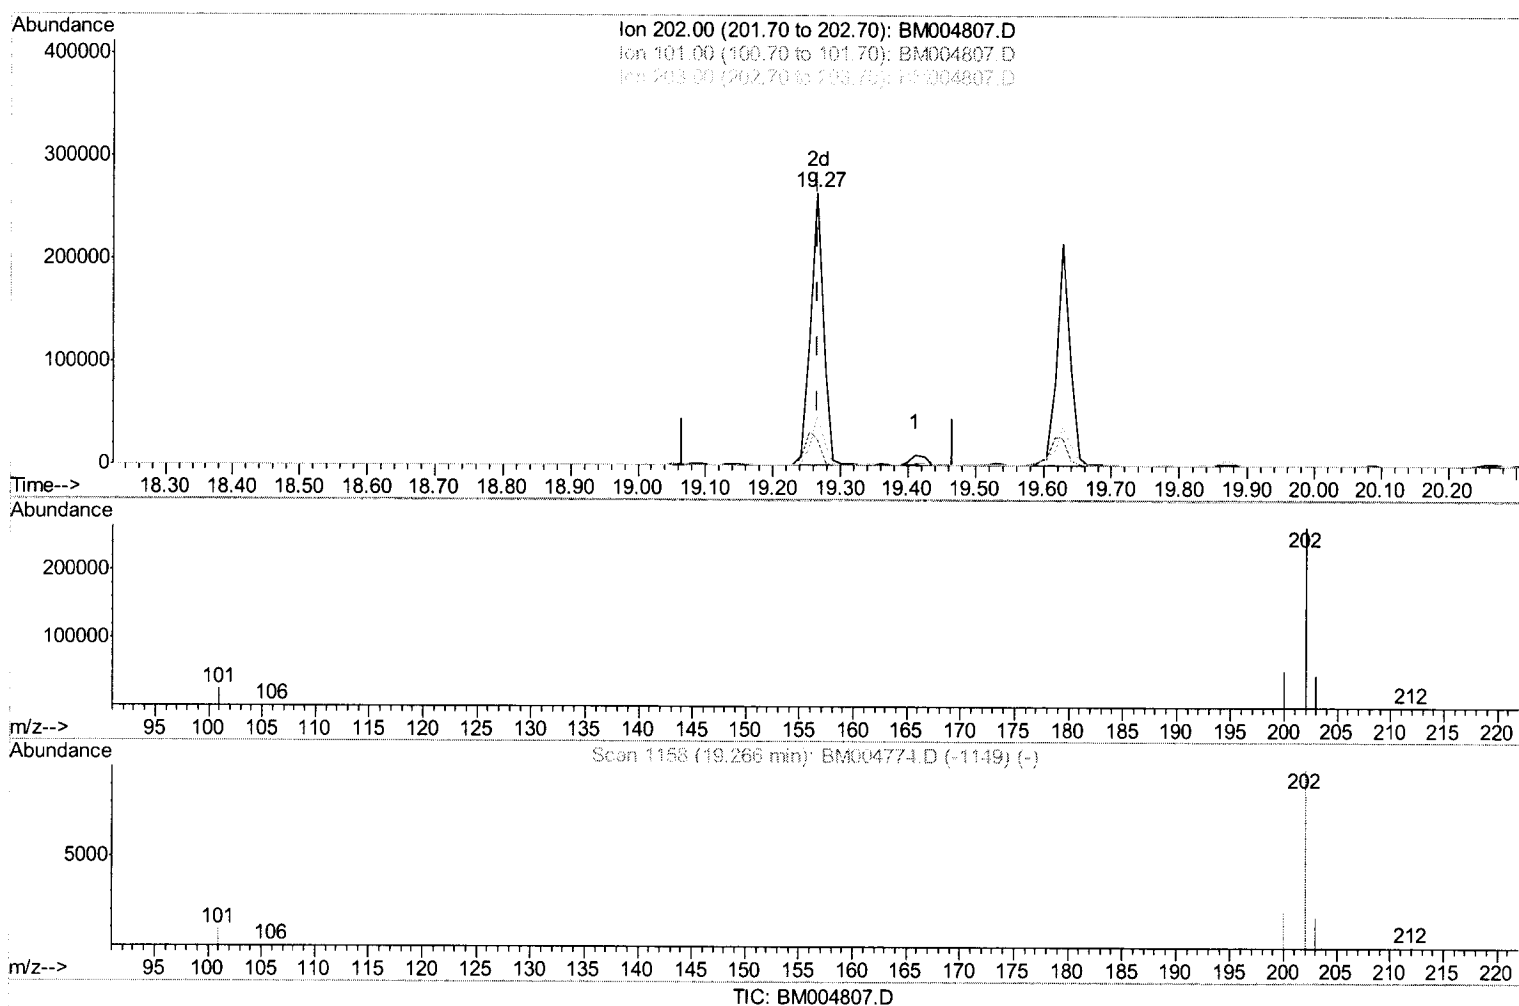

(17) Fluoranthene (C)

19.266min (-0.000) 17.57ng/ul m U.M

response 359692

04/07/16

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	9.62
203.00	16.30	17.80
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T41

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

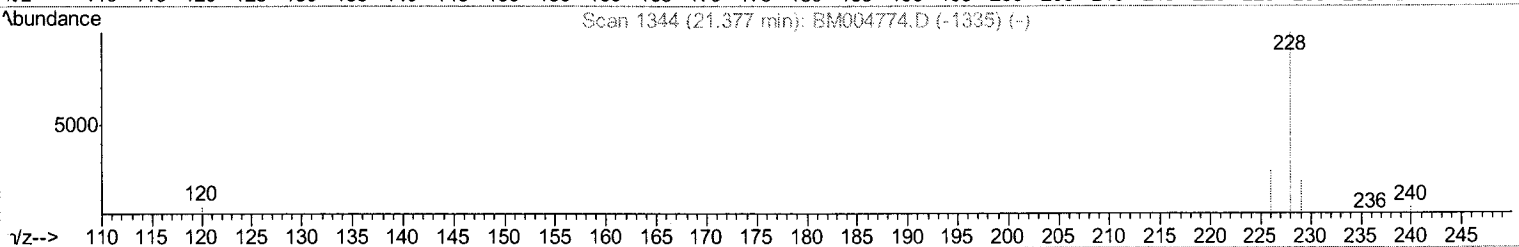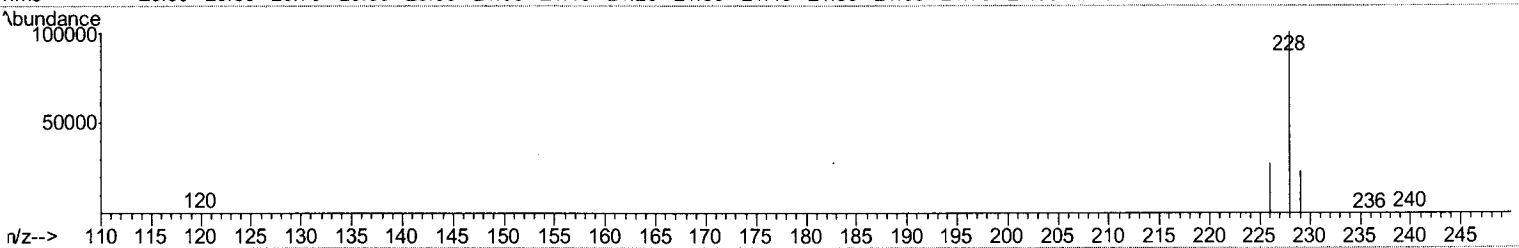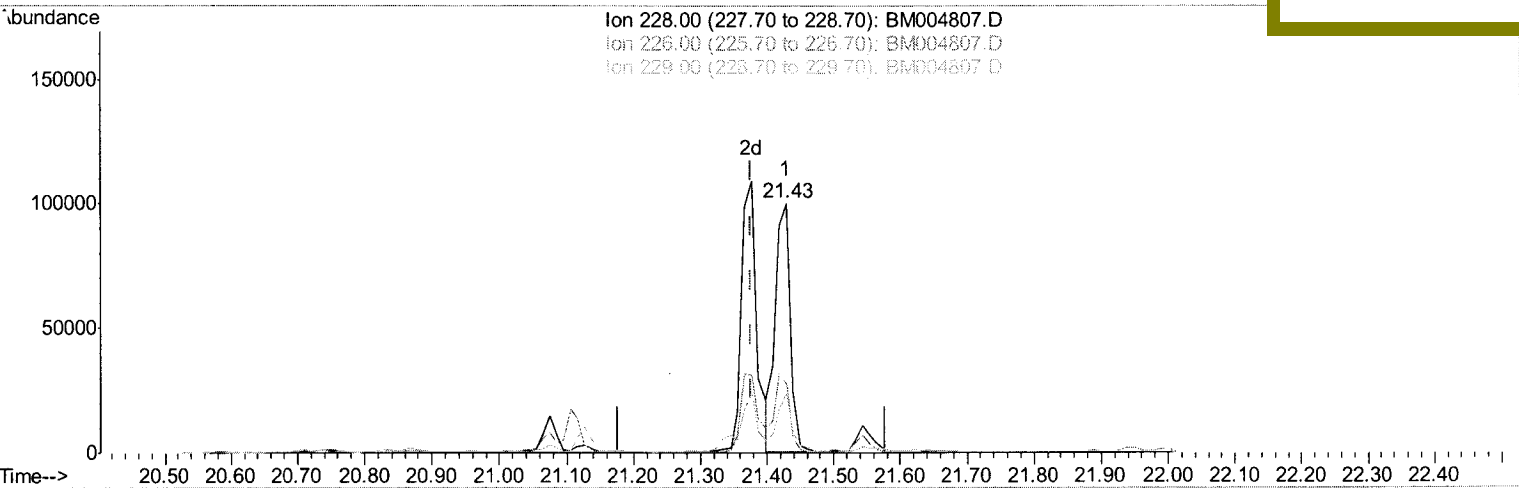

TIC: BM004807.D

(20) Benzo(a)anthracene

21.429min (+0.052) 7.87ng/ul

response 159269

Ion	Exp%	Act%
228.00	100	100
226.00	23.50	27.43
229.00	21.40	23.72
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

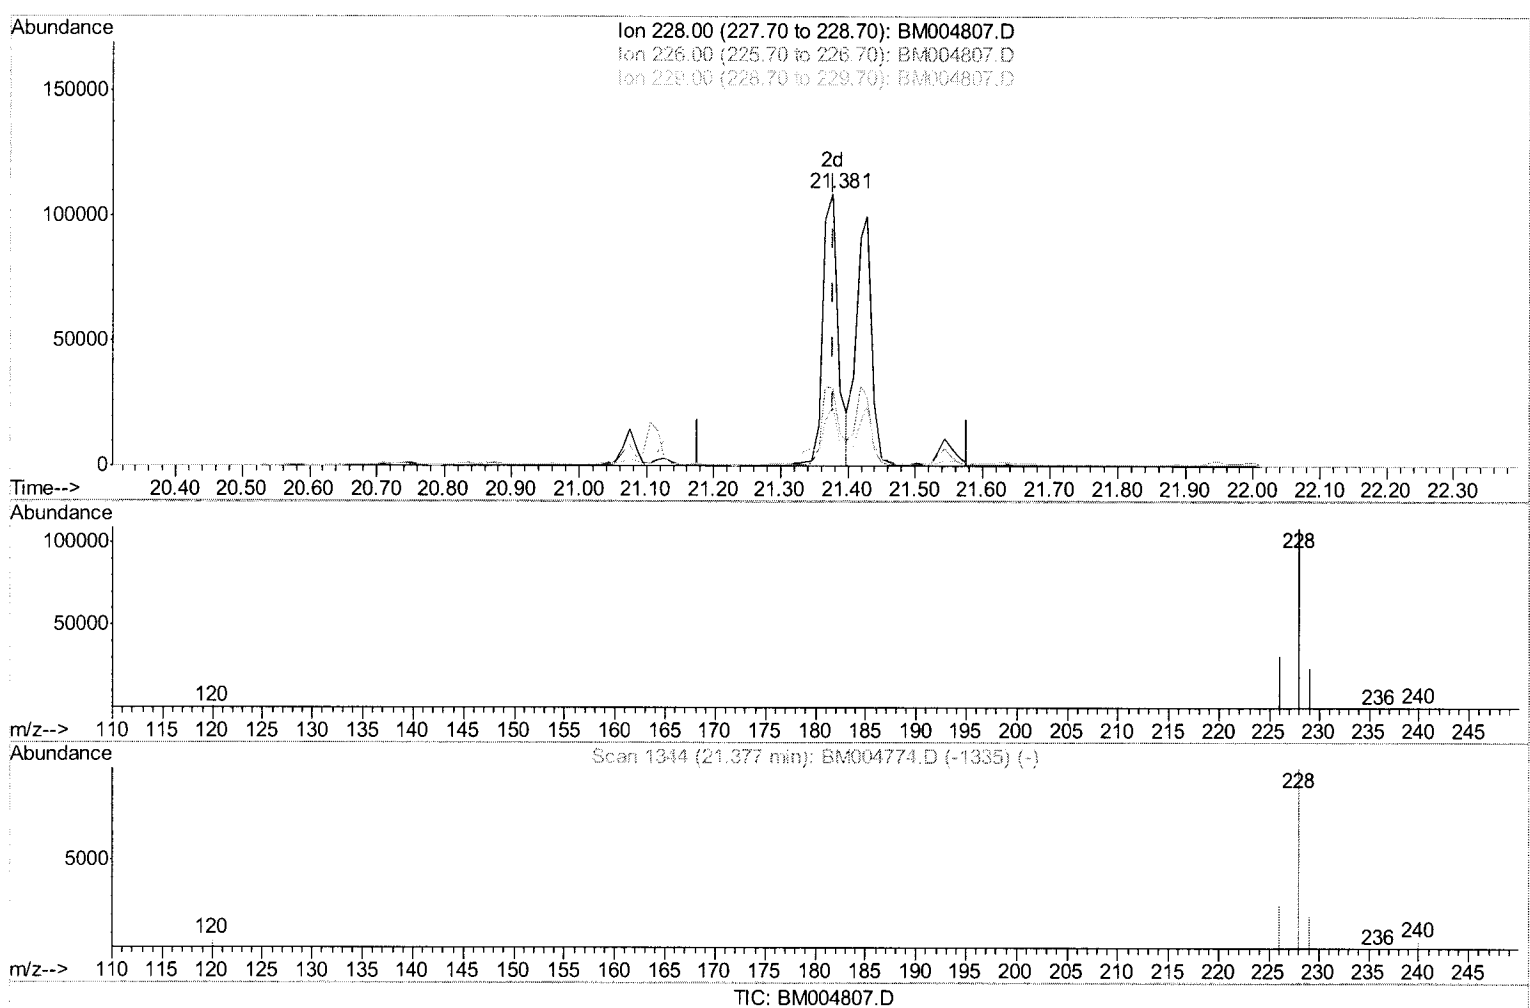

(20) Benzo(a)anthracene

21.377min (-0.000) 8.65ng/ul m

response 175128

Ion	Exp%	Act%
228.00	100	100
226.00	23.50	28.82#
229.00	21.40	22.20
0.00	0.00	0.00

U.M
 04/07/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T41

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

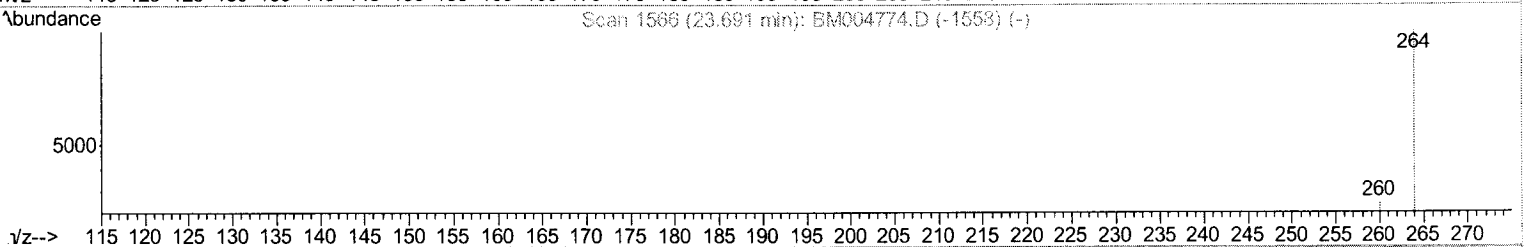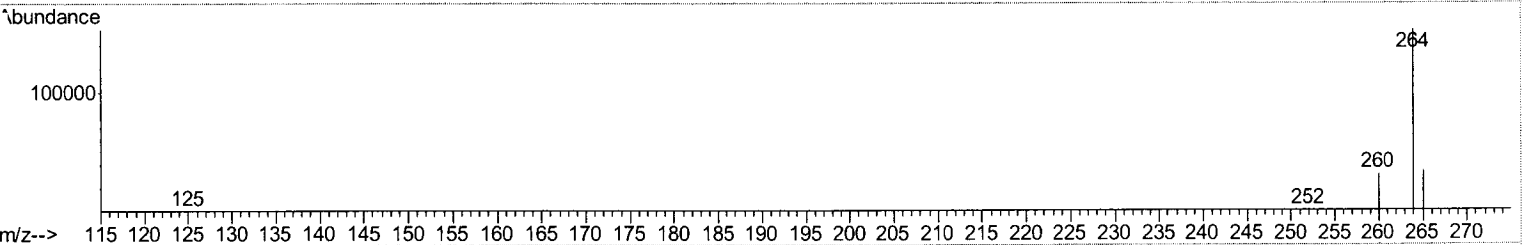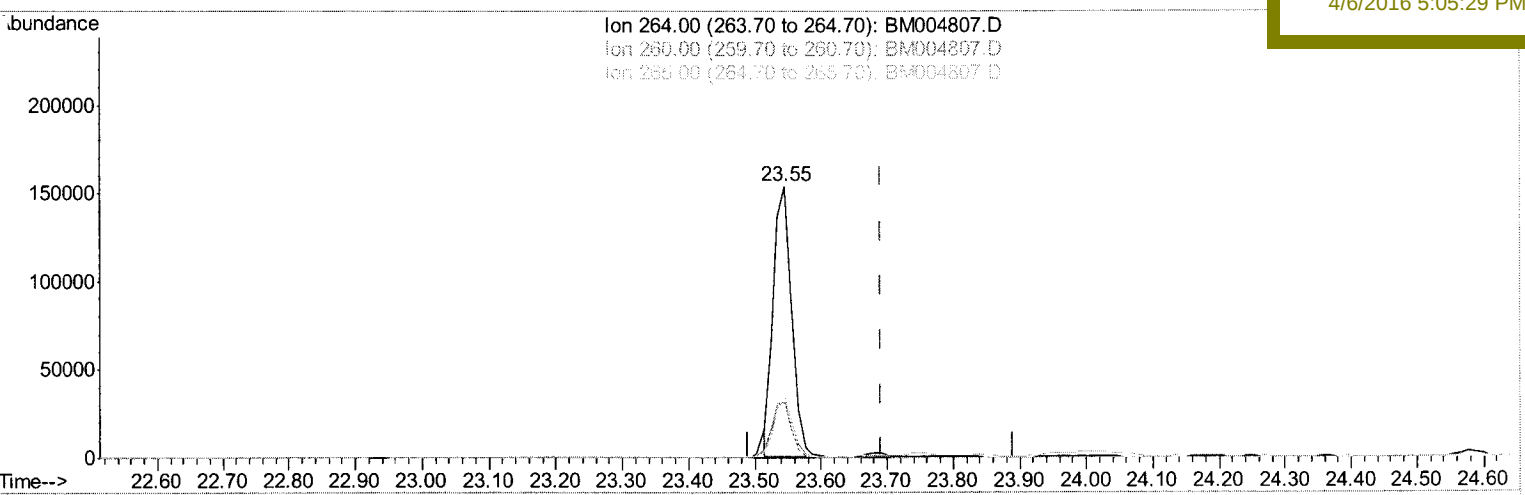

TIC: BM004807.D

(22) Perylene-d12 (I)

23.545min (-0.146) 0.40ng/ul

response 300248

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	20.37#
265.00	38.20	22.14#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

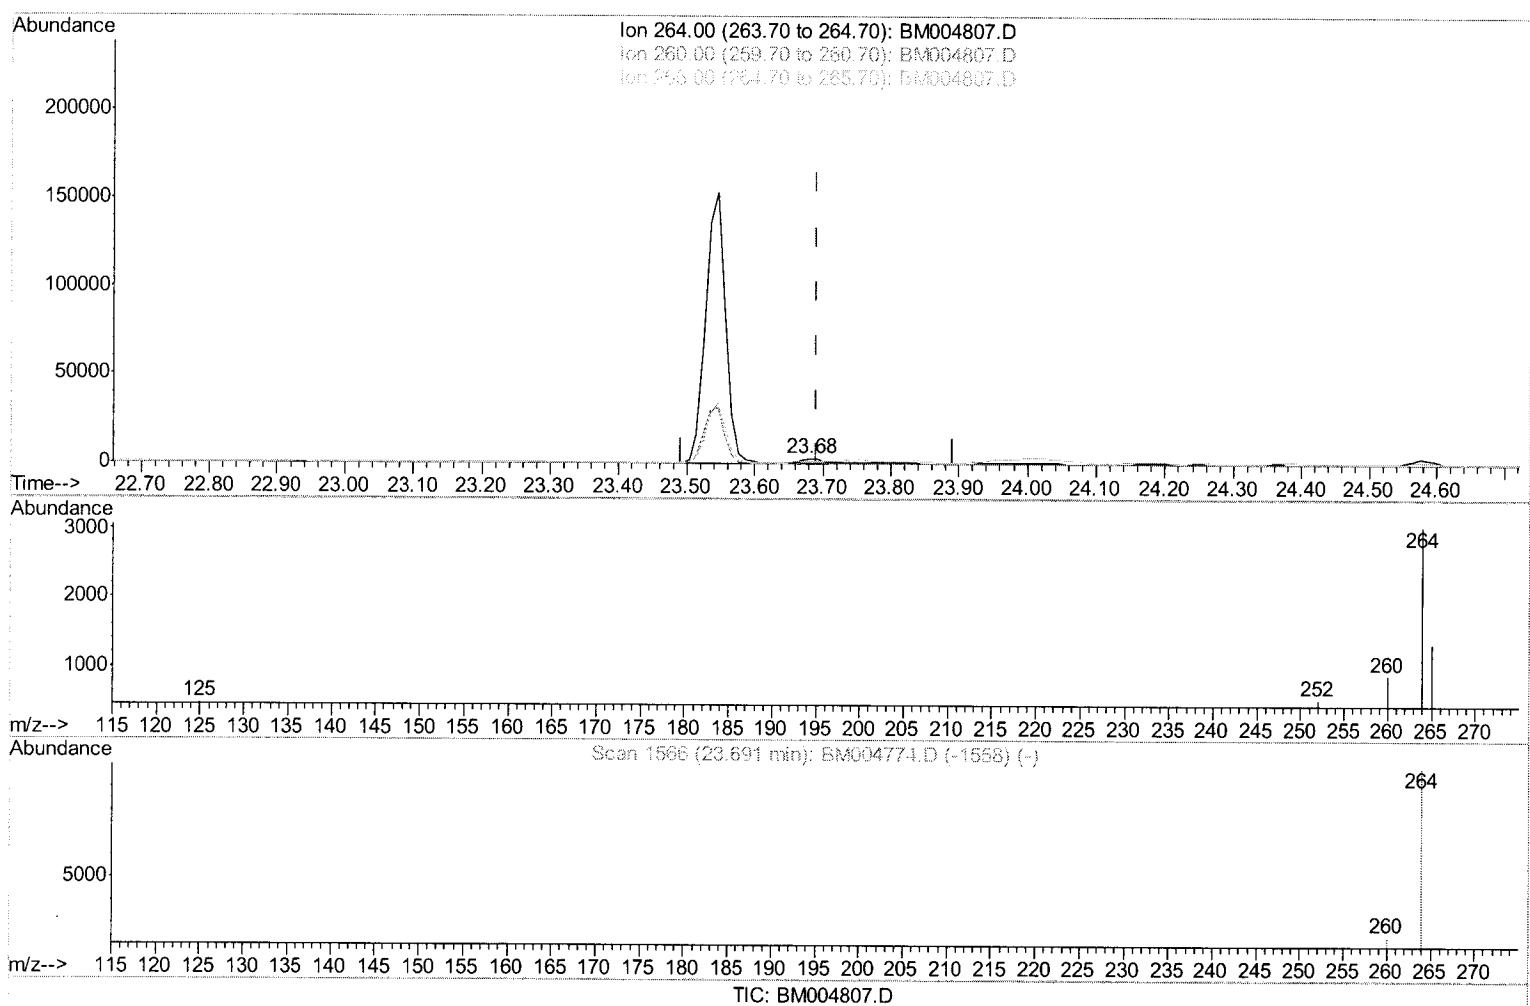

TIC: BM004807.D

(22) Perylene-d12 (I)

23.681min (-0.011) 0.40ng/ul m

response 4887

U.M
 04/07/16

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	29.55
265.00	38.20	44.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

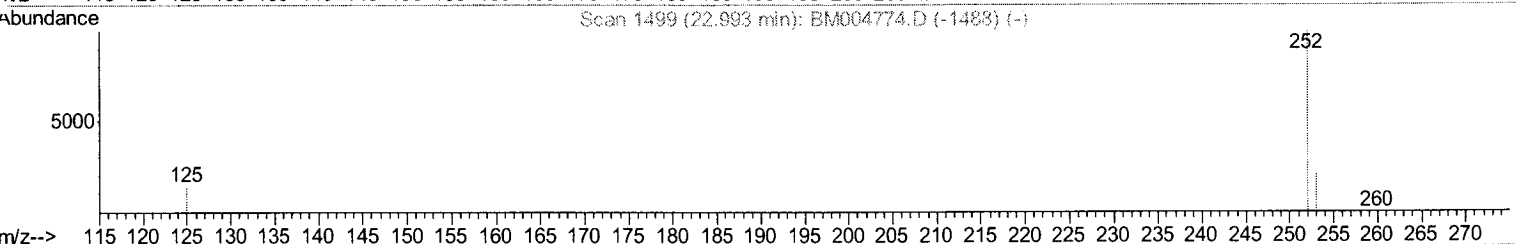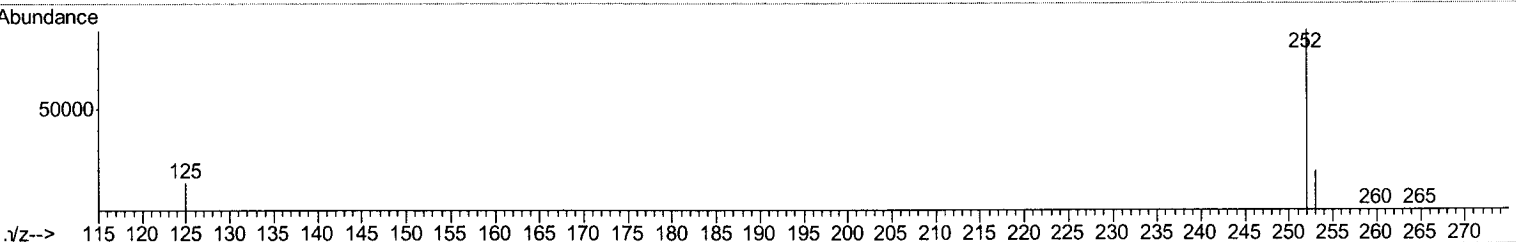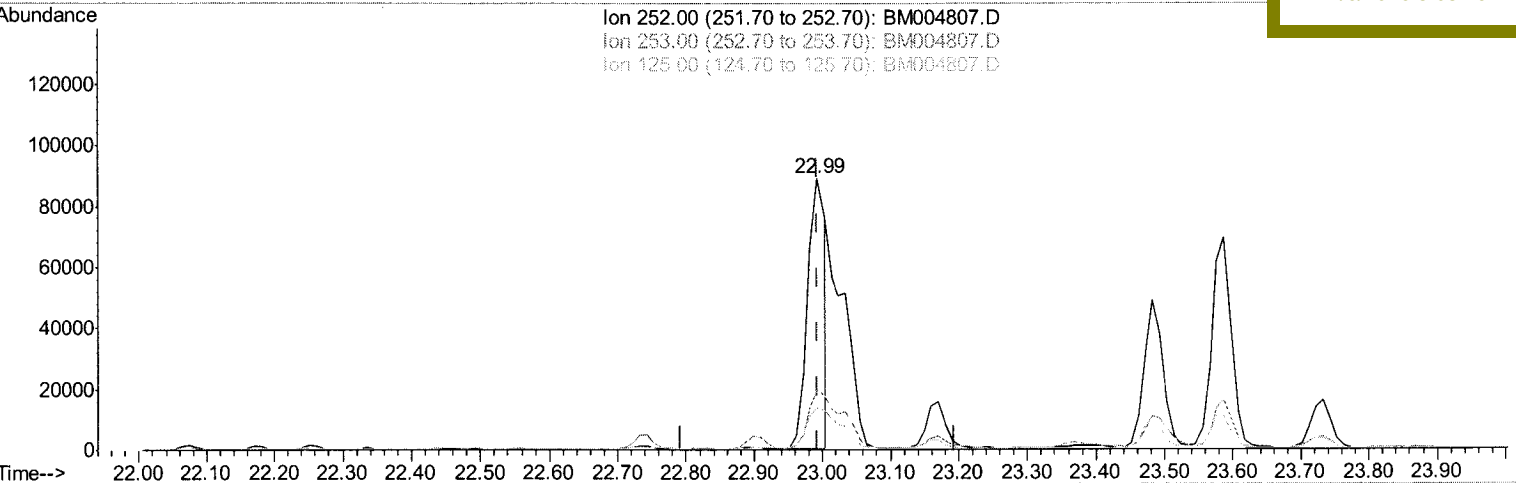

TIC: BM004807.D

(23) Benzo(b)fluoranthene

22.993min (-0.000) 9.85ng/ul

response 162239

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	22.36
125.00	14.40	15.66
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

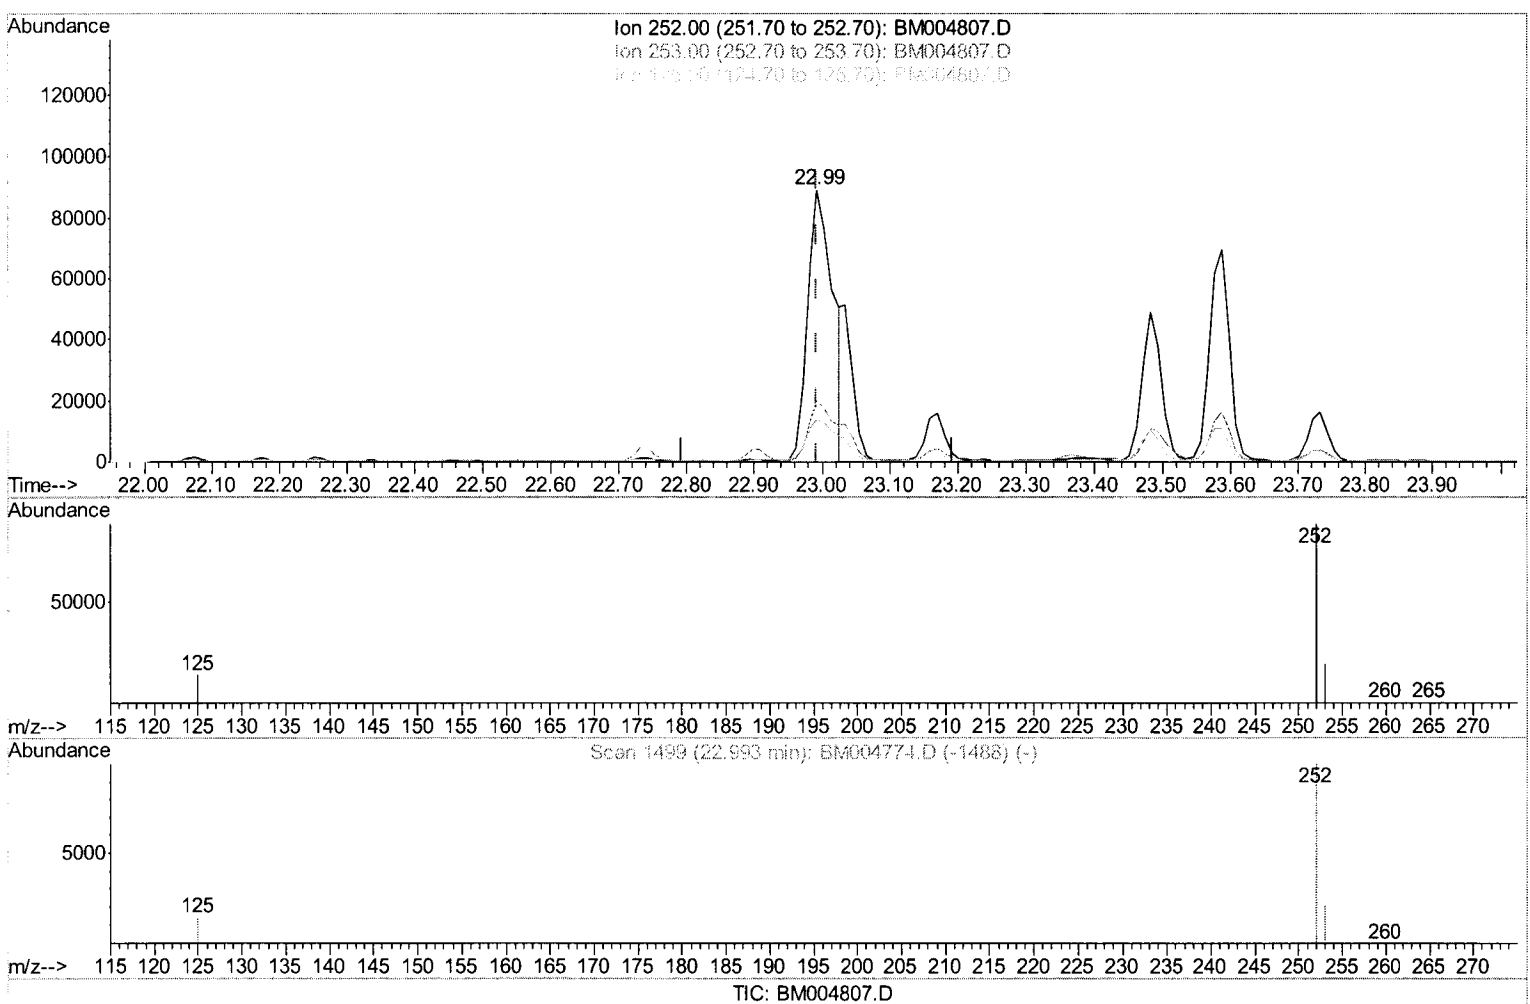

(23) Benzo(b)fluoranthene

22.993min (-0.000) 13.99ng/ul m

response 230262

V.M
 04/07/16

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	22.36
125.00	14.40	15.66
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration -

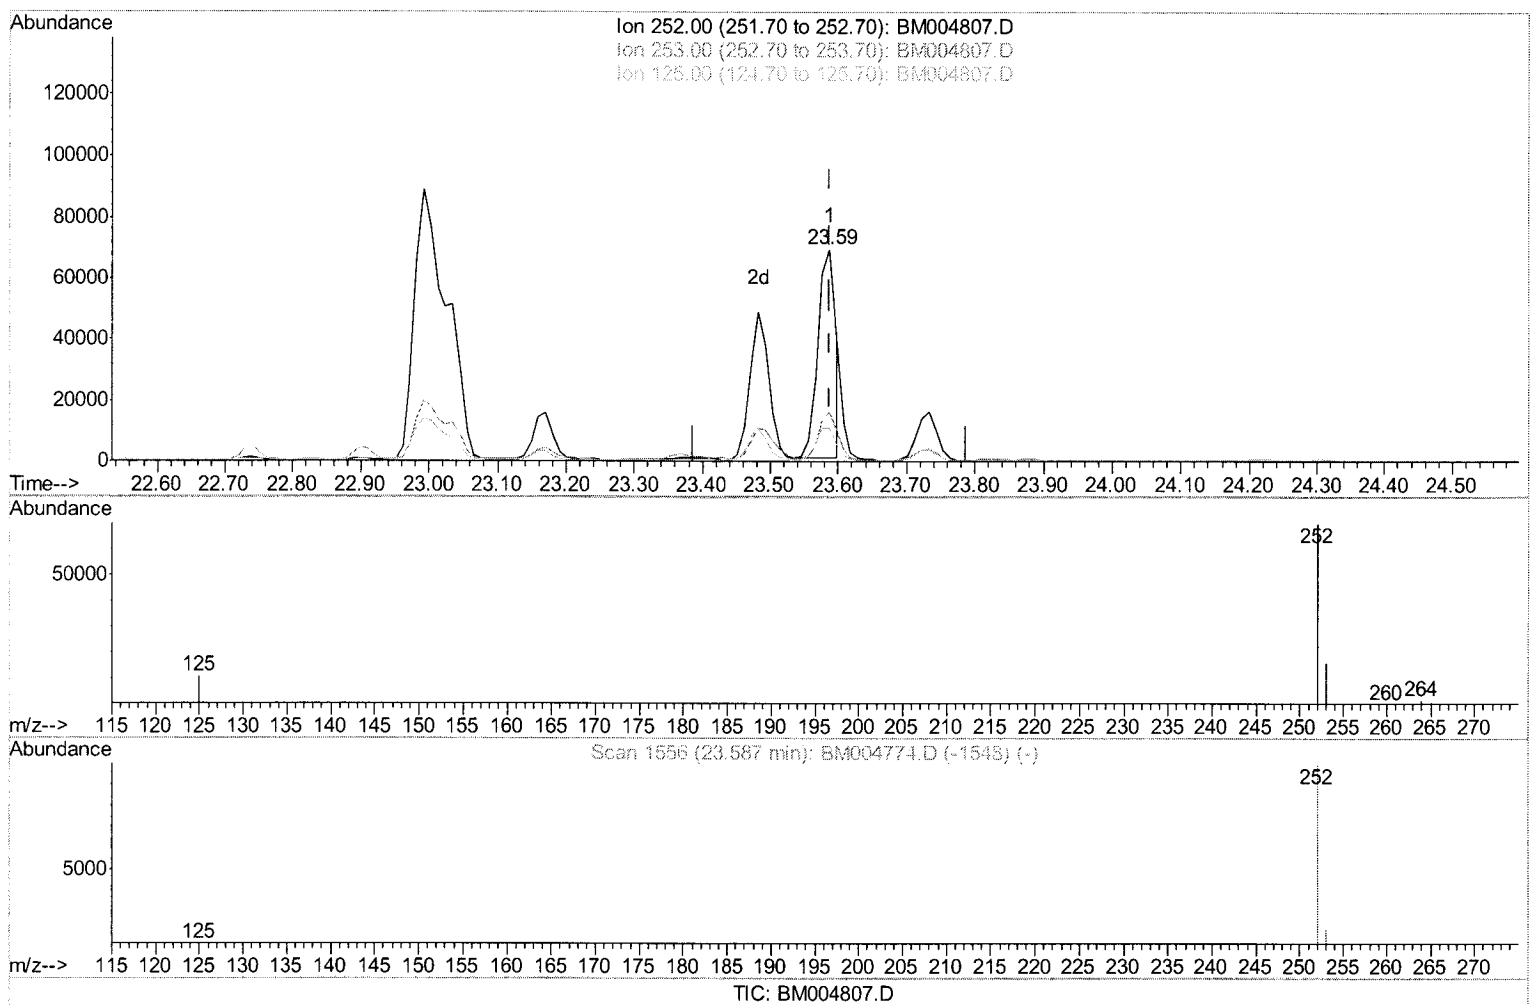

(25) Benzo(a)pyrene (C)

23.587min (-0.000) 8.25ng/ul

response 124224

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.32
125.00	15.90	15.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Apr 11 01:55:12 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 09 01:17:35 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

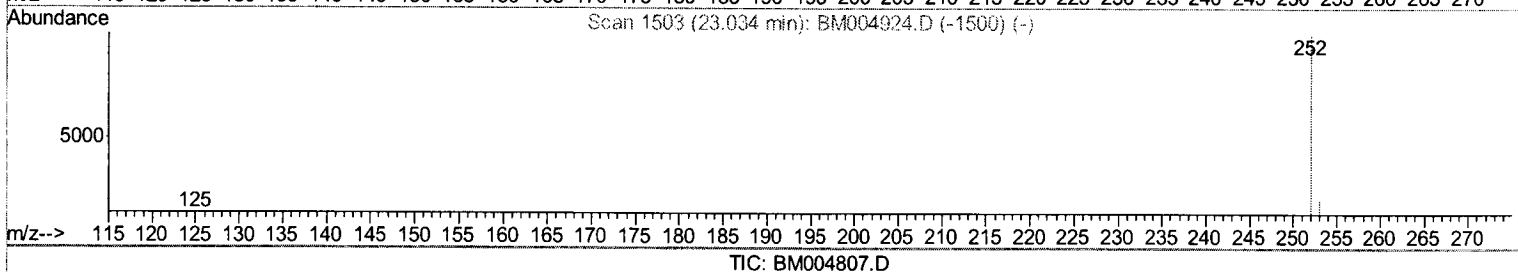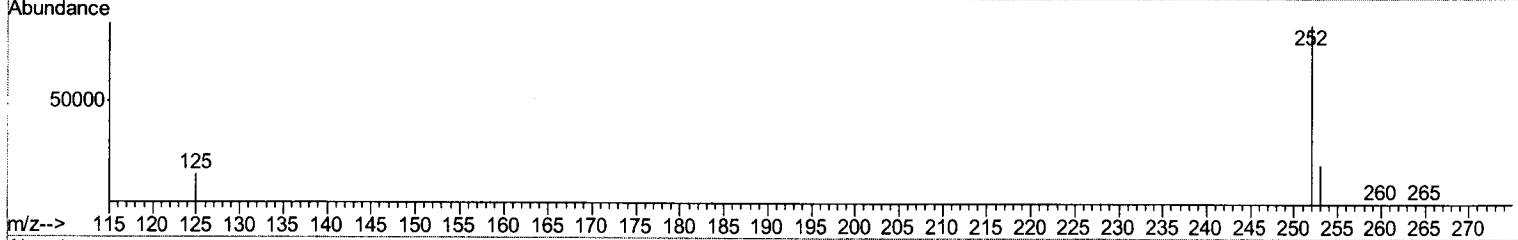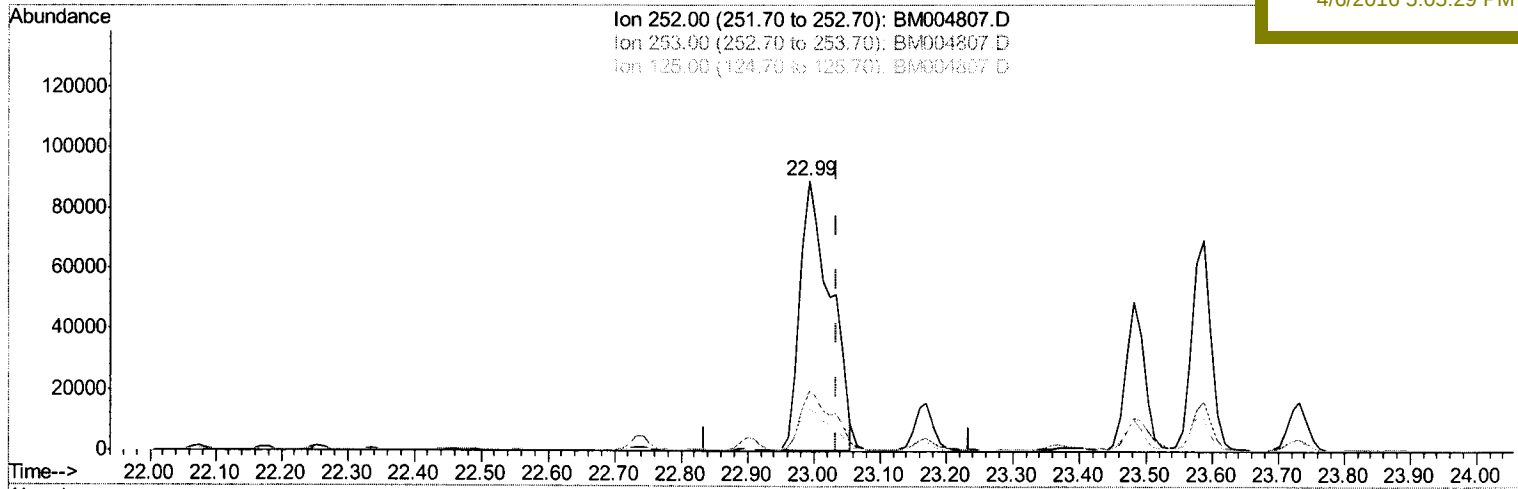

TIC: BM004807.D

(24) Benzo(k)fluoranthene
 22.993min (-0.042) 0.30ng/ul
 response 285352

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	22.36
125.00	13.00	15.66#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T41

Quant Time: Apr 05 19:51:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

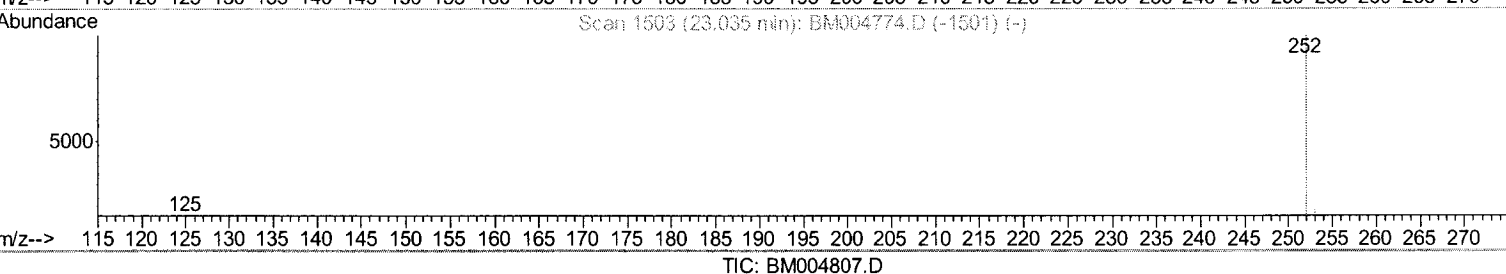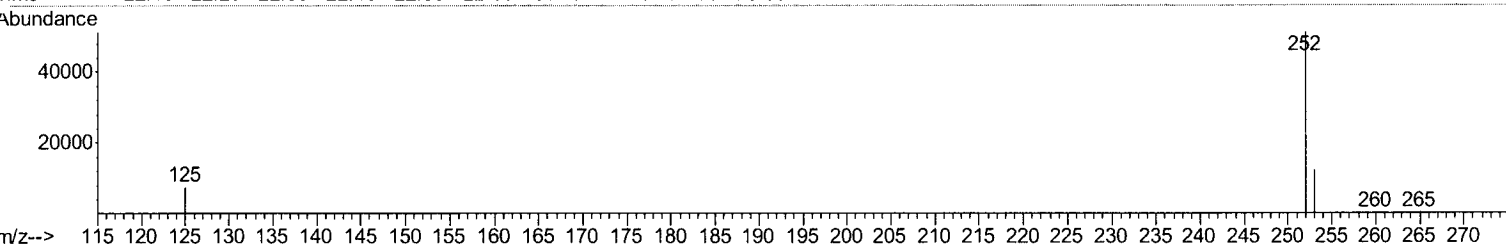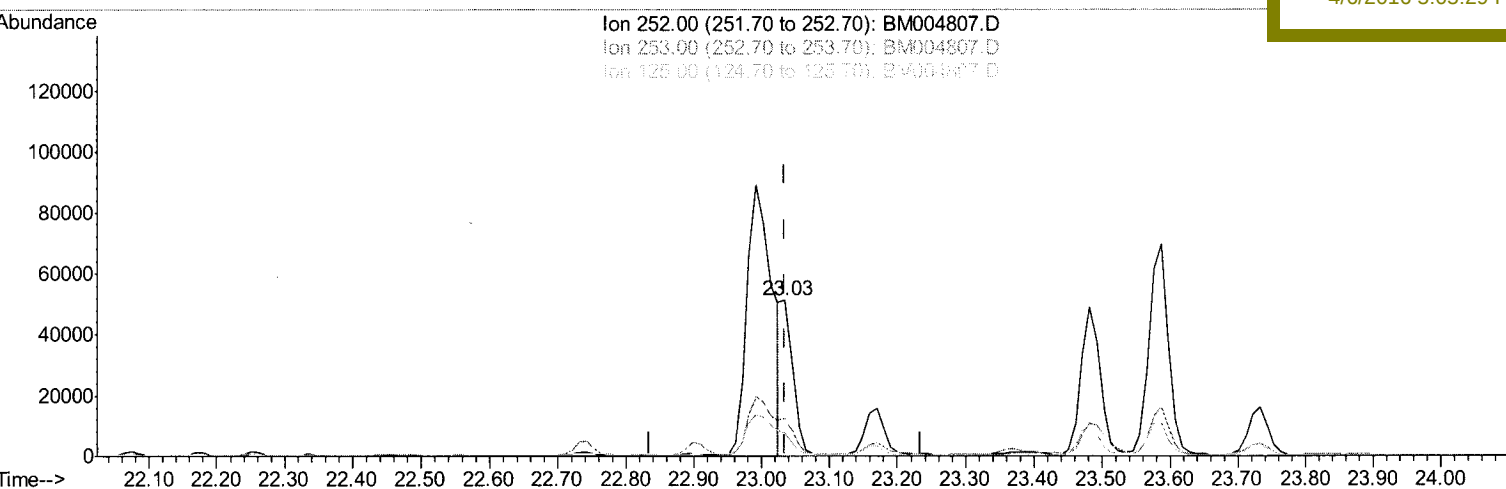

(24) Benzo(k)fluoranthene

23.034min (-0.000) 3.95ng/ul m

response 60199

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	24.37
125.00	13.00	14.76
0.00	0.00	0.00

U.M
04/07/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

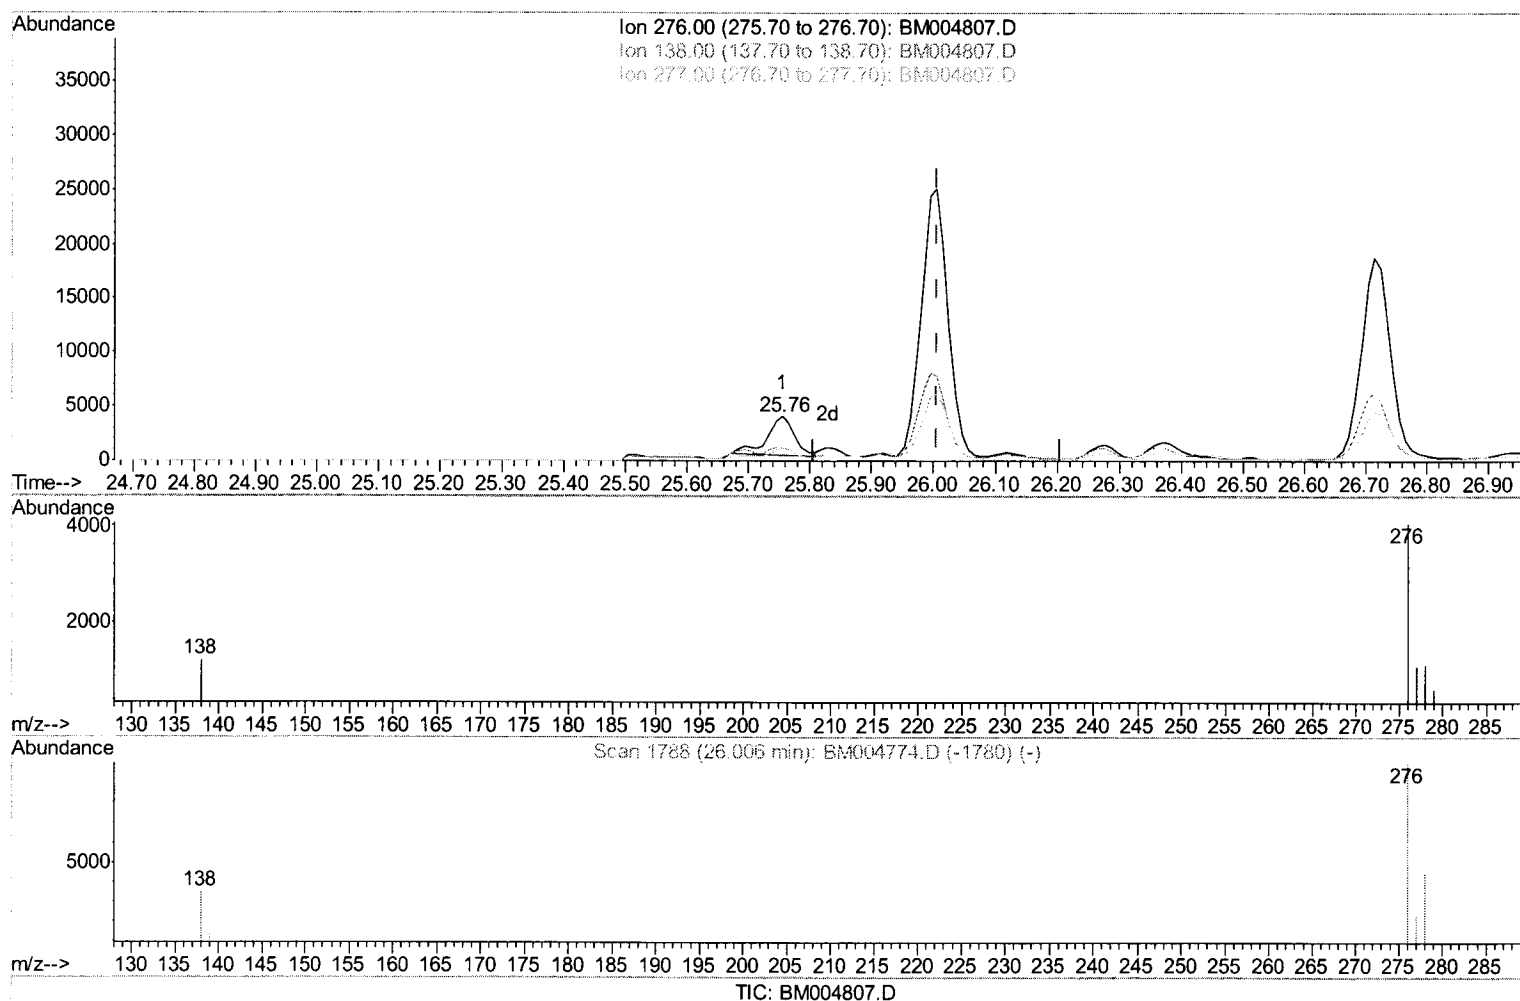

(26) Indeno(1,2,3-cd)pyrene

25.755min (-0.251) 0.78ng/ul

response 10879

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	18.50
277.00	24.80	23.41
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T41

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

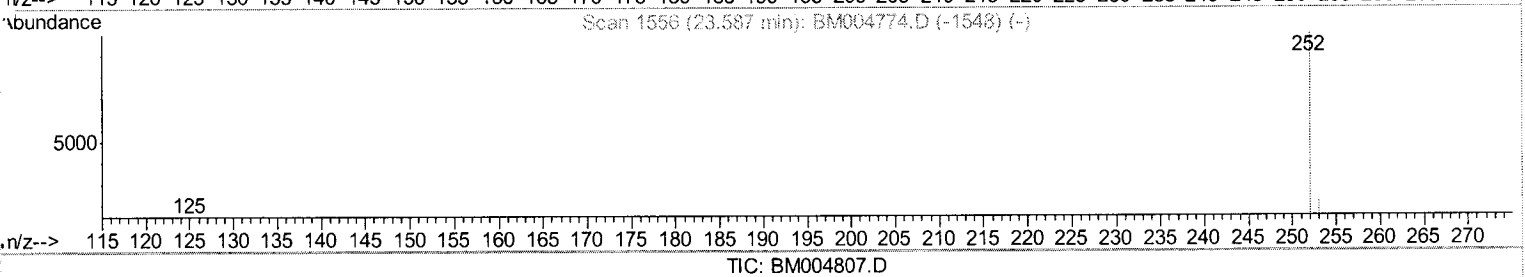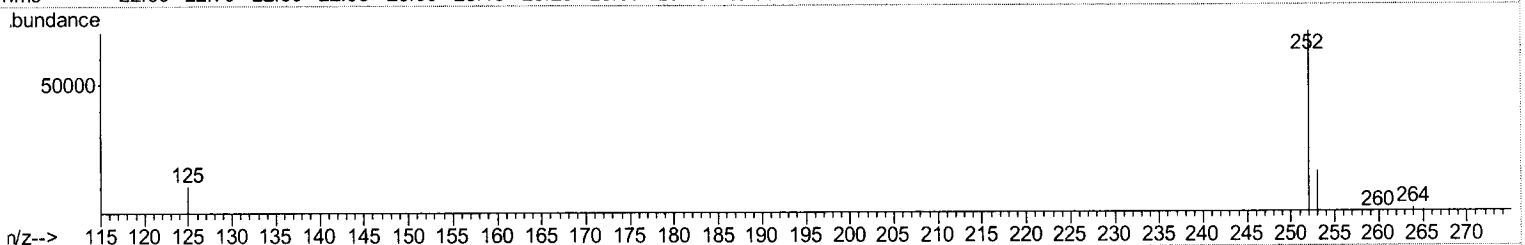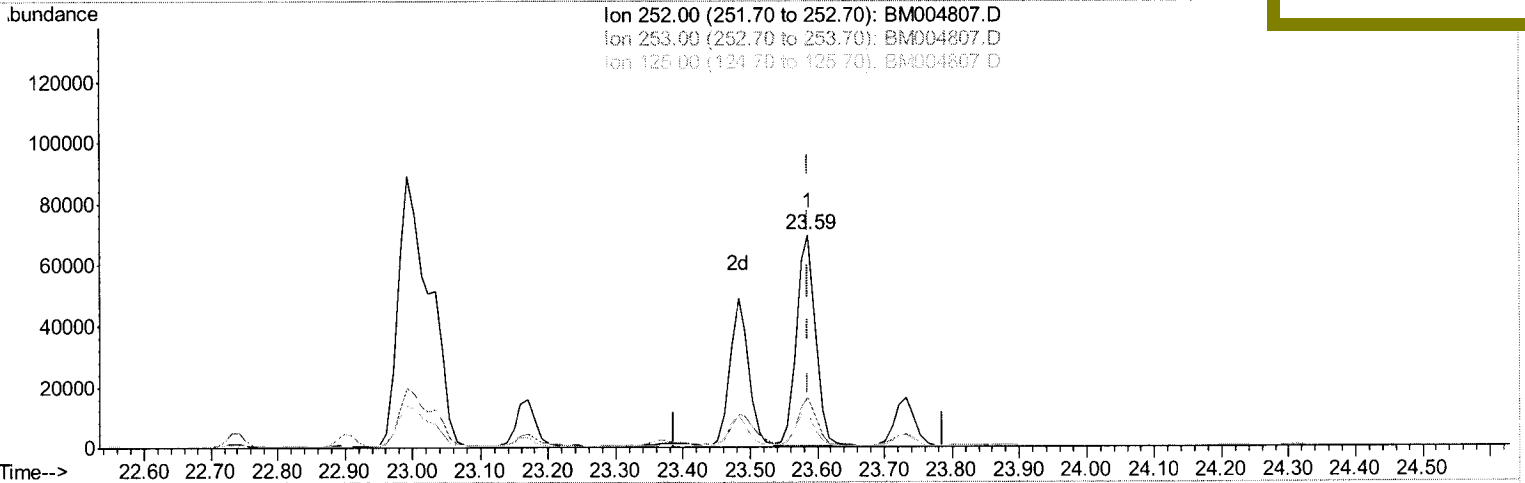

TIC: BM004807.D

(25) Benzo(a)pyrene (C)

23.587min (-0.000) 9.09ng/ul m

response 136766

U.M
04/07/16

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.32
125.00	15.90	15.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

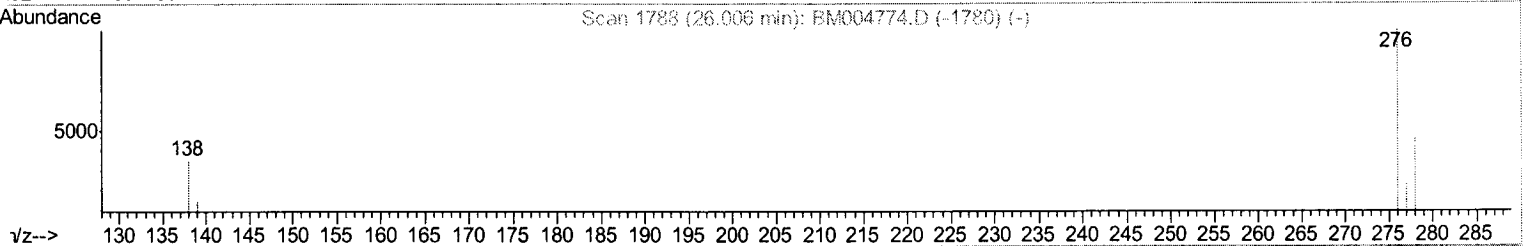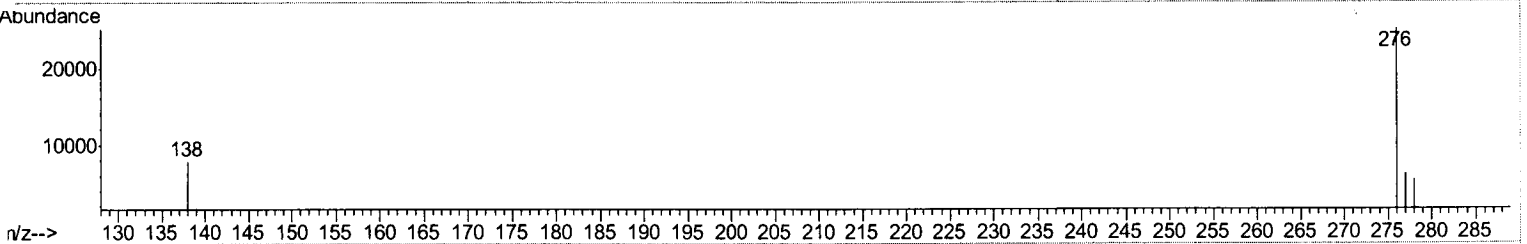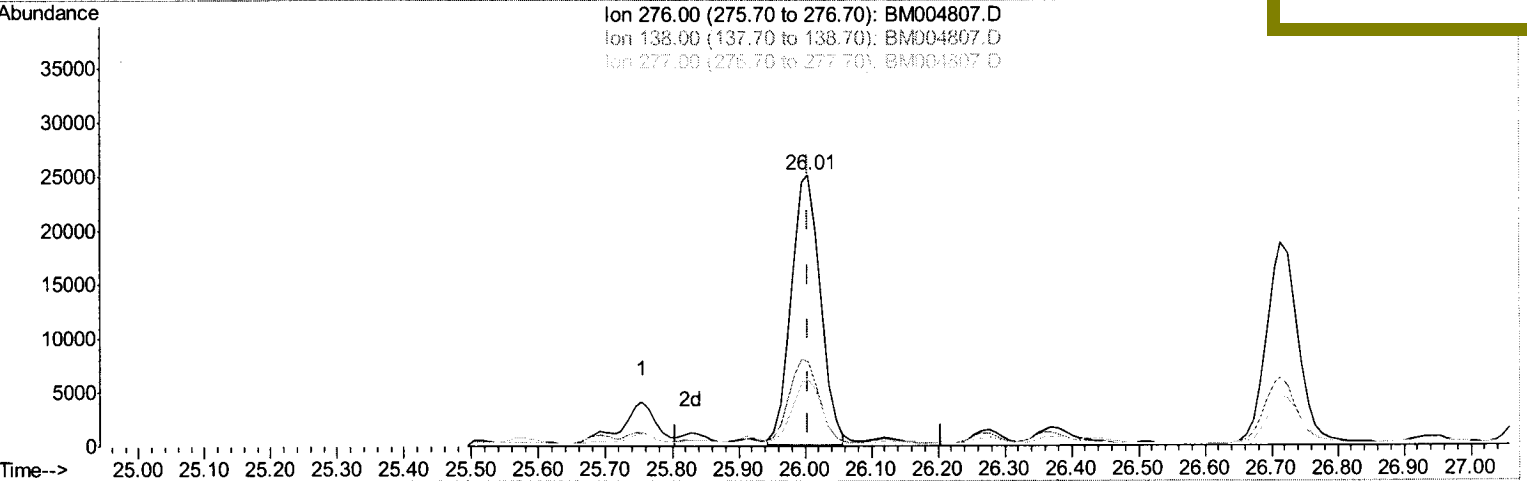

TIC: BM004807.D

(26) Indeno(1,2,3-cd)pyrene

26.005min (-0.000) 5.45ng/ul m

response 75896

U.M
 04/07/16

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	2.65#
277.00	24.80	3.36#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

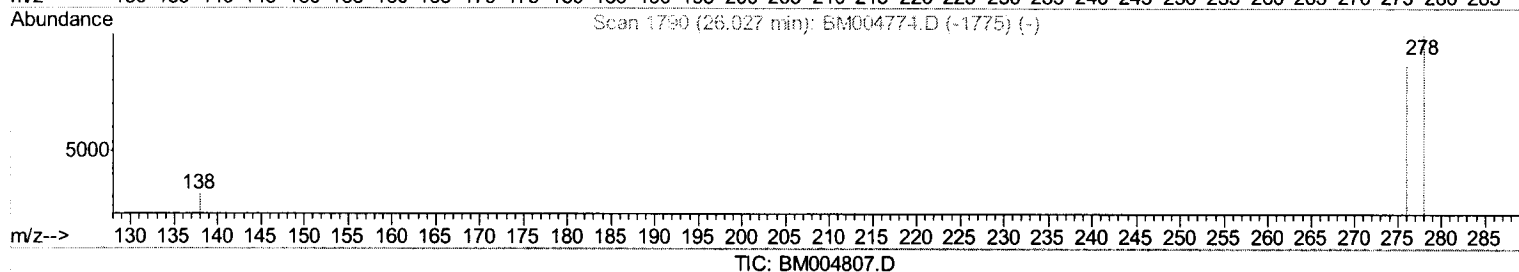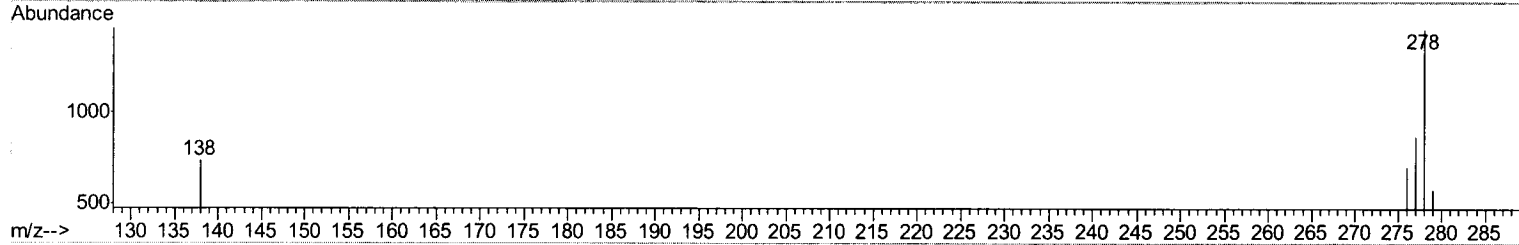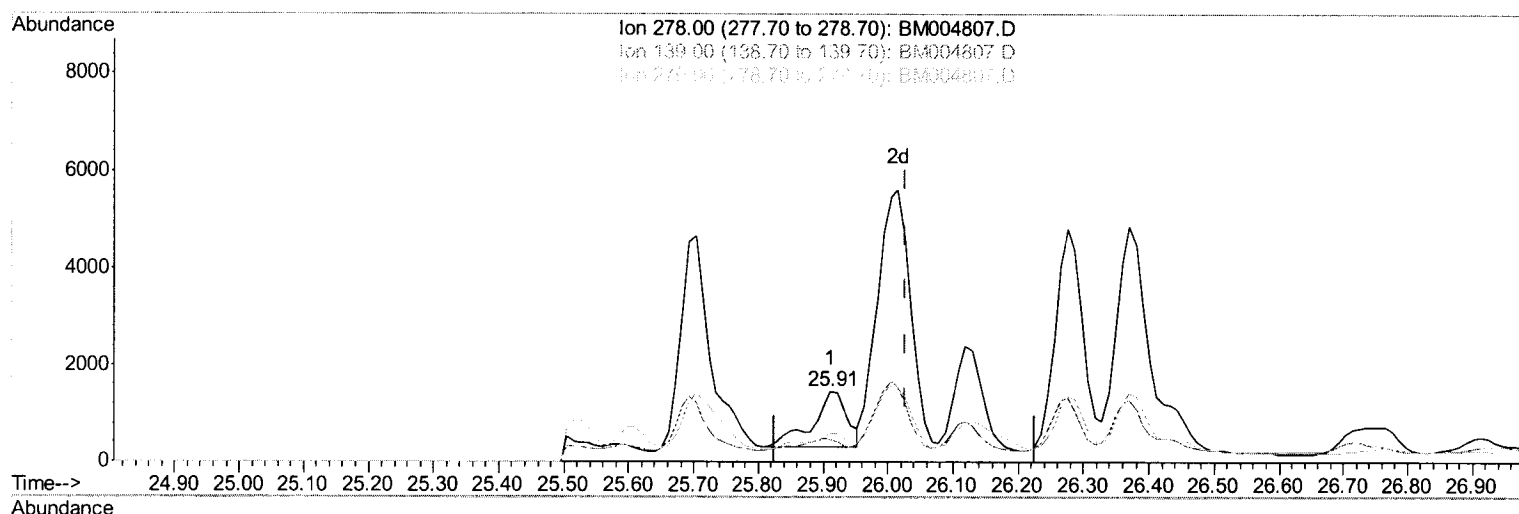

TIC: BM004807.D

(27) Dibenzo(a,h)anthracene

25.911min (-0.115) 0.39ng/ul

response 4322

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	32.44#
279.00	25.20	39.93#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

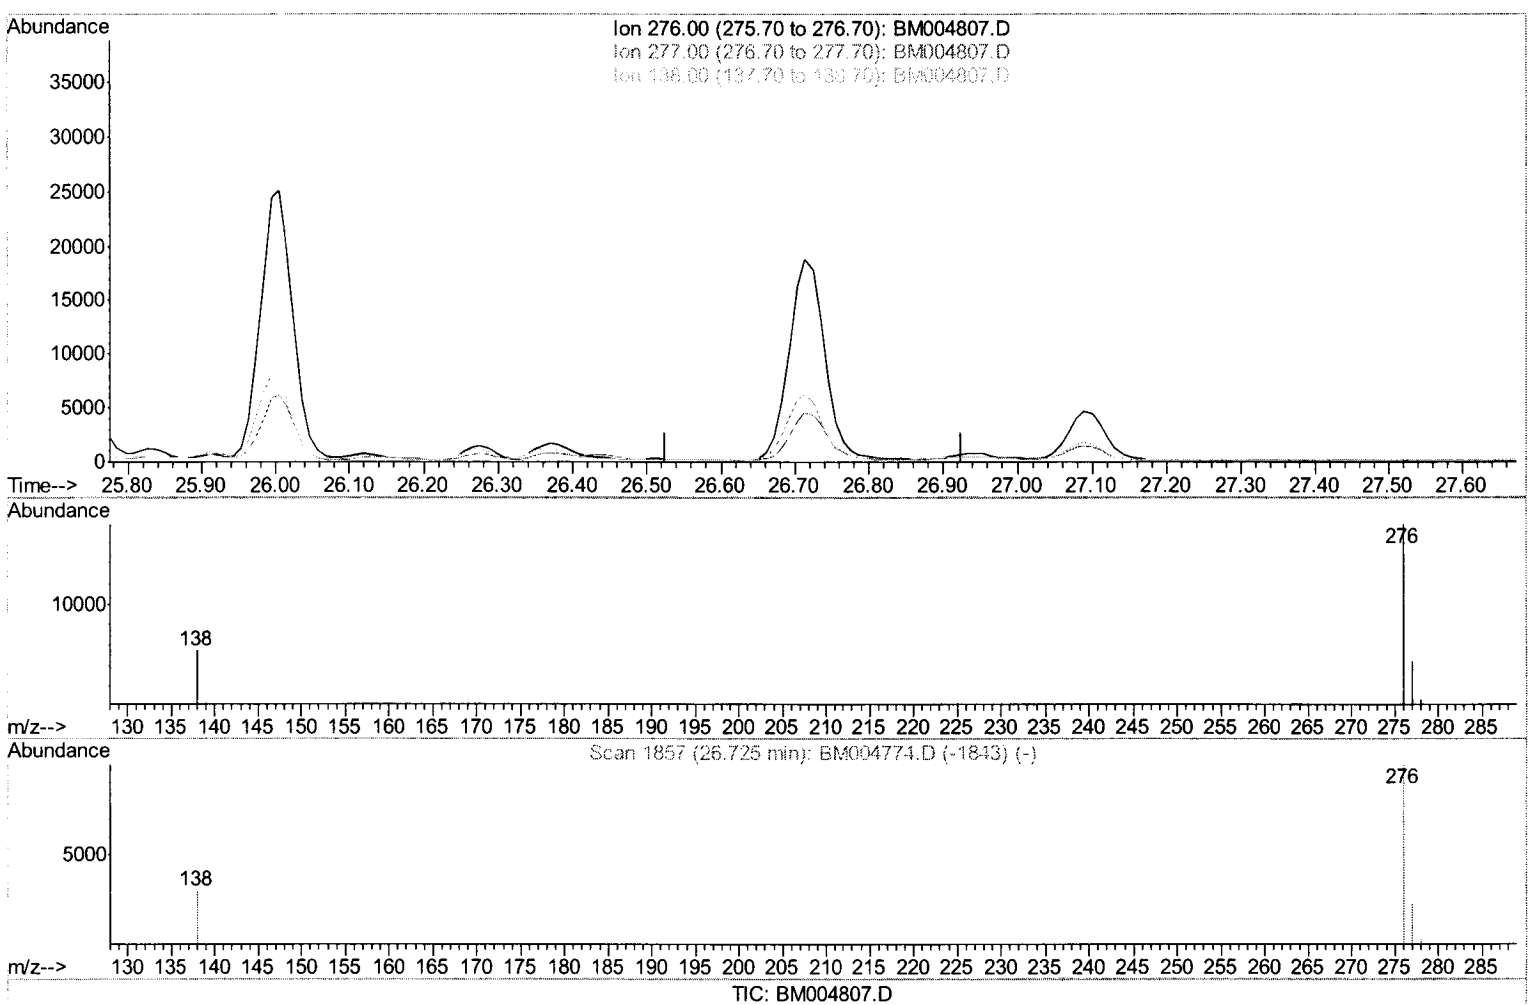

(28) Benzo(g,h,i)perylene

26.725min (-26.725) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	23.60	0.00#
138.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

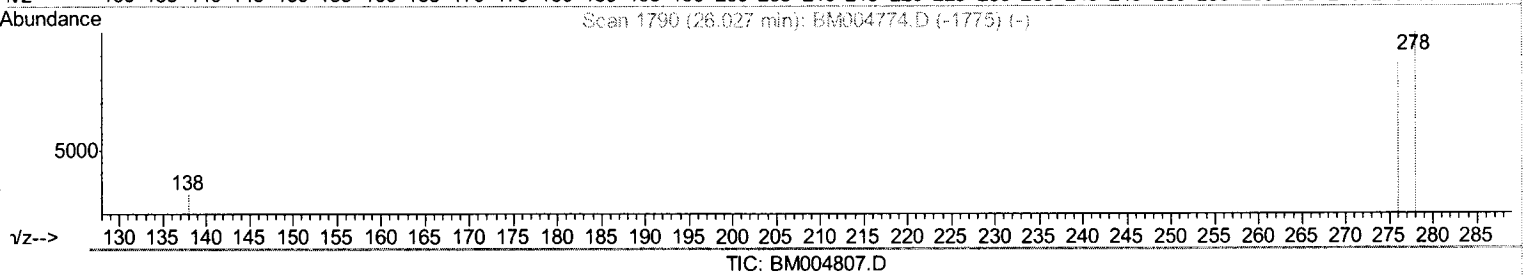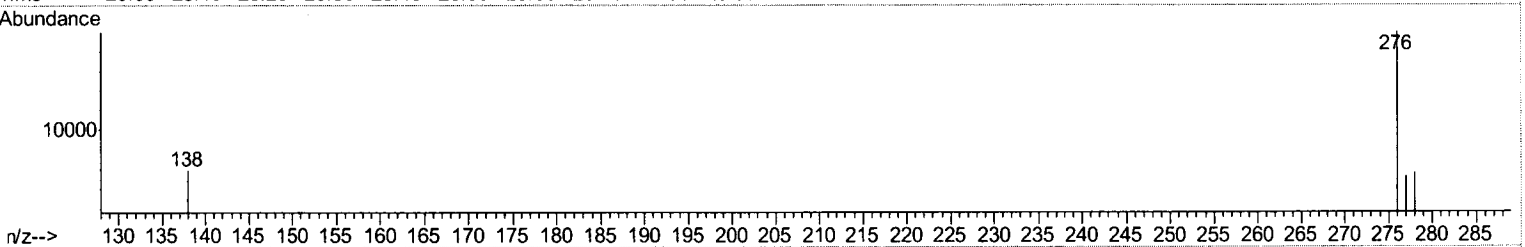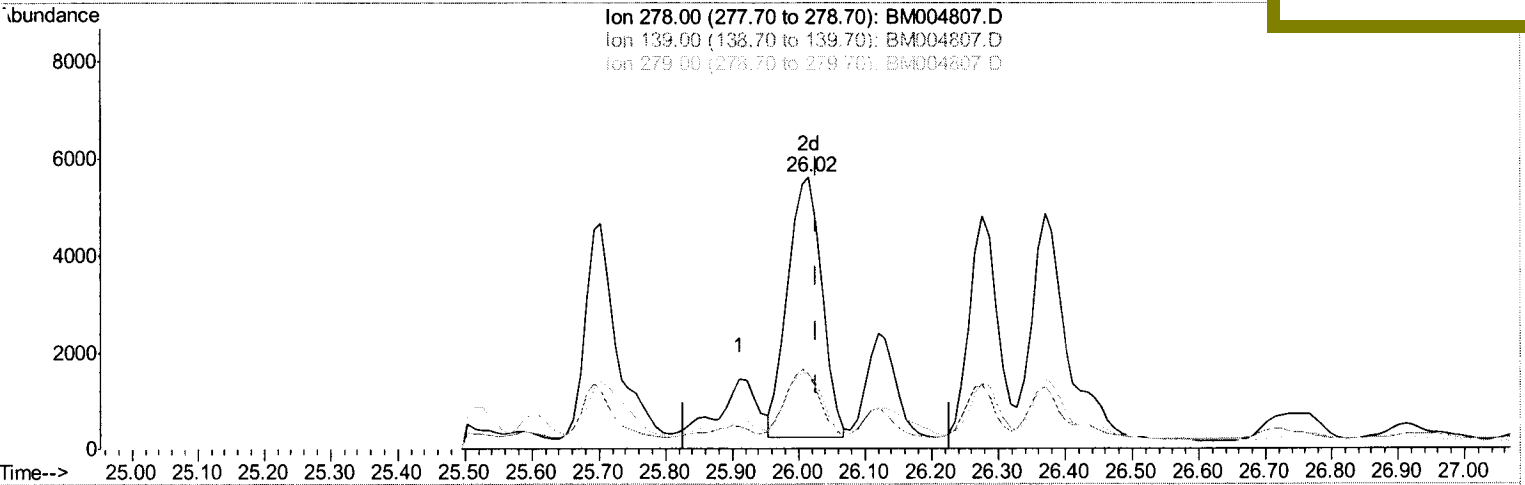

(27) Dibenzo(a,h)anthracene

26.016min (-0.011) 1.75ng/ul m

response 19161

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	27.76#
279.00	25.20	28.02
0.00	0.00	0.00

U.M
 04/07/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004807.D
 Acq On : 28 Mar 2016 15:20
 Operator : UM/SJ
 Sample : H1909-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T41

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

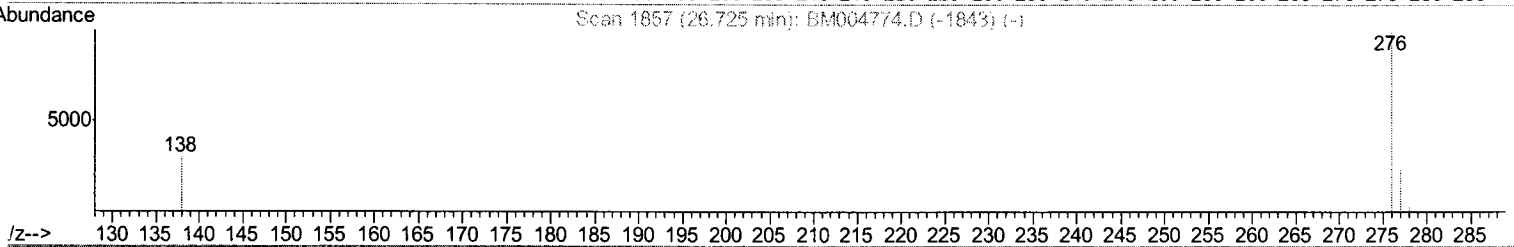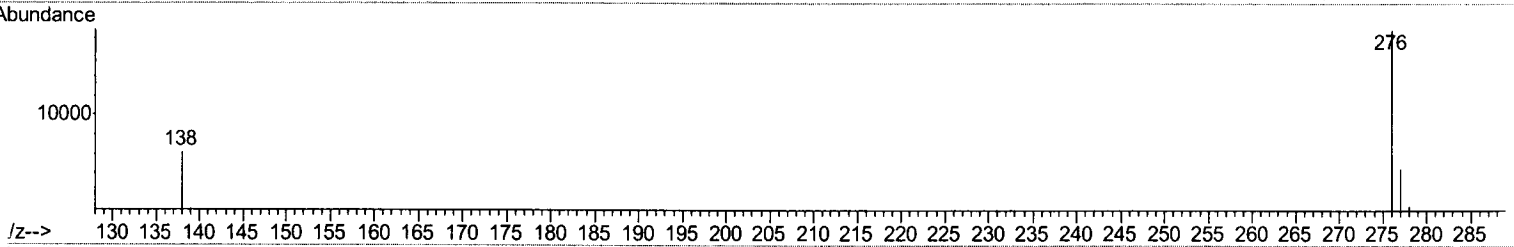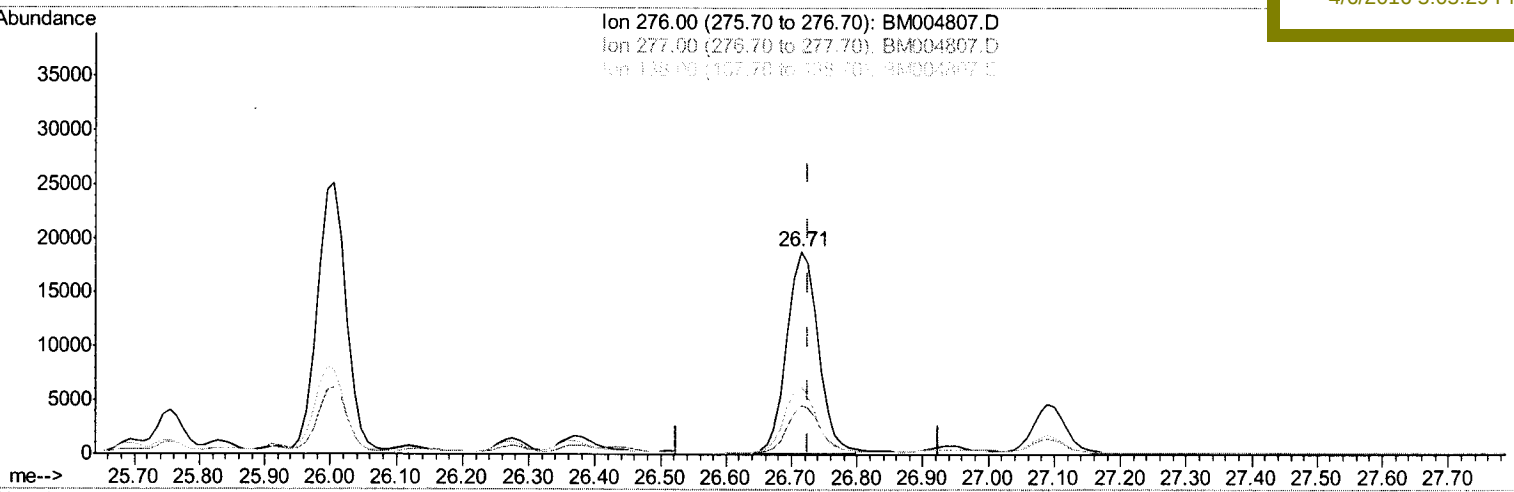

TIC: BM004807.D

(28) Benzo(g,h,i)perylene

26.714min (-0.011) 5.45ng/ul m U.M

response 62836

04/07/16

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	24.09
138.00	28.10	33.32
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004807.D
Acq On : 28 Mar 2016 15:20
Operator : UM/SJ
Sample : H1909-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample ID :
A4T41

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:29 PM

Quant Time: Apr 05 19:56:54 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1041	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	4882	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.47	164	2898	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.21	188	6401m	0.40	ng/ul	0.00
18) Chrysene-d12	21.40	240	6586	0.40	ng/ul	0.00
22) Perylene-d12	23.68	264	4887m	0.40	ng/ul	-0.01

U.M
04/07/16

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.32	96	3892	8.30	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.21	152	1676	0.25	ng/ul	0.00
16) Fluoranthene-d10	19.24	212	4381	0.29	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Naphthalene	10.67	128	8587	0.73	ng/ul	97
7) 2-Methylnaphthalene	12.28	142	1574	0.19	ng/ul	99
9) Acenaphthylene	14.18	152	21138	1.59	ng/ul	94
10) Acenaphthene	14.52	153	3163	0.34	ng/ul	89
11) Fluorene	15.51	166	6937	0.62	ng/ul	91
14) Phenanthrene	17.24	178	124116	6.90	ng/ul	96
15) Anthracene	17.33	178	33132	1.95	ng/ul	96
17) Fluoranthene	19.27	202	359692m	17.57	ng/ul	
19) Pyrene	19.63	202	296936	13.17	ng/ul	97
20) Benzo(a)anthracene	21.38	228	175128m	8.65	ng/ul	
21) Chrysene	21.43	228	159173	8.14	ng/ul	97
23) Benzo(b)fluoranthene	22.99	252	230262m	13.99	ng/ul	
24) Benzo(k)fluoranthene	23.03	252	60199m	3.95	ng/ul	
25) Benzo(a)pyrene	23.59	252	136766m	9.09	ng/ul	
26) Indeno(1,2,3-cd)pyrene	26.01	276	75896m	5.45	ng/ul	
27) Dibenzo(a,h)anthracene	26.02	278	19161m	1.75	ng/ul	
28) Benzo(a,h,i)perylene	26.71	276	62836m	5.45	ng/ul	

U.M
04/07/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed