

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 06 14:34:42 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

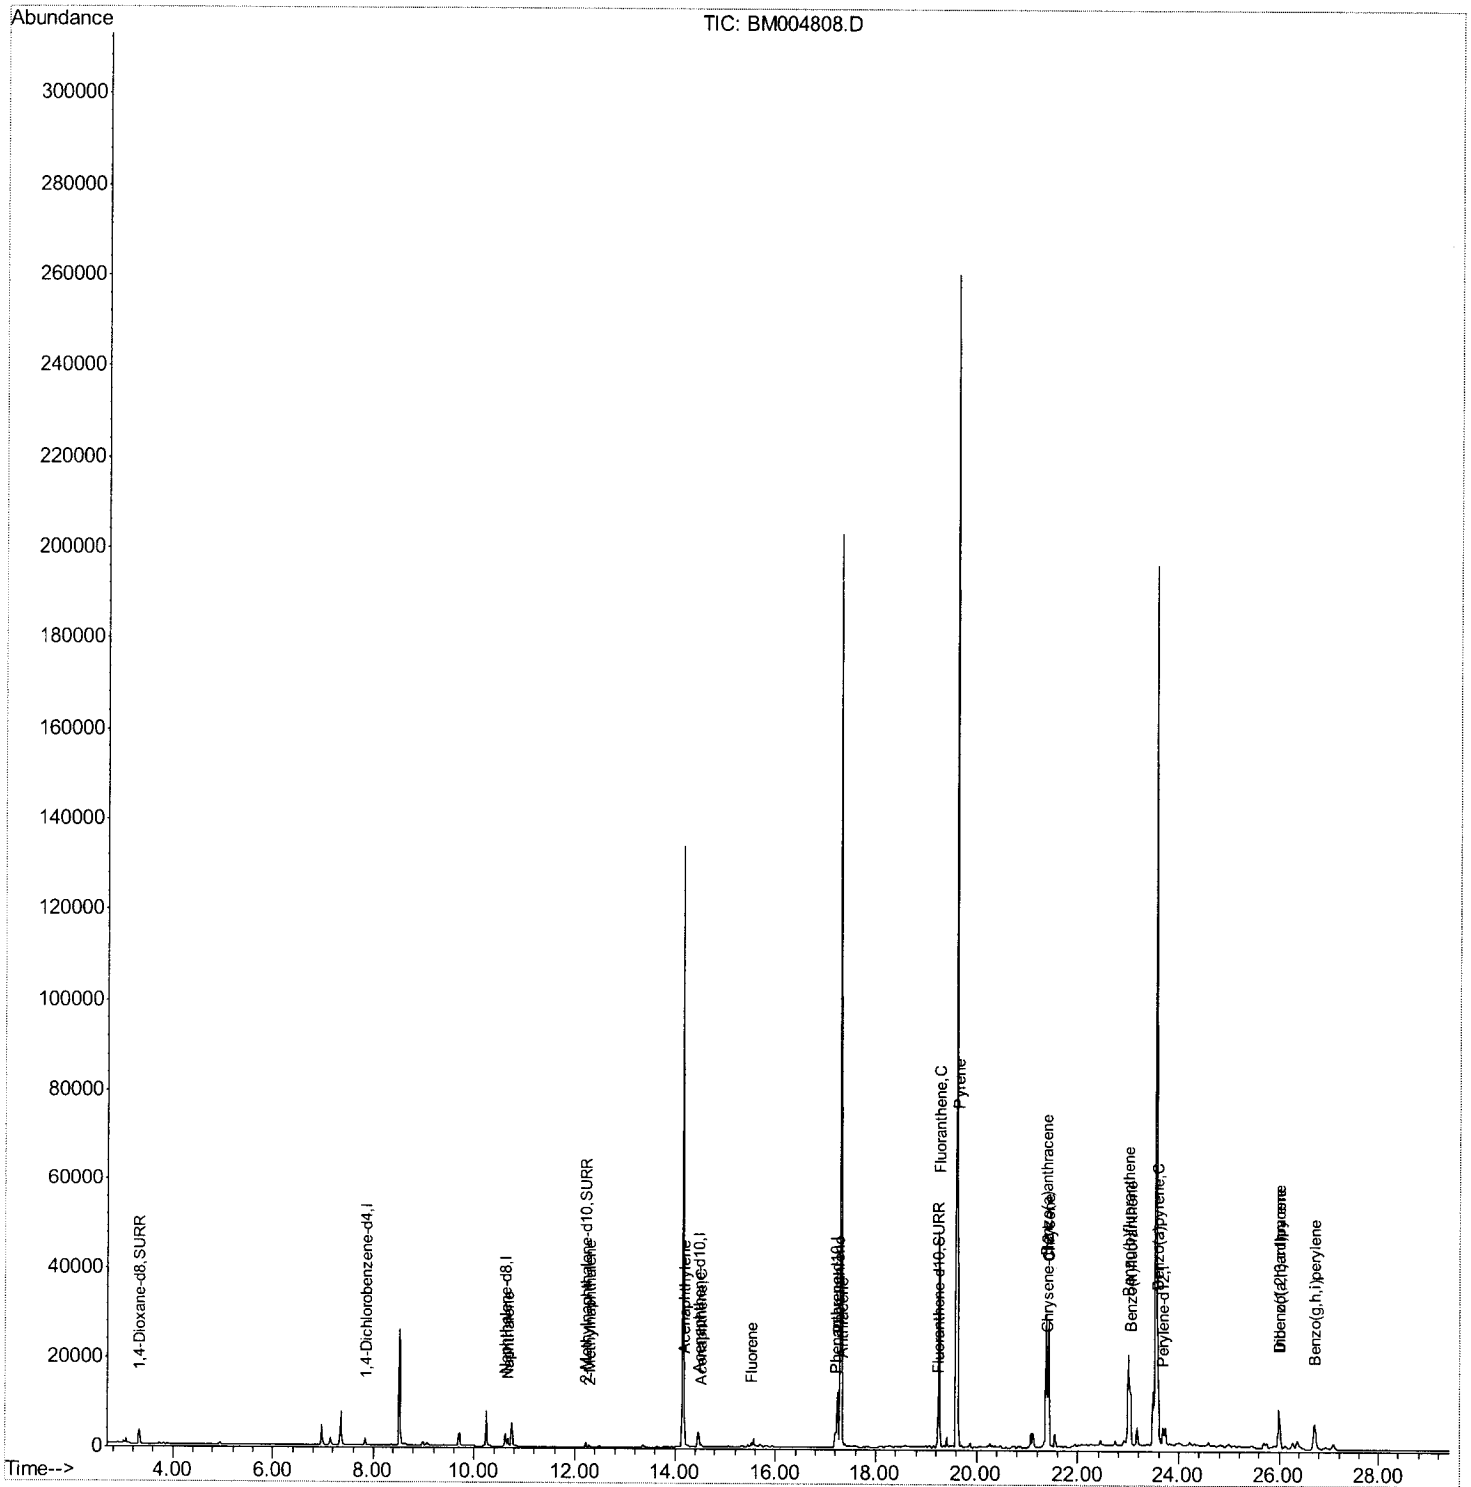

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:04 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

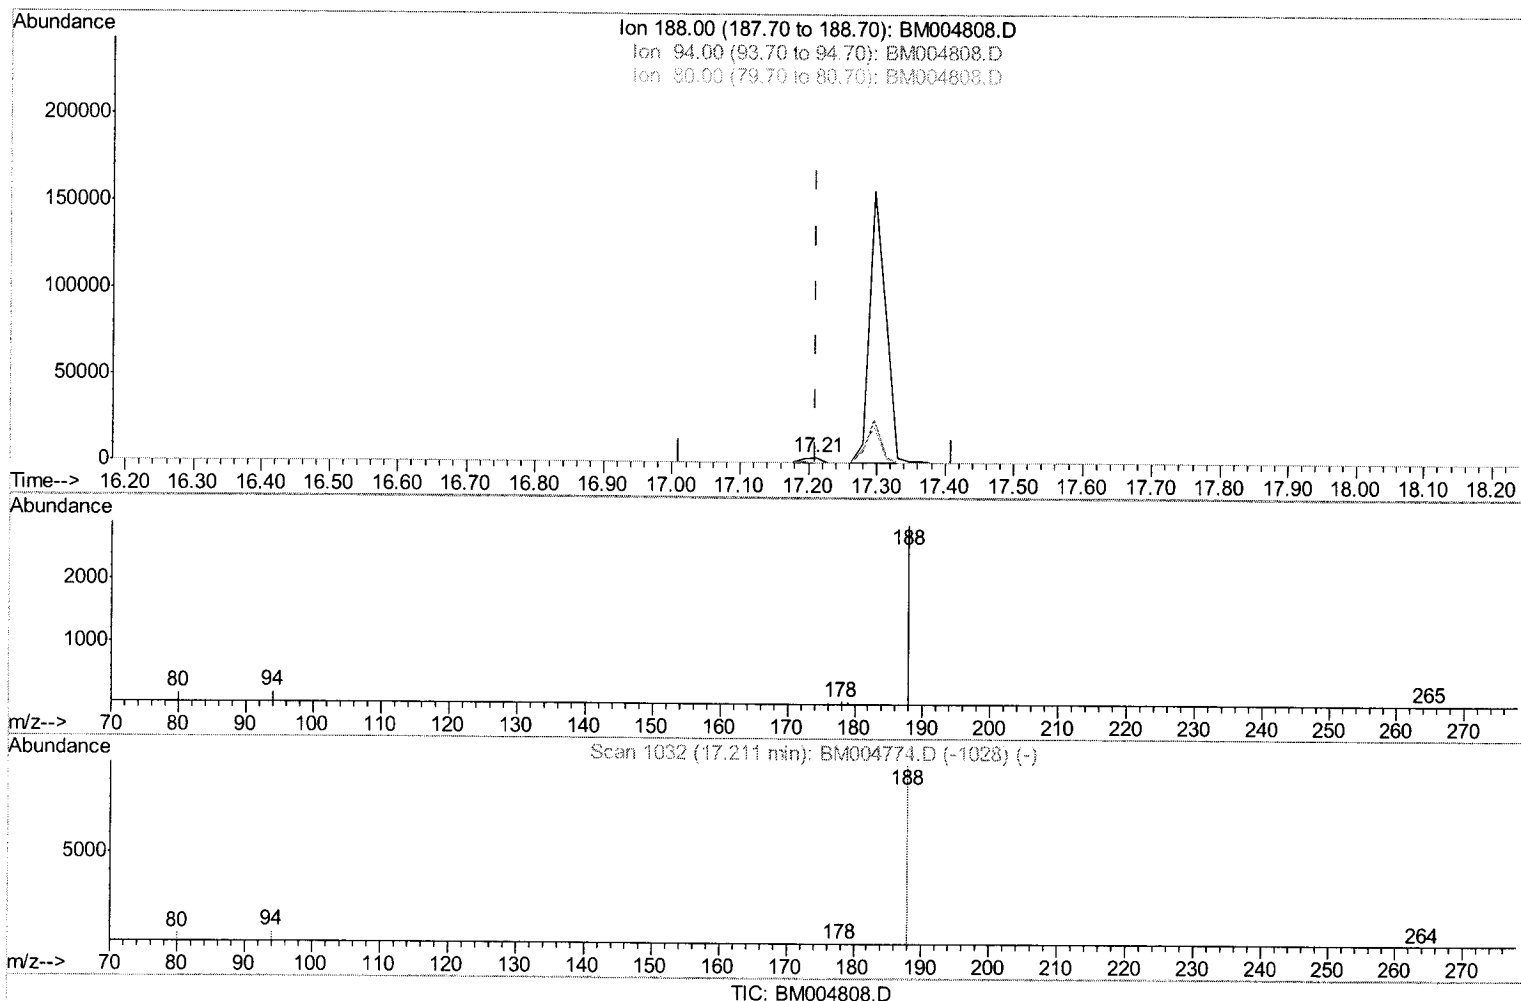

(12) Phenanthrene-d10 (I)

17.211min (-0.000) 0.40ng/ul m

response 5597

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.37#
80.00	11.90	6.62#
0.00	0.00	0.00

U.M
 04/07/16


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004808.D
Acq On : 28 Mar 2016 15:56
Operator : UM/SJ
Sample : H1909-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Apr 05 19:58:04 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4T46

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:03 PM

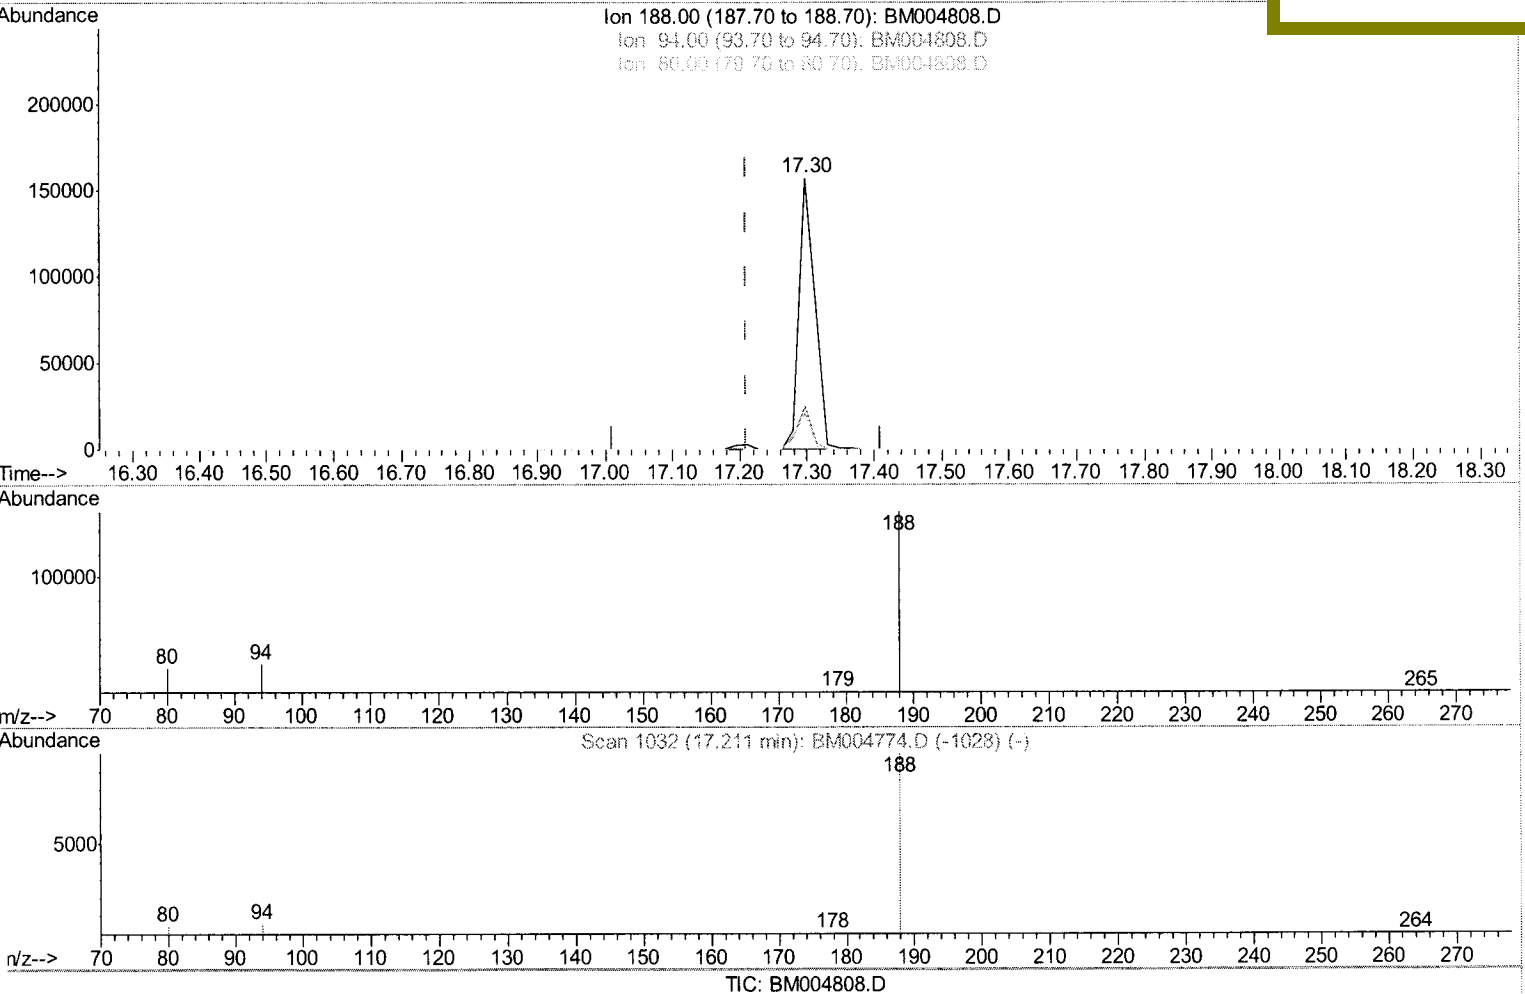

(12) Phenanthrene-d10 (I)

17.297min (+0.086) 0.40ng/ul

response 258124

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	15.75#
80.00	11.90	13.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

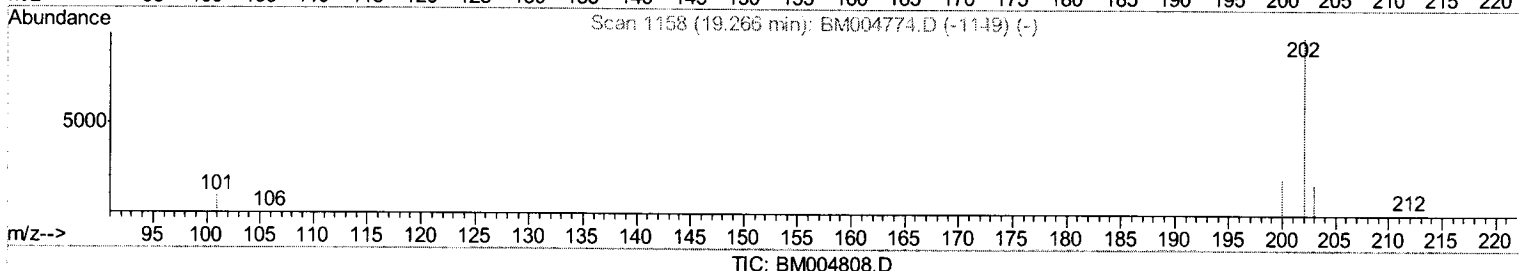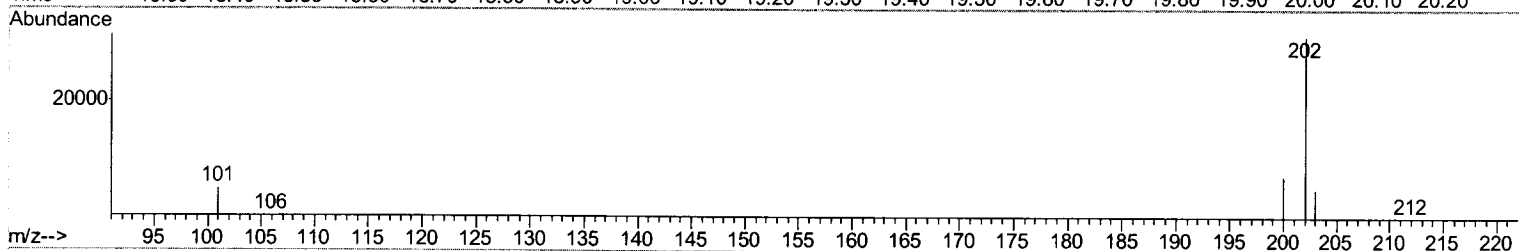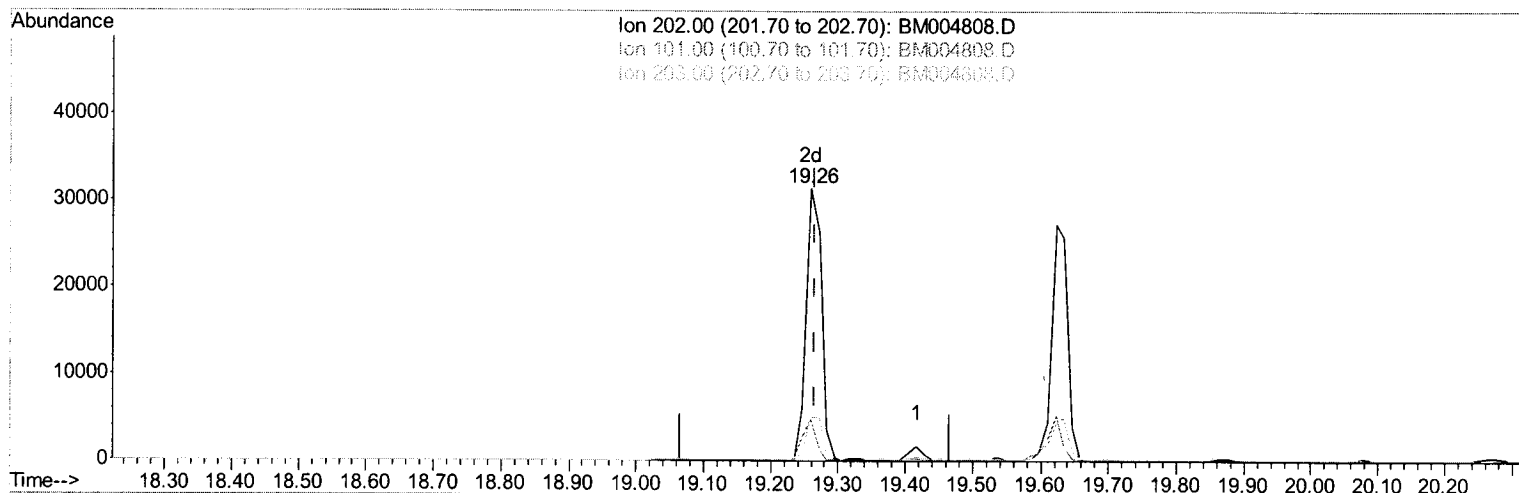

(17) Fluoranthene (C)

19.259min (-0.007) 2.75ng/ul m

response 49244

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	15.54
203.00	16.30	15.95
0.00	0.00	0.00

U.M
 04/07/16


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

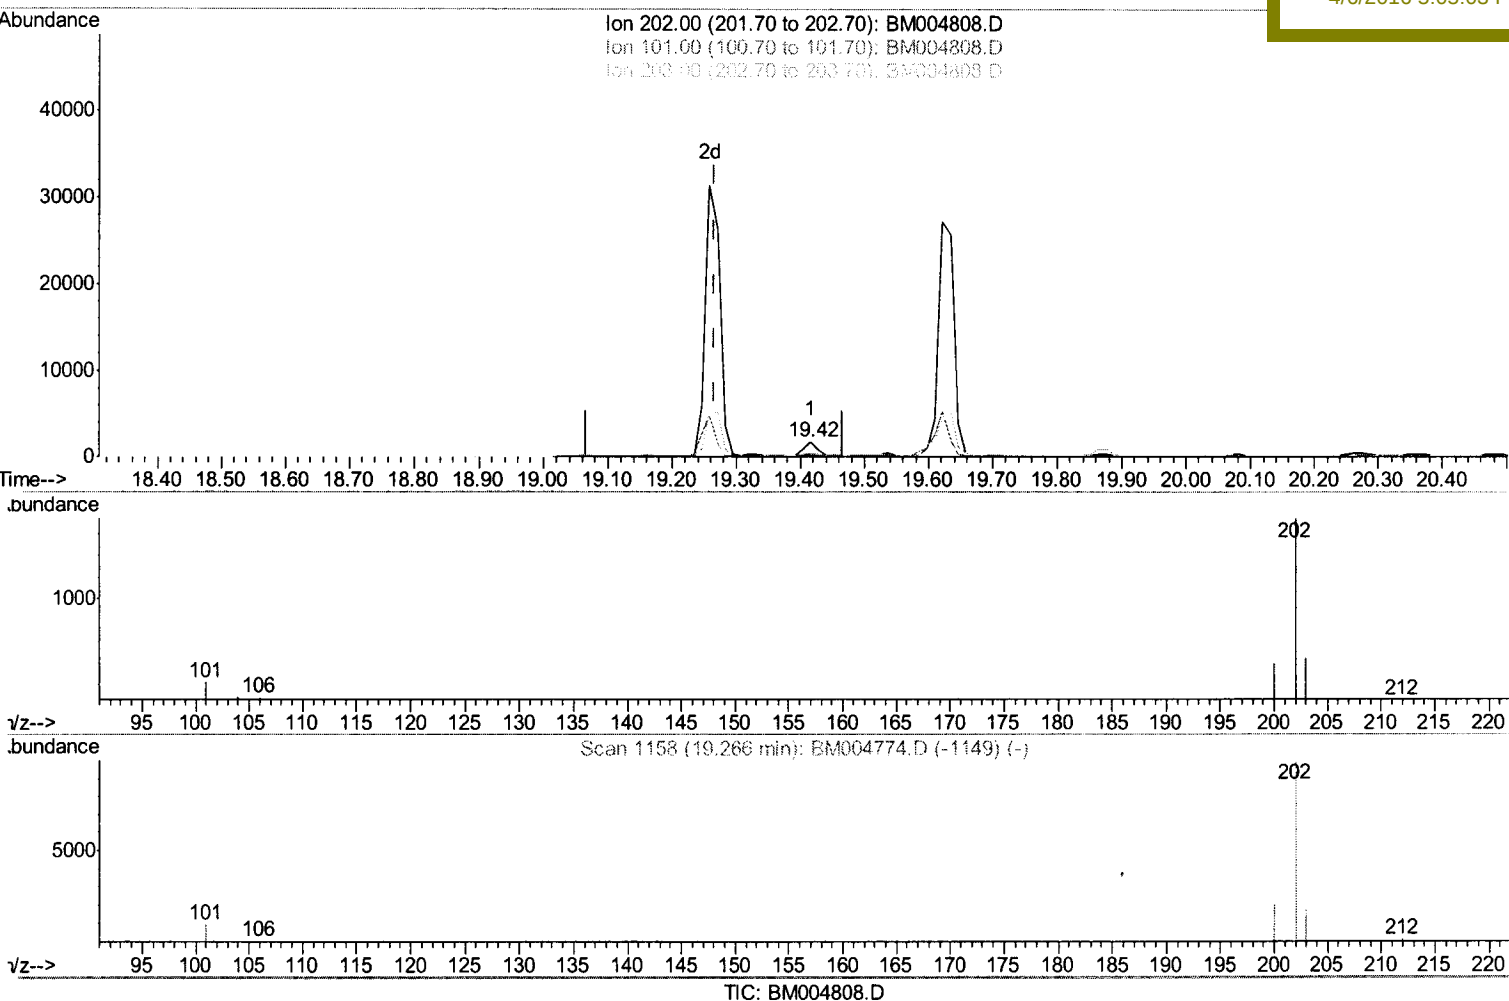

(17) Fluoranthene (C)

19.416min (+0.150) 0.13ng/ul

response 2297

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	12.88
203.00	16.30	25.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 20:06:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

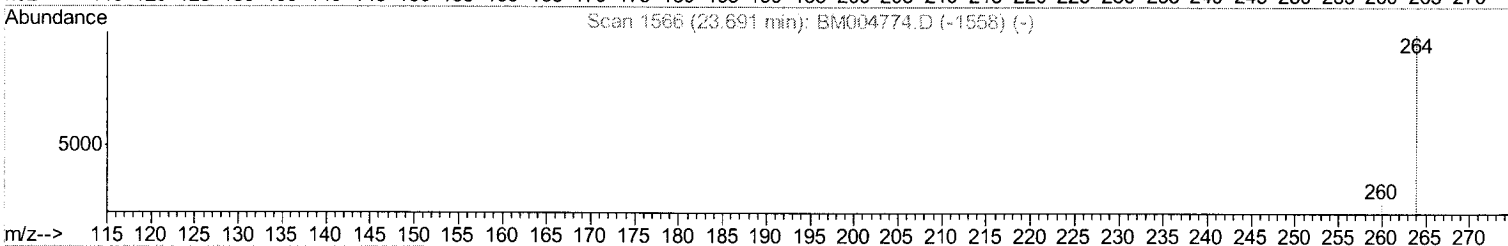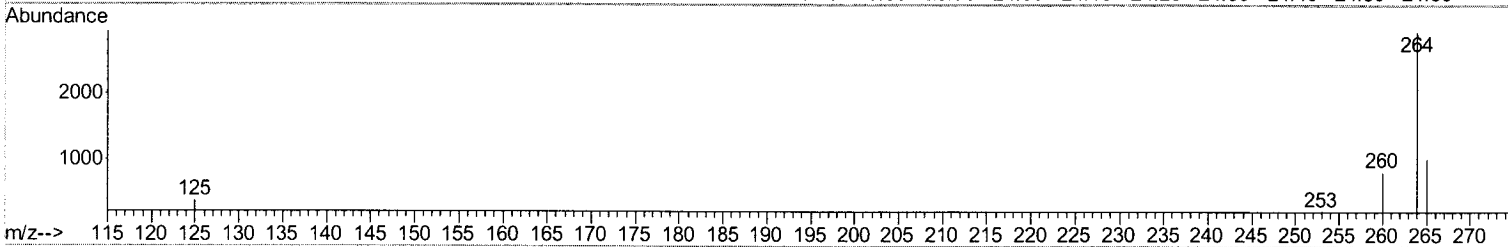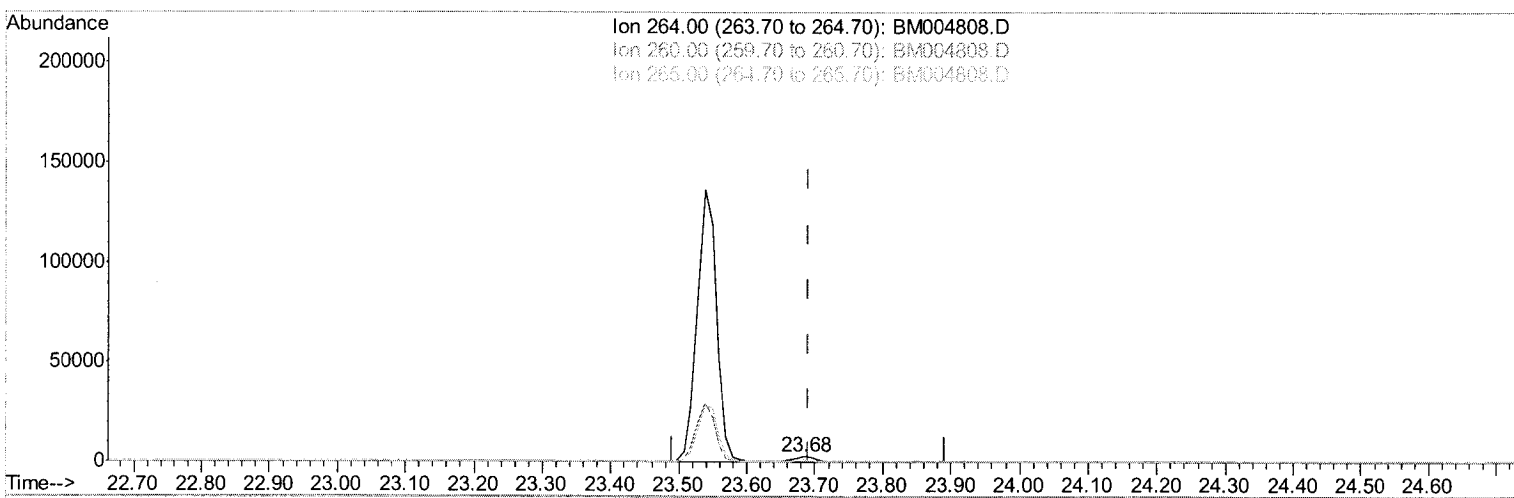

TIC: BM004808.D

(22) Perylene-d12 (I)

23.684min (-0.007) 0.40ng/ul m

response 5013

U.M
 04/07/16

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	27.70
265.00	38.20	34.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004808.D
Acq On : 28 Mar 2016 15:56
Operator : UM/SJ
Sample : H1909-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T46

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

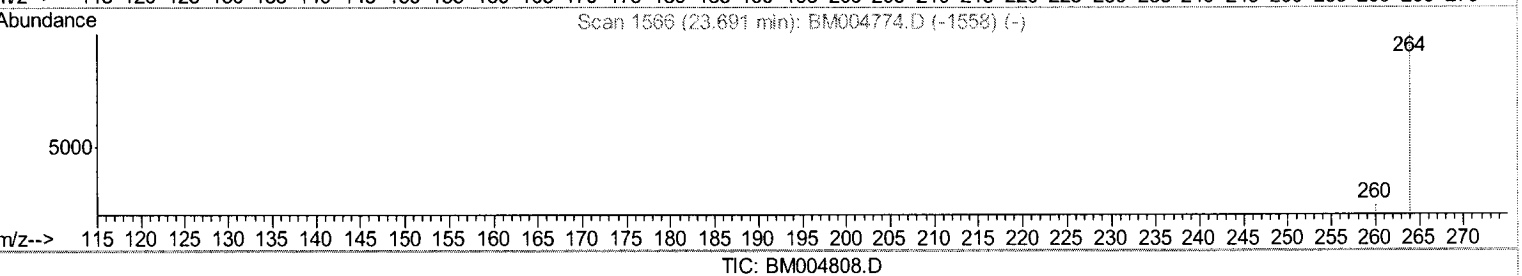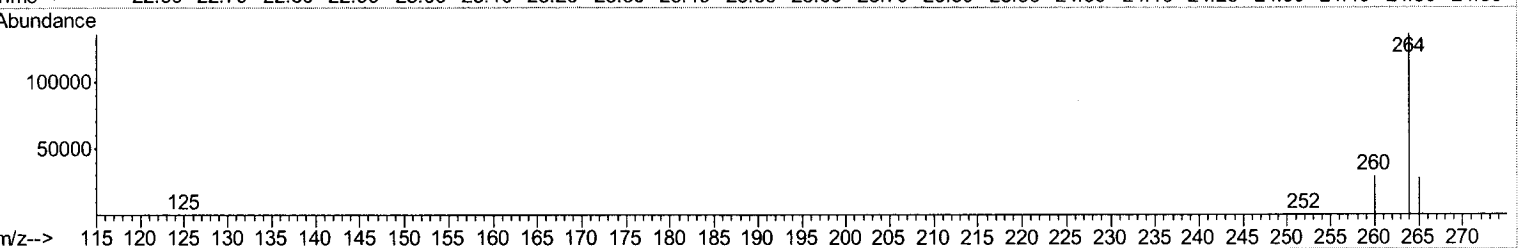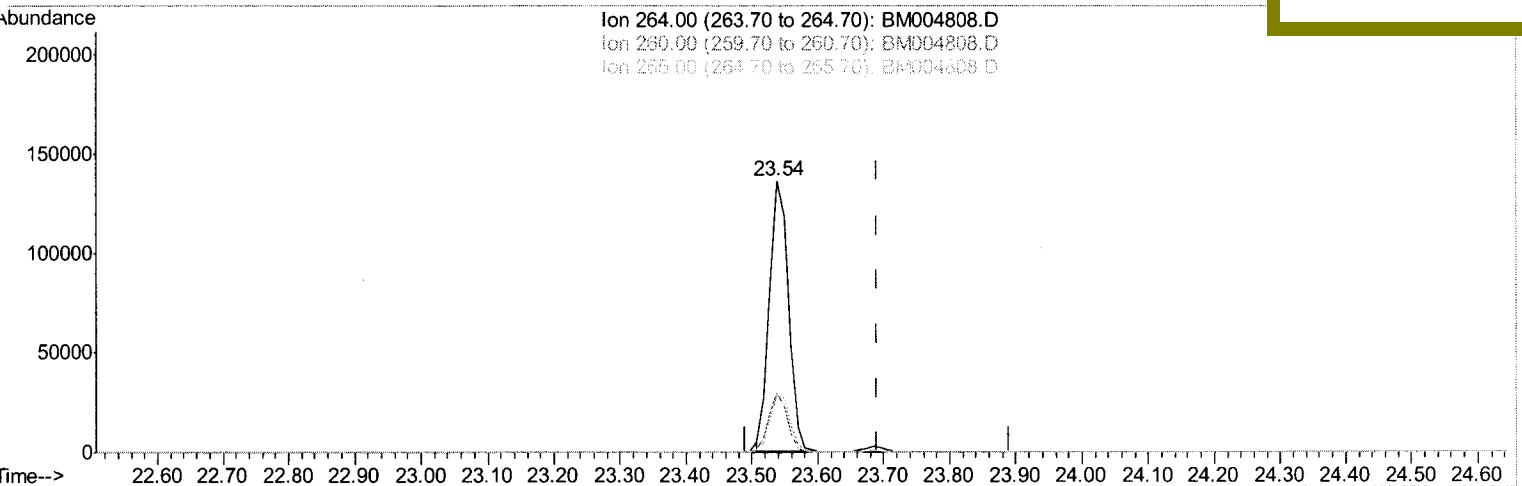

TIC: BM004808.D

(22) Perylene-d12 (I)

23.538min (-0.153) 0.40ng/ul

response 270071

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	21.74
265.00	38.20	20.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

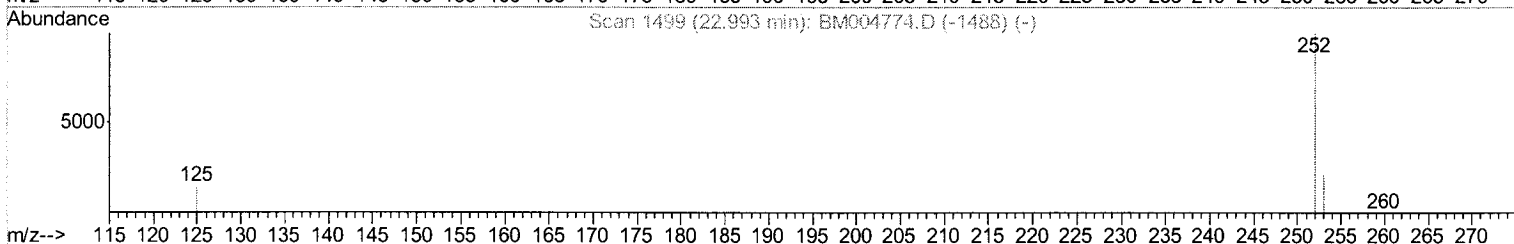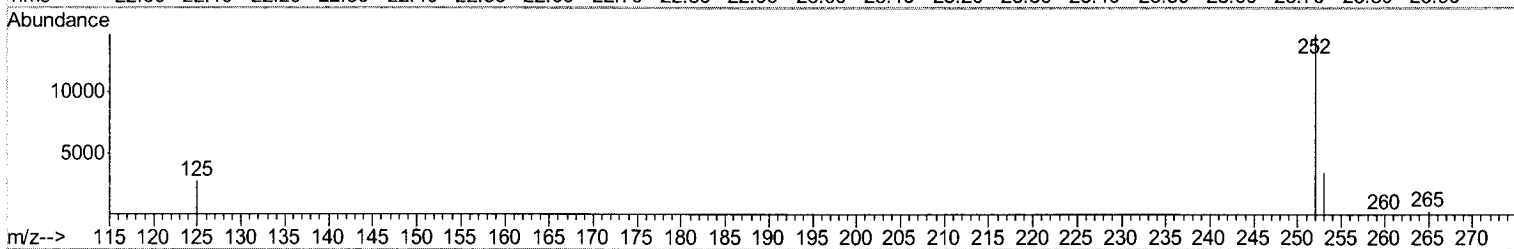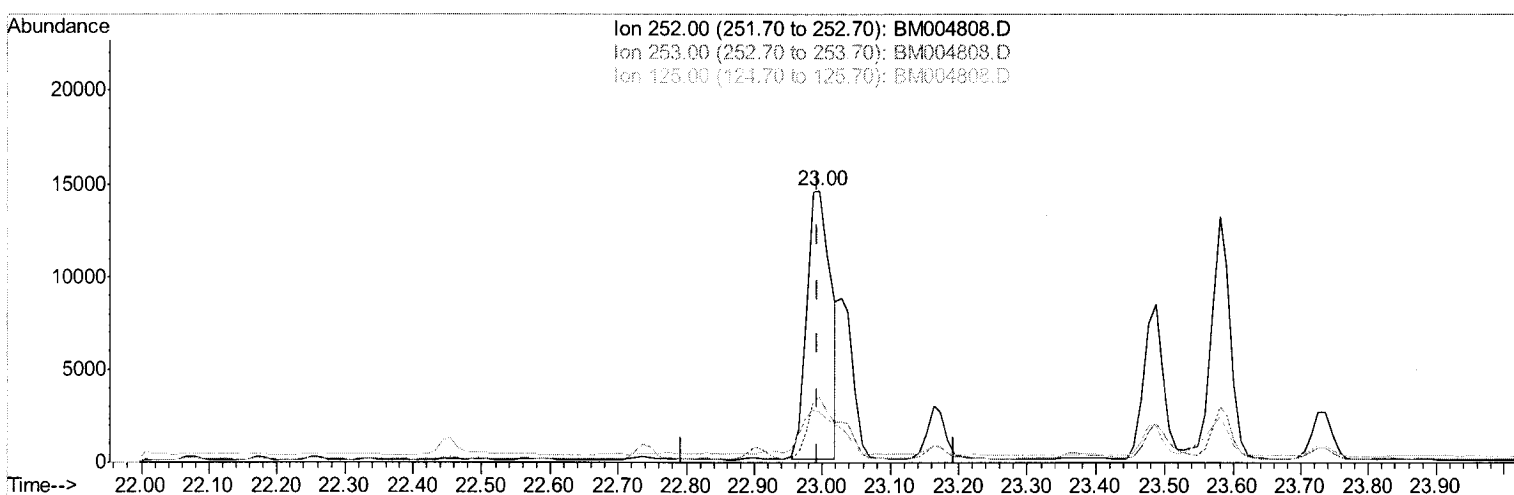

TIC: BM004808.D

(23) Benzo(b)fluoranthene

22.996min (+0.003) 2.77ng/ul m U.M

response 35912

04/07/16

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	23.91
125.00	14.40	18.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

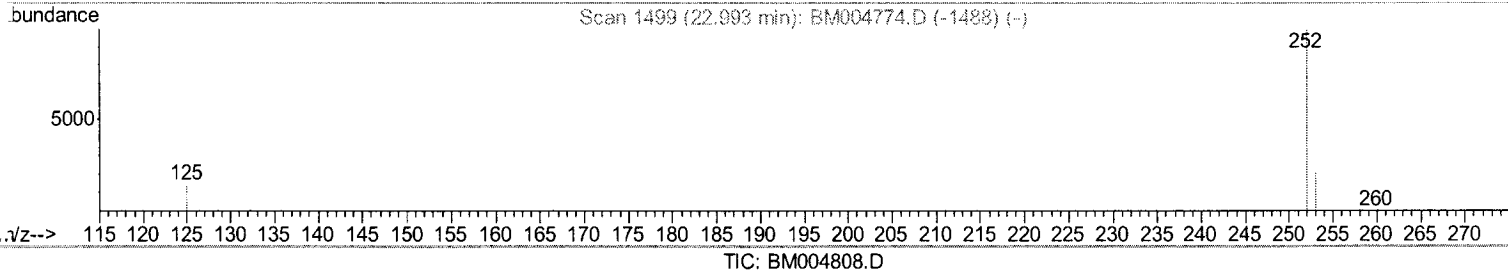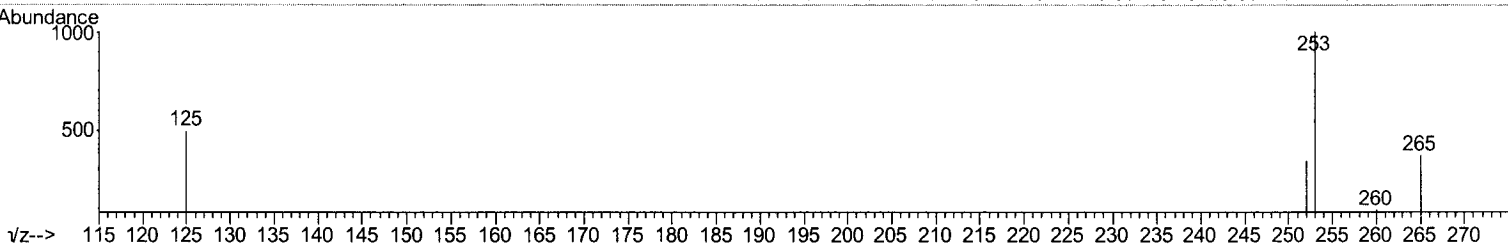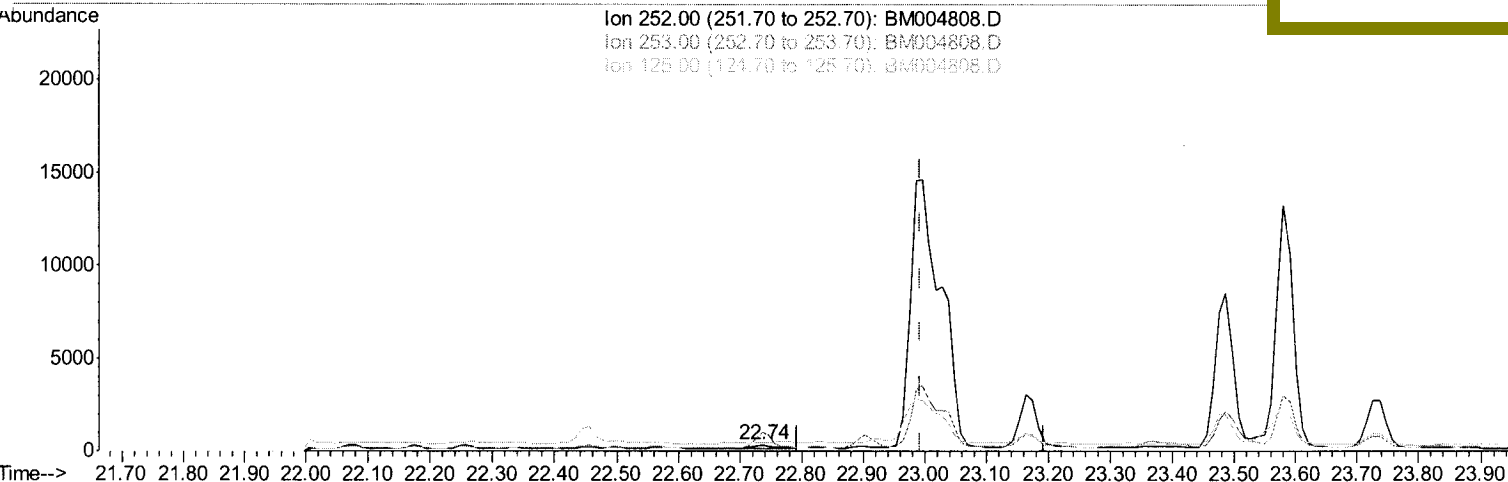

(23) Benzo(b)fluoranthene

22.736min (-0.257) 0.03ng/ul

response 417

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	291.59#
125.00	14.40	142.90#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

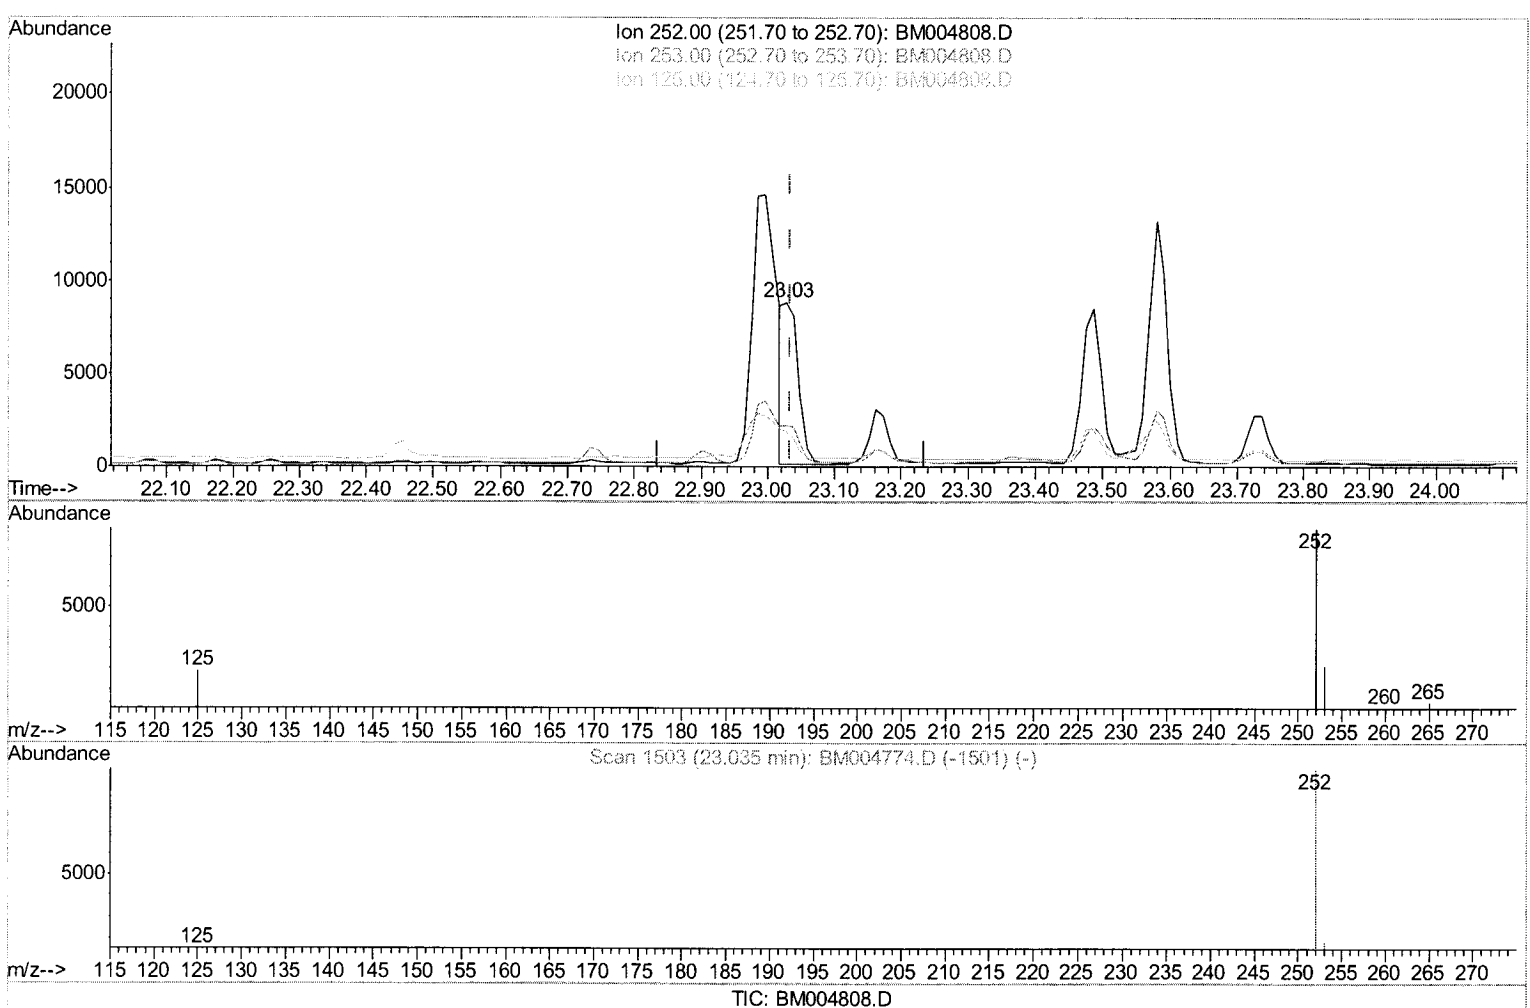

(24) Benzo(k)fluoranthene

23.028min (-0.007) 1.16ng/ul m

response 13928

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	24.38
125.00	13.00	21.07#
0.00	0.00	0.00




U.M
 24/07/16

Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004808.D
Acq On : 28 Mar 2016 15:56
Operator : UM/SJ
Sample : H1909-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T46

Quant Time: Apr 05 19:58:49 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Manual Integrations
APPROVED
Sohil
4/6/2016 5:05:03 PM

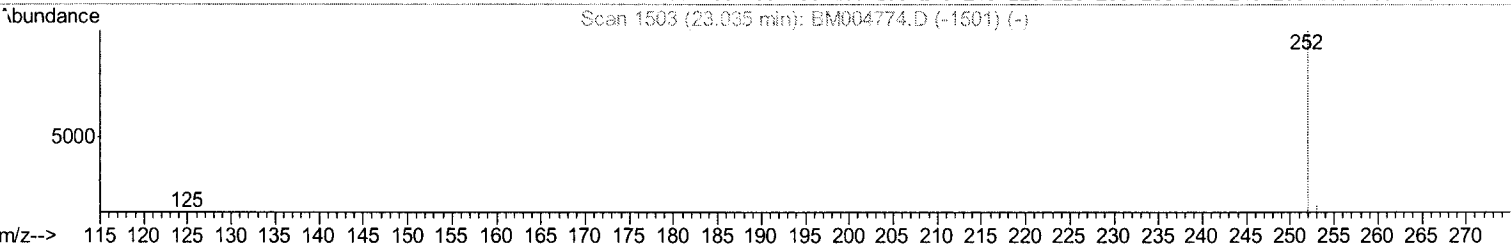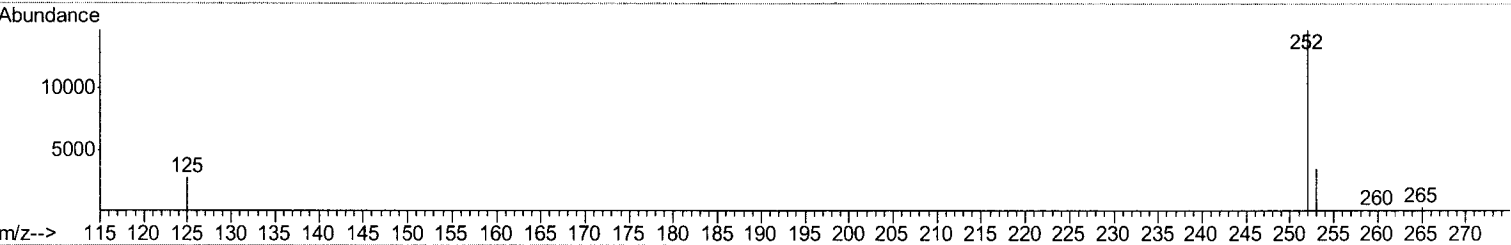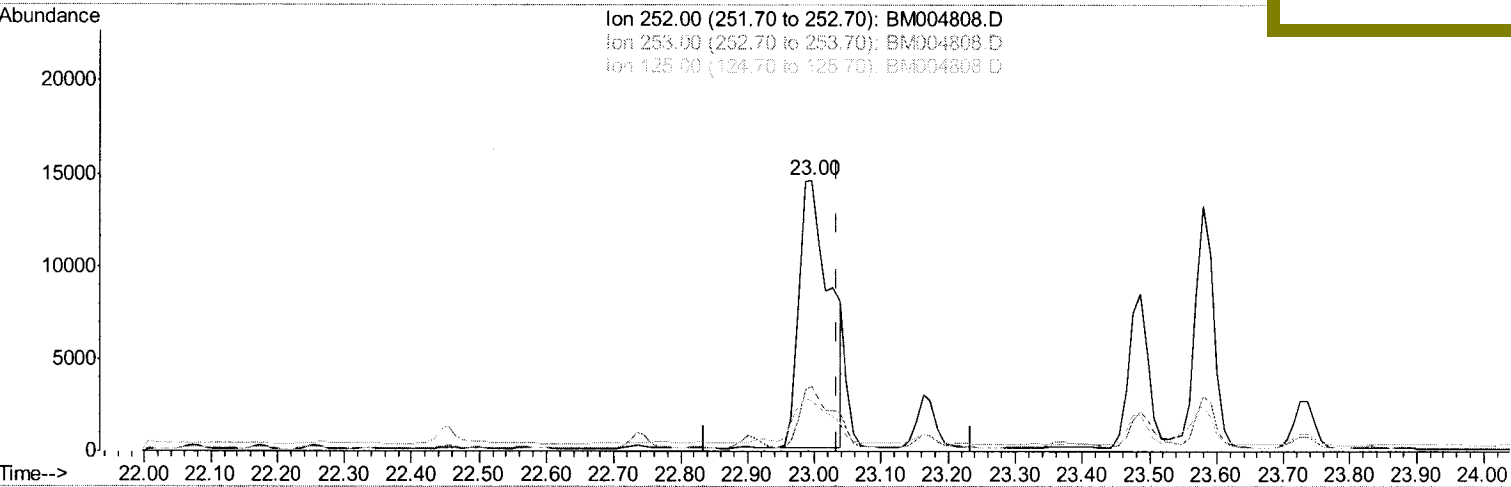

TIC: BM004808.D

(24) Benzo(k)fluoranthene

22.996min (-0.038) 3.87ng/ul

response 46512

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.91
125.00	13.00	18.83#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

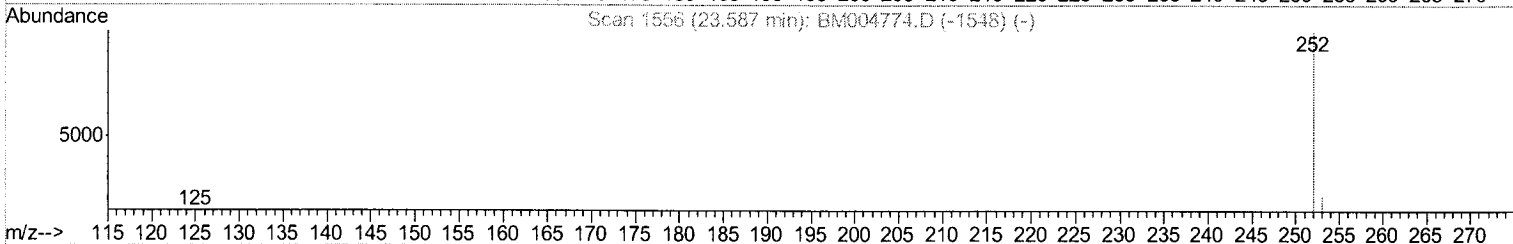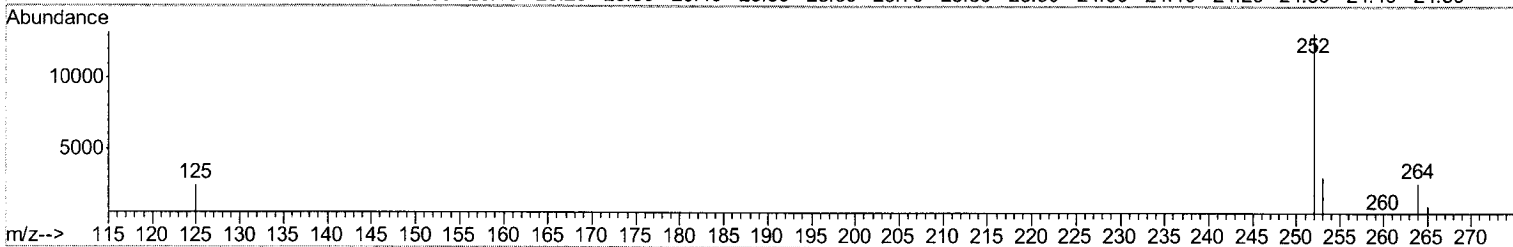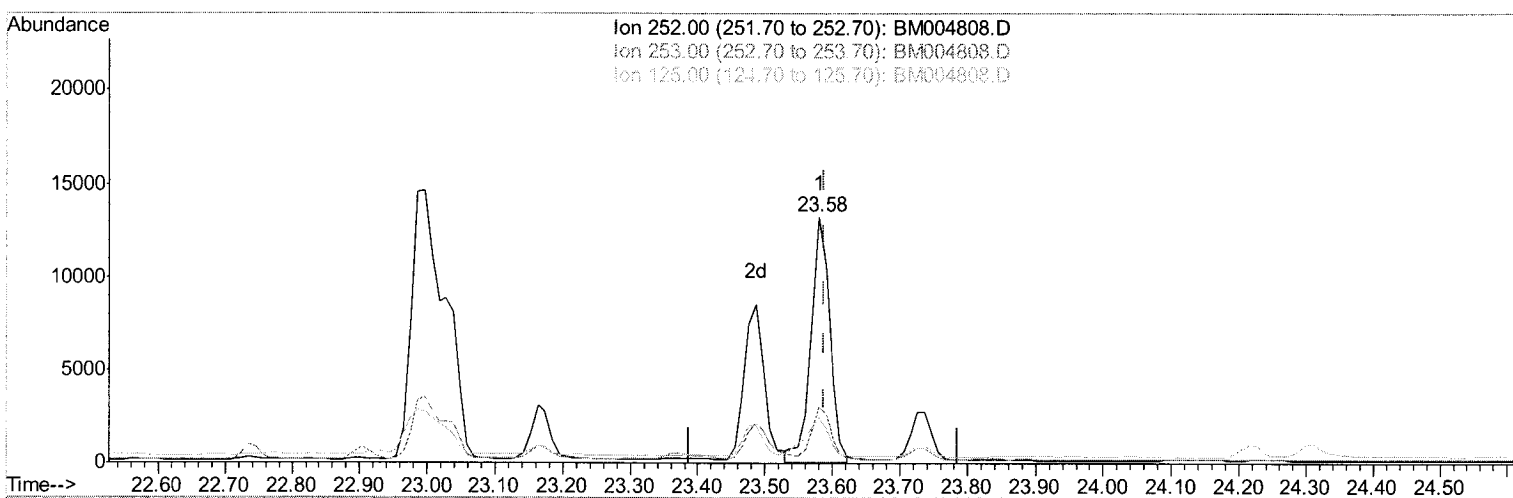

TIC: BM004808.D

(25) Benzo(a)pyrene (C)

23.580min (-0.007) 2.19ng/ul m U.M

response 26002

04/07/16


Ion	Exp%	Act%
252.00	100	100
253.00	24.30	22.85
125.00	15.90	18.69
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED
 Sohil
 4/6/2016 5:05:03 PM

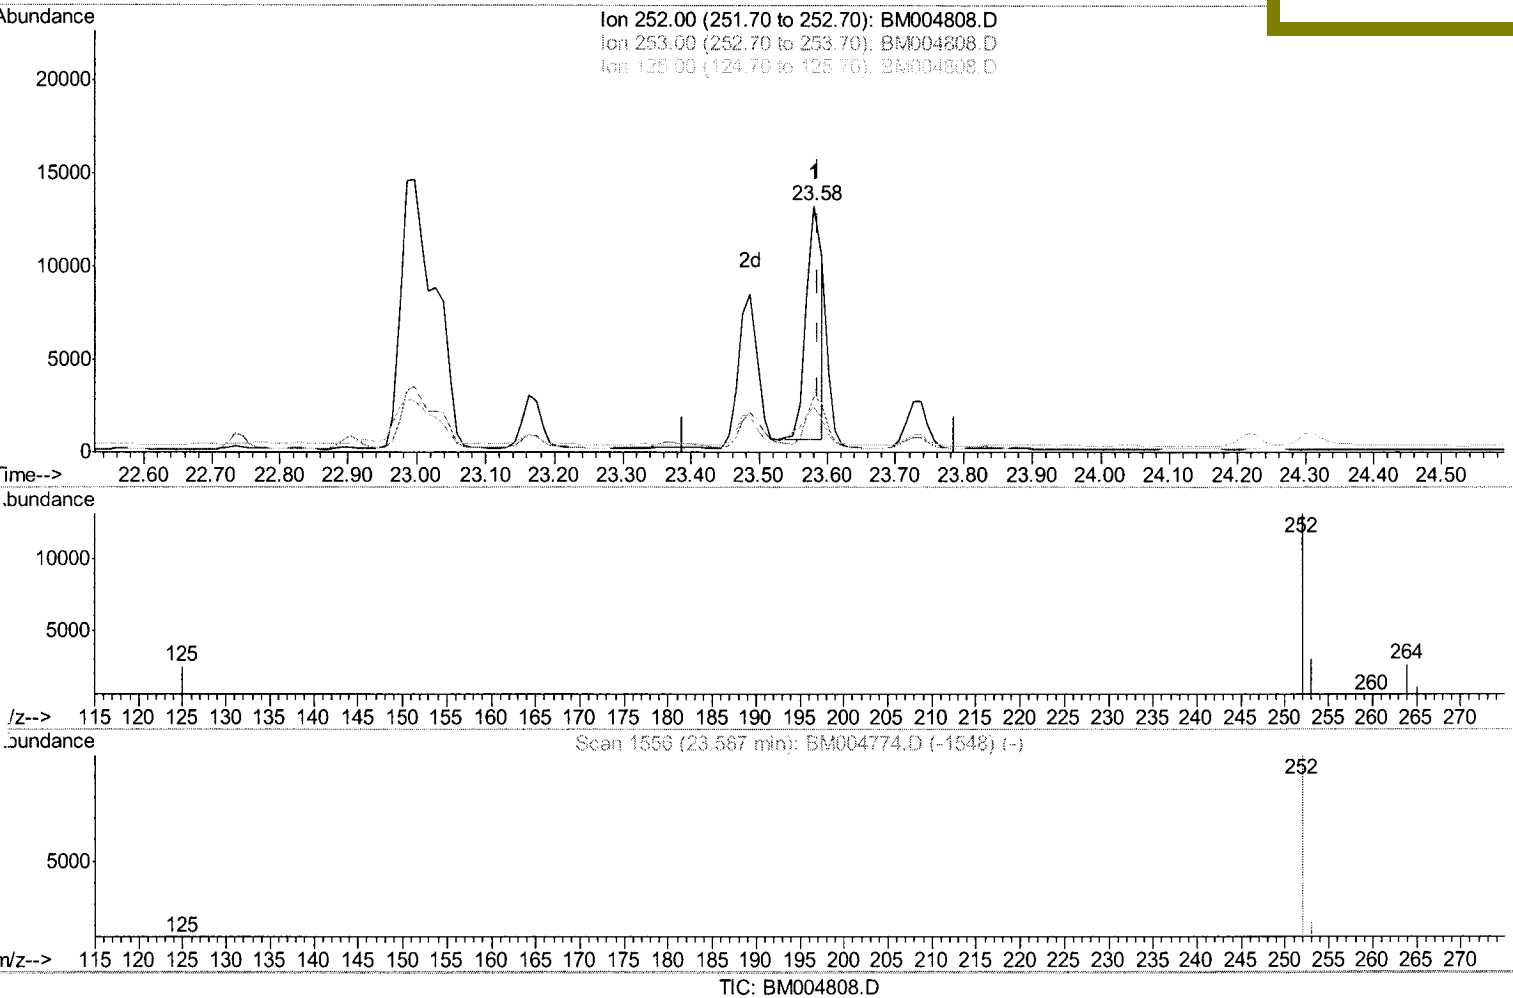

(25) Benzo(a)pyrene (C)

23.580min (-0.007) 1.69ng/ul

response 20098

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	22.85
125.00	15.90	18.69
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

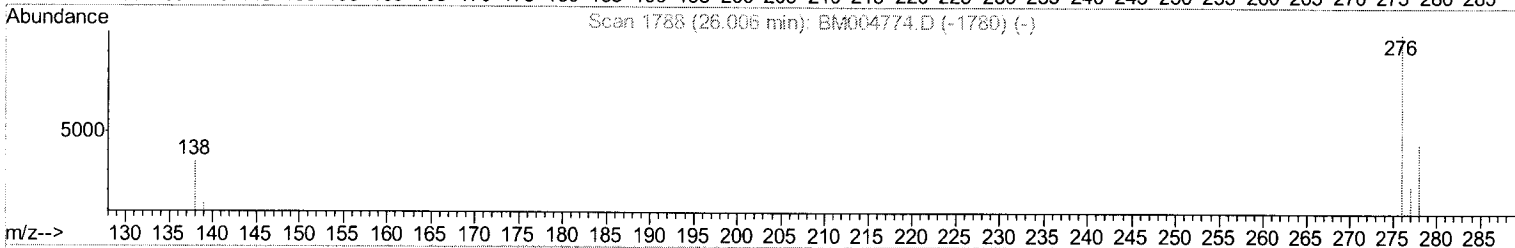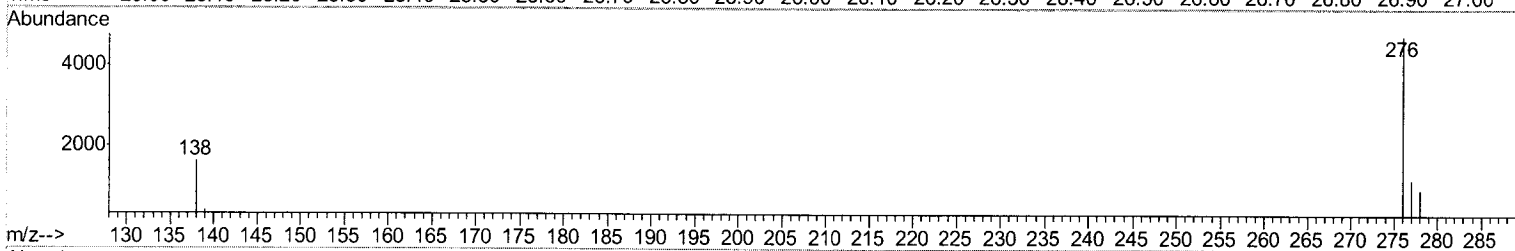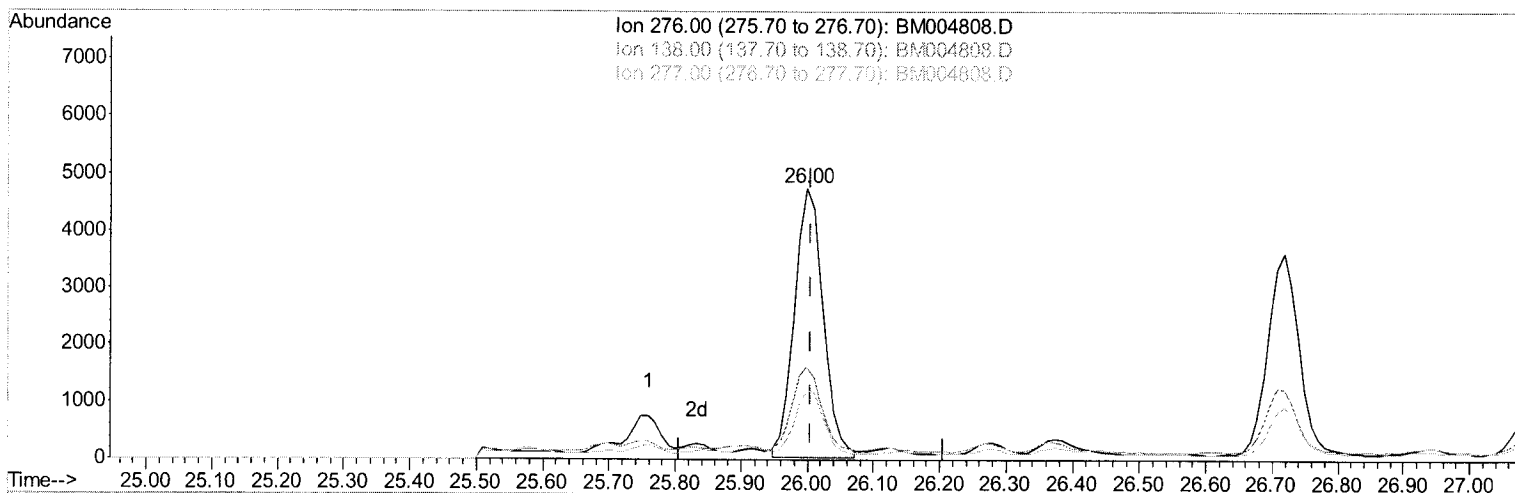

TIC: BM004808.D

(26) Indeno(1,2,3-cd)pyrene

25.999min (-0.007) 1.30ng/ul m U.M

response 14286

04/07/16

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	2.60#
277.00	24.80	3.70#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004808.D
Acq On : 28 Mar 2016 15:56
Operator : UM/SJ
Sample : H1909-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4T46

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

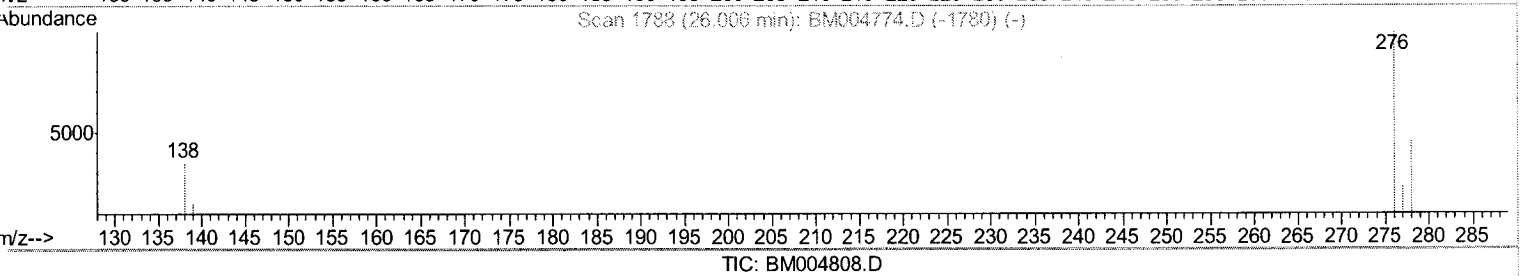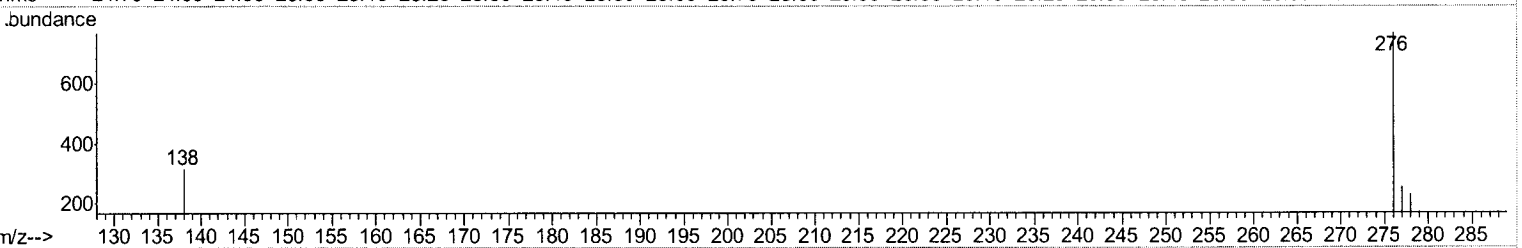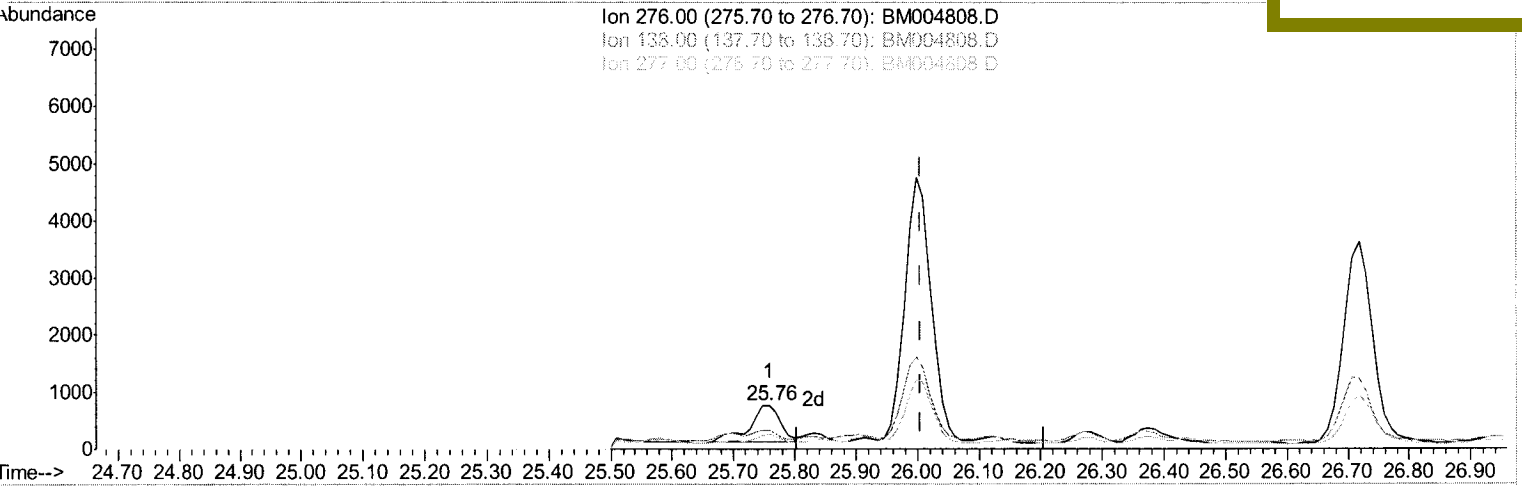

TIC: BM004808.D

(26) Indeno(1,2,3-cd)pyrene

25.759min (-0.247) 0.19ng/ul

response 2130

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	17.46
277.00	24.80	24.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

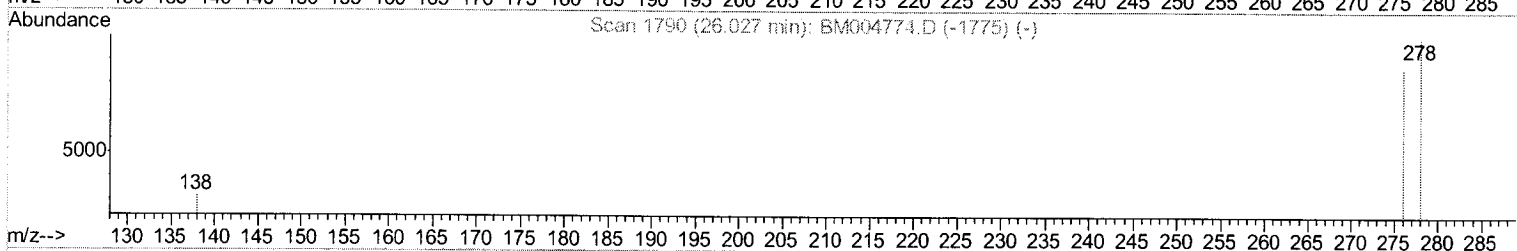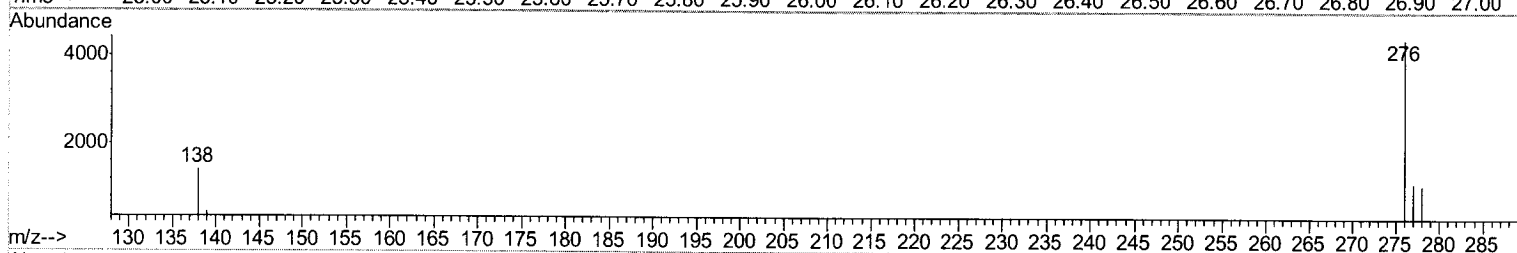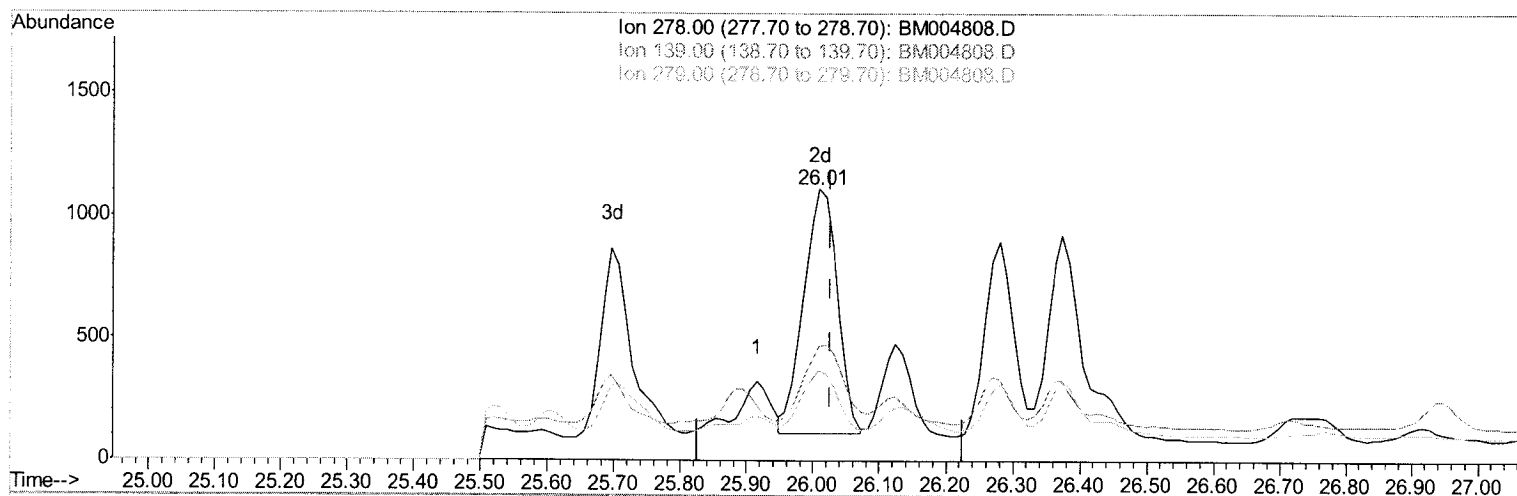

TIC: BM004808.D

(27) Dibenzo(a,h)anthracene

26.009min (-0.018) 0.41ng/ul m *U.M*
24/07/16
 response 3584

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	42.09#
279.00	25.20	33.09#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004808.D
Acq On : 28 Mar 2016 15:56
Operator : UM/SJ
Sample : H1909-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4T46

Quant Time: Apr 05 19:58:49 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:03 PM

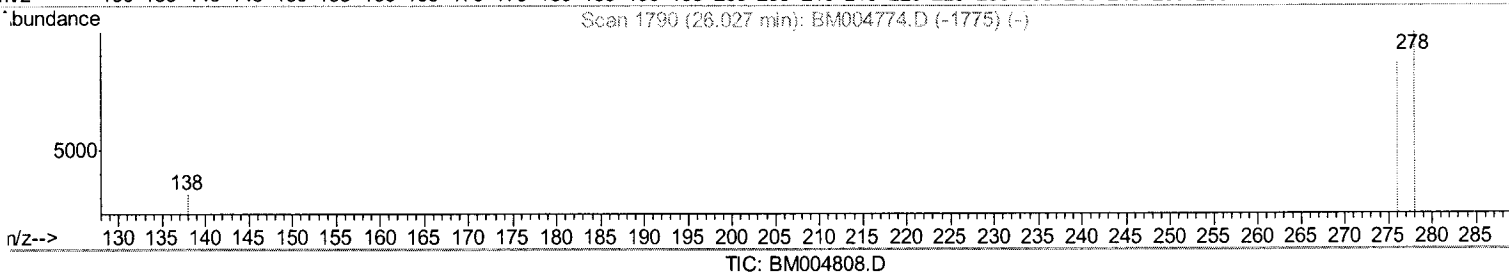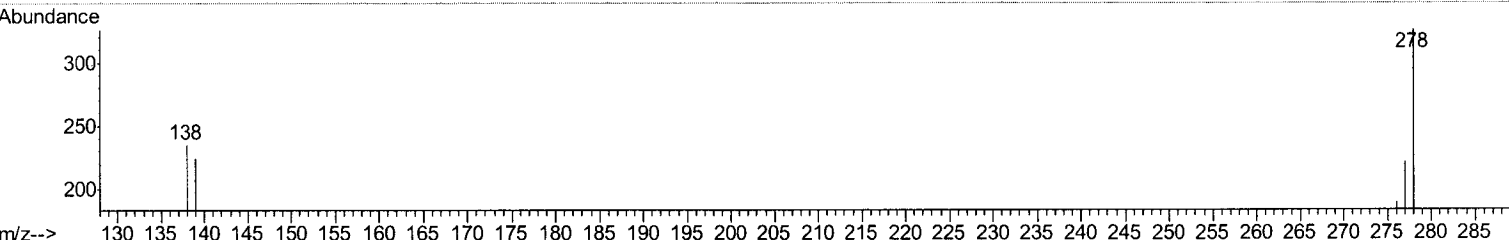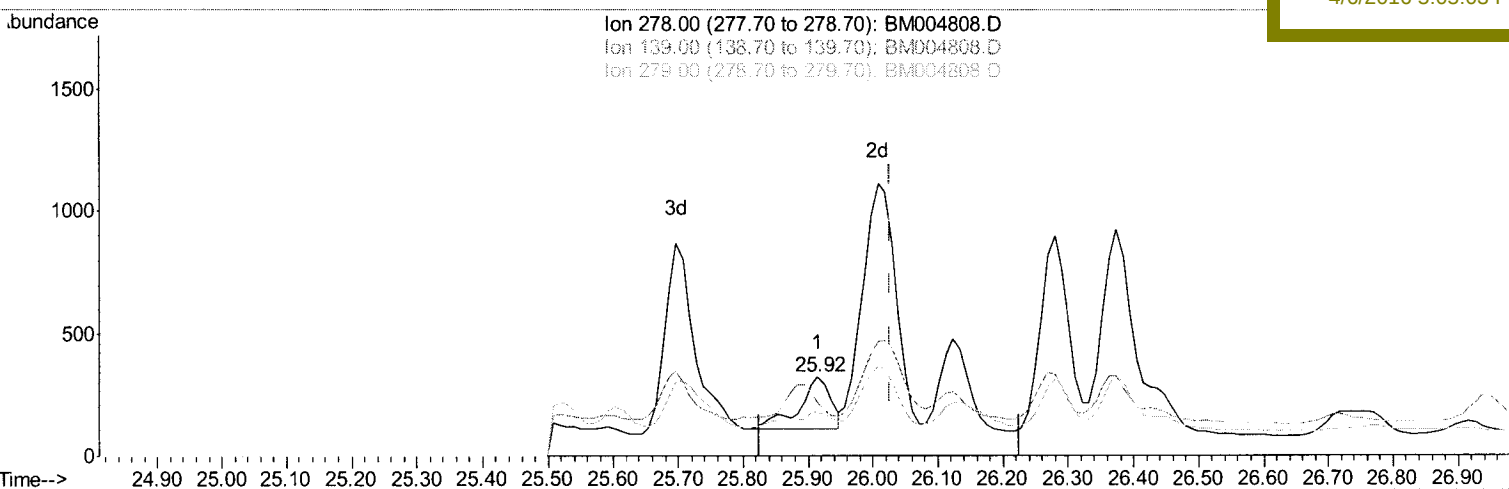

(27) Dibenzo(a,h)anthracene

25.915min (-0.111) 0.08ng/ul

response 734

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	68.71#
279.00	25.20	56.13#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 A4T46

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Quant Time: Apr 05 19:58:49 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

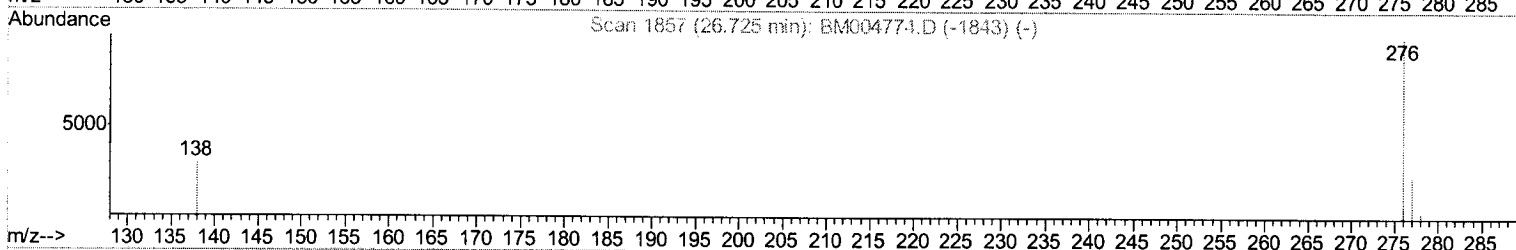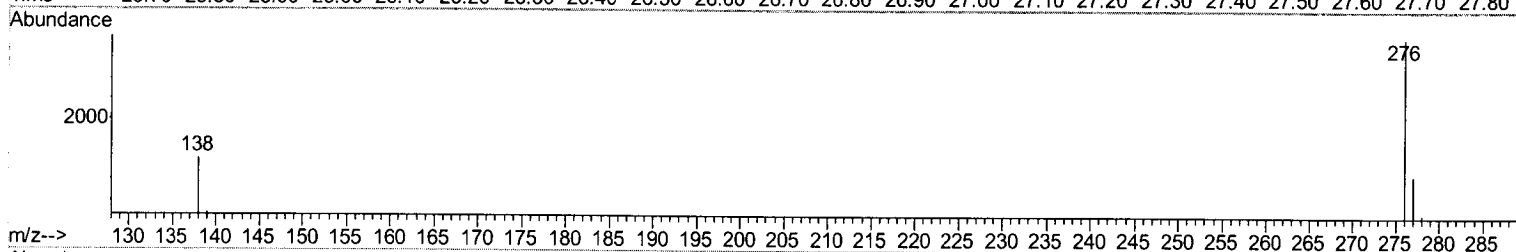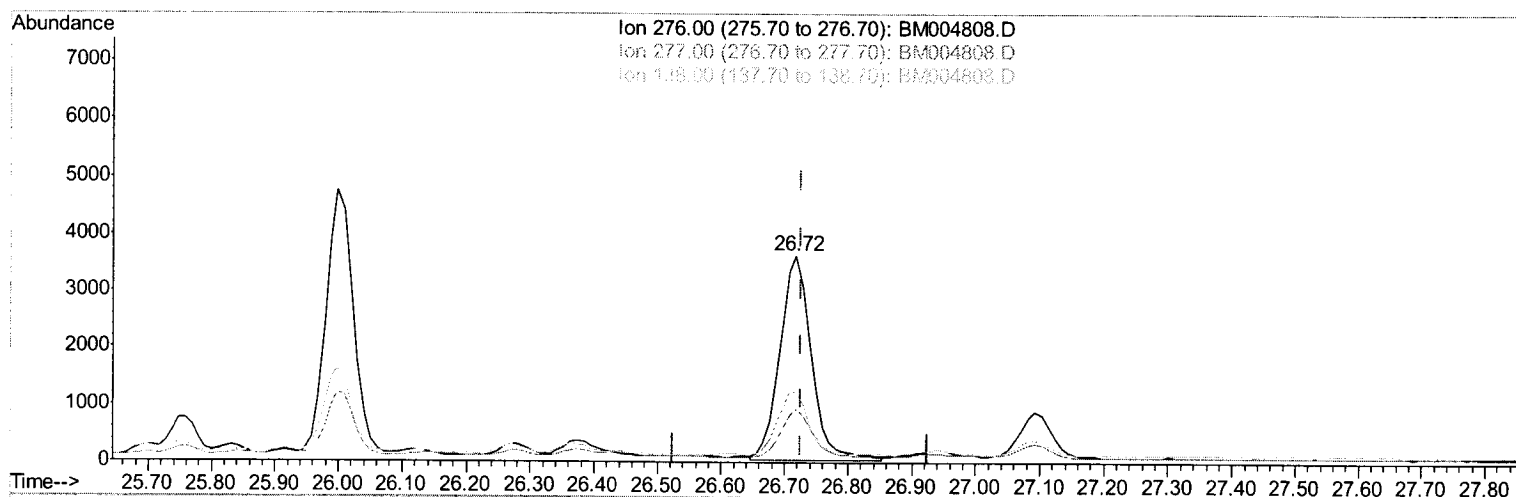

TIC: BM004808.D

(28) Benzo(g,h,i)perylene

26.718min (-0.007) 1.36ng/ul m U.M
 response 12332 04/07/16

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	25.36
138.00	28.10	33.87#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM032816\
Data File : BM004808.D
Acq On : 28 Mar 2016 15:56
Operator : UM/SJ
Sample : H1909-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Apr 05 19:58:49 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 18:29:16 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4T46

Manual Integrations
APPROVED

Sohil
4/6/2016 5:05:03 PM

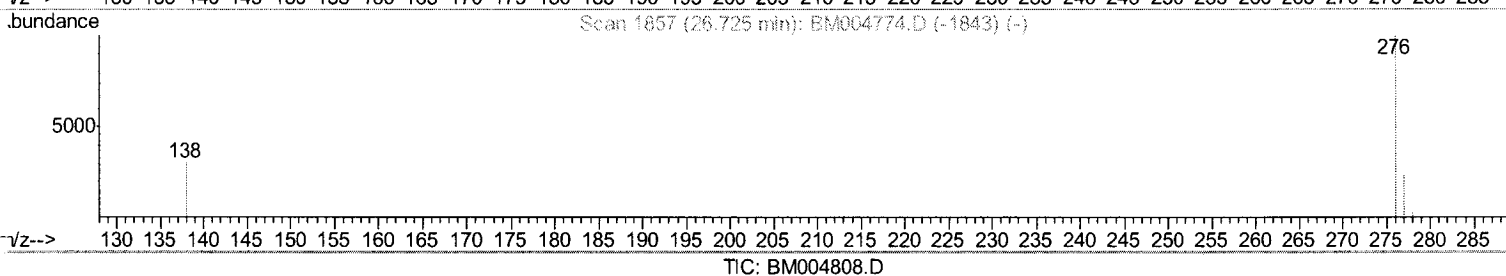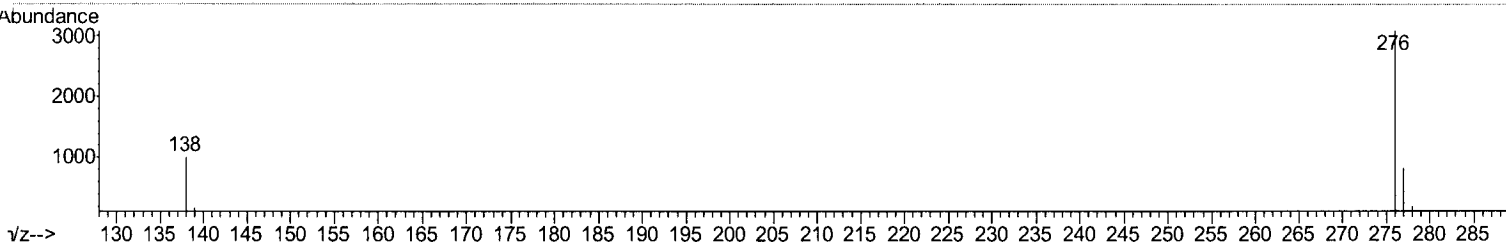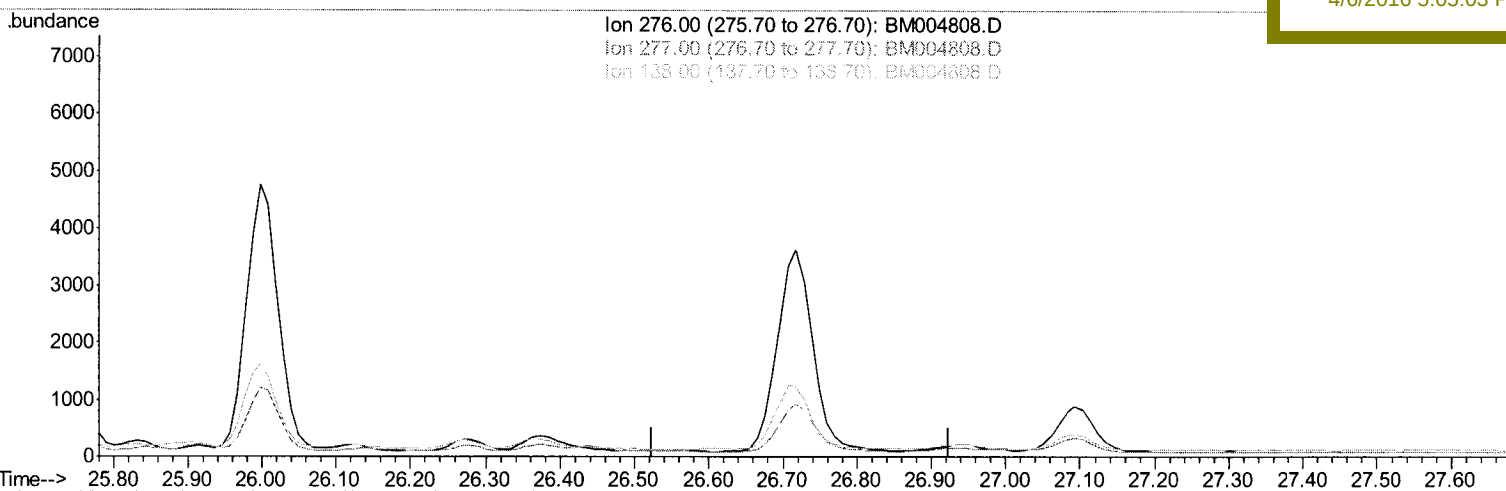

TIC: BM004808.D

(28) Benzo(g,h,i)perylene

26.725min (-26.725) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	23.60	0.00#
138.00	28.10	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032816\
 Data File : BM004808.D
 Acq On : 28 Mar 2016 15:56
 Operator : UM/SJ
 Sample : H1909-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T46

Quant Time: Apr 06 14:34:42 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 18:29:16 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 4/6/2016 5:05:03 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	928	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	4244	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.47	164	2496	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.21	188	5597m	0.40	ng/ul	0.00
18) Chrysene-d12	21.39	240	5962	0.40	ng/ul	0.00
22) Perylene-d12	23.68	264	5013m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.32	96	3034	7.26	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.21	152	1335	0.23	ng/ul	0.00
16) Fluoranthene-d10	19.23	212	3456	0.26	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Naphthalene	10.67	128	2460	0.24	ng/ul#	91
7) 2-Methylnaphthalene	12.28	142	368	0.05	ng/ul	99
9) Acenaphthylene	14.18	152	3630	0.32	ng/ul#	94
10) Acenaphthene	14.52	153	291	0.04	ng/ul#	85
11) Fluorene	15.51	166	751	0.08	ng/ul#	86
14) Phenanthrene	17.25	178	13791	0.88	ng/ul	96
15) Anthracene	17.33	178	4232	0.28	ng/ul	95
17) Fluoranthene	19.26	202	49244m	2.75	ng/ul	98
19) Pyrene	19.62	202	45379	2.22	ng/ul	98
20) Benzo(a)anthracene	21.37	228	27113	1.48	ng/ul#	91
21) Chrysene	21.42	228	28061	1.58	ng/ul	94
23) Benzo(b)fluoranthene	23.00	252	35912m	2.13	ng/ul	
24) Benzo(k)fluoranthene	23.03	252	13928m	0.89	ng/ul	
25) Benzo(a)pyrene	23.58	252	26002m	1.68	ng/ul	
26) Indeno(1,2,3-cd)pyrene	26.00	276	14286m	1.00	ng/ul	
27) Dibenzo(a,h)anthracene	26.01	278	3584m	0.32	ng/ul	
28) Benzo(g,h,i)perylene	26.72	276	12332m	1.04	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed