

Data Path : Z:\HPCHEM1\BNA M\DATA\BM032817\
 Data File : BM009417.D
 Acq On : 27 Mar 2017 17:59
 Operator : SJ/MA
 Sample : I2358-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BM3

Quant Time: Mar 28 02:24:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 28 02:24:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	116890	20.00	ng/ul	0.00
18) Naphthalene-d8	10.65	136	468943	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.50	164	286179	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	662709	20.00	ng/ul	0.00
77) Chrysene-d12	21.42	240	940460	20.00	ng/ul	0.00
85) Perylene-d12	23.74	264	929870	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	15940	5.20	ng/uL	0.00
5) Phenol-d5	7.01	99	70052	6.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	209777	27.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.39	132	168982	23.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	119650	15.16	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	96057	27.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.74	143	97000	25.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.27	165	193103	26.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.80	131	15759	1.86	ng/ul	0.01
43) Dimethylphthalate-d6	13.90	166	643157	31.96	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	786270	31.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	19253	5.19	ng/ul	0.00
57) Fluorene-d10	15.49	176	594176	32.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	95308	22.75	ng/ul	0.00
70) Anthracene-d10	17.34	188	988468	31.27	ng/ul	0.00
78) Pyrene-d10	19.64	212	1205988	30.25	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.60	264	1312802	30.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.95	163	53868	2.68	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM032817\
Data File : BM009417.D
Acq On : 27 Mar 2017 17:59
Operator : SJ/MA
Sample : I2358-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BM3

Quant Time: Mar 28 02:24:52 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 28 02:24:25 2017
Response via : Initial Calibration

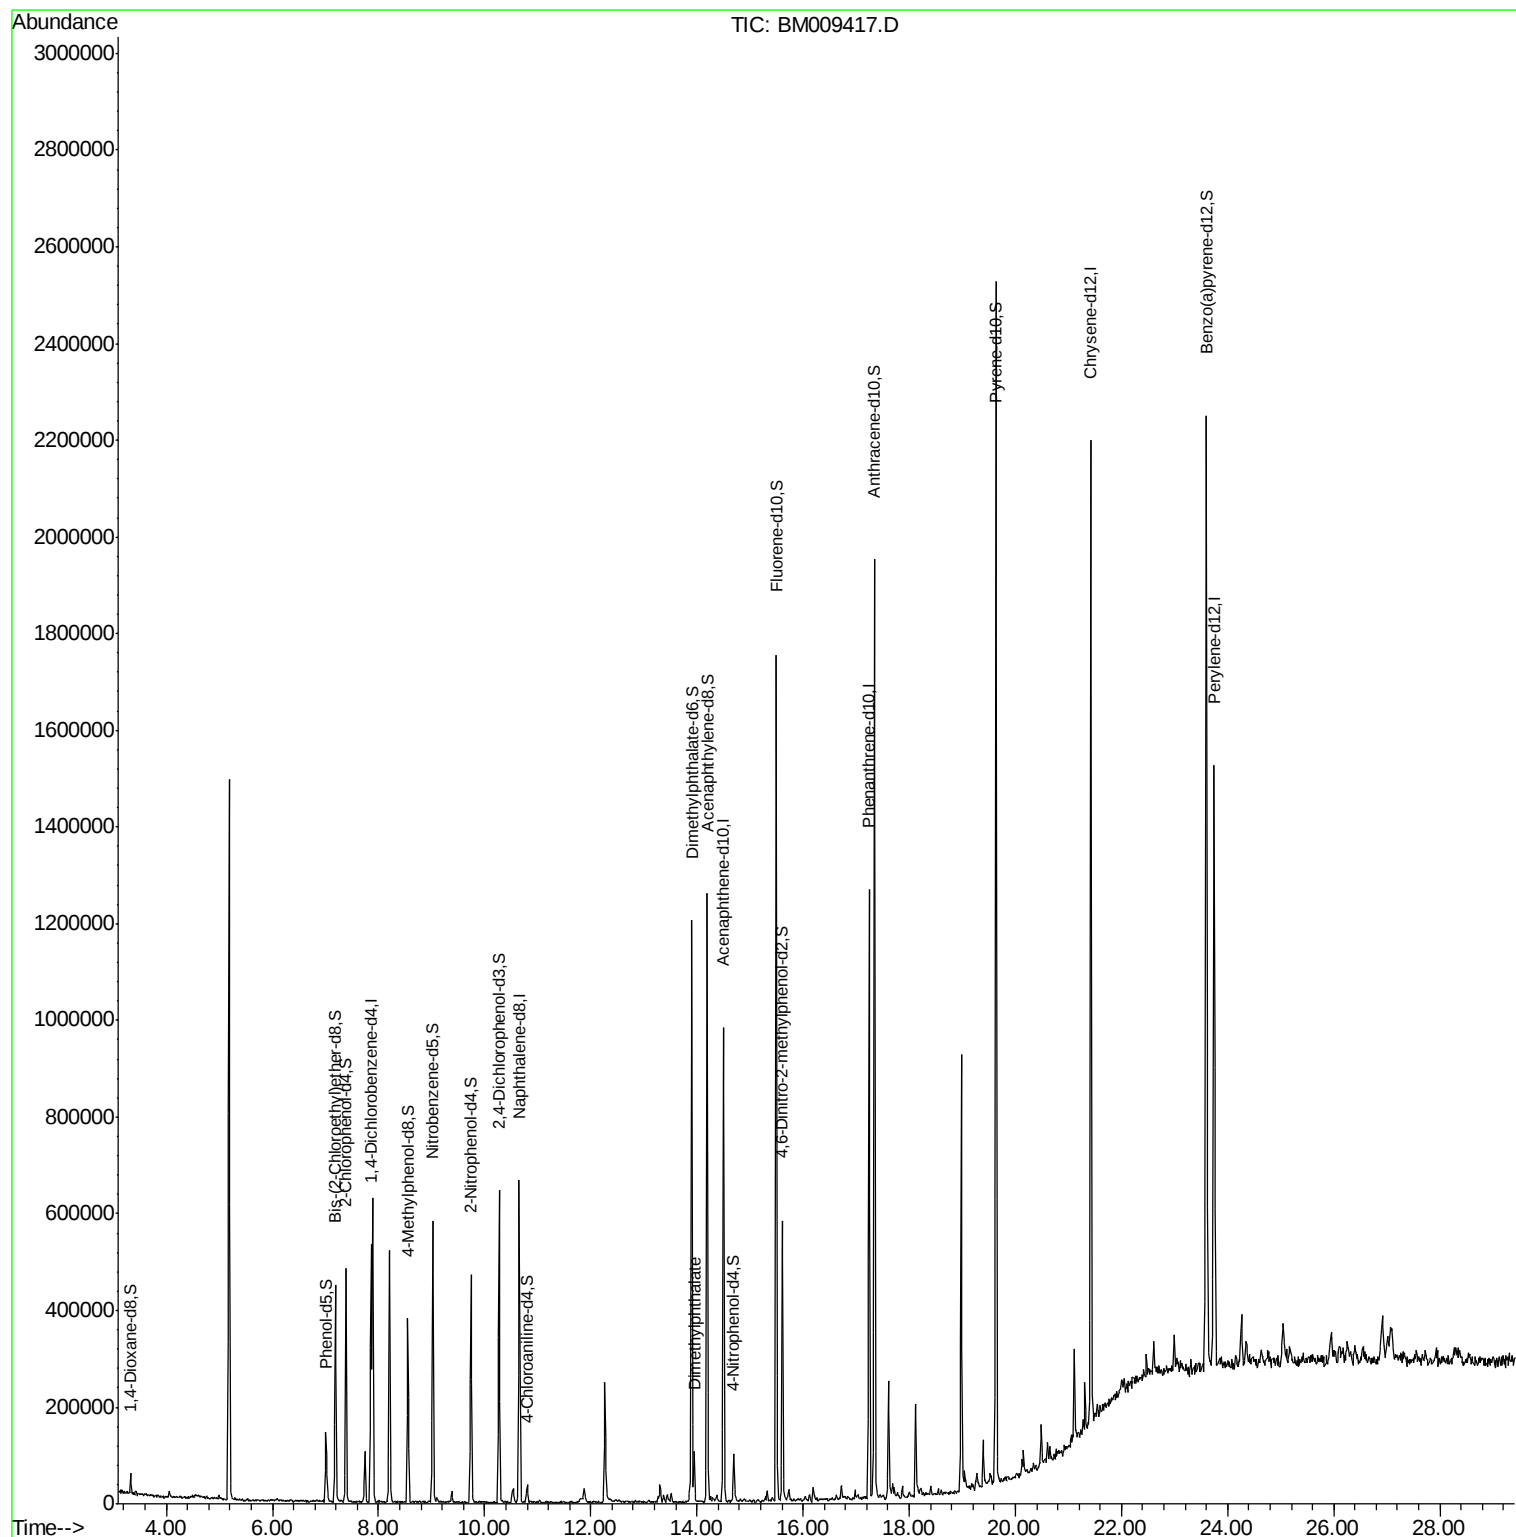

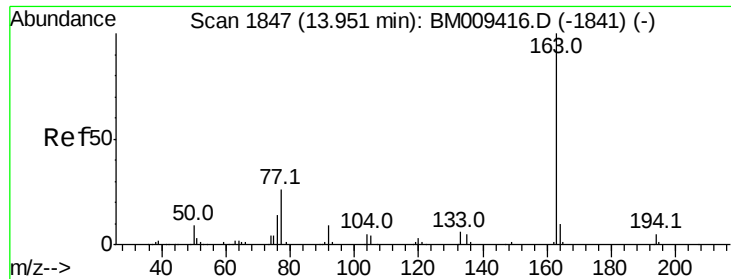

#44

Dimethylphthalate

Concen: 2.68 ng/ul

RT: 13.95 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BM009417.D

Acq: 27 Mar 2017 17:59

Instrument :

BNA_M

ClientSampleId :

C0BM3

Tot Ion:163 Resp: 53868

Ion Ratio Lower Upper

163 100

194 5.5 3.2 4.8#

164 9.9 7.8 11.8

