

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
 Data File : BM009420.D
 Acq On : 27 Mar 2017 19:47
 Operator : SJ/MA
 Sample : I2372-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9XZ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rBV	53320	68497	1.63%	0.179%
2	7.004	660	666	674	rVV	183314	294053	6.99%	0.769%
3	7.181	690	696	709	rBV	643760	1012095	24.04%	2.647%
4	7.381	721	730	741	rBV	703127	1116096	26.52%	2.919%
5	7.851	804	810	816	rBV	587719	920532	21.87%	2.408%
6	8.545	922	928	936	rBV	501279	784382	18.63%	2.052%
7	9.016	1000	1008	1017	rBV	844882	1366786	32.47%	3.575%
8	9.734	1121	1130	1139	rBV	678959	1099816	26.13%	2.877%
9	10.263	1213	1220	1230	rBV	907166	1494013	35.49%	3.908%
10	10.651	1279	1286	1293	rBV	713018	1221906	29.03%	3.196%
11	13.904	1829	1839	1847	rBV	1618074	2273551	54.01%	5.947%
12	14.186	1881	1887	1897	rBV	1217449	1764335	41.92%	4.615%
13	14.498	1932	1940	1948	rBV2	962128	1518673	36.08%	3.972%
14	14.686	1967	1972	1982	rBV2	114673	195927	4.65%	0.512%
15	15.486	2102	2108	2117	rBV	2346822	3366687	79.98%	8.806%
16	15.610	2123	2129	2138	rBV	829126	1140452	27.09%	2.983%
17	17.245	2400	2407	2417	rBV2	1240591	1781210	42.32%	4.659%
18	17.345	2417	2424	2433	rBV	2486383	3613689	85.85%	9.452%
19	19.268	2746	2751	2757	rBV	29650	42241	1.00%	0.110%
20	19.527	2790	2795	2802	rVB4	26614	43918	1.04%	0.115%
21	19.633	2806	2813	2822	rBV	3027536	4209267	100.00%	11.010%
22	21.415	3111	3116	3124	rBV	1859319	2409255	57.24%	6.302%
23	23.591	3479	3486	3497	rBV	2091015	4190754	99.56%	10.962%
24	23.739	3505	3511	3522	rVB2	1181359	2302458	54.70%	6.023%


Sum of corrected areas: 38230593

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
Data File : BM009420.D
Acq On : 27 Mar 2017 19:47
Operator : SJ/MA
Sample : I2372-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XZ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

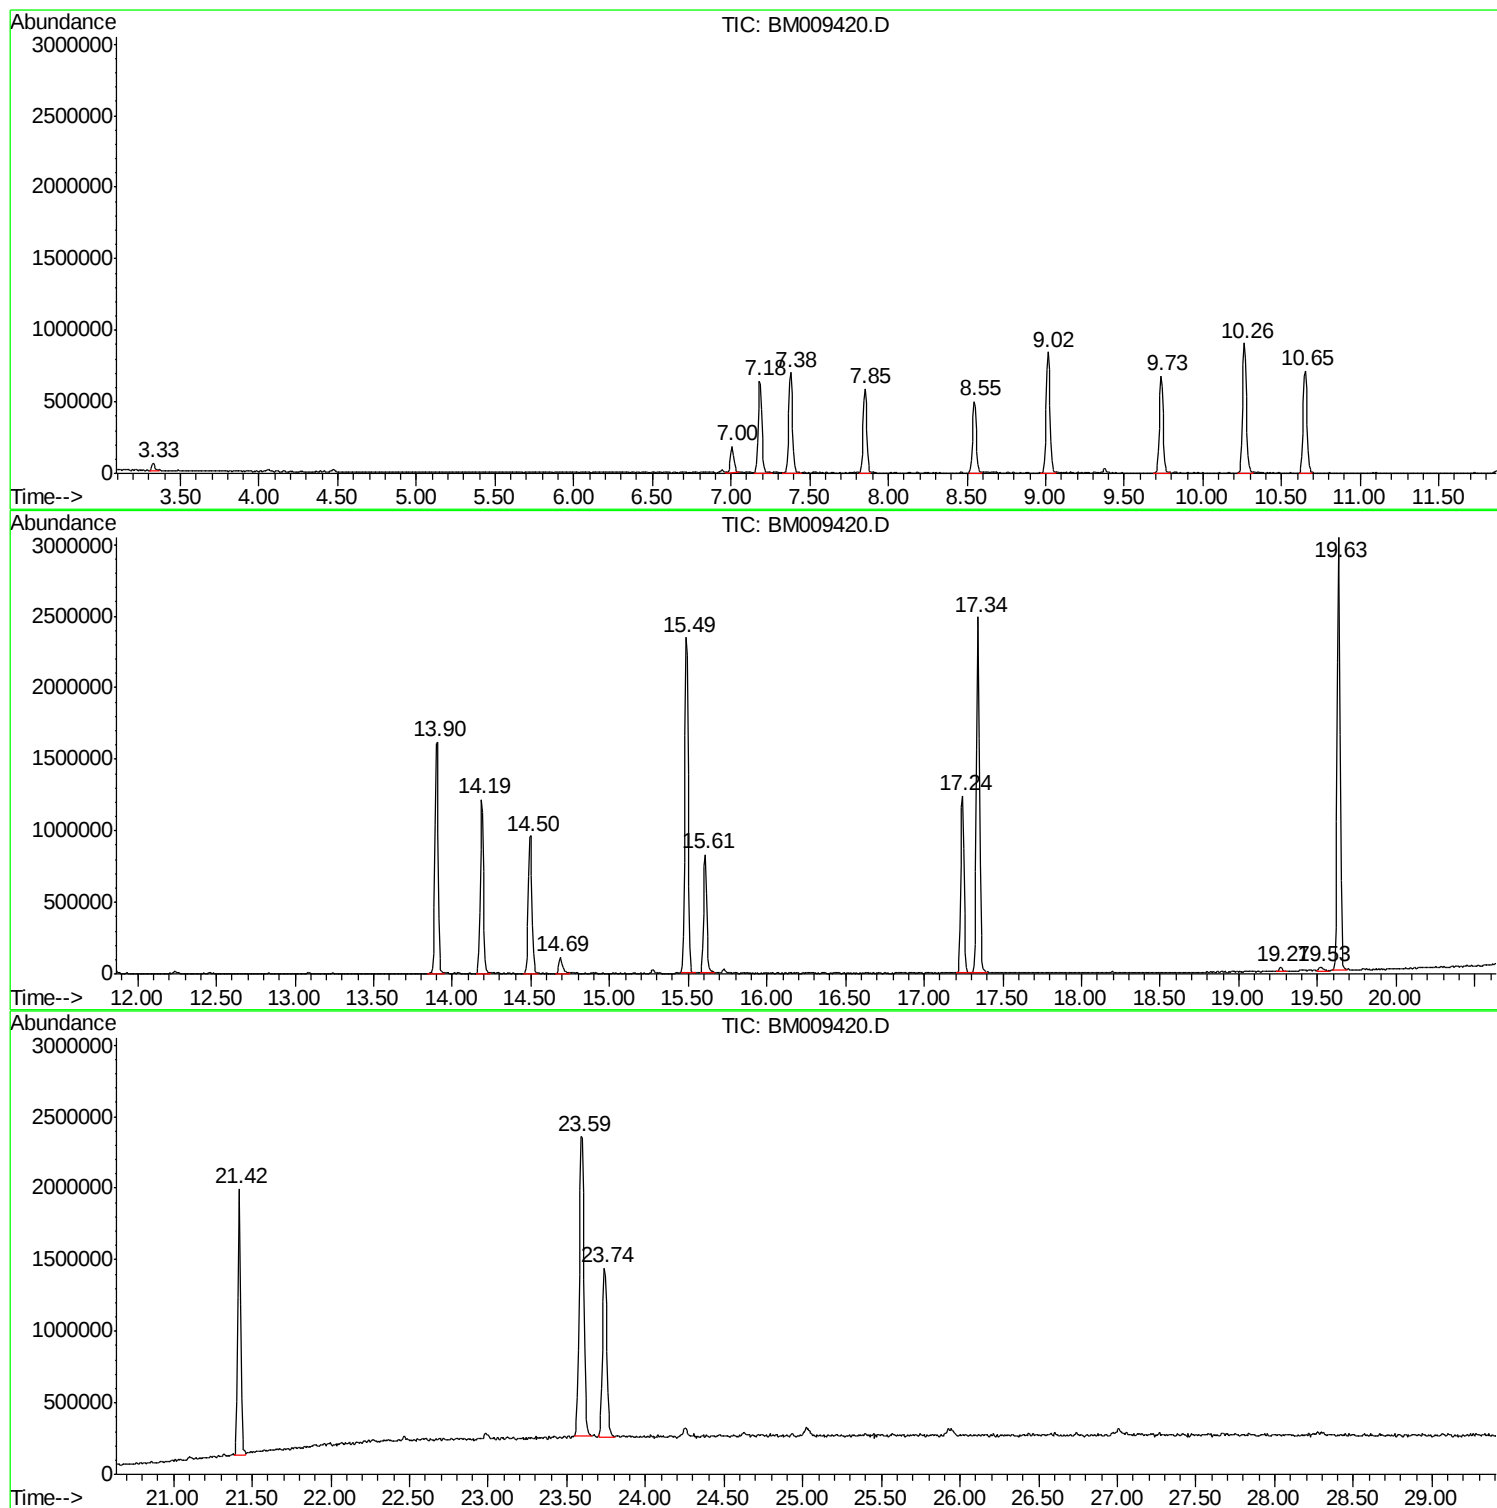

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
Data File : BM009420.D
Acq On : 27 Mar 2017 19:47
Operator : SJ/MA
Sample : I2372-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XZ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
Data File : BM009420.D
Acq On : 27 Mar 2017 19:47
Operator : SJ/MA
Sample : I2372-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9XZ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc