

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
 Data File : BM009423.D
 Acq On : 27 Mar 2017 21:35
 Operator : SJ/MA
 Sample : I2372-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G9Y60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rVB	47998	61946	1.46%	0.159%
2	7.004	661	666	675	rVB	197407	314914	7.42%	0.810%
3	7.181	690	696	706	rVB	671983	1049039	24.71%	2.697%
4	7.381	723	730	740	rBV	753787	1166488	27.48%	2.999%
5	7.851	804	810	818	rVB	612059	966859	22.77%	2.486%
6	8.545	922	928	938	rBV	543037	855436	20.15%	2.199%
7	9.016	999	1008	1017	rBV	851399	1430862	33.70%	3.679%
8	9.733	1121	1130	1139	rBV	711188	1148932	27.06%	2.954%
9	10.263	1212	1220	1229	rBV	945107	1581145	37.24%	4.065%
10	10.651	1279	1286	1295	rVB	743429	1278052	30.11%	3.286%
11	11.398	1404	1413	1417	rBV4	23400	44776	1.05%	0.115%
12	13.898	1832	1838	1847	rVB	1656273	2249811	53.00%	5.784%
13	14.186	1881	1887	1894	rBV	1248853	1830320	43.11%	4.706%
14	14.492	1931	1939	1947	rBV2	1036093	1566804	36.91%	4.028%
15	14.686	1967	1972	1981	rBV2	116413	206681	4.87%	0.531%
16	15.486	2102	2108	2116	rBV	2436993	3372169	79.43%	8.670%
17	15.604	2123	2128	2139	rBV	793299	1120831	26.40%	2.882%
18	17.245	2400	2407	2414	rBV2	1265486	1832301	43.16%	4.711%
19	17.345	2417	2424	2437	rVV	2505435	3647121	85.91%	9.377%
20	19.521	2790	2794	2801	rBV5	28904	46667	1.10%	0.120%
21	19.633	2807	2813	2820	rBV	3196024	4187588	98.64%	10.766%
22	21.415	3111	3116	3123	rBV	1869576	2396047	56.44%	6.160%
23	23.591	3479	3486	3495	rBV2	2188491	4245307	100.00%	10.915%
24	23.738	3505	3511	3520	rVB	1179551	2294517	54.05%	5.899%


Sum of corrected areas: 38894613

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
Data File : BM009423.D
Acq On : 27 Mar 2017 21:35
Operator : SJ/MA
Sample : I2372-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9Y60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

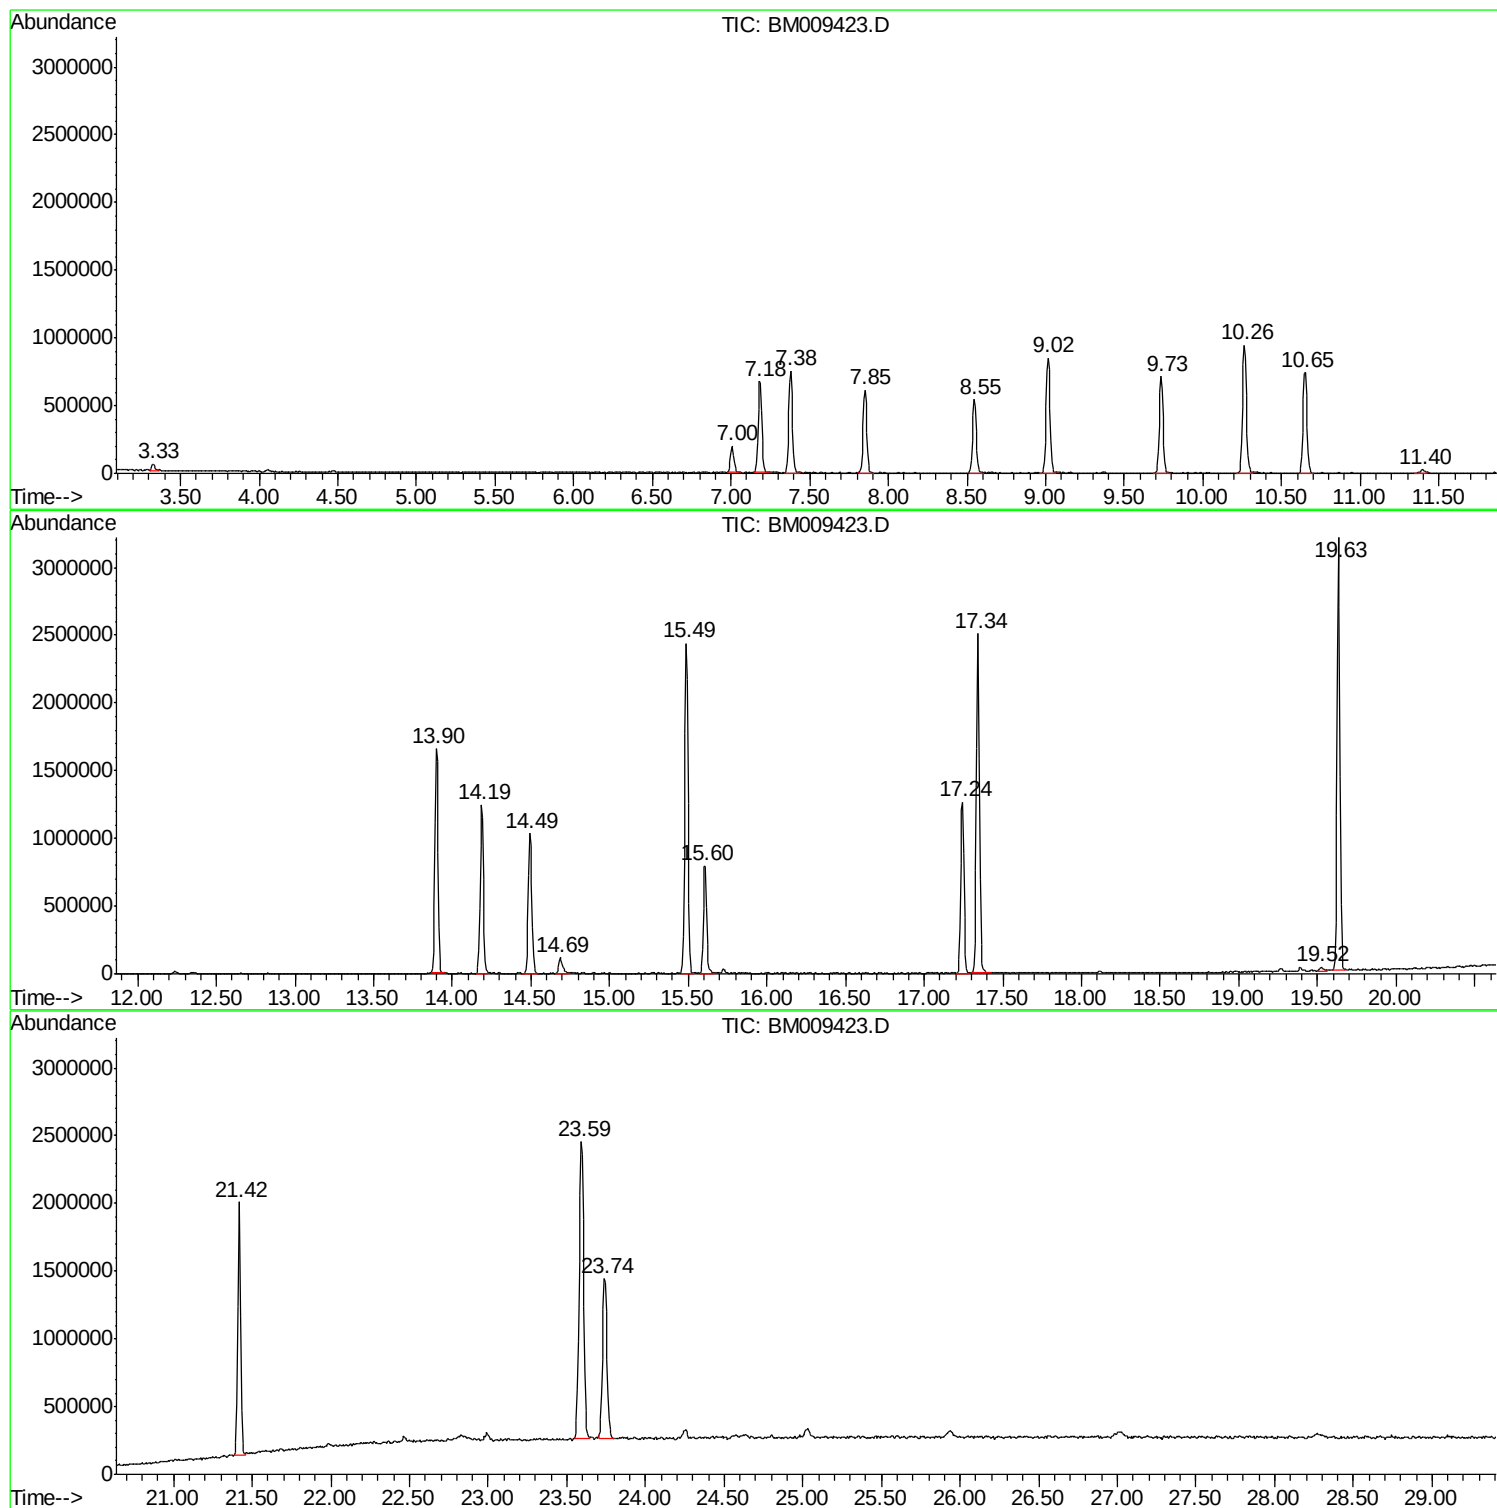

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
Data File : BM009423.D
Acq On : 27 Mar 2017 21:35
Operator : SJ/MA
Sample : I2372-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9Y60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM032817\
Data File : BM009423.D
Acq On : 27 Mar 2017 21:35
Operator : SJ/MA
Sample : I2372-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G9Y60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032317MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc