
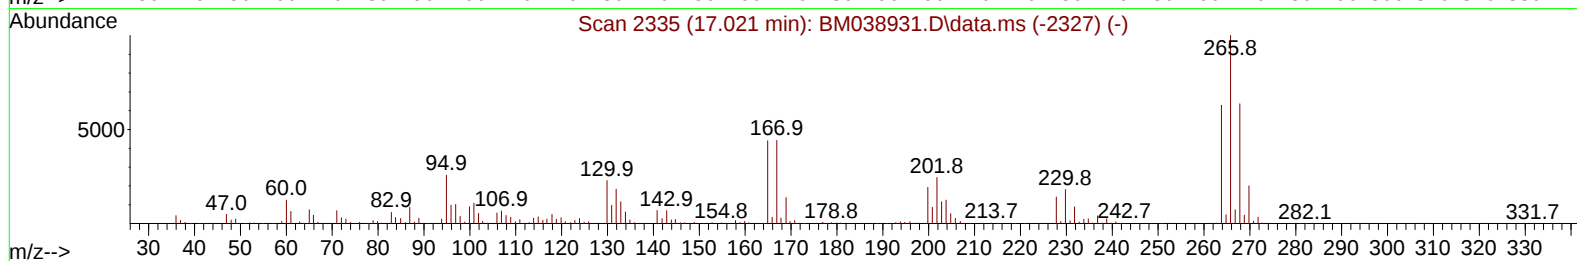
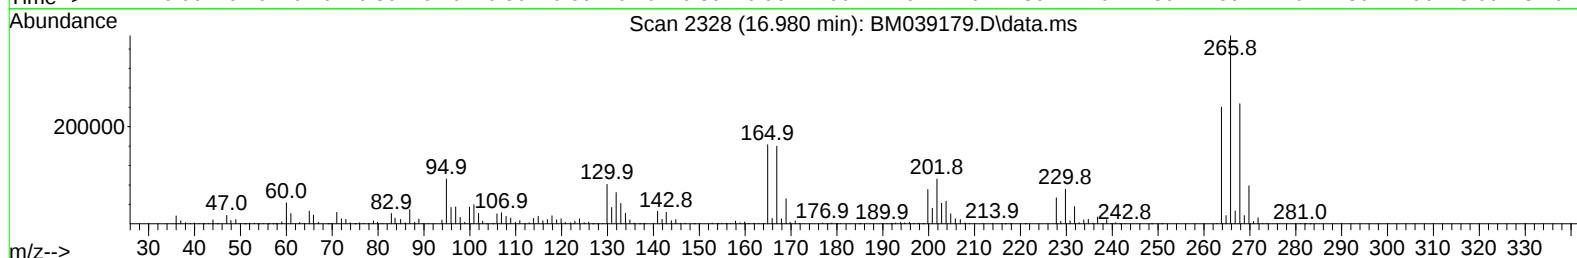


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032823\
 Data File : BM039179.D
 Acq On : 28 Mar 2023 14:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 05:35:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 29 01:28:31 2023
 Response via : Initial Calibration

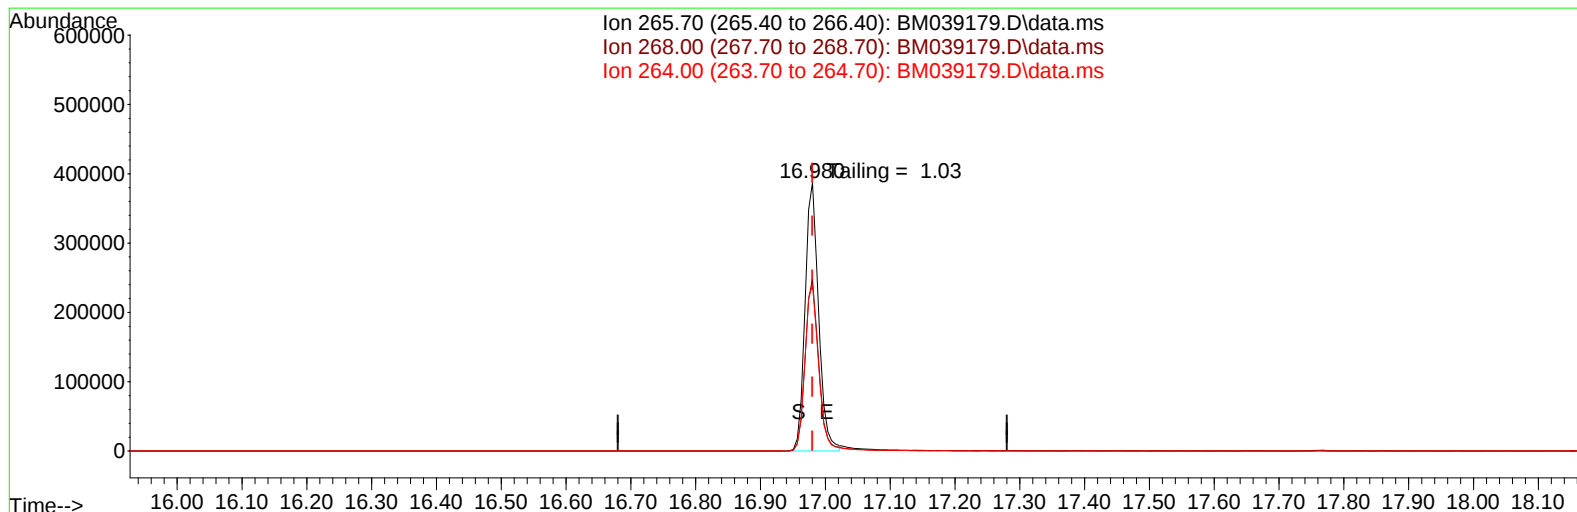

TIC: BM039179.D\data.ms

(70) Pentachlorophenol (C)




16.980min (+ 0.000) 0.00 ng

response 578749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.87
264.00	62.90	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032823\
Data File : BM039179.D
Acq On : 28 Mar 2023 14:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 05:35:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 29 01:28:31 2023
Response via : Initial Calibration

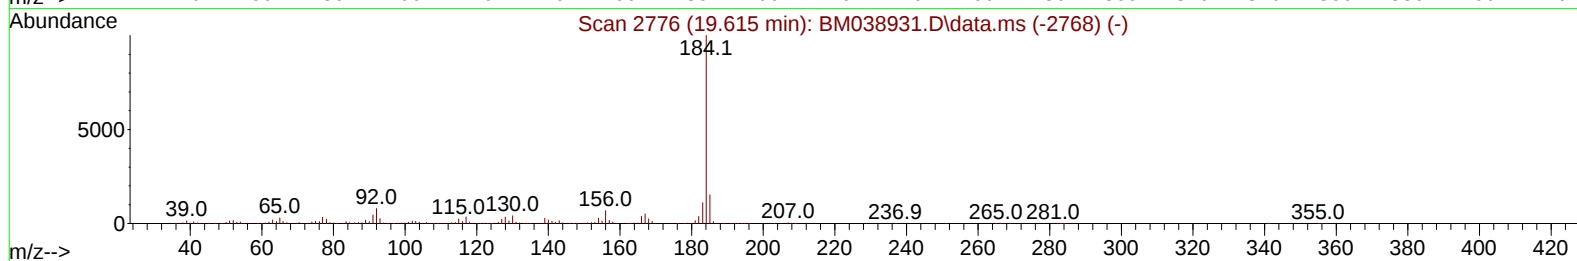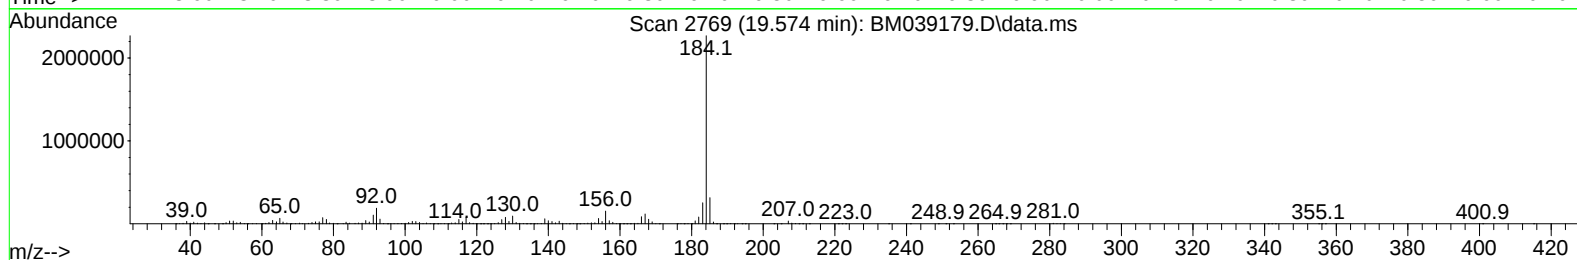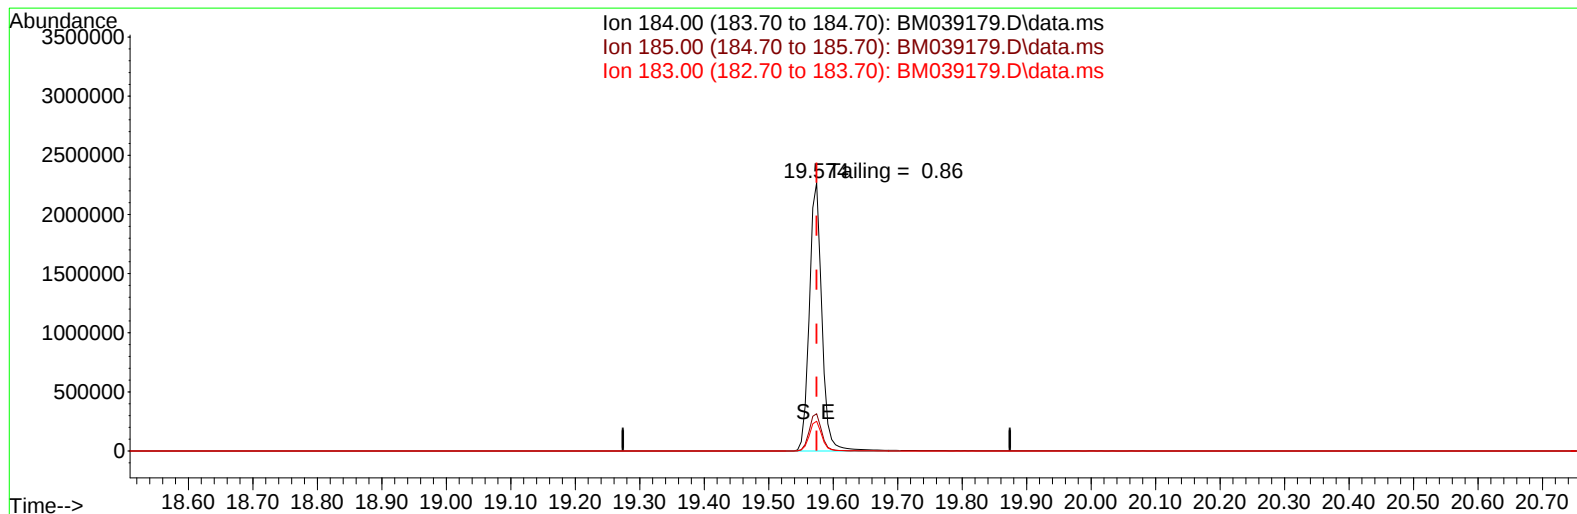

TIC: BM039179.D\data.ms

(77) Benzidine**19.574min (+ 0.000) 50430.41 ng****response 3075646**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	13.90
183.00	11.00	11.13
0.00	0.00	0.00