
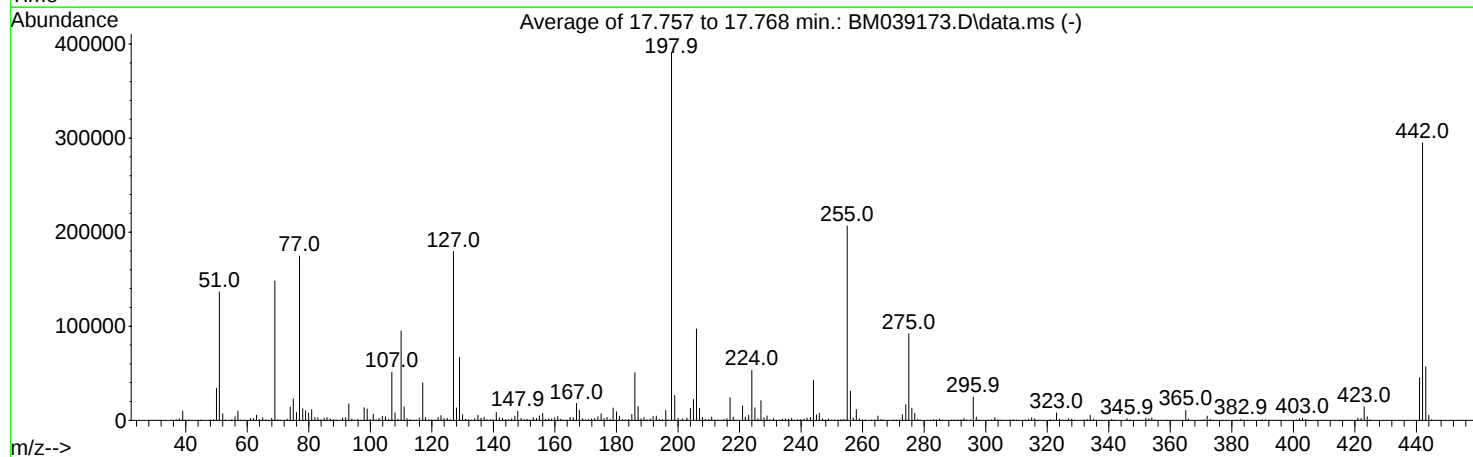


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032823\
Data File : BM039173.D
Acq On : 28 Mar 2023 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 29 01:28:31 2023

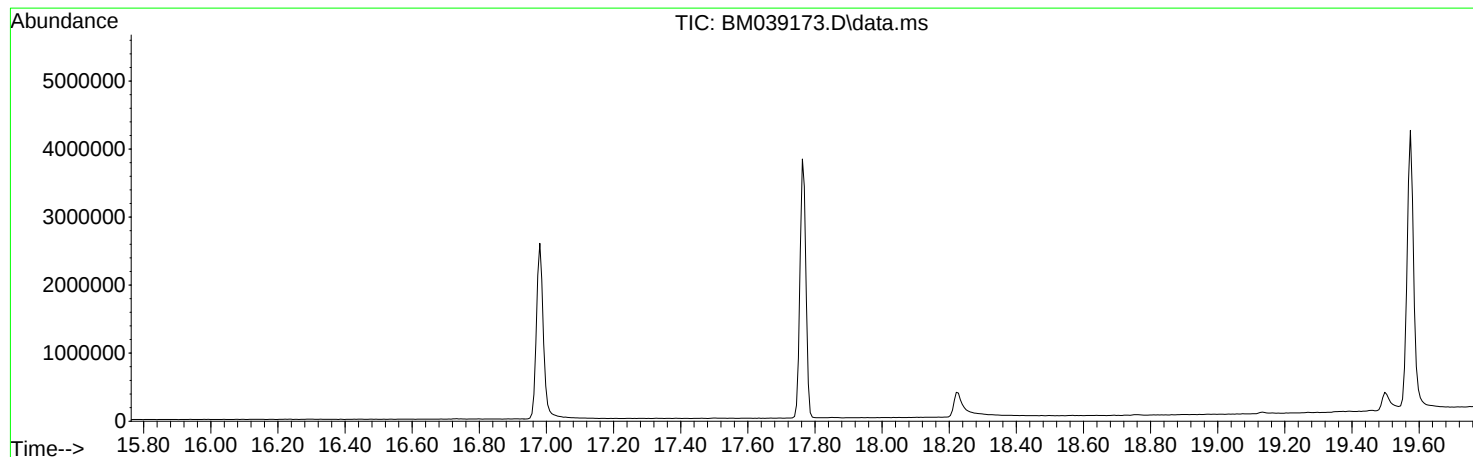




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	136512	PASS
68	69	0.00	2	1.5	2218	PASS
69	198	0.00	100	37.8	148015	PASS
70	69	0.00	2	0.5	695	PASS
127	198	10	80	45.9	179392	PASS
197	198	0.00	2	0.1	494	PASS
198	198	100	100	100.0	391083	PASS
199	198	5	9	6.8	26421	PASS
275	198	10	60	23.5	92072	PASS
365	198	1	100	2.7	10588	PASS
441	198	0.01	100	11.6	45176	PASS
442	442	50	100	100.0	295061	PASS
443	442	15	24	19.3	57093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032823\
 Data File : BM039173.D
 Acq On : 28 Mar 2023 10:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 05:32:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 29 01:28:31 2023
 Response via : Initial Calibration

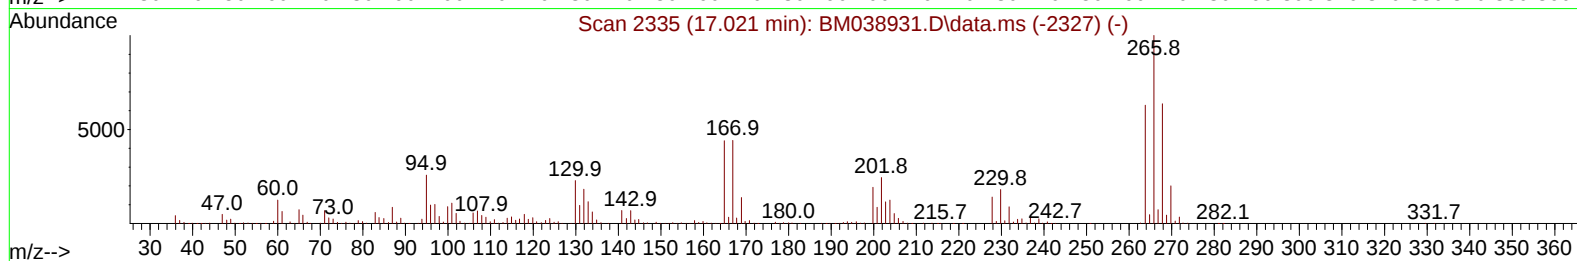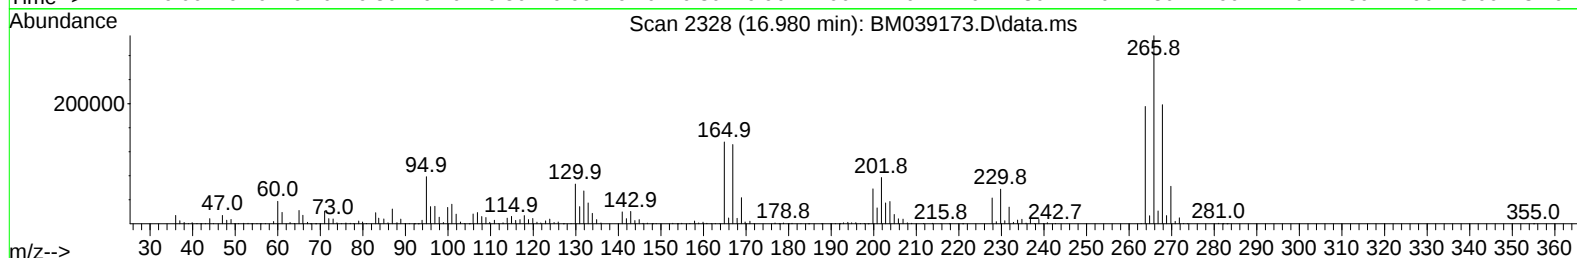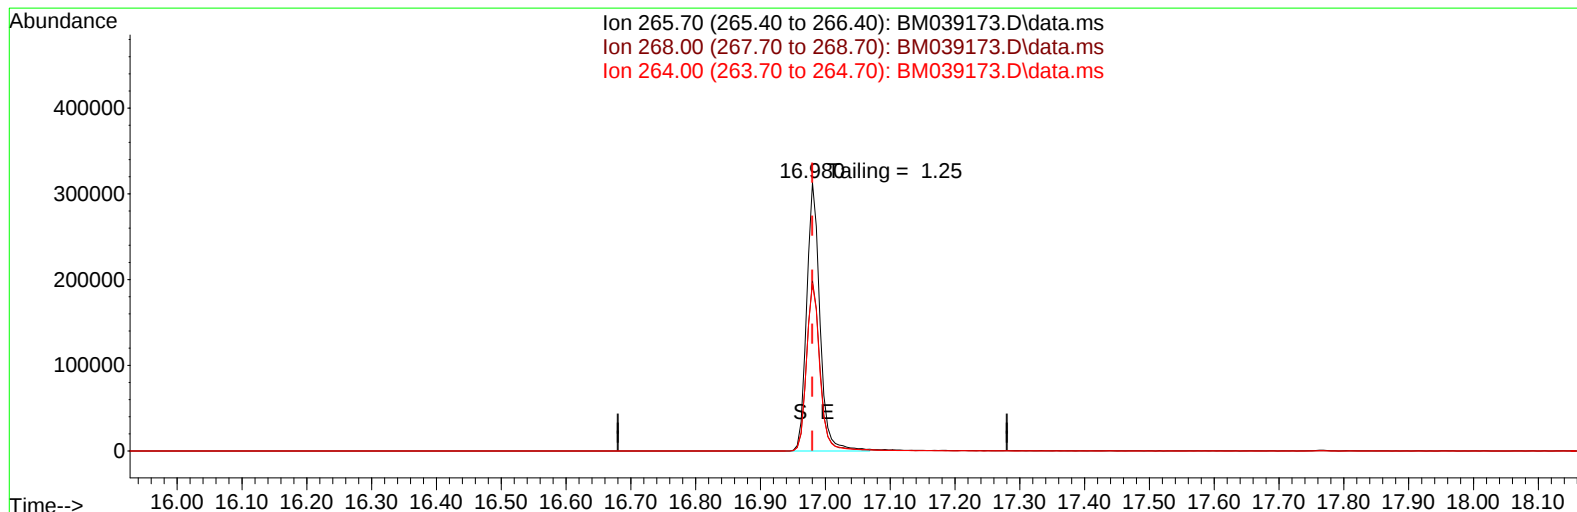

TIC: BM039173.D\data.ms

(70) Pentachlorophenol (C)

16.980min (+ 0.000) 445326.33 ng




response 450855

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.33
264.00	62.90	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032823\
Data File : BM039173.D
Acq On : 28 Mar 2023 10:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 29 05:32:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 29 01:28:31 2023
Response via : Initial Calibration

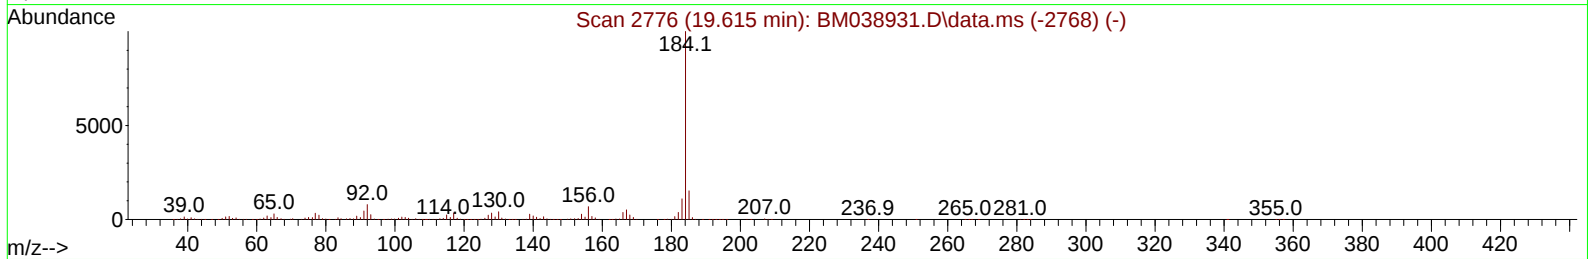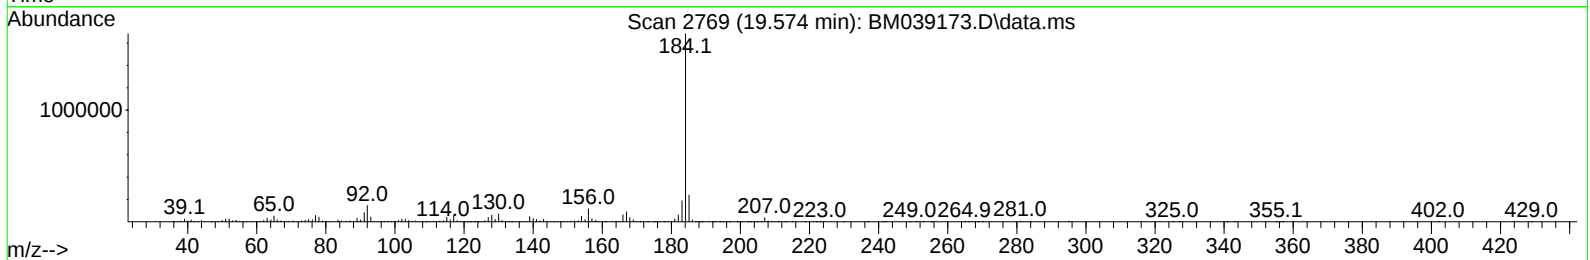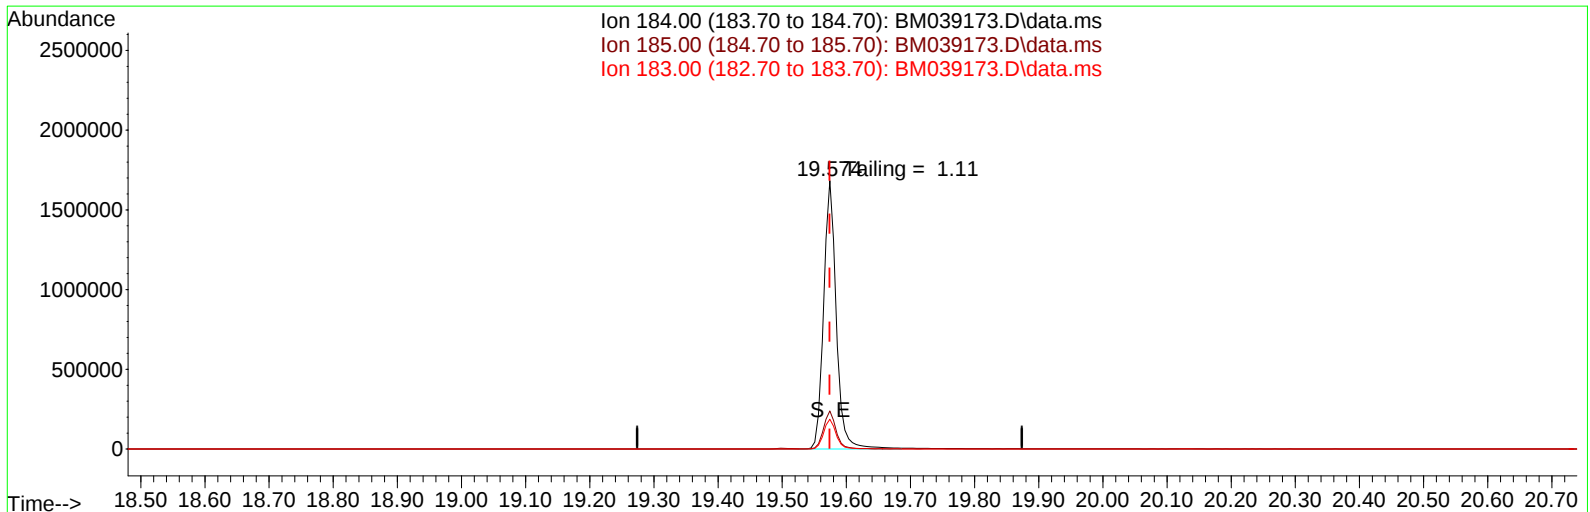

TIC: BM039173.D\data.ms

(77) Benzidine

19.574min (+ 0.000) 25705.62 ng

response 2324645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.23
183.00	11.00	11.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2023	BNA_M	<u>BM039173.D</u>
Compound Name	Response	Retention Time
DDT	1177272	20.803
DDD	35431	20.362
DDE	1865	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37296	1214568	3.07

Instrument :
BNA_M
ClientSampleId :
DFTPP